

1/8

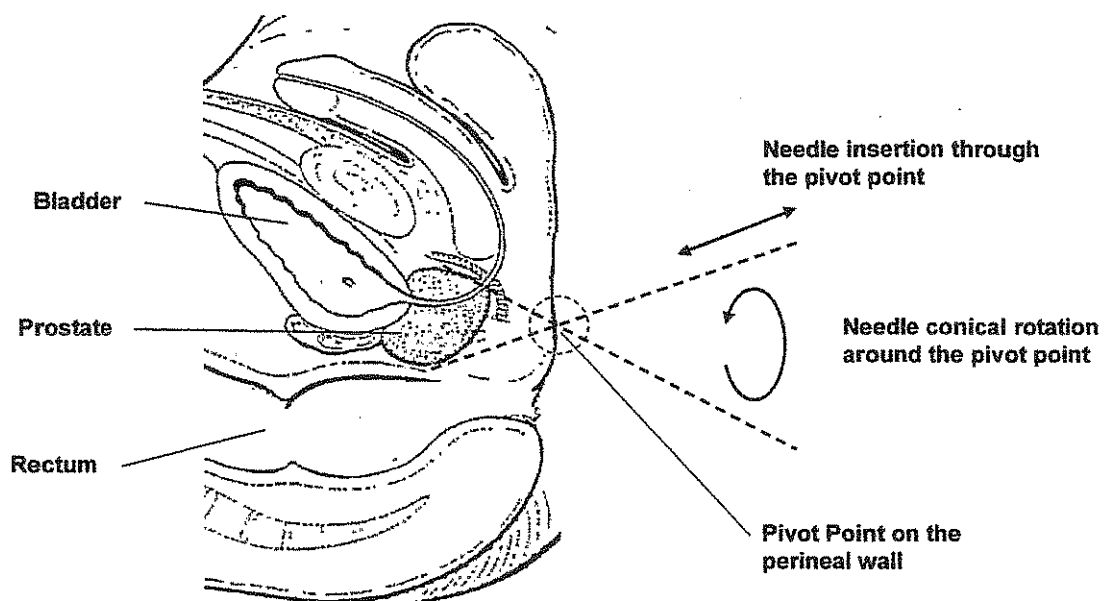


FIG. 1

2/8

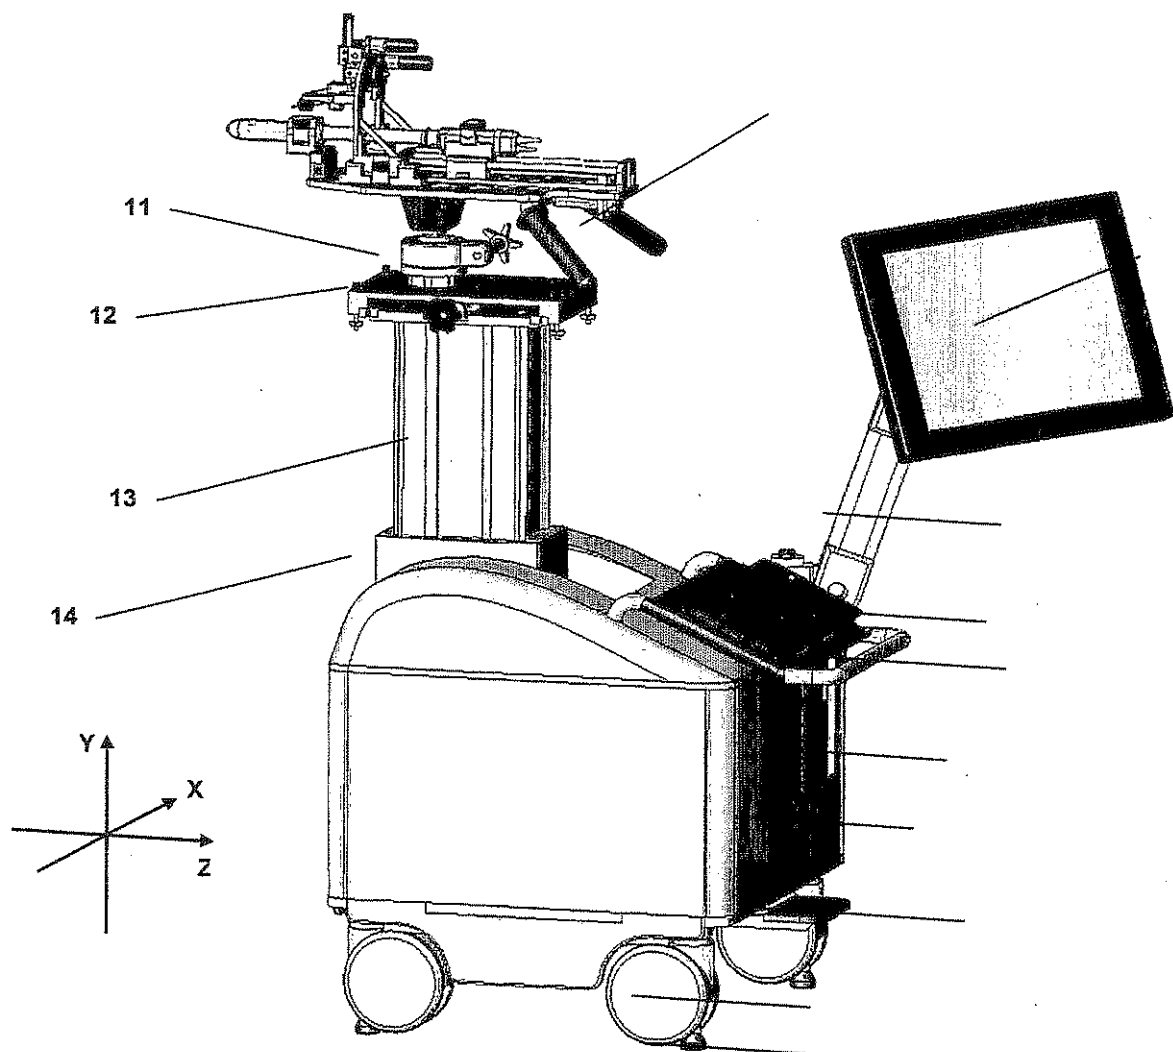


FIG. 2

3/8

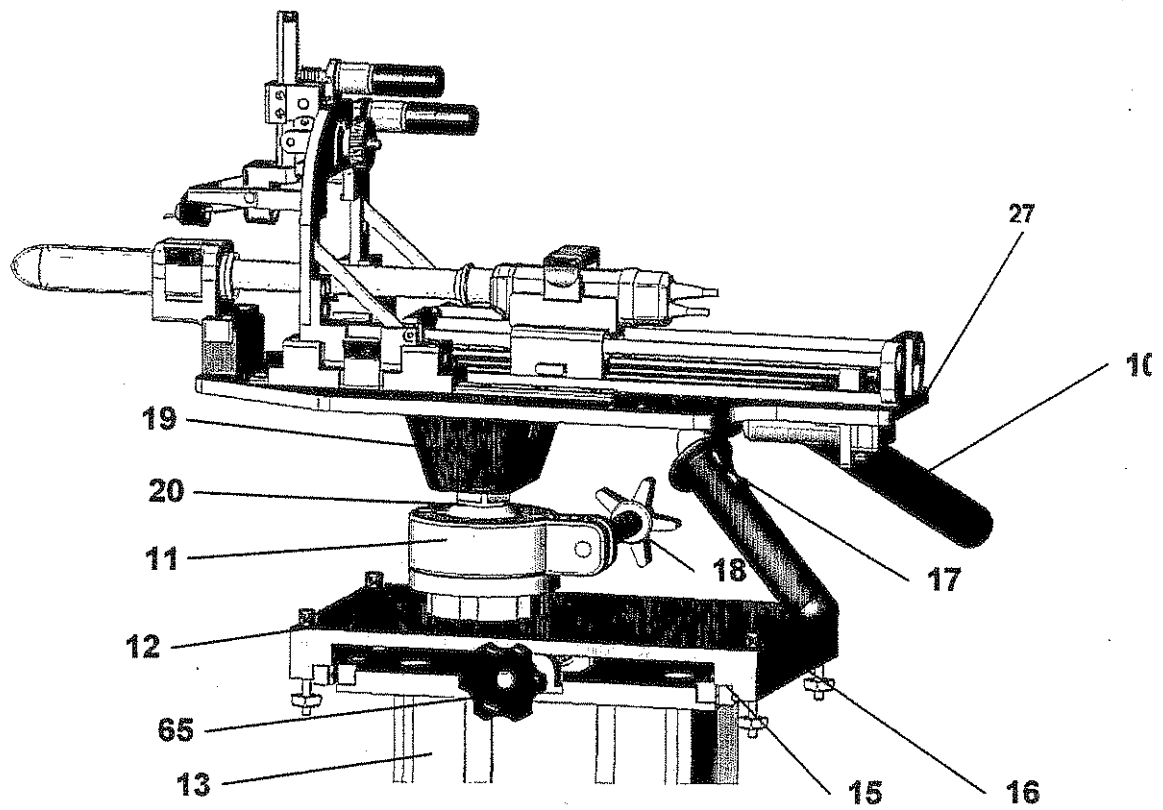


FIG. 3

4/8

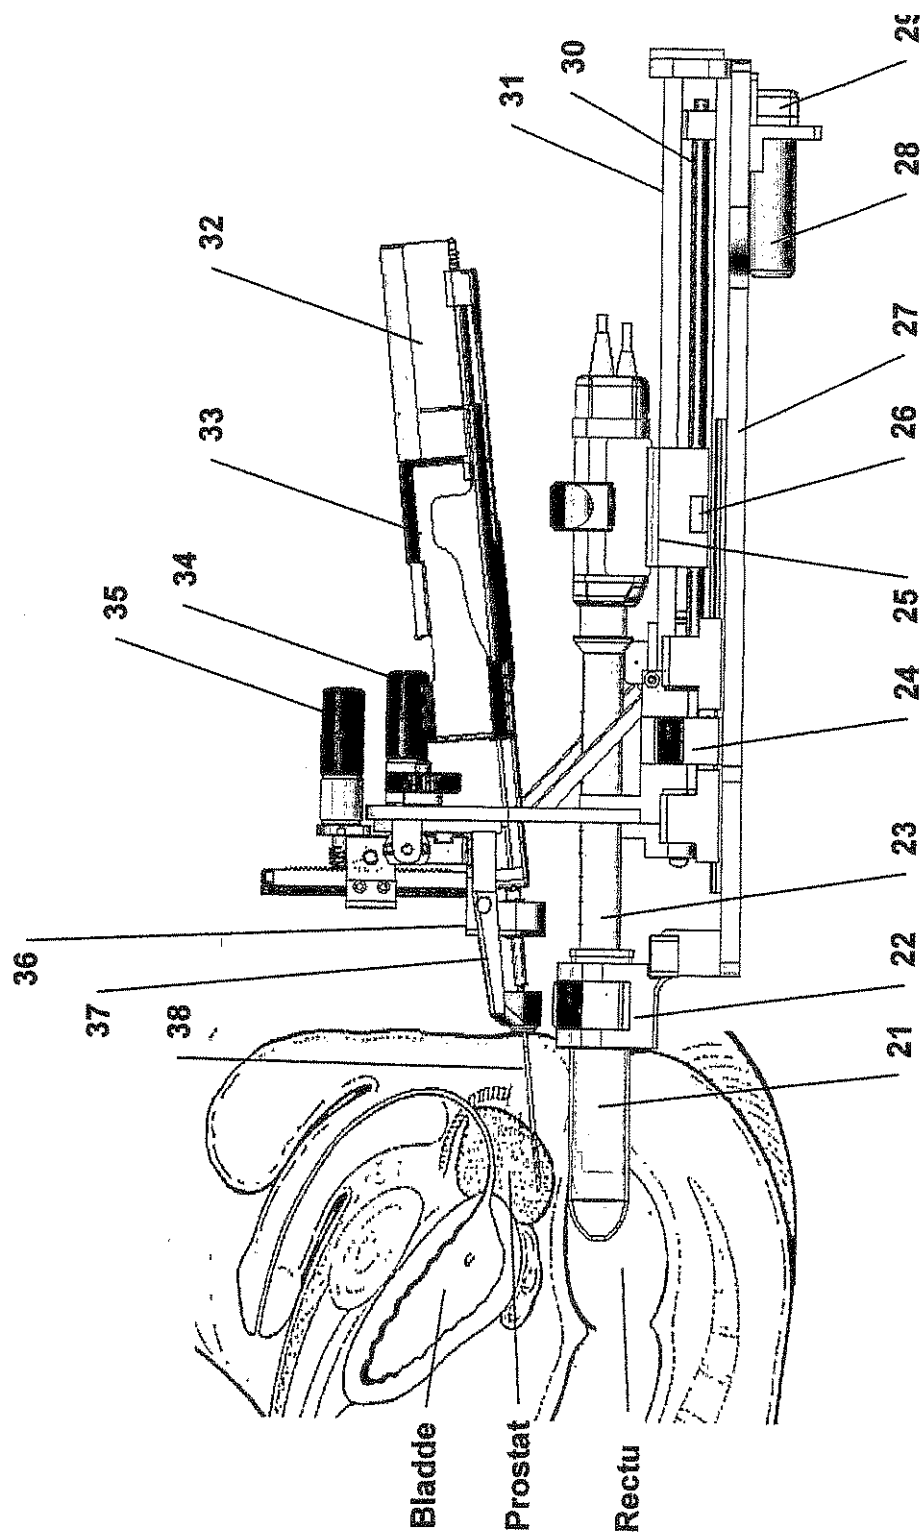


FIG. 4

5/8

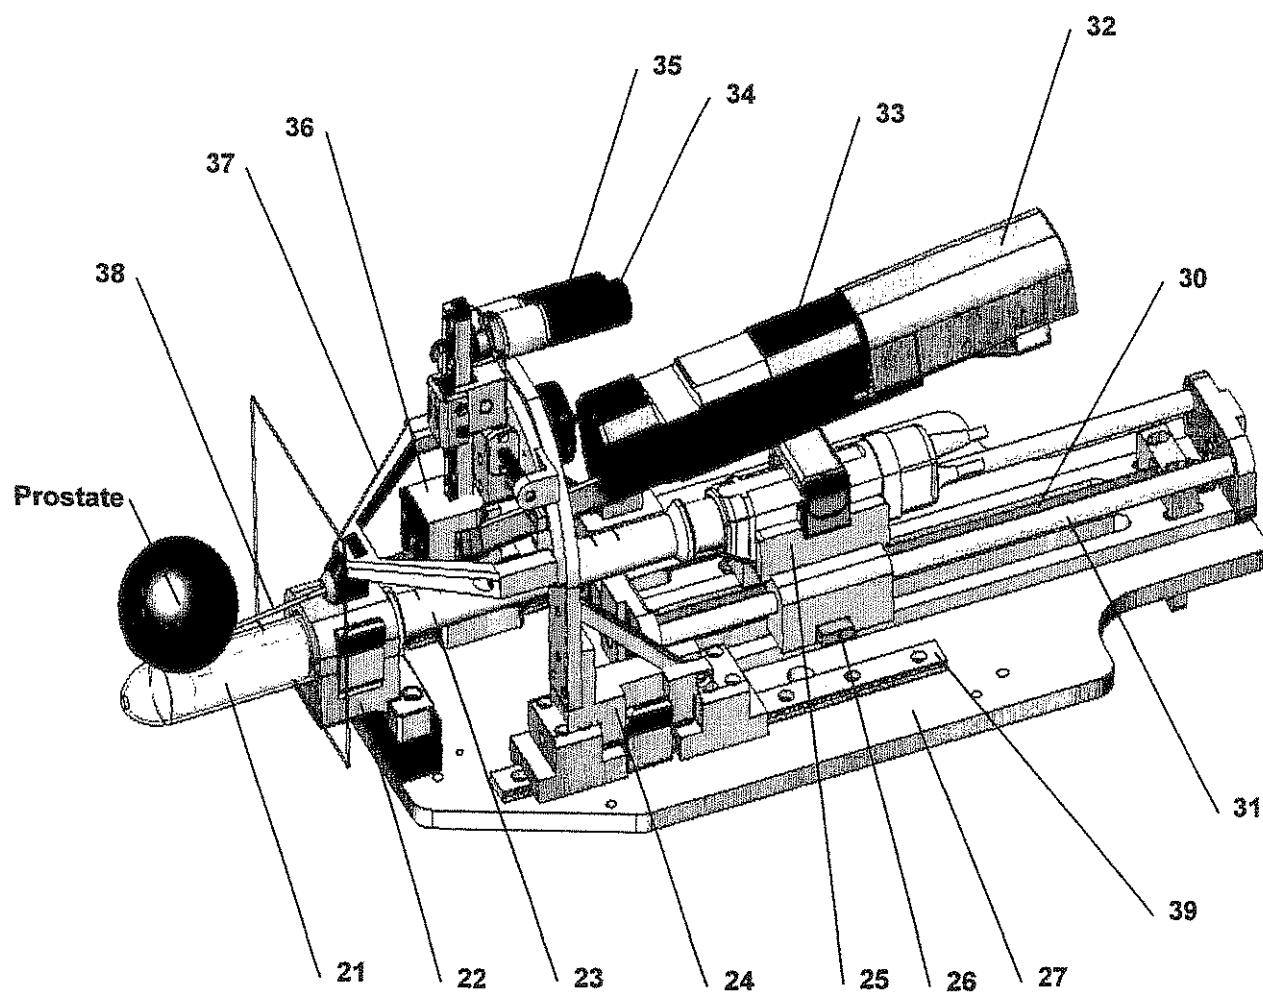


FIG. 5



7/8

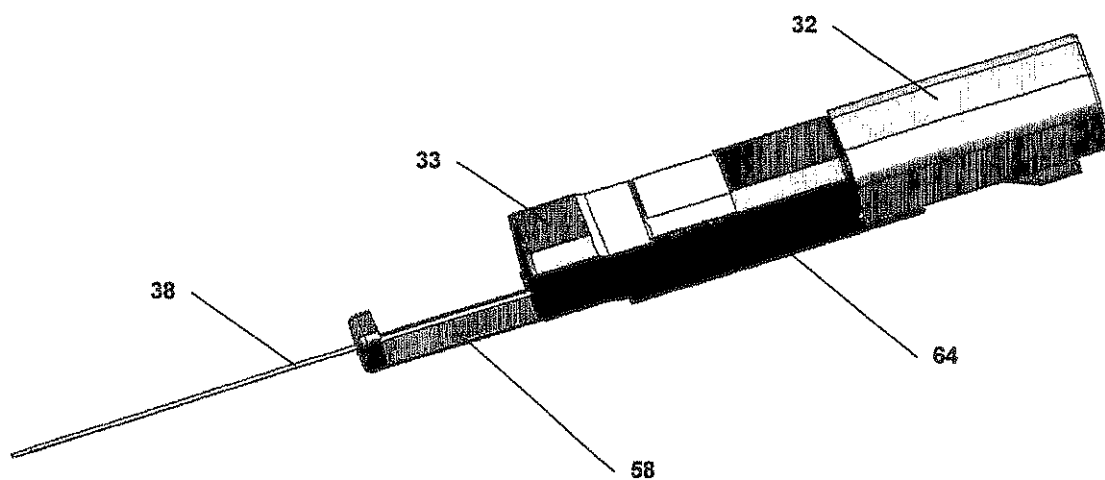


FIG. 7A

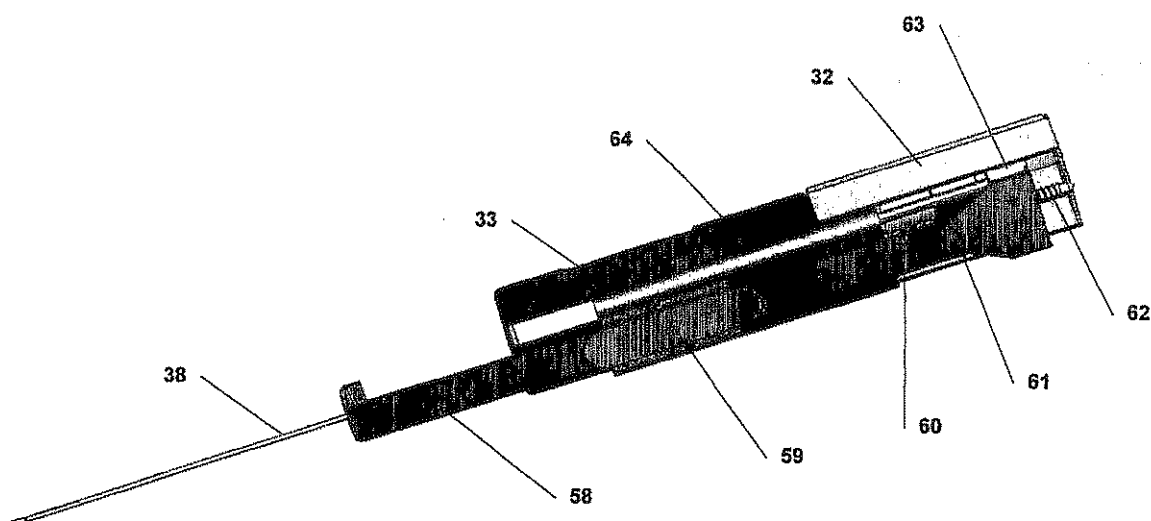


FIG. 7B

8/8

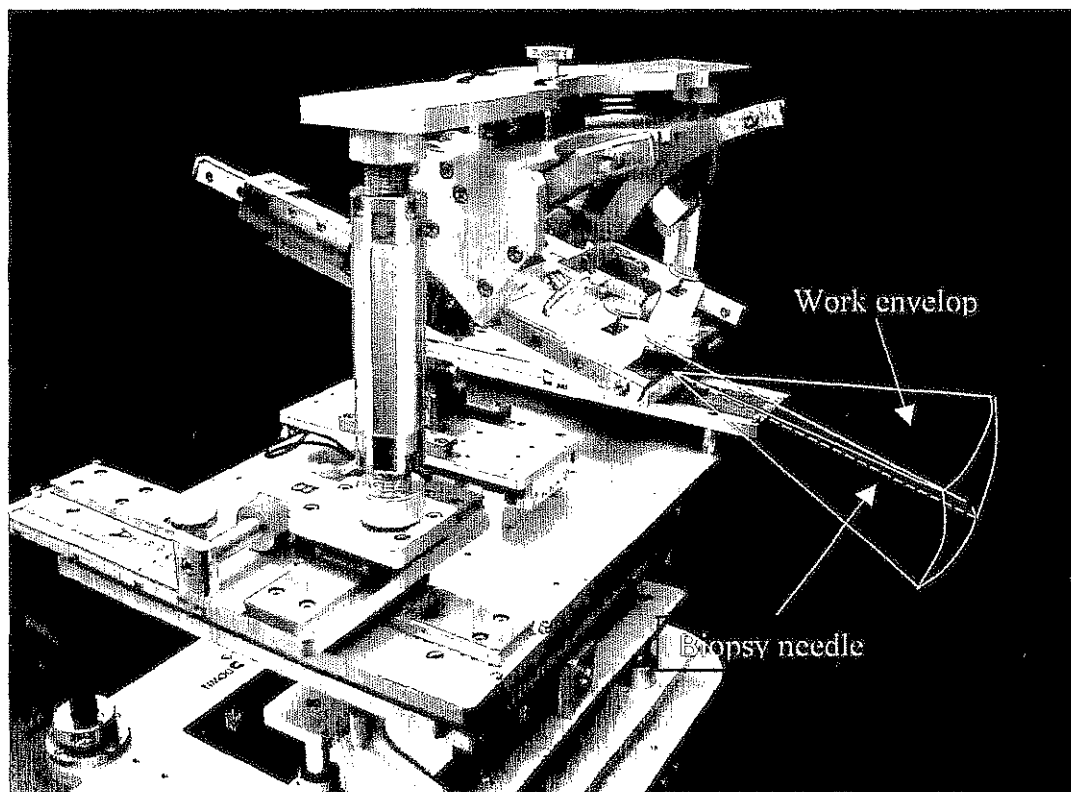


FIG. 8 Inventors' previous biopsy robot system design

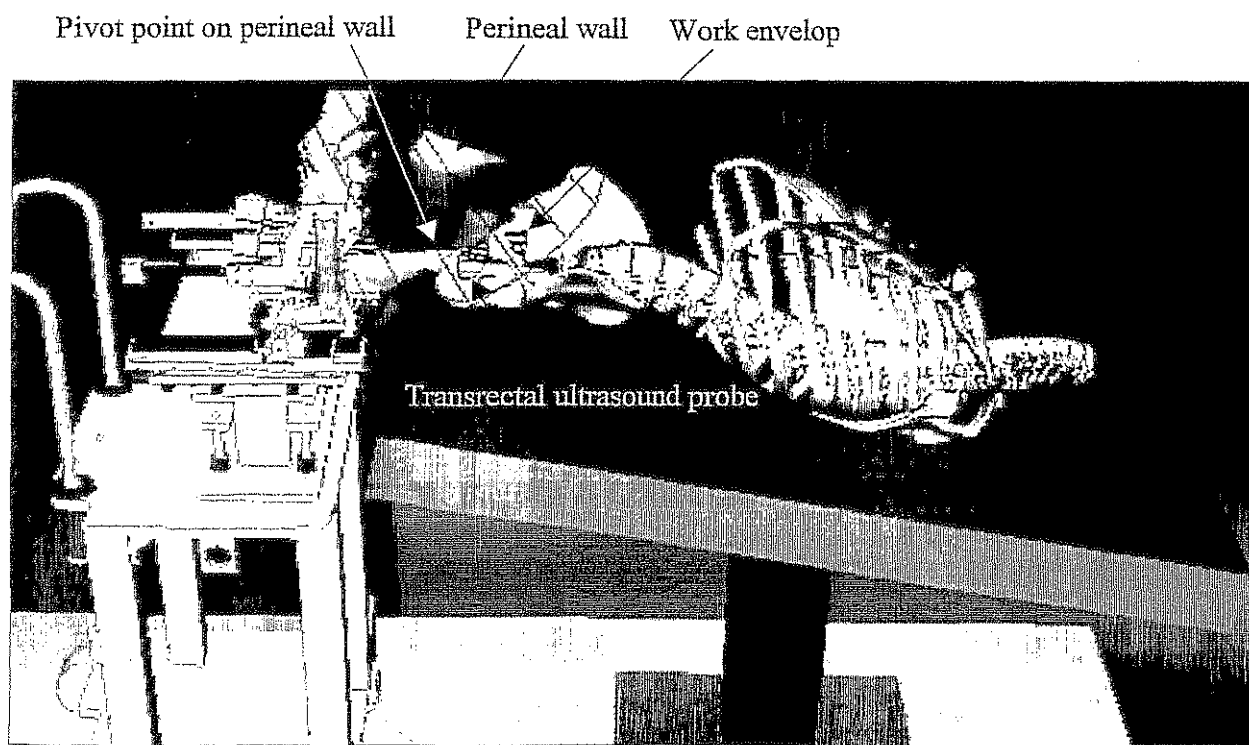


FIG. 9 Operating table tilted down to allow better coverage of anterior part of prostate with the work envelop shown in FIG. 8