

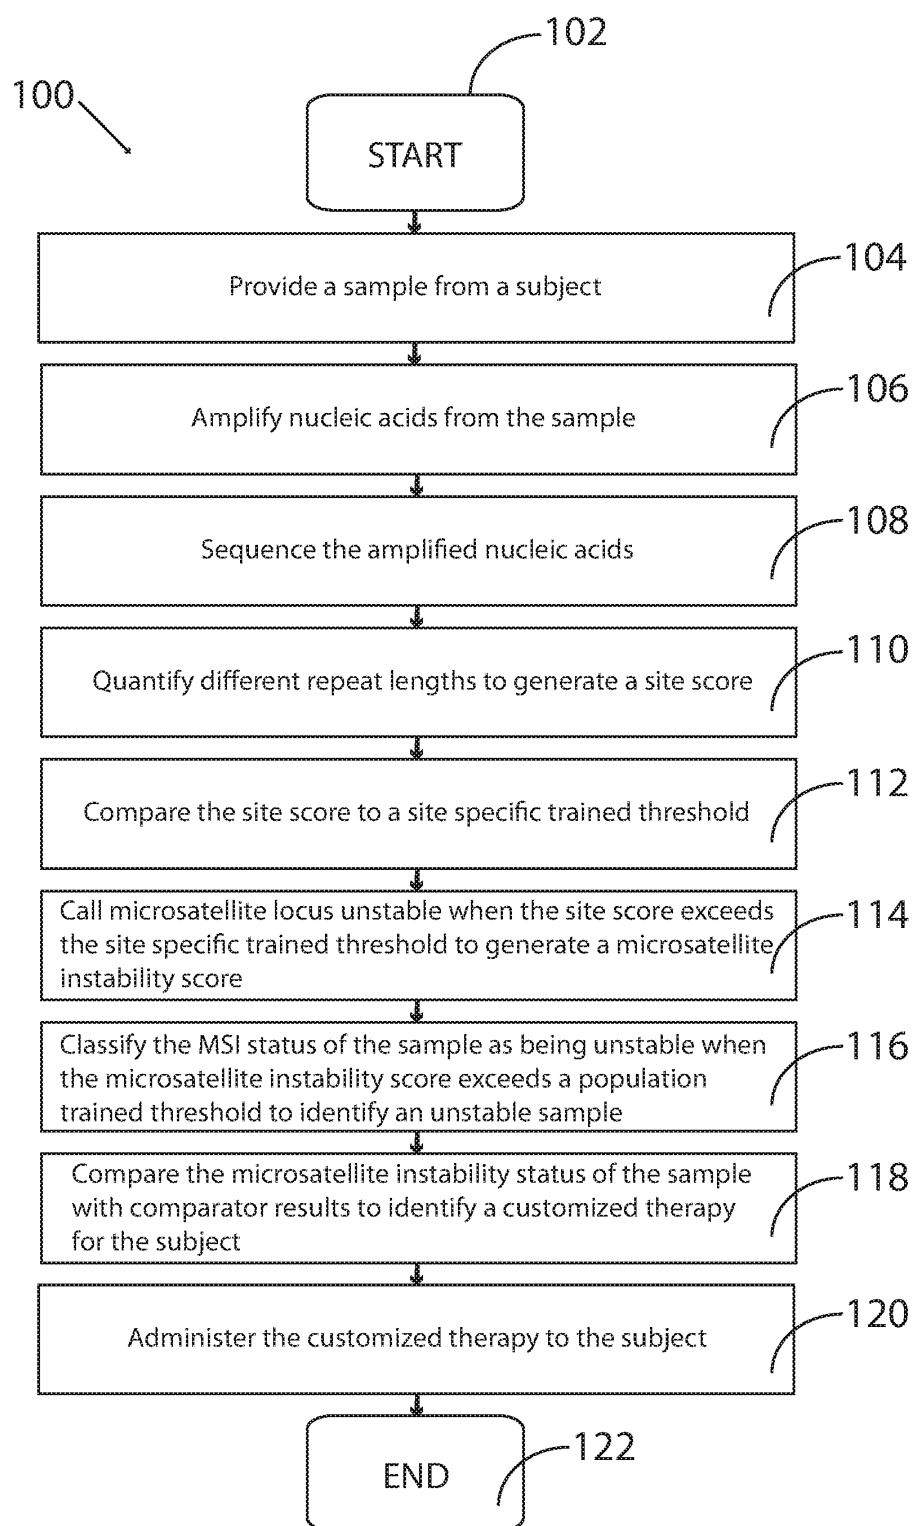


FIGURE 1

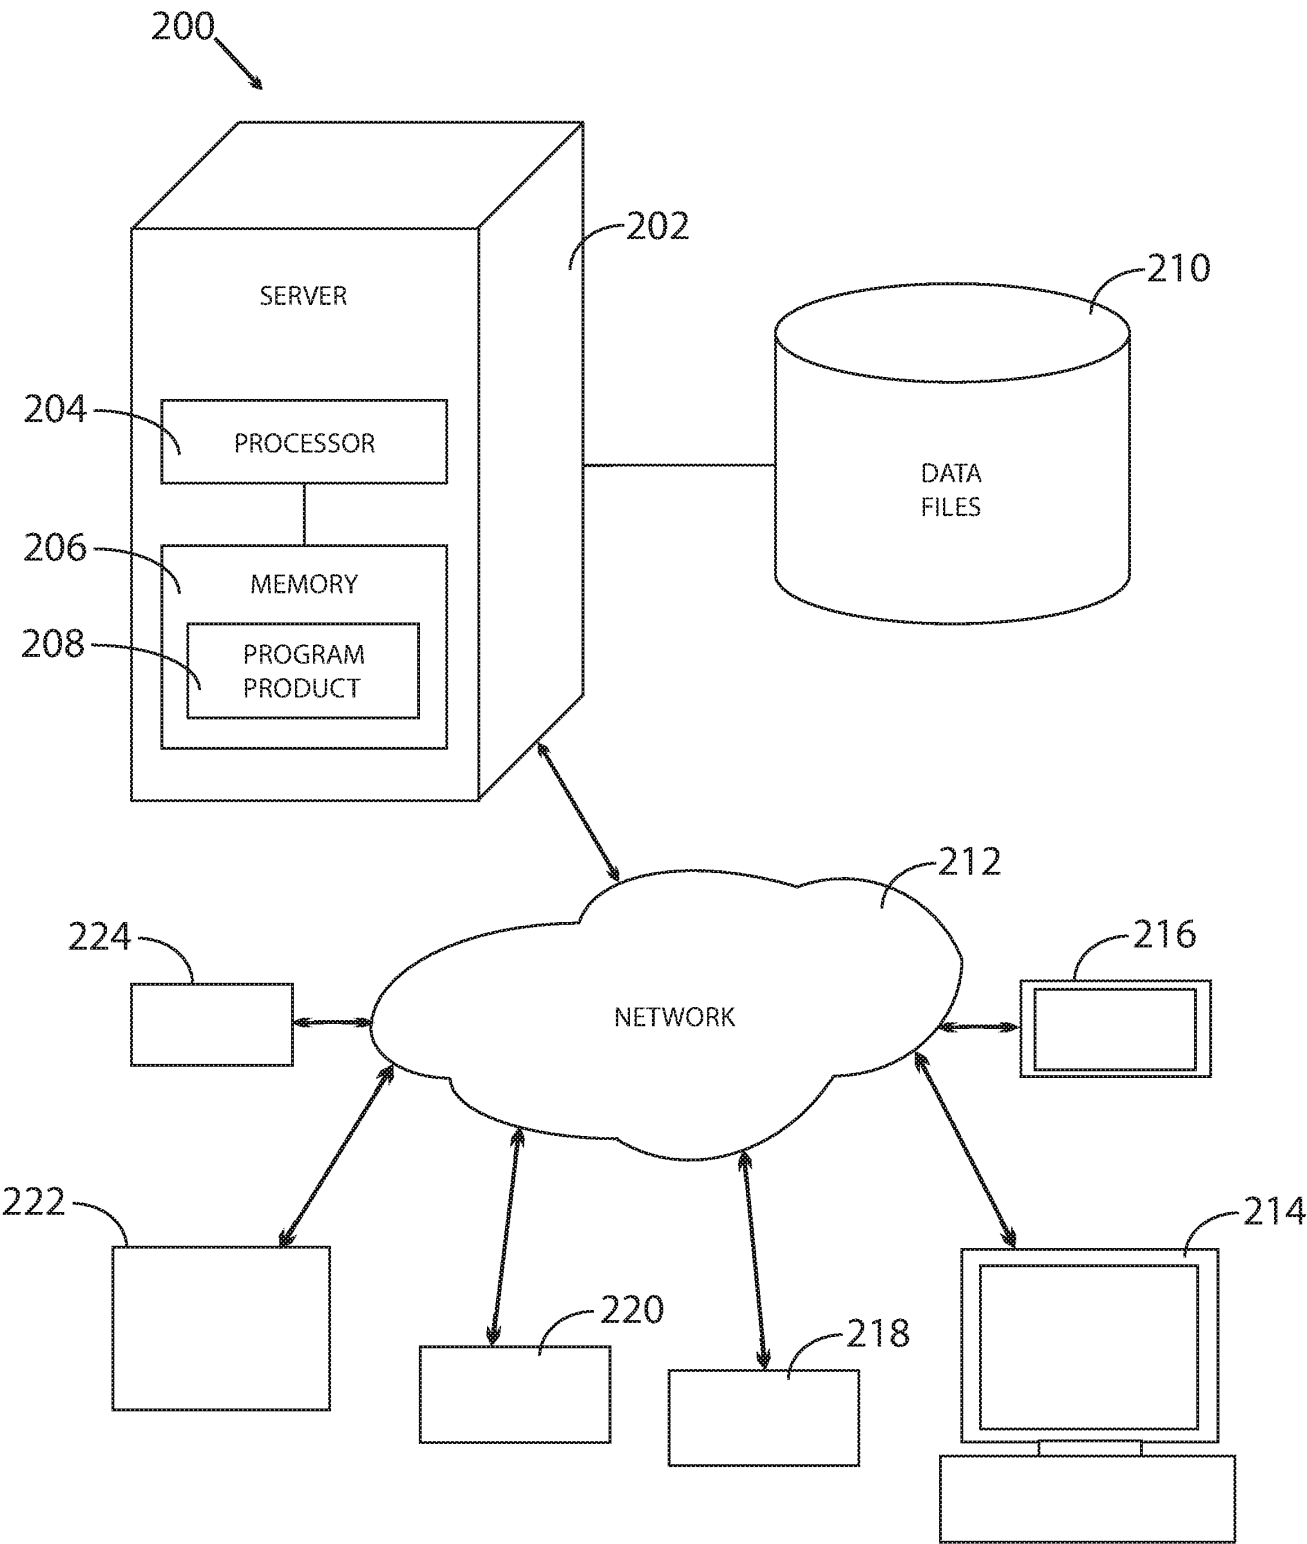


FIGURE 2

LoD, simulated samples

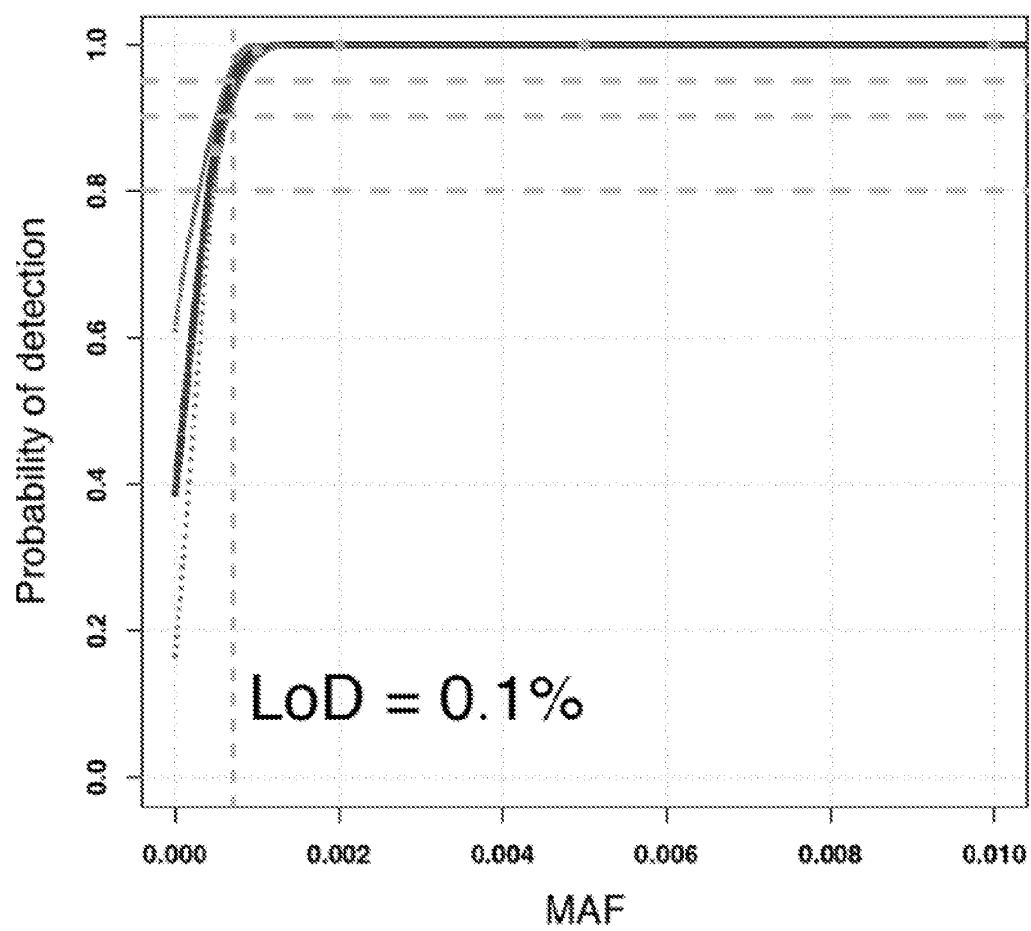


FIGURE 3

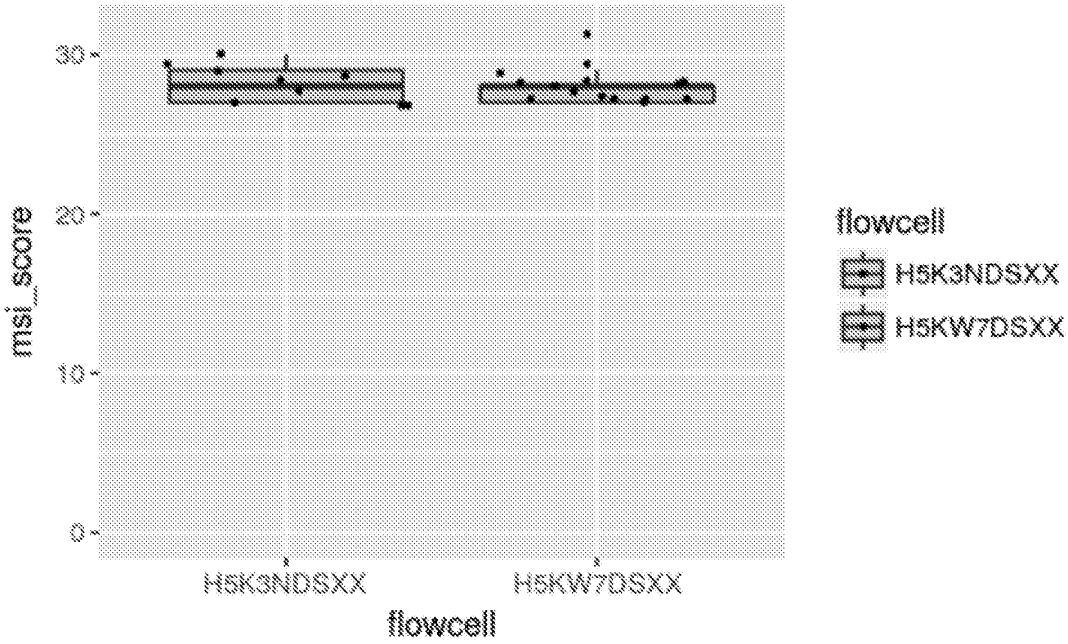


FIGURE 4A

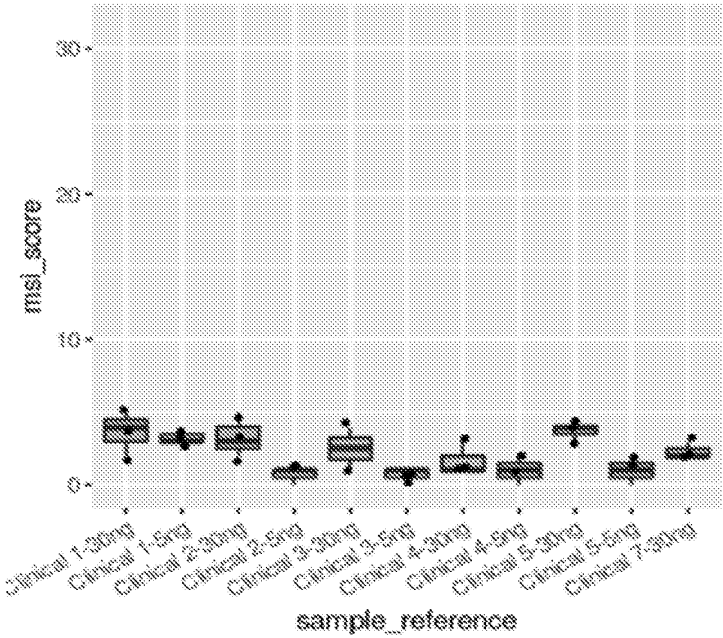


FIGURE 4B

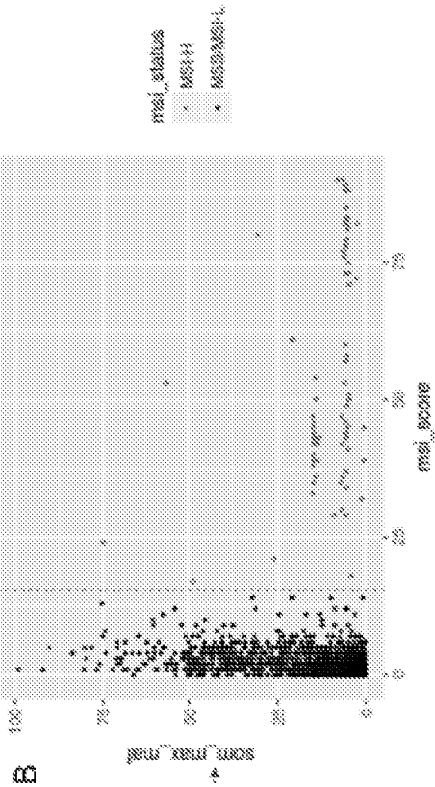


FIGURE 5B

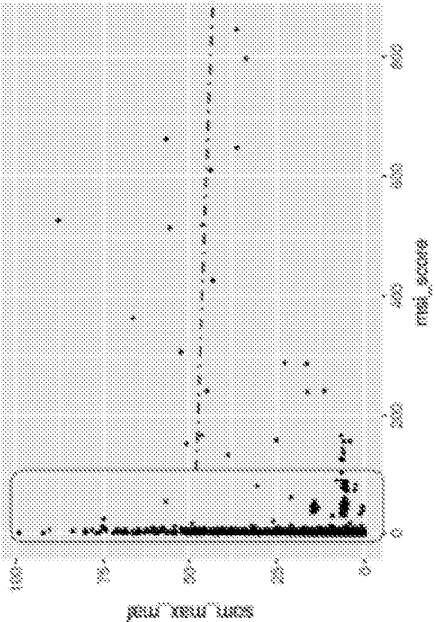


FIGURE 5A

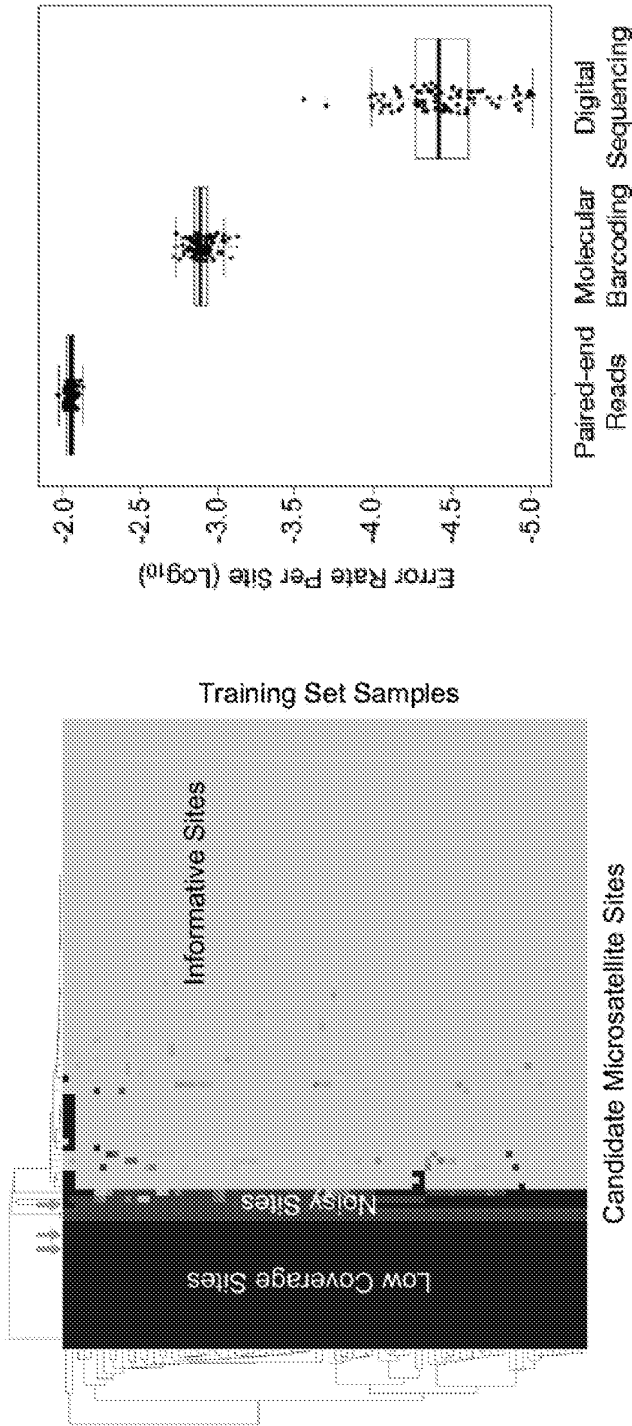


FIGURE 6A

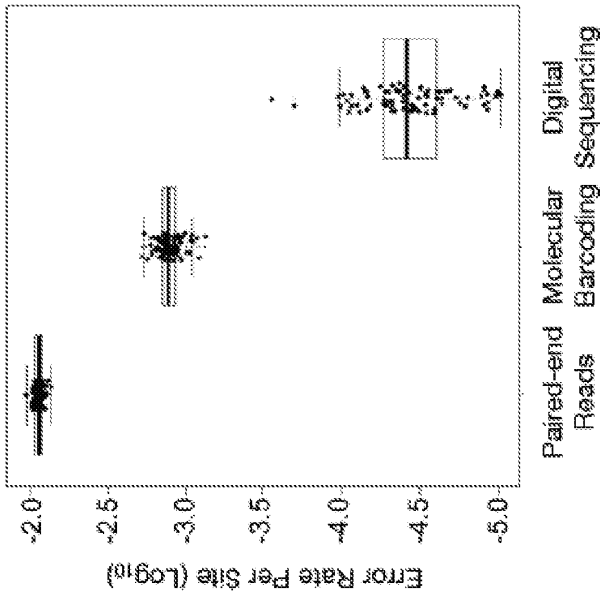


FIGURE 6B

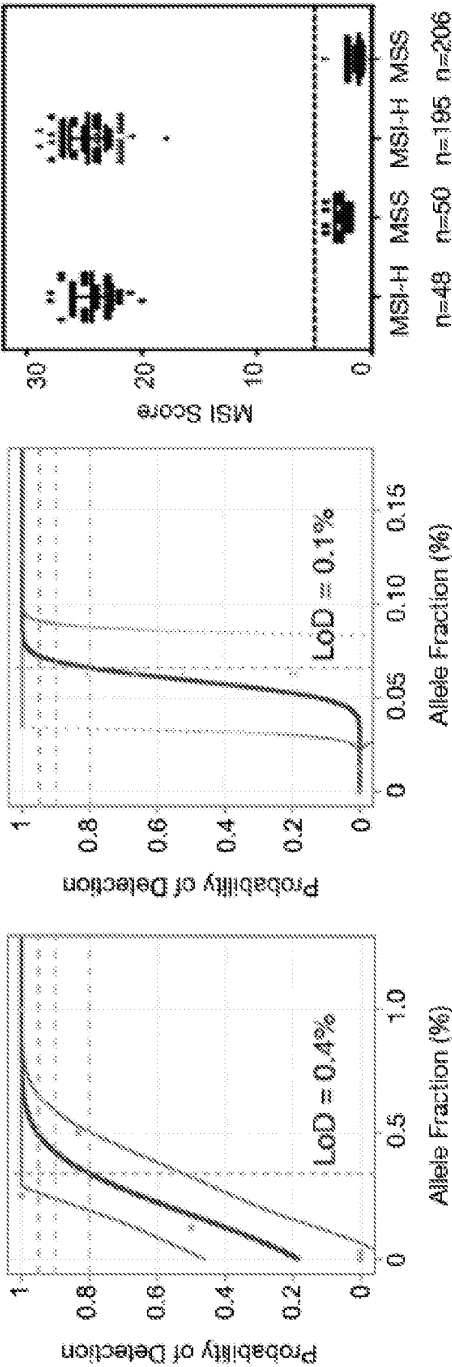


FIGURE 7A

FIGURE 7B

FIGURE 7C

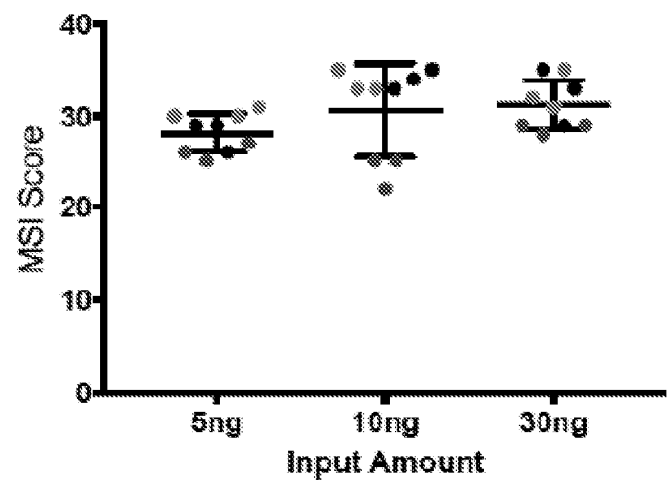


FIGURE 8

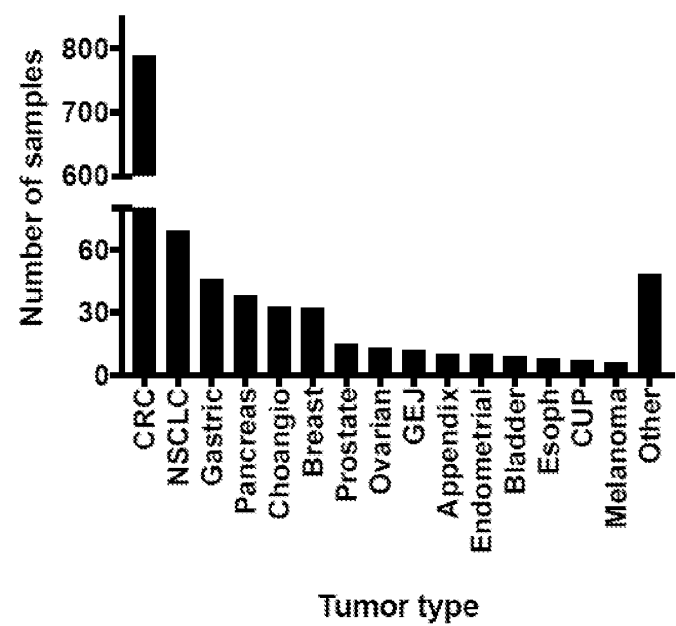


FIGURE 9

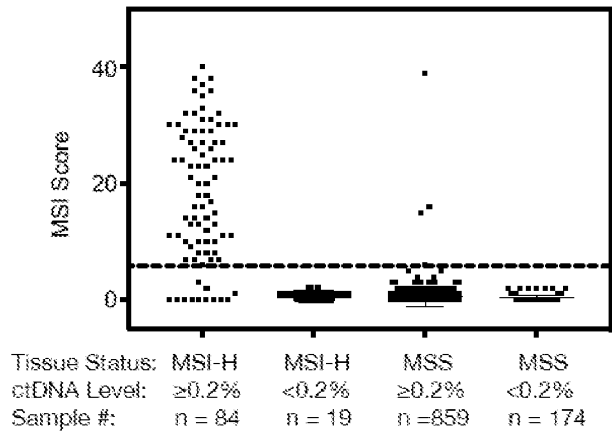


FIGURE 10A

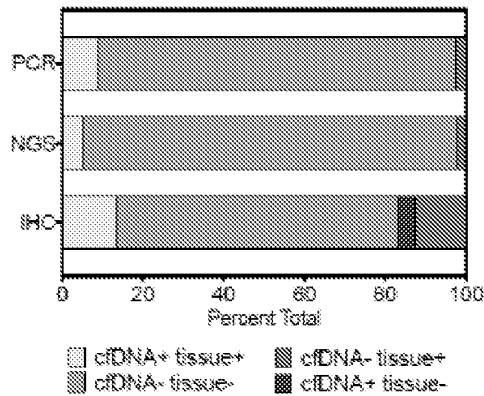


FIGURE 10B

Total Samples	1145
Unique Evaluable Patients	949
PPA	87% (71/82, 77-93%)
NPA	99.5% (863/867, 98.7-99.8%)
PPV	95% (71/75, 86-98%)
Accuracy	98.4% (934/949, 97.3-99.1%)

FIGURE 10C



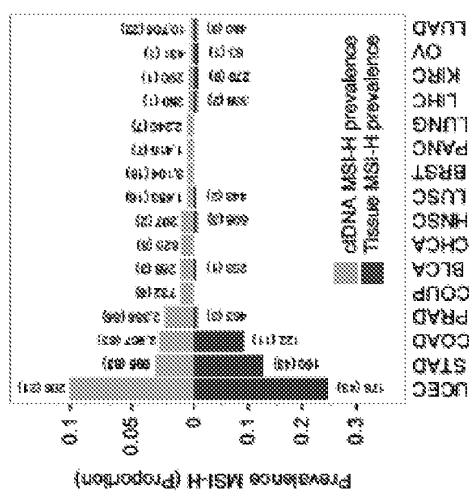


FIGURE 11B

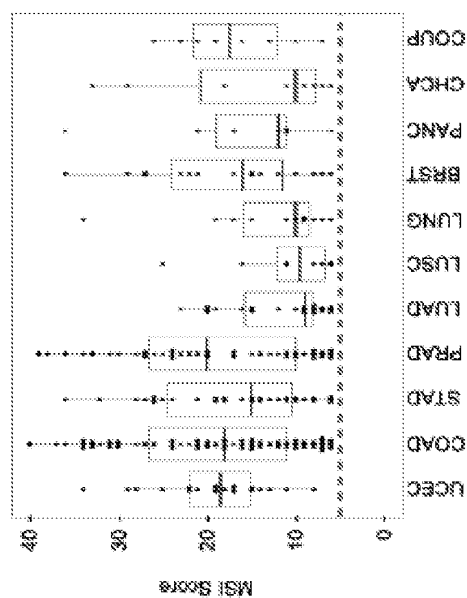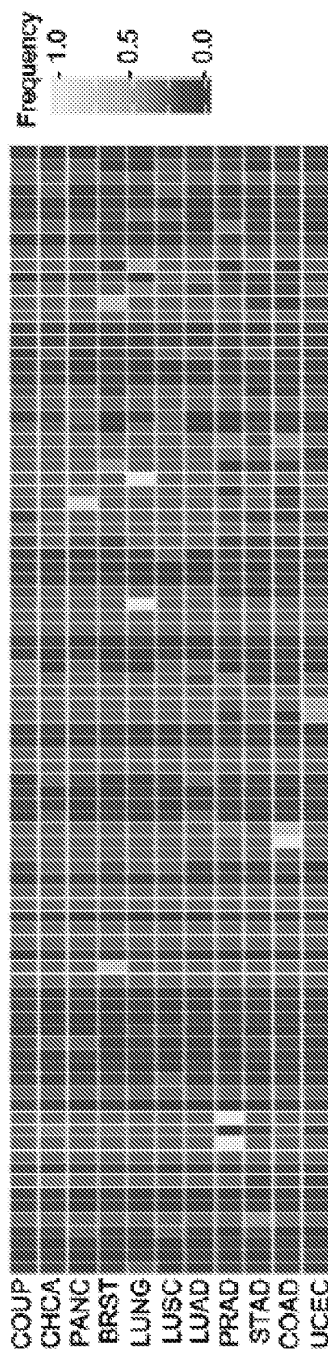

Microscopic Site

FIGURE 11C

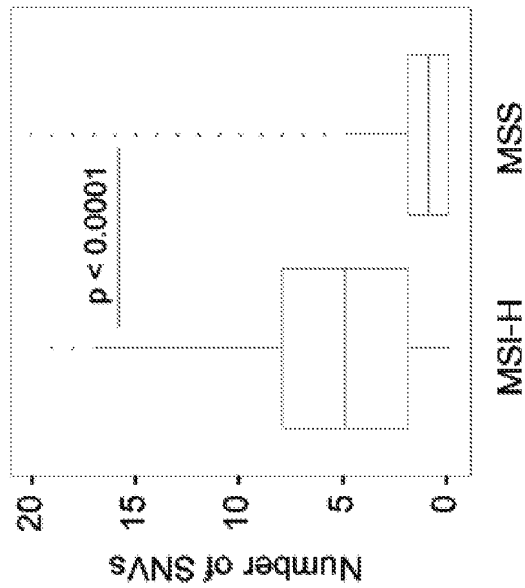


FIGURE 12A

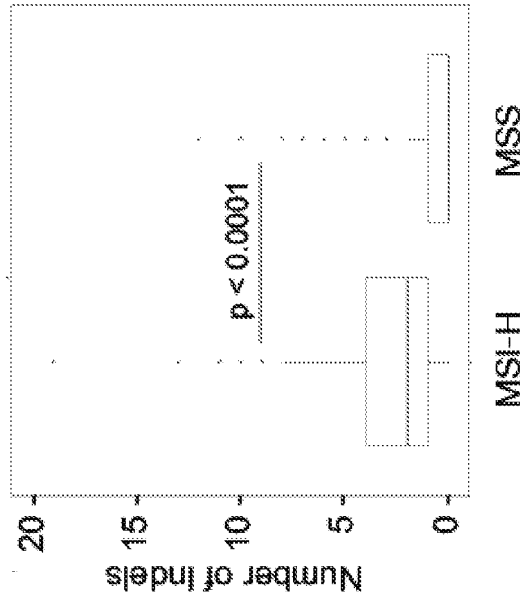


FIGURE 12B

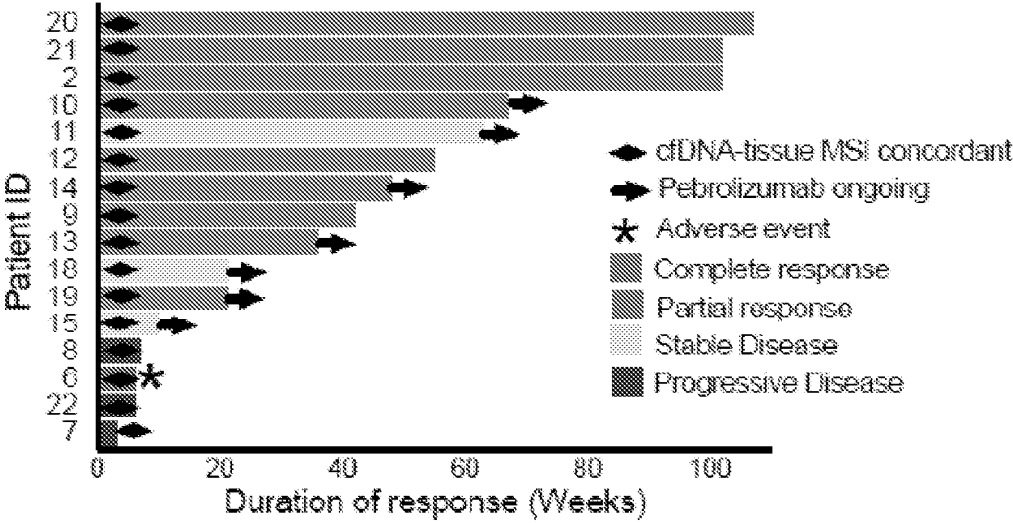


FIGURE 13A

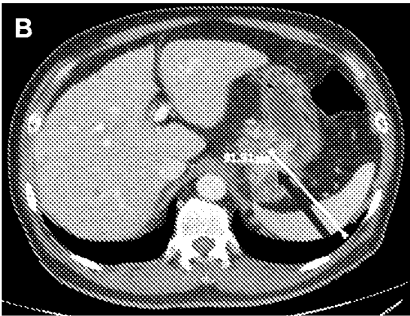


FIGURE 13B

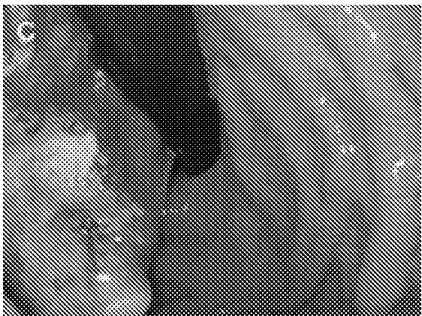


FIGURE 13C

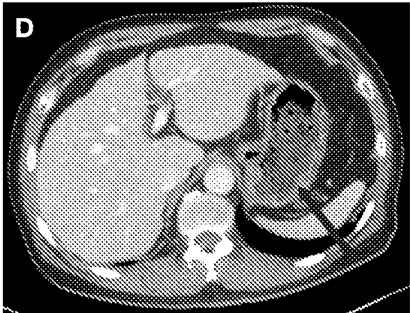


FIGURE 13D

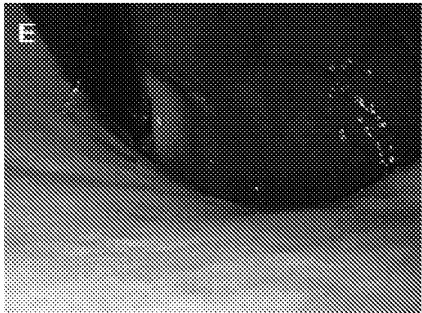


FIGURE 13E