

FIG. 1A

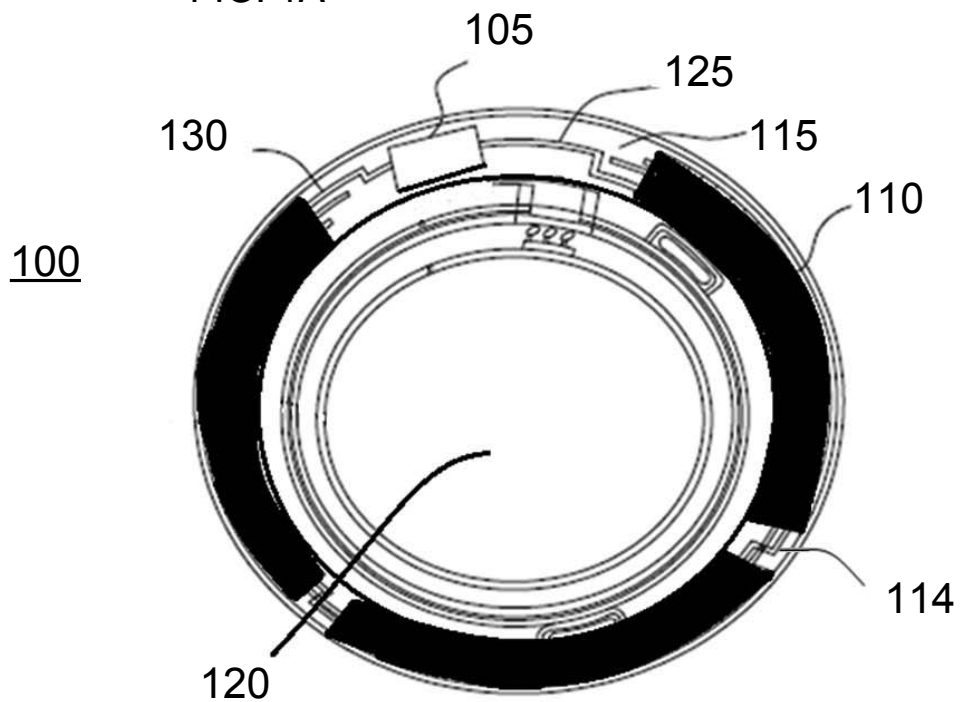
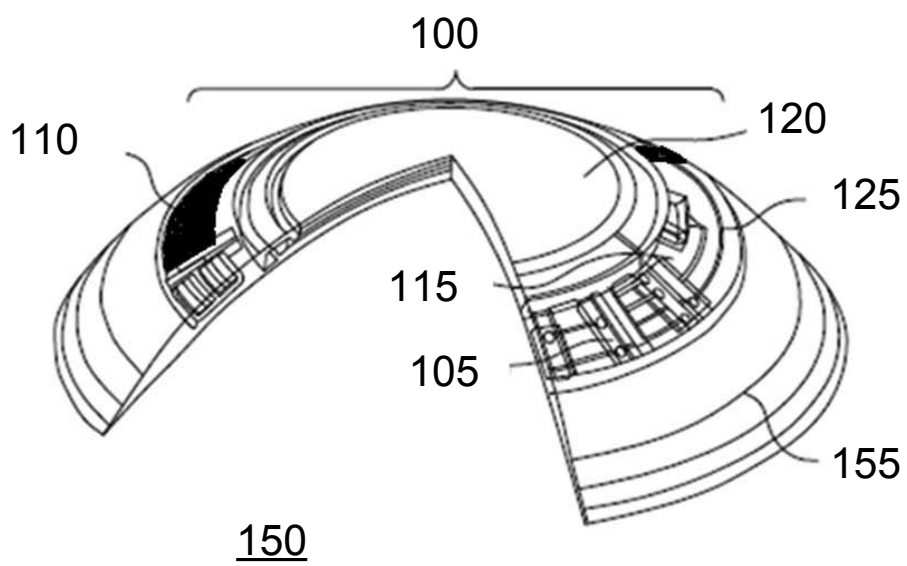


FIG. 1B

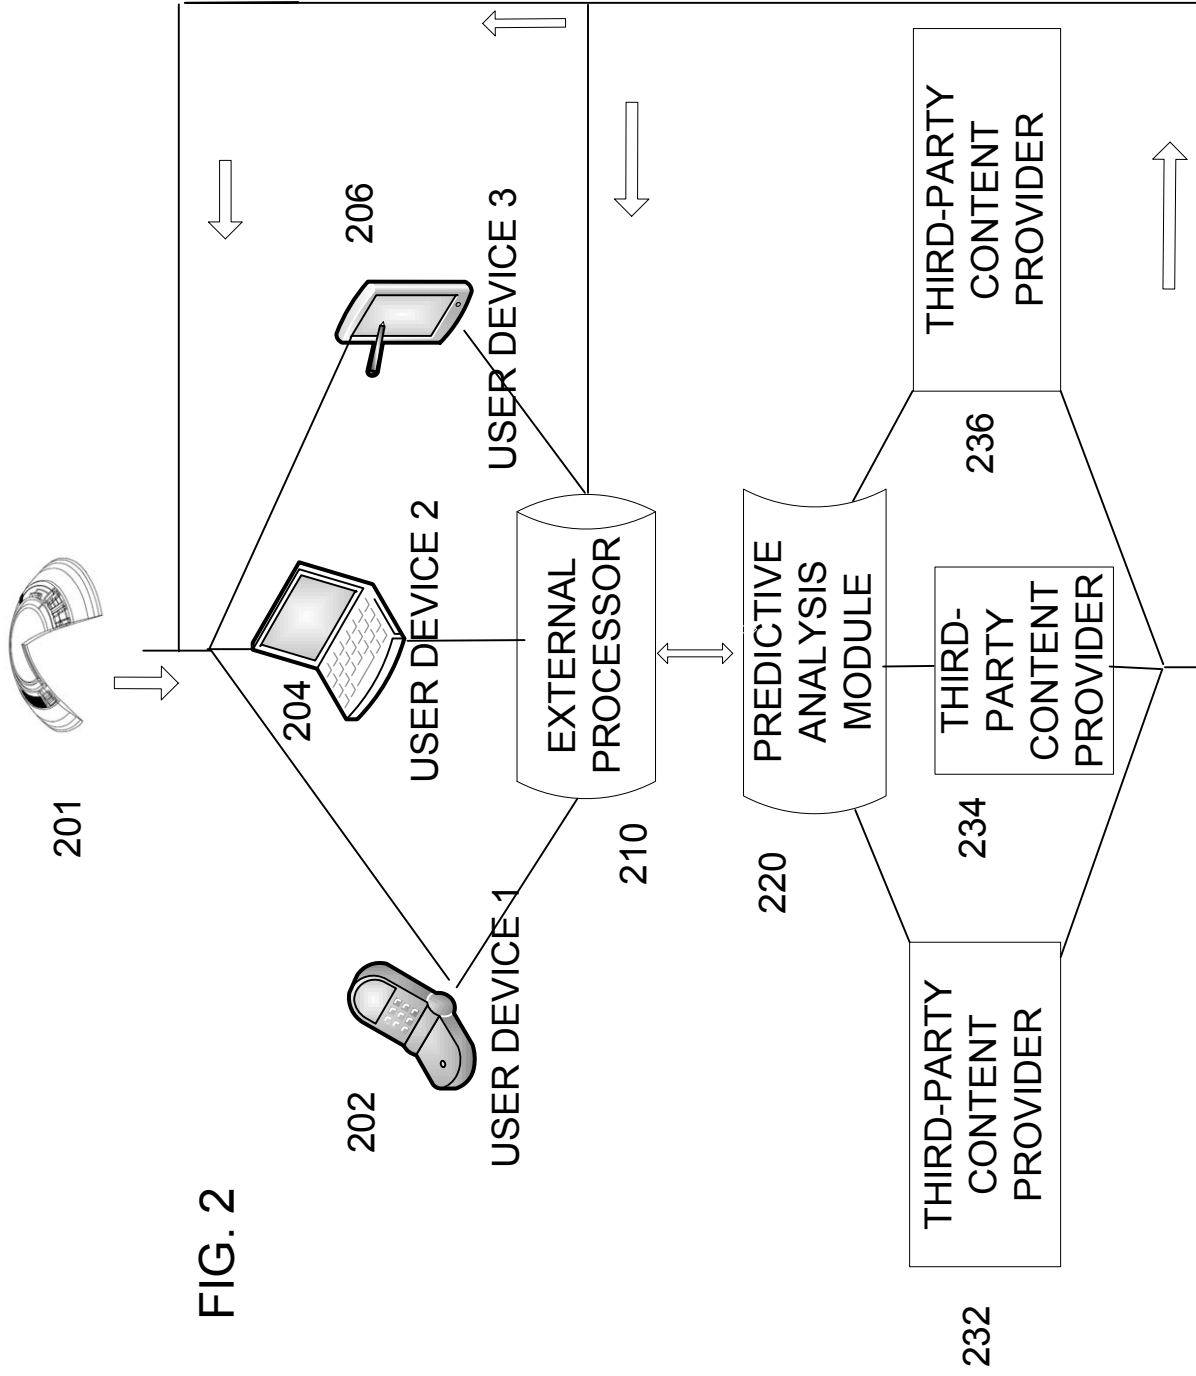
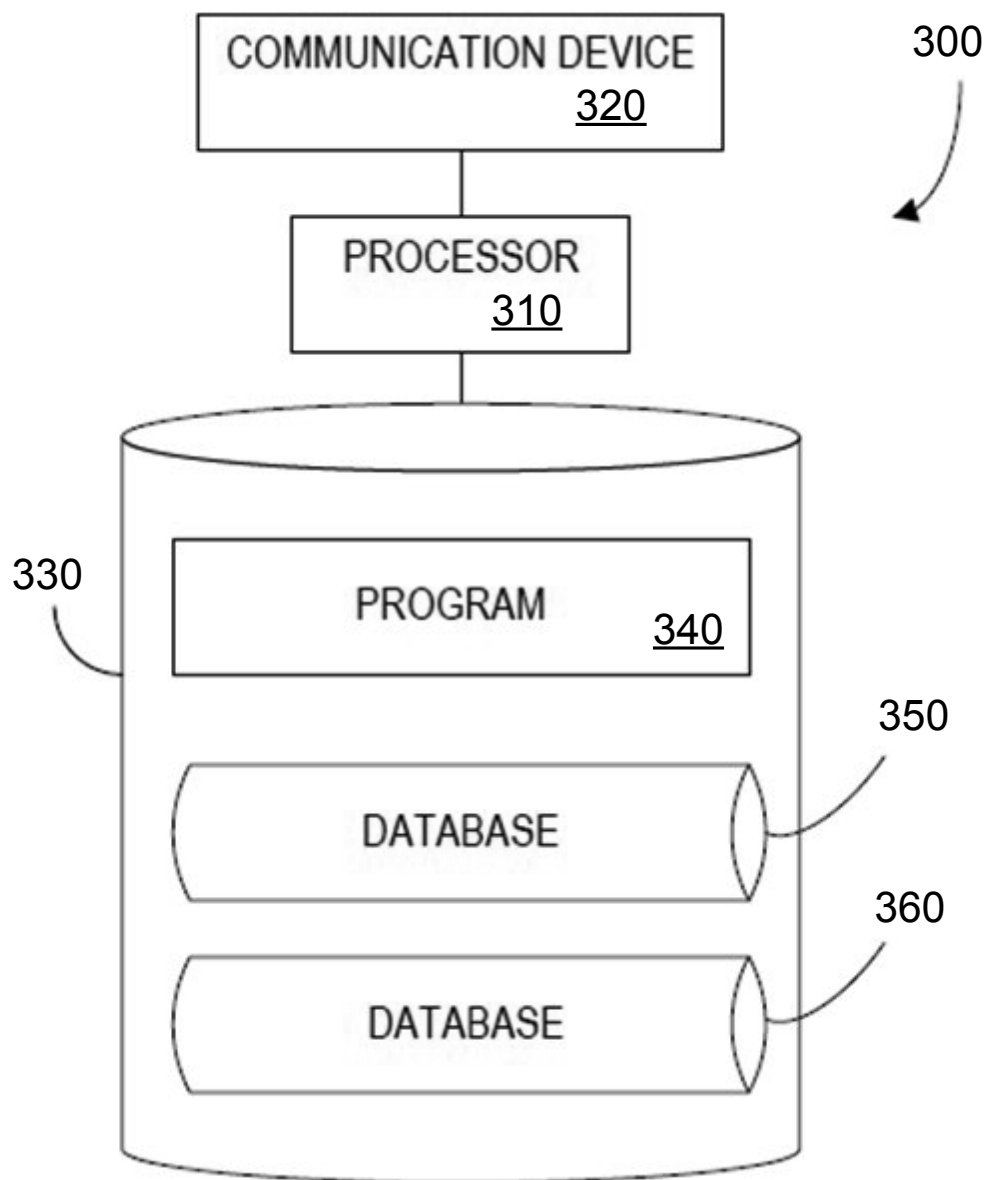


FIG. 3



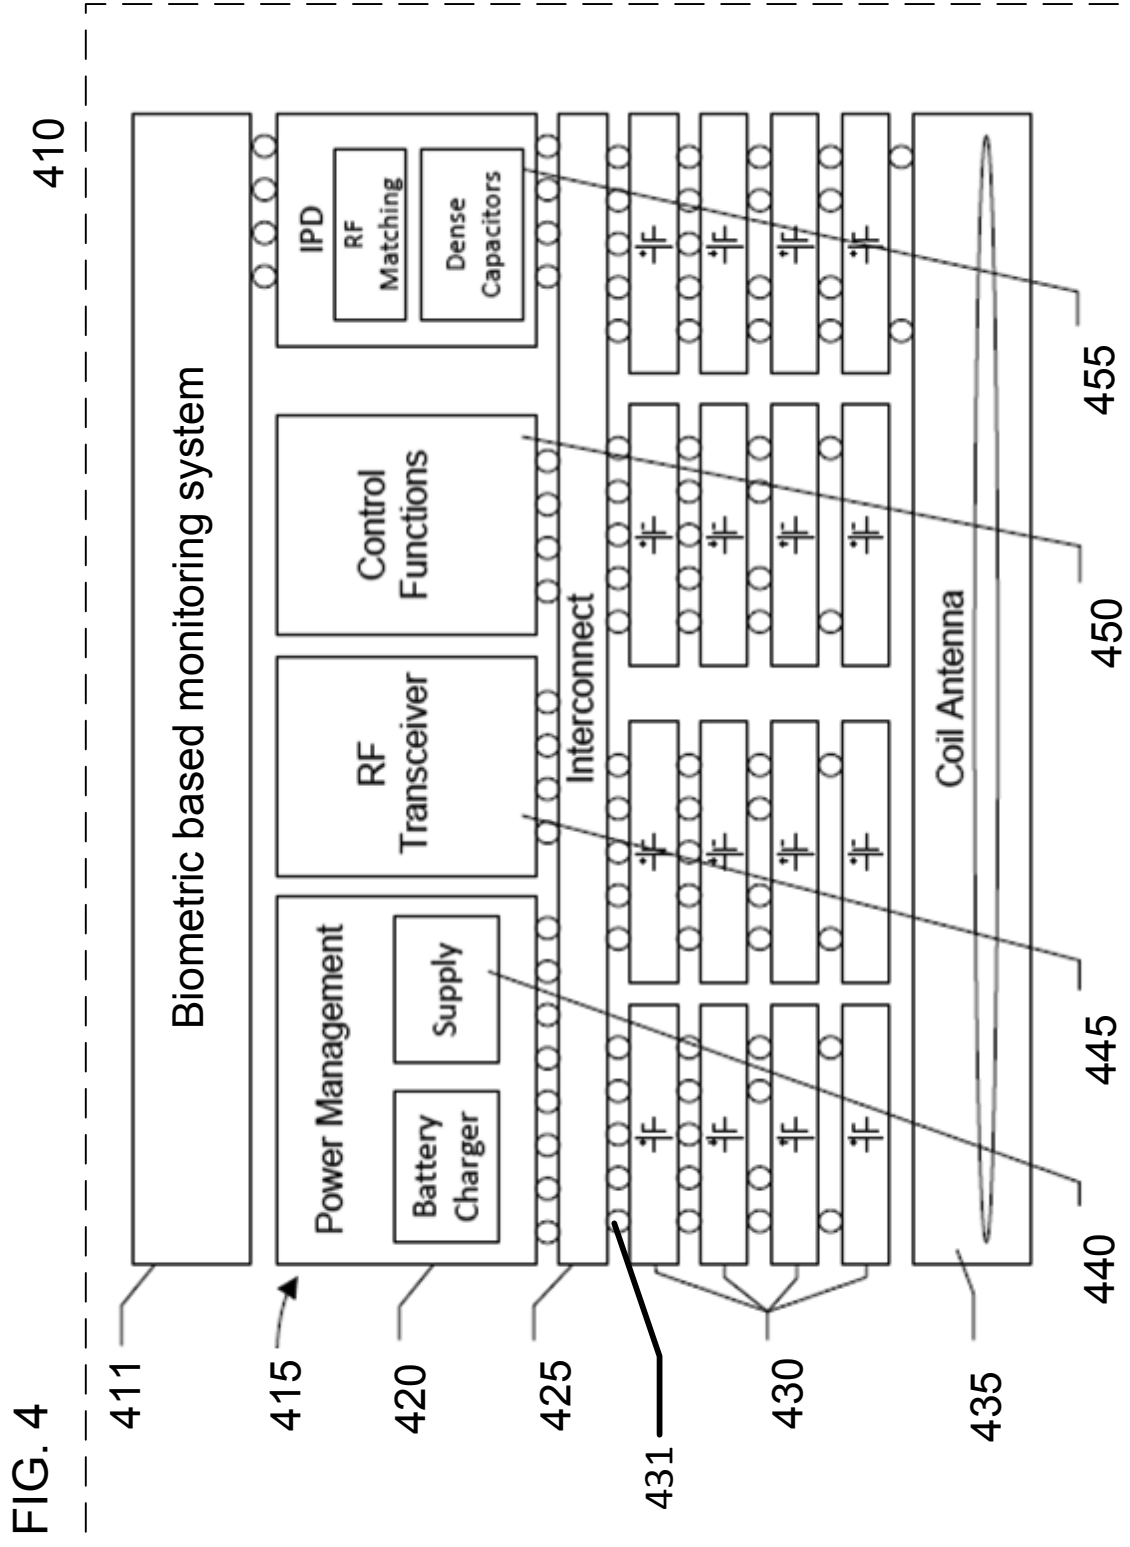


FIG. 5

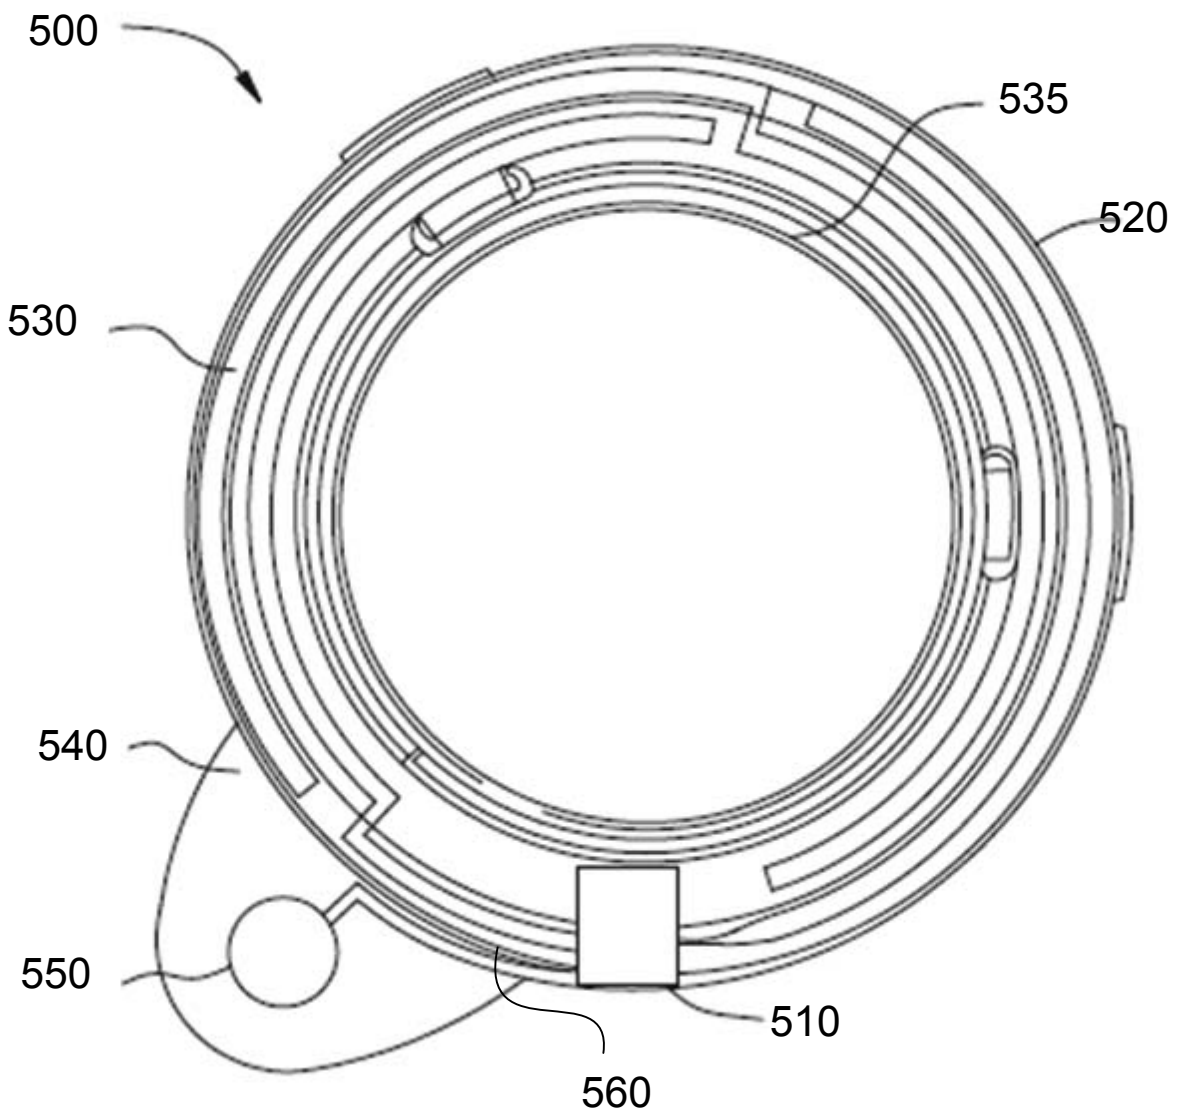


FIG. 6A

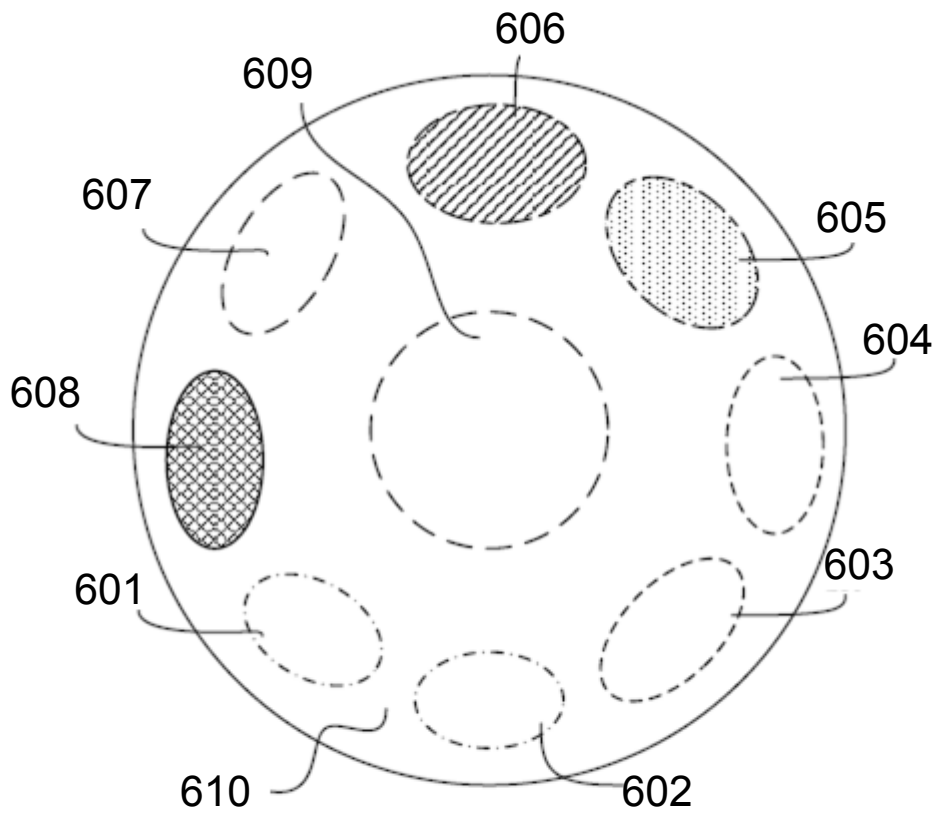


FIG. 6B

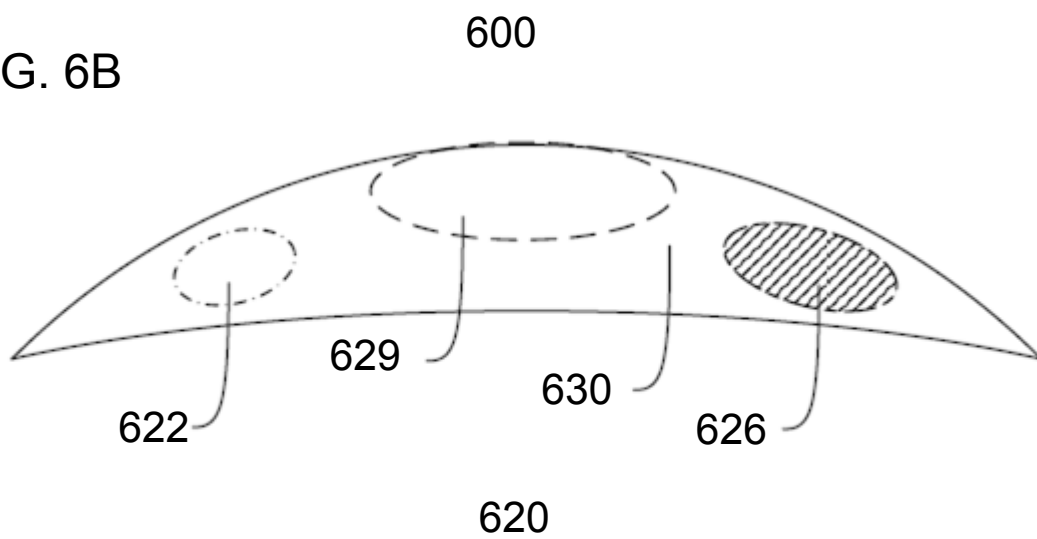


Fig. 7A

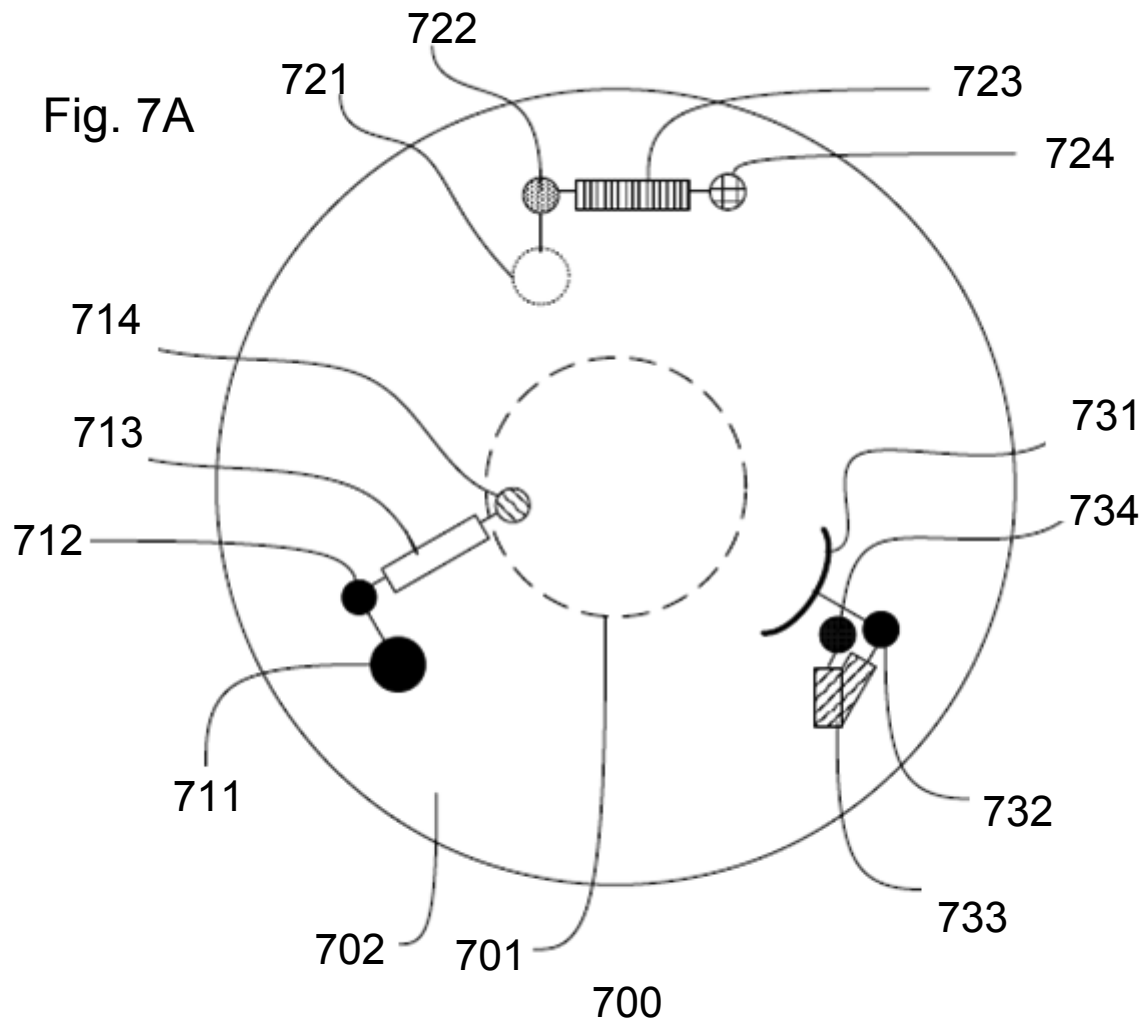


Fig. 7B

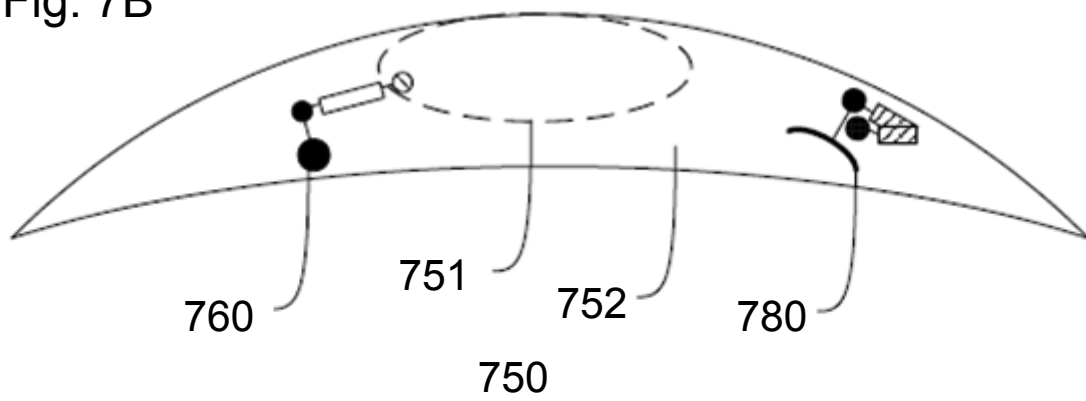
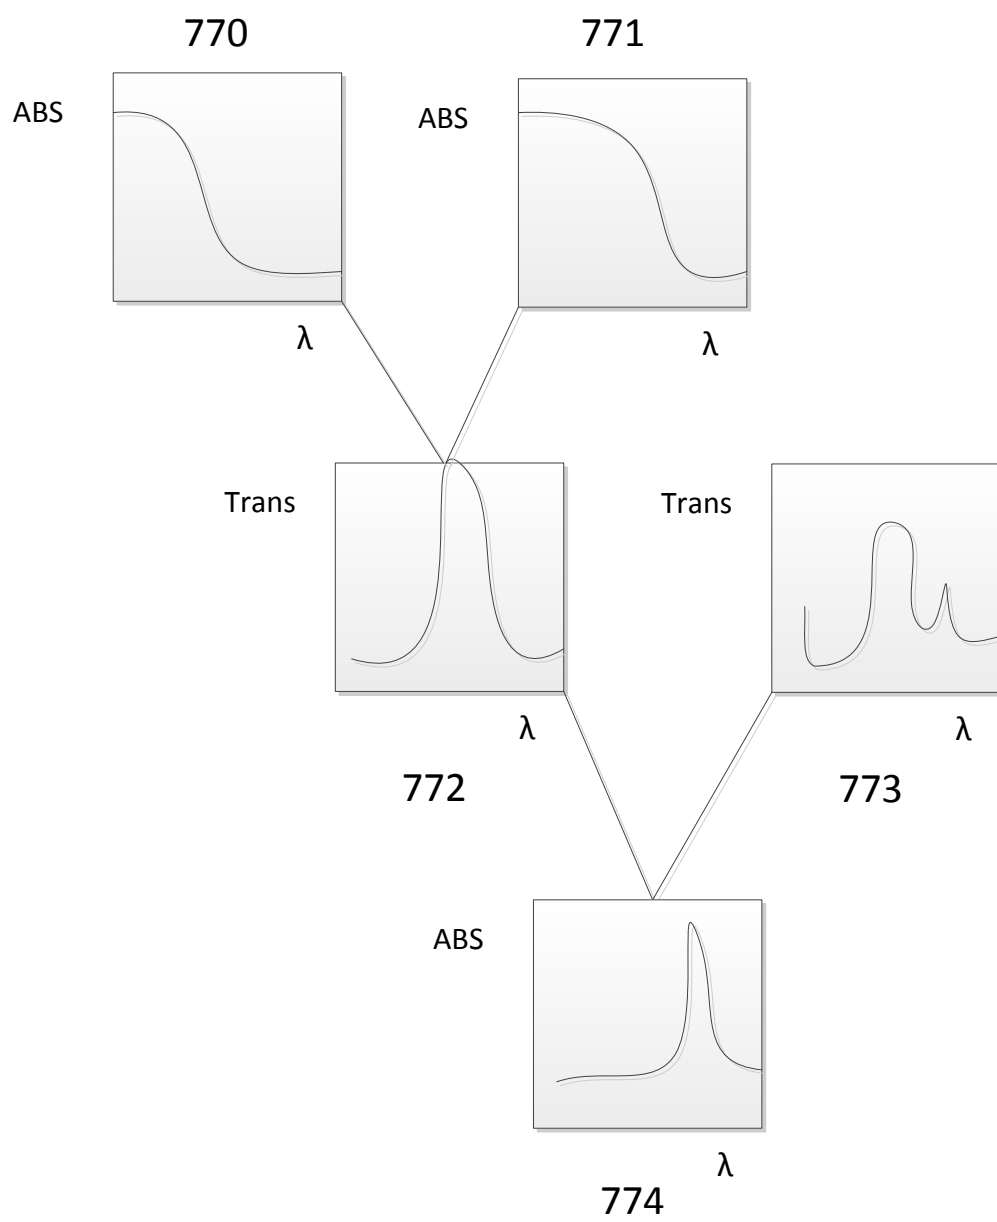


Fig. 7C



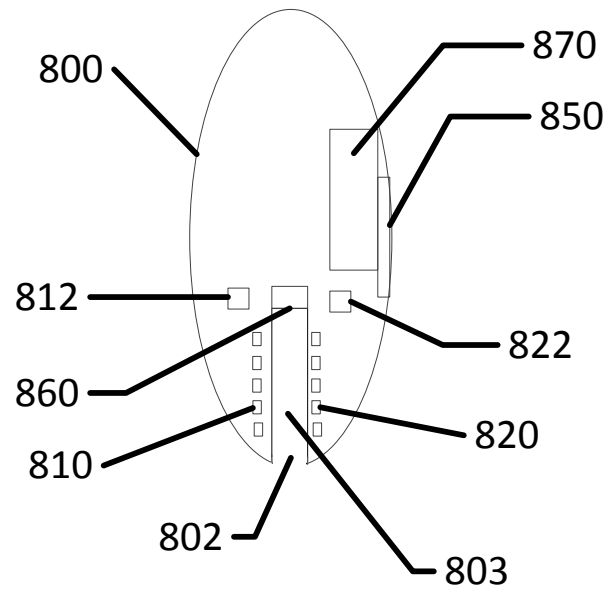


FIG. 8A

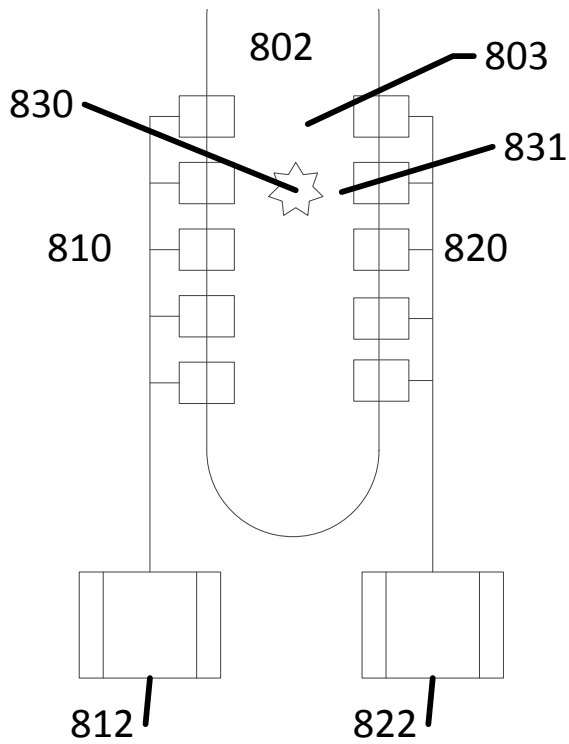


FIG. 8B

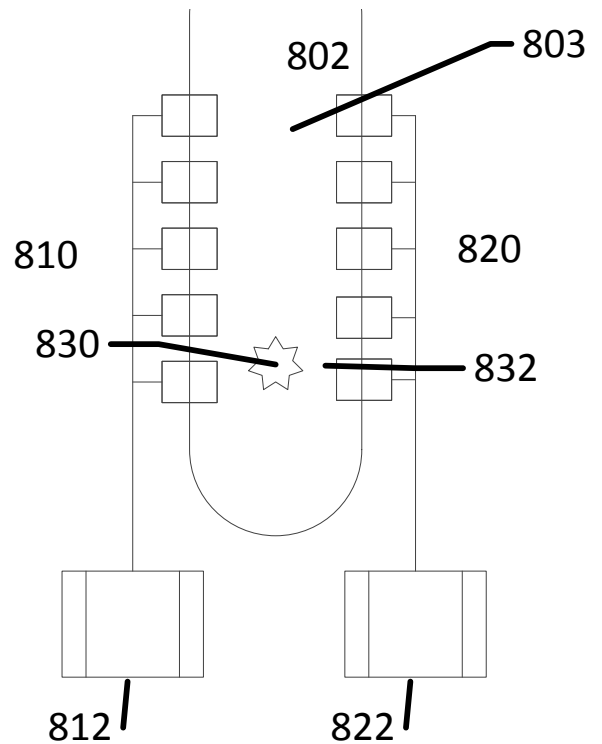


FIG. 8C

FIG. 9A

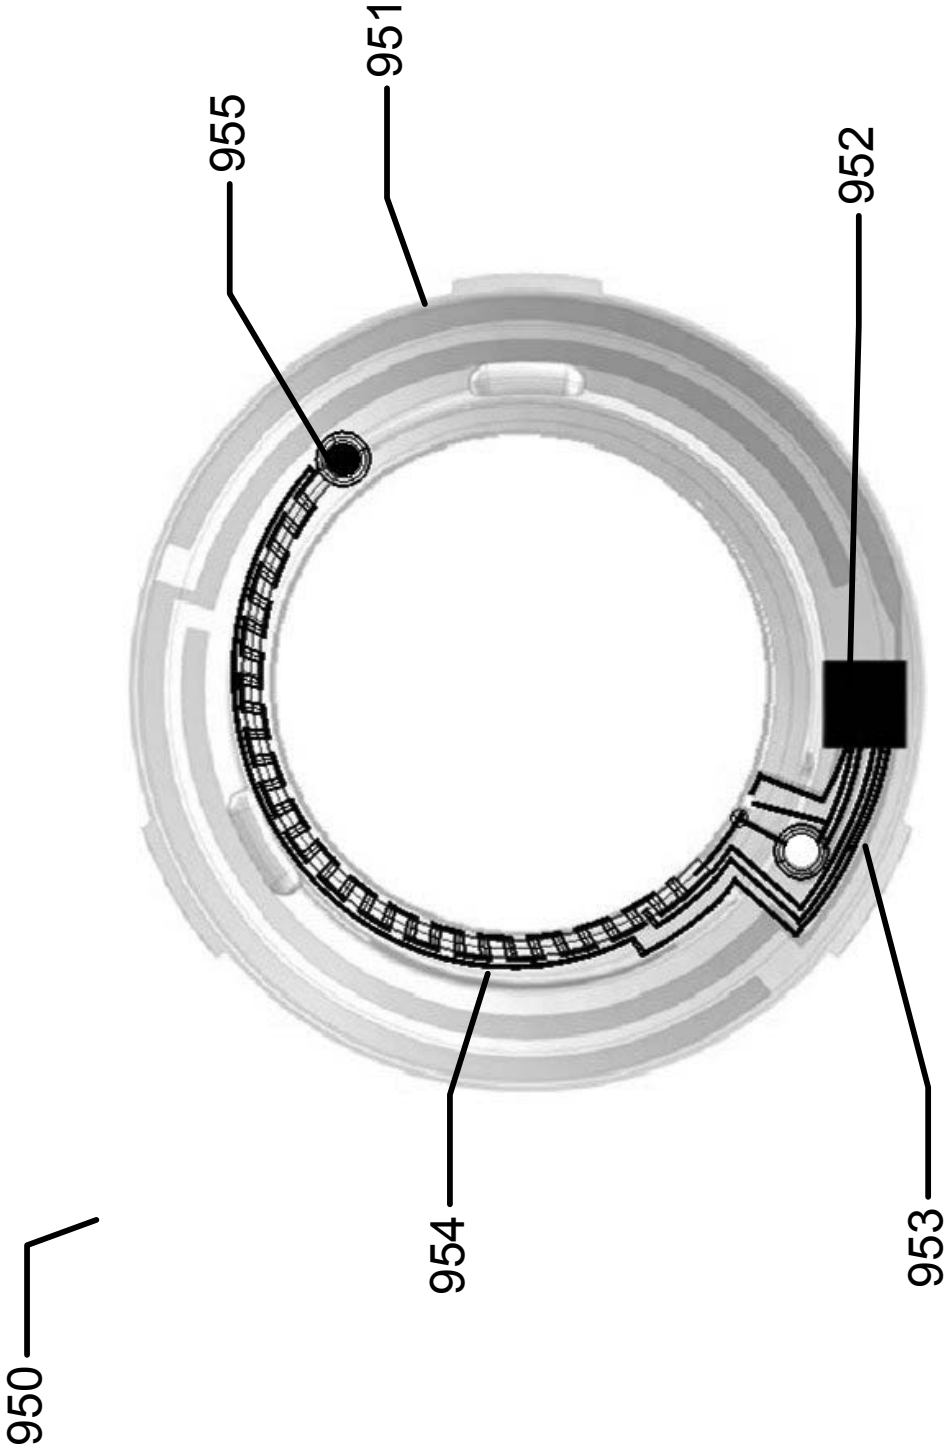
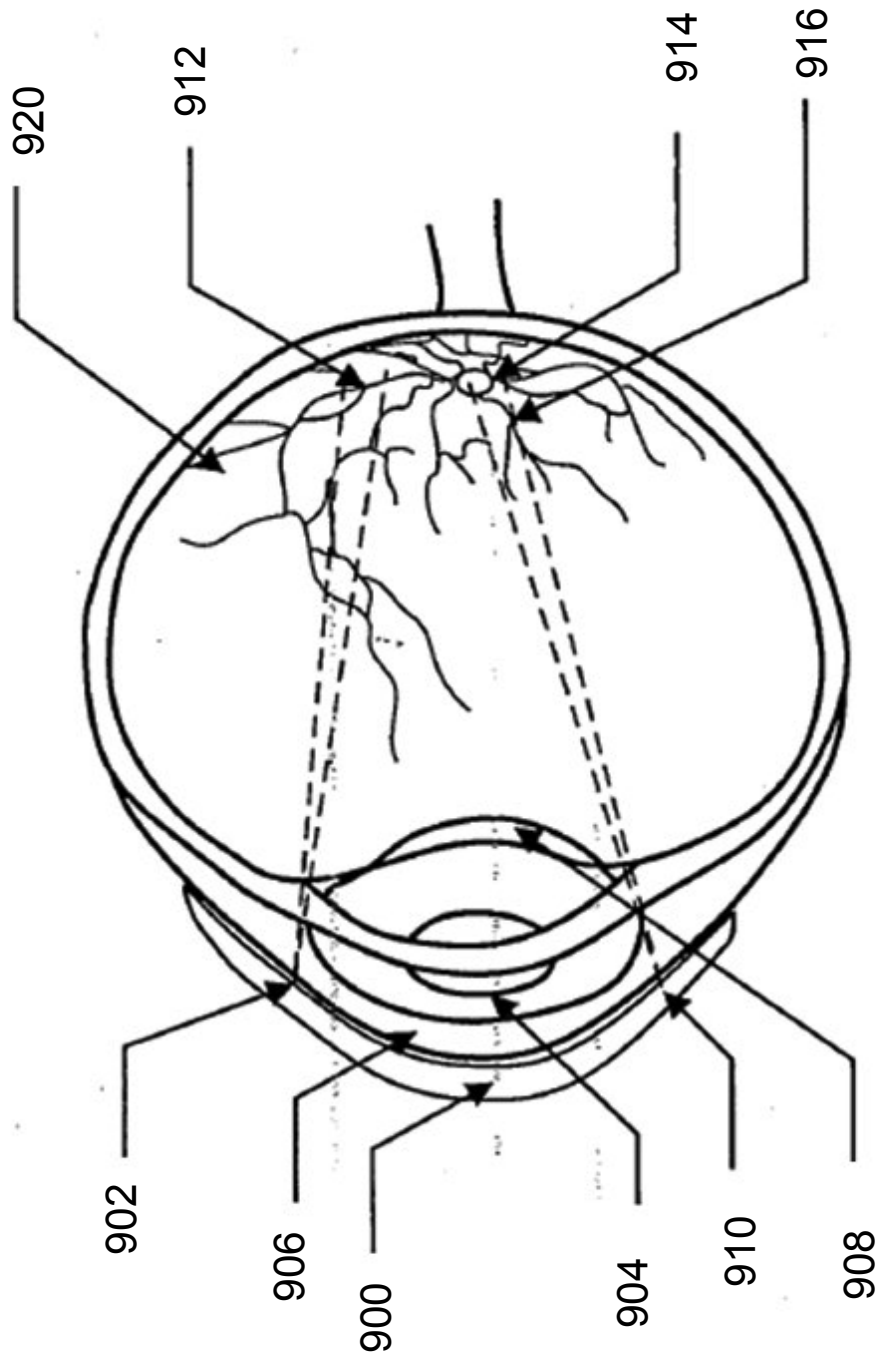


FIG. 9B



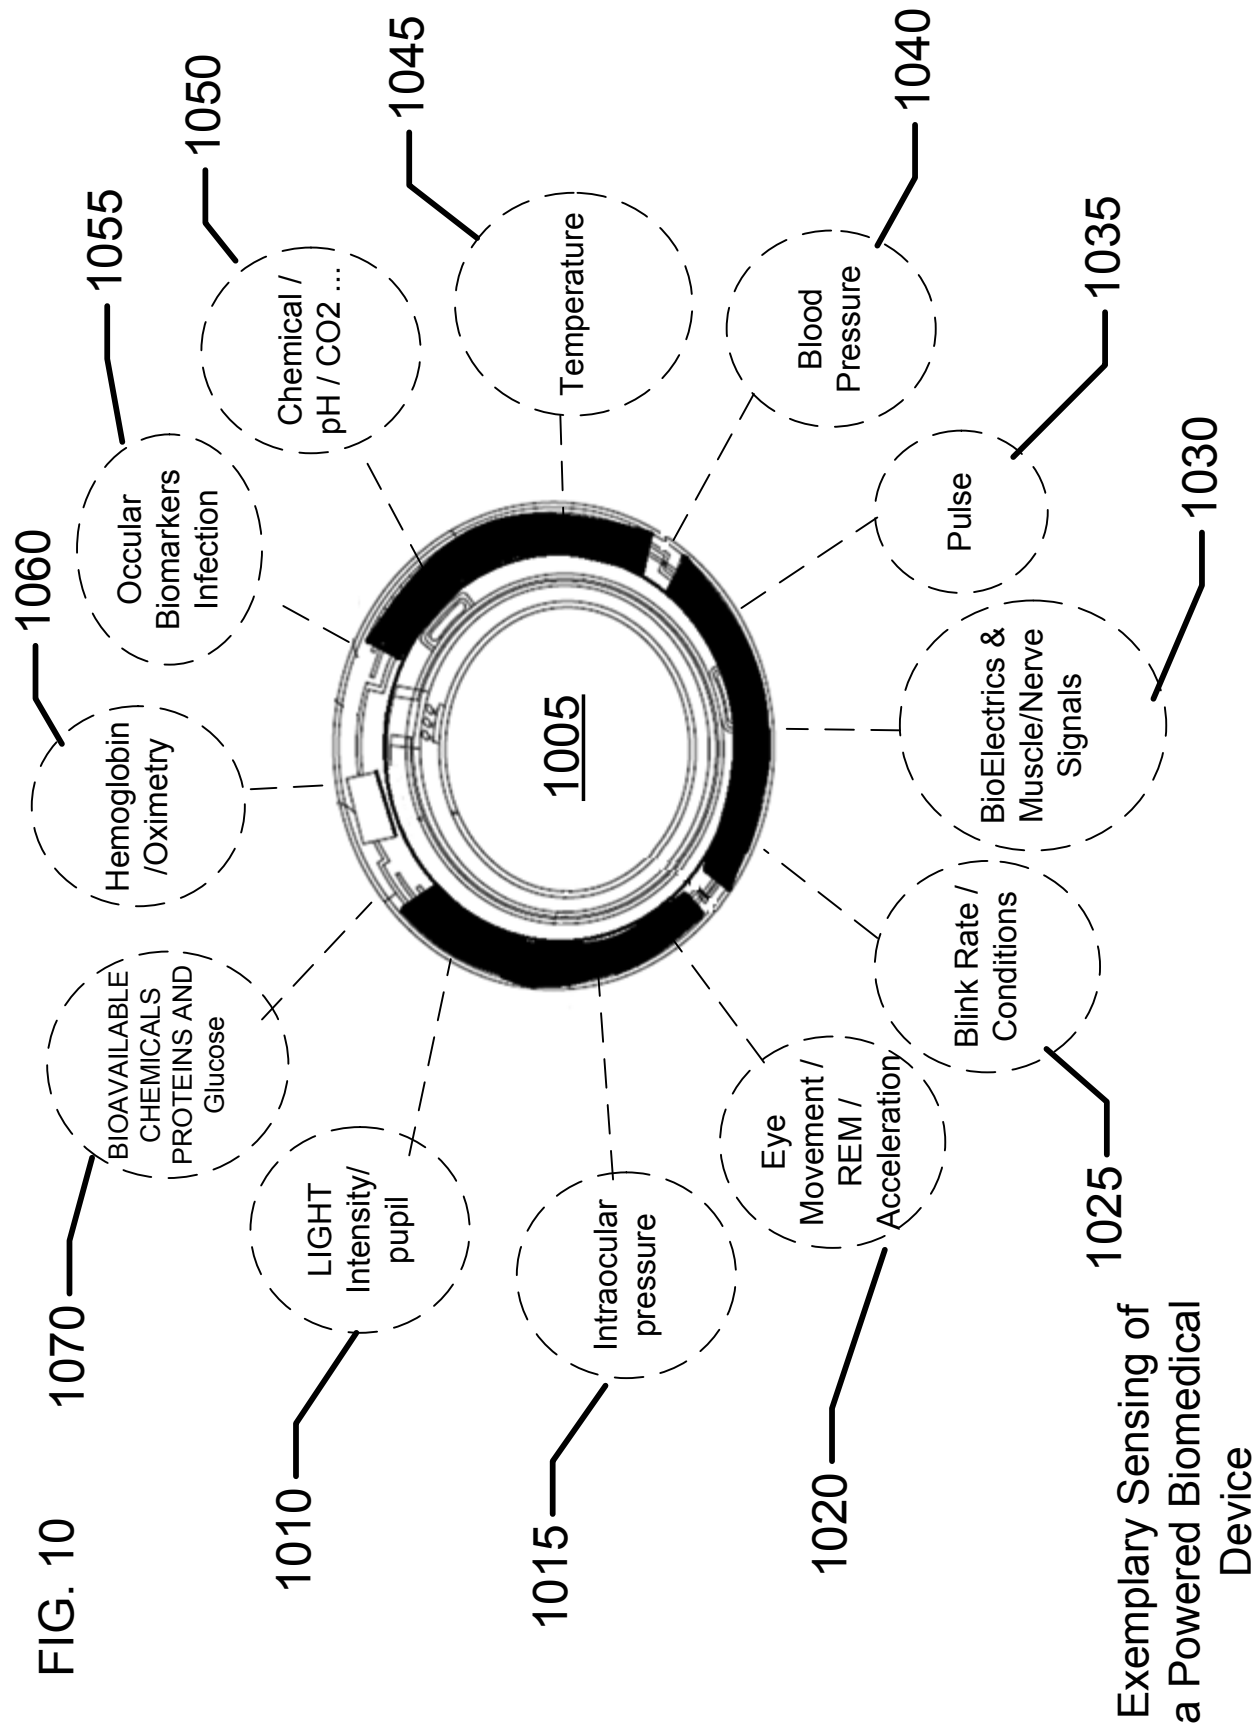


FIG. 10

Exemplary Sensing of  
a Powered Biomedical  
Device

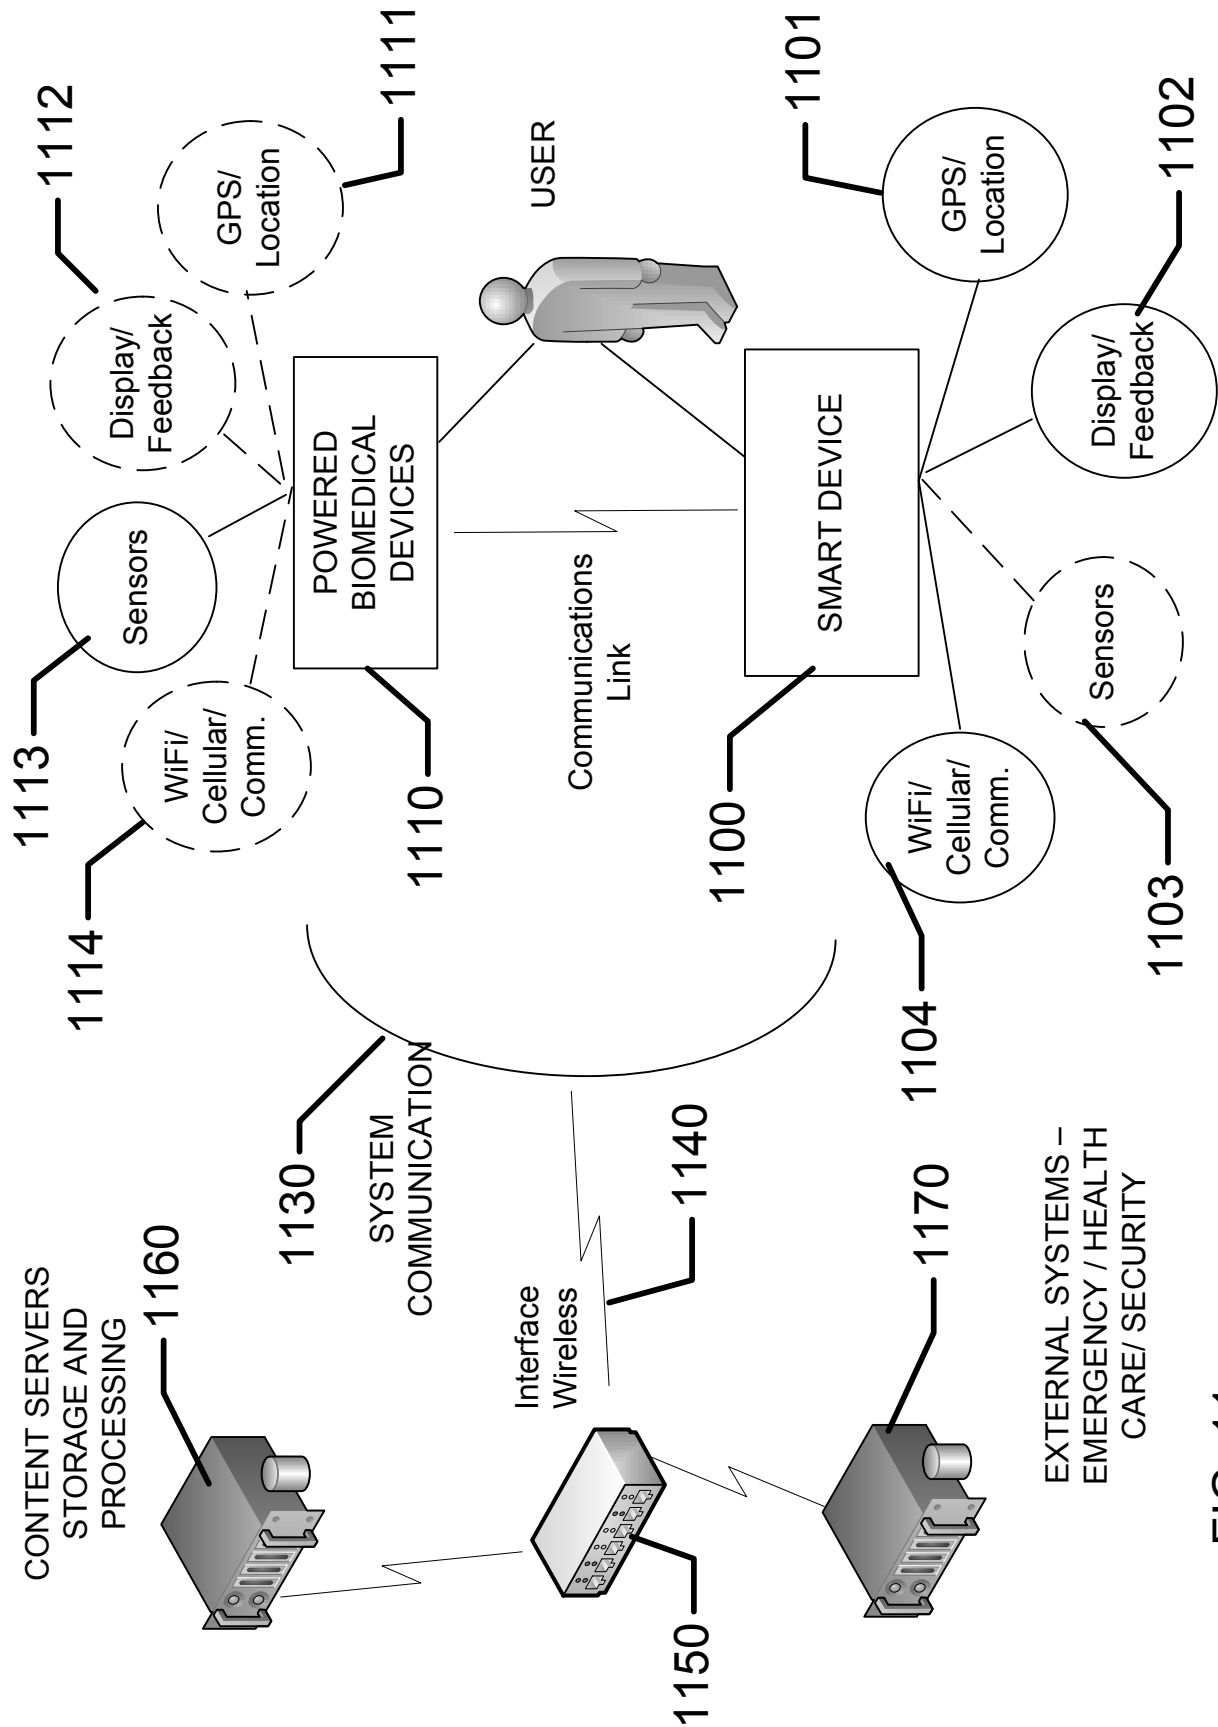


FIG. 11



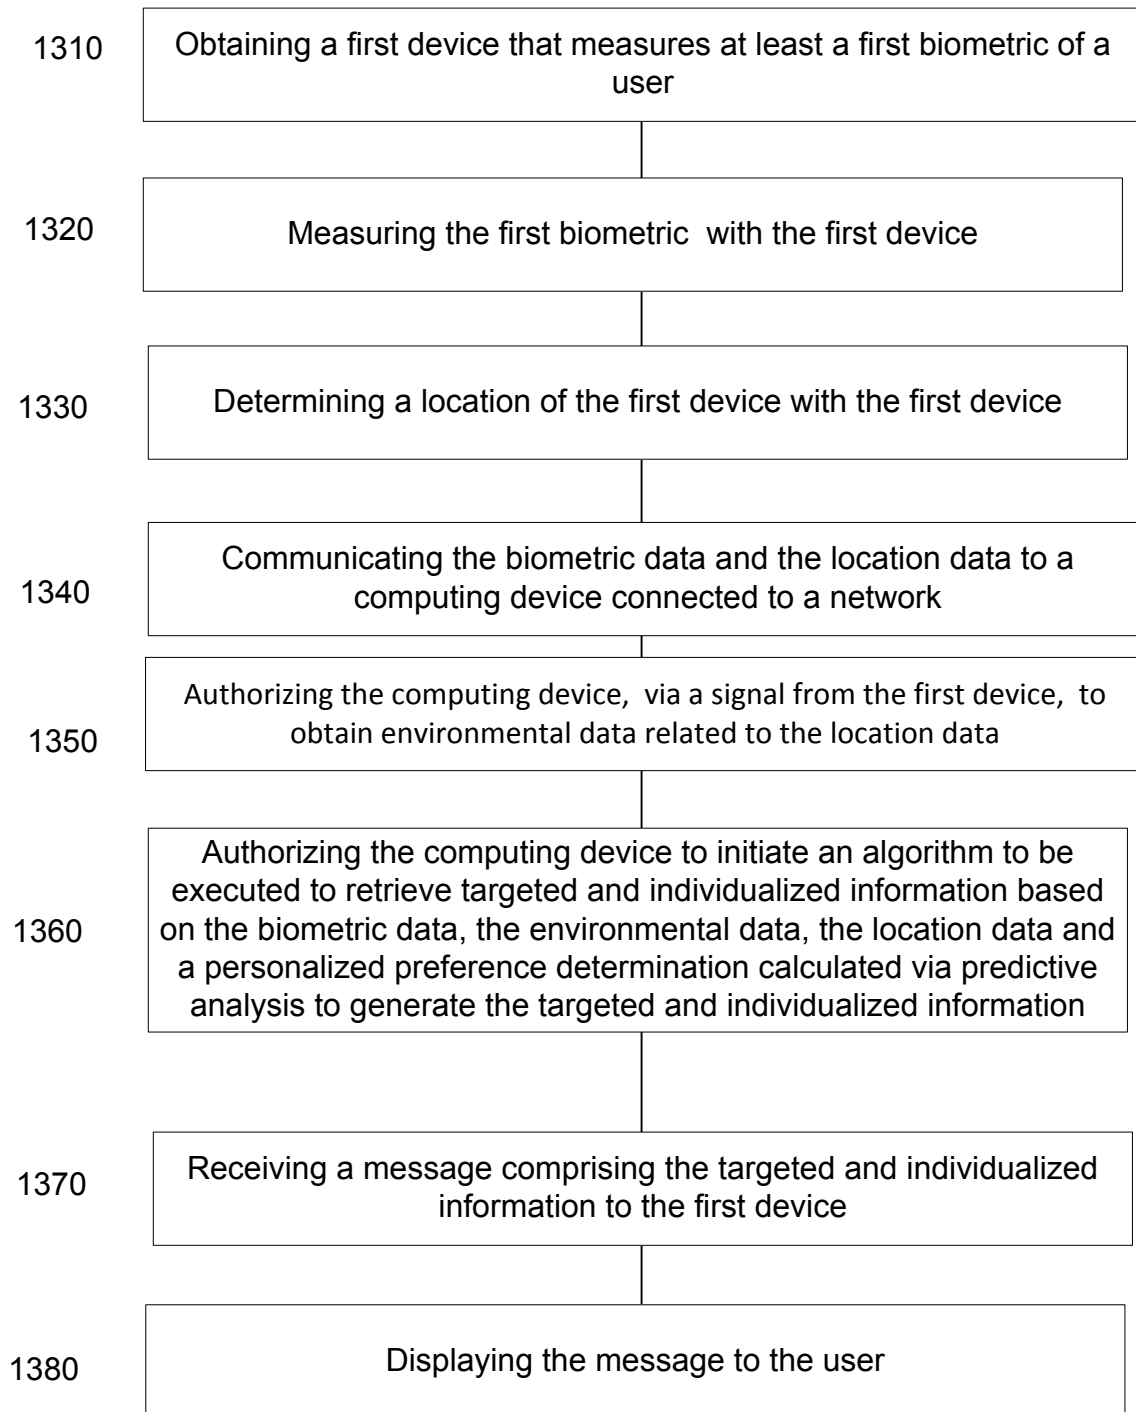


FIG. 13

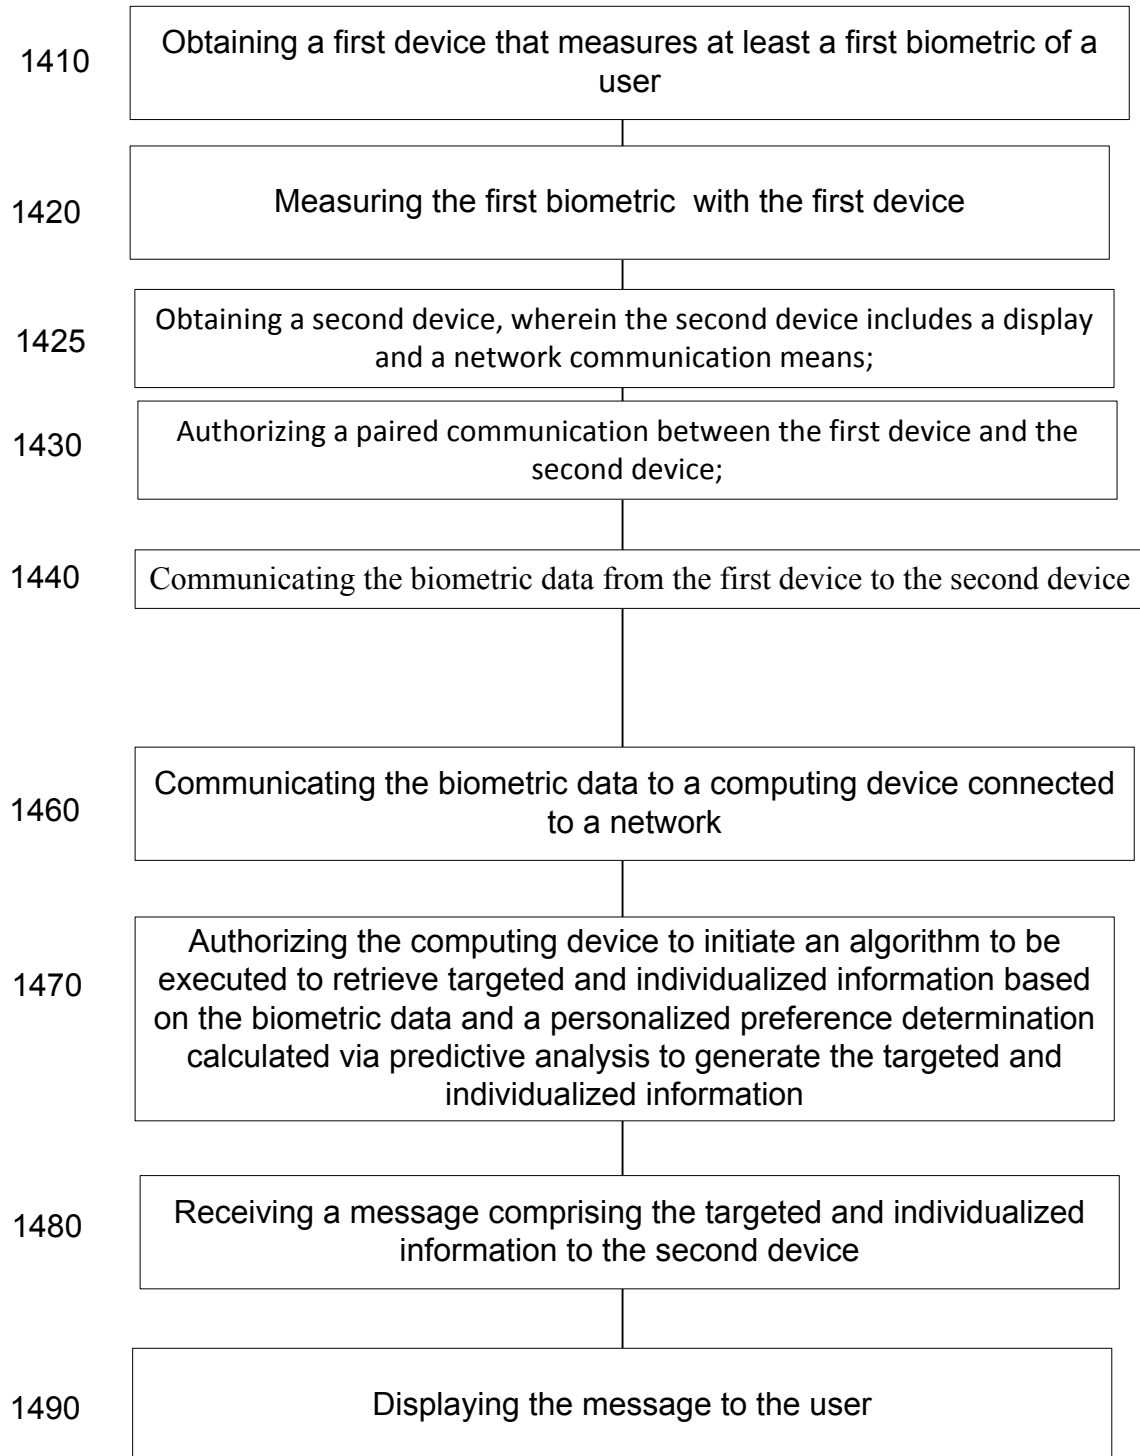


FIG. 14

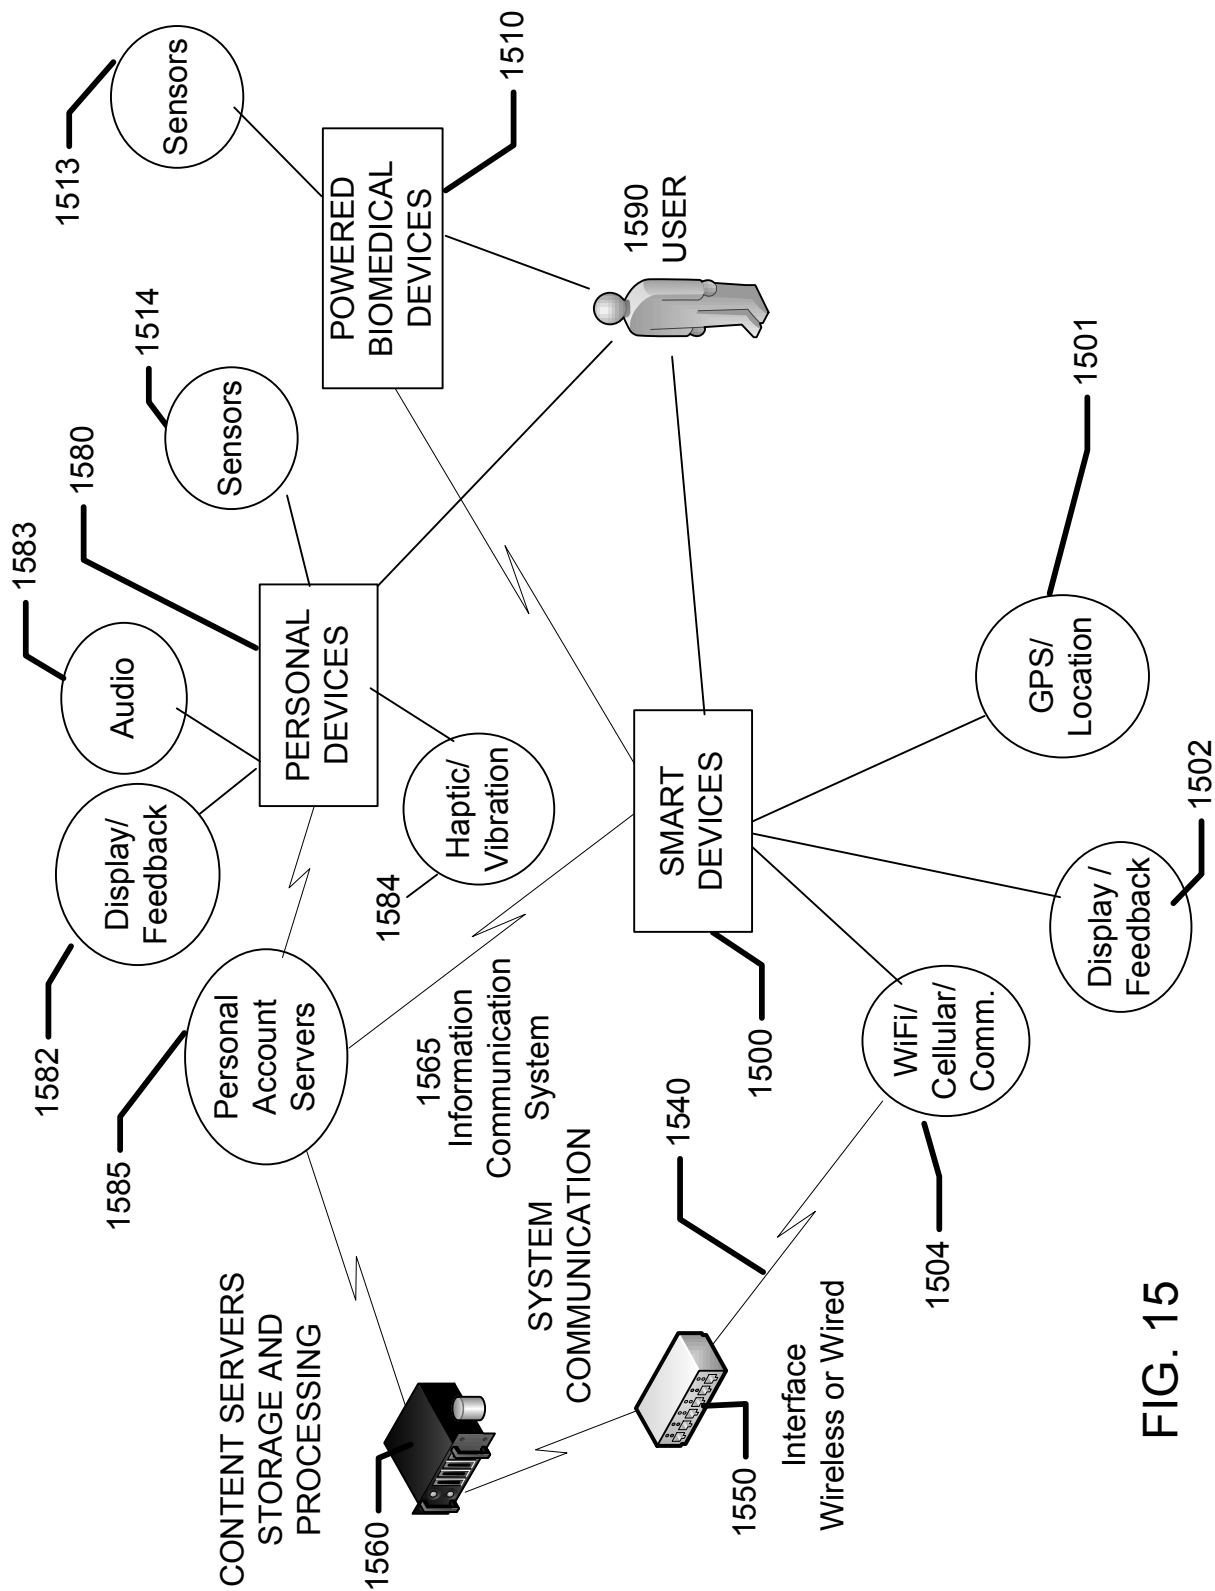


FIG. 15

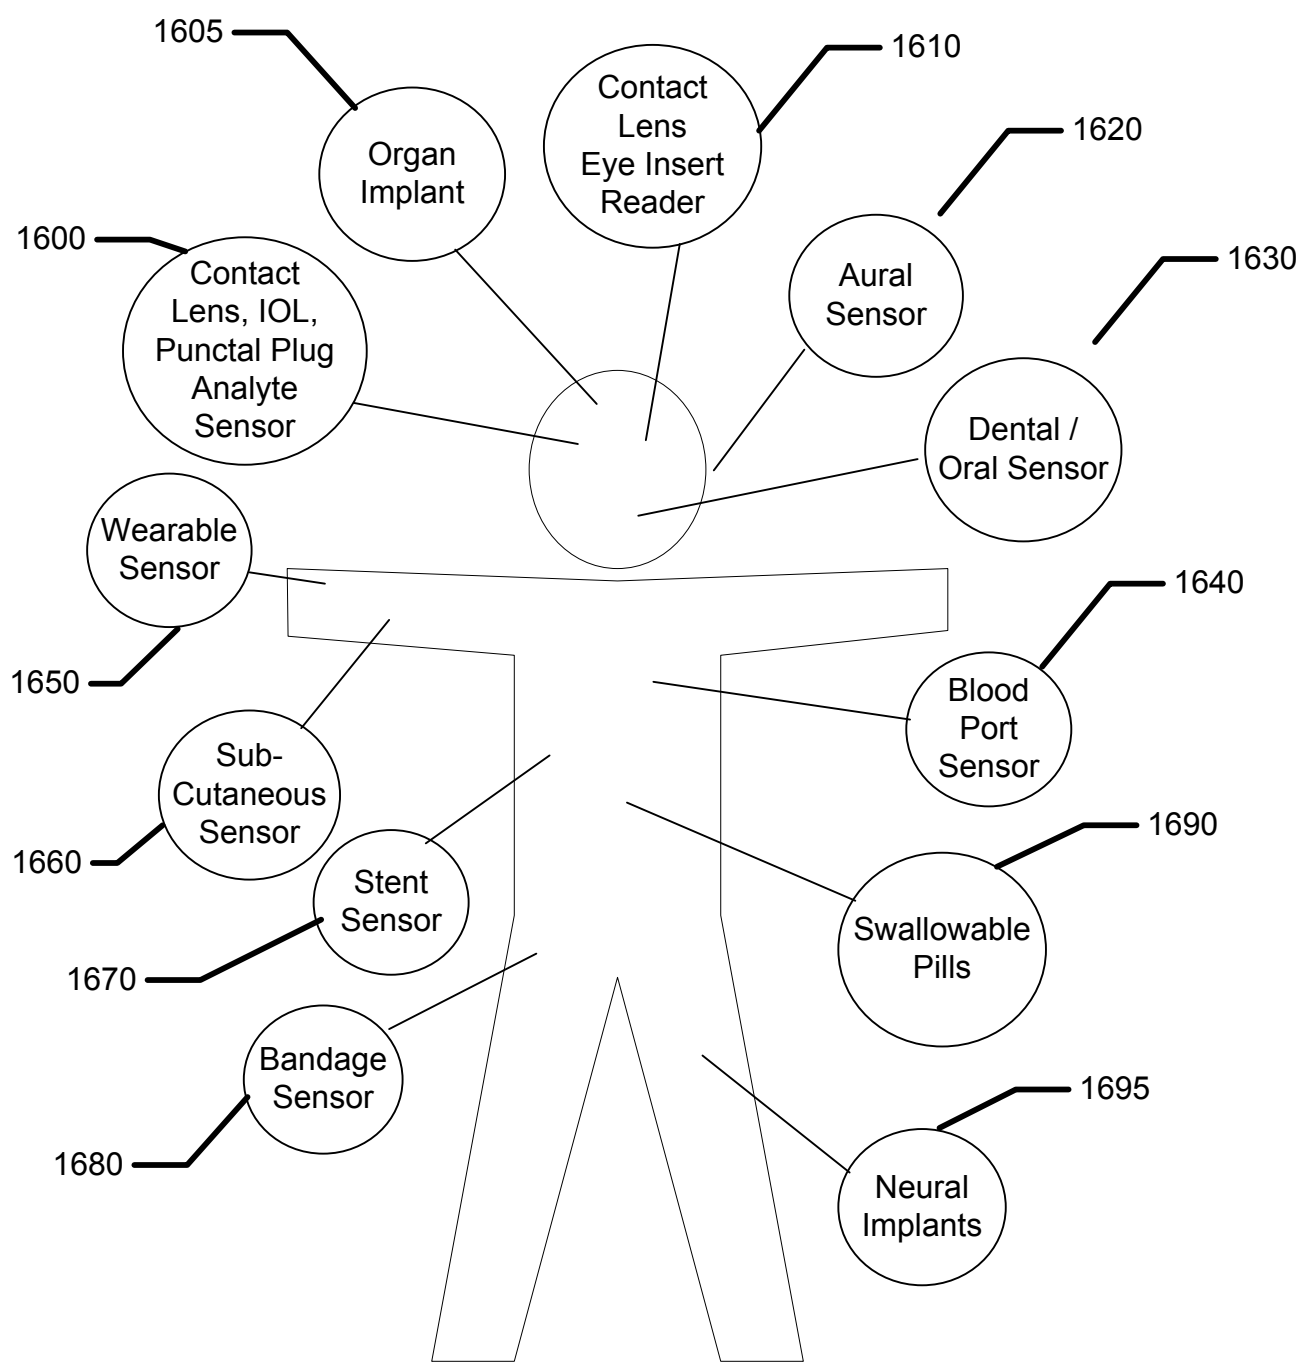


FIG. 16

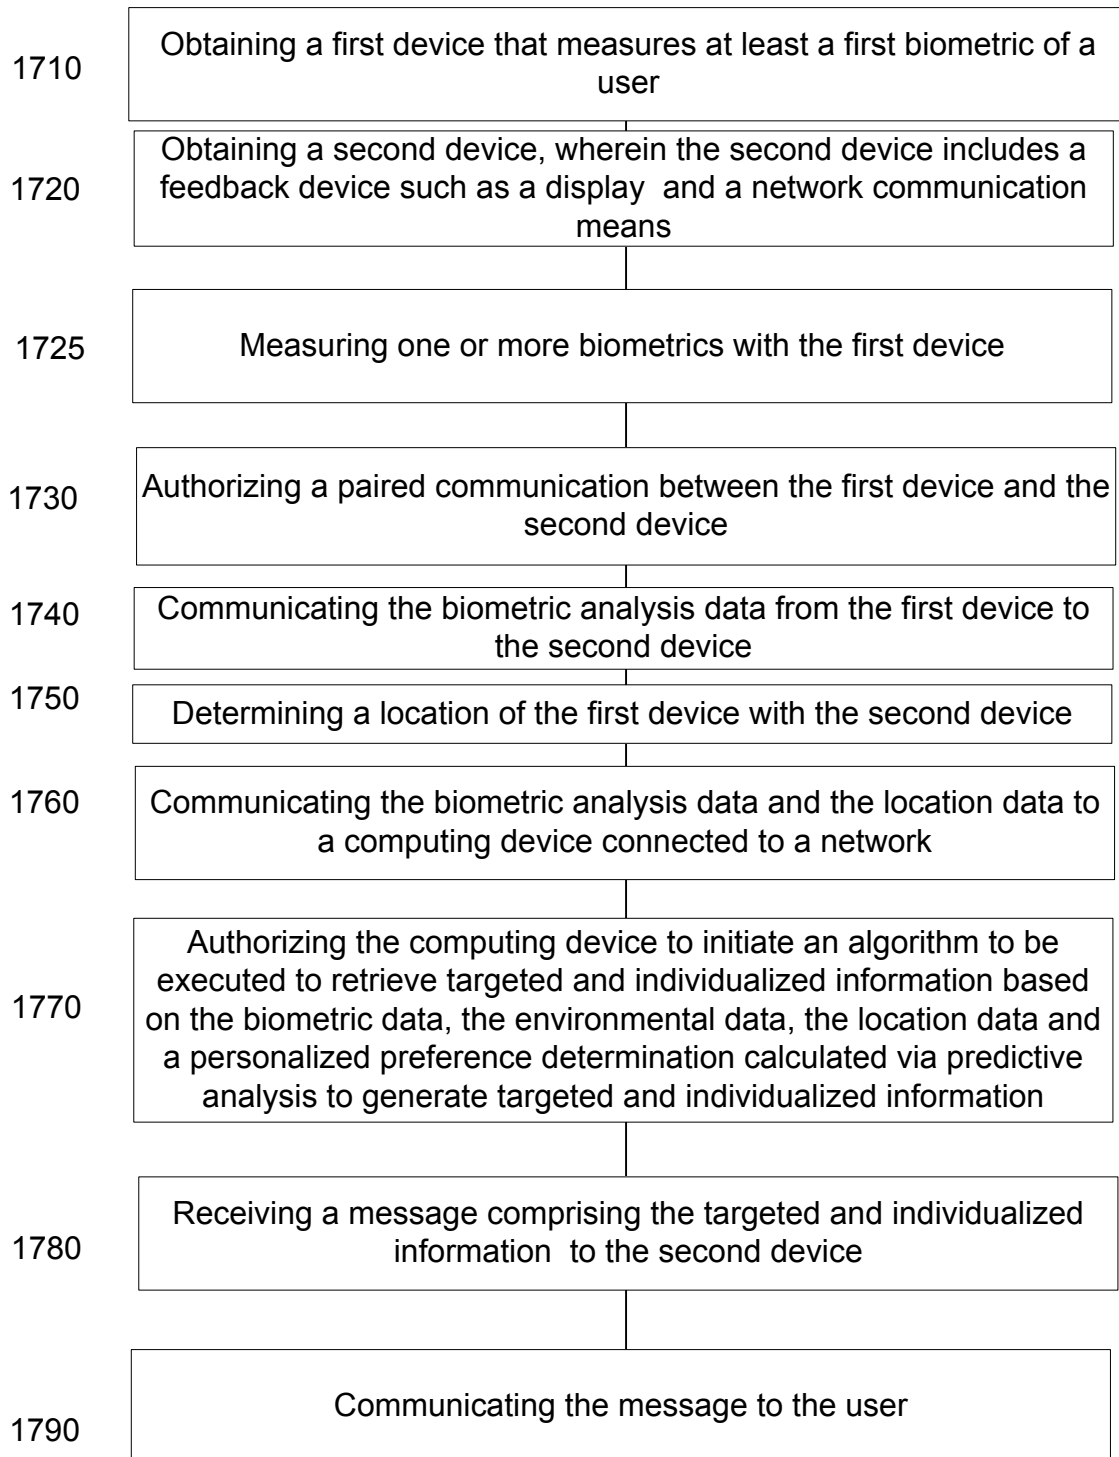


FIG. 17

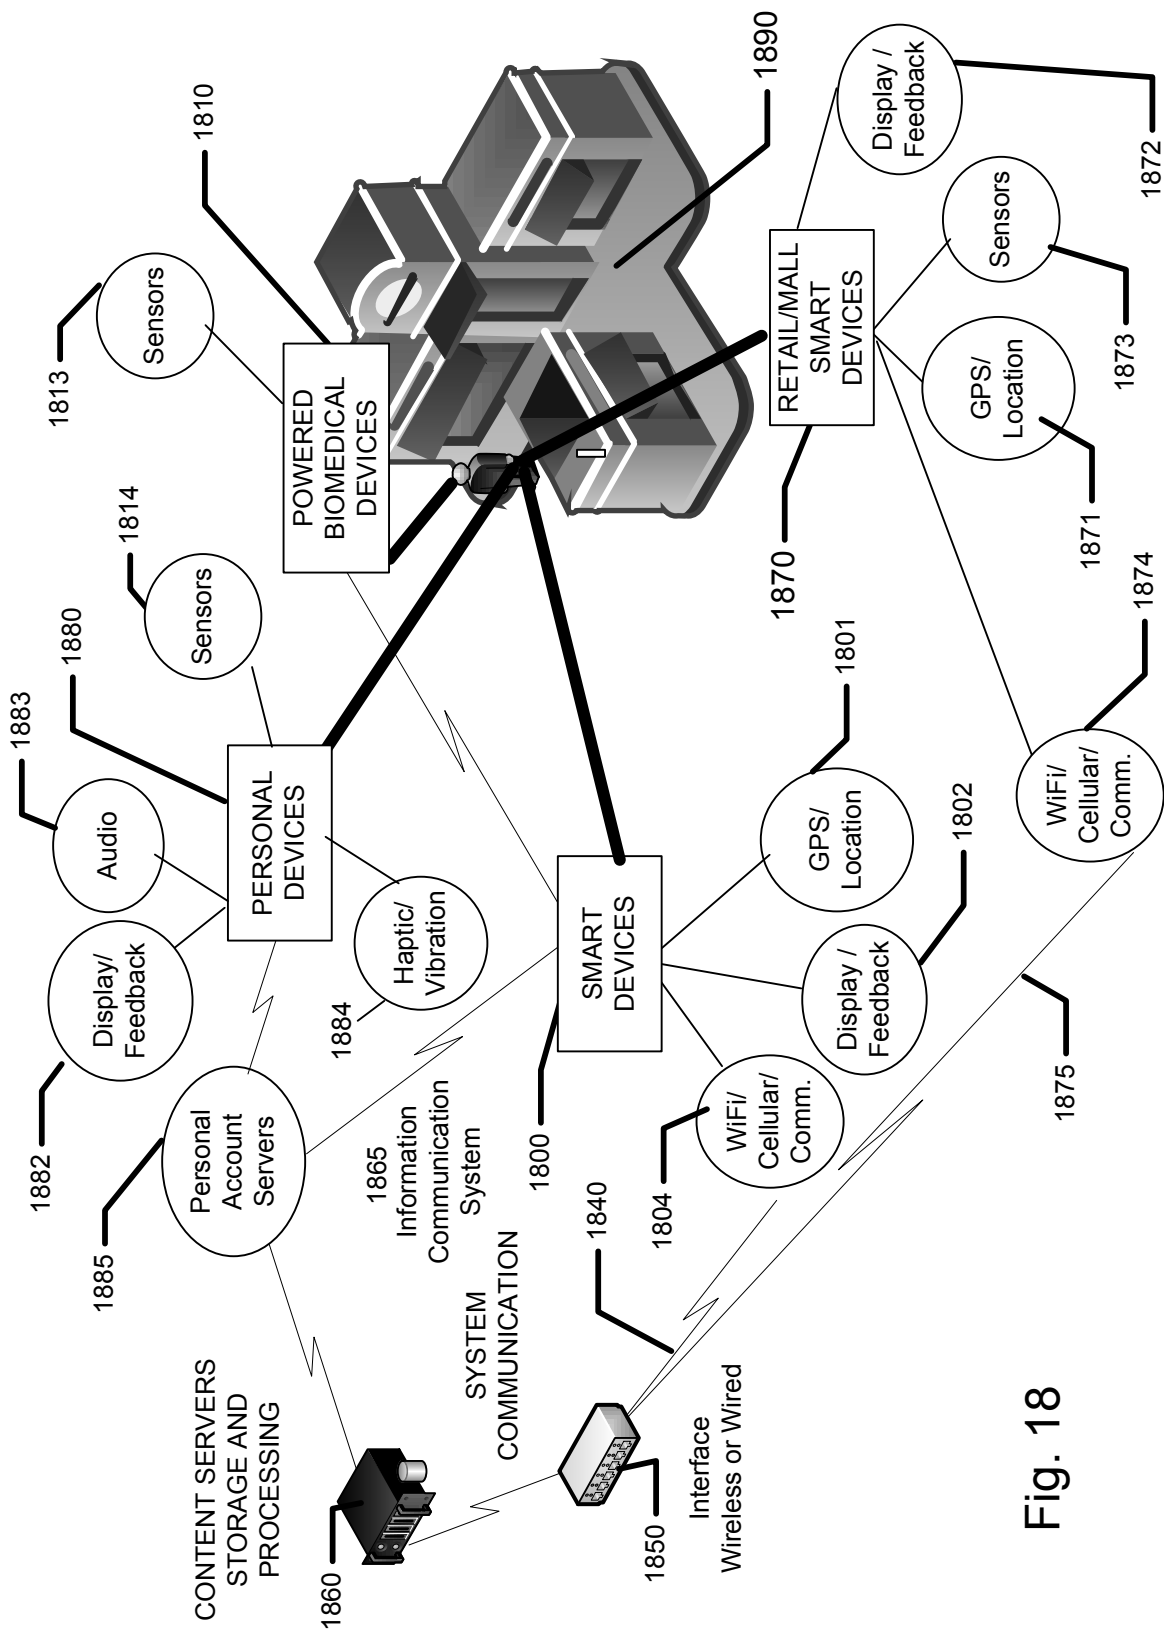


Fig. 18



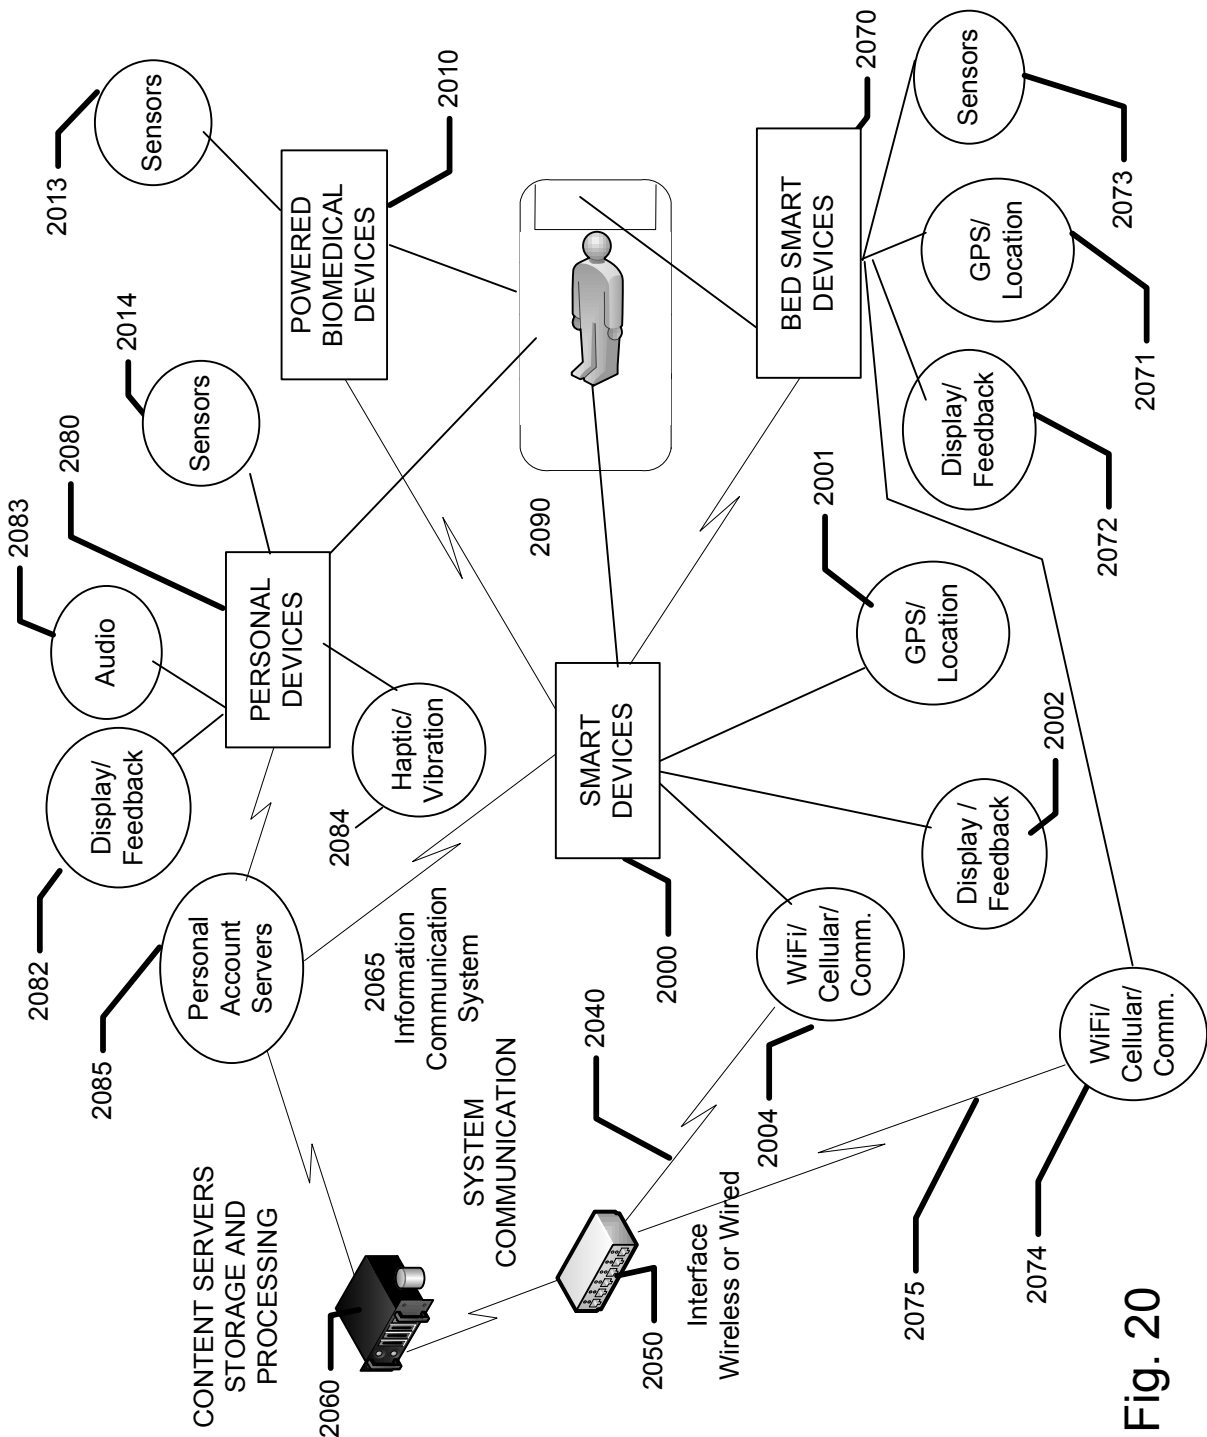


Fig. 20

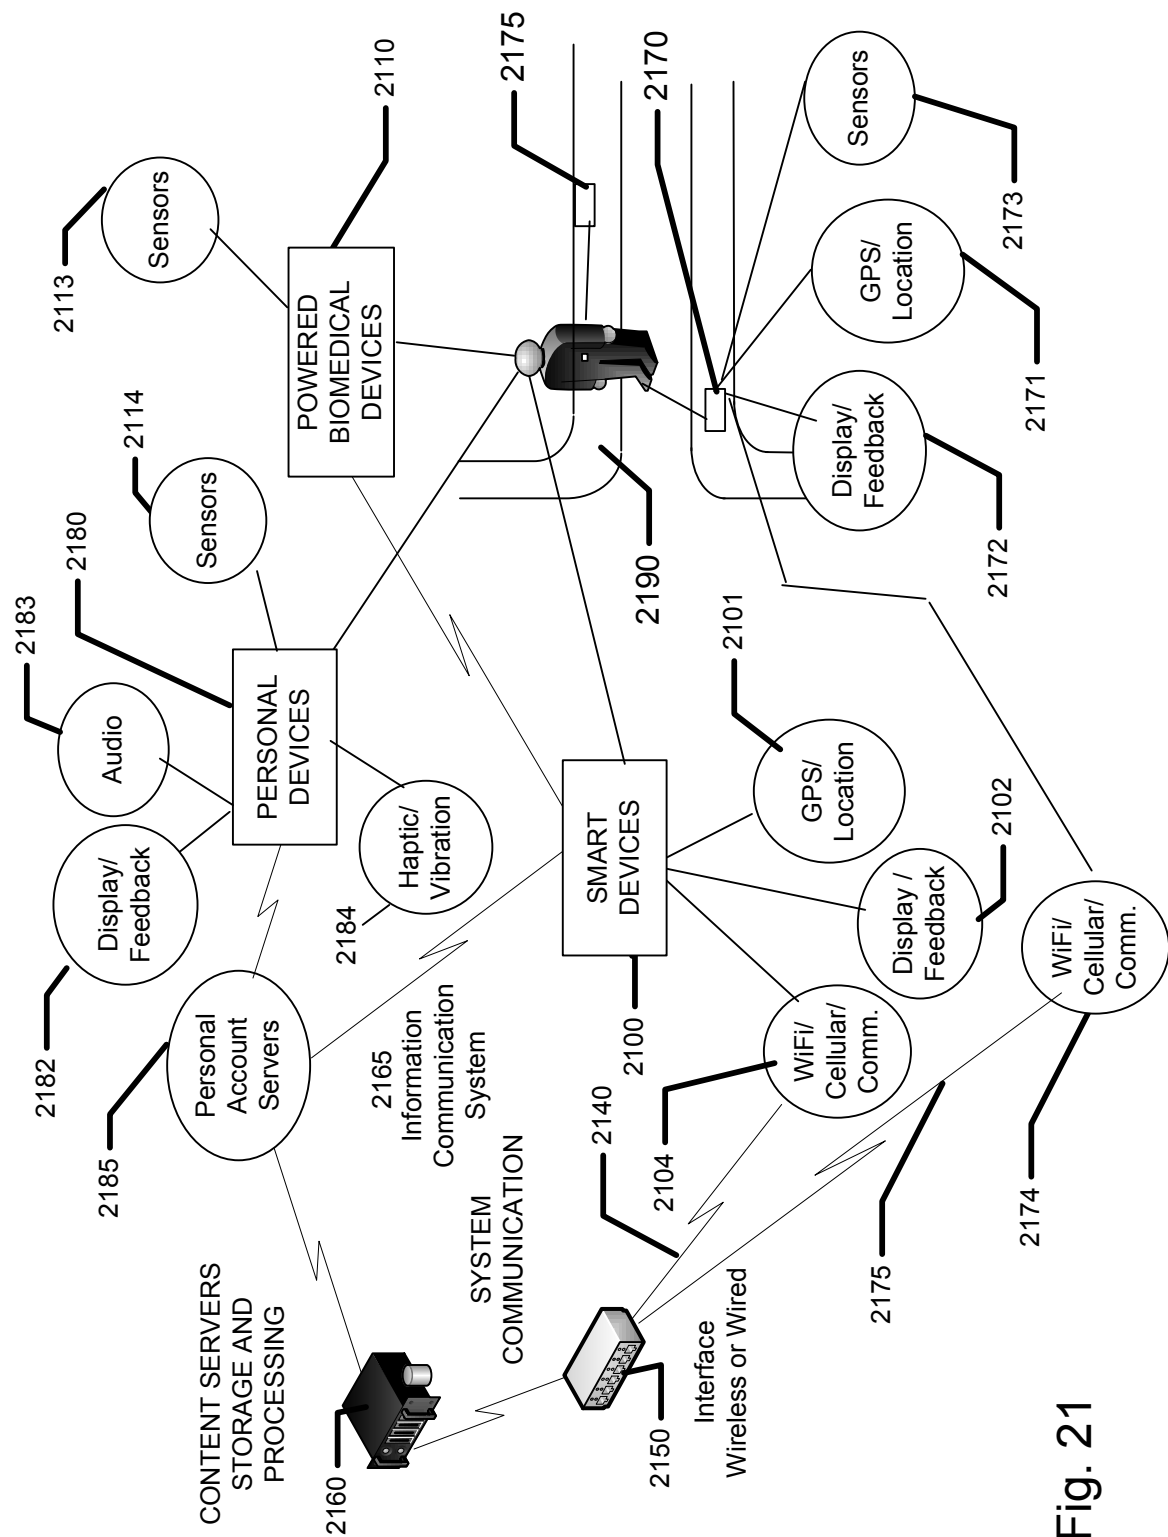


Fig. 21

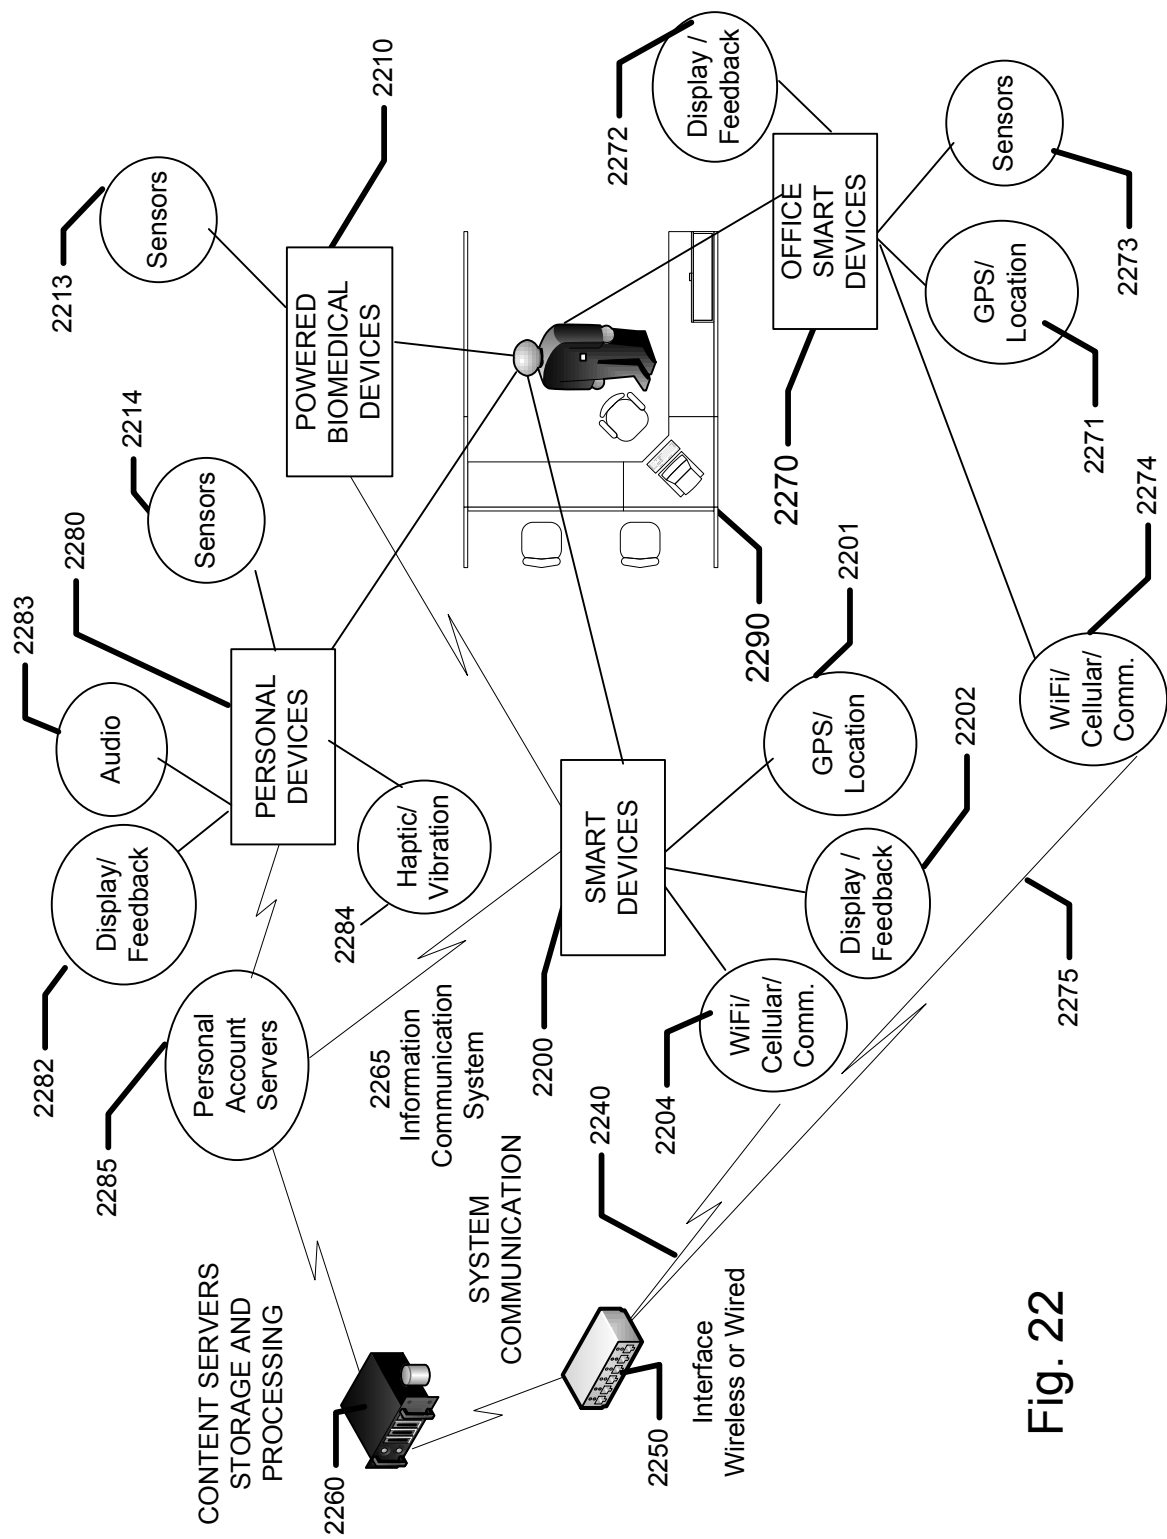


Fig. 22

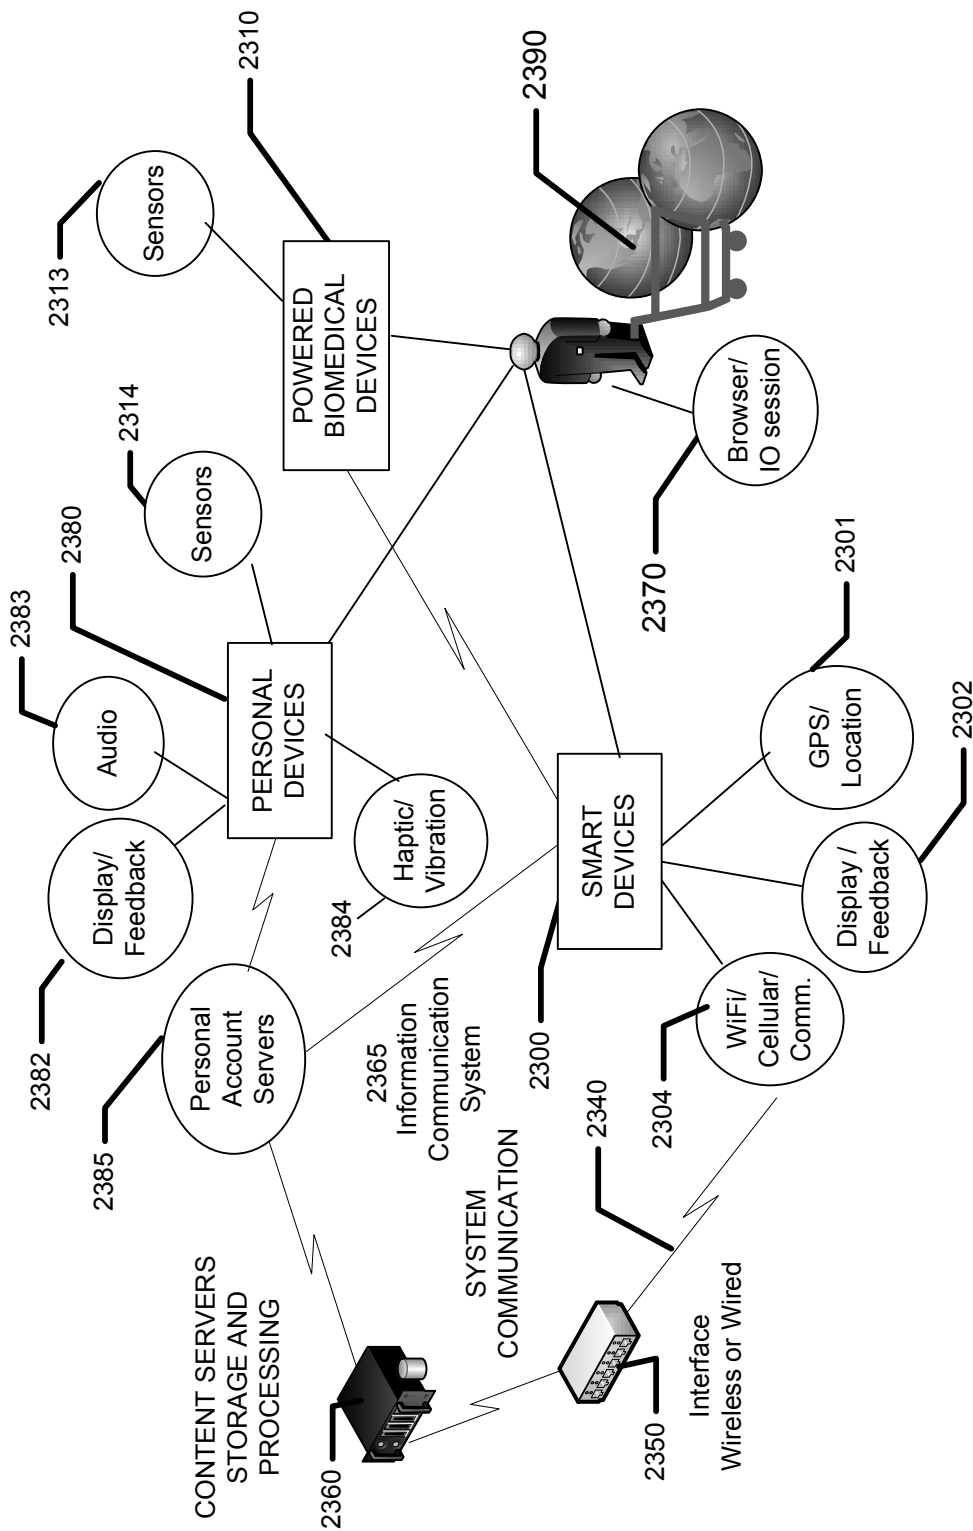


Fig. 23

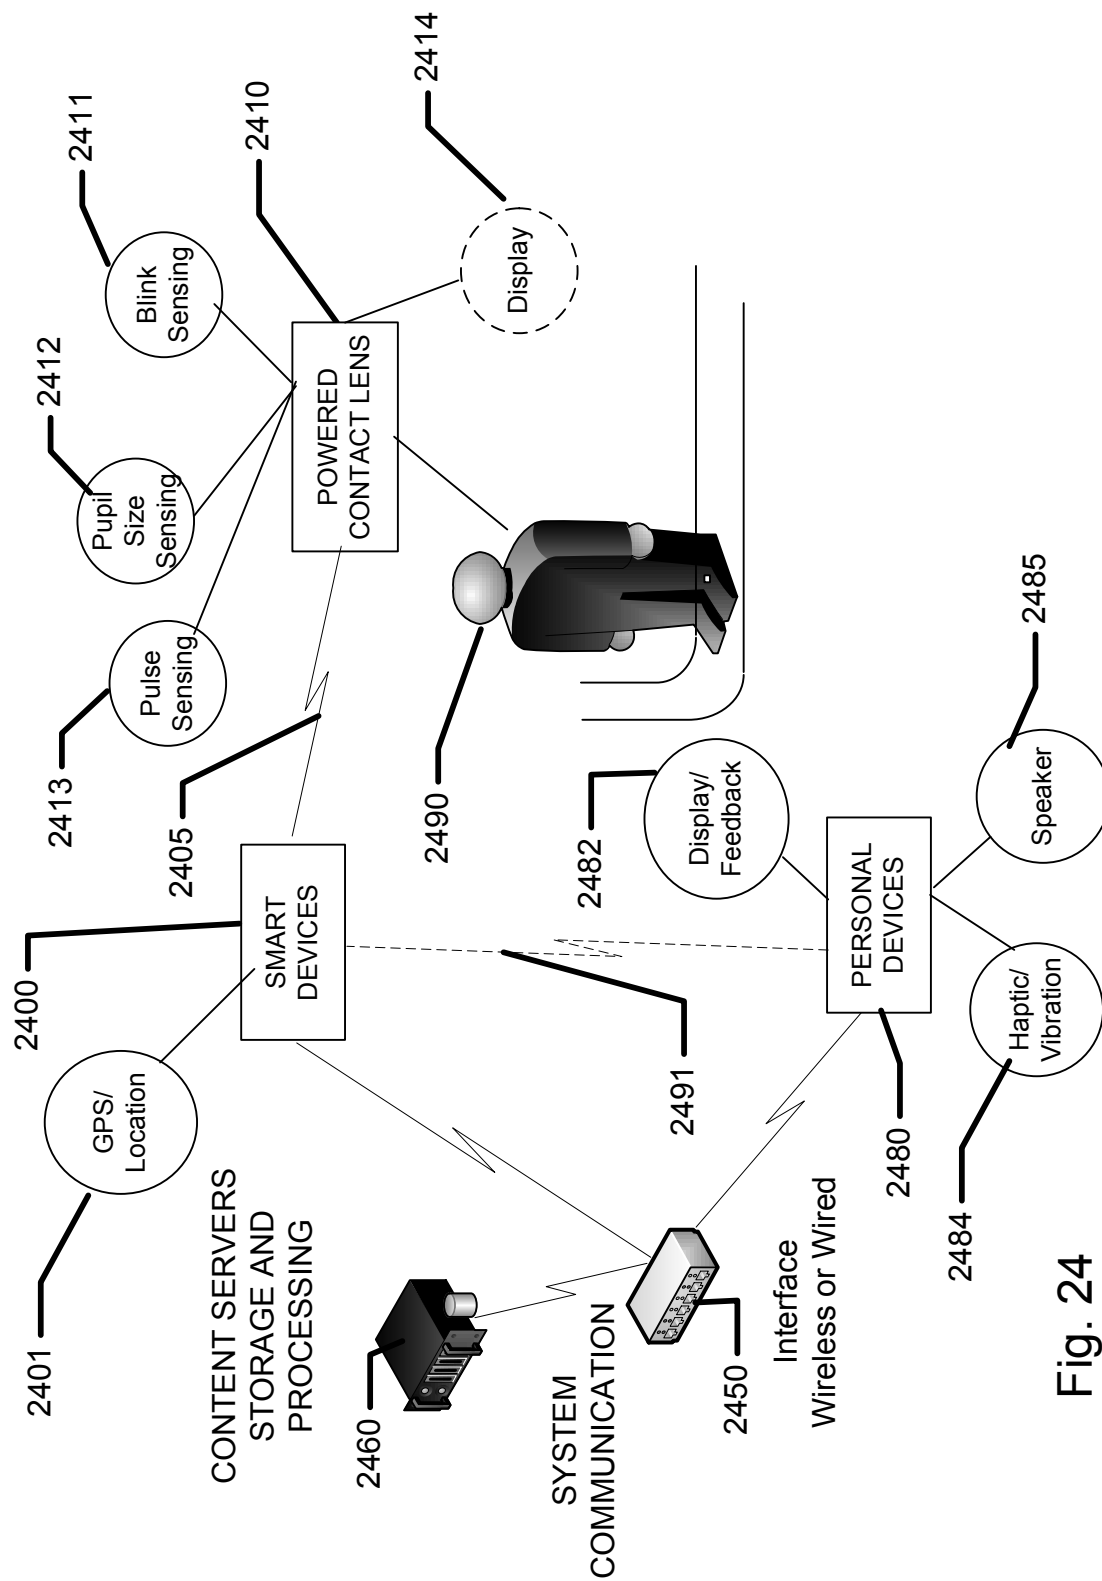


Fig. 24