



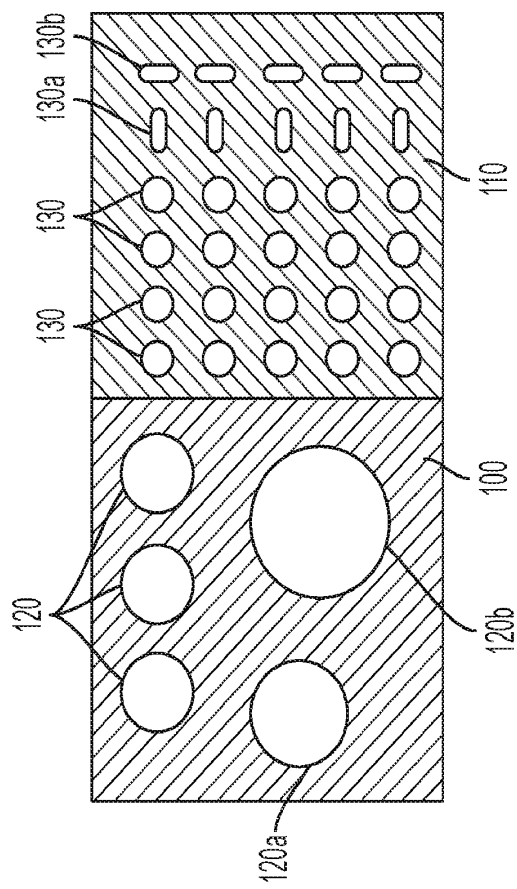

ᲕᲠᲣᲚᲗ

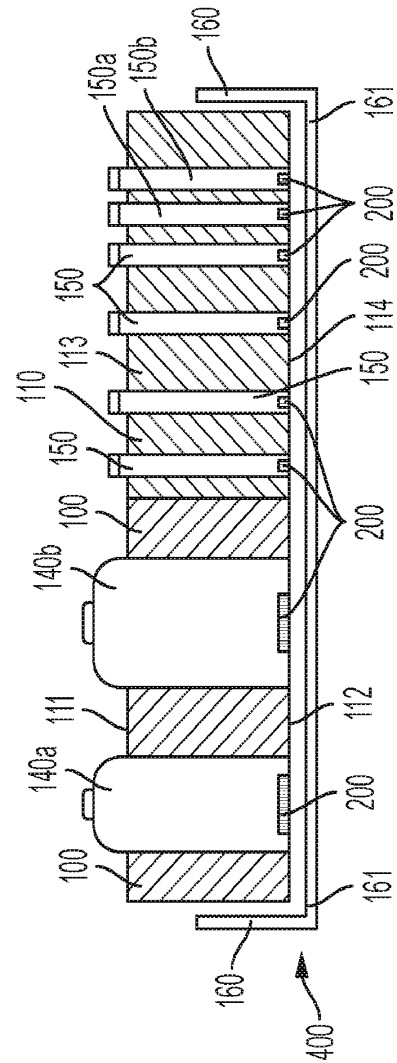

2.
G.
F.

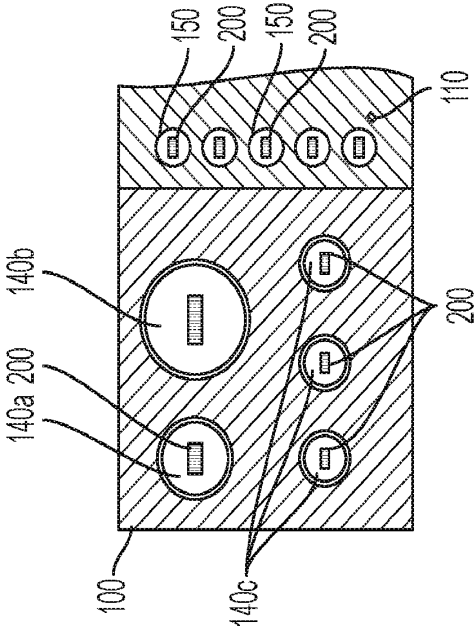


FIG. 3

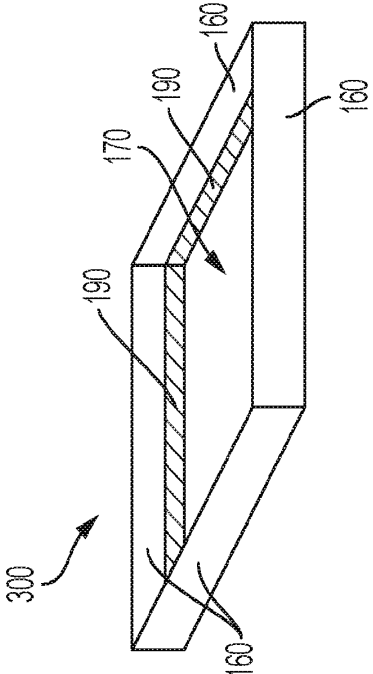


FIG. 4

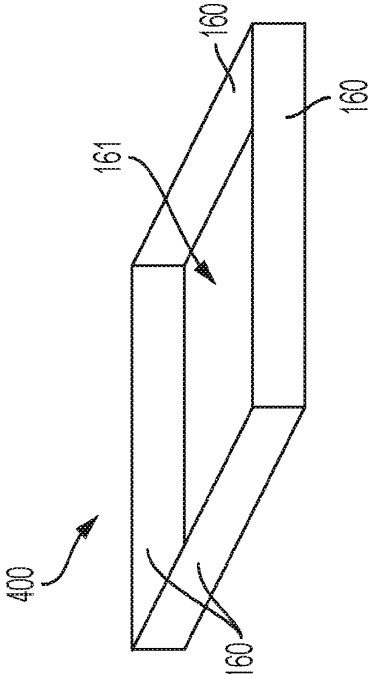


FIG. 5

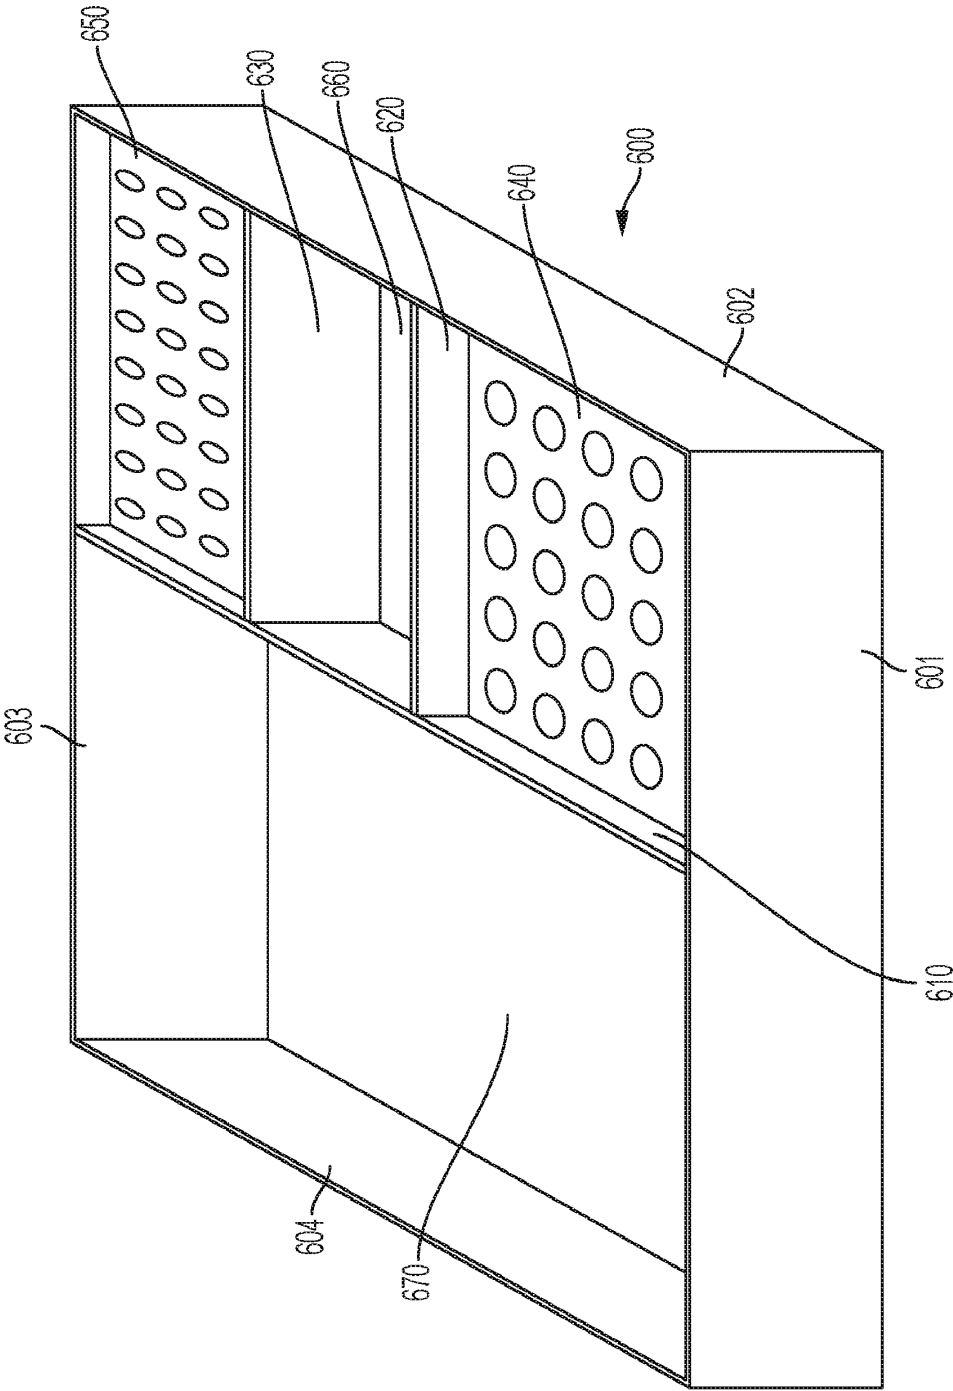


FIG. 6

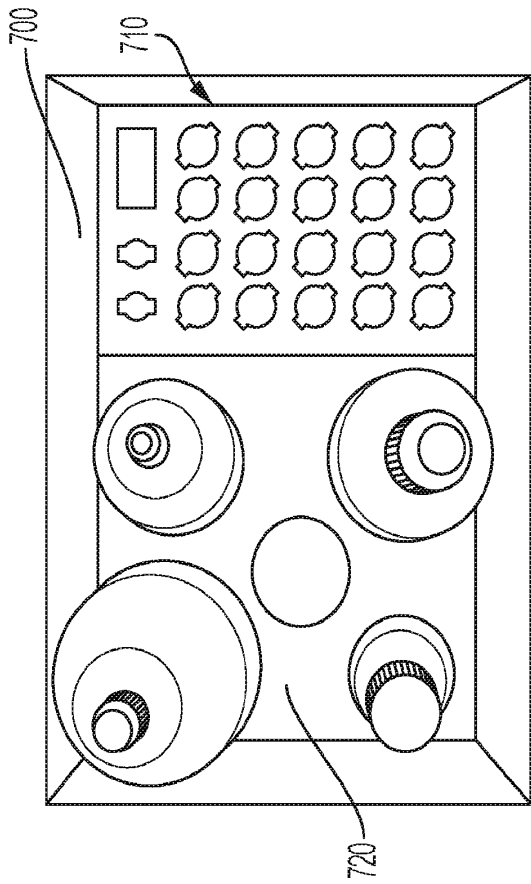


FIG. 7A

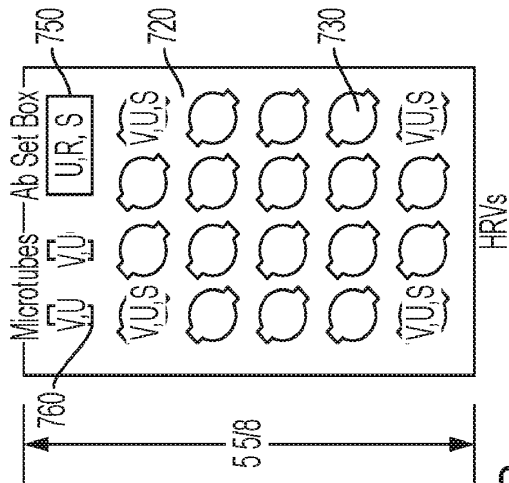
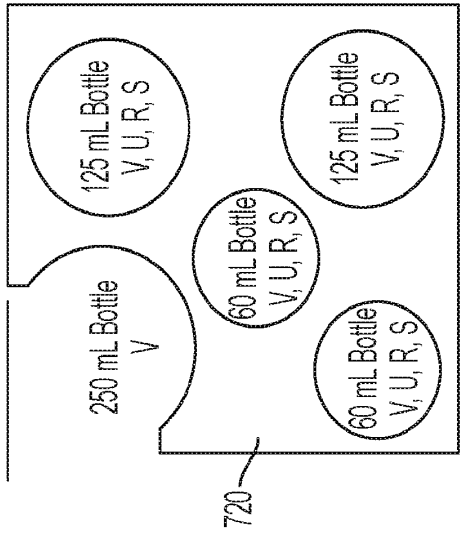
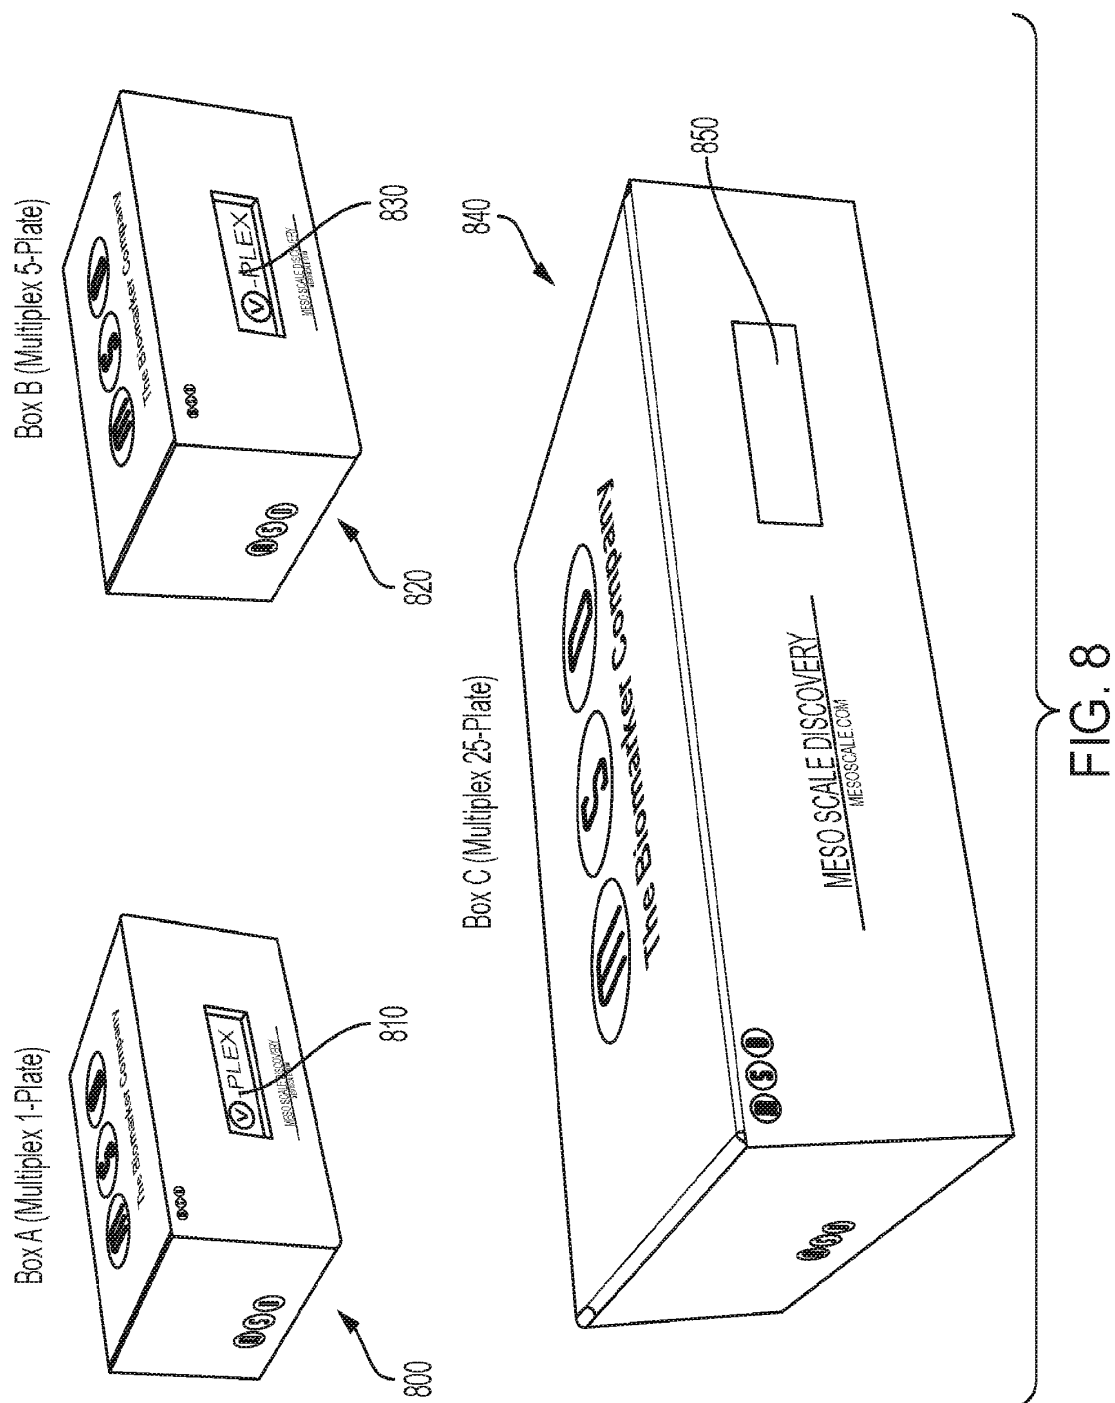


FIG. 7B





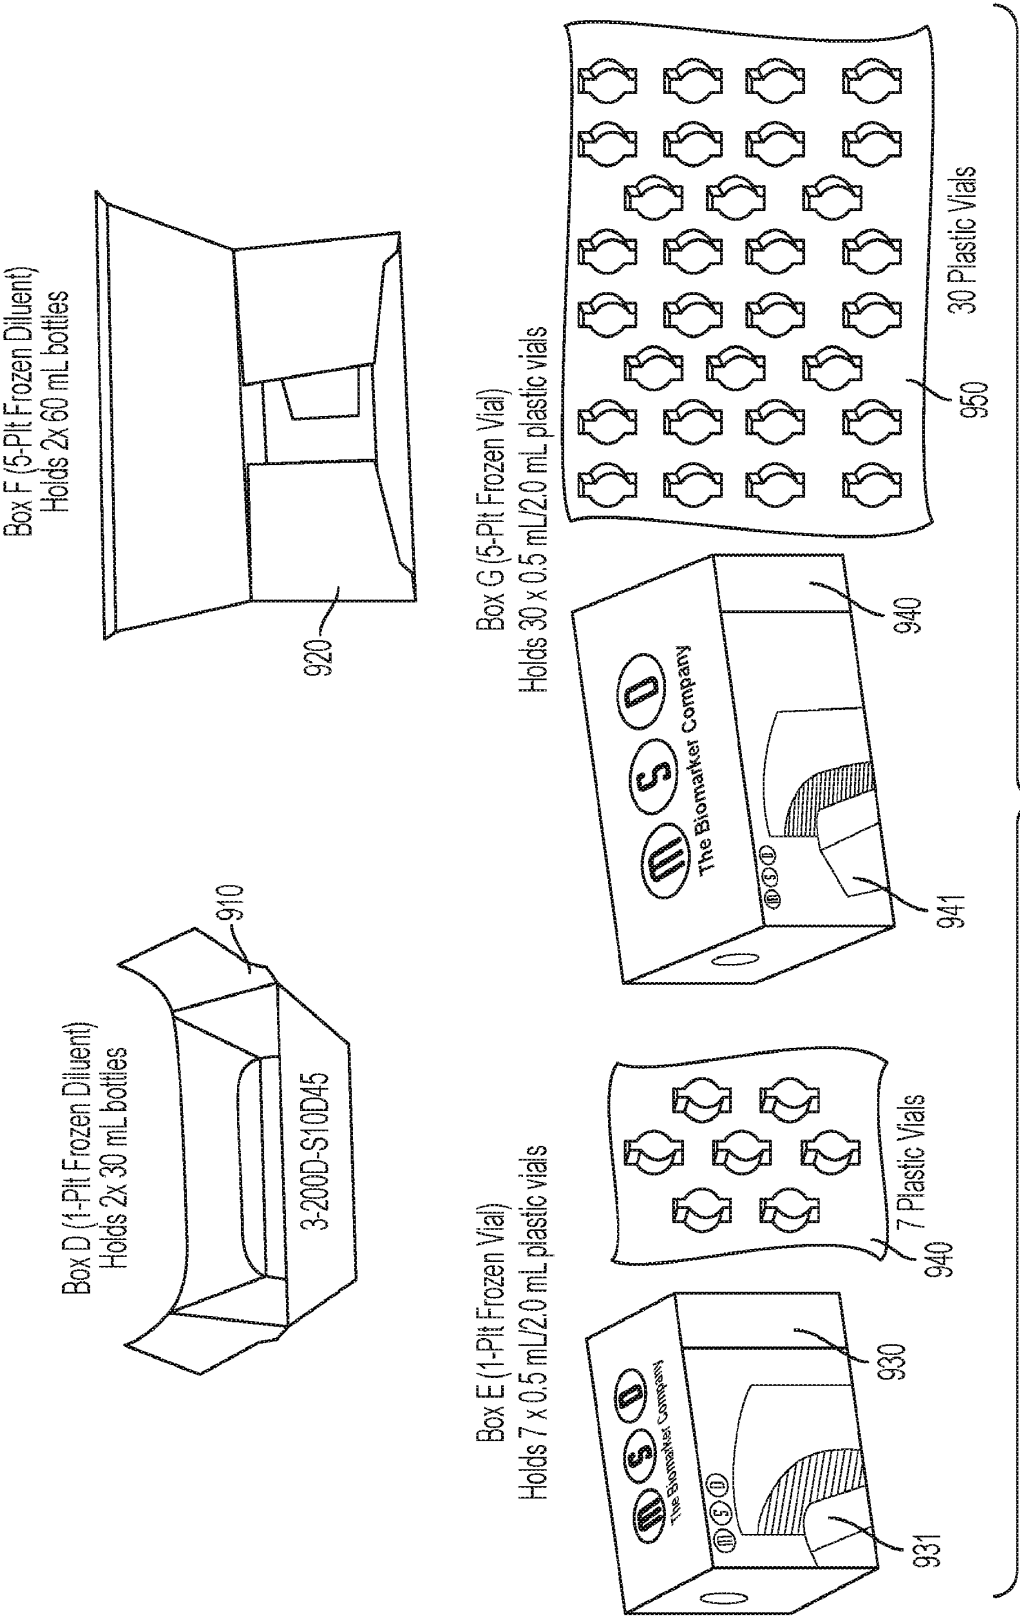
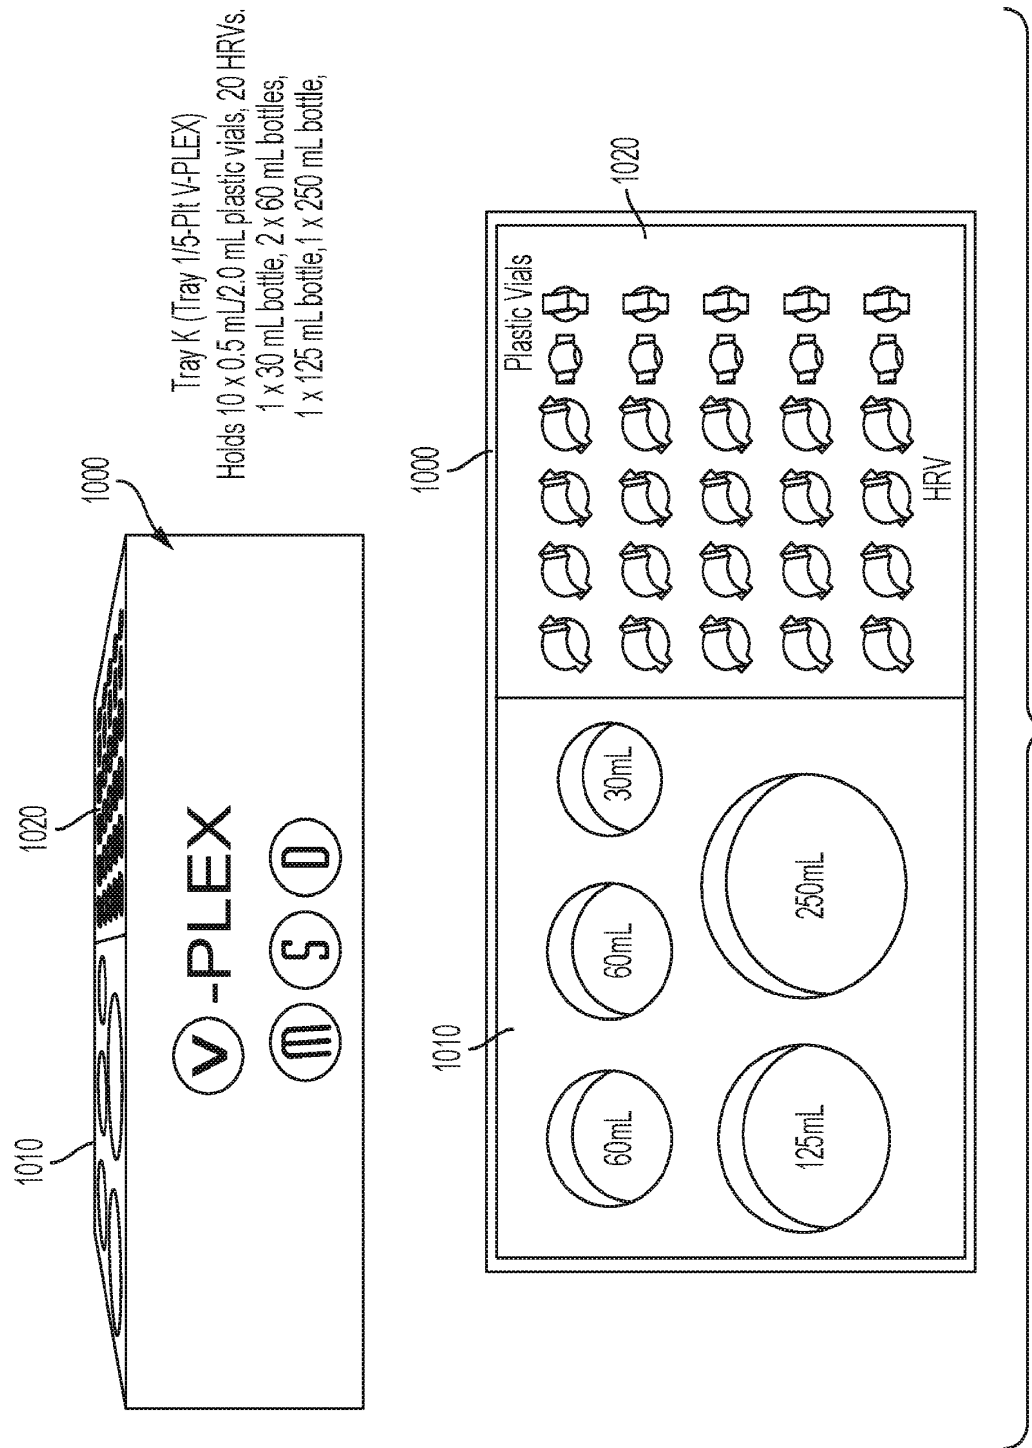
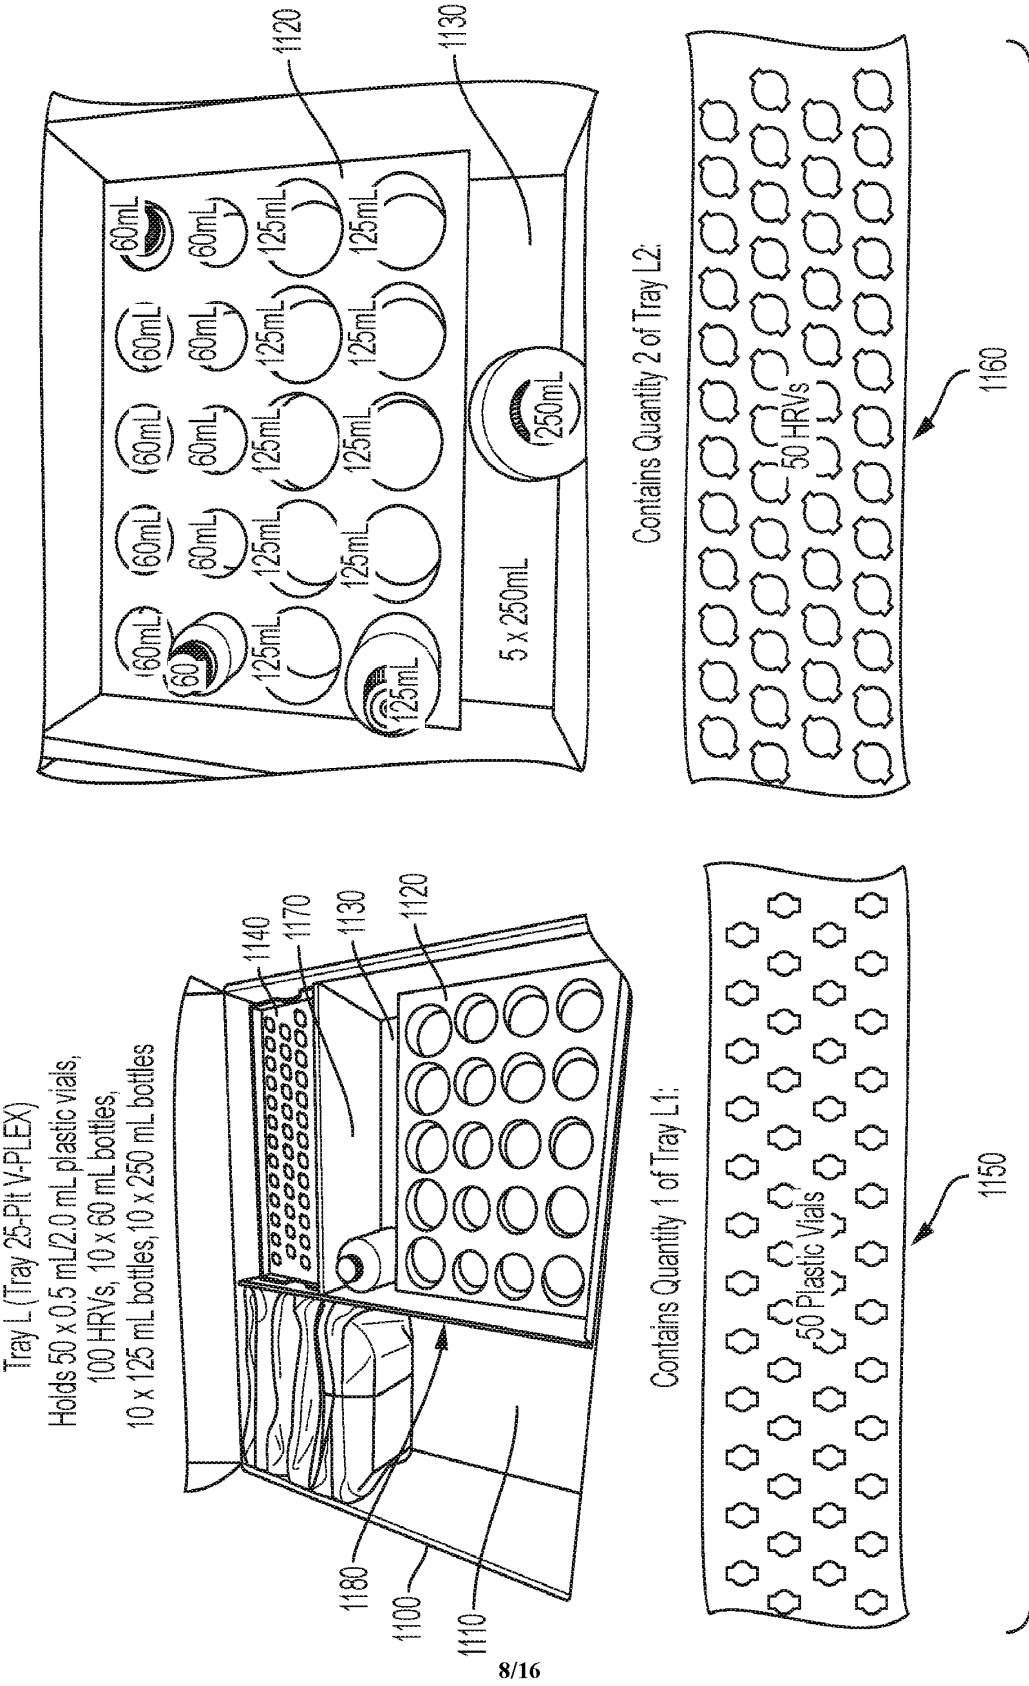


FIG. 9





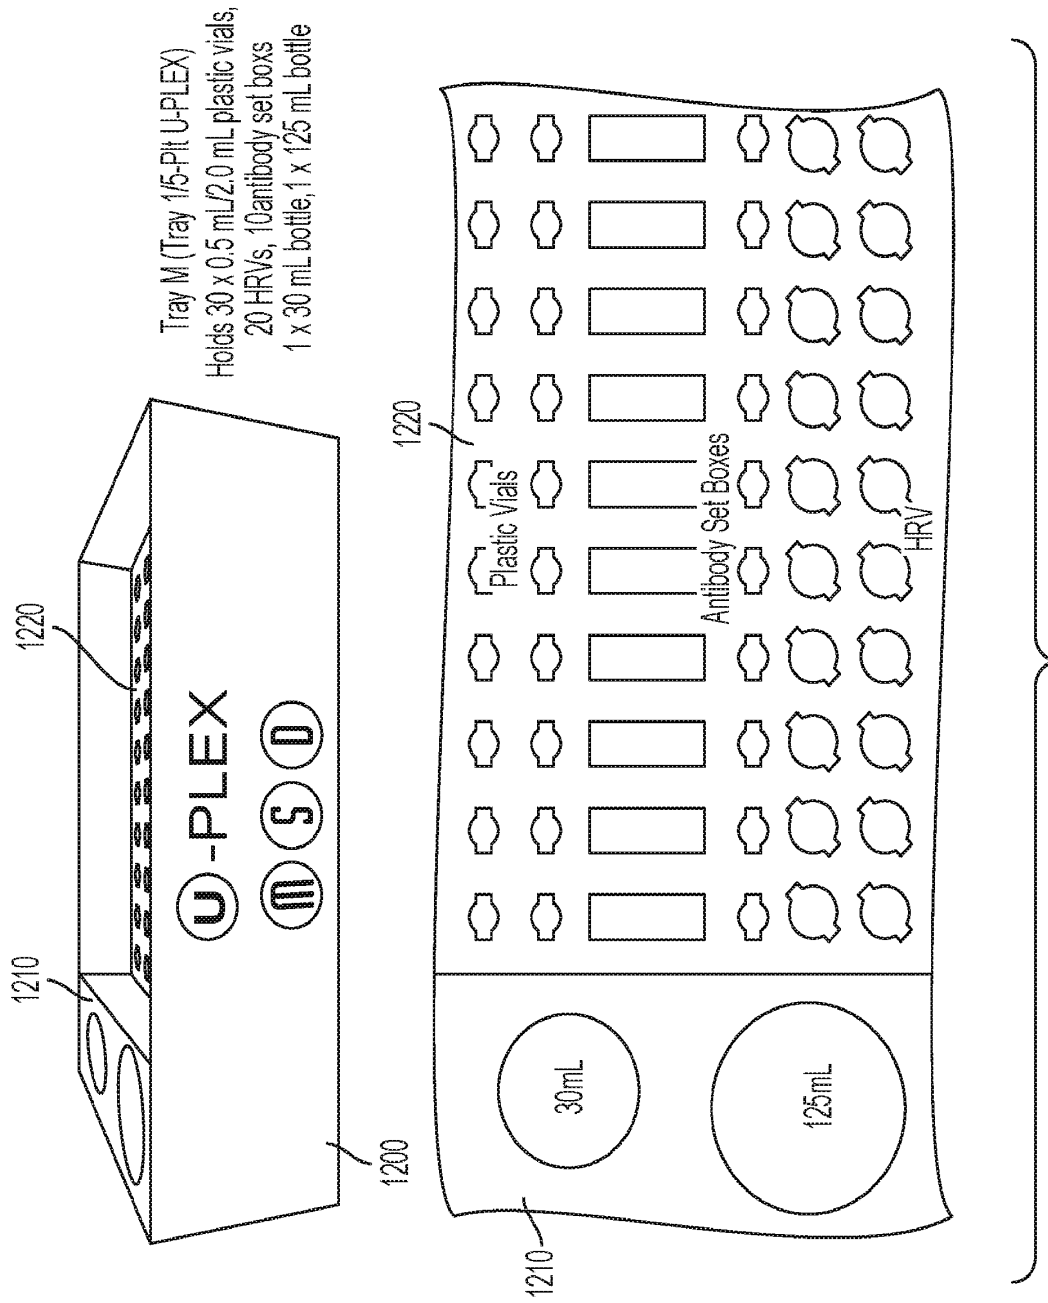
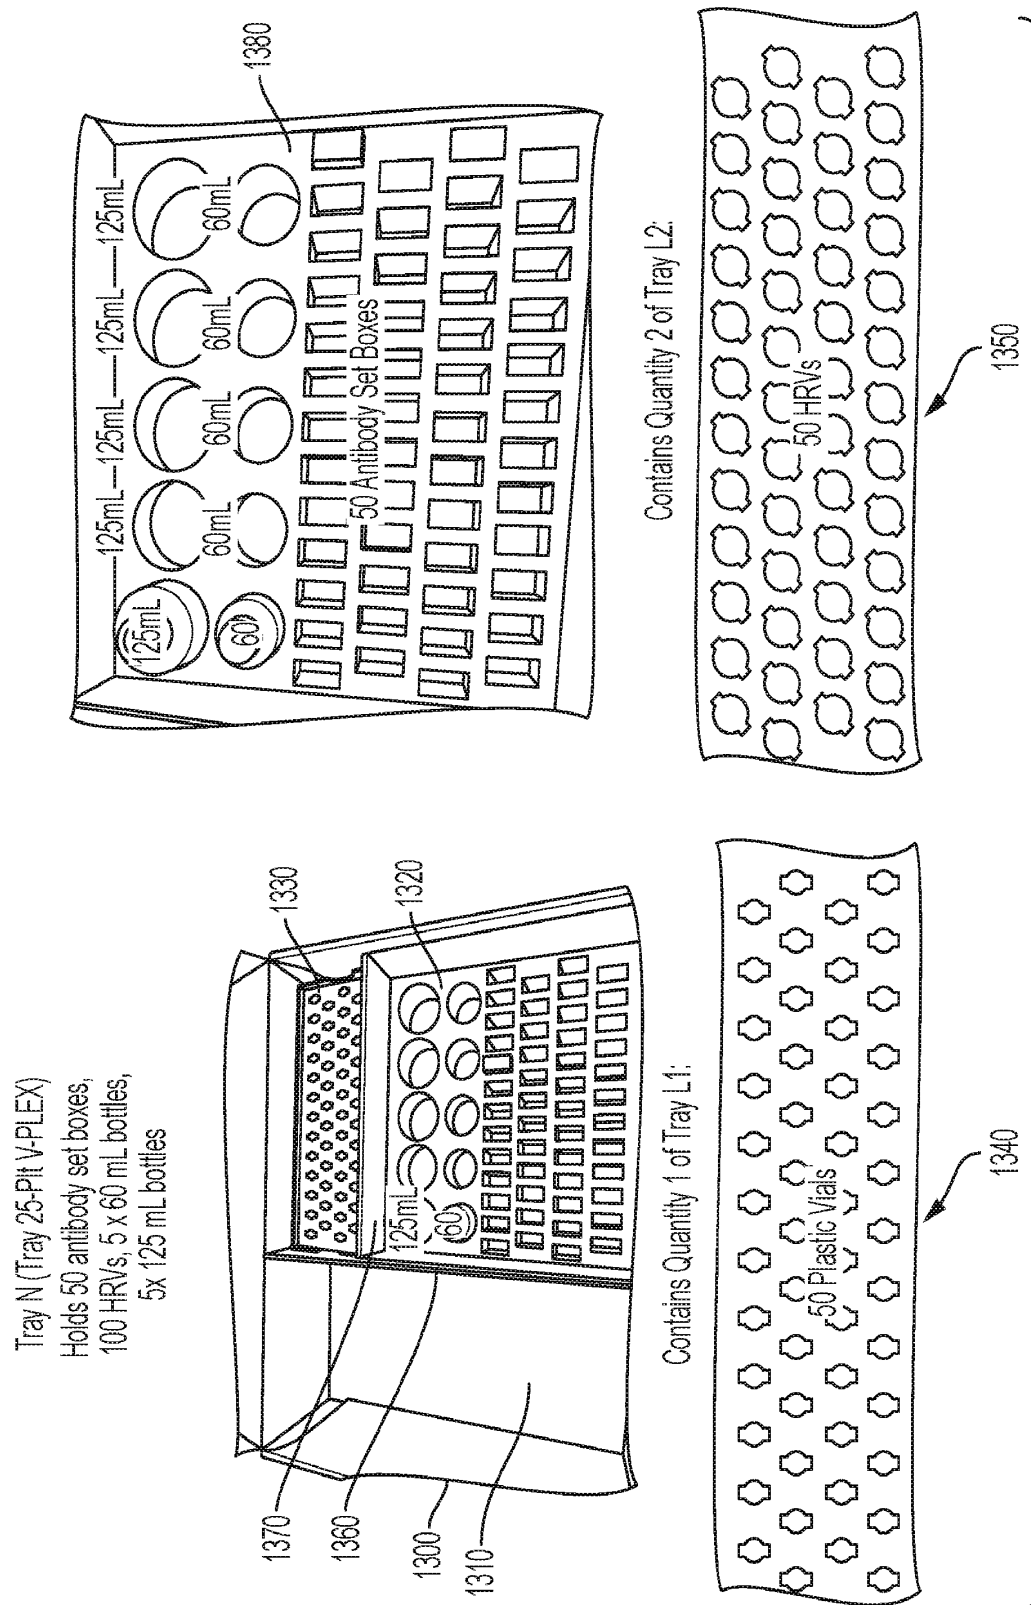


FIG. 12



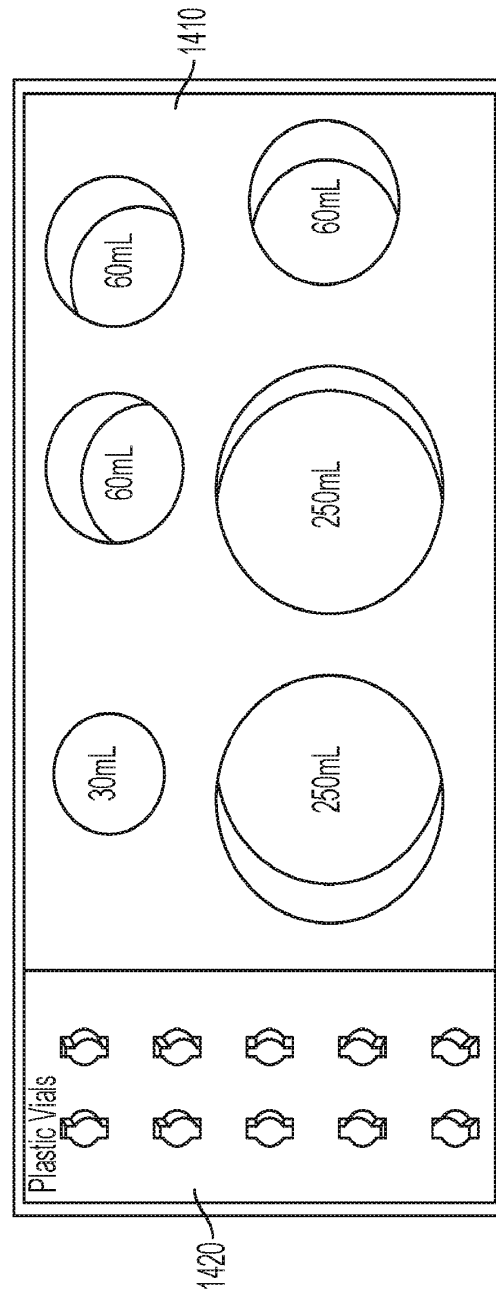
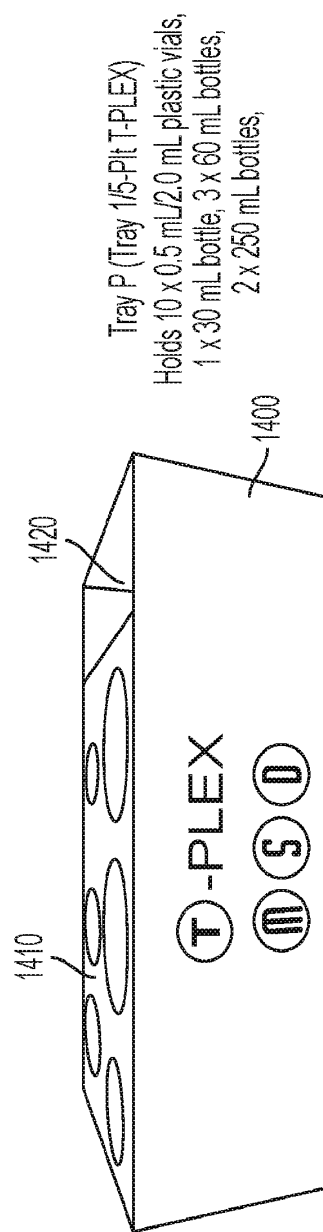


FIG. 14



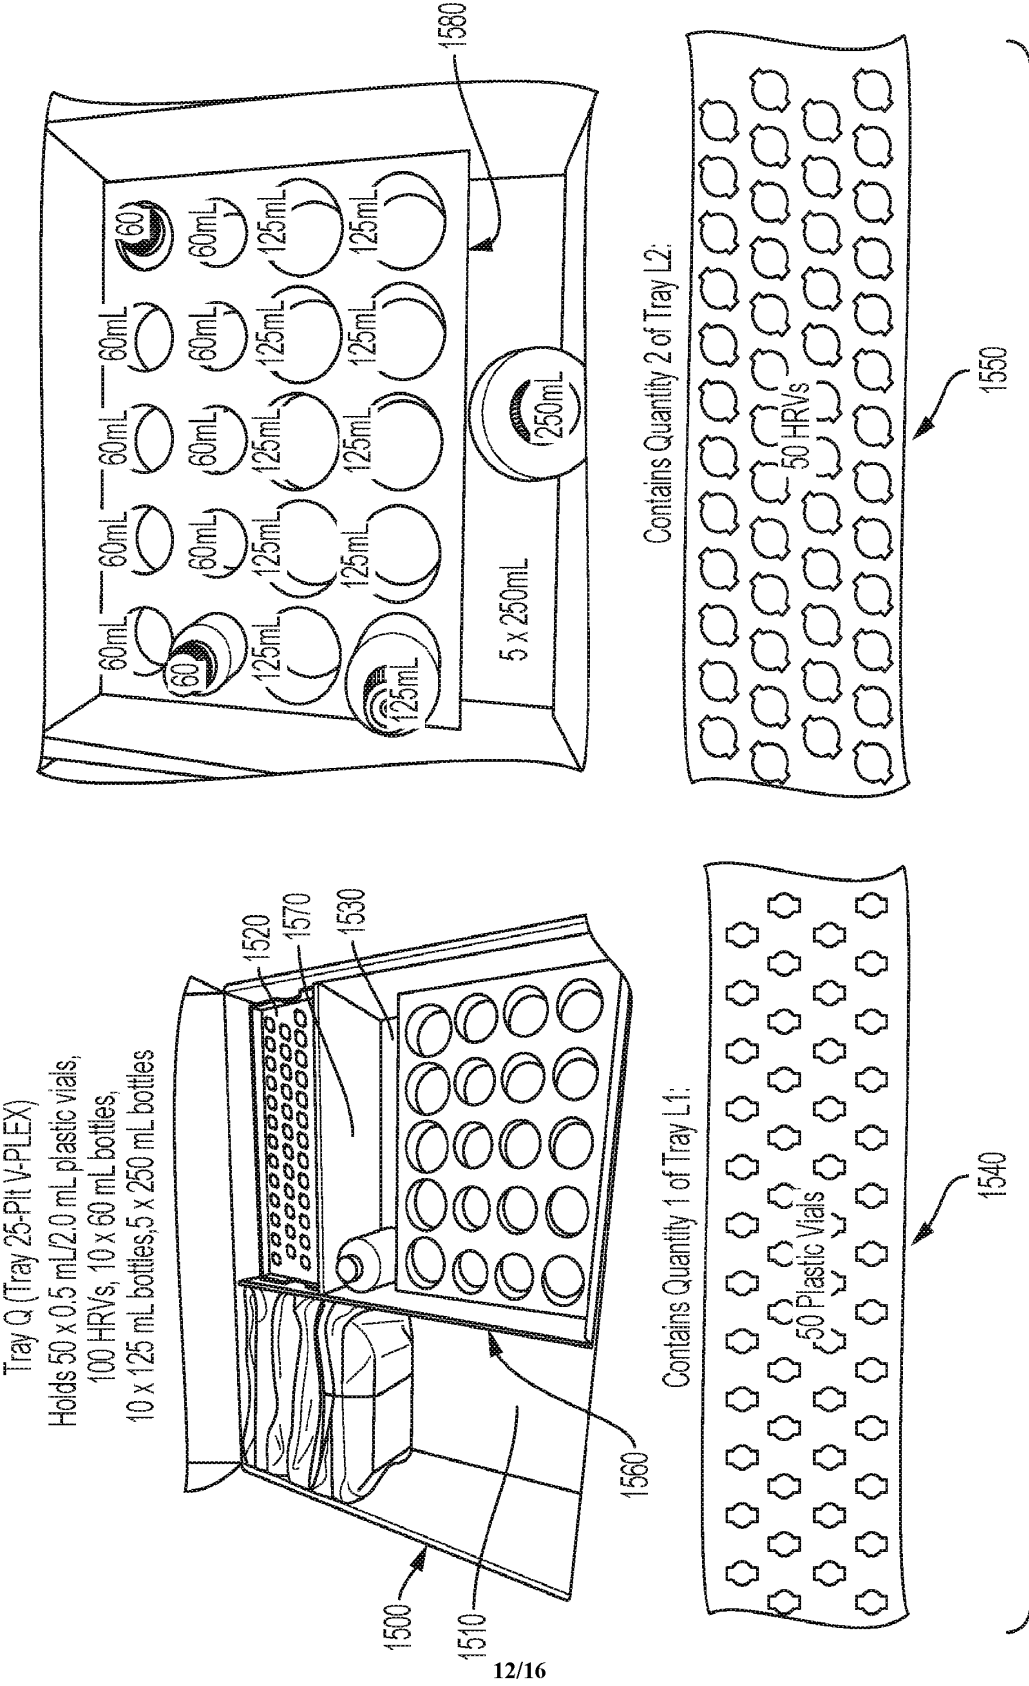


FIG. 15

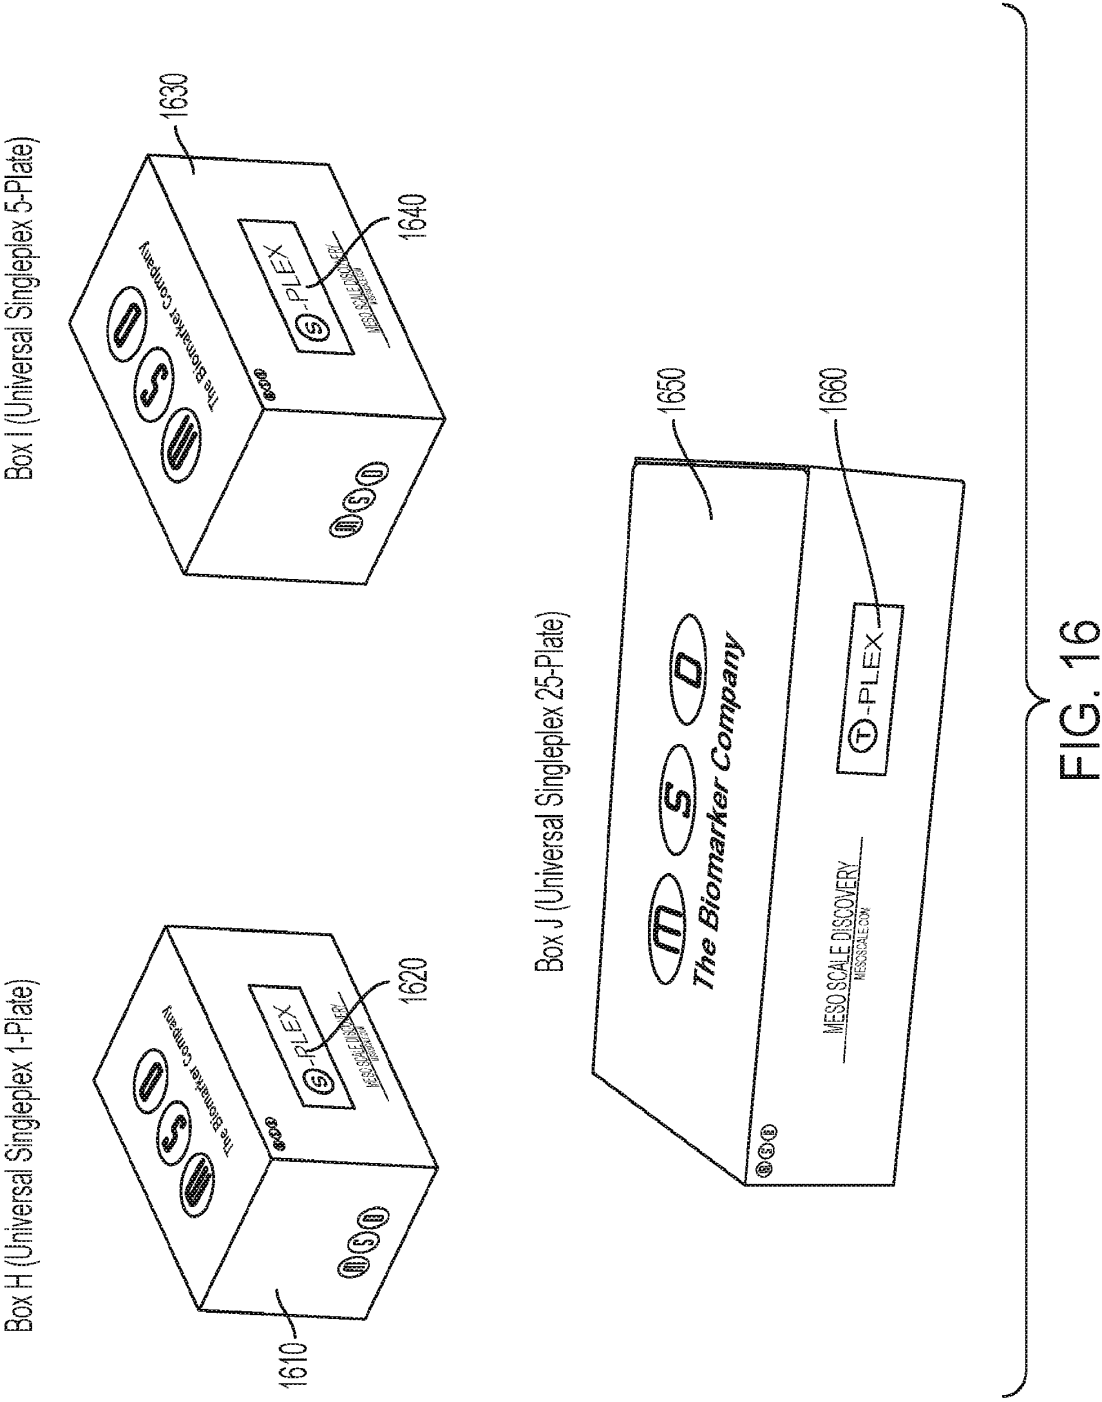

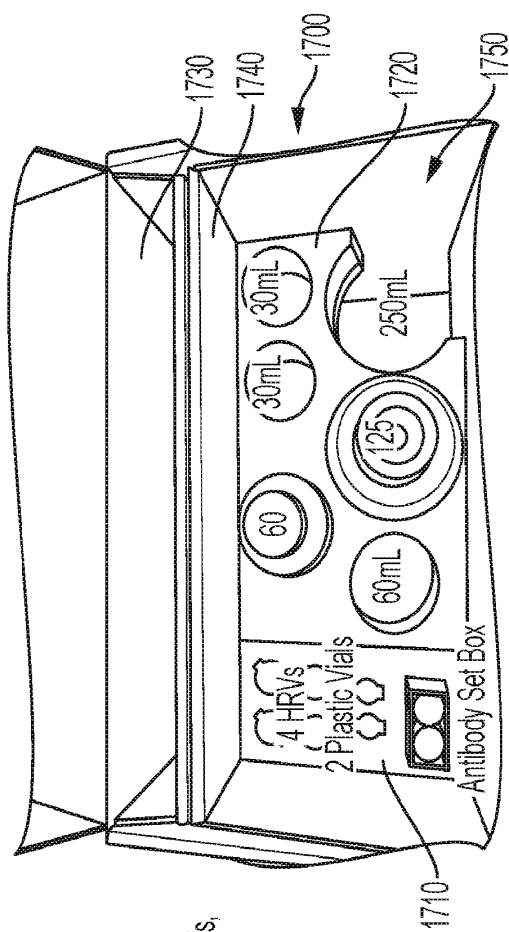

Tray R (Univ Singleplex Tray 1-Pit)
Holds 2 x 0.5 mL/2.0 mL plastic vials, 4 HRVs,
1 antibody setbox
2 x 30 mL bottles, 2 x 60 mL bottles,
1 x 125 mL bottle, 1 x 250 mL bottle

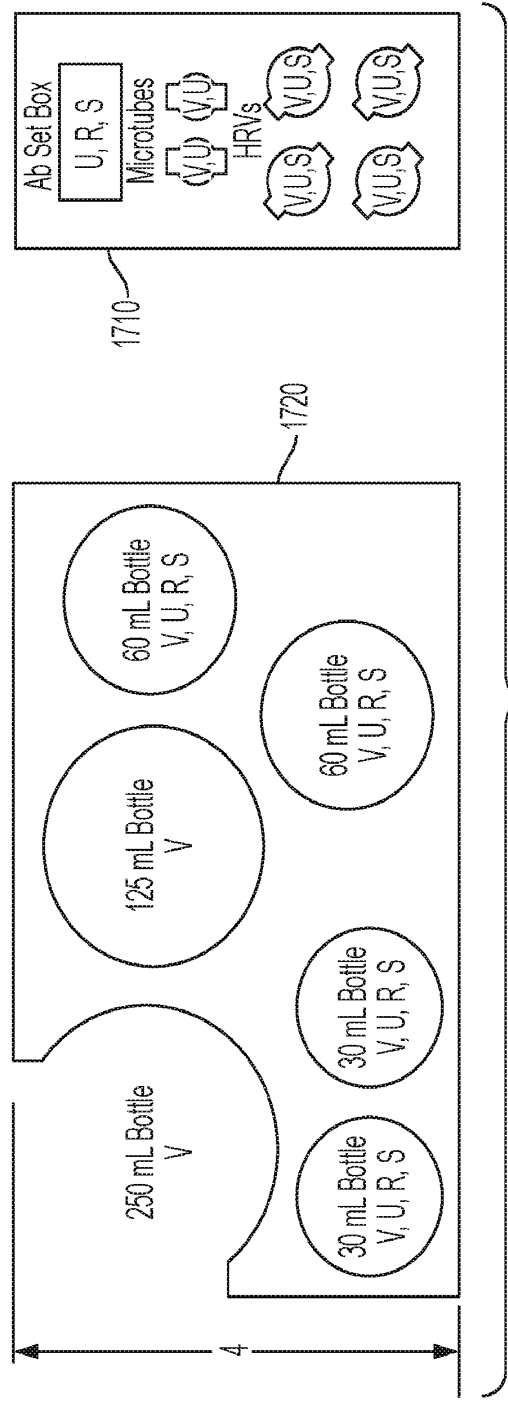


FIG. 17

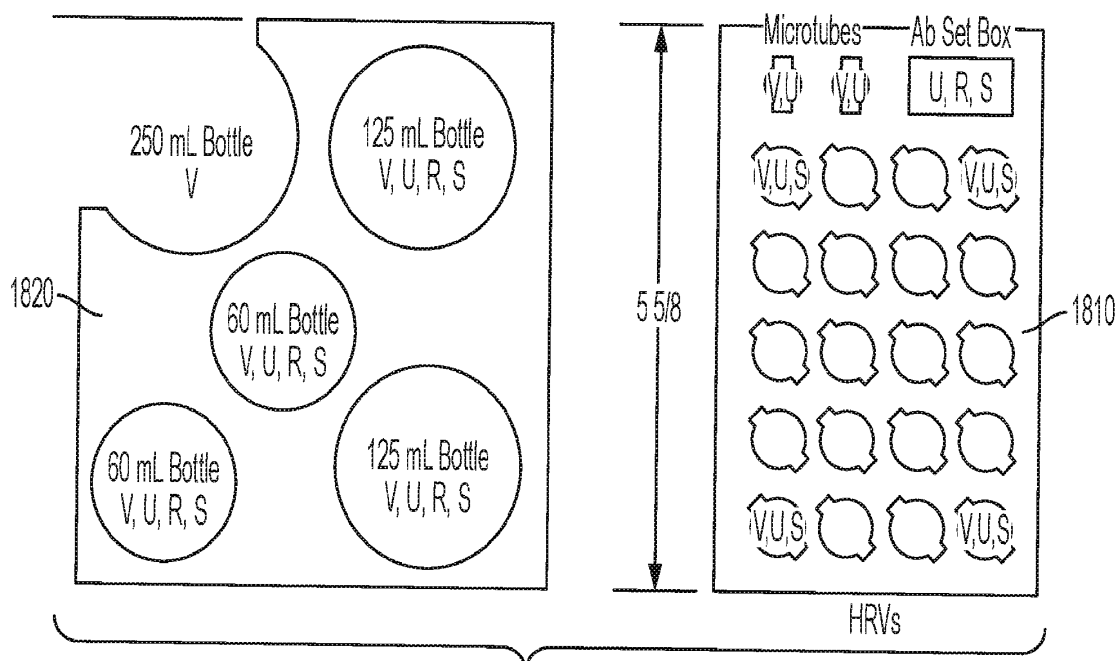
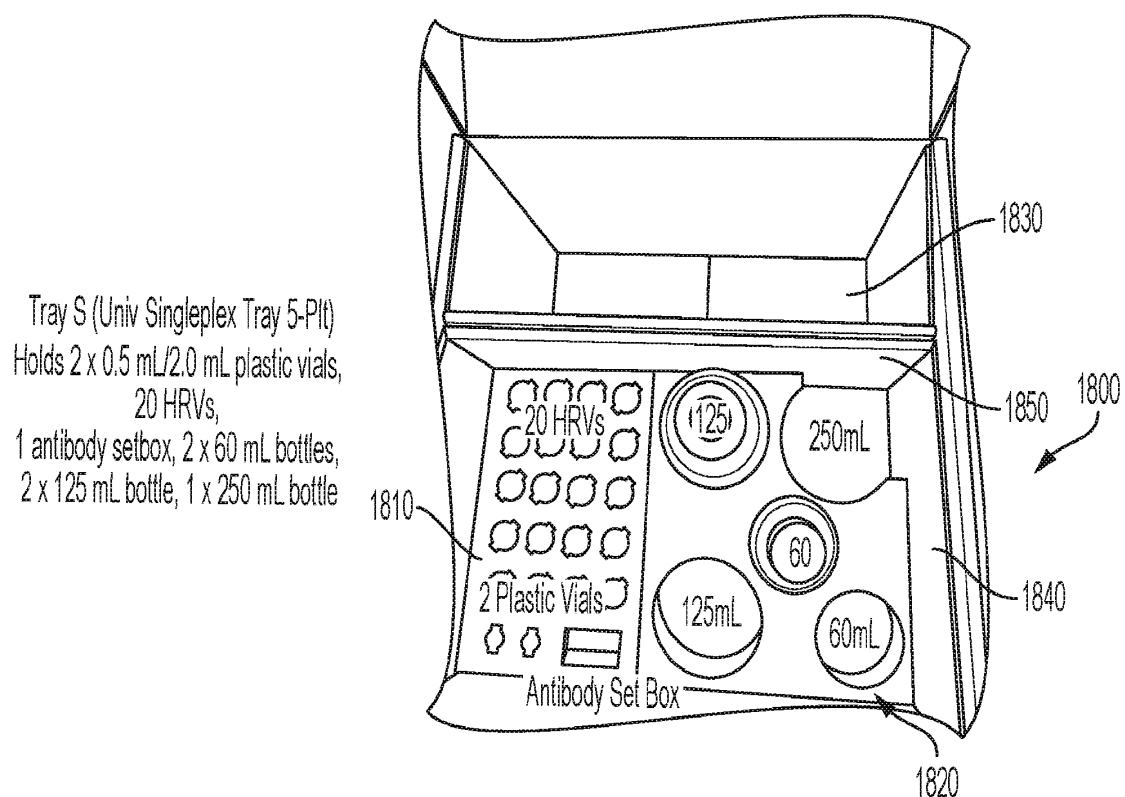


FIG. 18

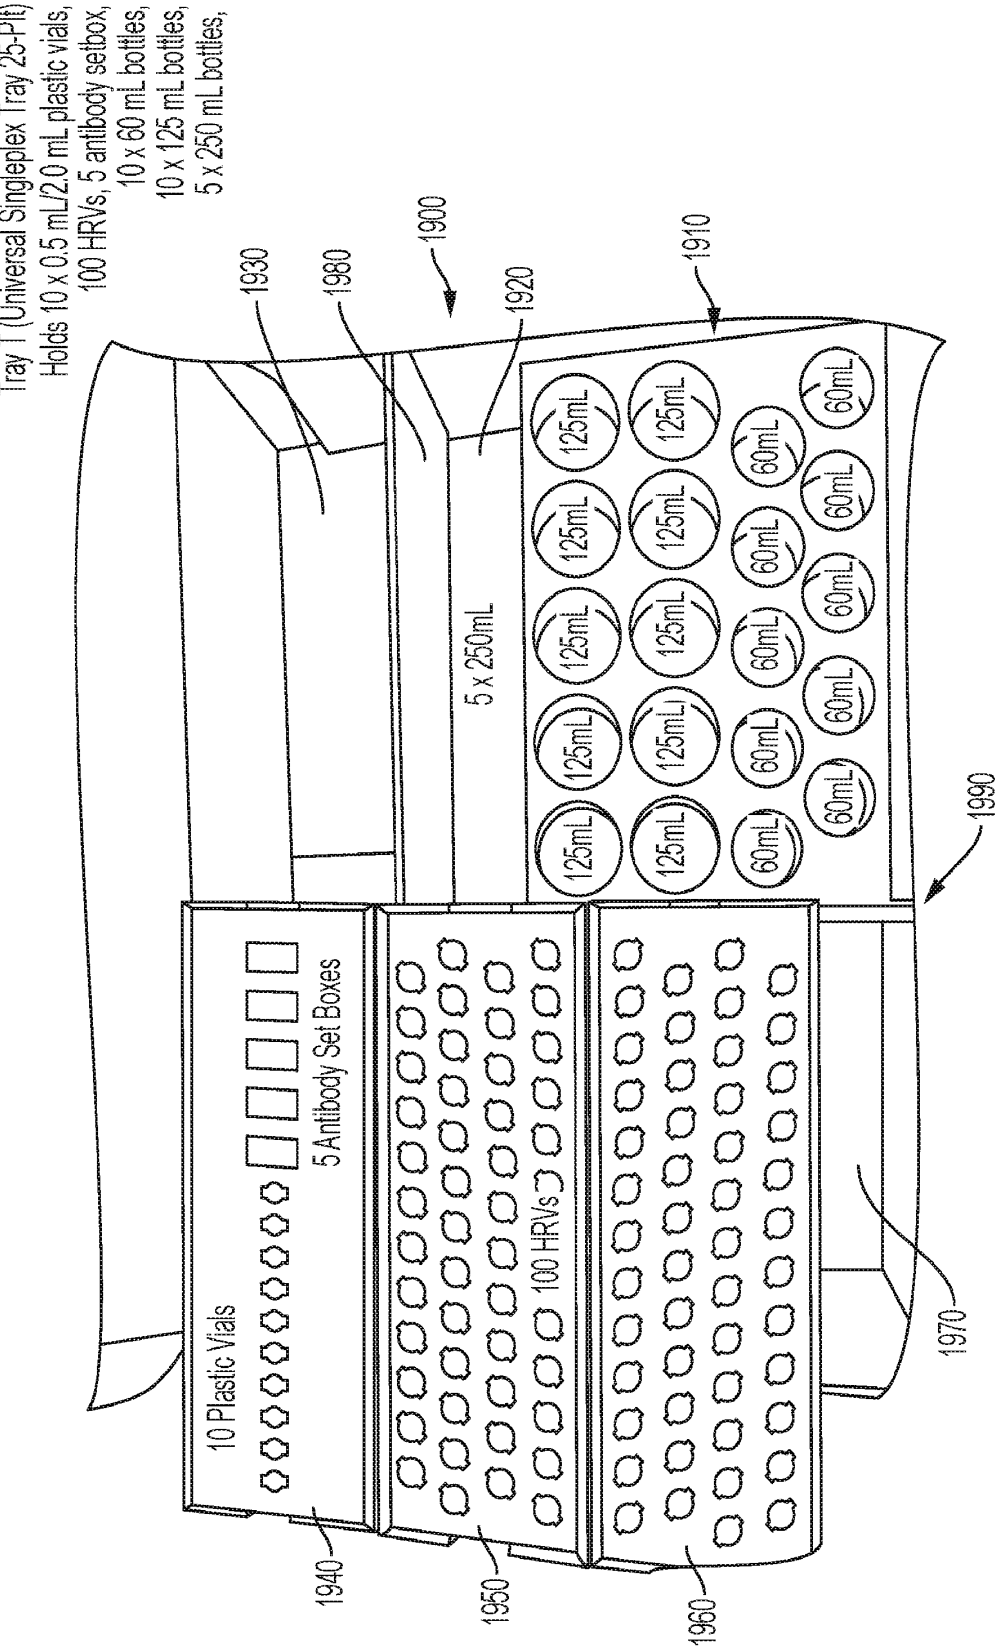


FIG. 19