

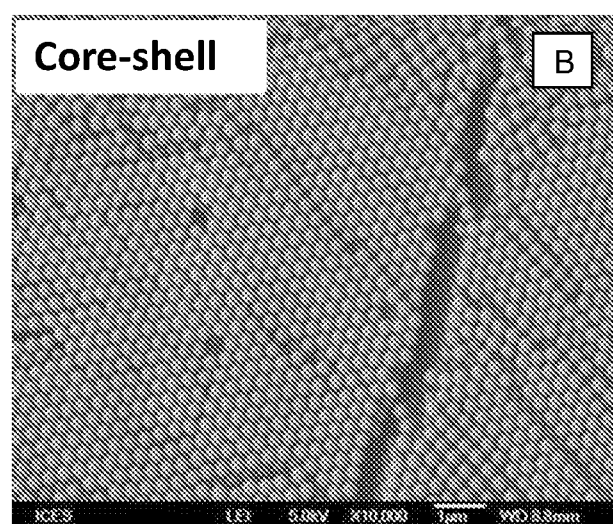
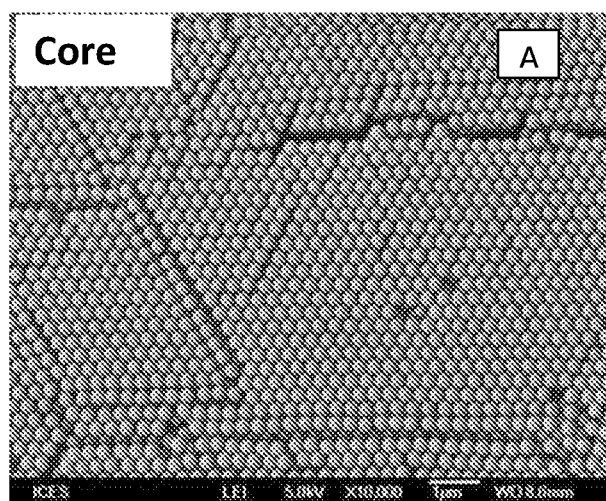



[Fig. 1]

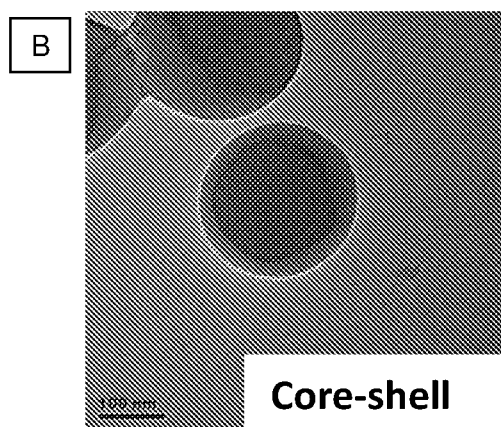


[Fig. 2]

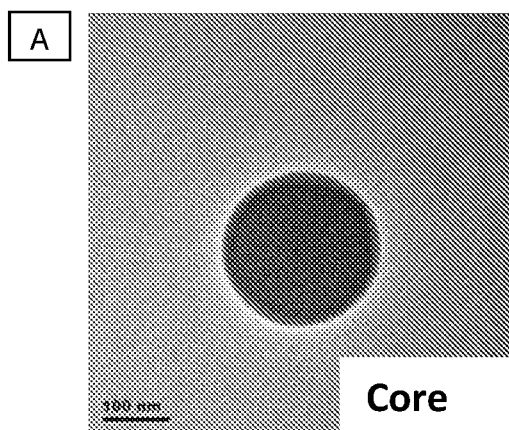


[Fig. 3]

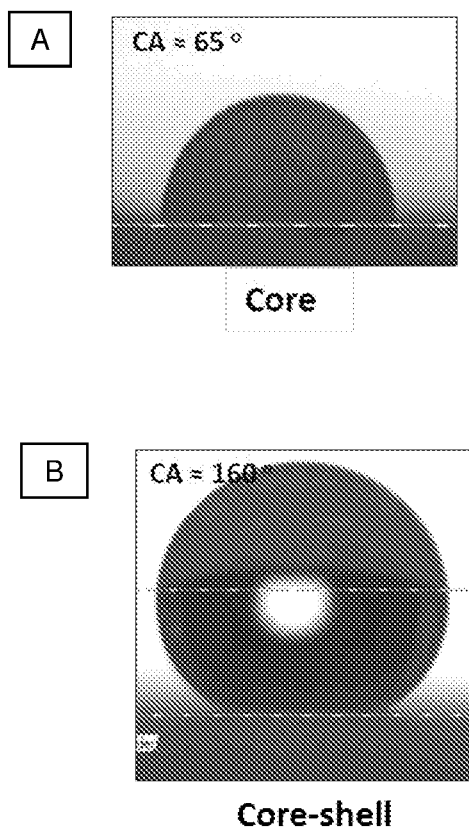



[Fig. 4]

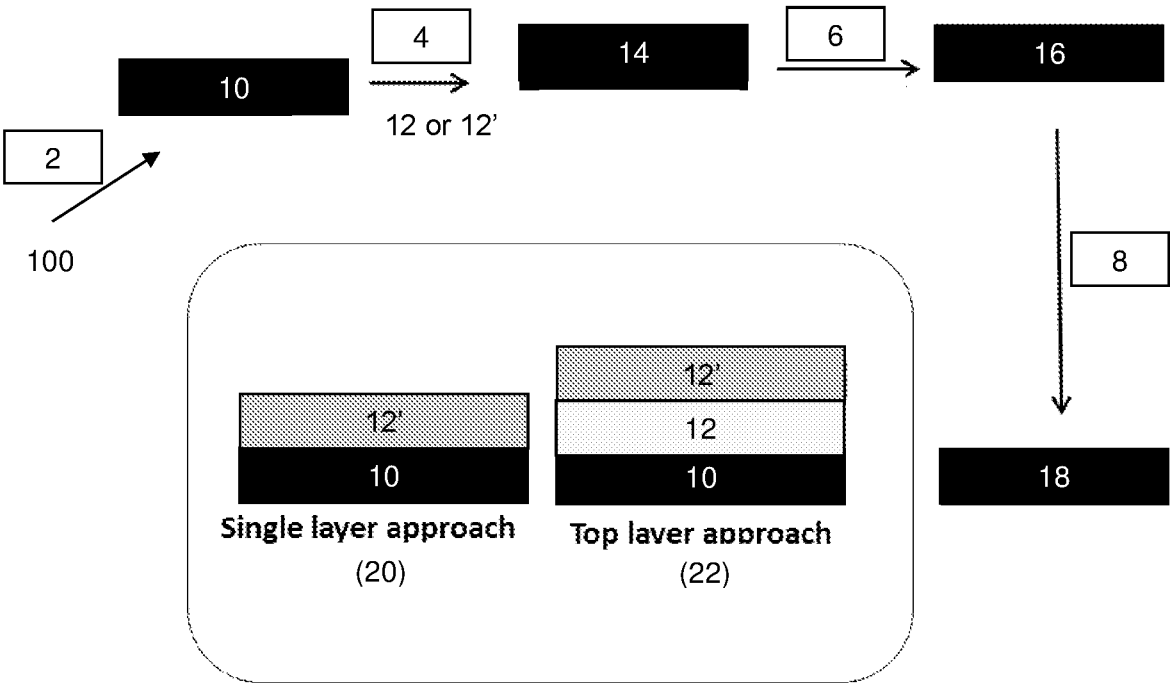


[Fig. 5]

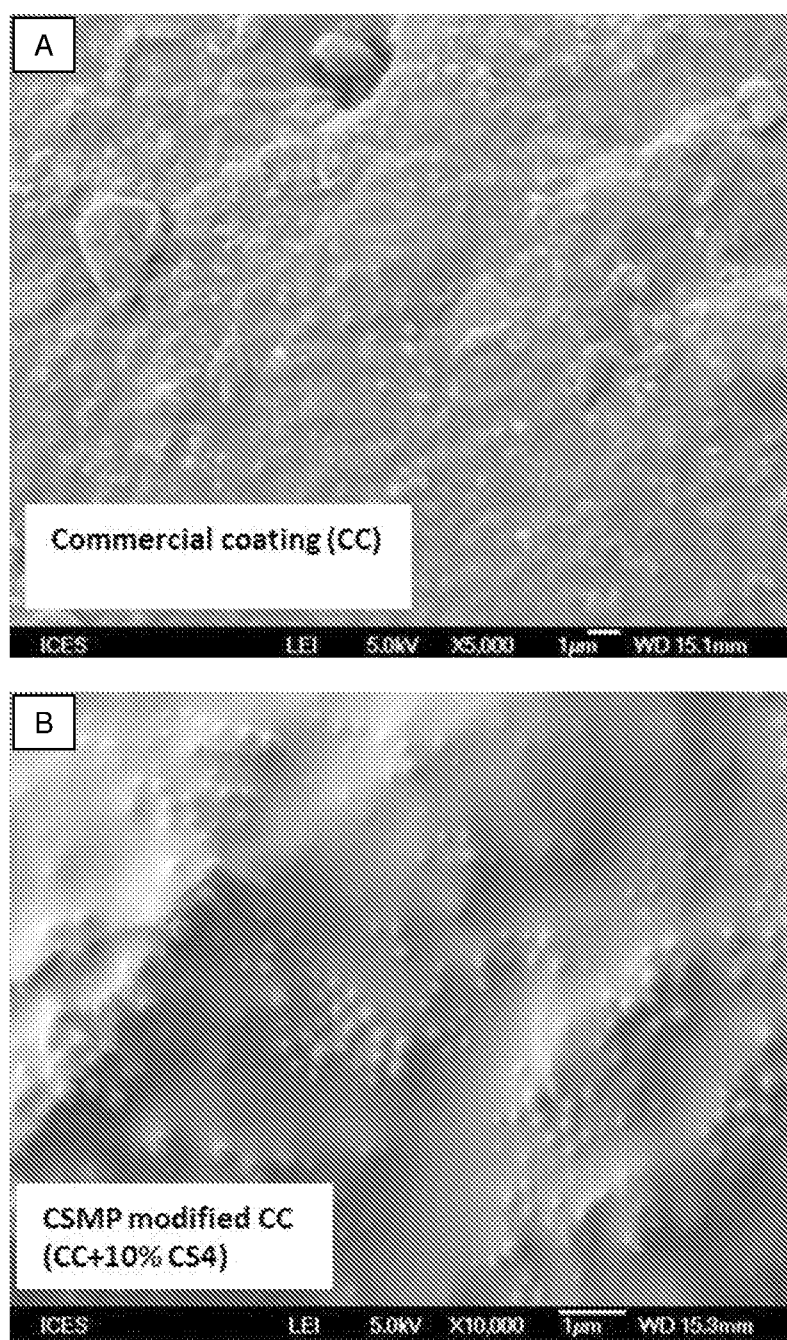


[Fig. 5]

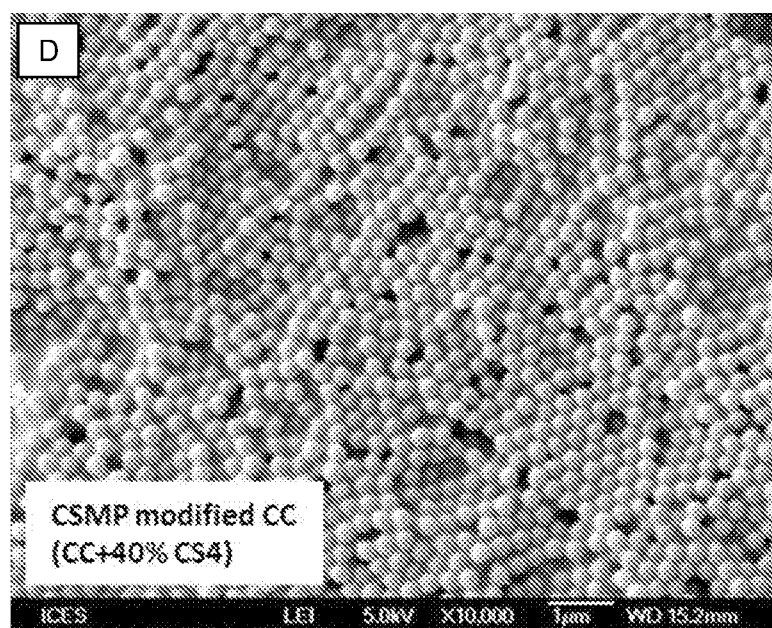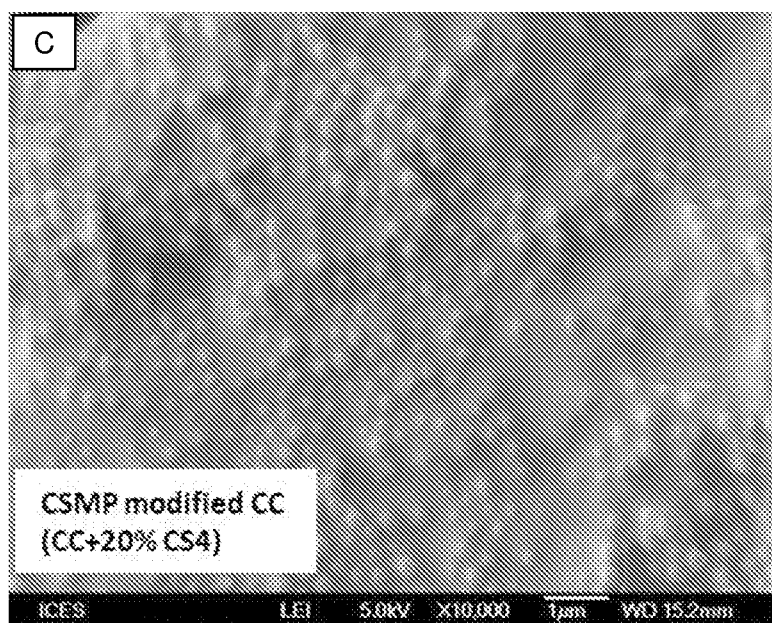


[Fig. 6]

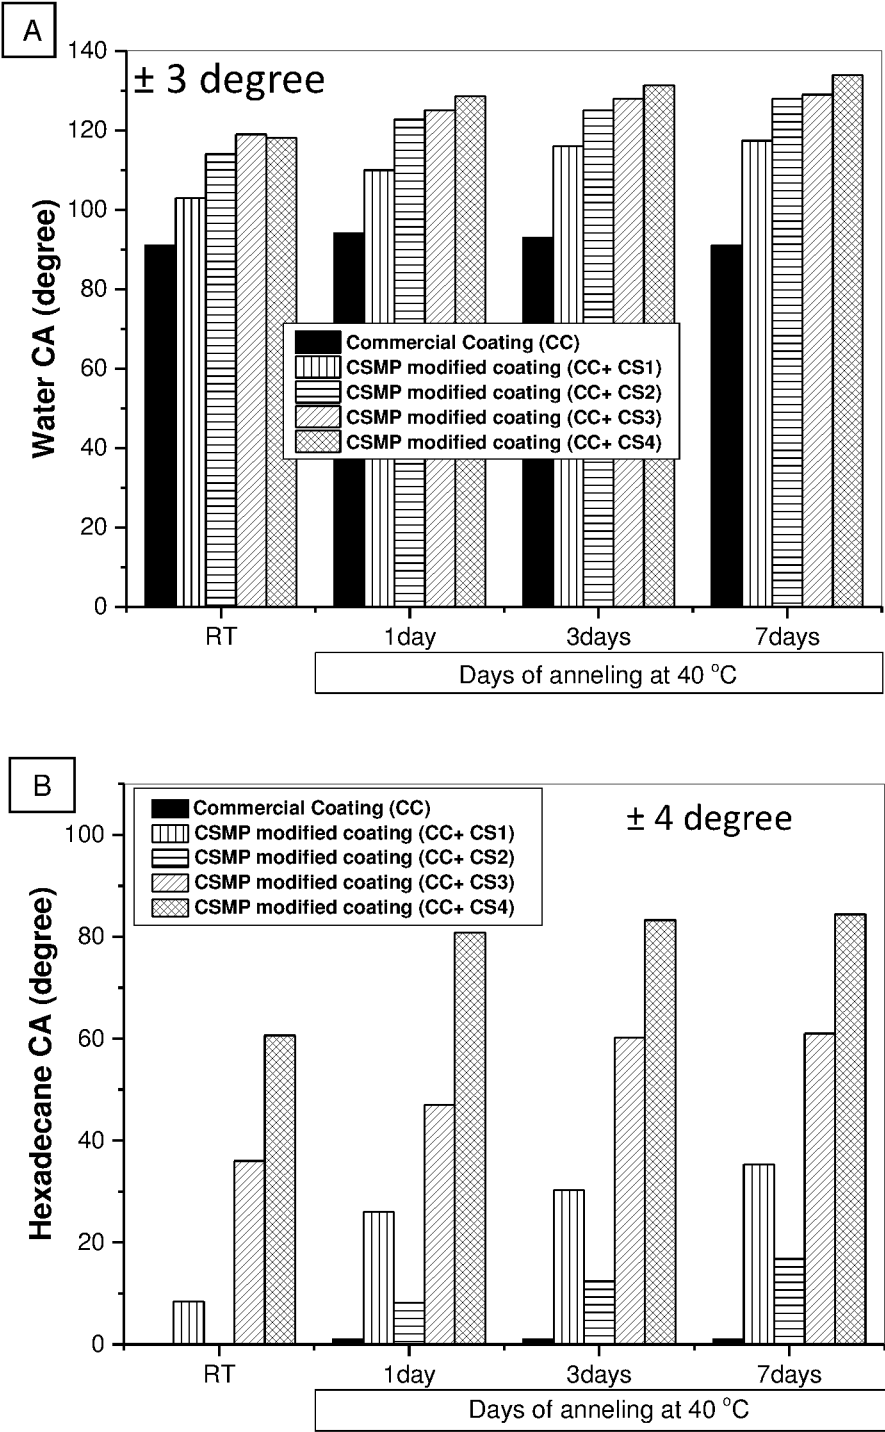


[Fig. 7]

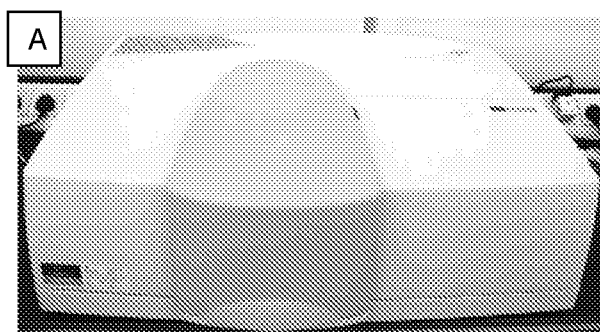


**Perkin-Elmer Lambda 950 UV/Vis/NIR
Spectrometer
(360 degree contour measurement)**

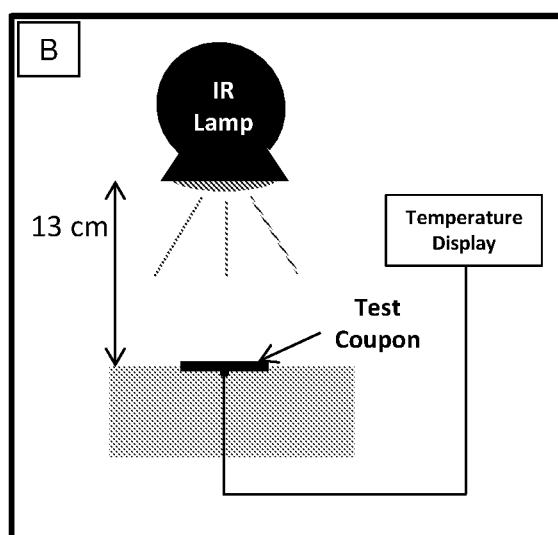

[Fig. 8]

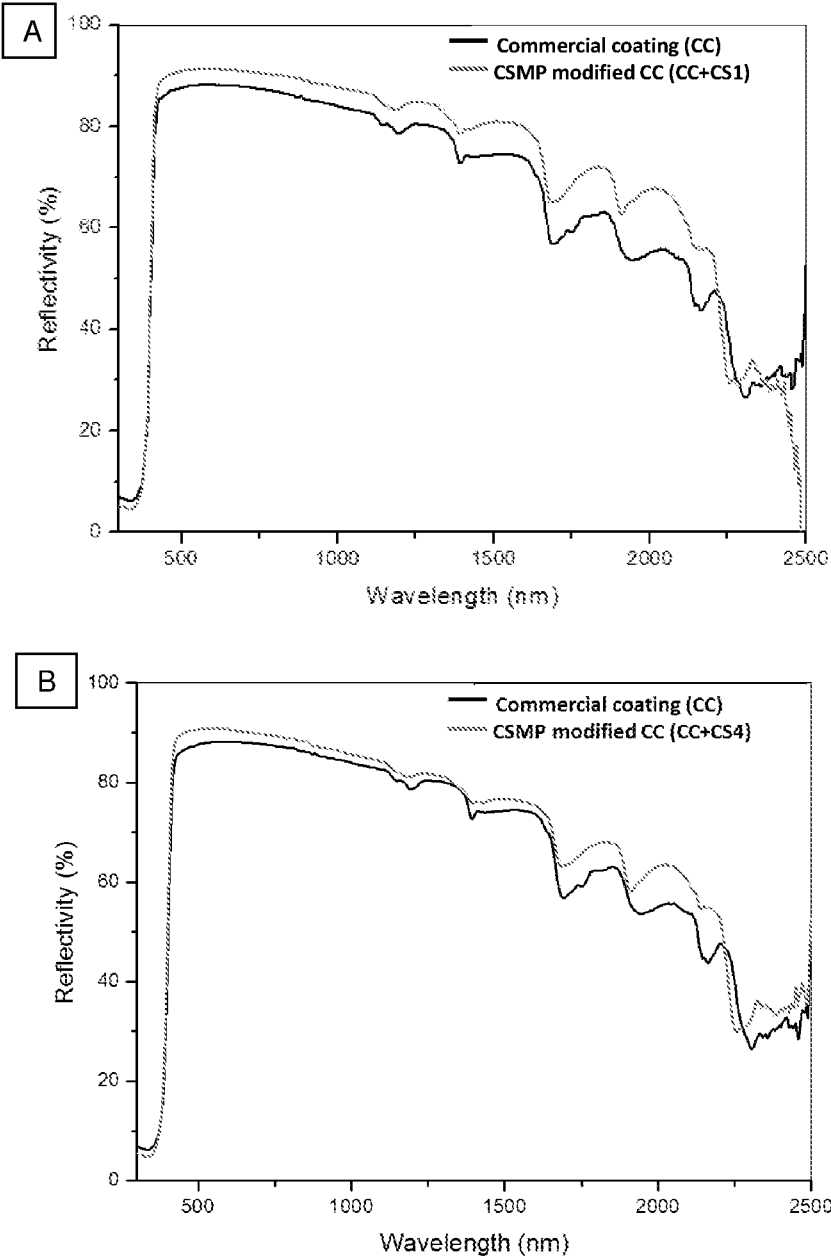


[Fig. 9]

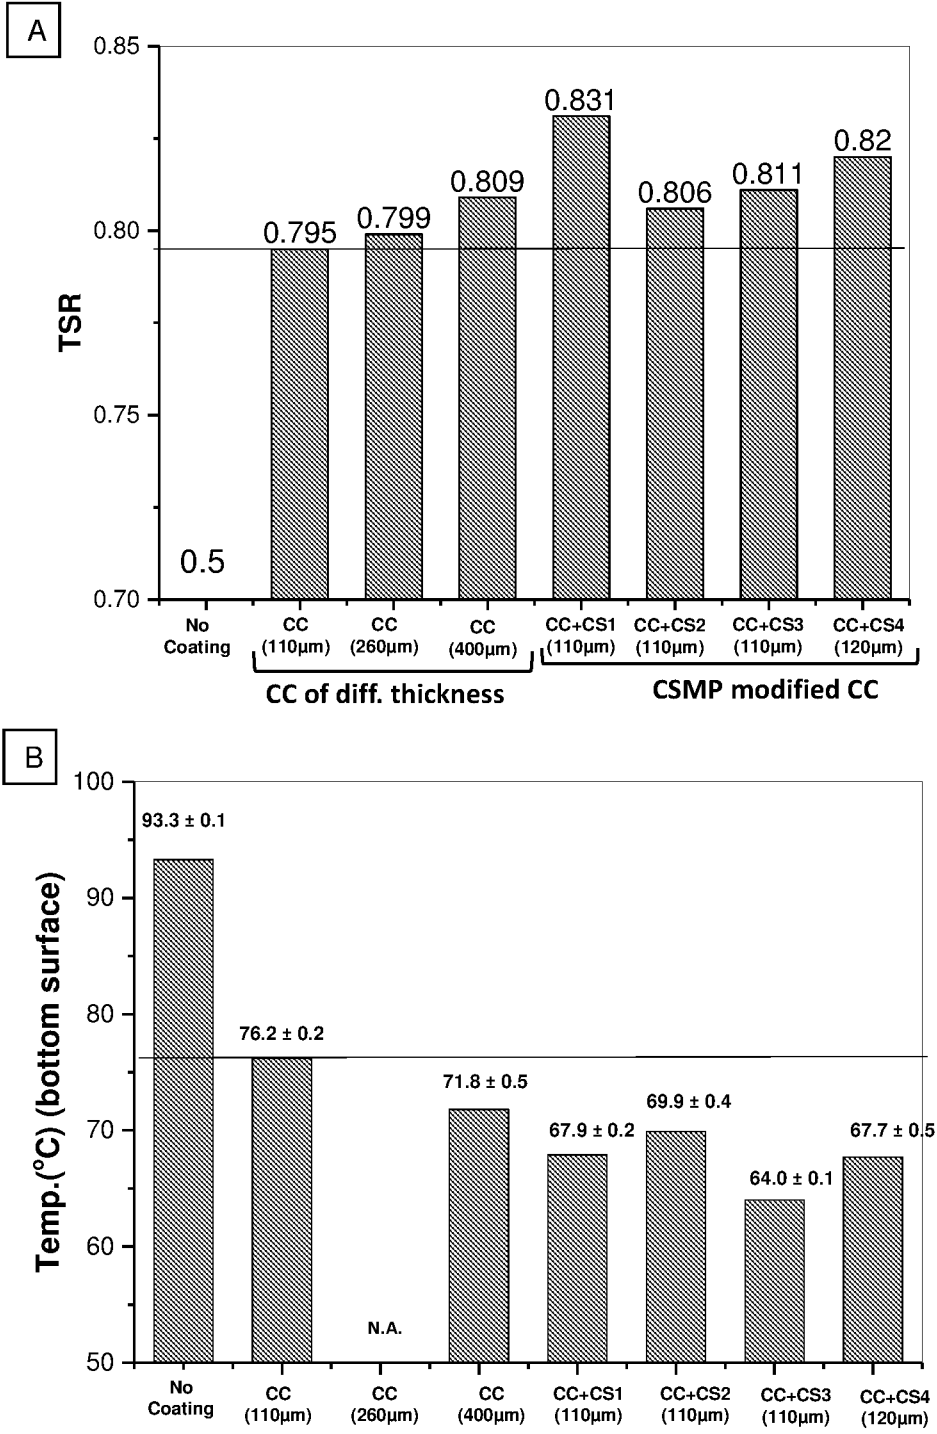


[Fig. 10]



A

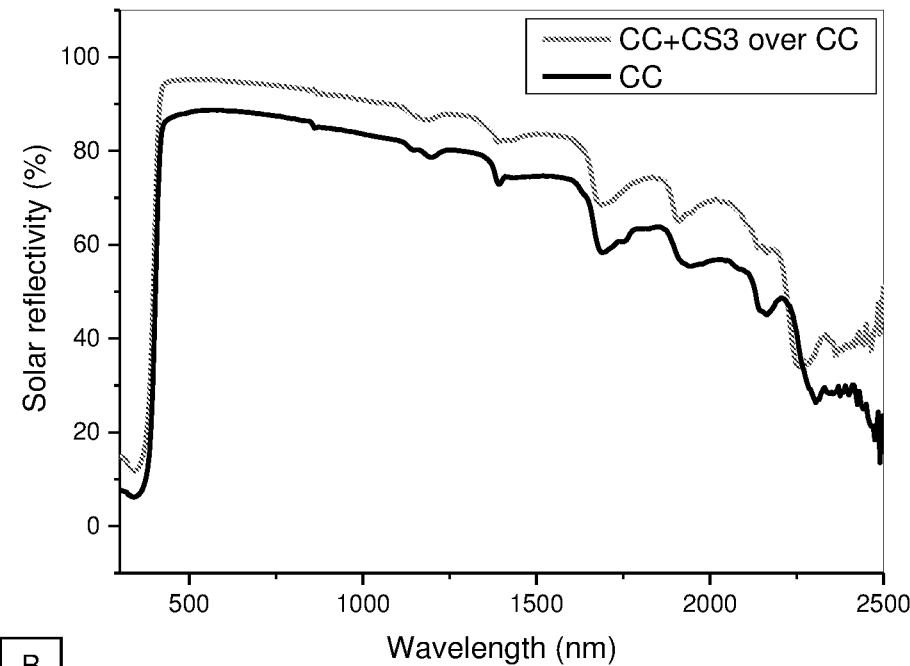


B

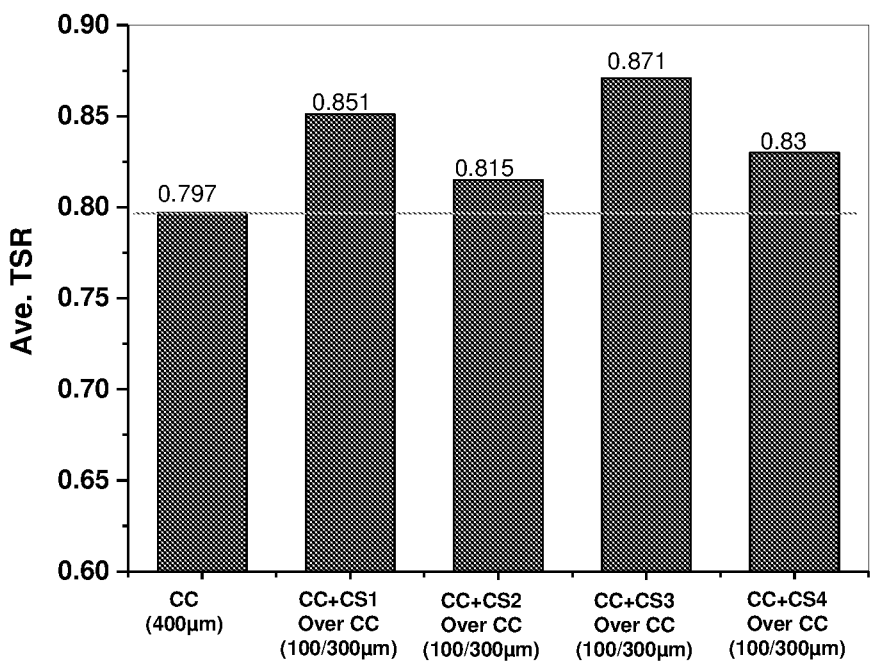


[Fig. 10]

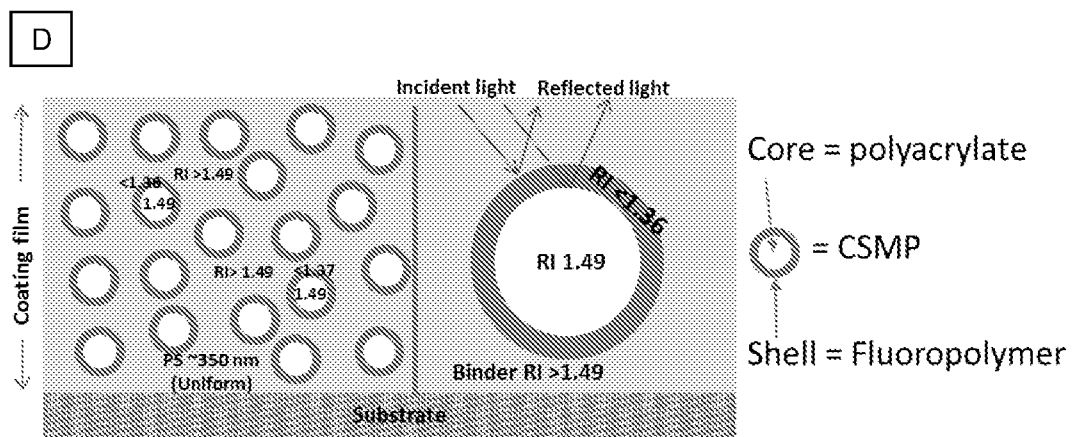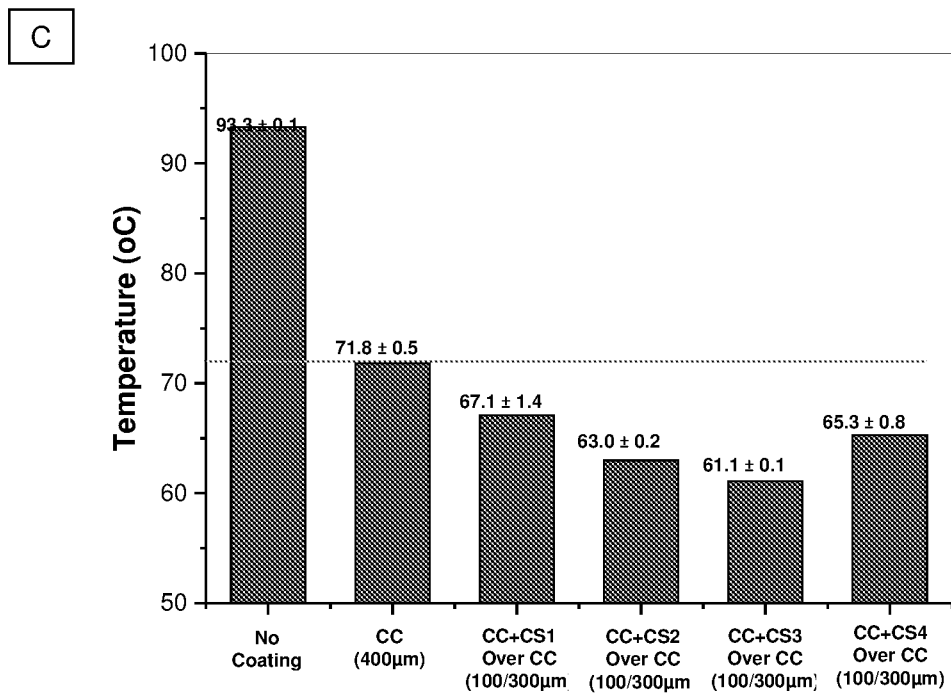


[Fig. 11]

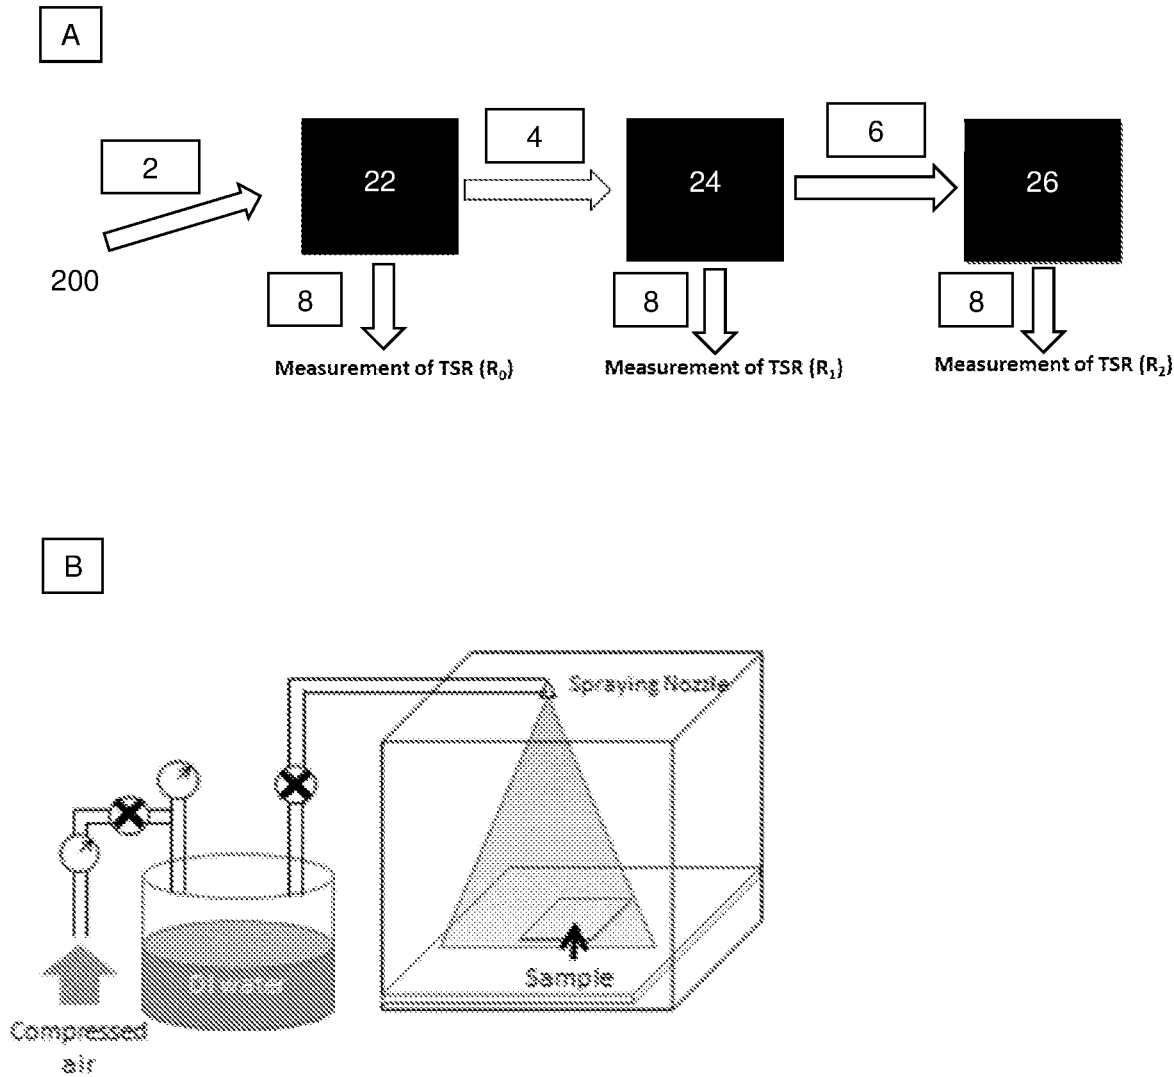


[Fig. 12]

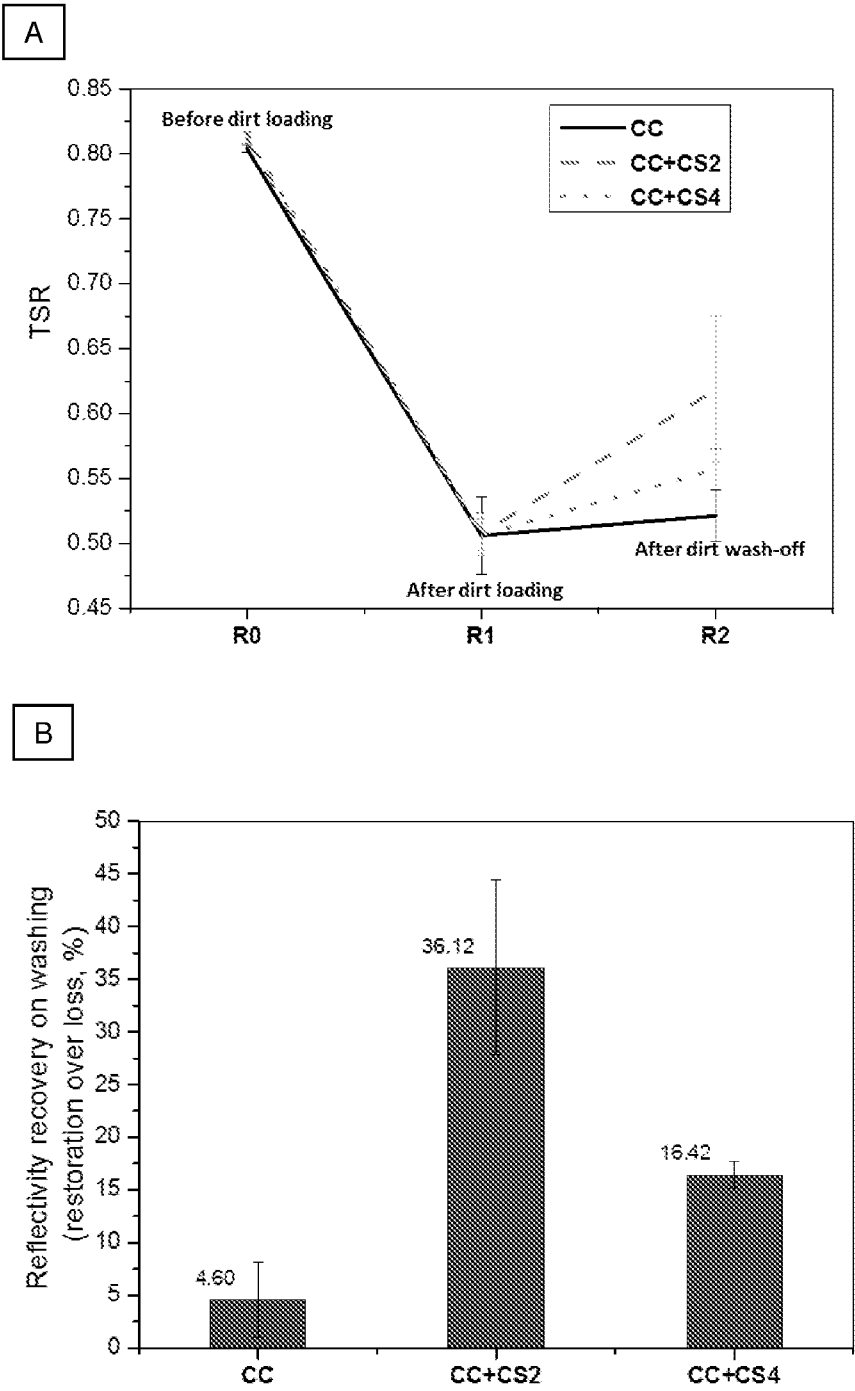

[Fig. 13]

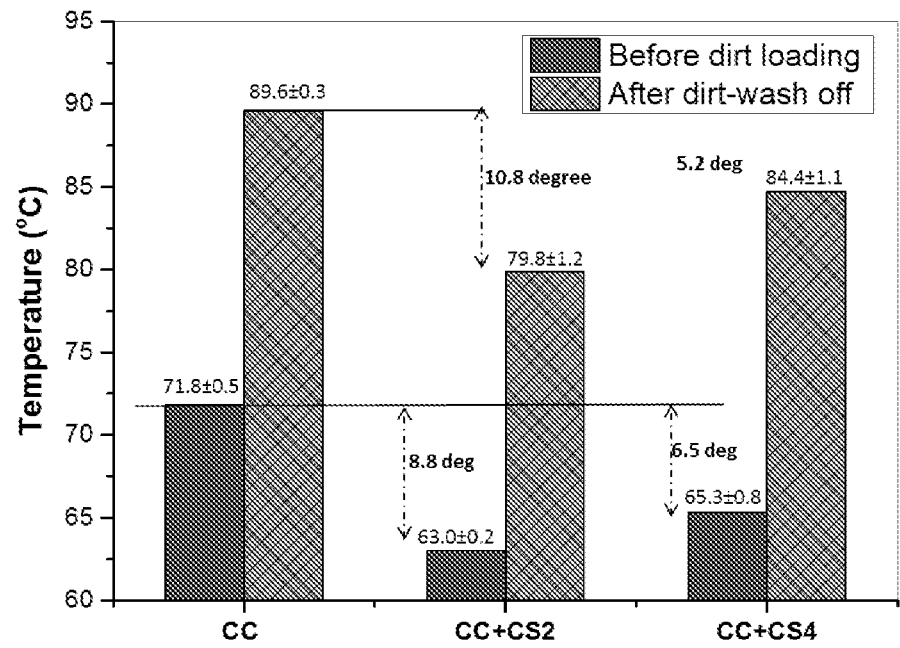


[Fig. 14]

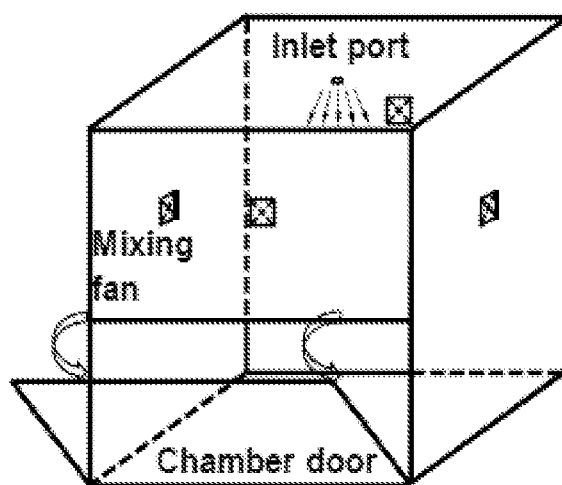

[Fig. 15]

A

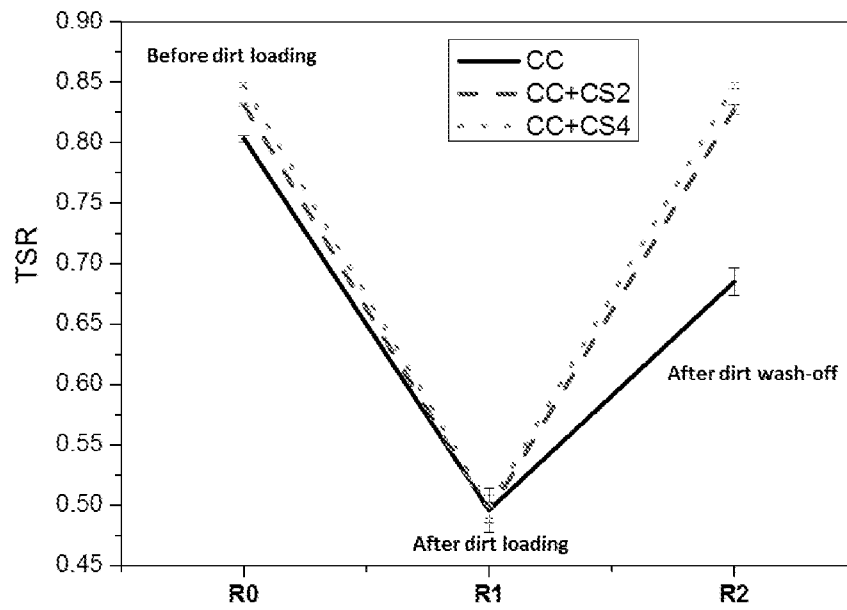

B

