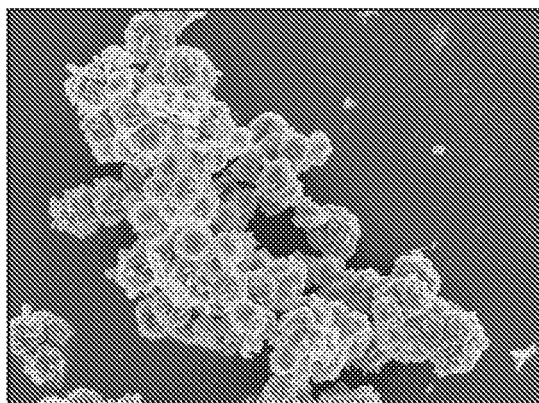
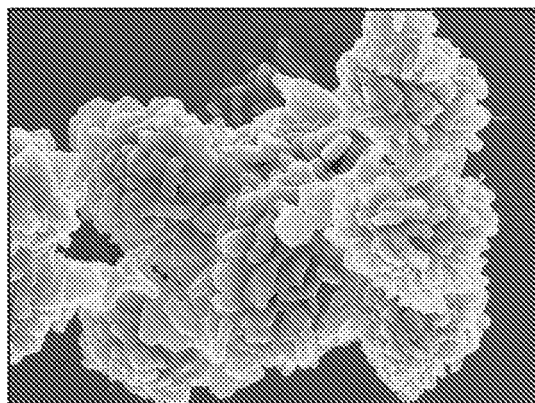
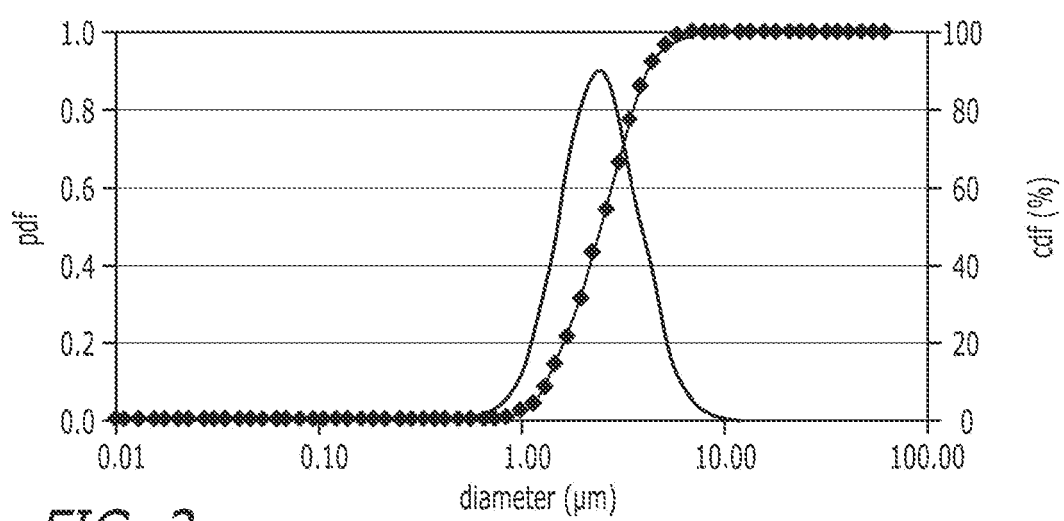


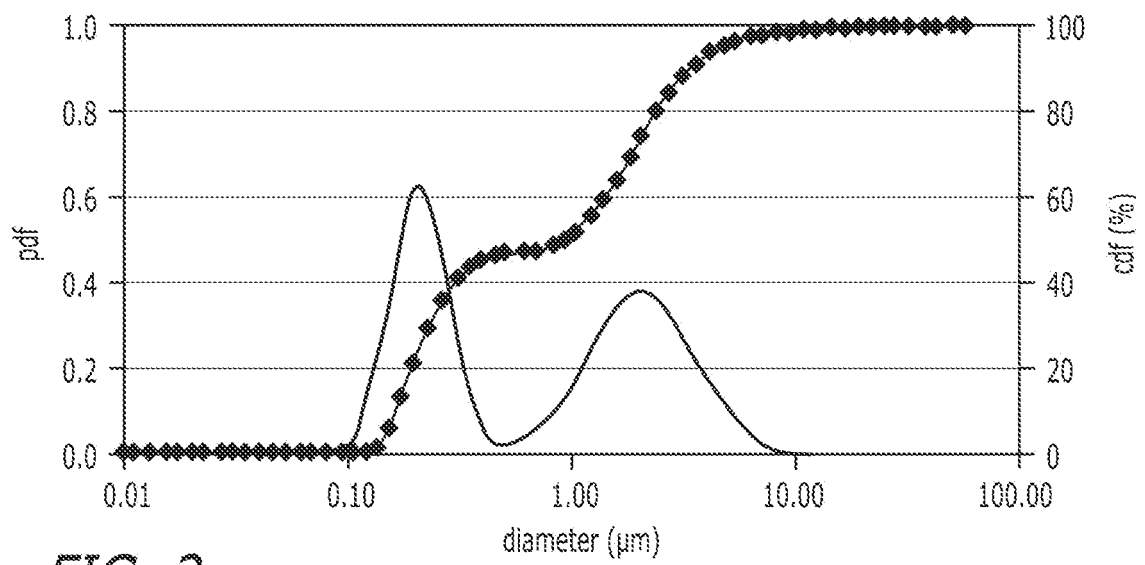
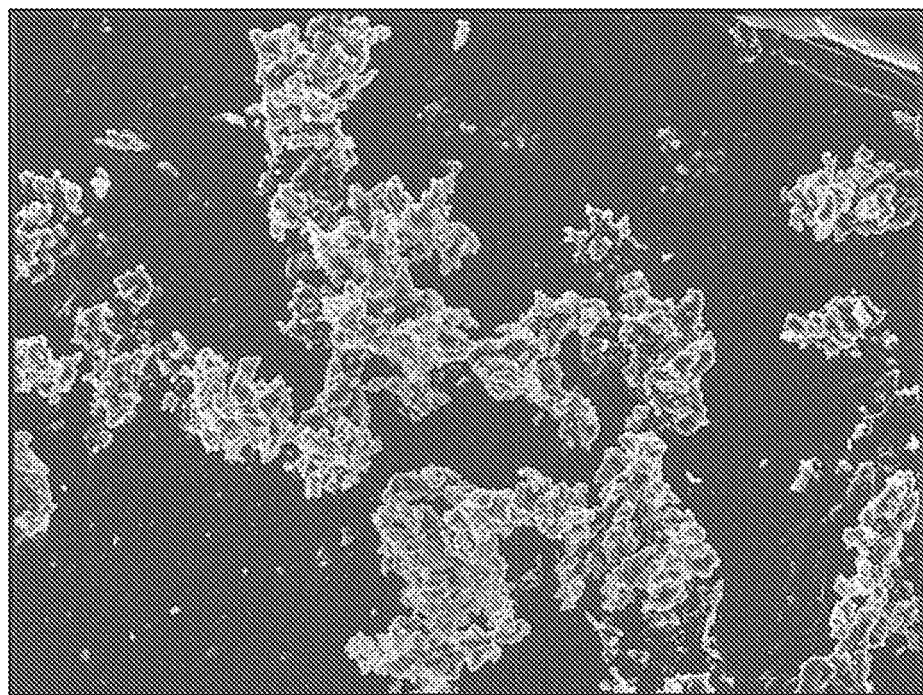
FIG. 1A

5 μm

FIG. 1B

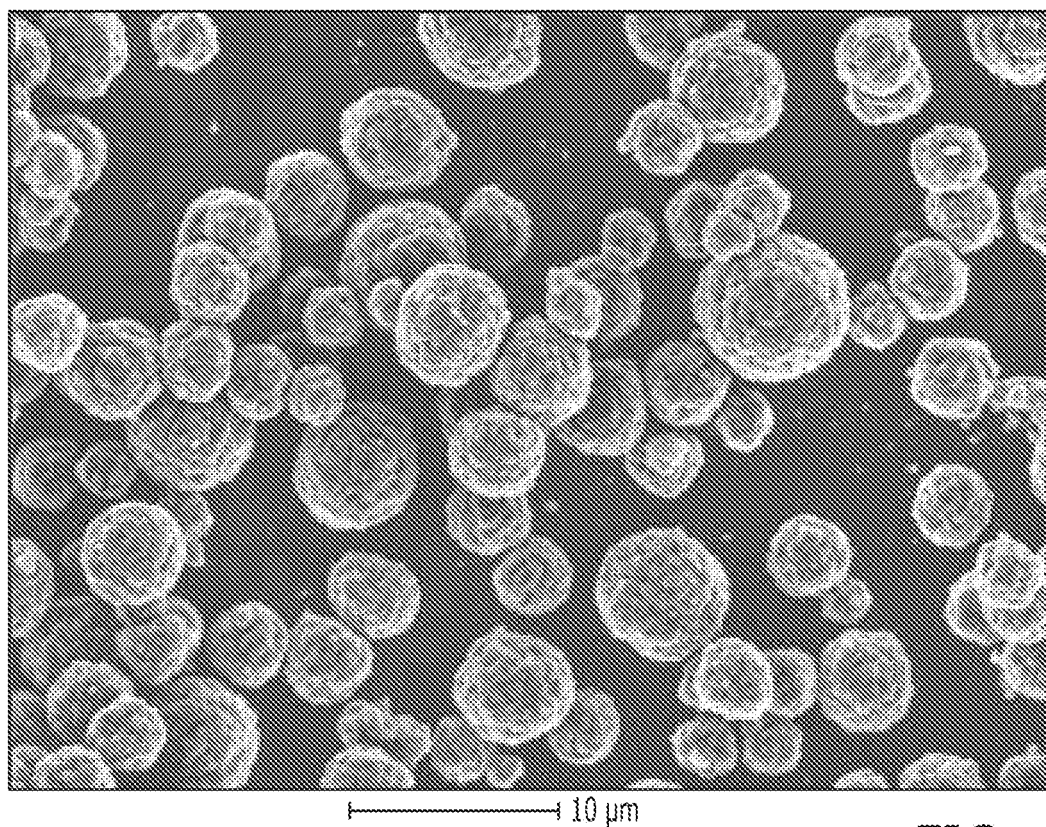
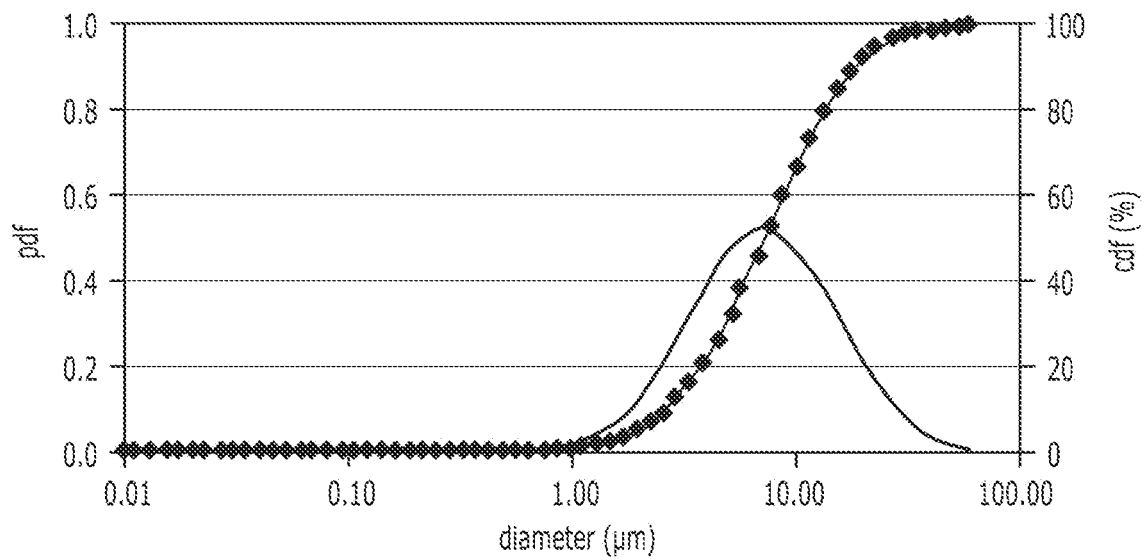
1 μm

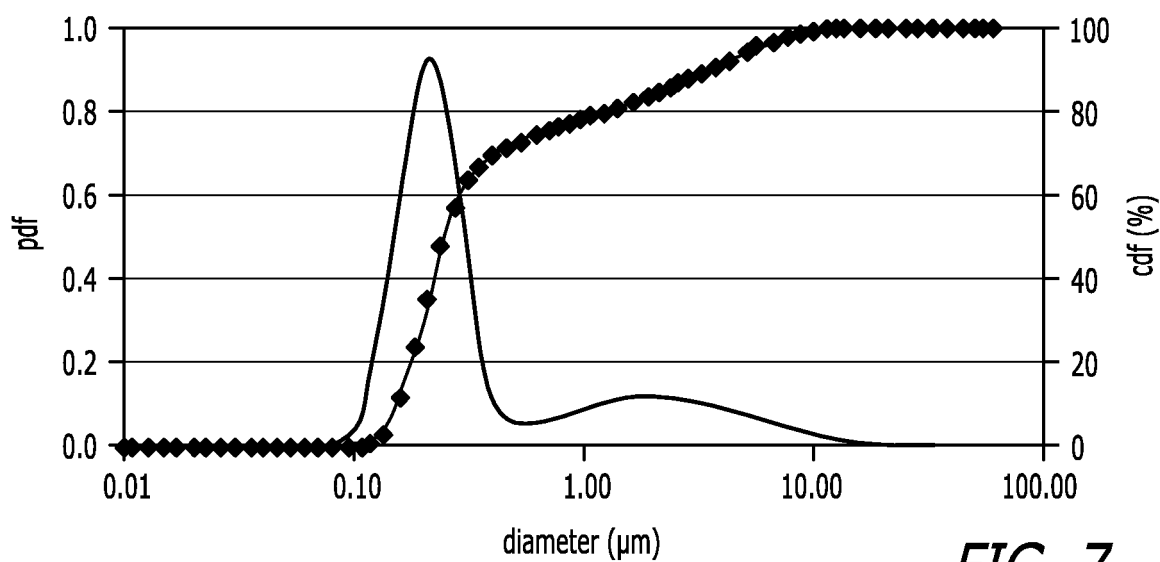
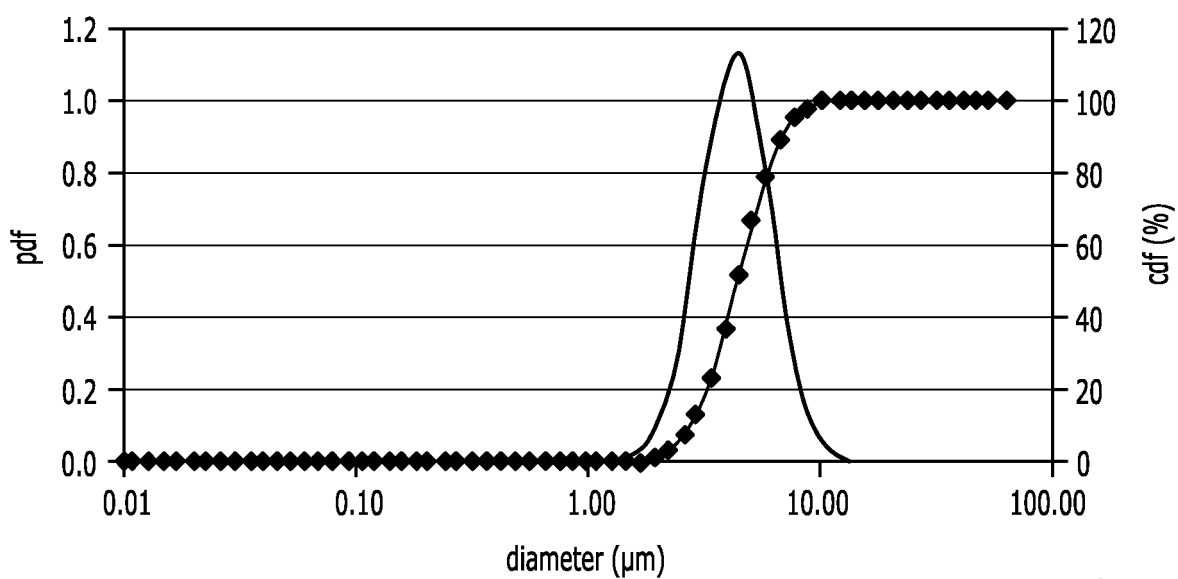
*FIG. 2*

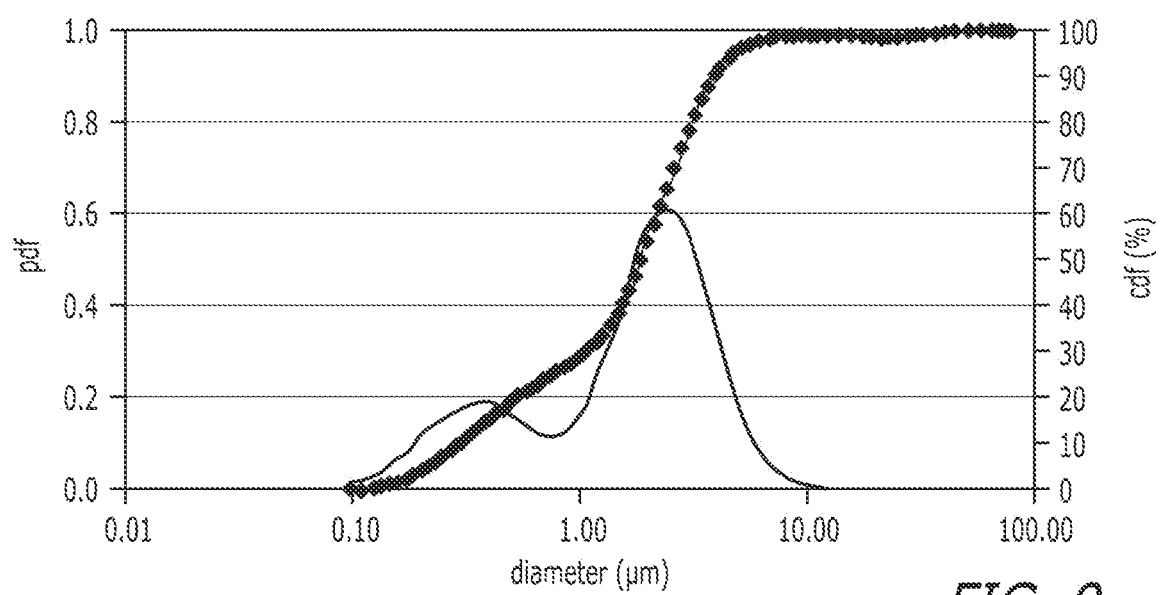
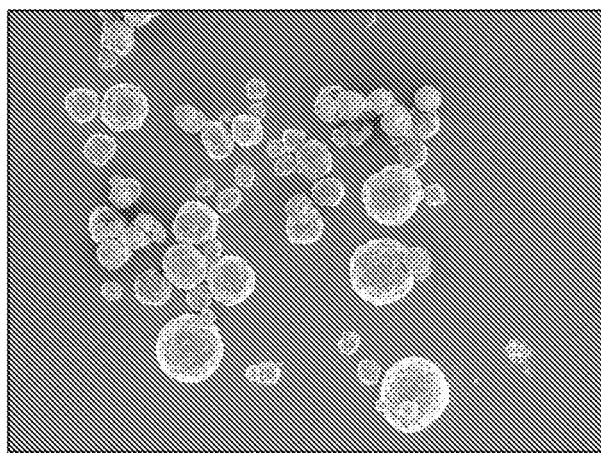
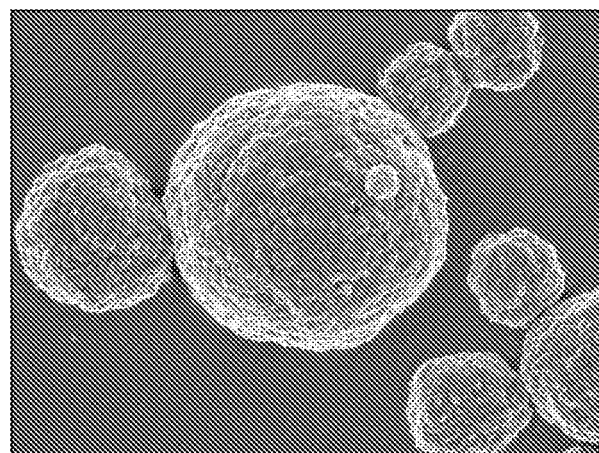
*FIG. 3*

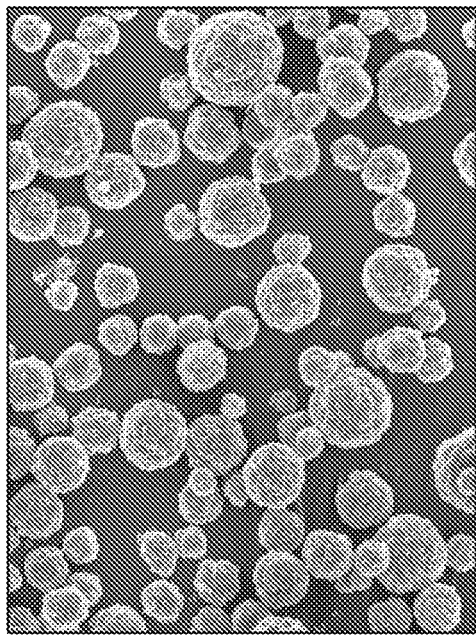
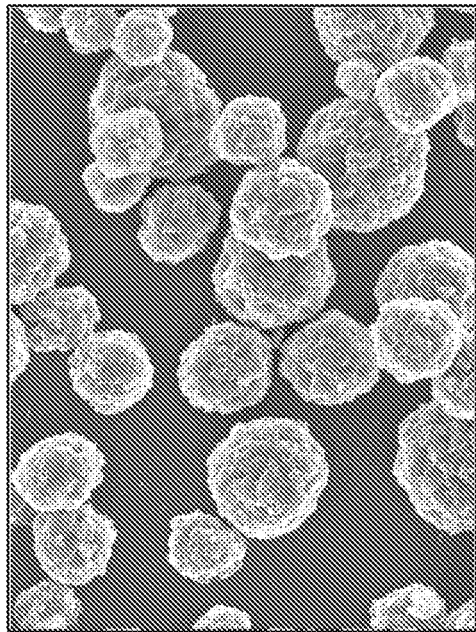
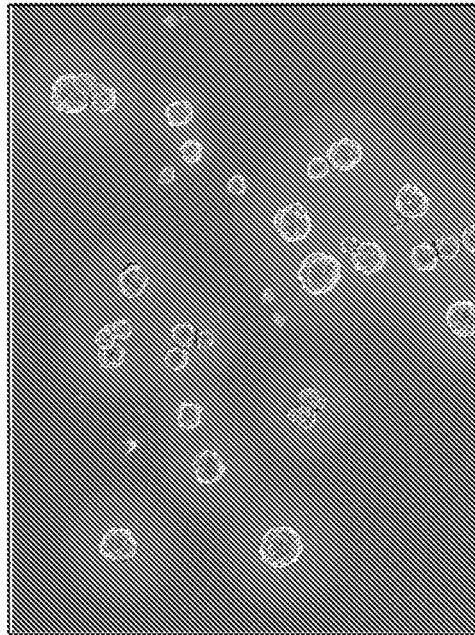
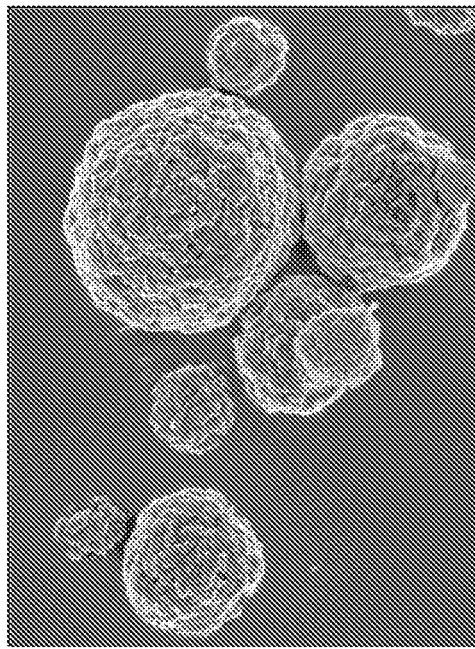
10 μm

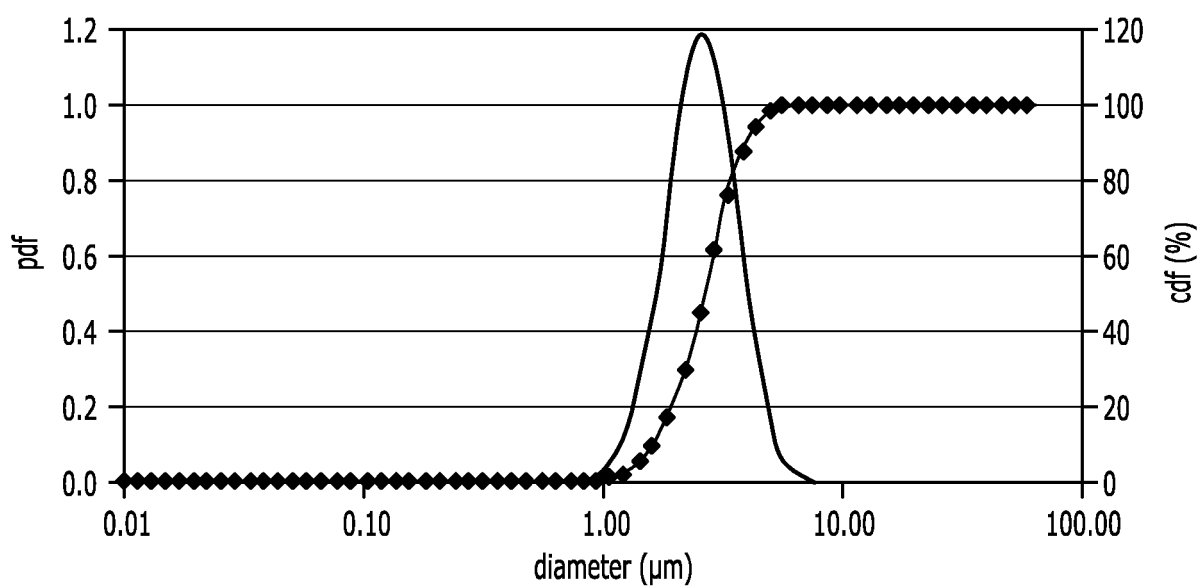
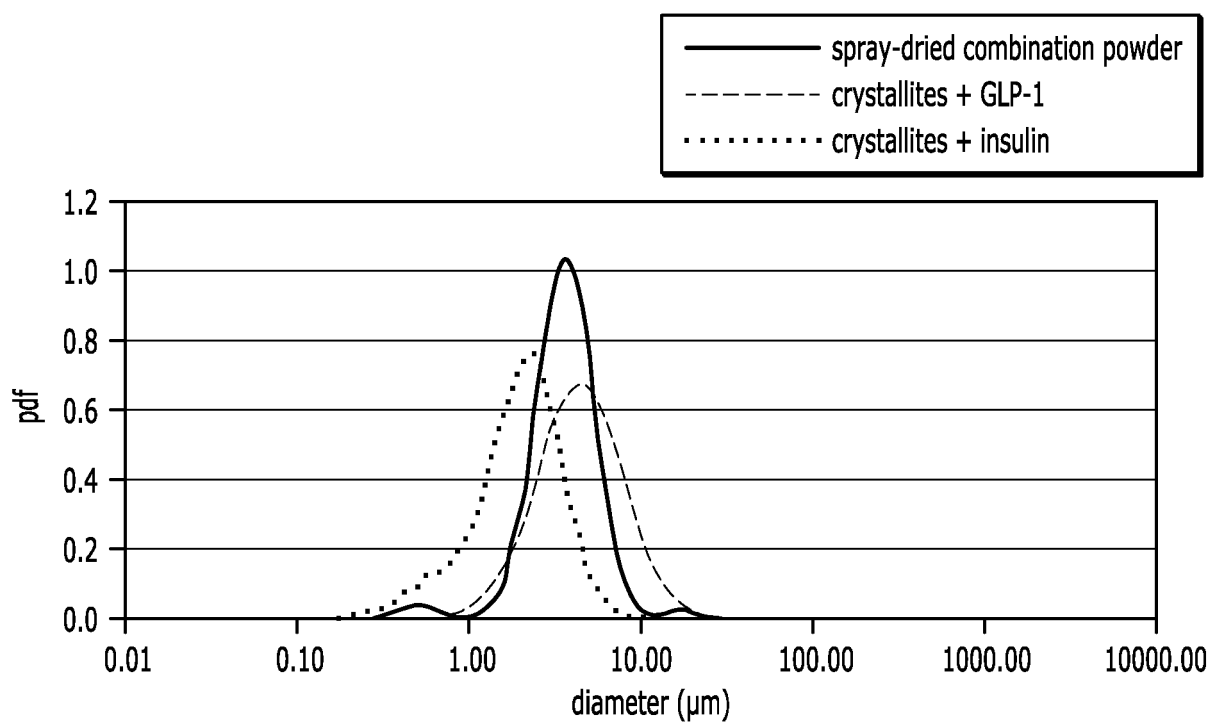
FIG. 4

FIG. 5*FIG. 6*

*FIG. 7**FIG. 8*

*FIG. 9*10 μm *FIG. 10A*2 μm *FIG. 10B*

*FIG. 11A**FIG. 11B**FIG. 12A**FIG. 12B*

*FIG. 13**FIG. 14*