

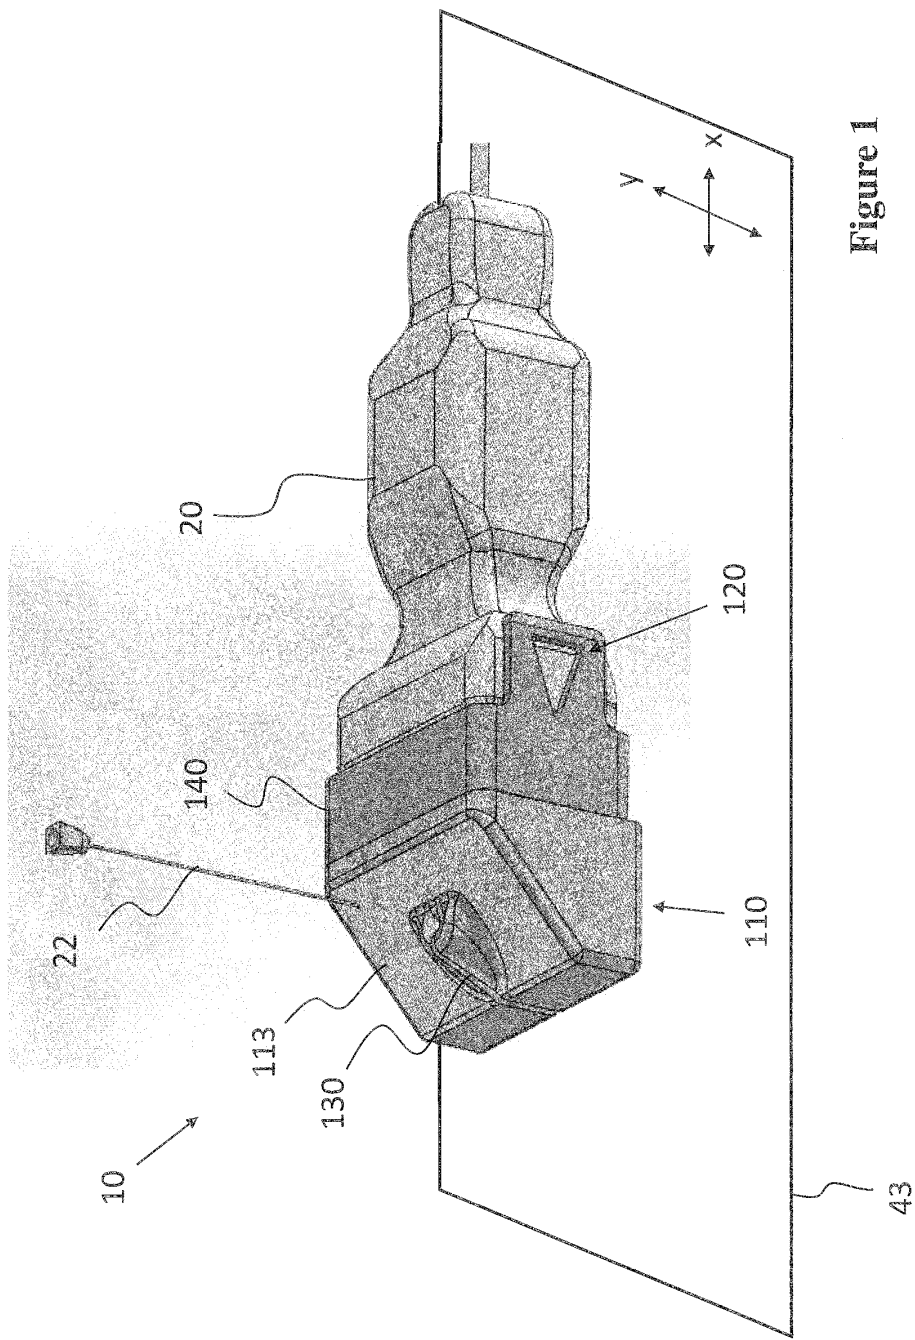


Figure 1

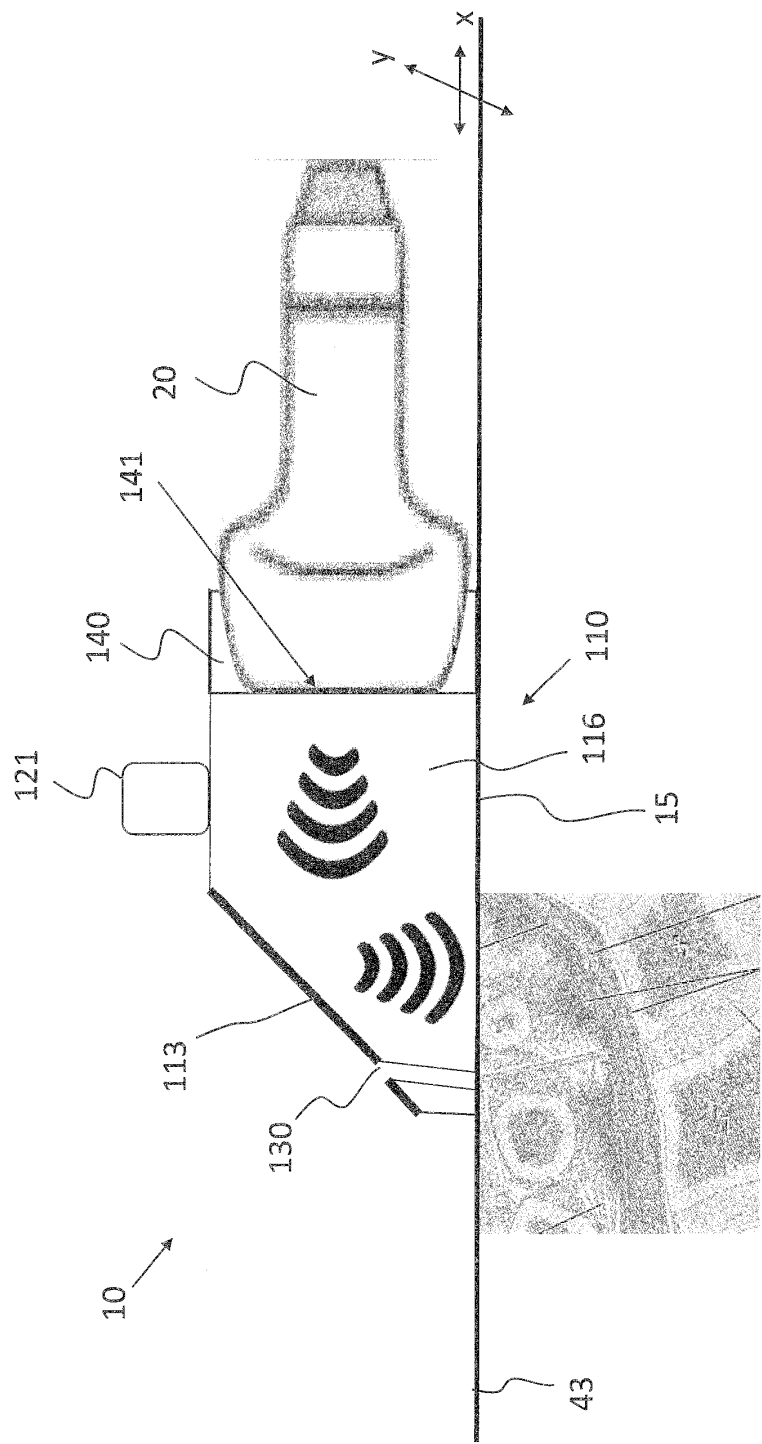


Figure 2

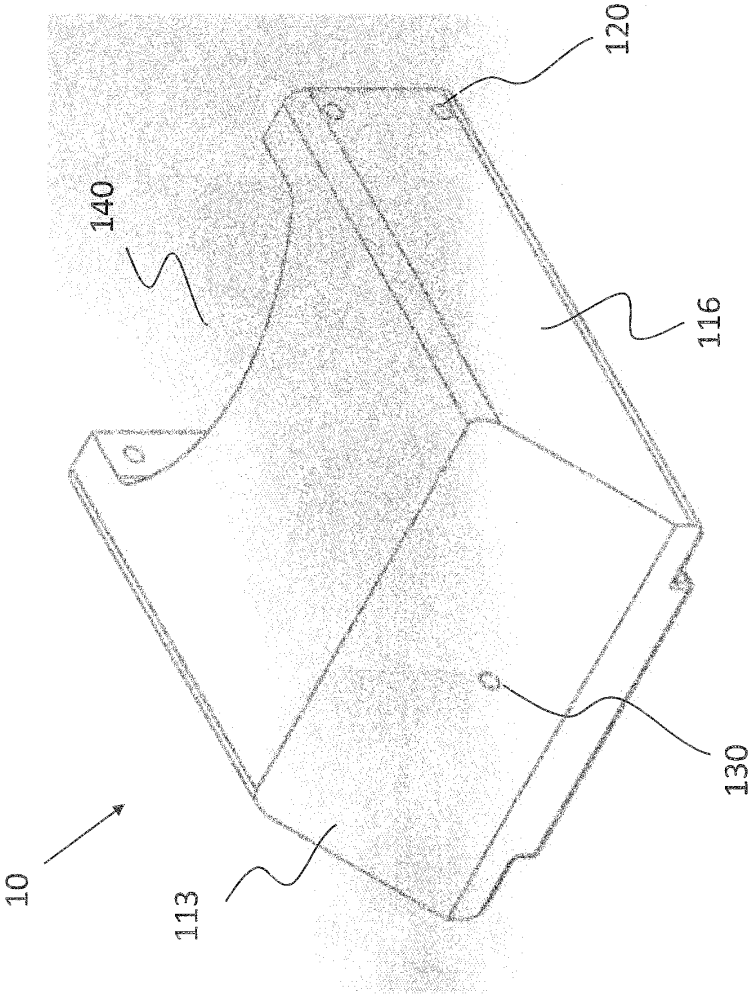


Figure 3

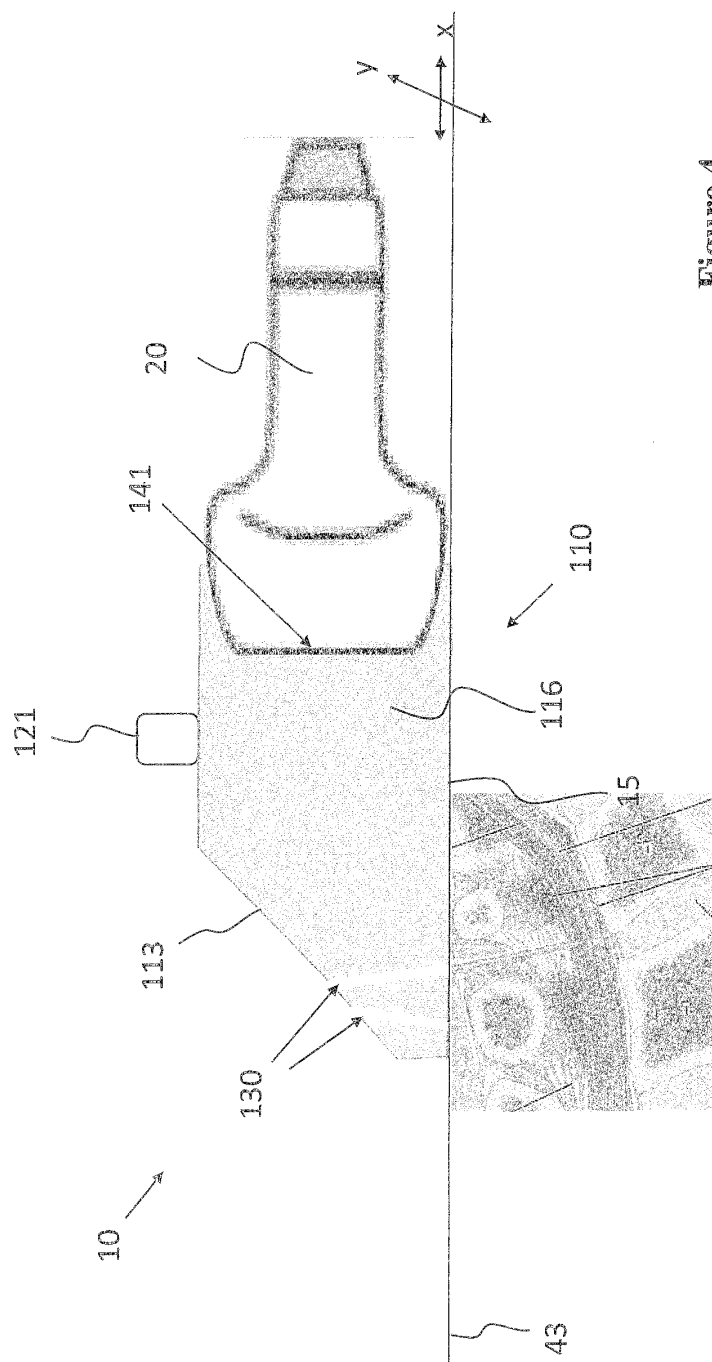


Figure 4

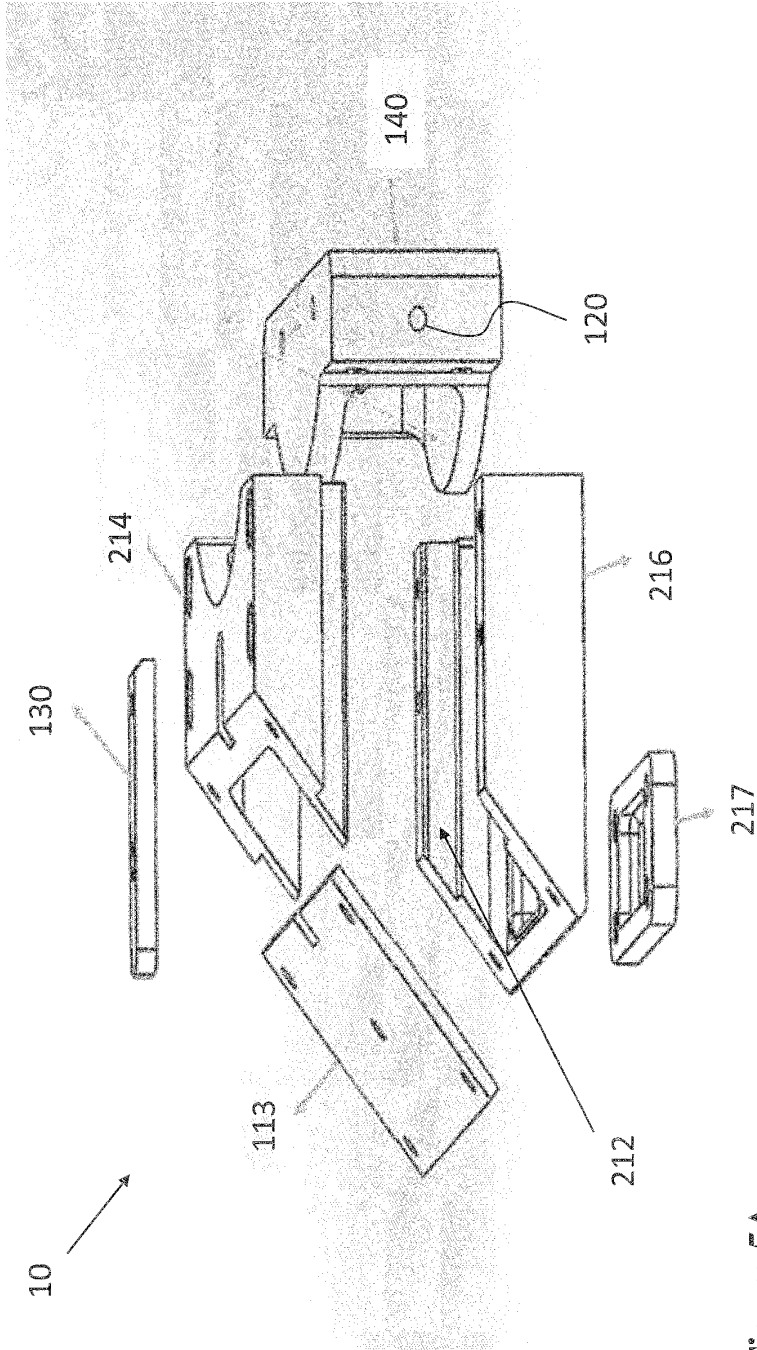


Figure 5A

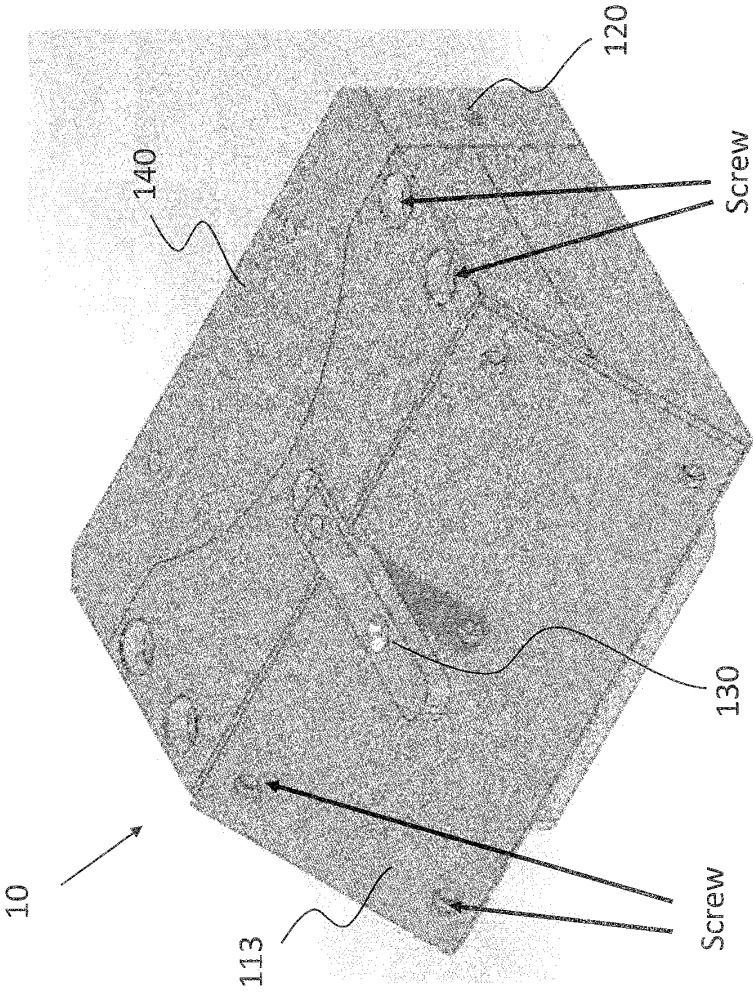


Figure 5B

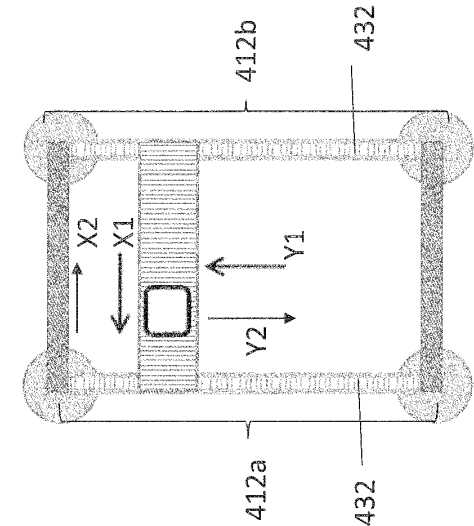


Figure 6B

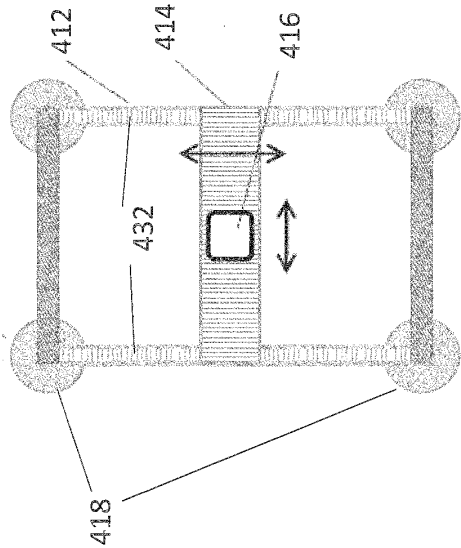


Figure 6A

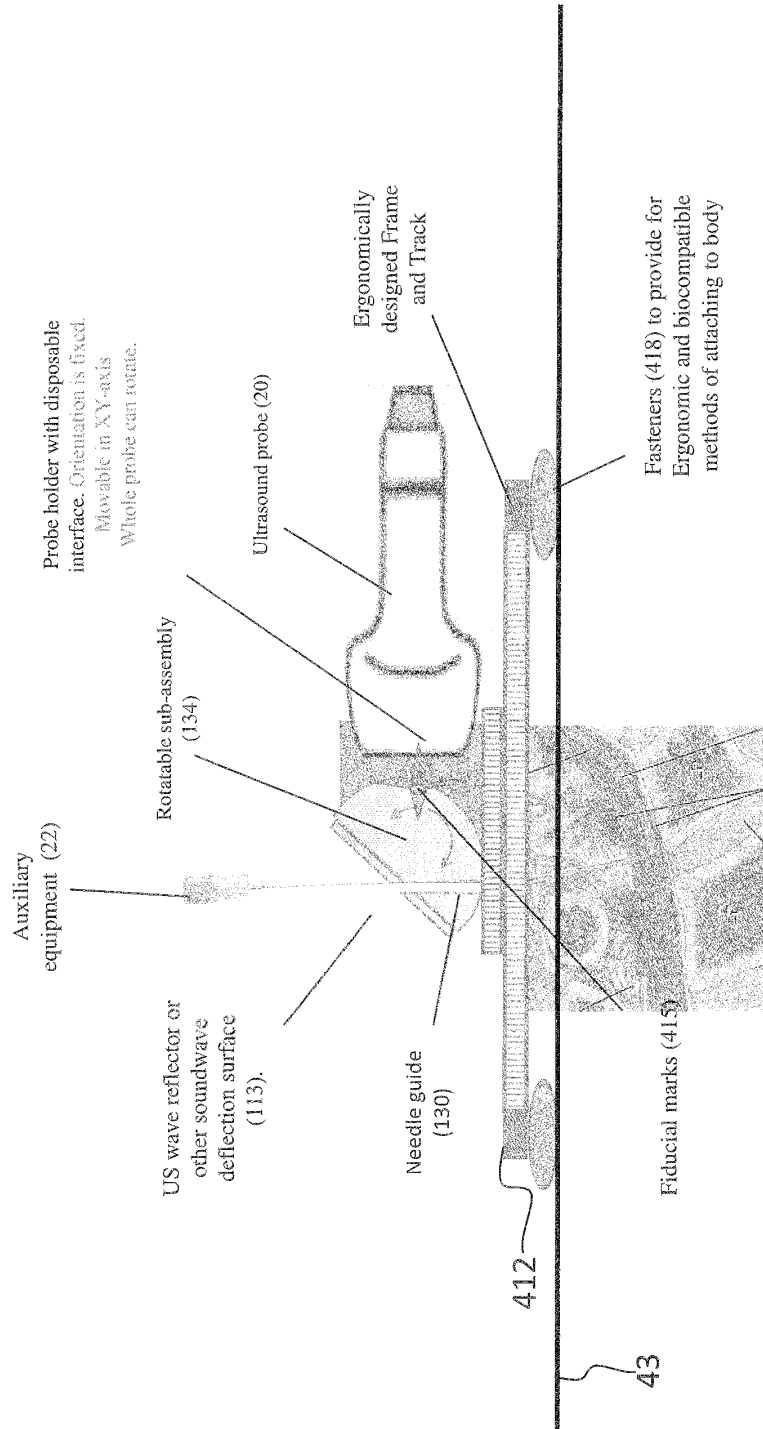


Figure 7A

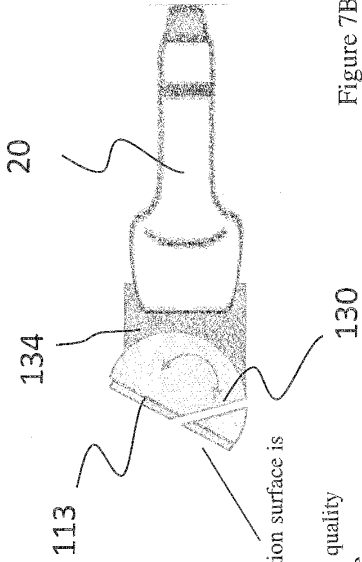


Figure 7B

The angle of the soundwave deflection surface is adjustable to:

- 1) Get the best ultrasound image quality
- 2) Change the focus of the image

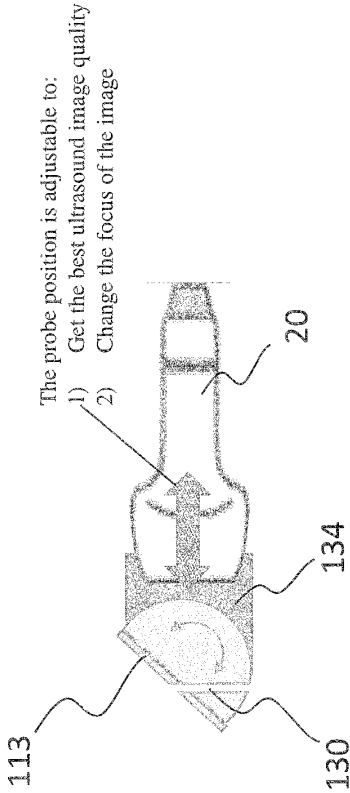


Figure 7C

The probe position is adjustable to:

- 1) Get the best ultrasound image quality
- 2) Change the focus of the image

The angle of the probe and the auxiliary equipment receiver is adjustable to:

- 1) Get the best ultrasound image quality
- 2) Get the best angle for needle penetration

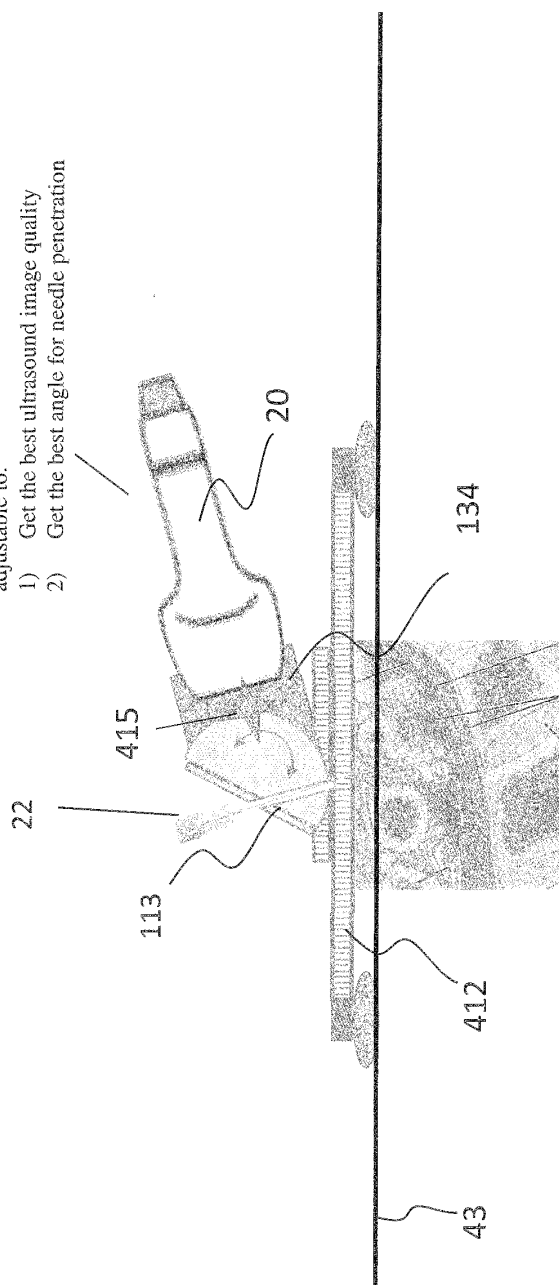


Figure 7D


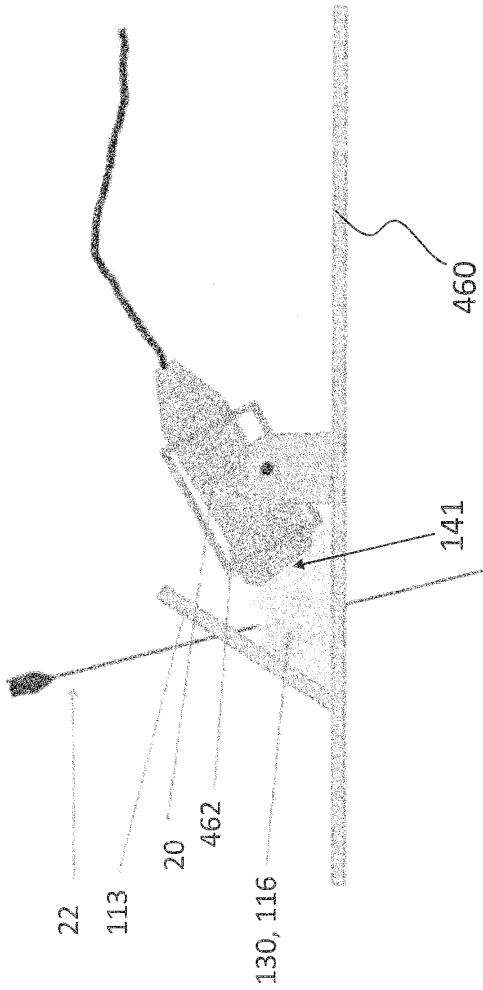


Figure 8

12/13

Figure 9

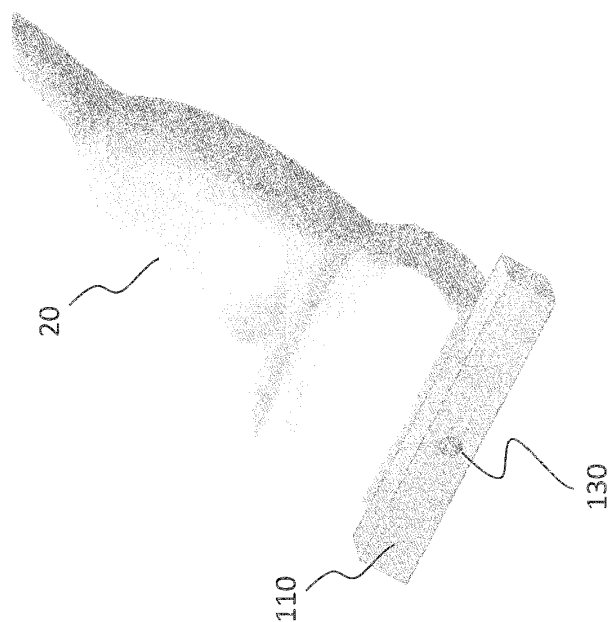

13/13




Figure 10B




Figure 10A