

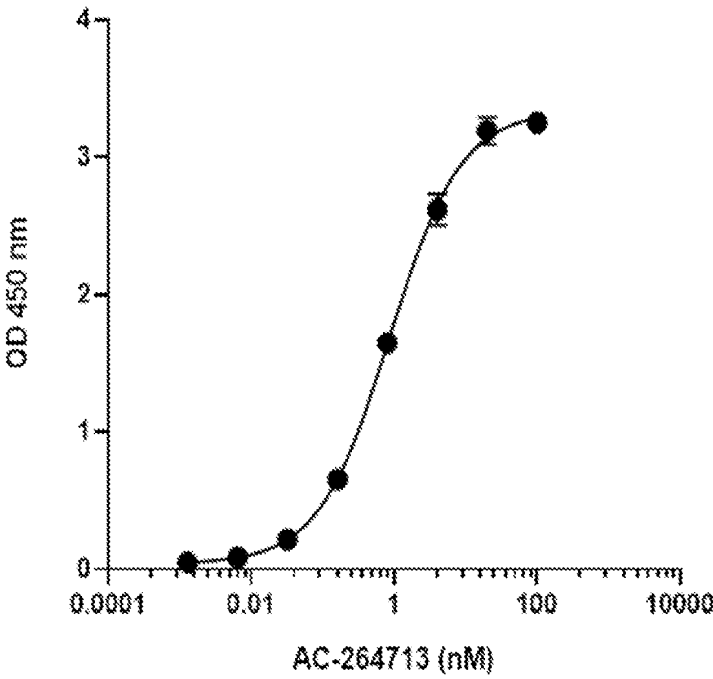


FIG. 1



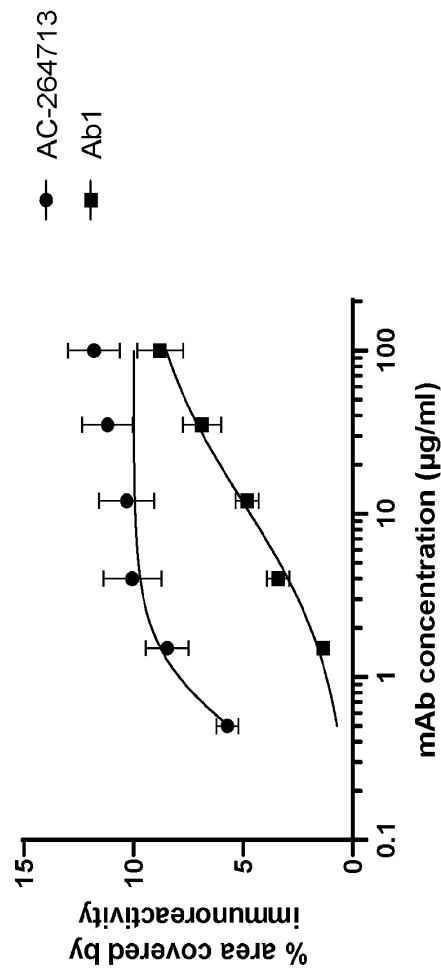


FIG 2

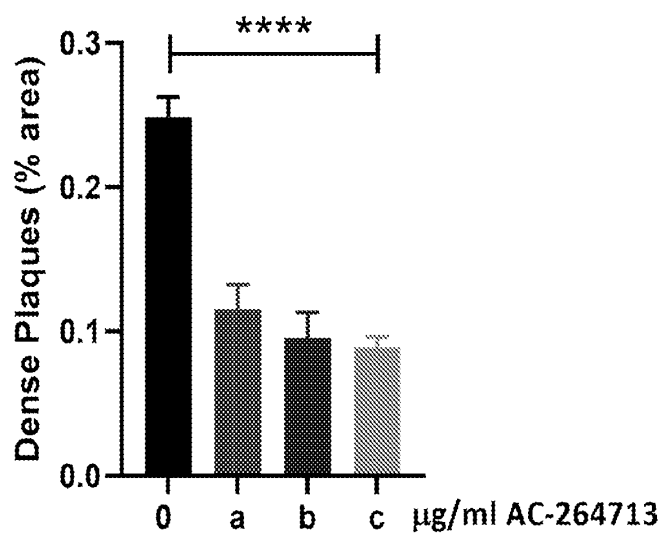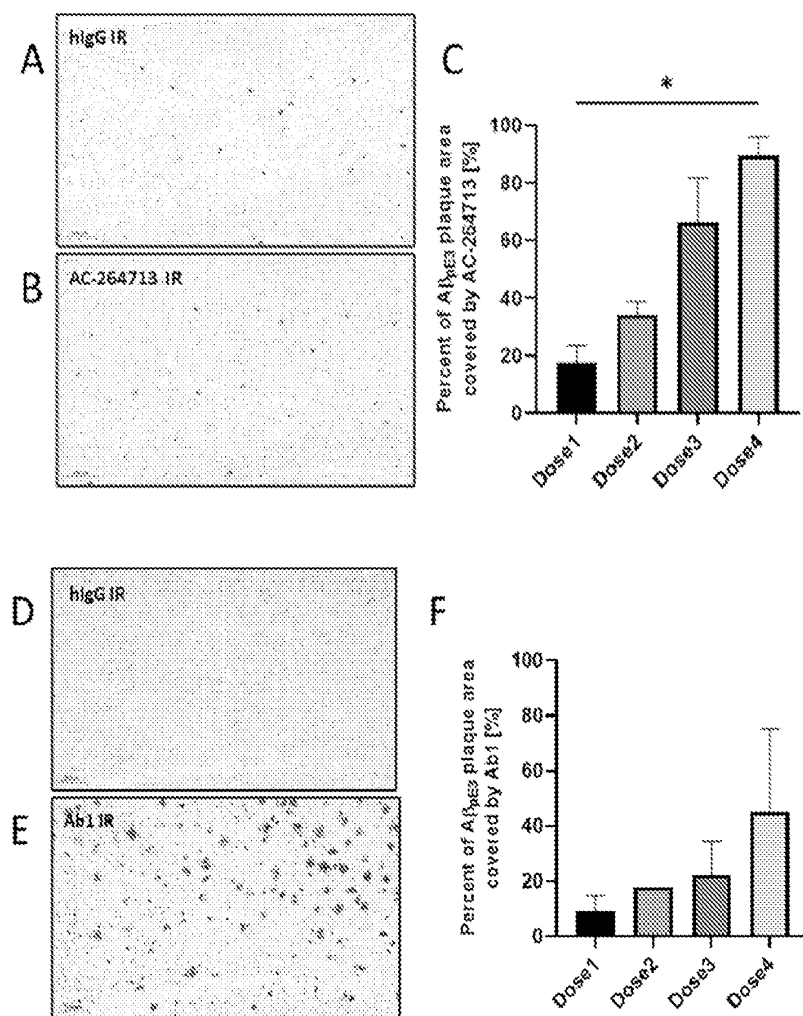

**** $P < 0.0001$ for comparison of concentrations a, b or c µg/mL to 0 ug/mL (One-way ANOVA followed by Dunnett's multiple comparisons test).

FIG 3

**FIG 4**

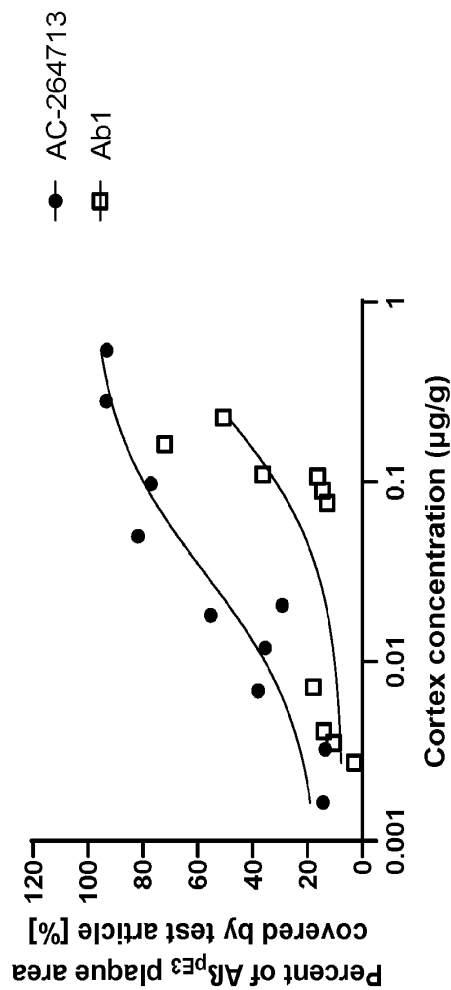


FIG 5

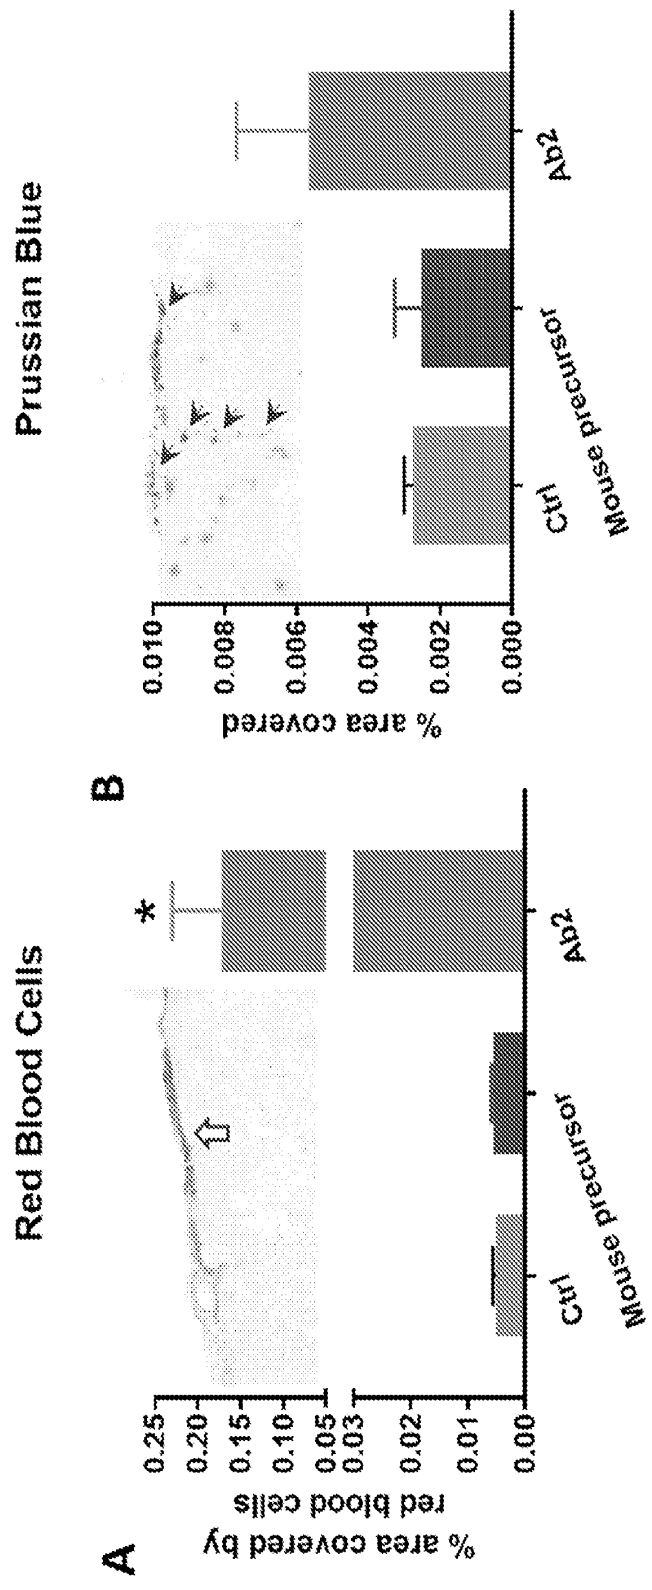


FIG 6