



[図1]

Fig.1

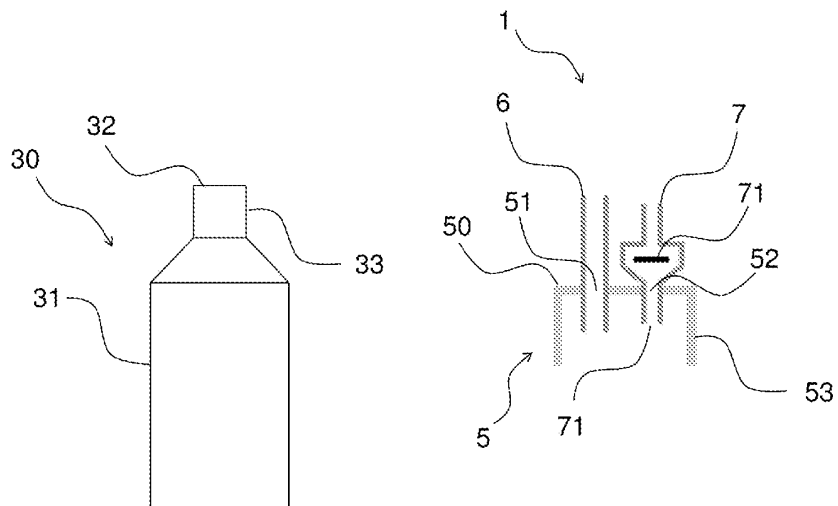


[図2]


Fig.2

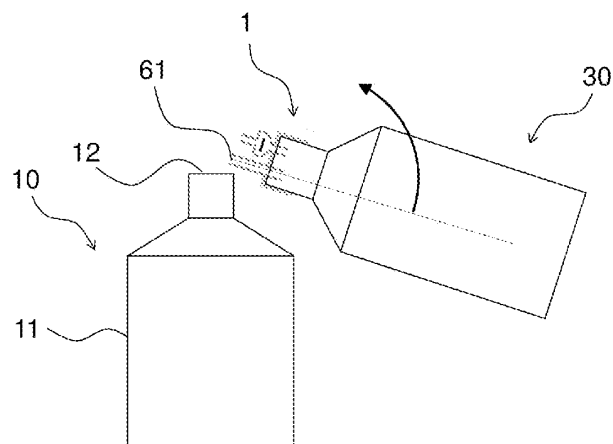

[図3]

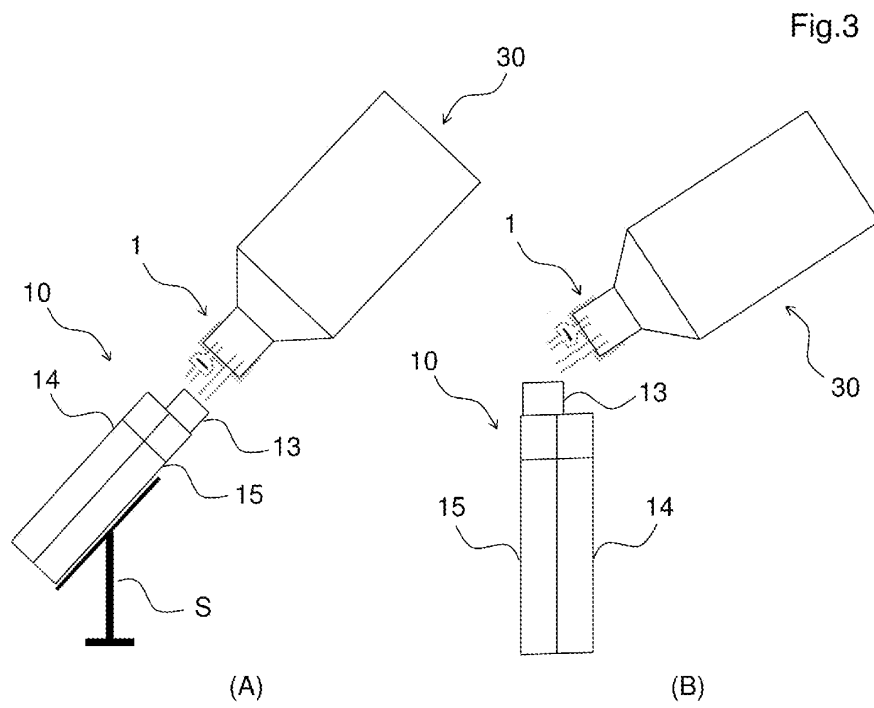

[図4]

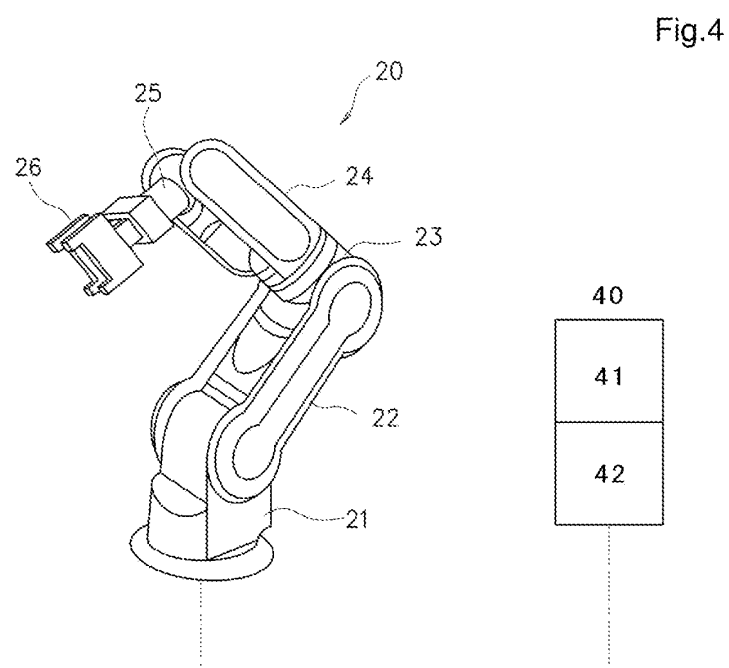

[図5]

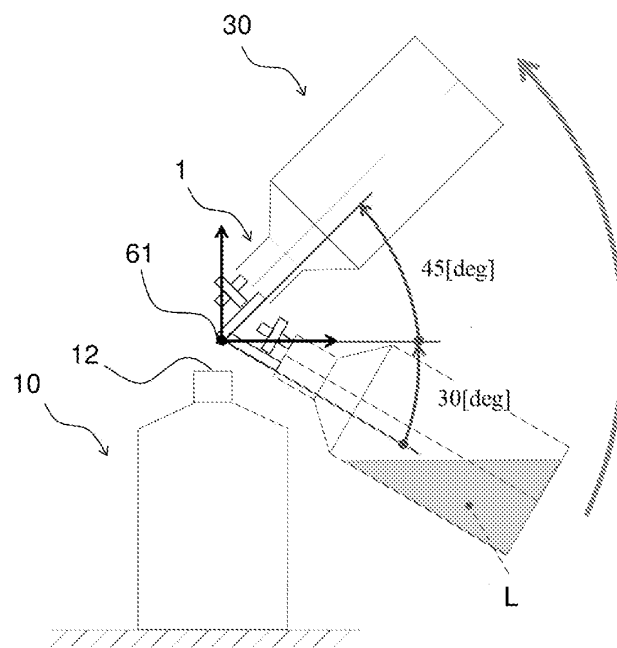


Fig. 5

[図6]


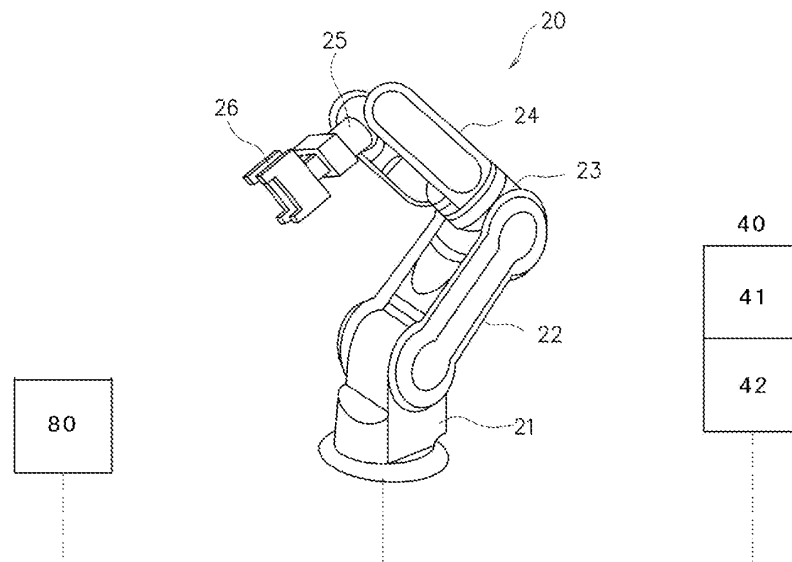


Fig. 6


[図7]

Fig.7

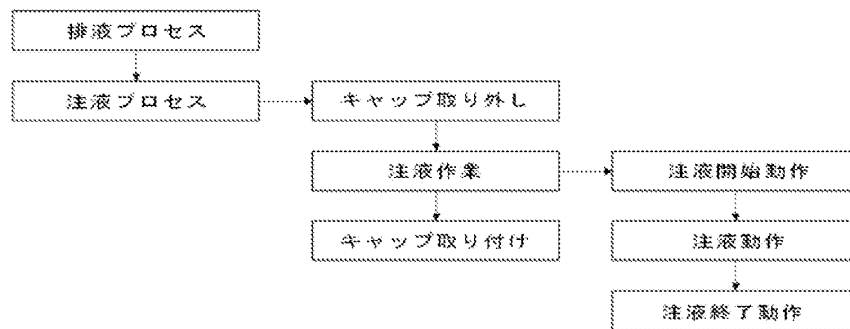


[図8]

Fig.8

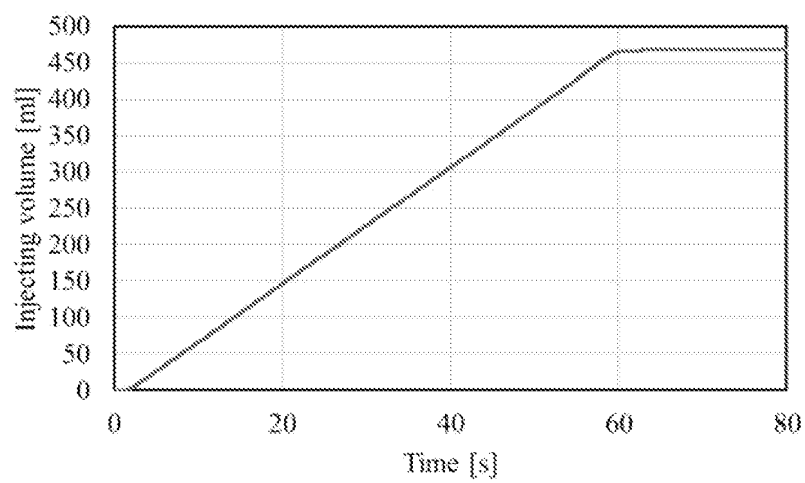


[図9]

Fig.9

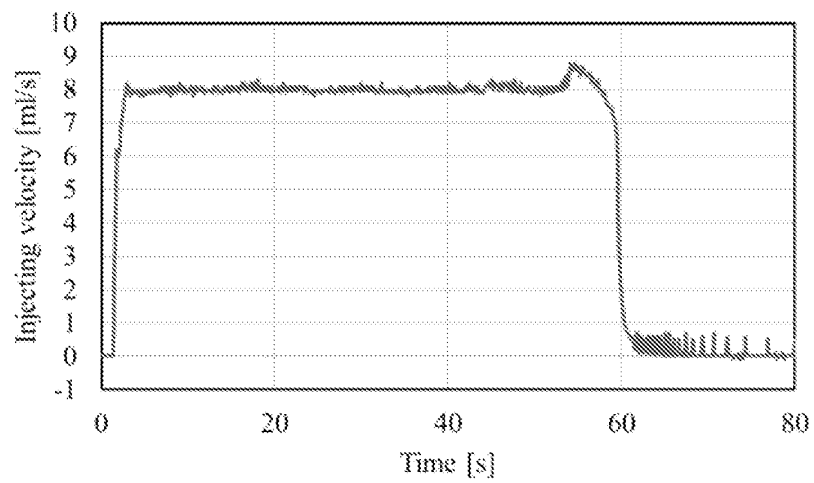


[図10]

Fig.10

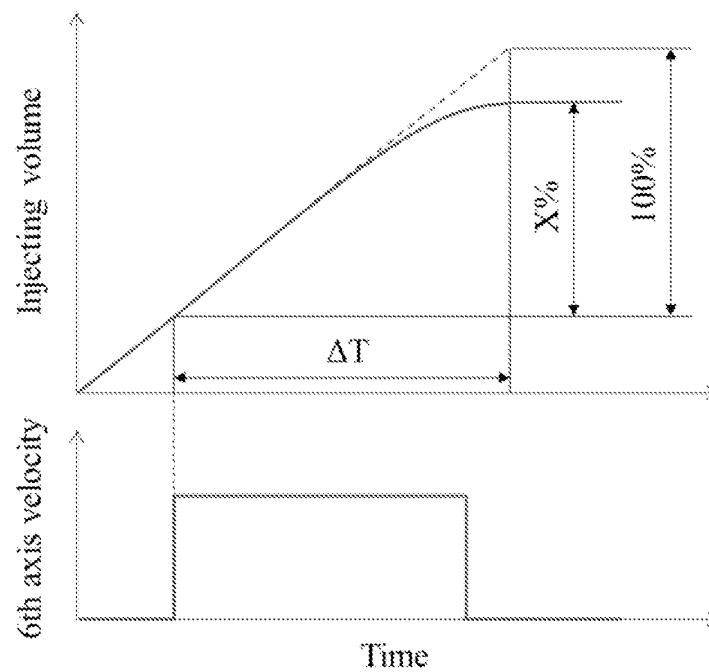


[図11]

Fig.11

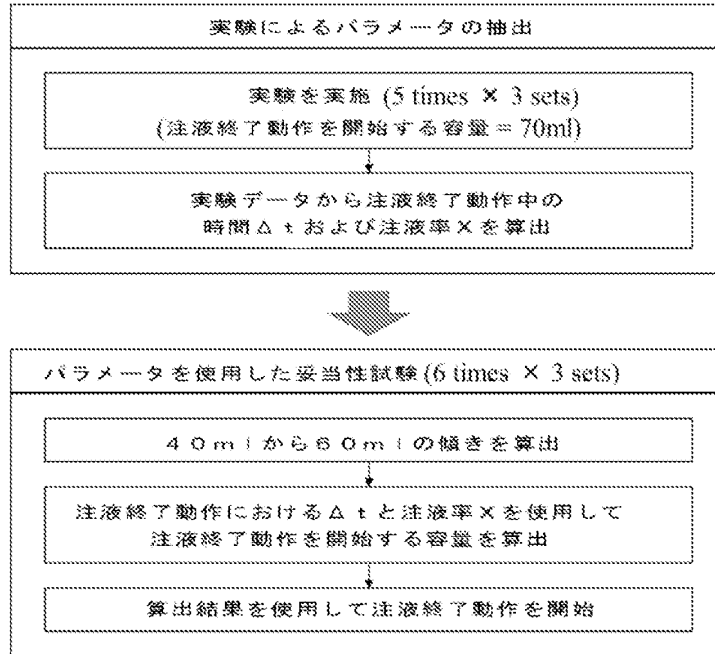


[図12]


Fig.12

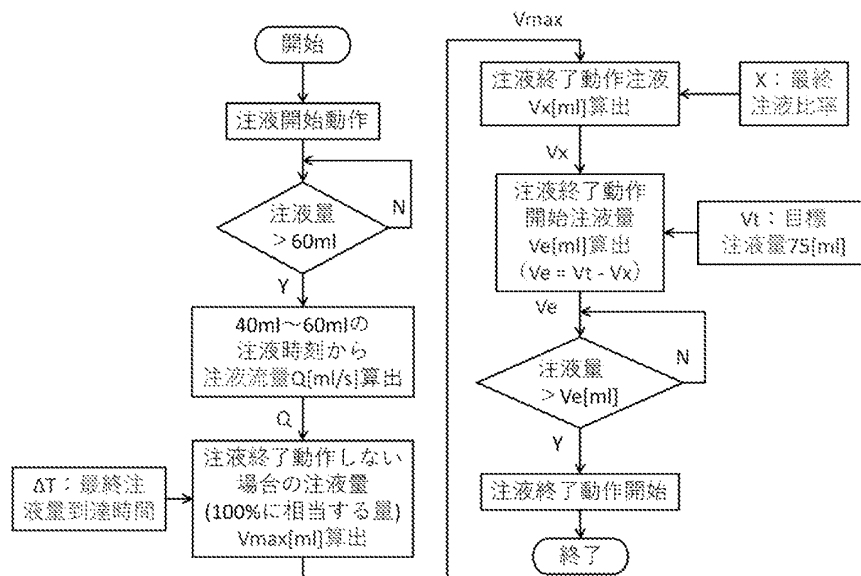

[図13]

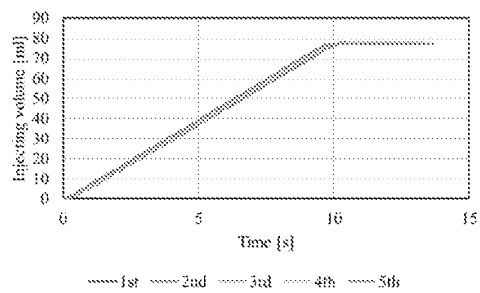

(1) Overall view

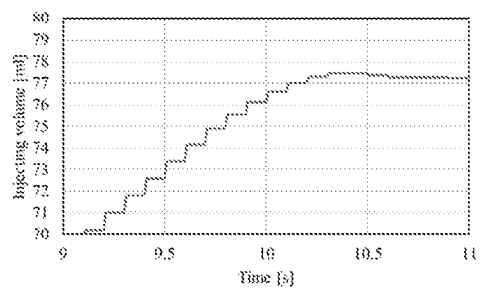

(2) Enlarged view

Fig.13

[図14]


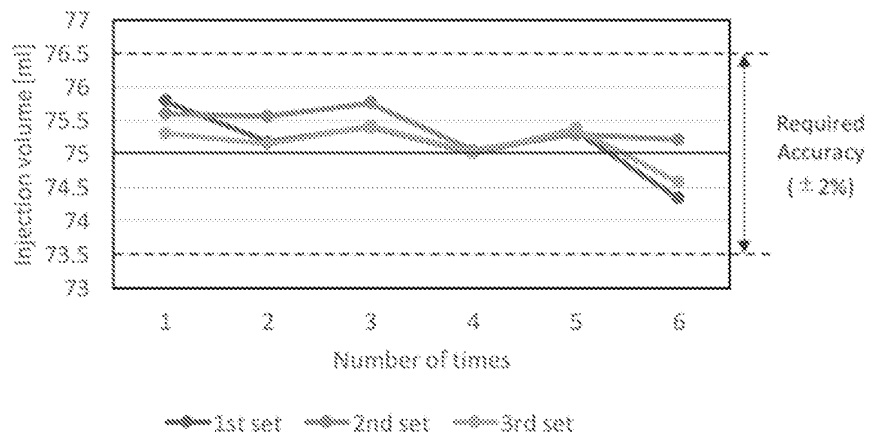


Fig.14


[図15]

Fig. 15

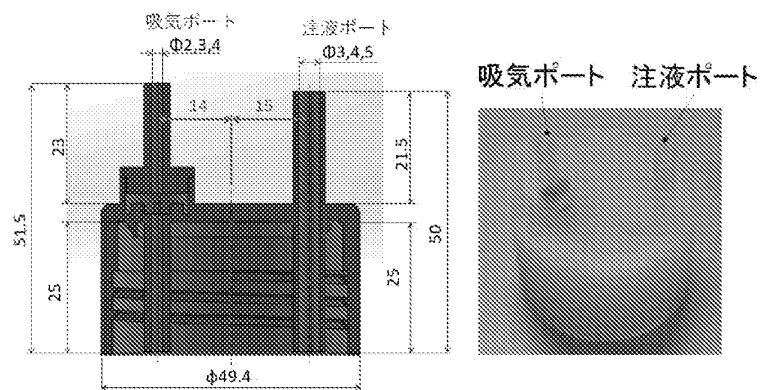


[図16]

Fig. 16

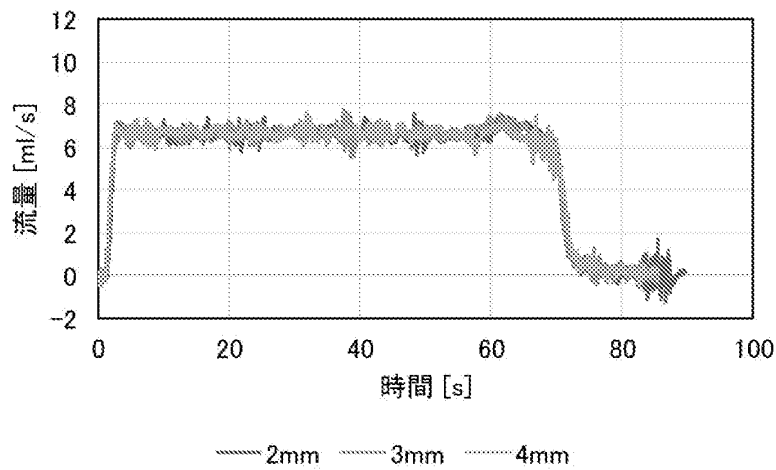


[図17]

Fig. 17

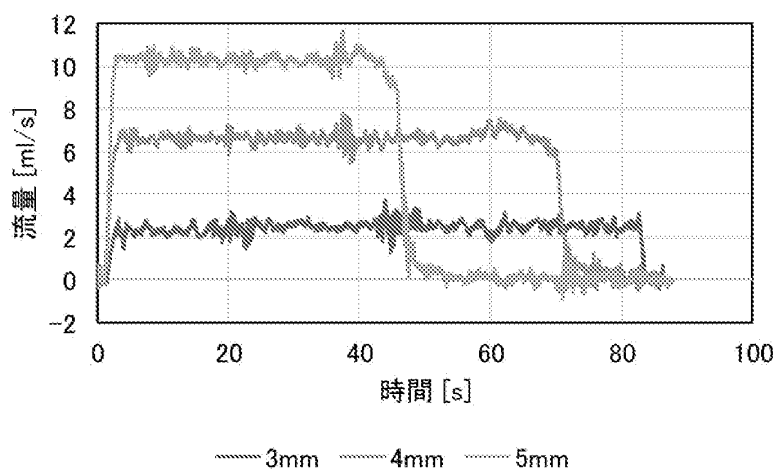


[図18]

Fig. 18

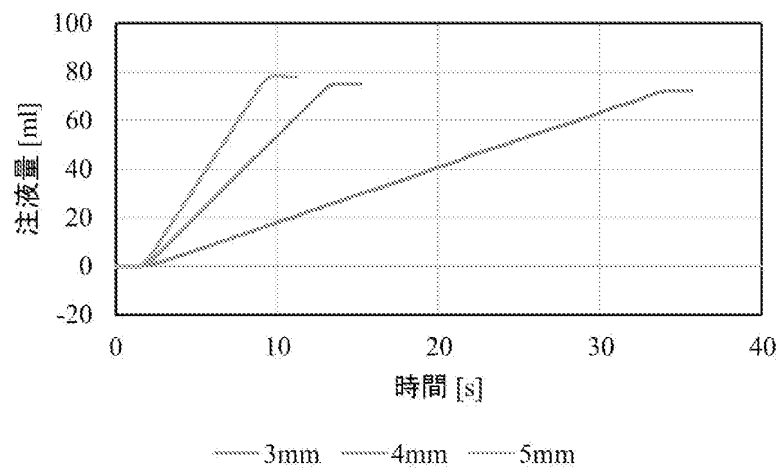


(1) 全体図

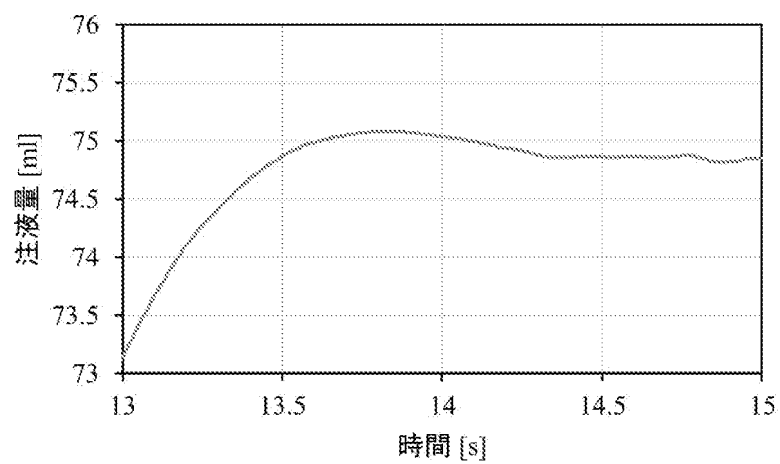

(2) 拡大図 (注液ポート内径=4mm)


[図19]

Fig.19

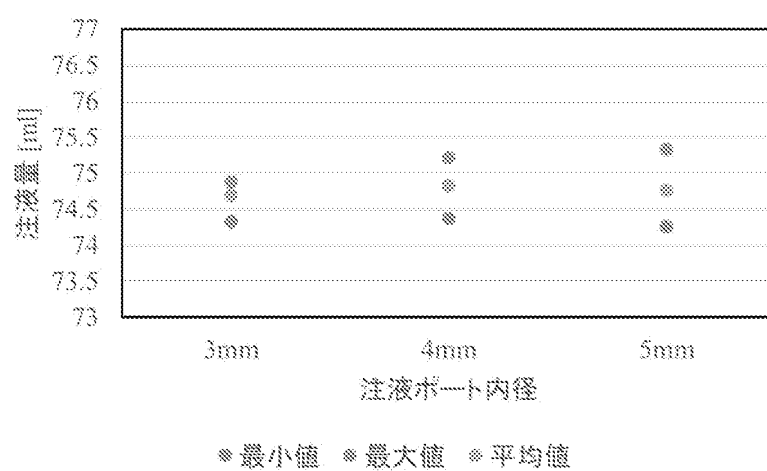


[図20]

Fig. 20

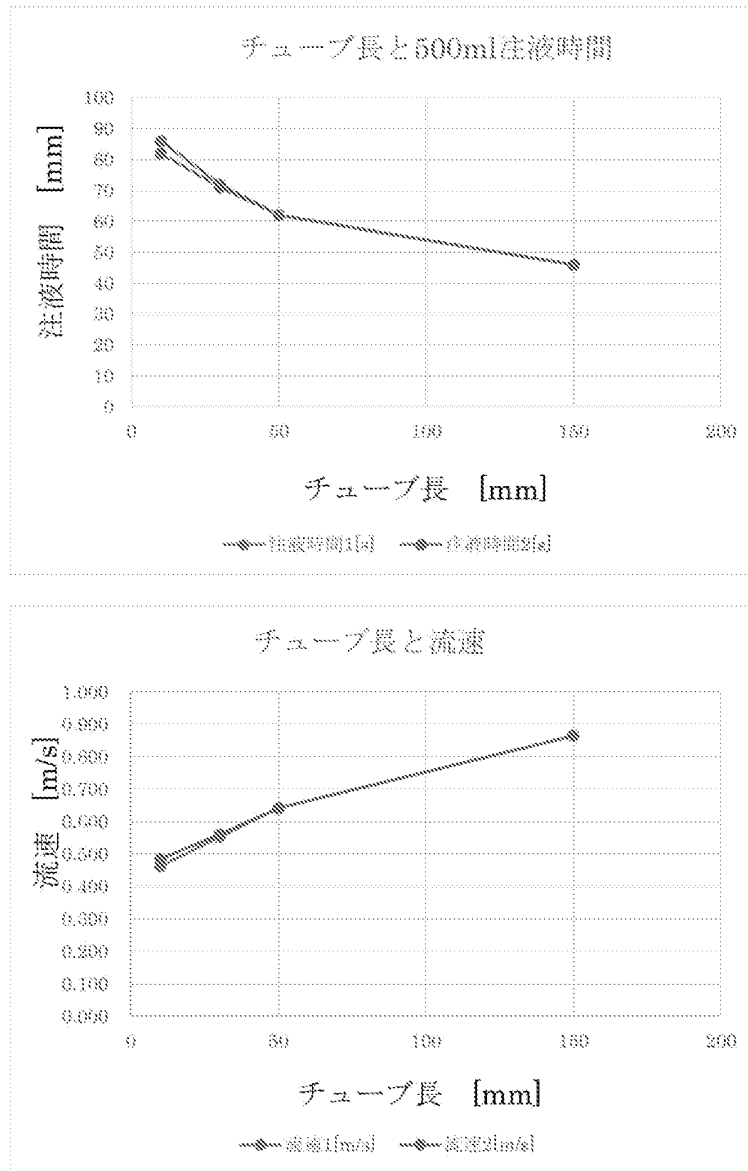


[図21]

Fig. 21

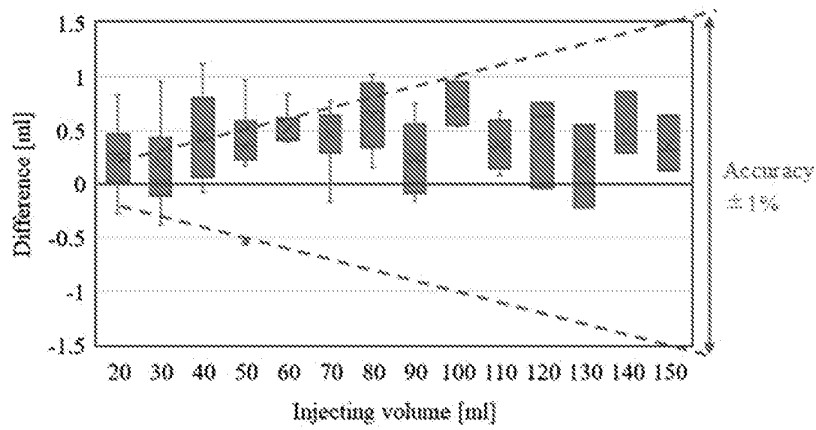

[図22]

Fig. 22

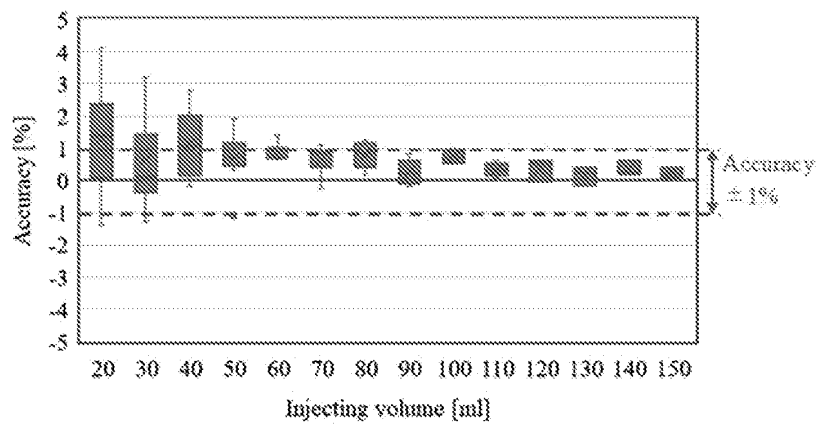

[図23]

Fig. 23

