

FIGURE 1

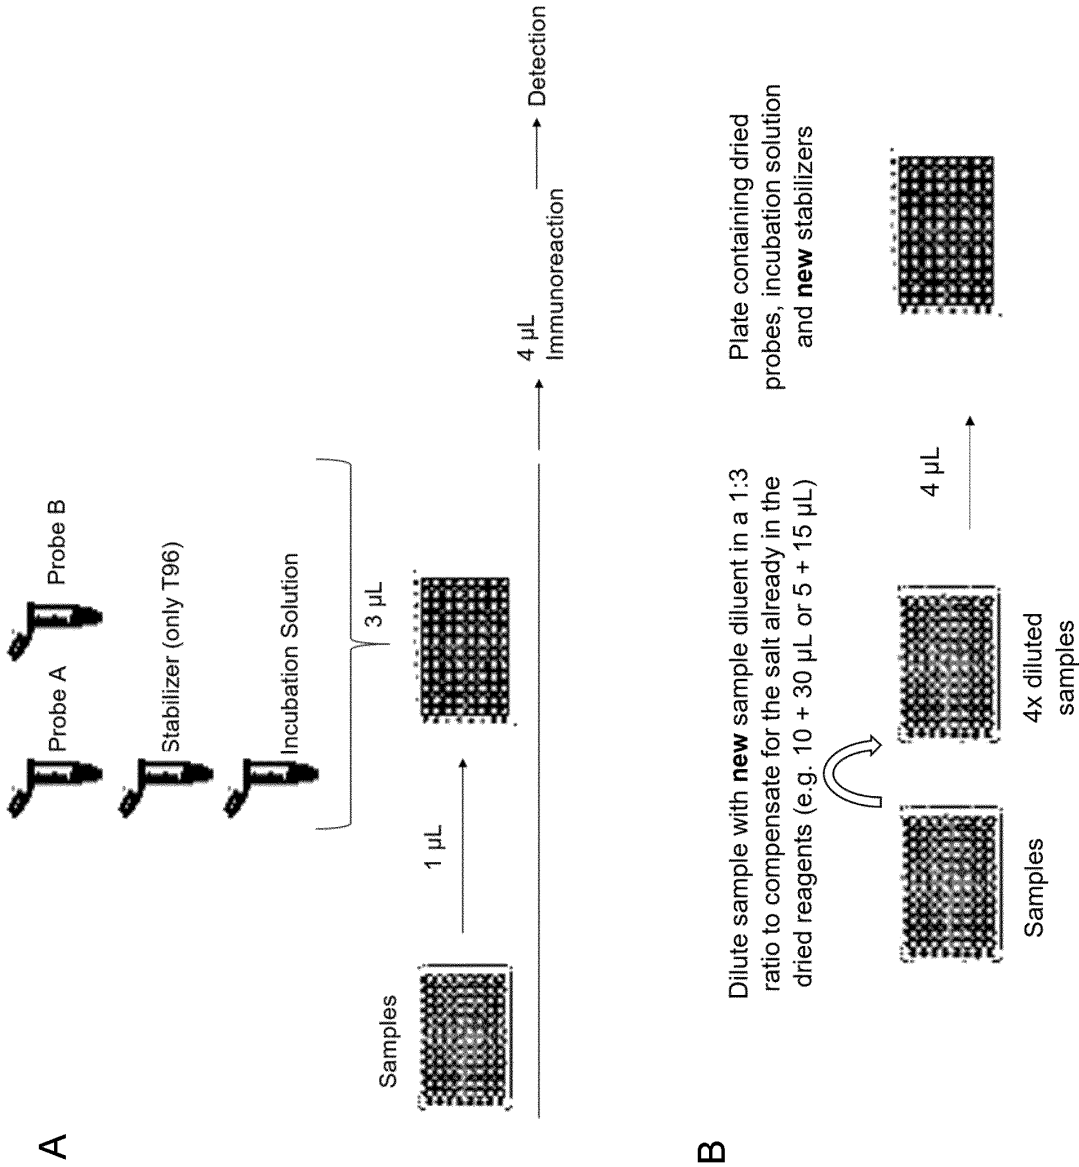


FIGURE 2

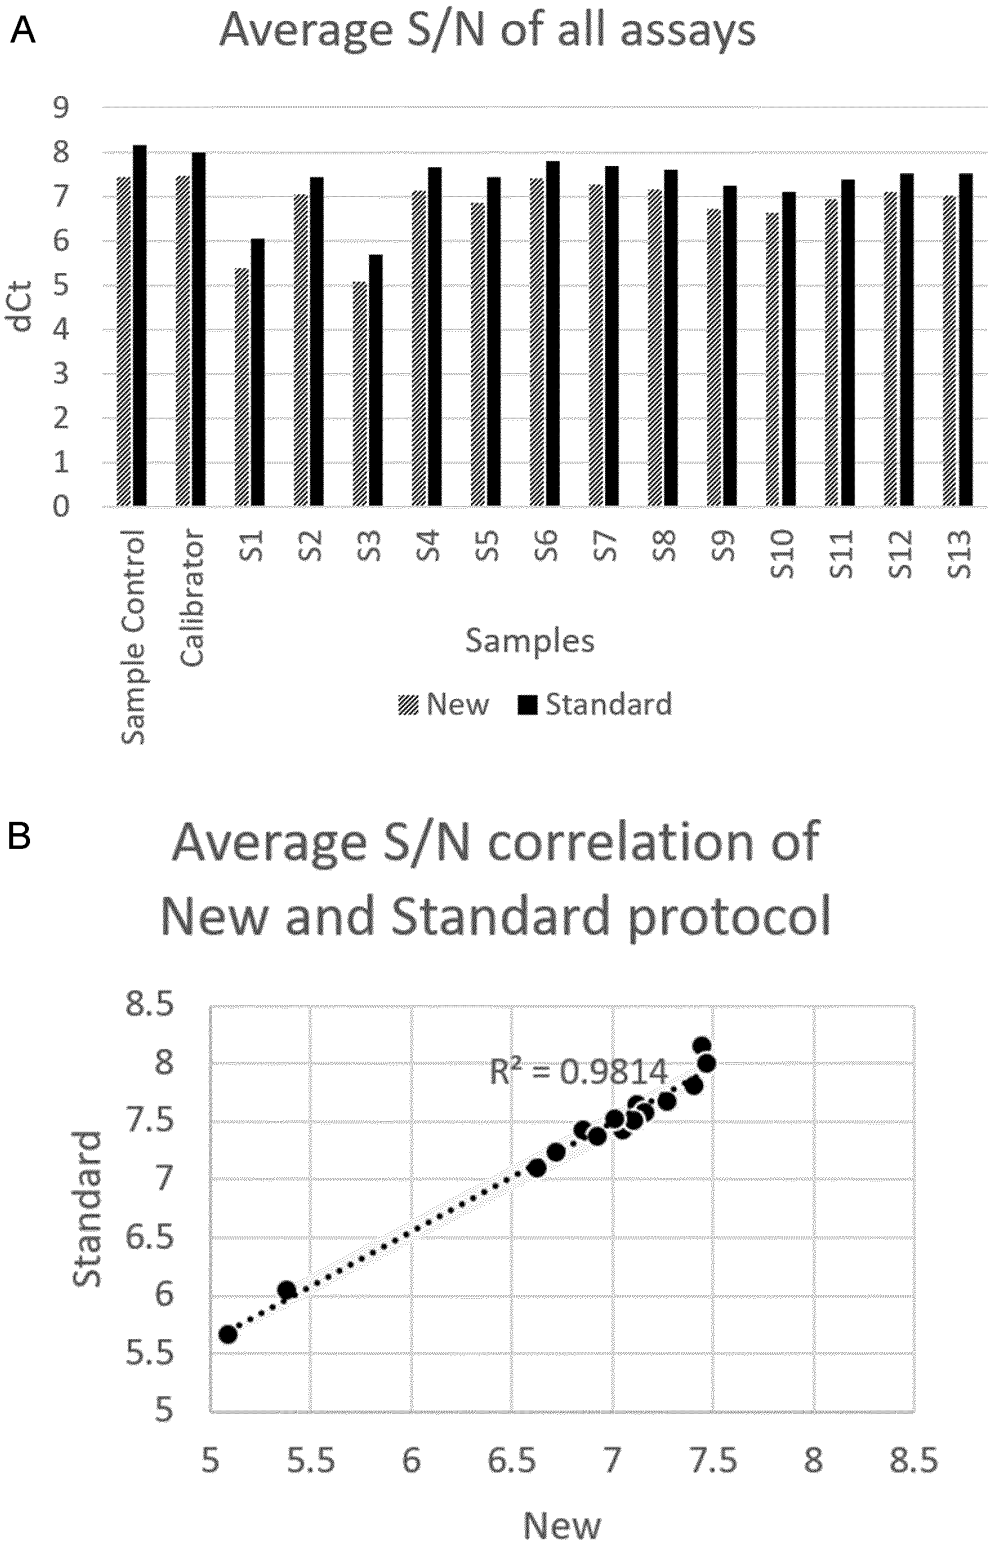


FIGURE 3

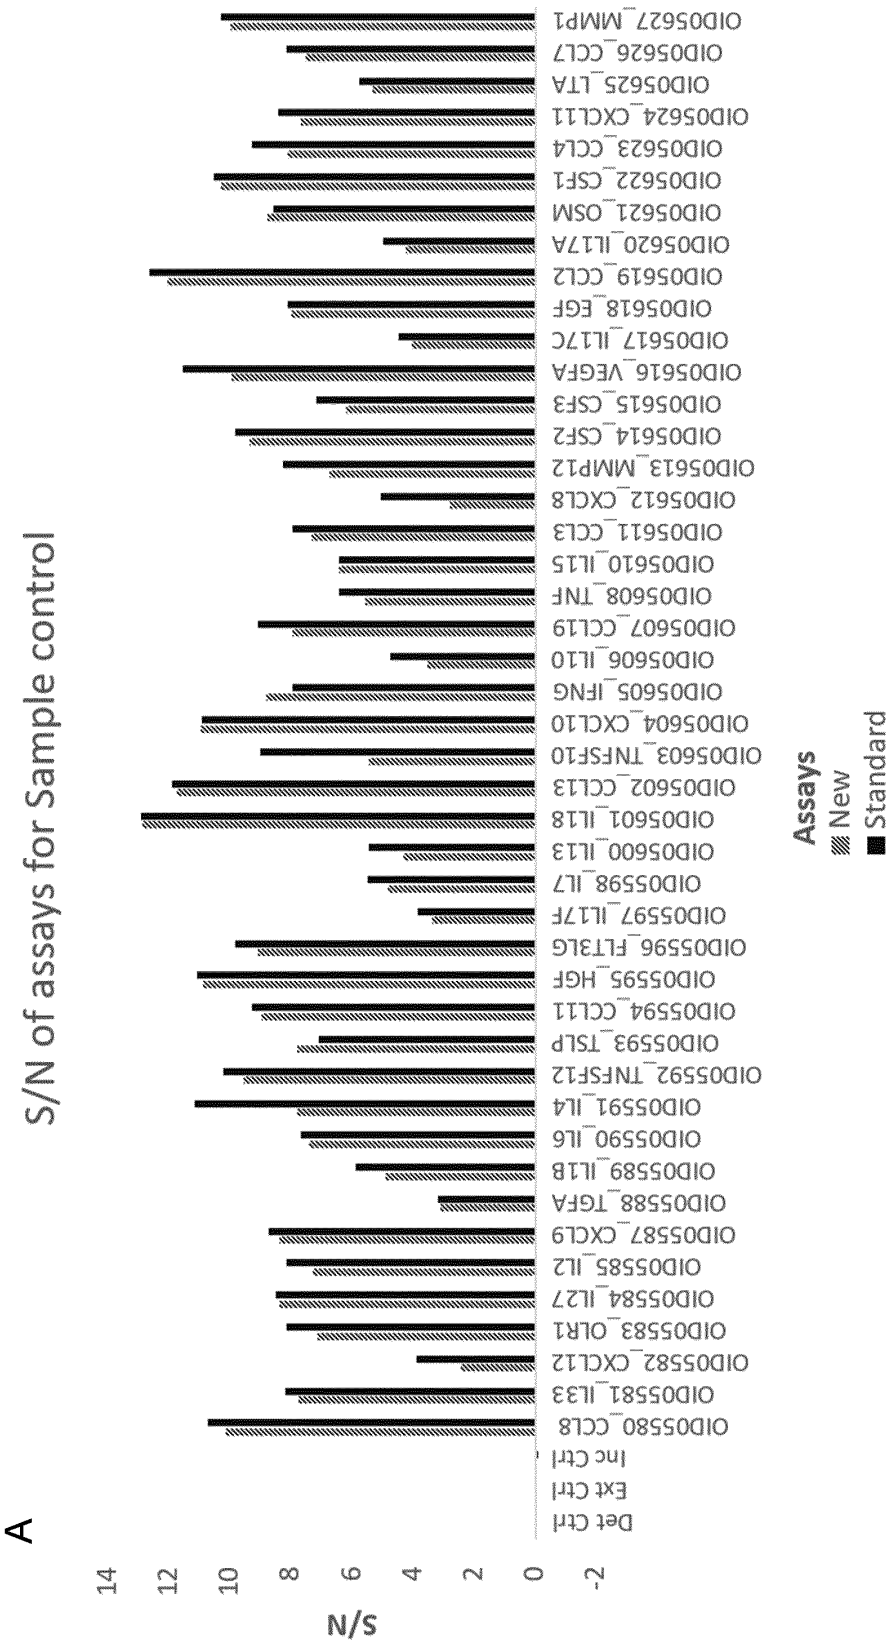


FIGURE 3 CONTINUED

B      Correlation of S/N of assays for two protocols for sample control

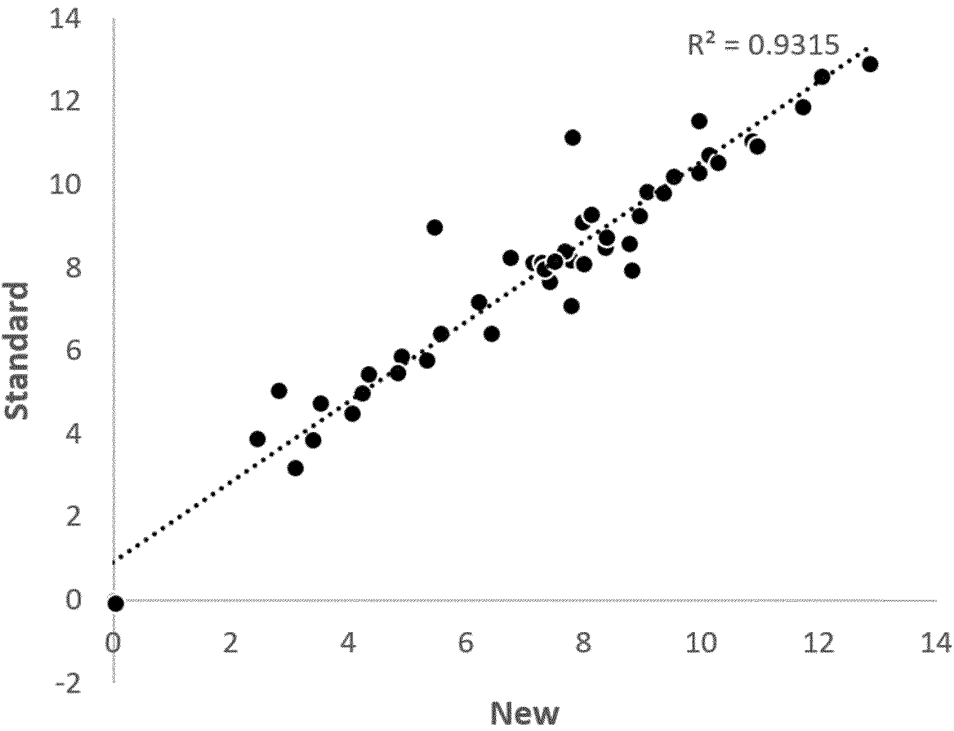


FIGURE 4

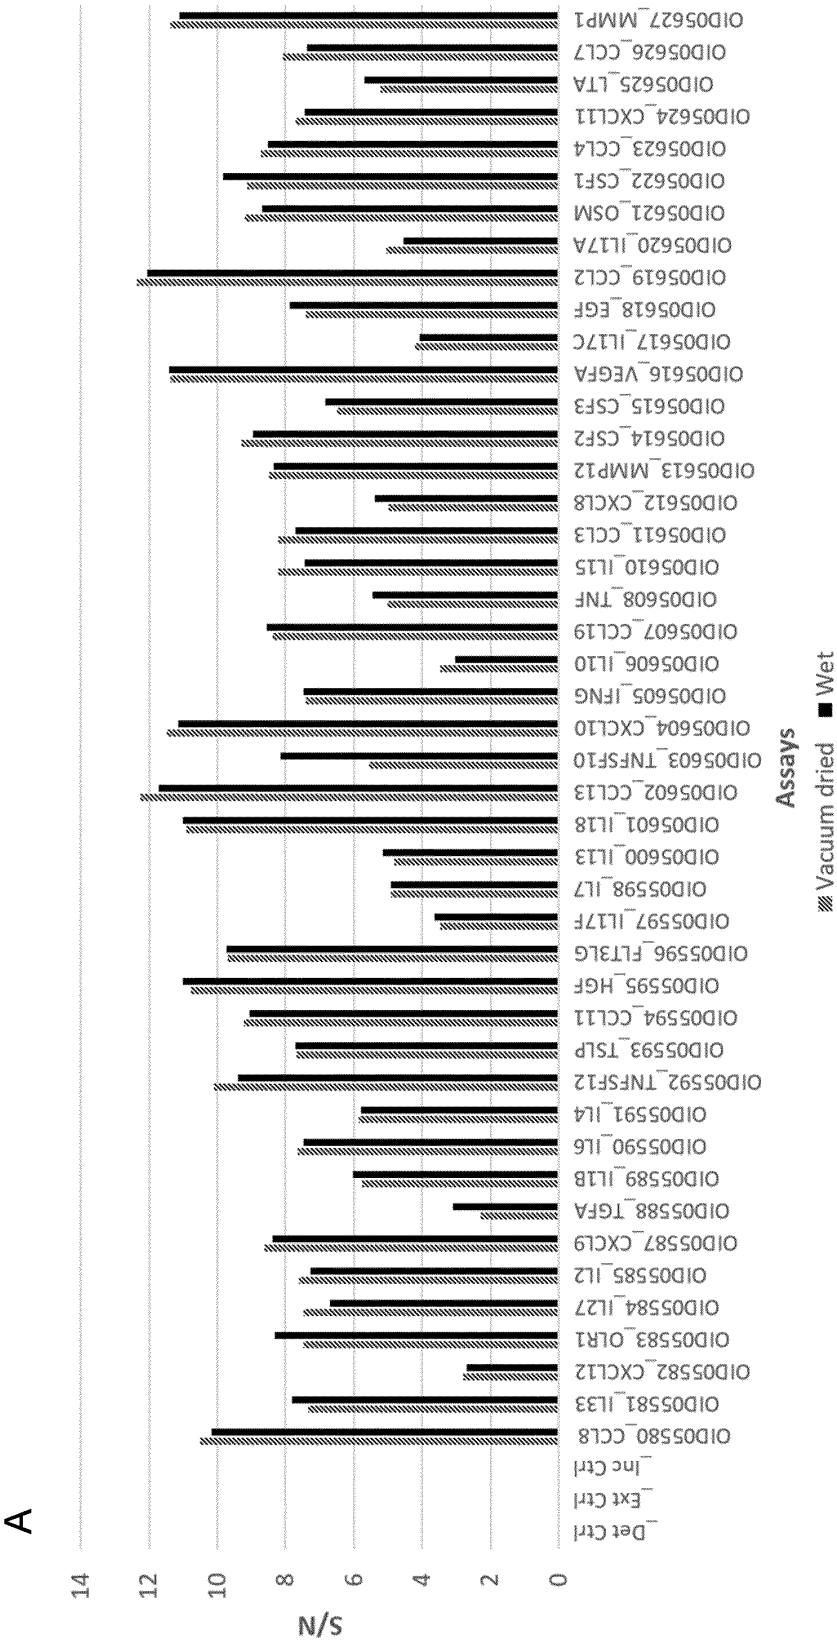


FIGURE 4 CONTINUED

B S/N correlation of each assay for vacuum dried and Wet probes

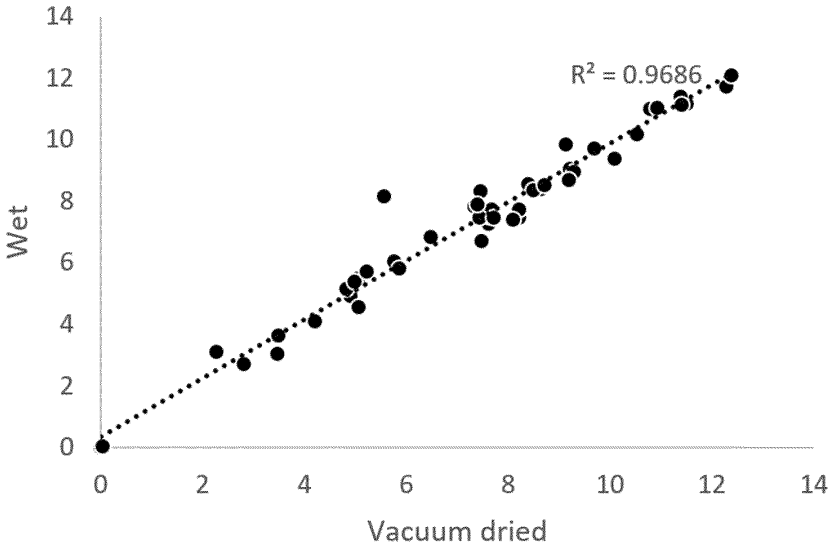


FIGURE 5

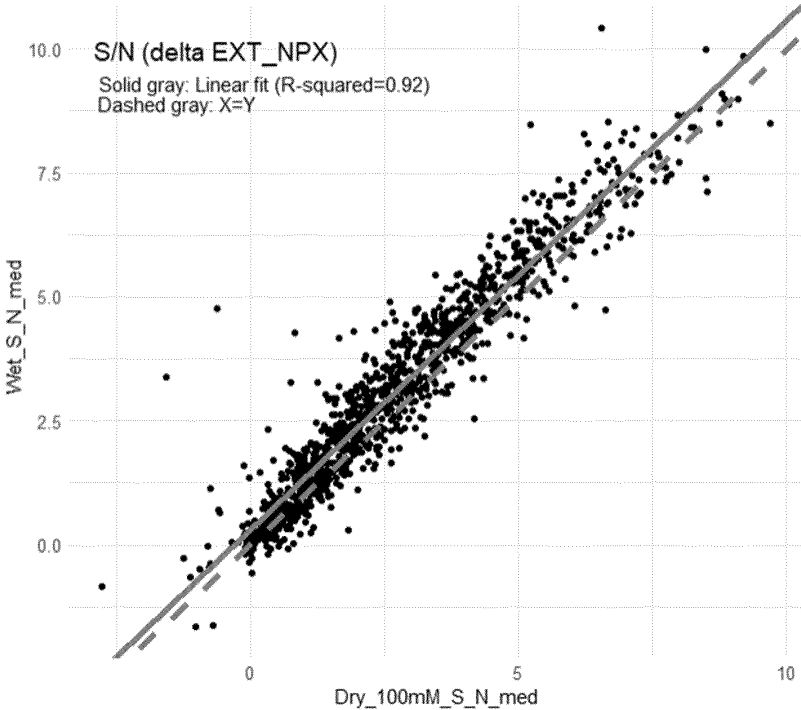


FIGURE 6

