

1/13

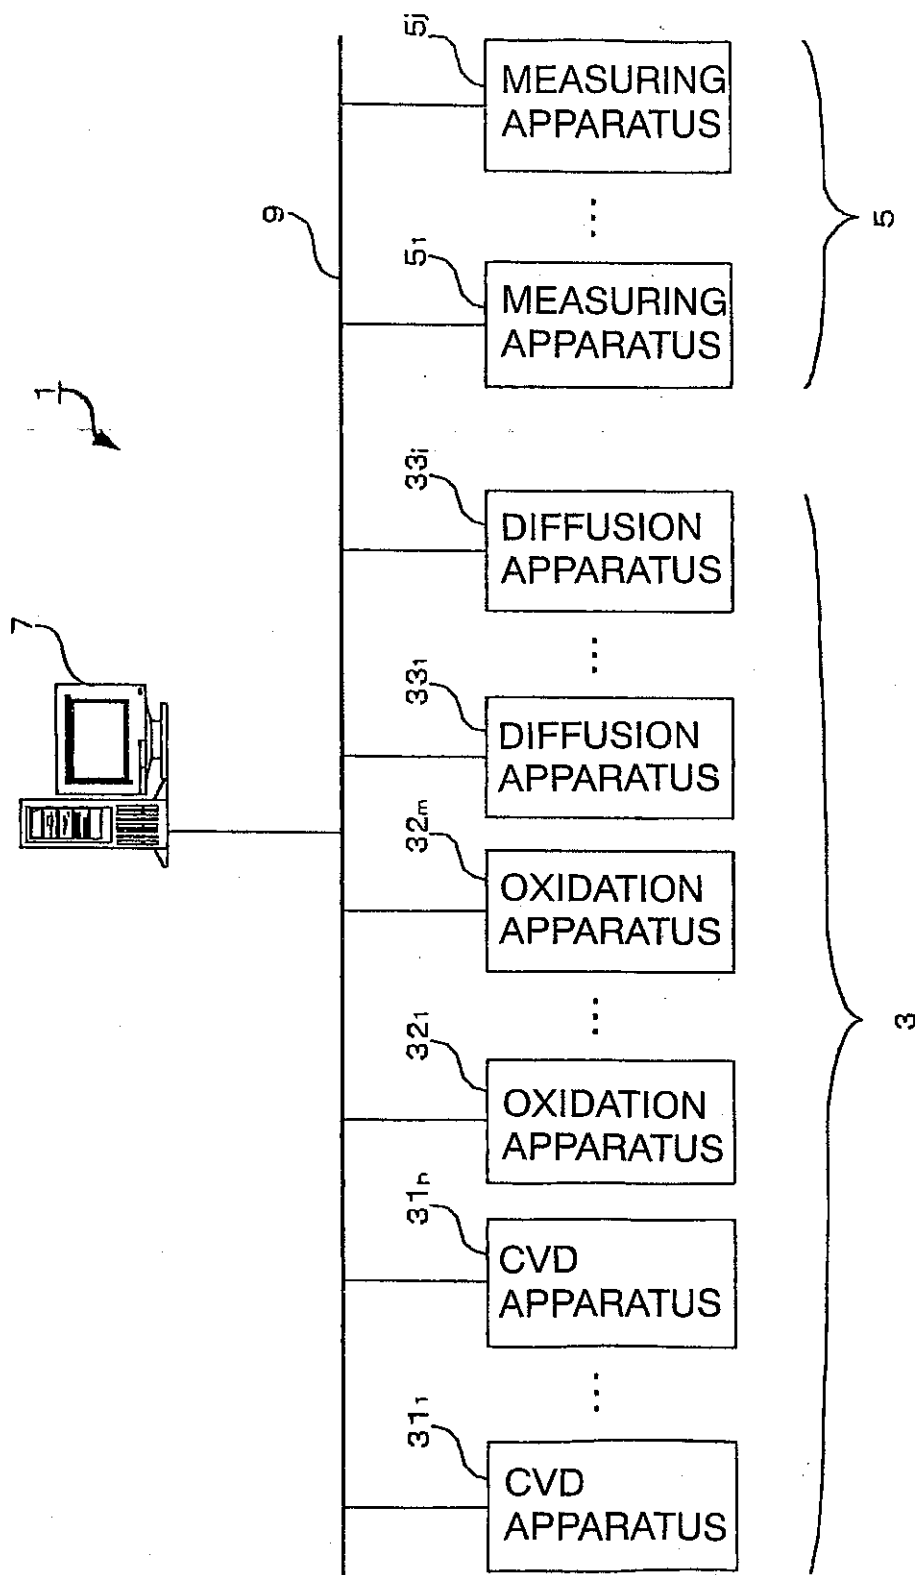


FIG. 1



3/13

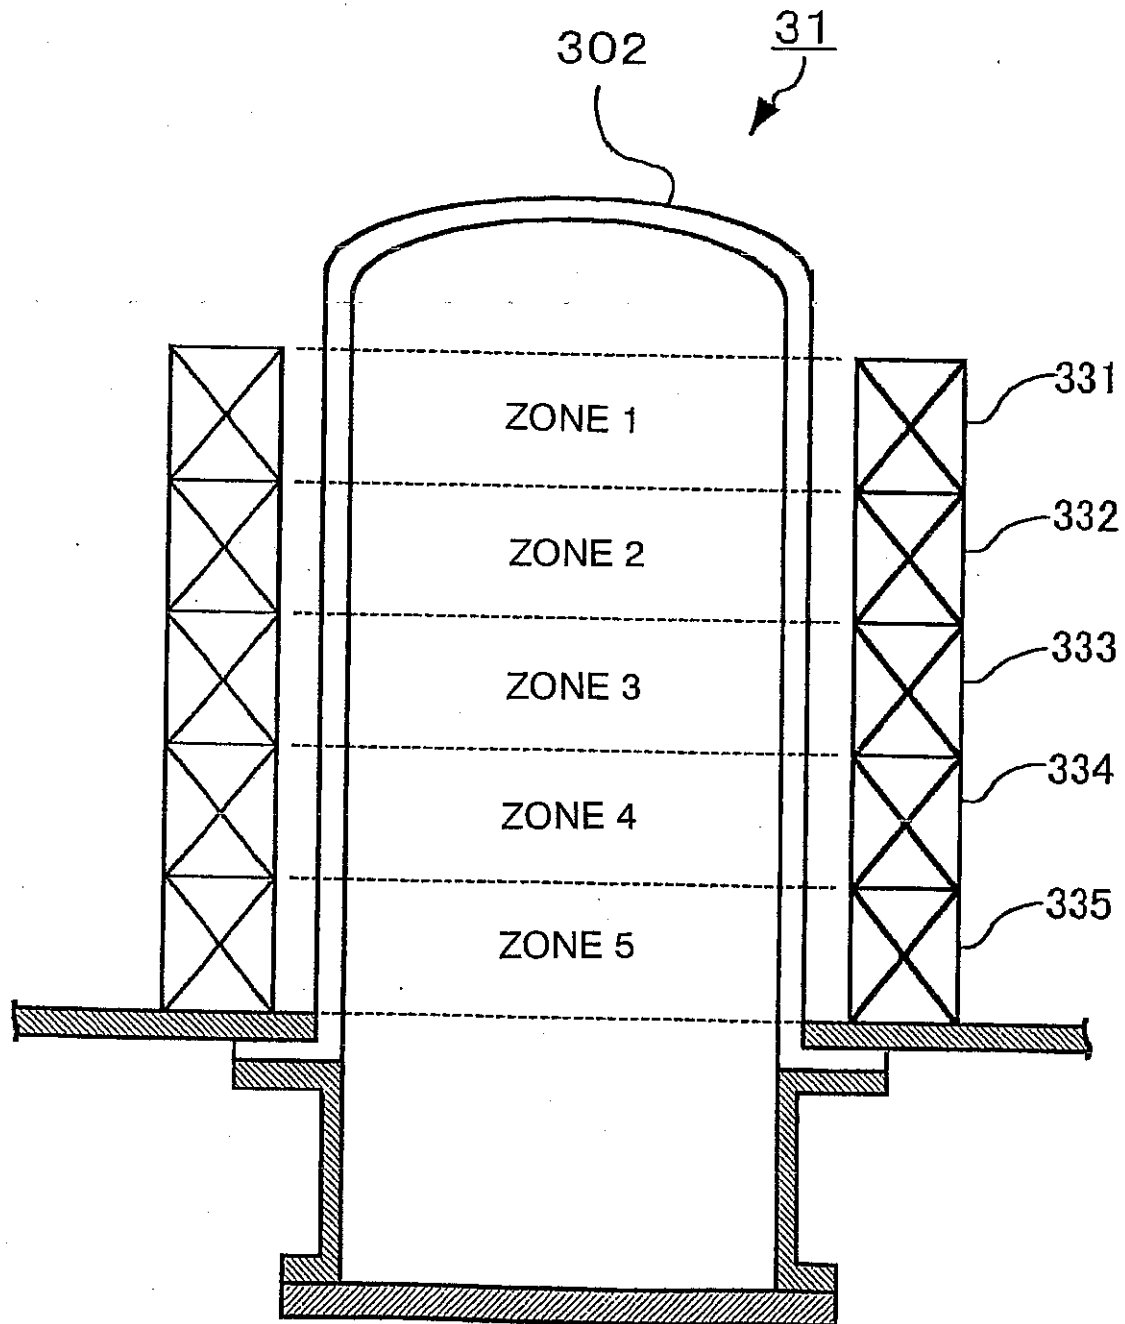


FIG. 3

4/13

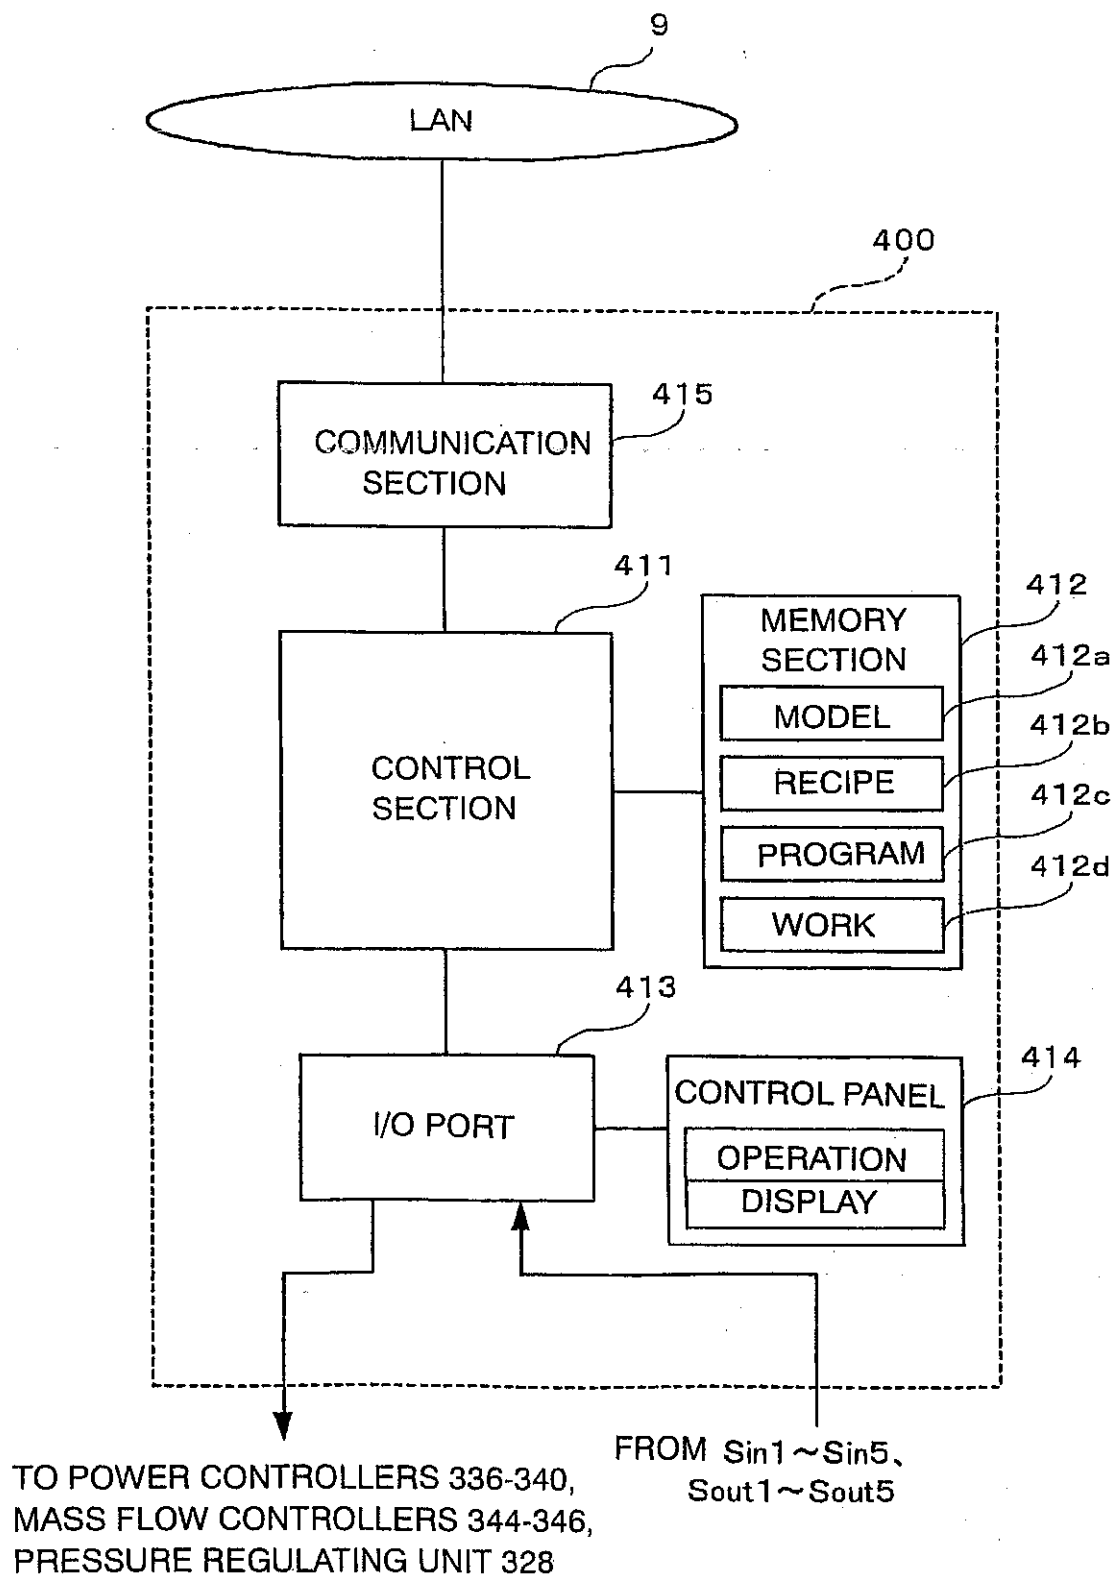


FIG. 4

5/13

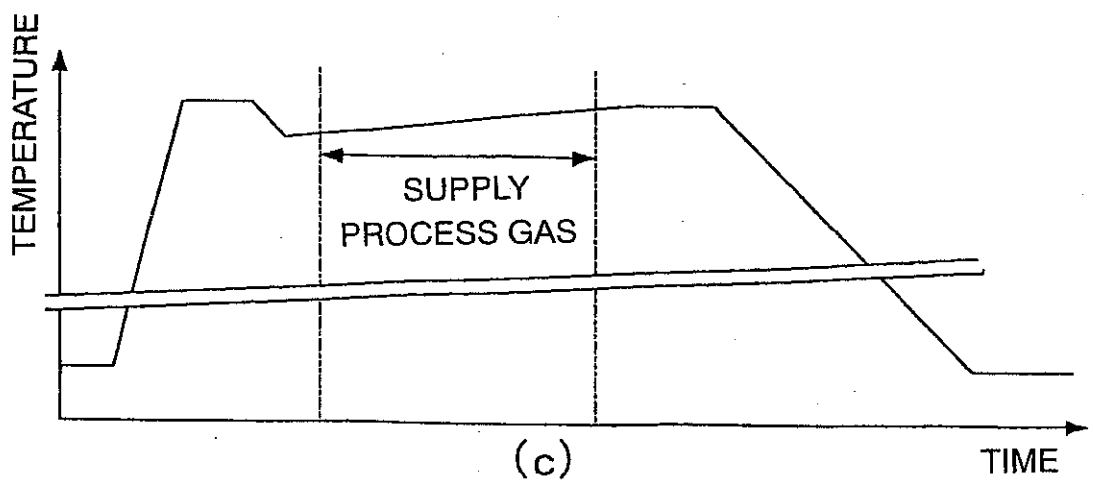
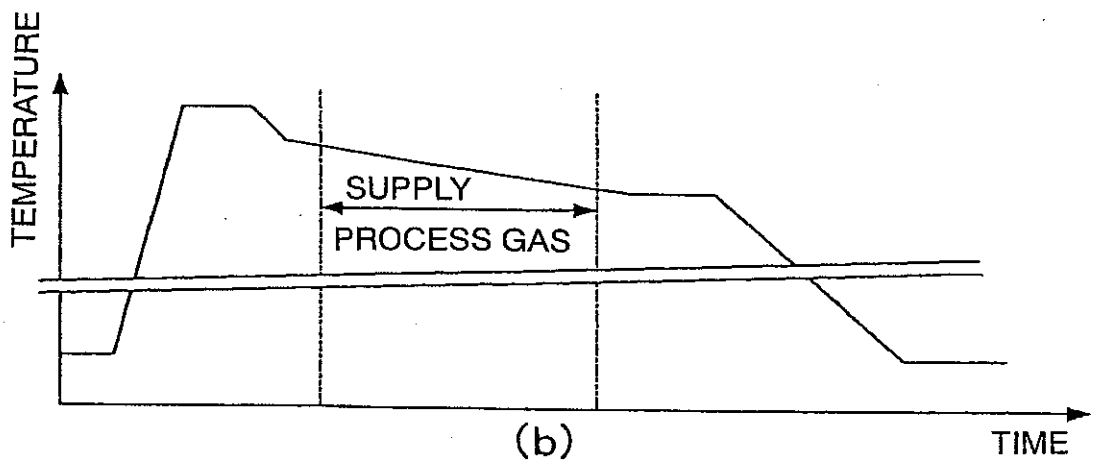
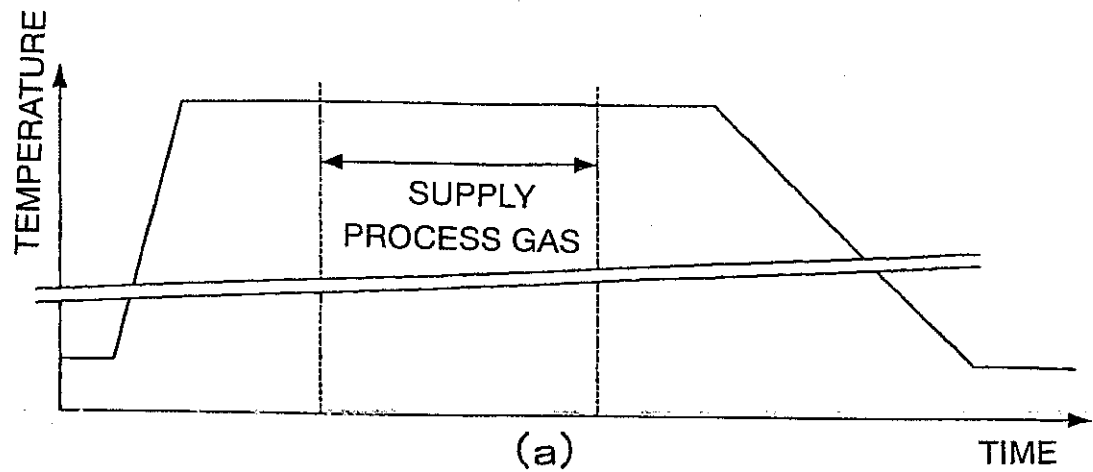


FIG. 5

6/13

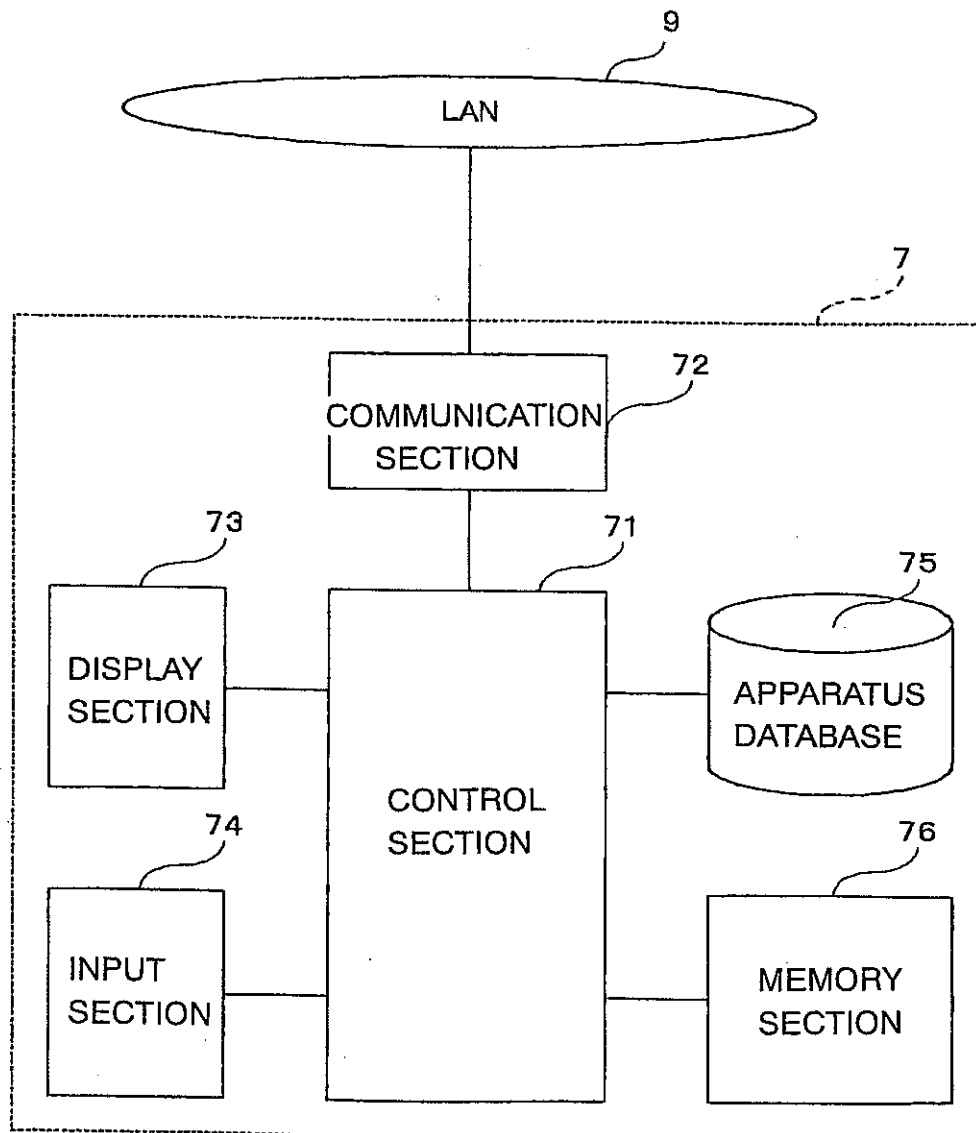


FIG. 6

7/13

MANAGEMENT TABLE FOR CVD APPARATUS

APPARATUS ID	TOTAL NUMBER OF TREATMENTS	NUMBER OF TREATMENTS AFTER MODEL CALIBRATION	MODEL	NUMBER OF TREATMENTS AFTER RECIPE CALIBRATION	RECIPE	TARGET FILM THICKNESS	OTHERS
CVD 1	432	3	*※@§	7	*b‡\$#	234nm	...
CVD 2	123	7	#*※+§	5	•b\$¥*	234nm	...
CVD 3	224	11	*※@§*	2	*b‡\$#↑	234nm	...
...	...	...	...	...	...	...	...
BASIC MODEL			BASIC RECIPE				

FIG. 7

8/13

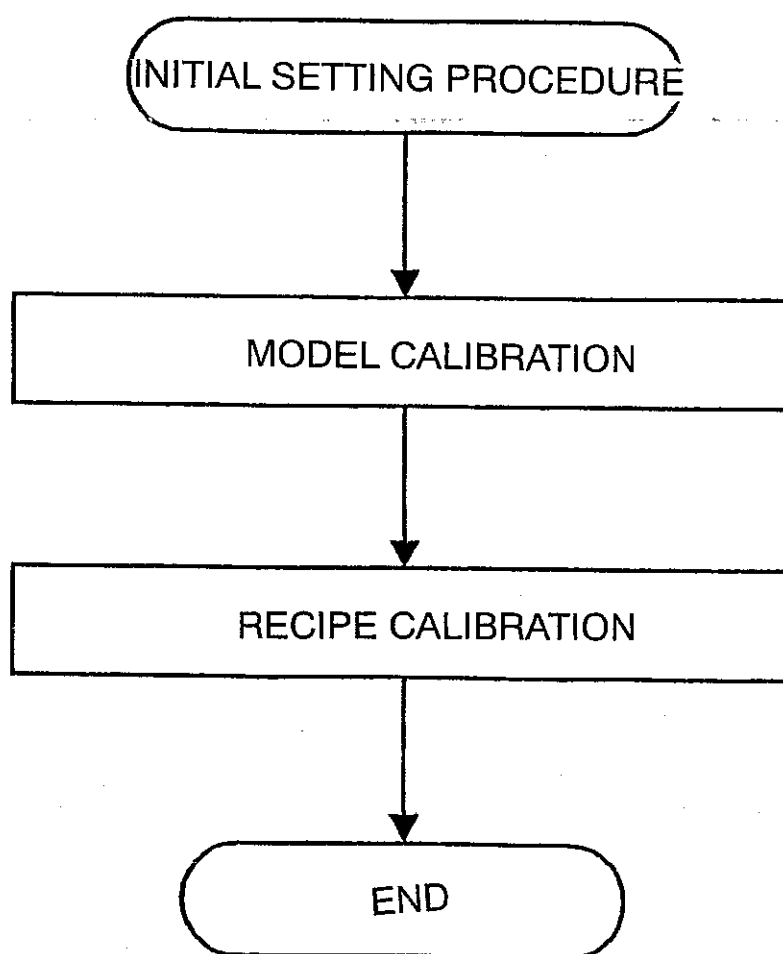


FIG. 8

9/13

MODEL CALIBRATION PROCEDURE

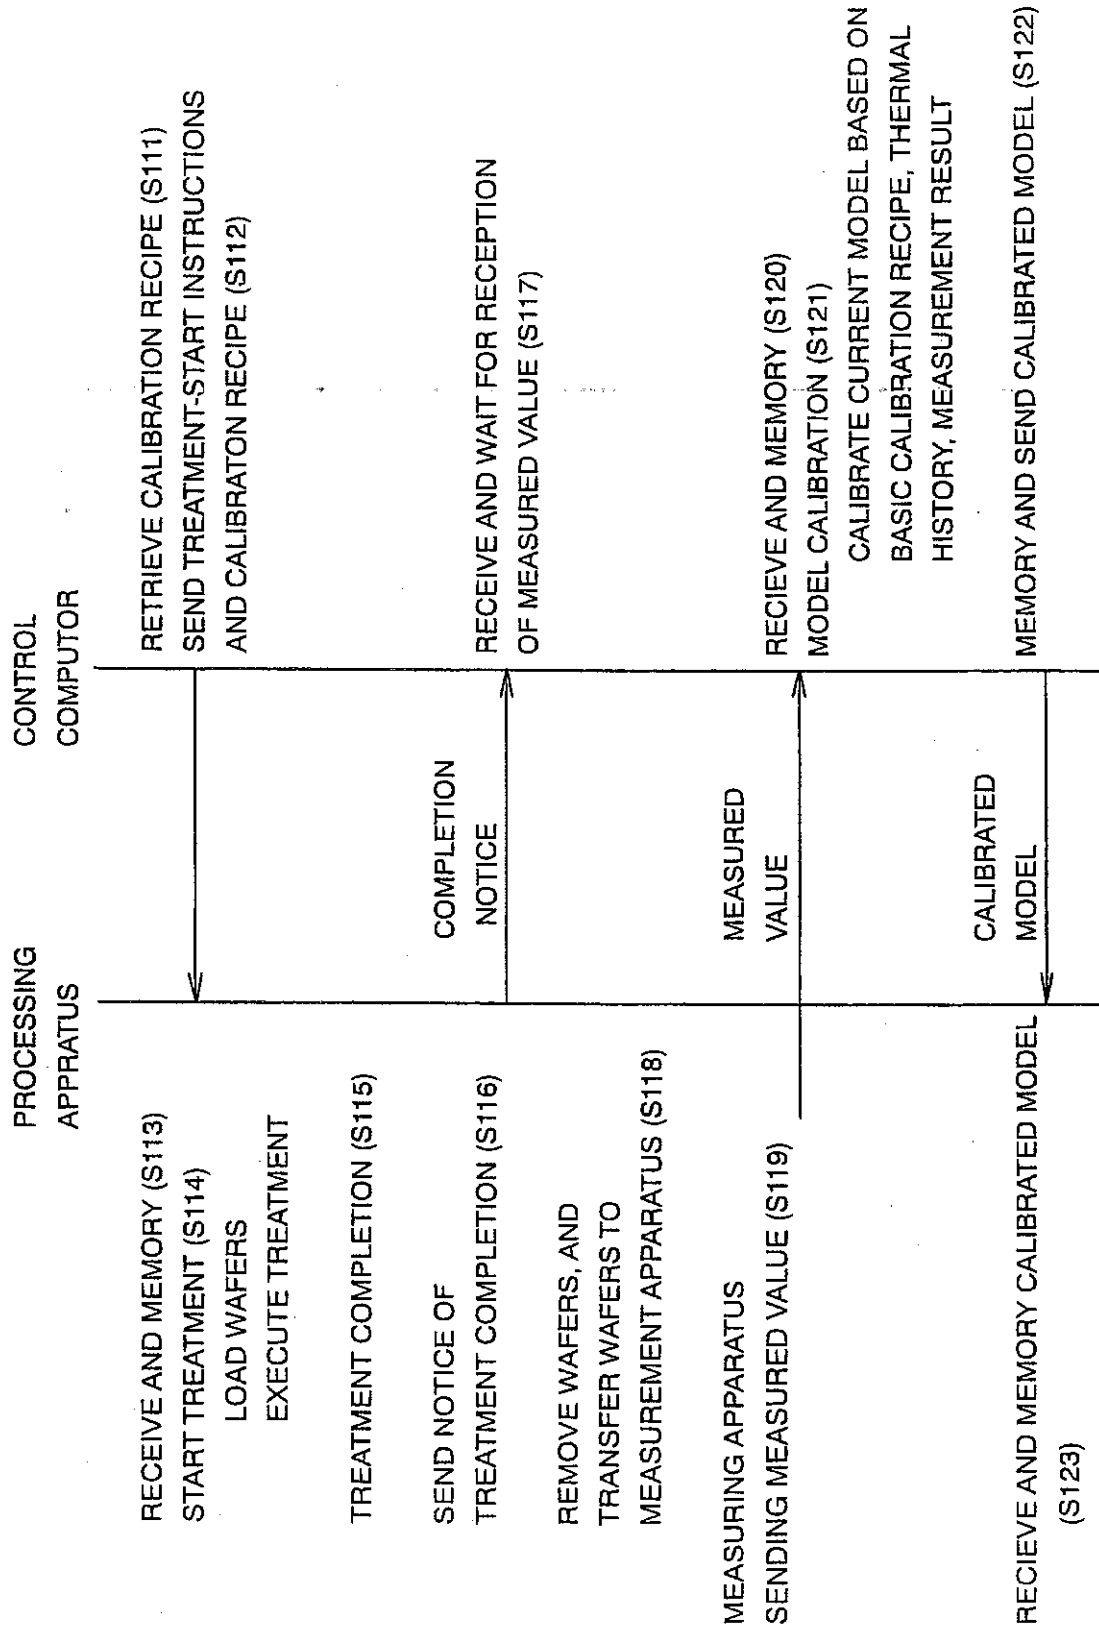


FIG. 9

10/13

RECIPE CALIBRATION PROCEDURE

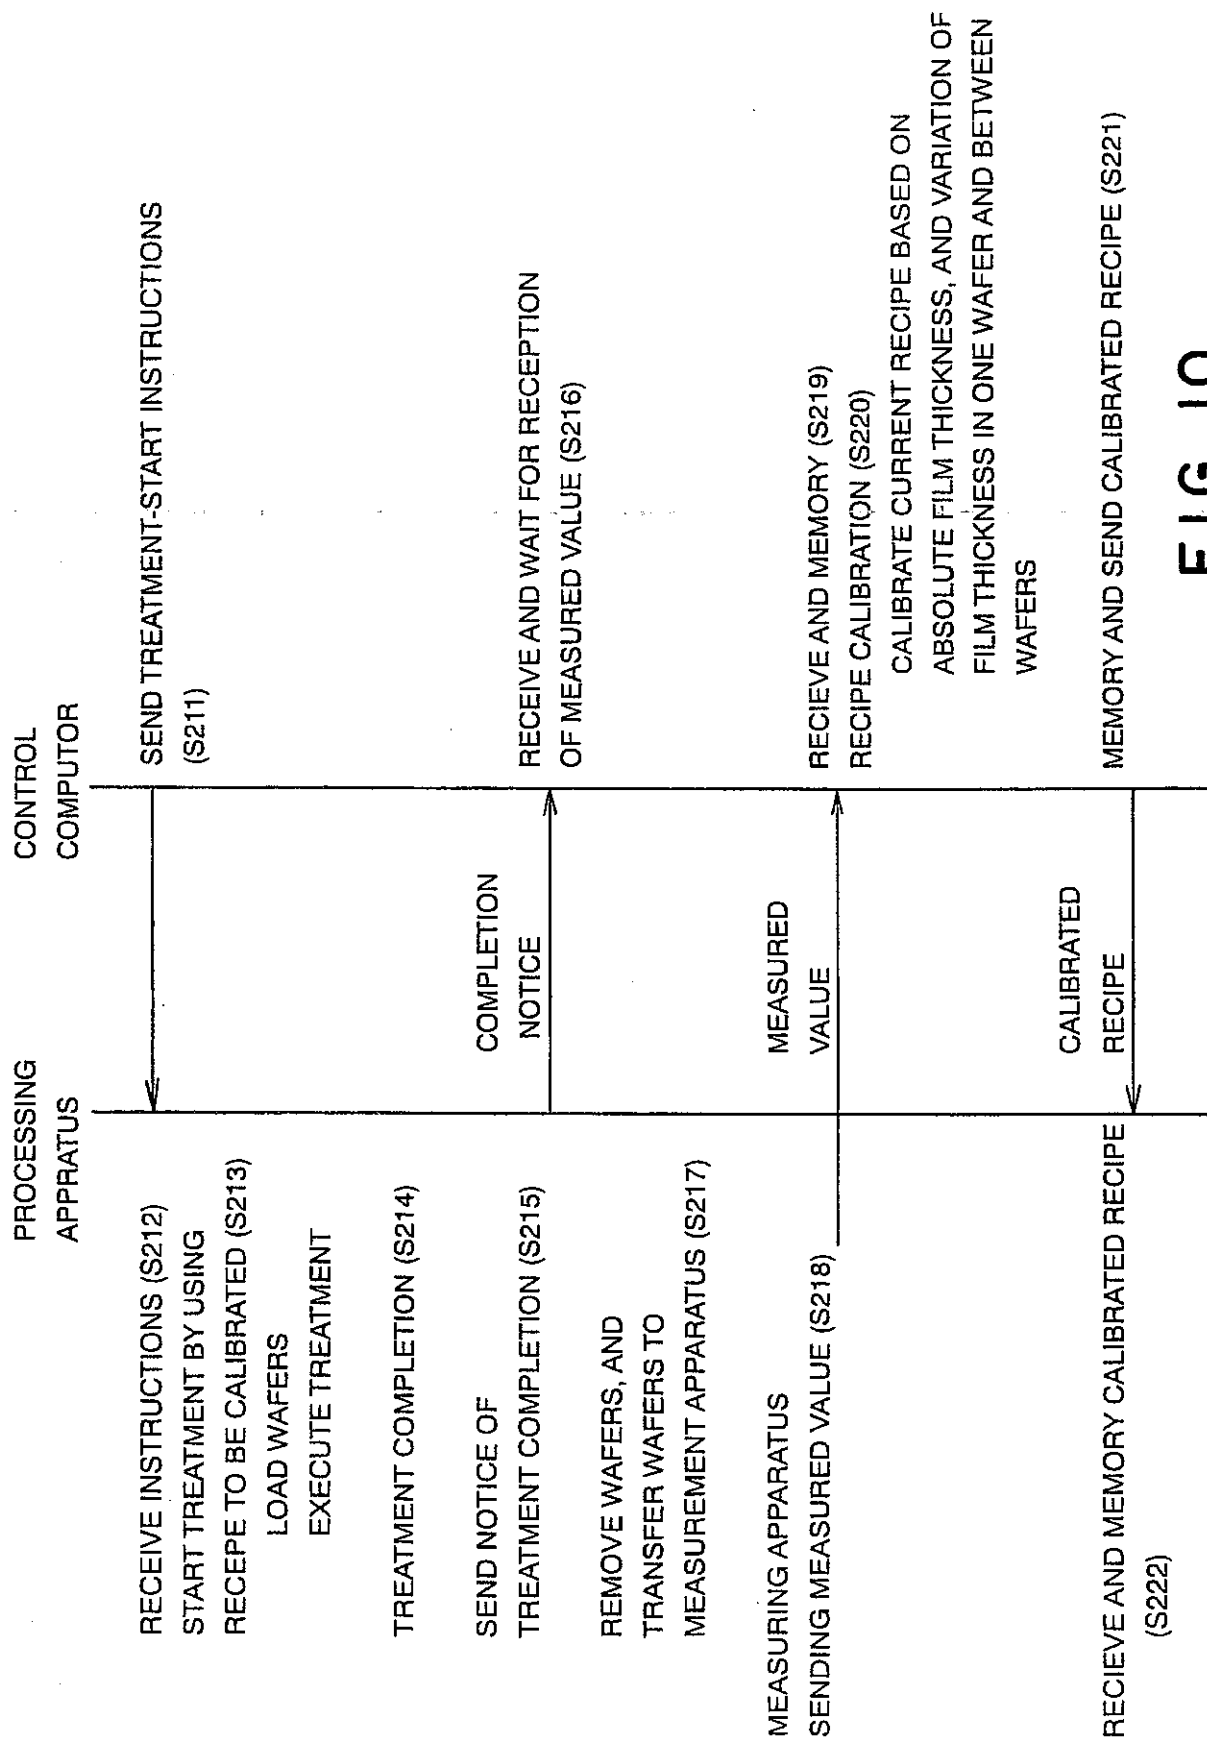


FIG. 10

11/13

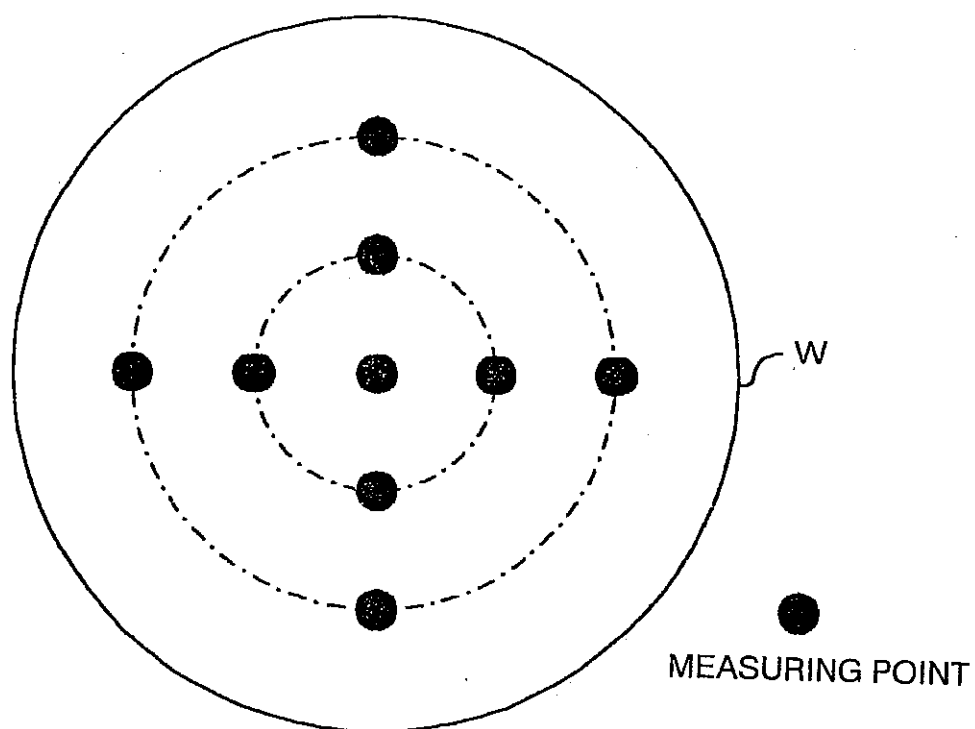


FIG. 11

12 / 13

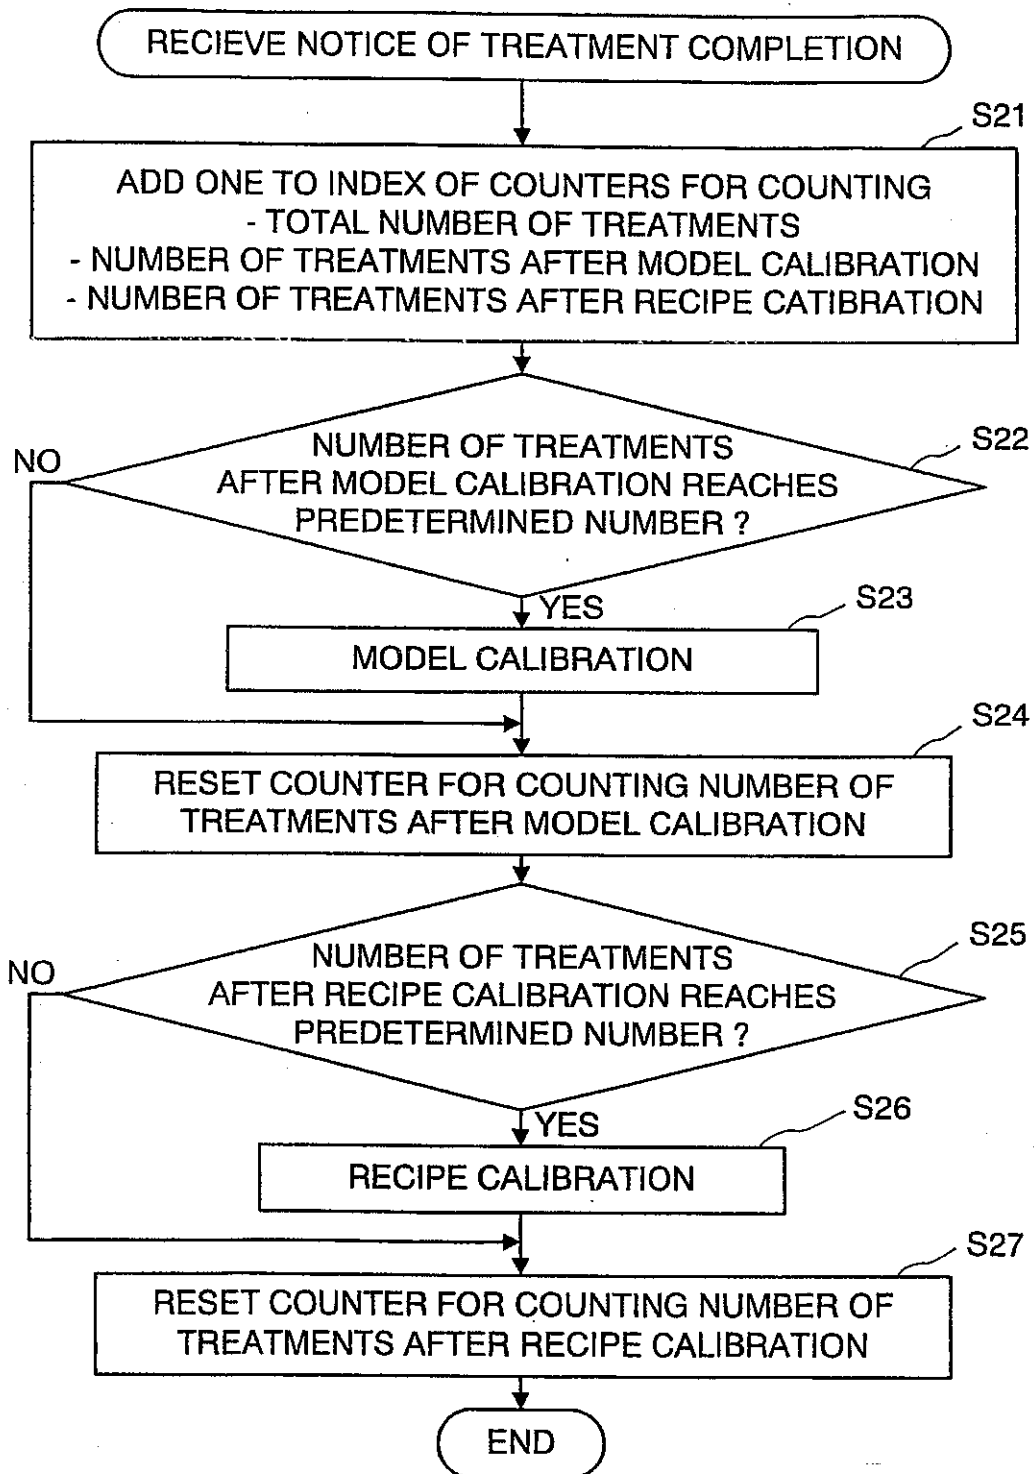


FIG. 12

13/13

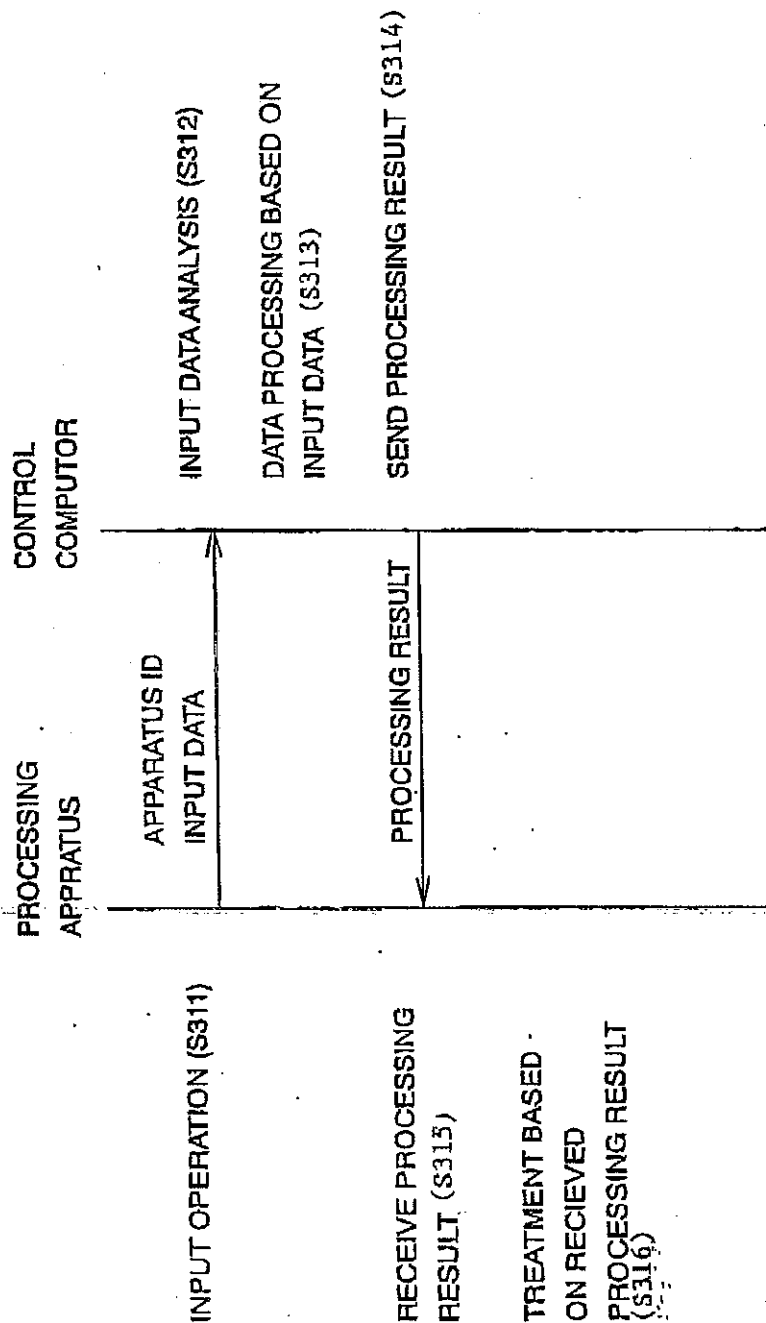


FIG. 13