

FIG. 1A

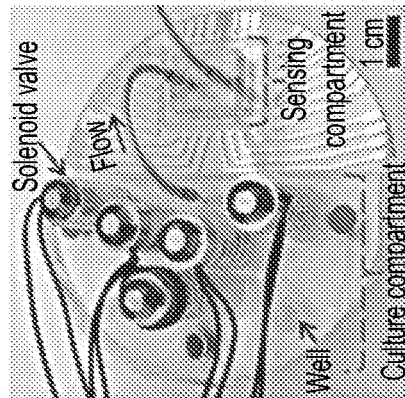


FIG. 1B

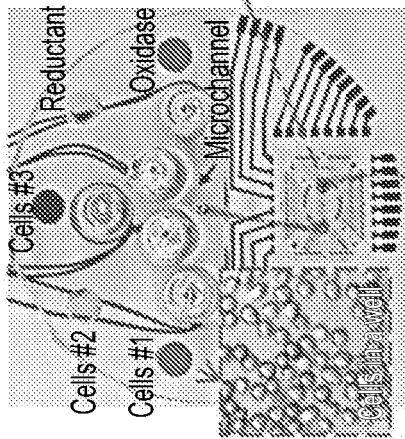


FIG. 1C

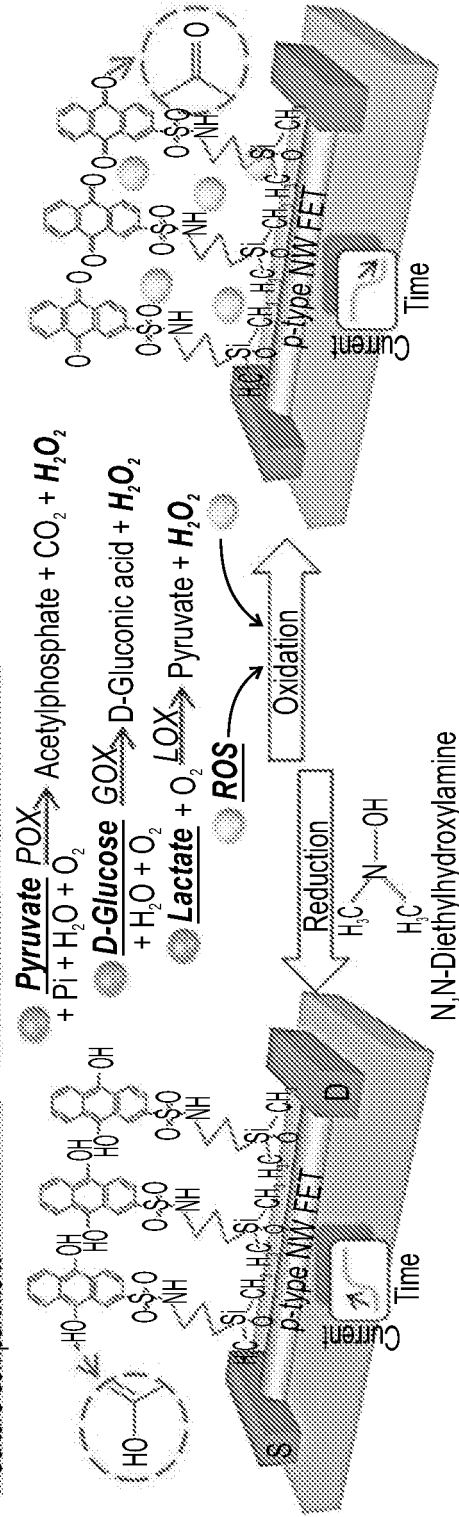
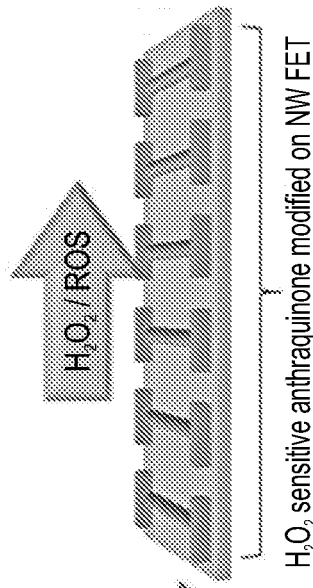


FIG. 1D

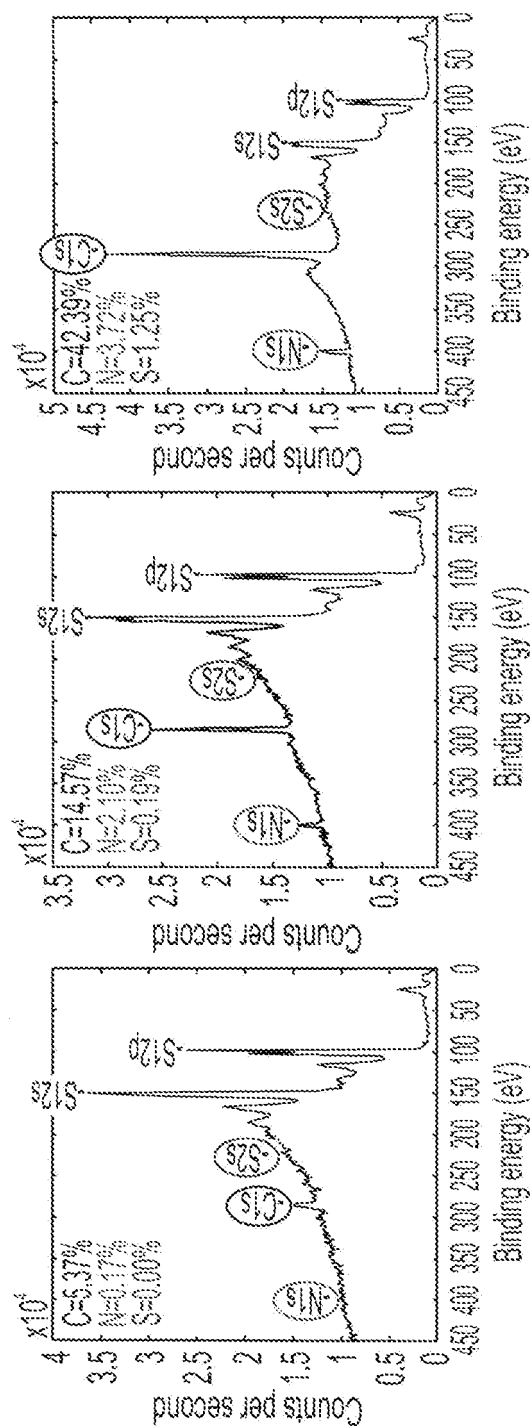
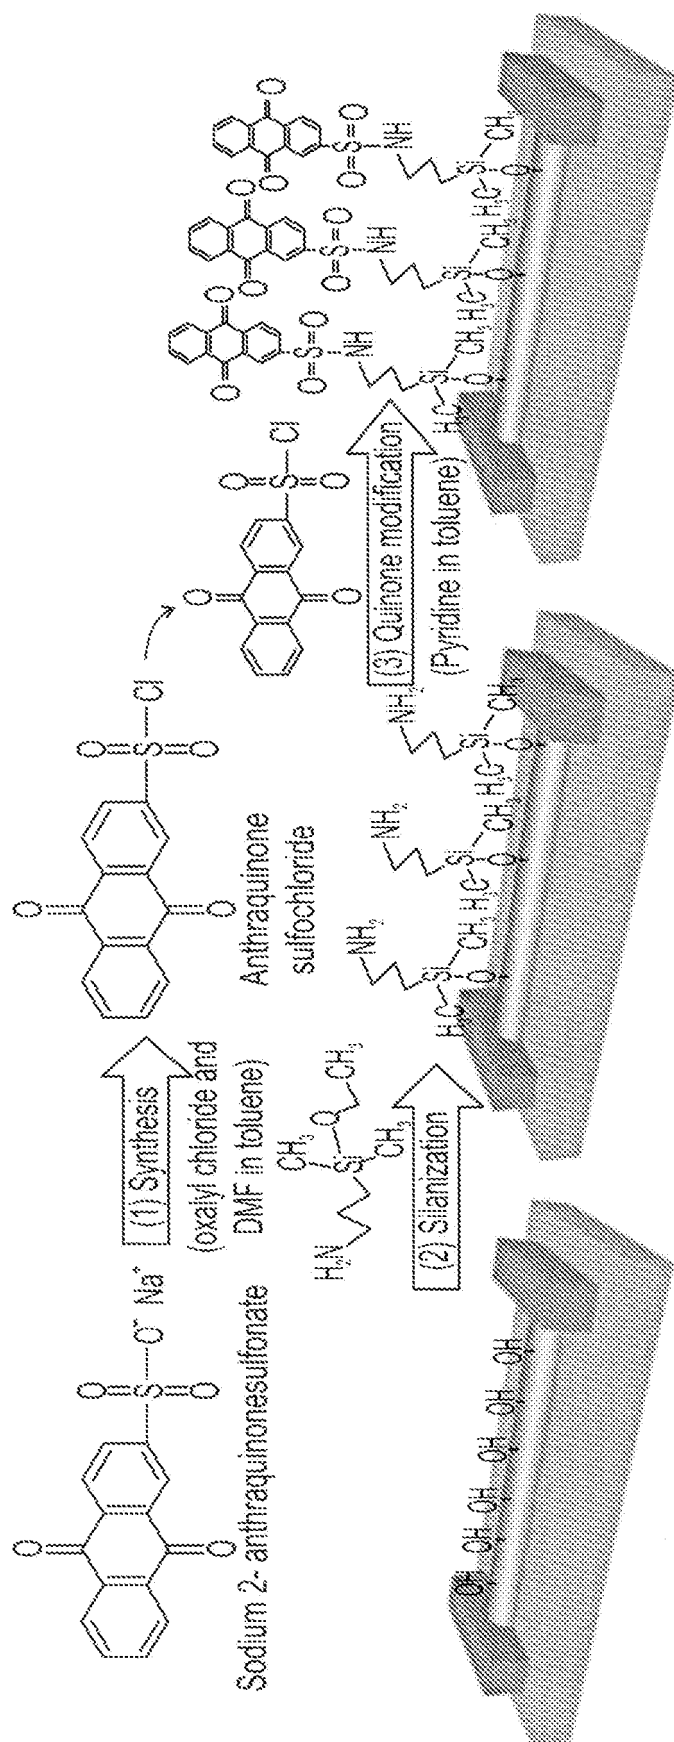


FIG. 2C

FIG. 2B

FIG. 2A

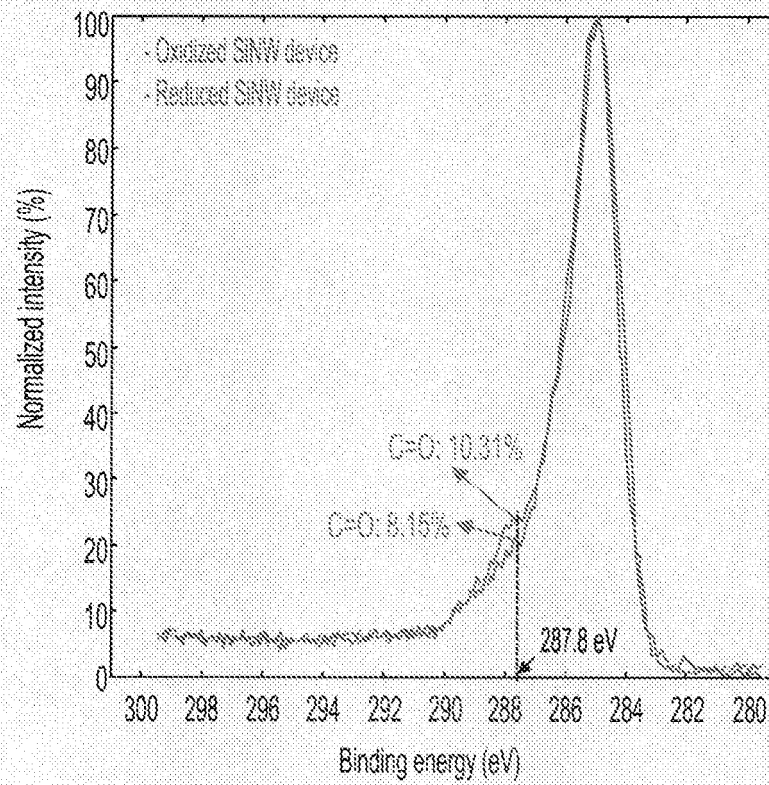
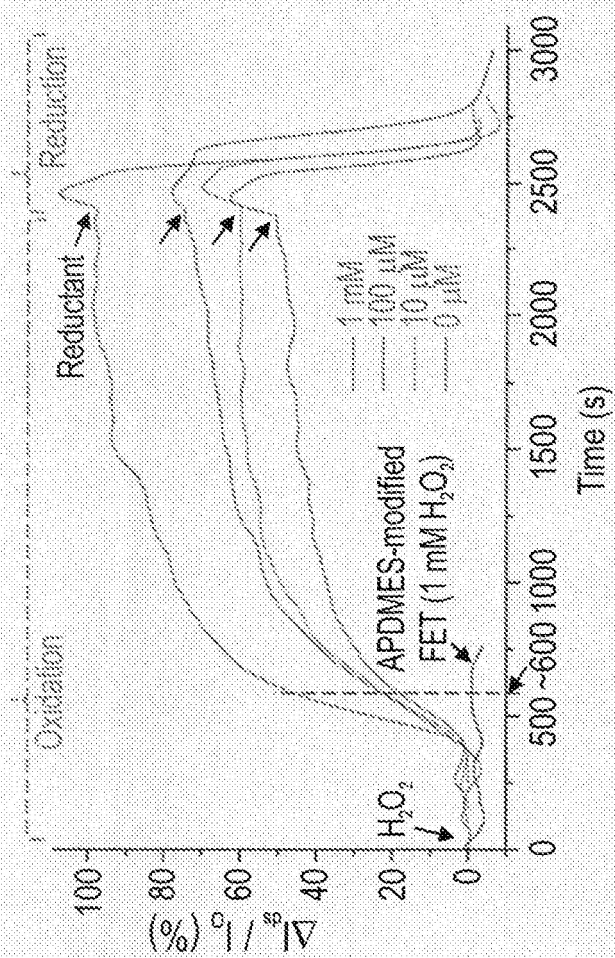


FIG. 2D



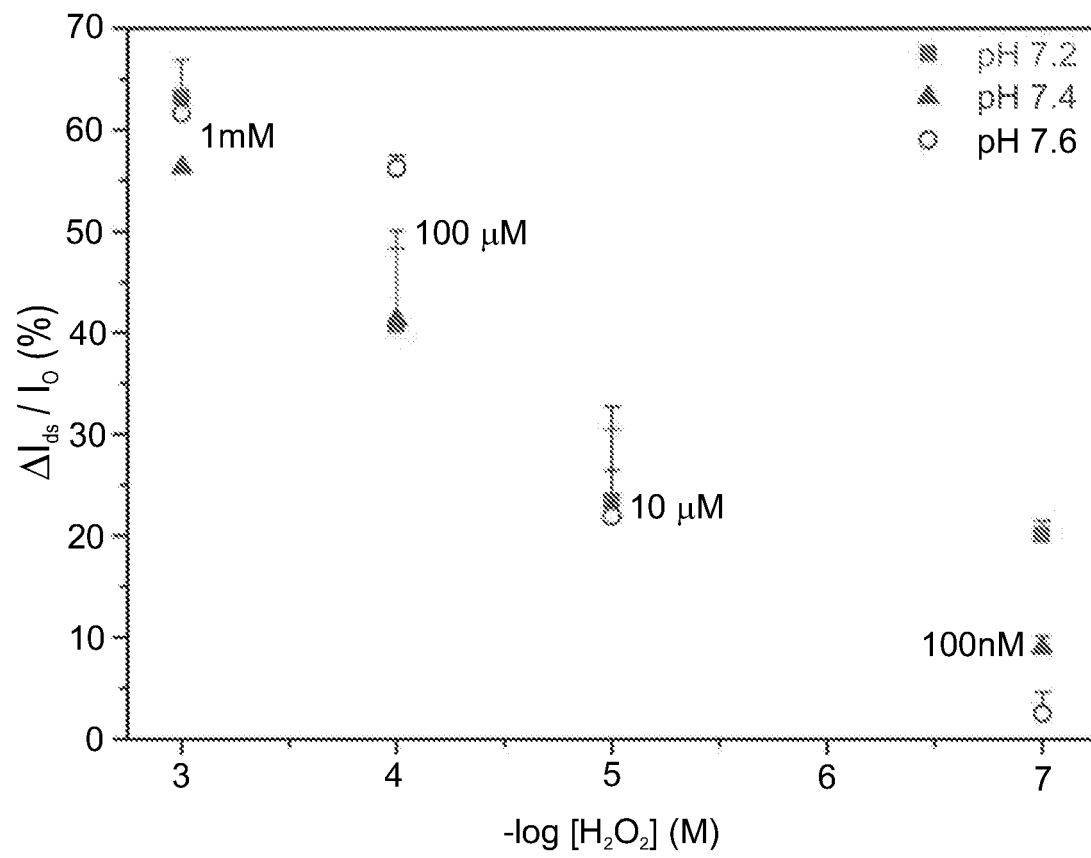


FIG. 3B

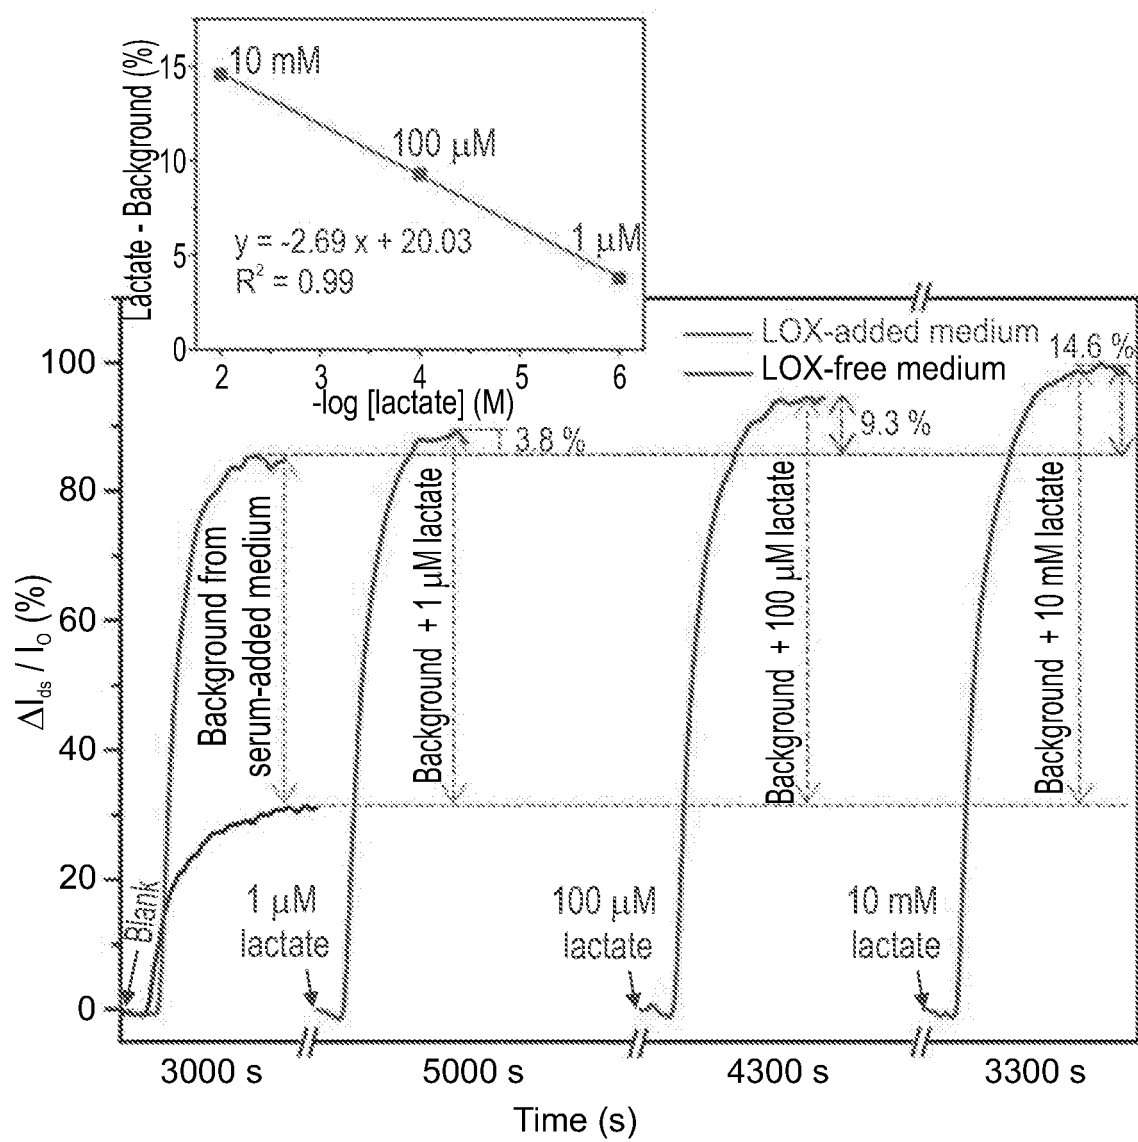


FIG. 4A

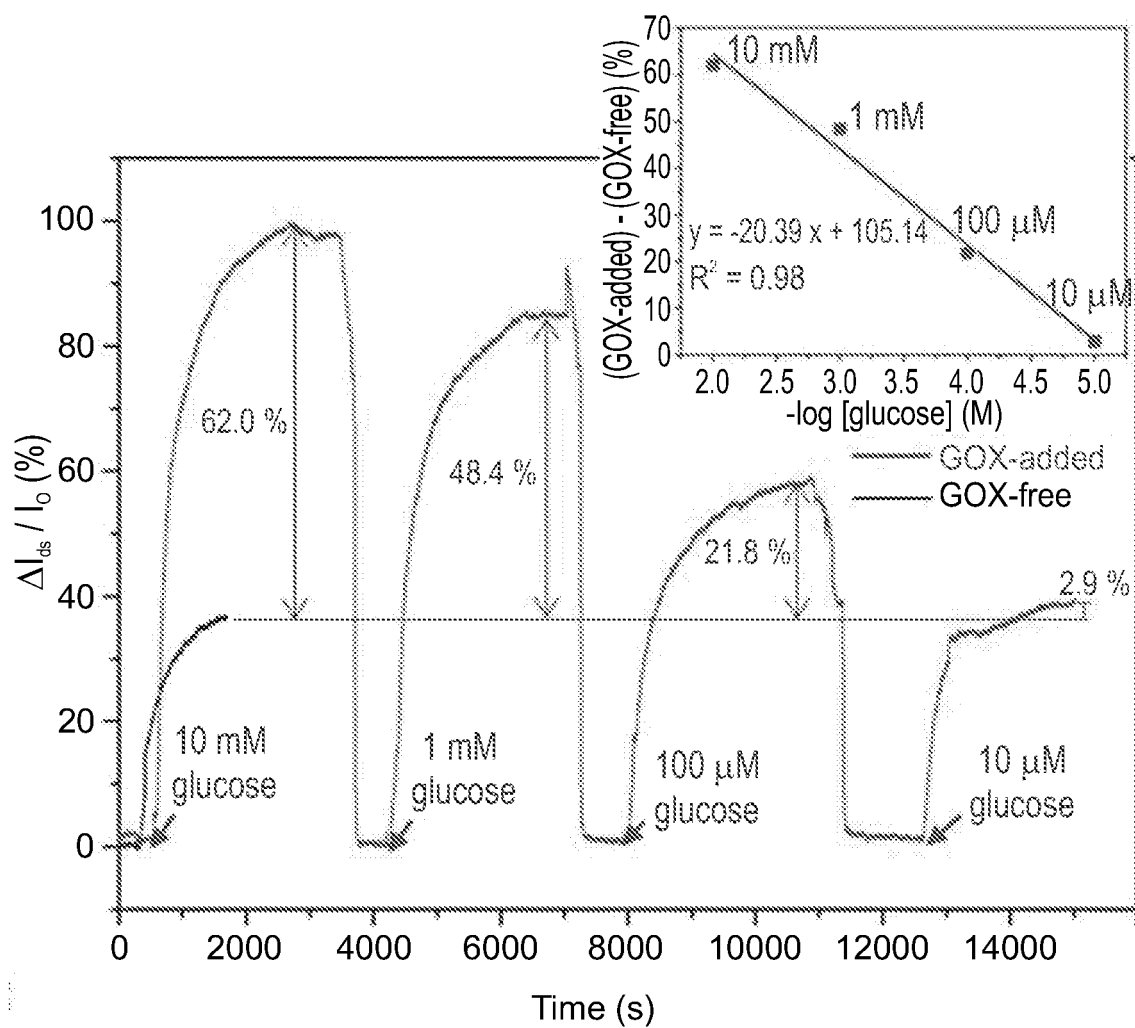


FIG. 4B

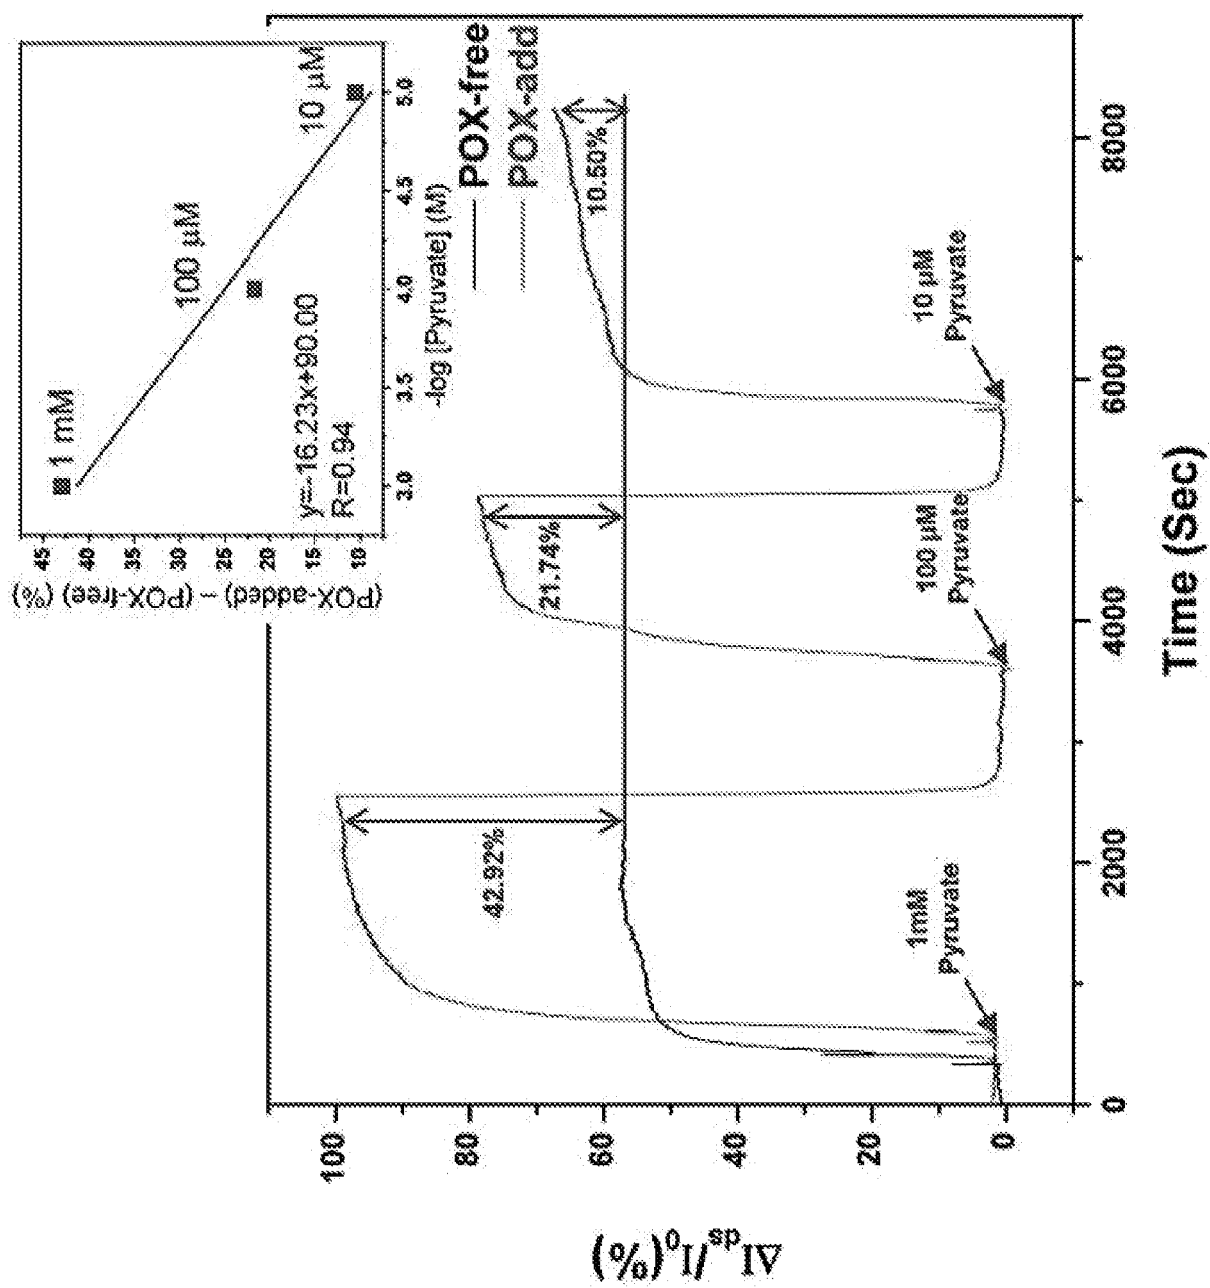


FIG. 4C

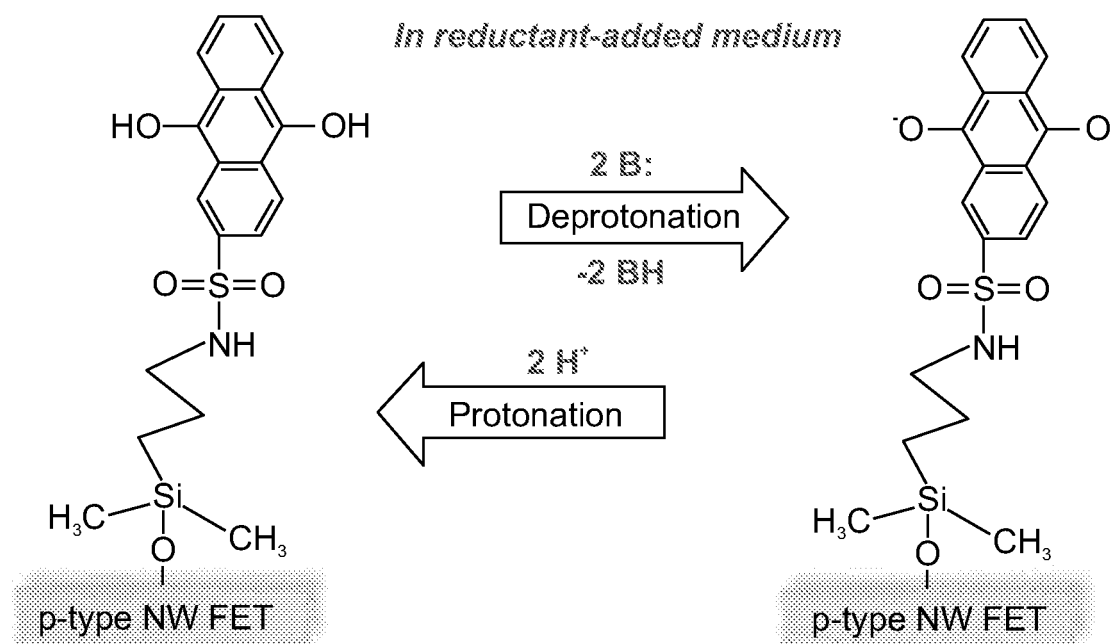


FIG. 5A

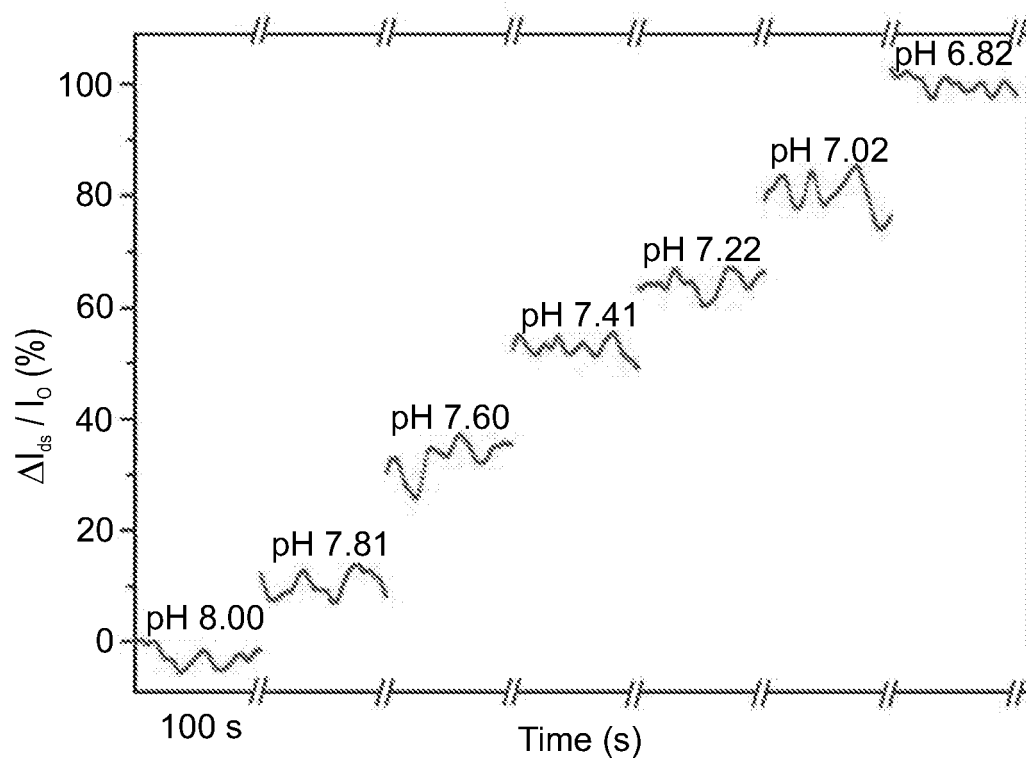


FIG. 5B

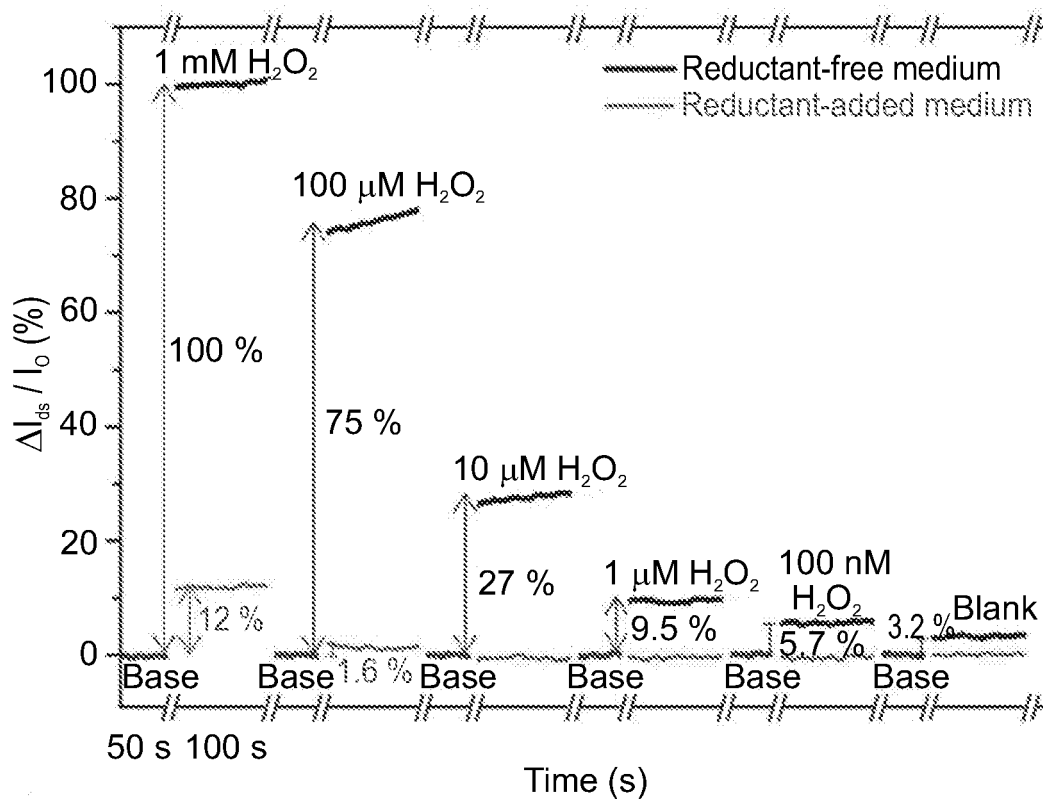


FIG. 5C

FIG. 6A

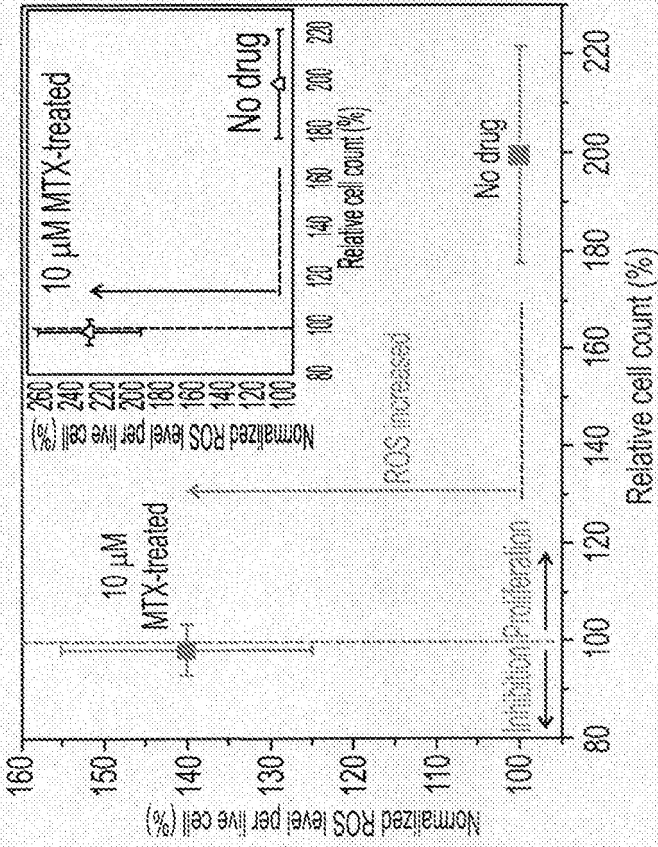
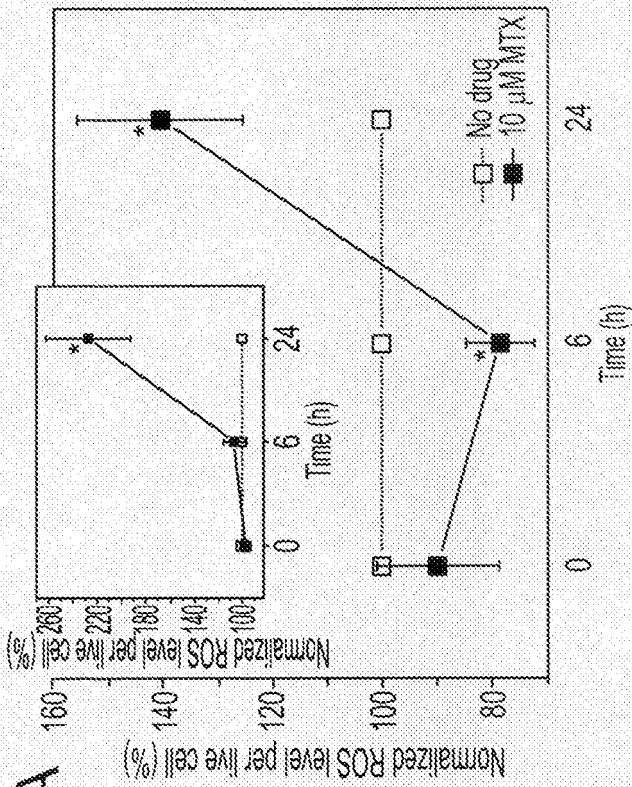


FIG. 6C

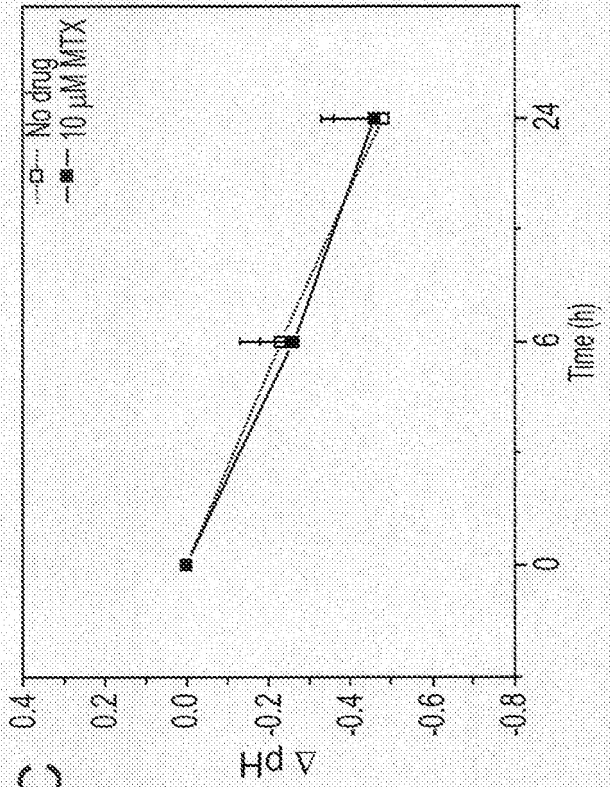


FIG. 6B

FIG. 6D

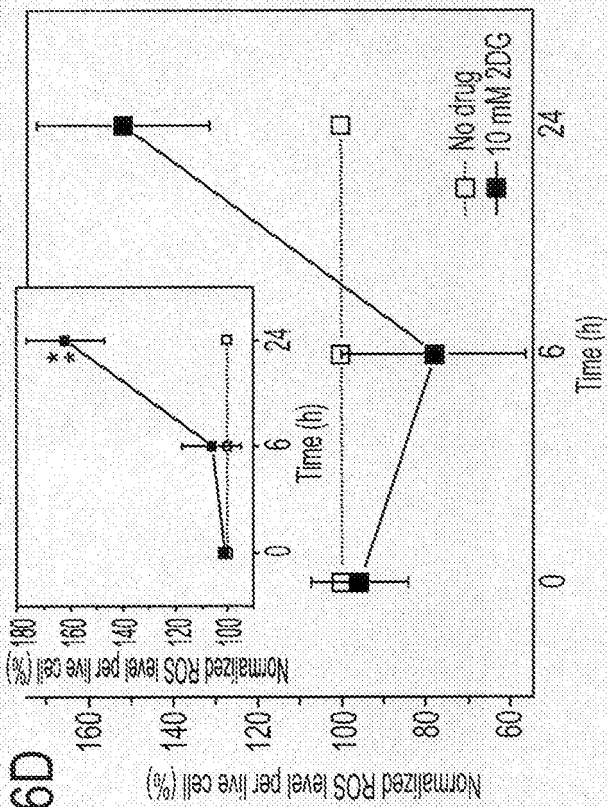


FIG. 6E

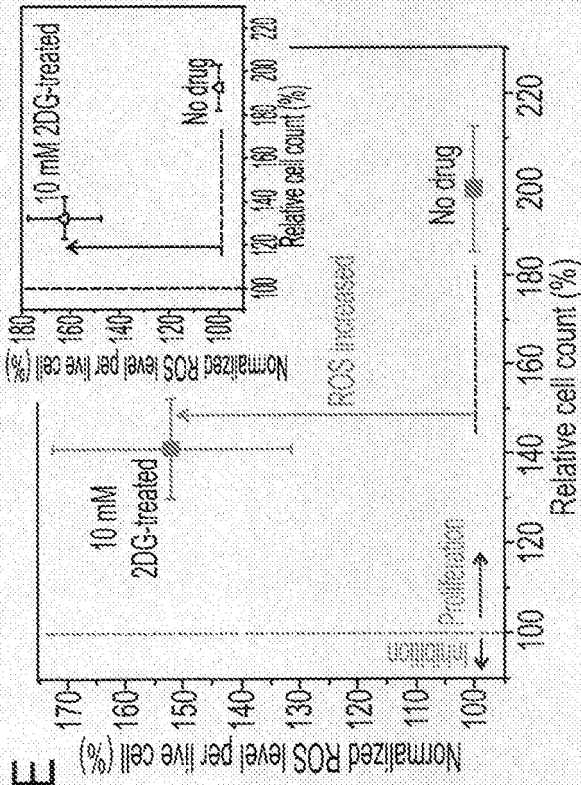


FIG. 6F

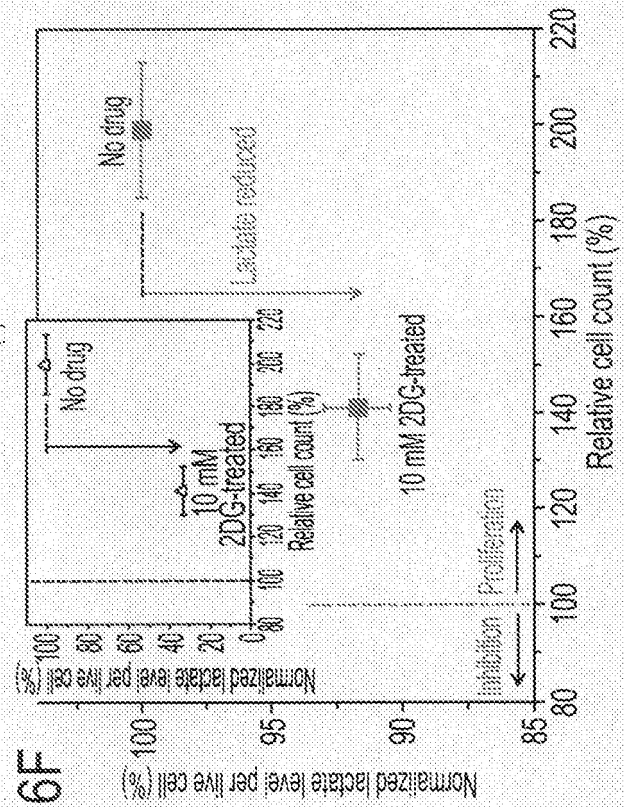
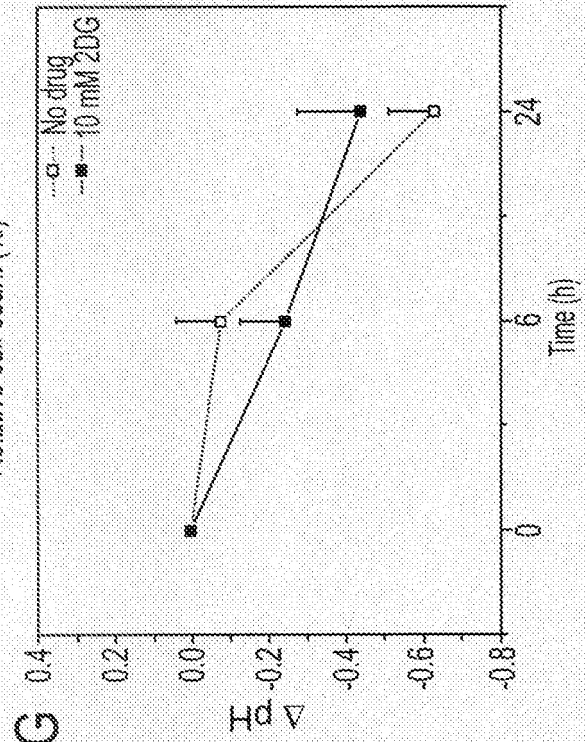


FIG. 6G



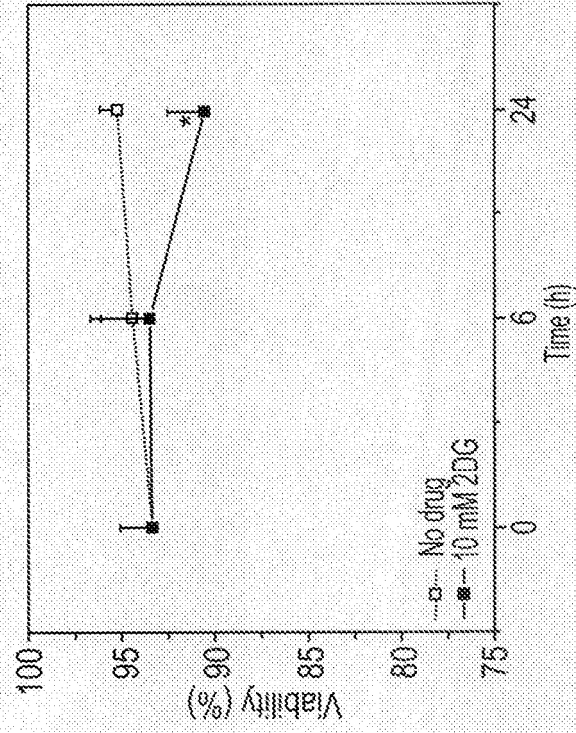


FIG. 6I

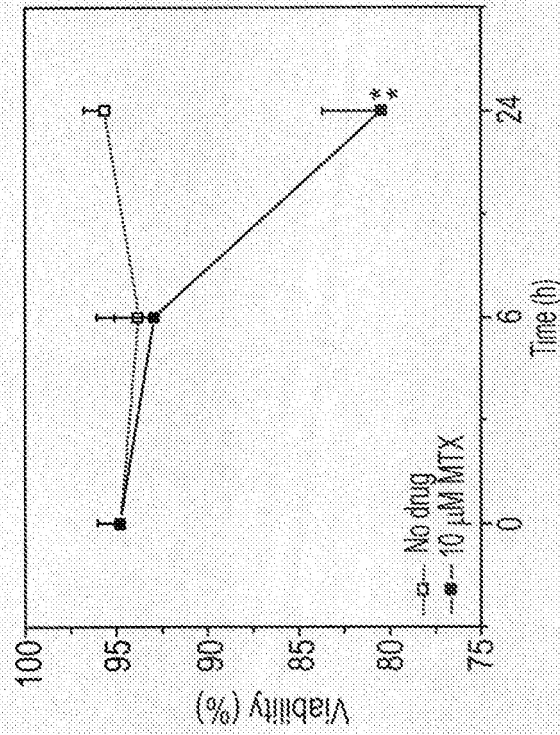


FIG. 6H

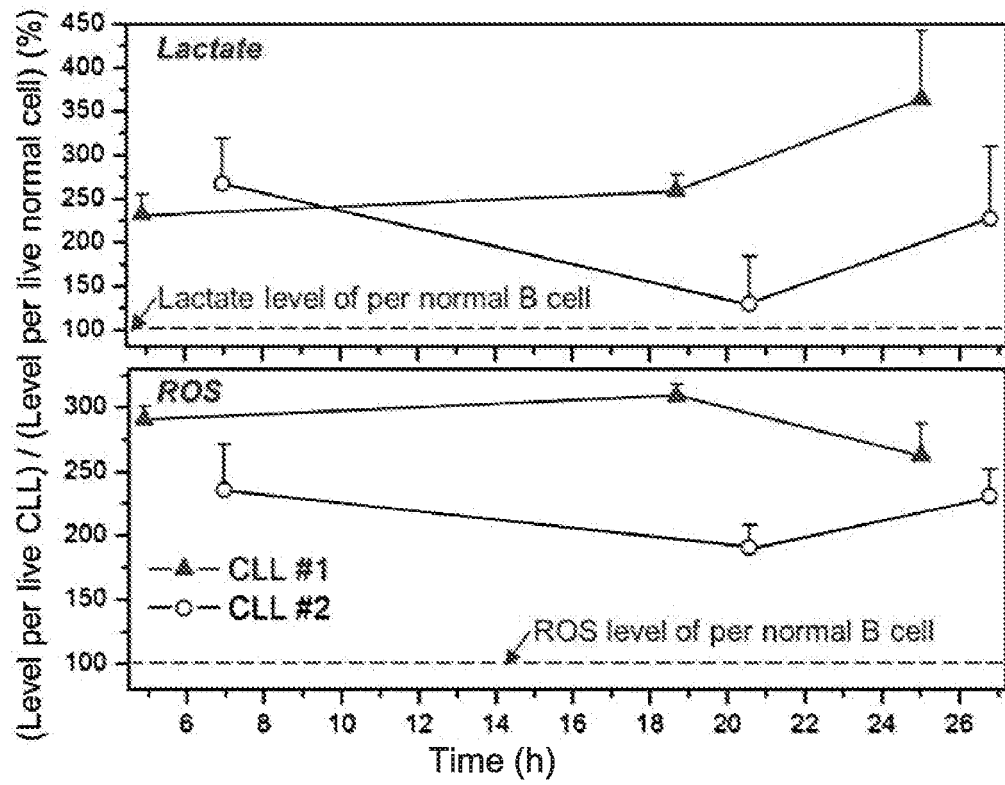


FIG. 7A


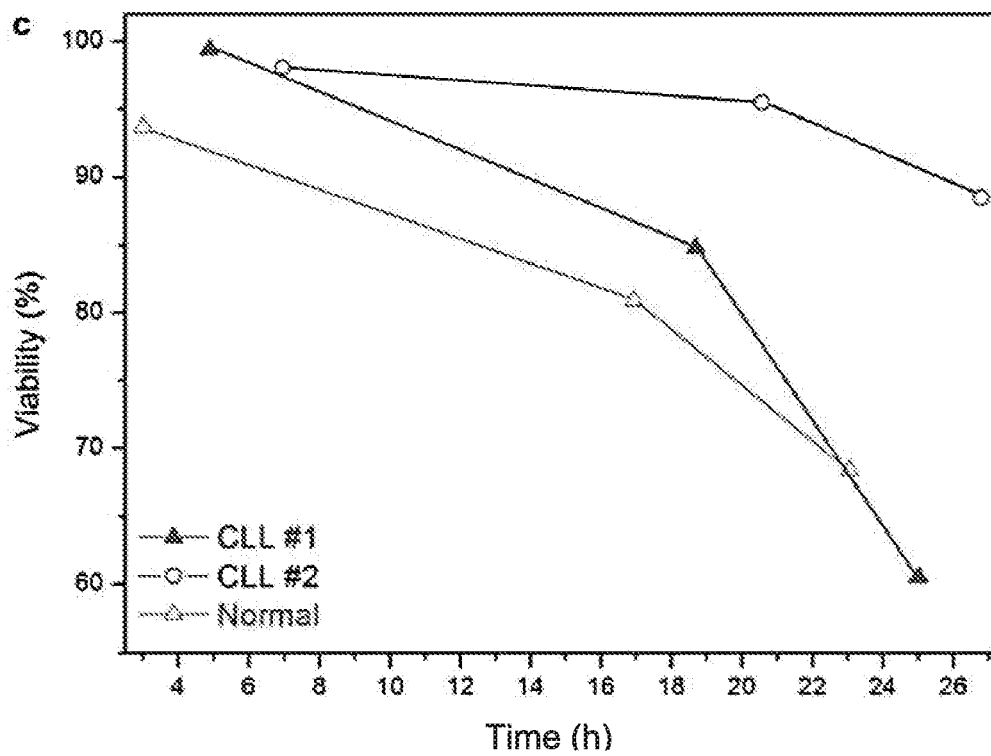


FIG. 7B

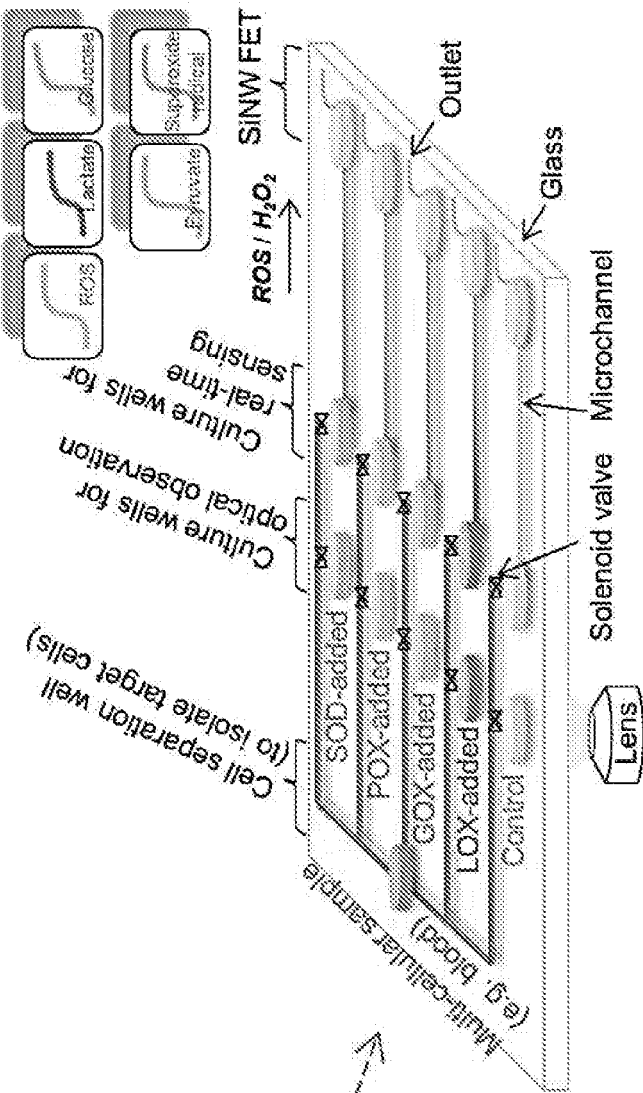

Microscope with a stage-top incubator

FIG. 8

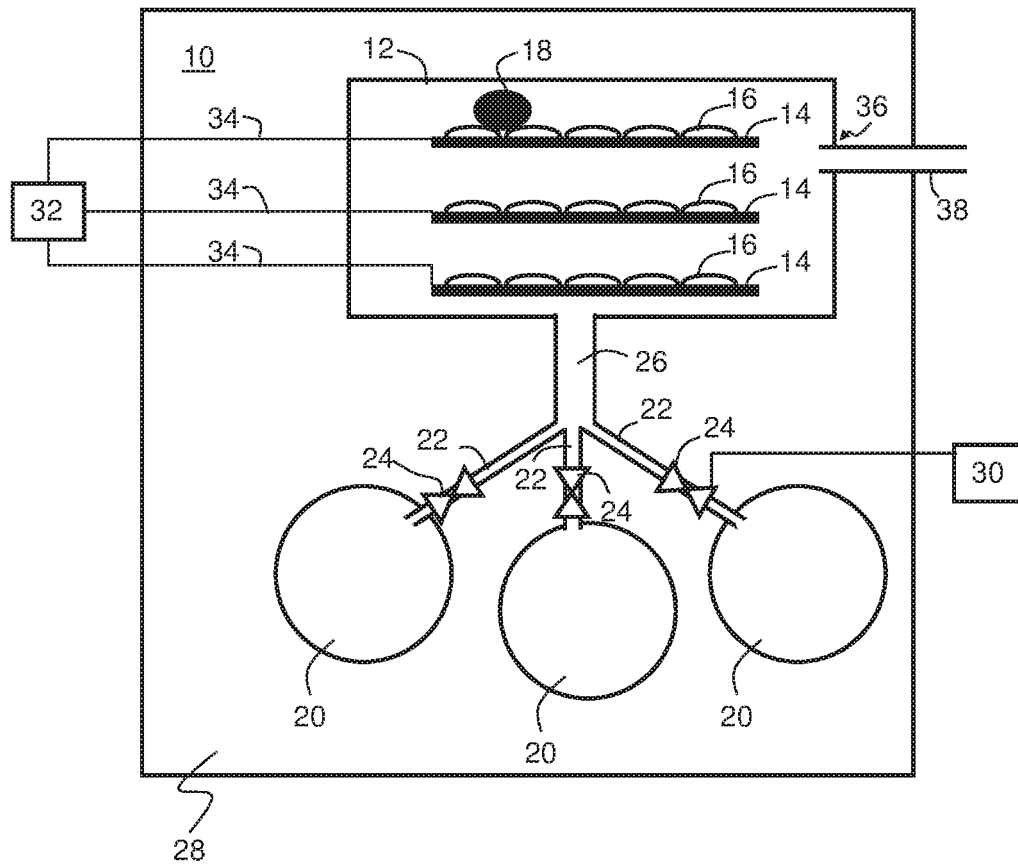


FIG. 9A

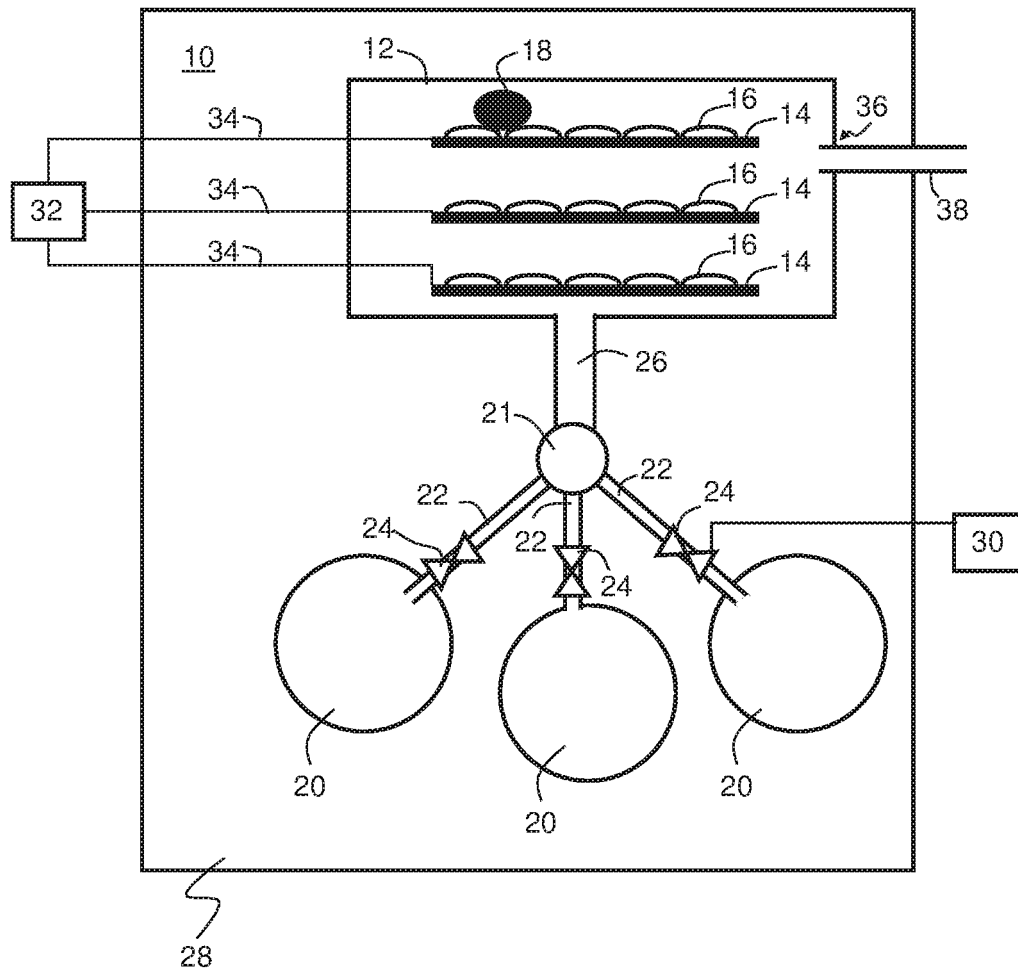


FIG. 9B

150

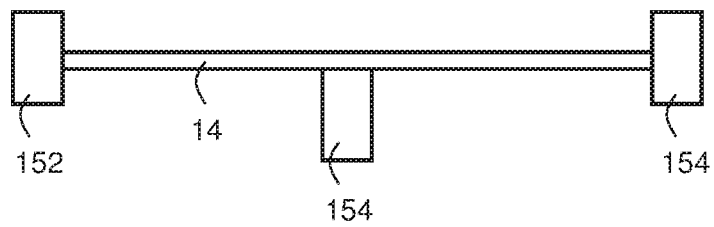


FIG. 10

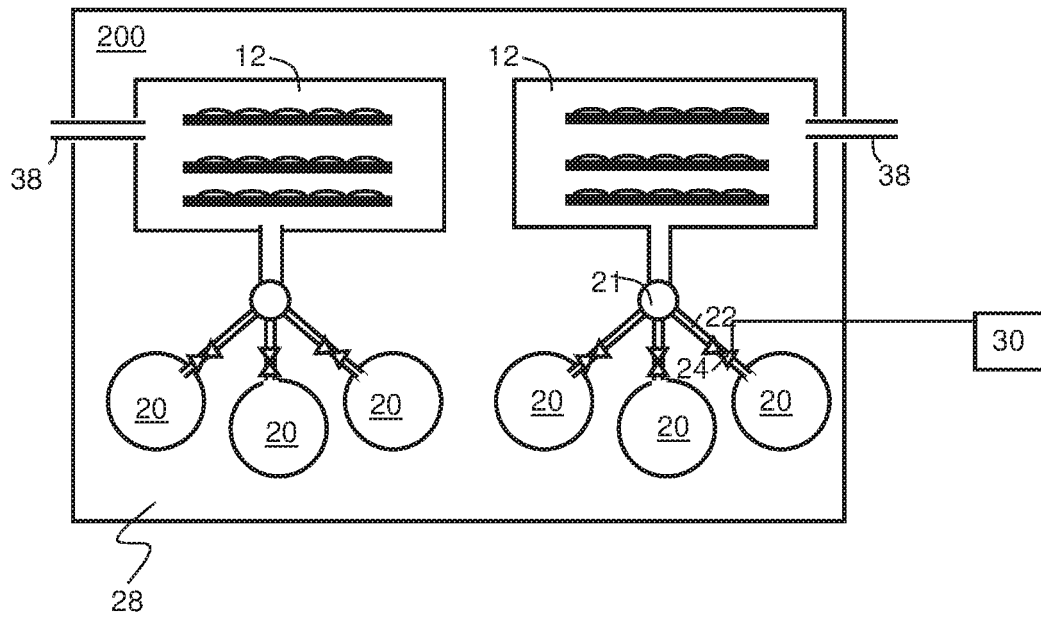


FIG. 11A

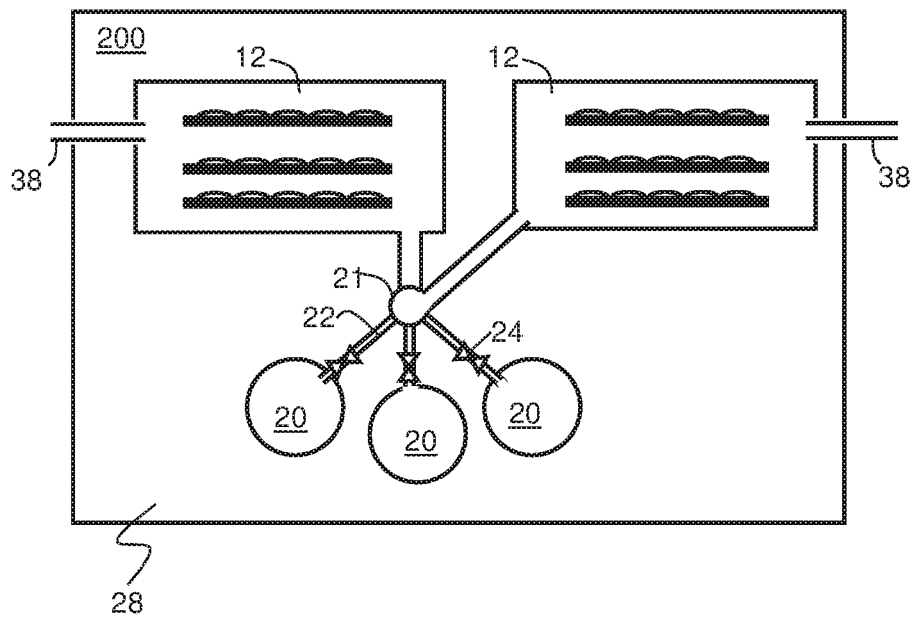


FIG. 11B

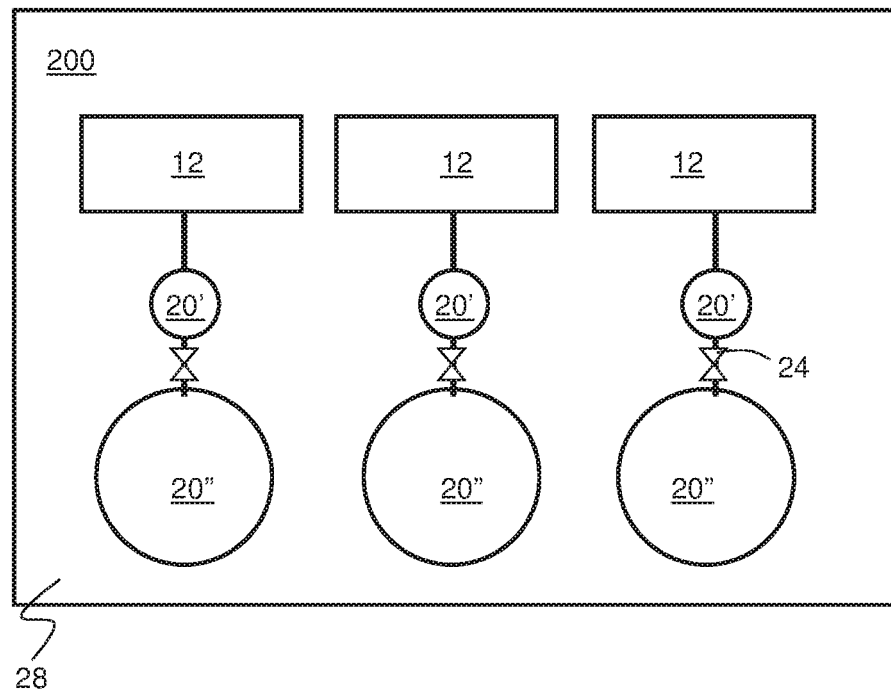


FIG. 11C