




[FIG. 1]


FIG. 1

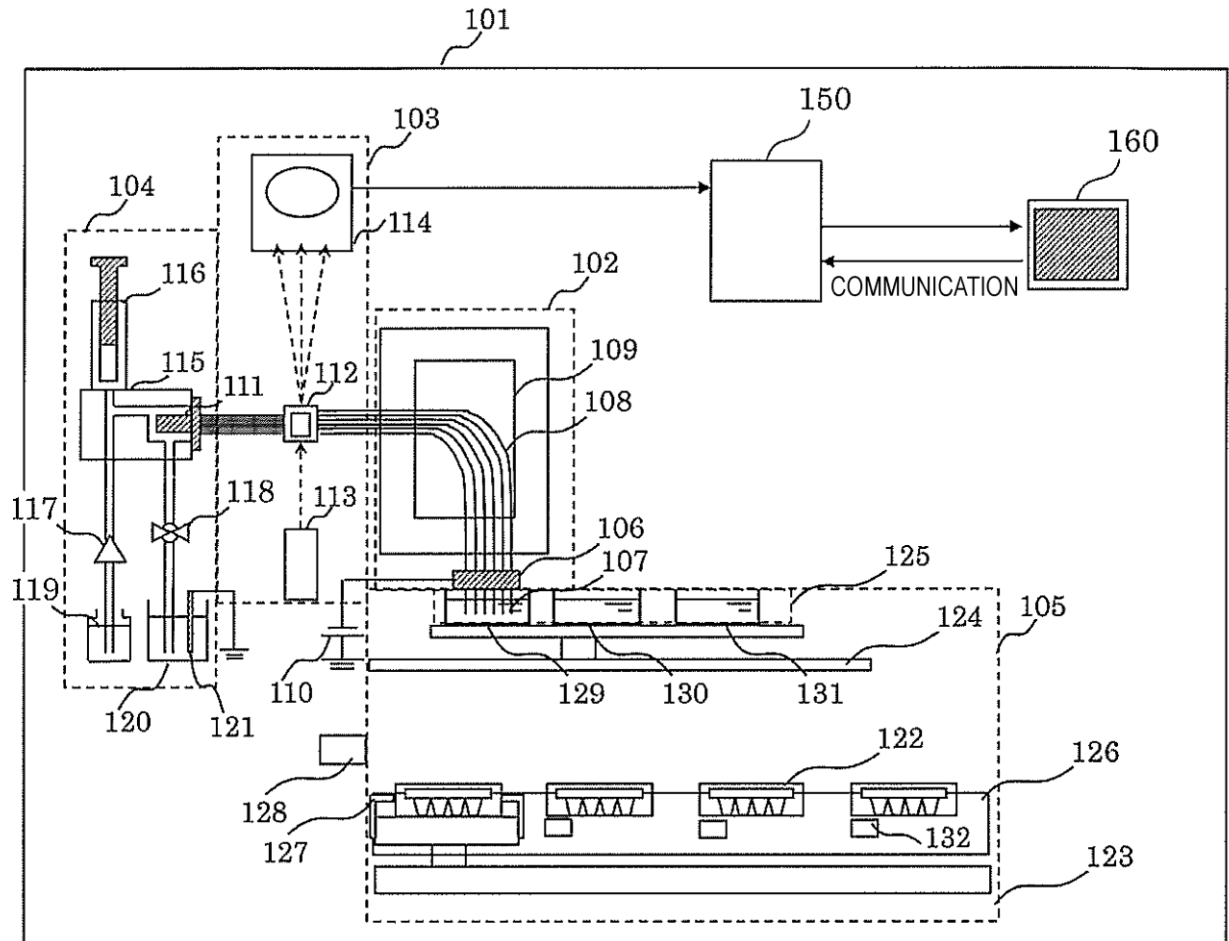


[FIG. 2]

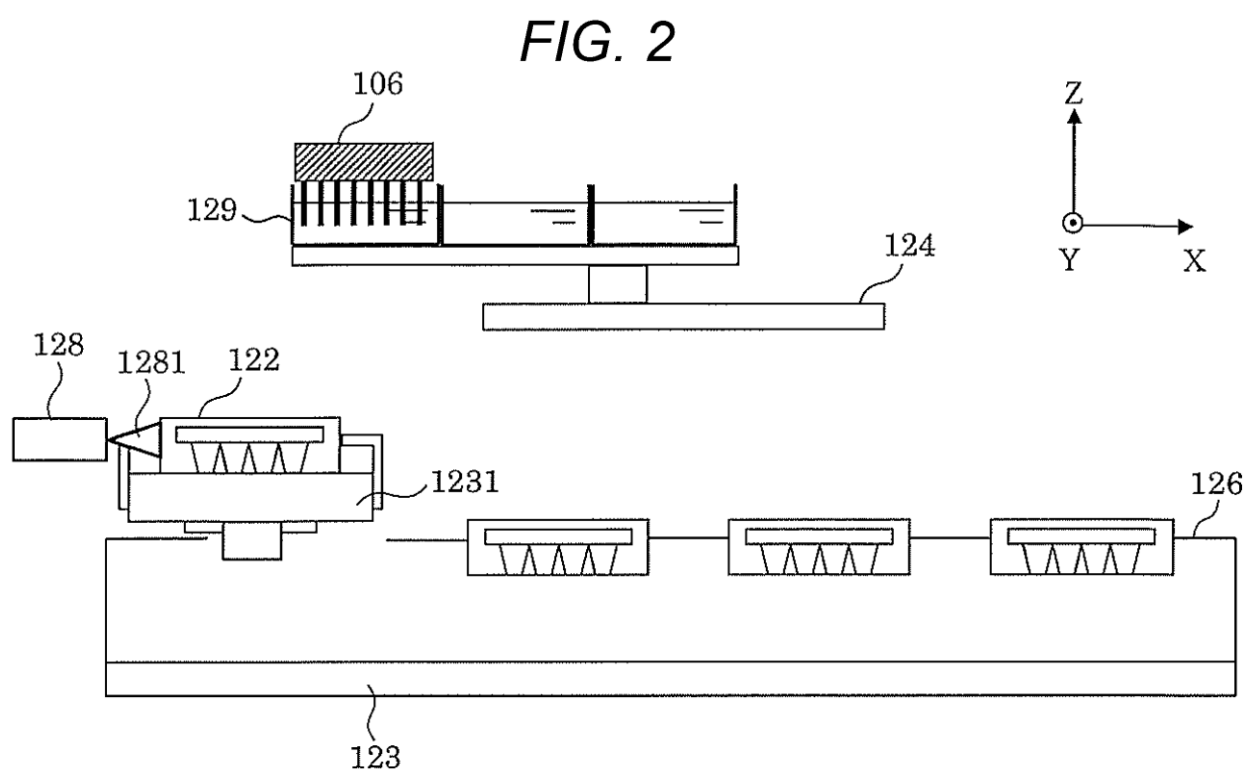


[FIG. 3]

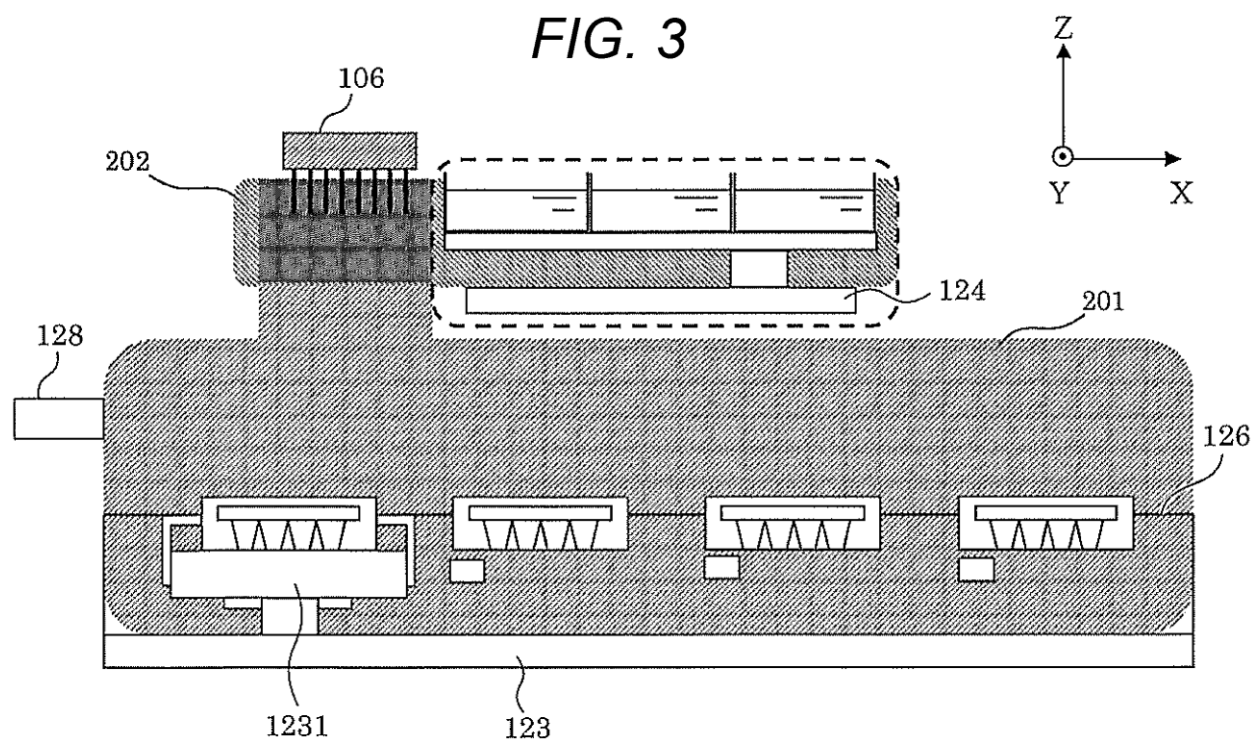


[FIG. 4A]

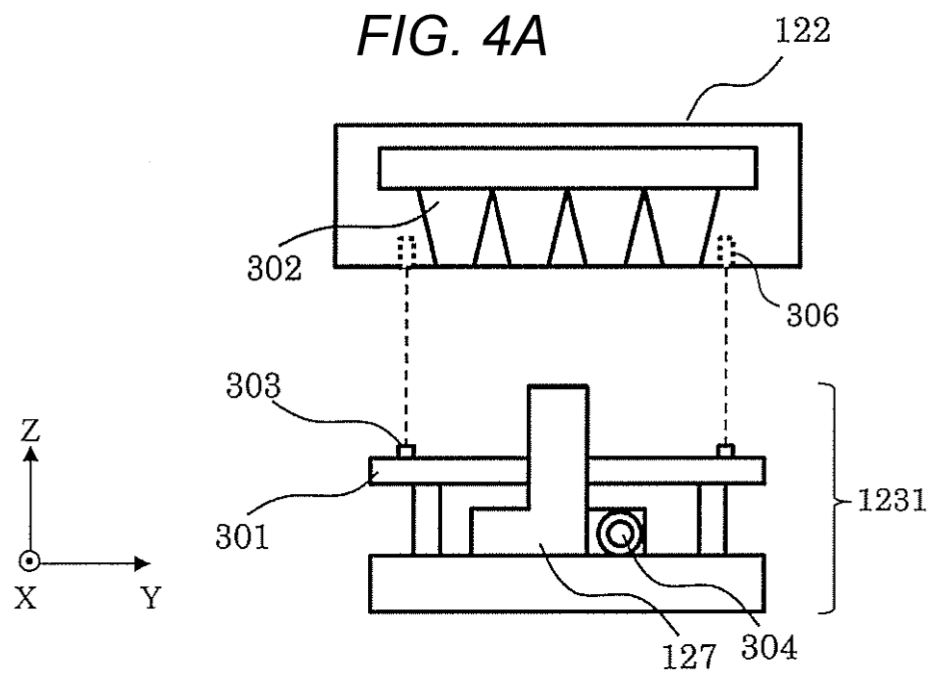


[FIG. 4B]

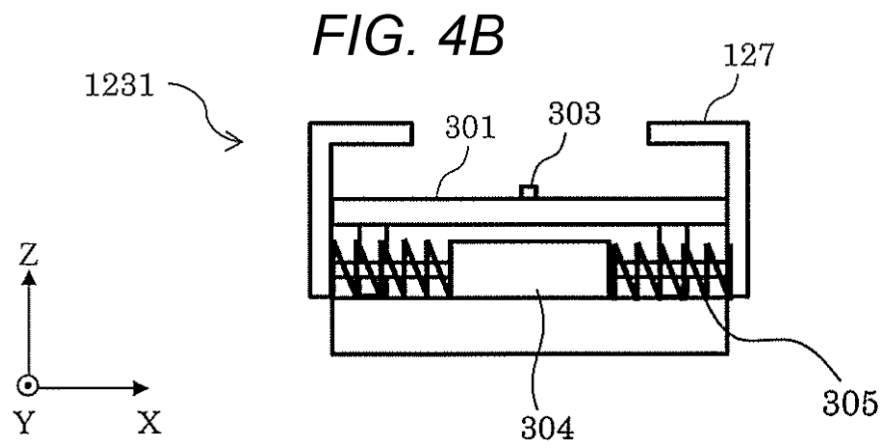


[FIG. 5A]

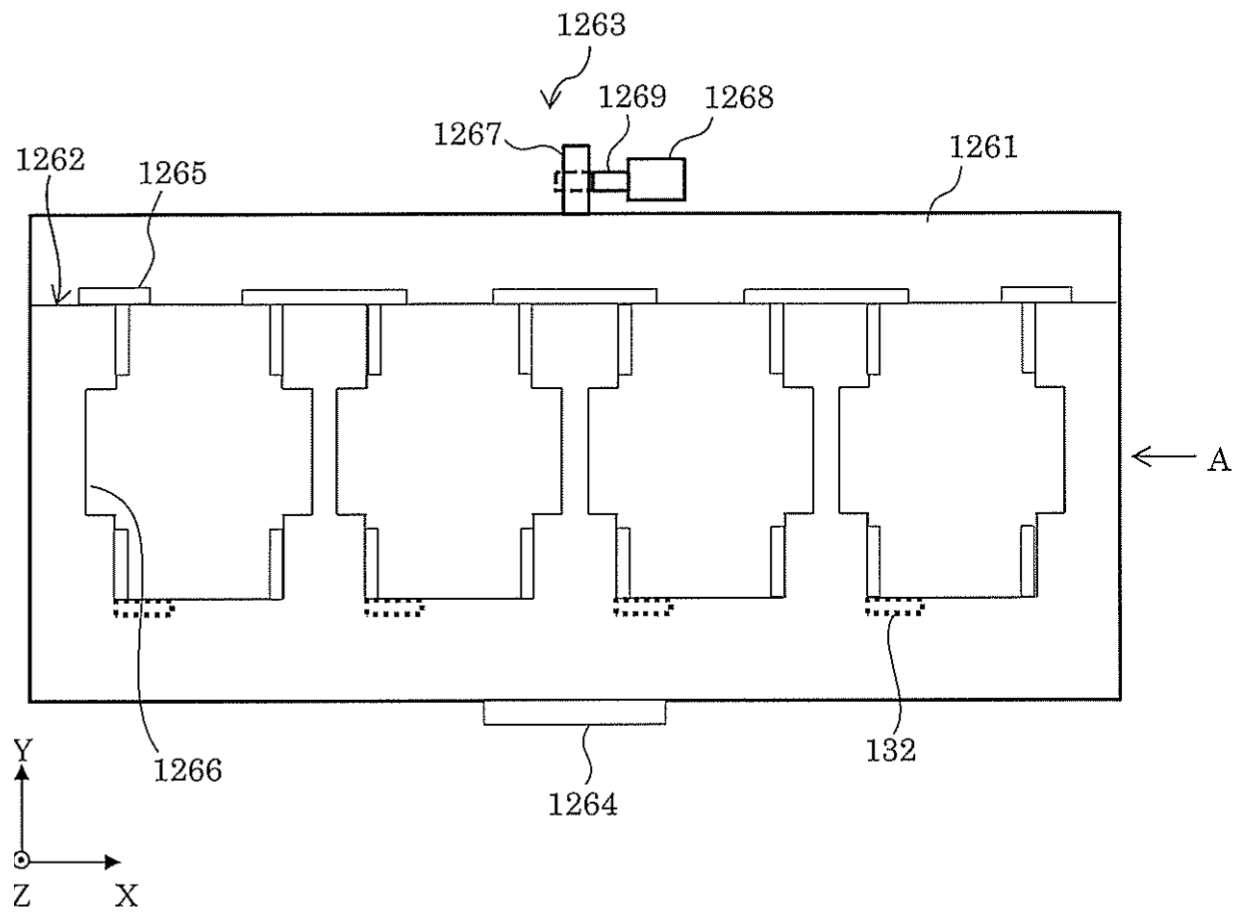FIG. 5A


[FIG. 5B]

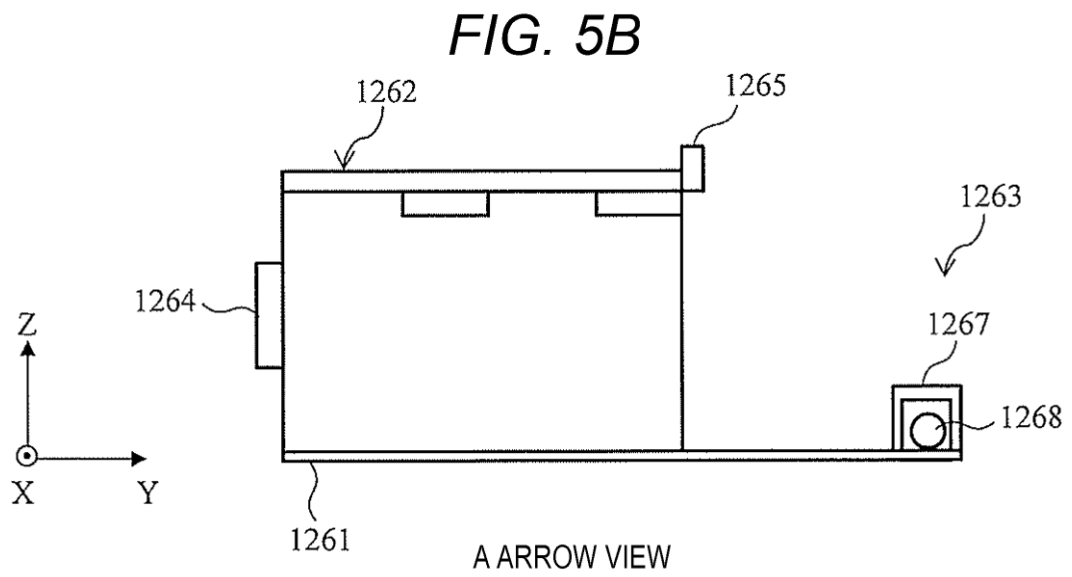

[FIG. 6]

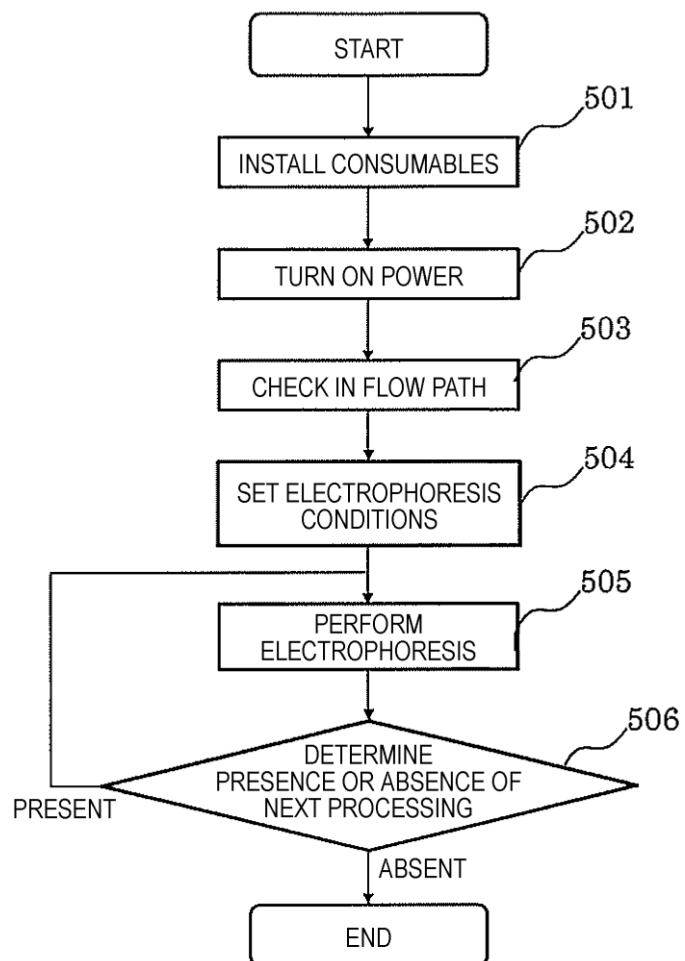FIG. 6


[FIG. 7]

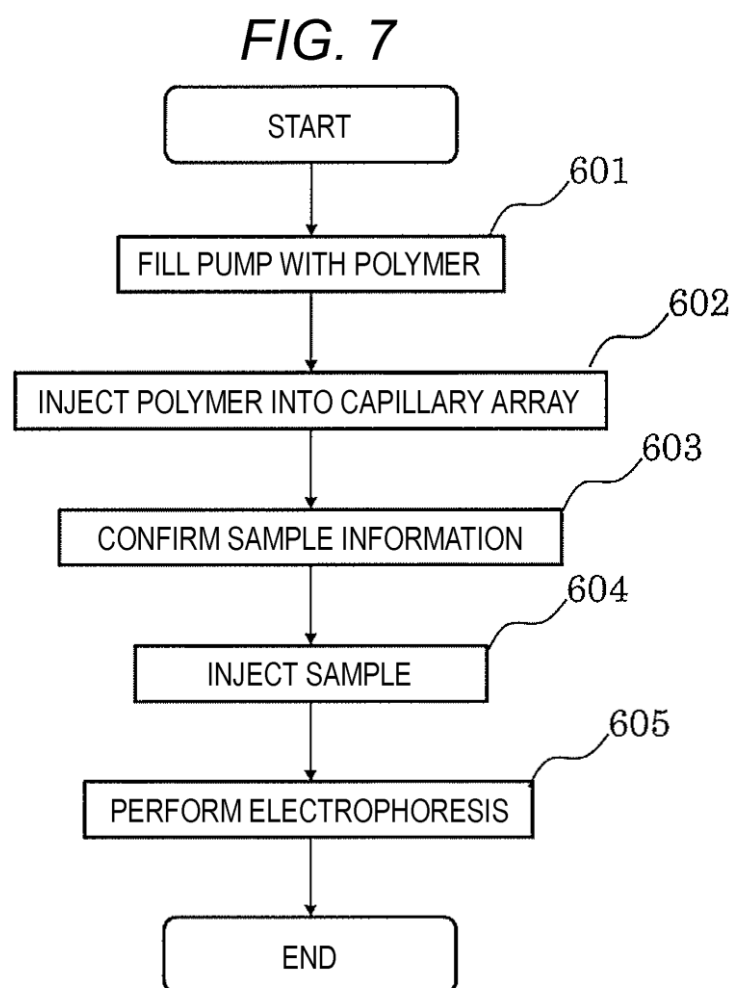


[FIG. 8]

FIG. 8


(1) SAMPLE INFORMATION READING

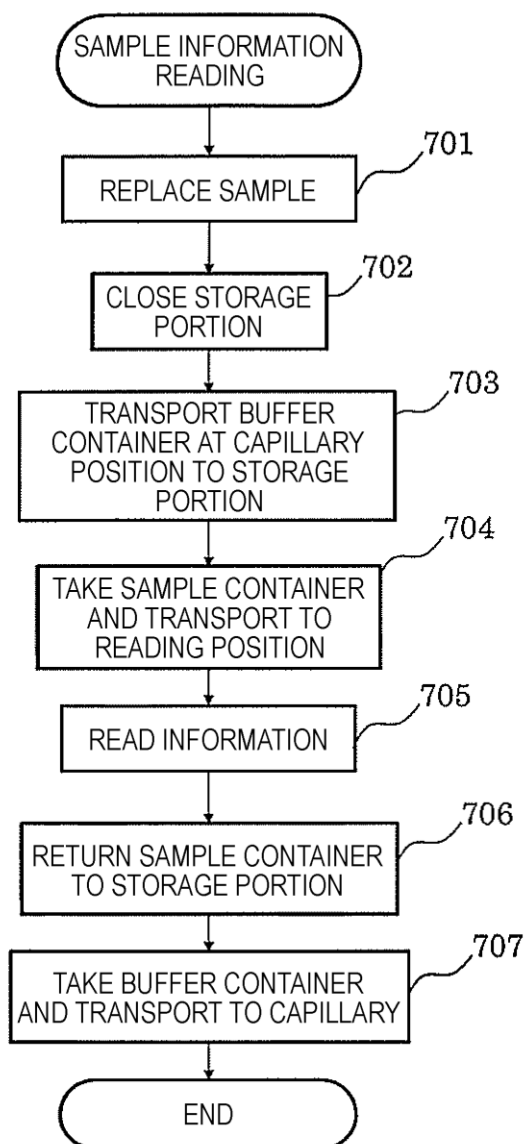

(2) REPLACEMENT OF SAMPLE CONTAINER AND BUFFER CONTAINER TO CAPILLARY IN INJECTING SAMPLE

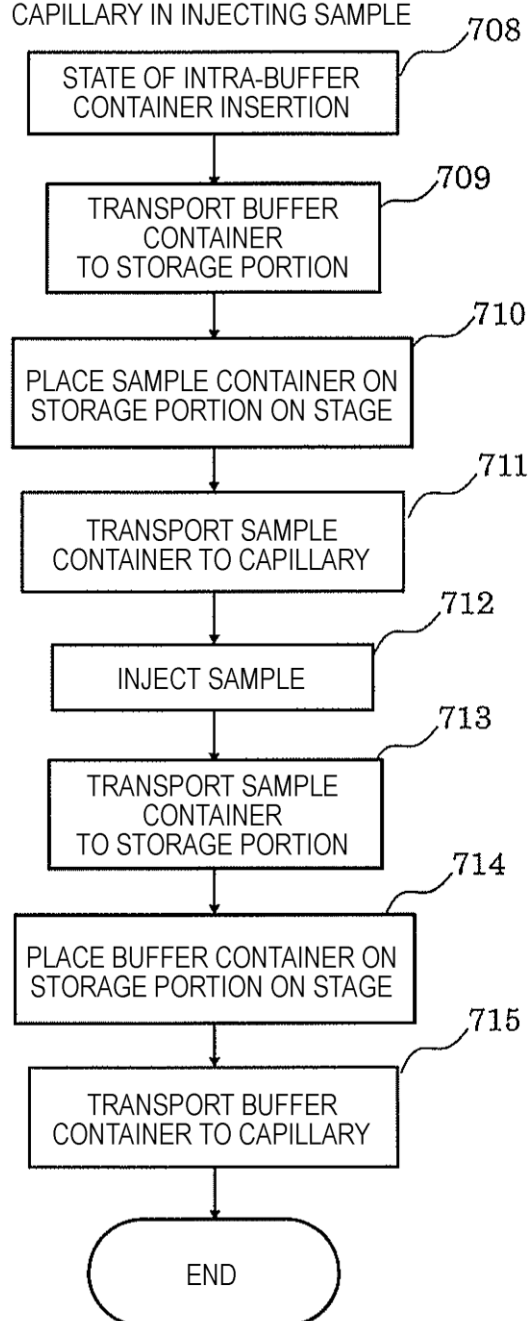


[FIG. 9]

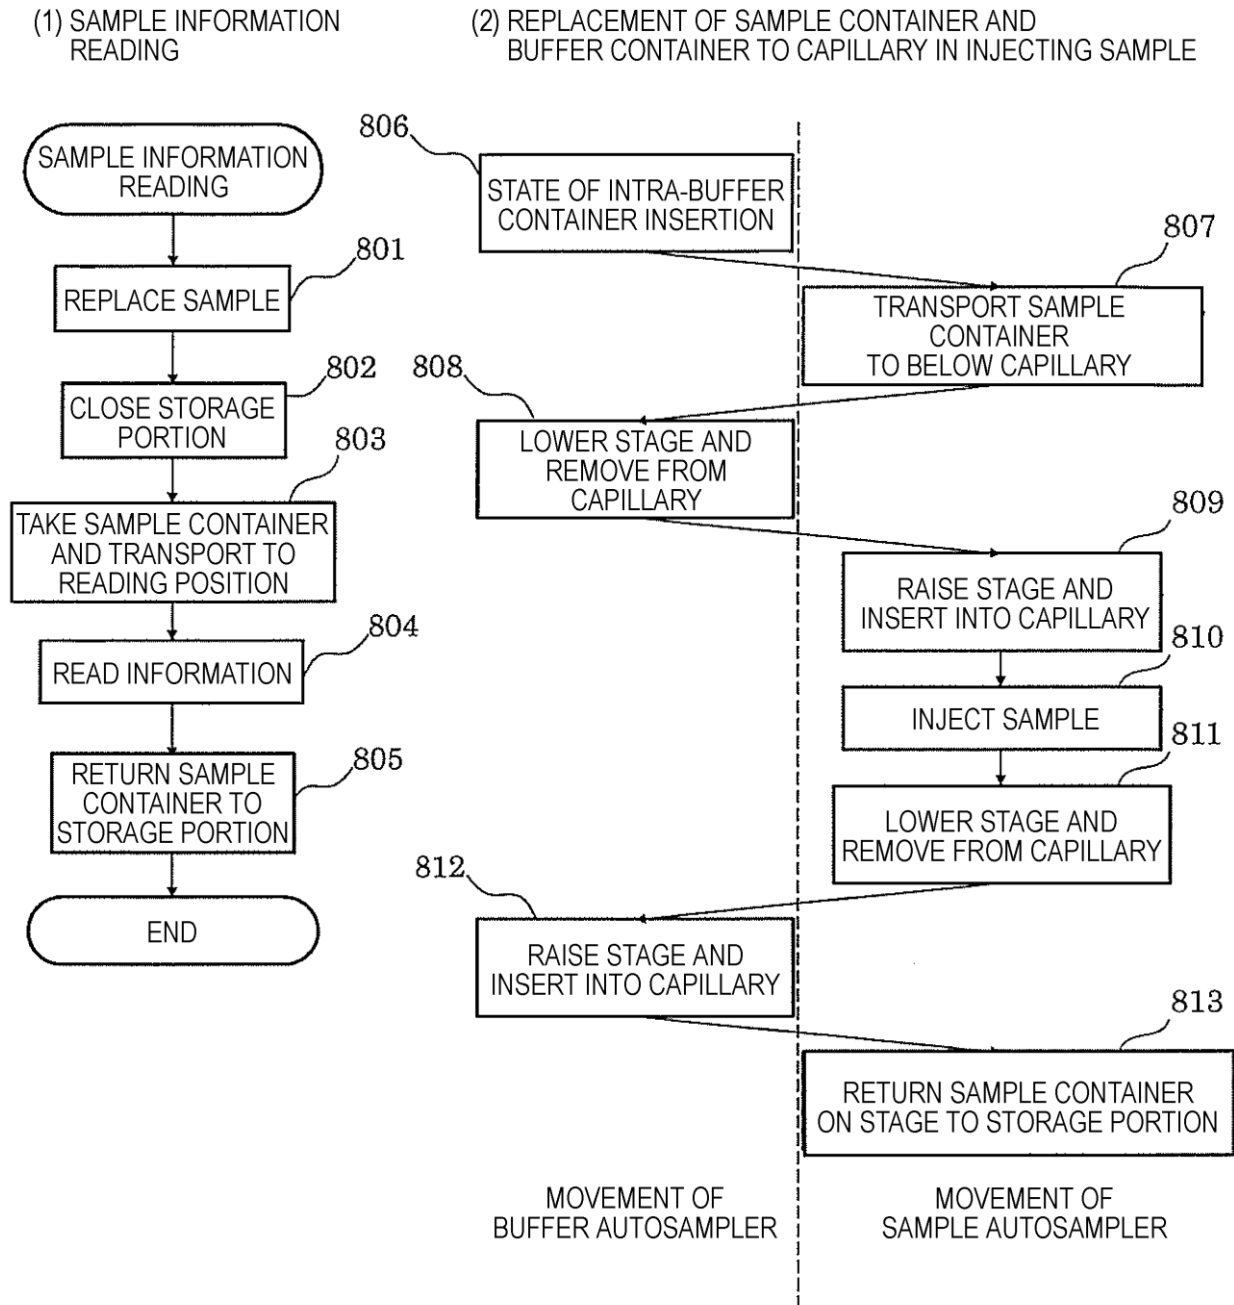
FIG. 9

[FIG. 10]


FIG. 10

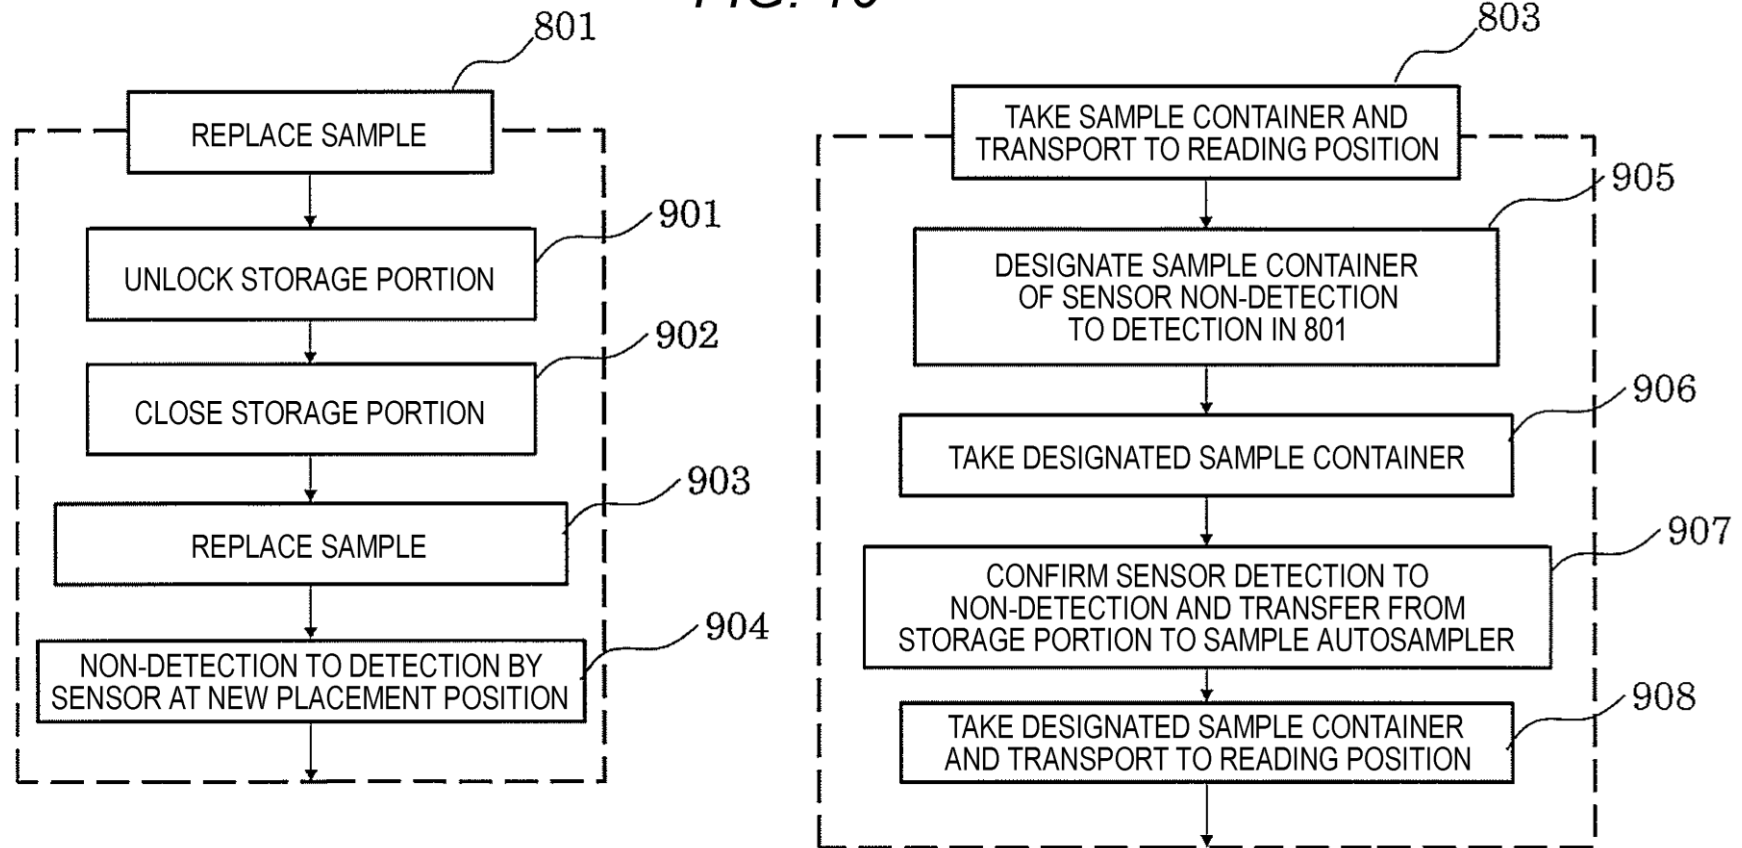

[FIG. 11]

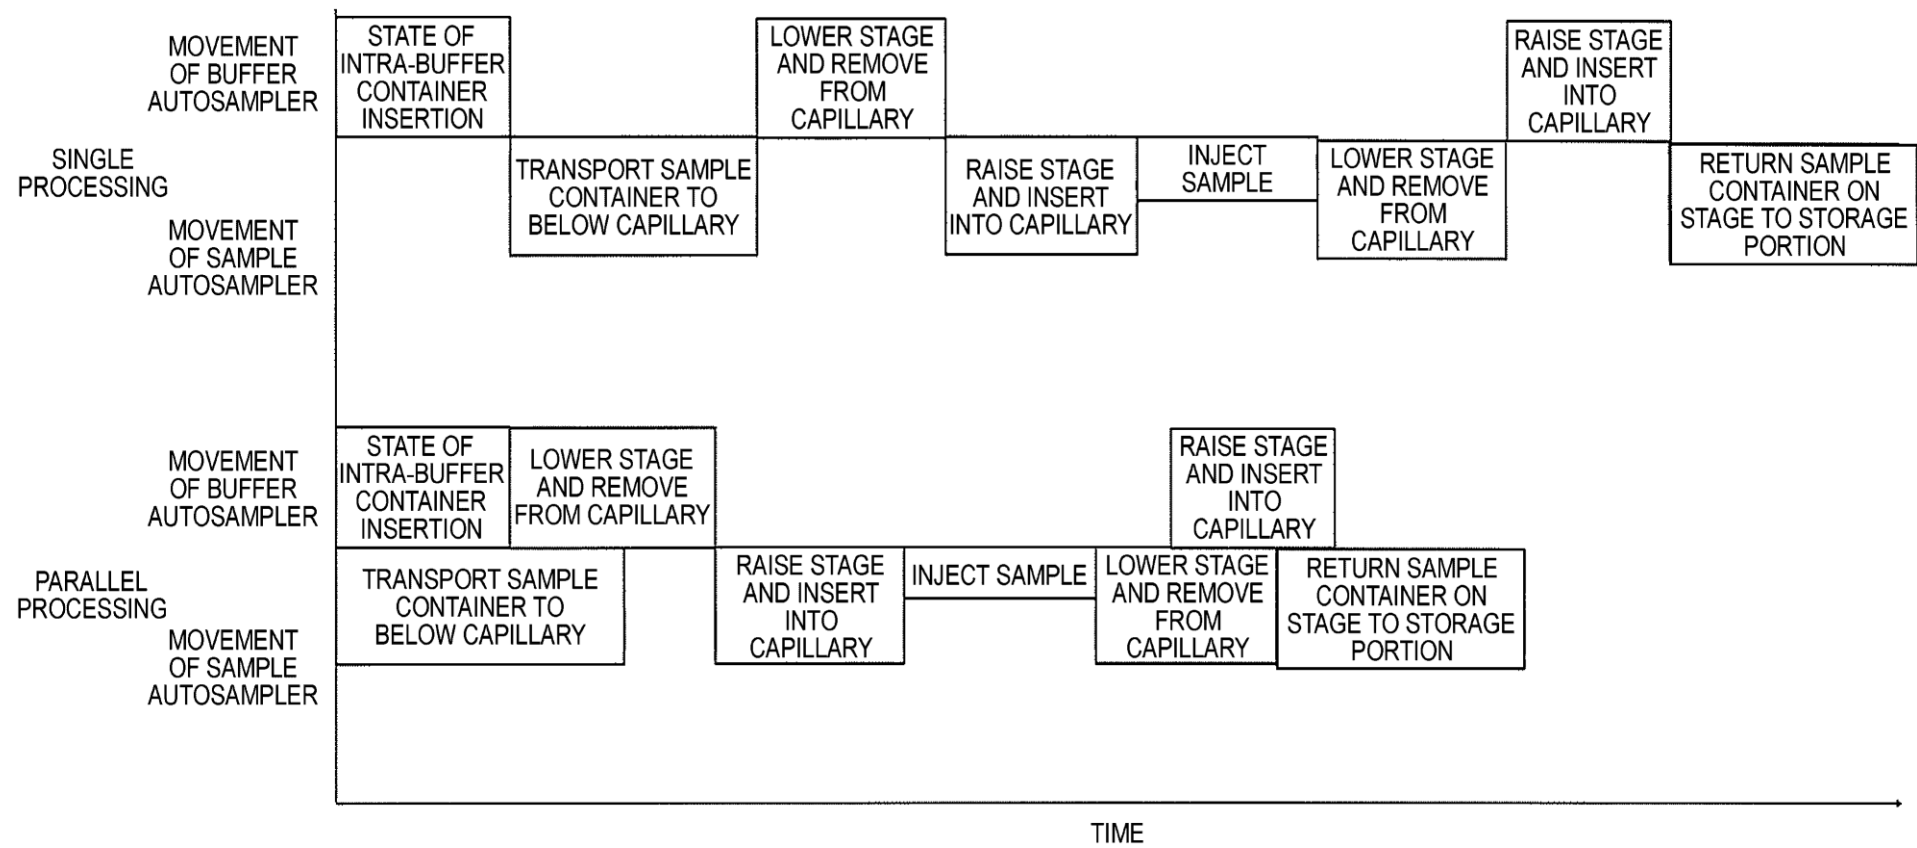FIG. 11

[FIG. 12]

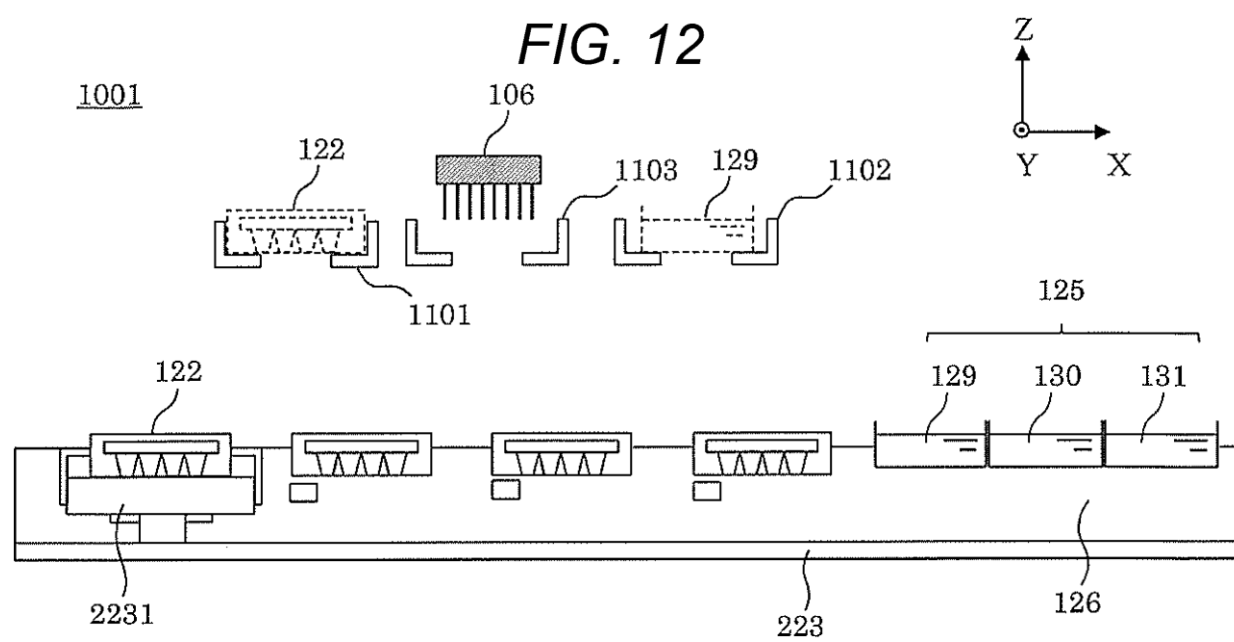

[FIG. 13]

FIG. 13