



(51) International Patent Classification:
G16H 70/40 (2018.01)

(21) International Application Number:
PCT/US2024/018615

(22) International Filing Date:
06 March 2024 (06.03.2024)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
63/489,060 08 March 2023 (08.03.2023) US

(71) Applicant: **EMD MILLIPORE CORPORATION**
[US/US]; 400 Summit Drive, Burlington, Massachusetts
01803 (US).

(72) Inventors: **AMARA, Ryan**; c/o EMD Millipore Corpo-
ration, 400 Summit Dr, Burlington, Massachusetts 01803
(US). **MILLER, Michael**; c/o EMD Millipore Corporation,
400 Summit Dr, Burlington, Massachusetts 01803 (US).

LOZEAU, Lindsay D.; c/o EMD Millipore Corporation,
400 Summit Dr, Burlington, Massachusetts 01803 (US).

(74) Agent: **WYNNEGAR, JR., James D.**; c/o EMD Millipore
Corporation, 400 Summit Drive, Burlington, Massachusetts
01803 (US).

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ,
CA, CH, CL, CN, CO, CR, CU, CV, CZ, DE, DJ, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IQ, IR, IS, IT, JM, JO, JP, KE, KG,
KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY,
MA, MD, MG, MK, MN, MU, MW, MX, MY, MZ, NA,
NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO,
RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, ST, SV, SY, TH,
TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, WS,
ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, CV,
GH, GM, KE, LR, LS, MW, MZ, NA, RW, SC, SD, SL, ST,

(54) Title: SYSTEM, METHOD, AND APPARATUS FOR LABELING AND TRACKING LABORATORY SAMPLES


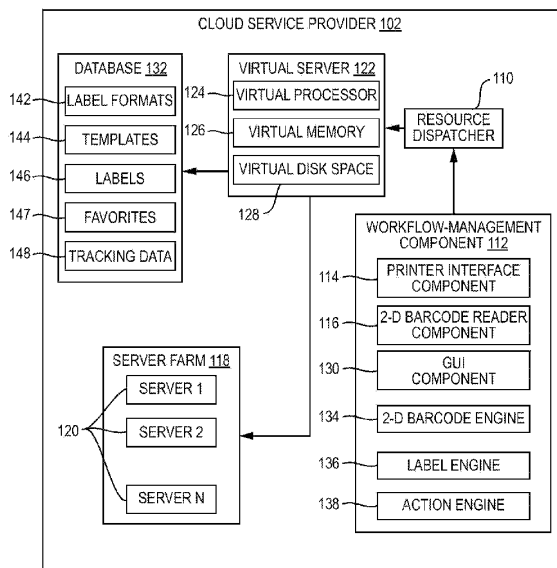


FIG. 1

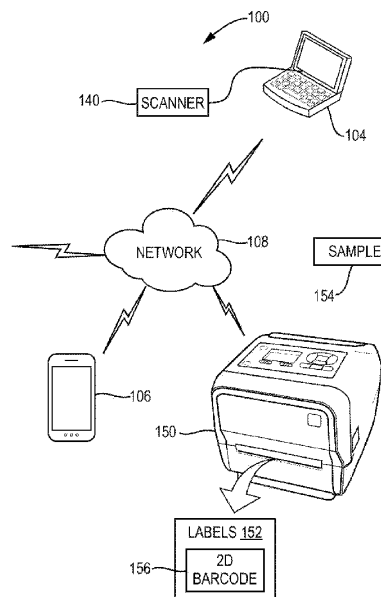

(57) Abstract: A device and related method for laboratory workflow handling is disclosed. The device may include one or more processors configured to provide a plurality of actions for selection by a user. A user can select an action of the plurality of actions and the device can determine an identification corresponding to a sample. The device can embed within a two-dimensional barcode the identification and workflow data corresponding to the sample and print a label with the two-dimensional barcode on an adhesive material using a printer.

[Continued on next page]

SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, ME, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- *as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))*

Published:

- *with international search report (Art. 21(3))*
- *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))*