


[図1]

HORIBA LA-920for Windows (TM) [WET (LA-920)] Ver. 3.37
LA-920 system for Windows

試料名 : Y-CPT (13615) R


メジアン径 : 10.5841 (μm)

ファイル名	:	比表面積	:	12307 (cm ² /cm ³)
循環速度	:	メジアン径	:	10.5841 (μm)
超音波	:	%積算径	:	(1) 5.000 (%) - 1.2084 (μm)
透過率 (L)	:		:	(2) 10.00 (%) - 1.9080 (μm)
透過率 (H)	:		:	(9) 90.00 (%) - 20.6688 (μm)
粒子径基準	:		:	(10) 95.00 (%) - 23.7018 (μm)
相対屈折率	:	積算径%	:	100.0 (μm) - 100.000 (%)
物質名	:		:	10.00 (μm) - 46.916 (%)
ロット番号	:	算術平均径	:	11.0017 (μm)
分散媒	:	算術分散	:	48.920 (μm ²)
	:	算術標準偏差	:	6.9943 (μm)
	:	モード径	:	13.9963 (μm)

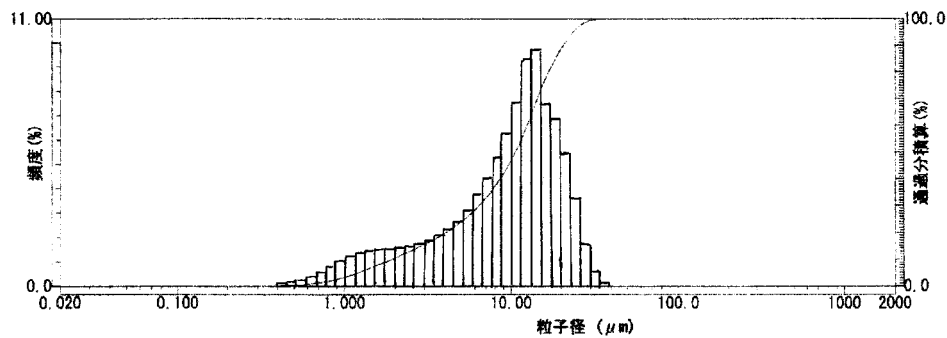


No.	粒子径 (μm)	頻度 (%)	積算 (%)	No.	粒子径 (μm)	頻度 (%)	積算 (%)	No.	粒子径 (μm)	頻度 (%)	積算 (%)
1	0.022	0.000	0.000	30	1.151	1.230	4.505	59	58.953	0.000	100.000
2	0.026	0.000	0.000	31	1.318	1.379	5.884	60	67.523	0.000	100.000
3	0.029	0.000	0.000	32	1.510	1.474	7.358	61	77.339	0.000	100.000
4	0.034	0.000	0.000	33	1.729	1.521	8.879	62	88.583	0.000	100.000
5	0.039	0.000	0.000	34	1.981	1.548	10.427	63	101.460	0.000	100.000
6	0.044	0.000	0.000	35	2.289	1.581	12.008	64	116.210	0.000	100.000
7	0.051	0.000	0.000	36	2.599	1.645	13.652	65	133.103	0.000	100.000
8	0.058	0.000	0.000	37	2.976	1.750	15.402	66	152.453	0.000	100.000
9	0.067	0.000	0.000	38	3.409	1.888	17.291	67	174.616	0.000	100.000
10	0.076	0.000	0.000	39	3.905	2.103	19.394	68	200.000	0.000	100.000
11	0.087	0.000	0.000	40	4.472	2.363	21.757	69	229.075	0.000	100.000
12	0.100	0.000	0.000	41	5.122	2.657	24.413	70	262.376	0.000	100.000
13	0.115	0.000	0.000	42	5.867	3.130	27.543	71	300.518	0.000	100.000
14	0.131	0.000	0.000	43	6.720	3.788	31.331	72	344.206	0.000	100.000
15	0.150	0.000	0.000	44	7.697	4.440	35.772	73	394.244	0.000	100.000
16	0.172	0.000	0.000	45	8.816	5.302	41.073	74	451.556	0.000	100.000
17	0.197	0.000	0.000	46	10.097	6.291	47.364	75	517.200	0.000	100.000
18	0.226	0.000	0.000	47	11.565	7.595	54.959	76	592.387	0.000	100.000
19	0.259	0.000	0.000	48	13.246	9.349	64.308	77	678.504	0.000	100.000
20	0.296	0.000	0.000	49	15.172	9.740	74.048	78	777.141	0.000	100.000
21	0.339	0.000	0.000	50	17.377	7.514	81.562	79	890.116	0.000	100.000
22	0.389	0.000	0.000	51	19.904	6.909	88.471	80	1019.515	0.000	100.000
23	0.445	0.108	0.108	52	22.797	5.500	93.971	81	1167.725	0.000	100.000
24	0.510	0.165	0.273	53	26.111	3.589	97.560	82	1337.481	0.000	100.000
25	0.584	0.258	0.531	54	29.907	1.721	99.281	83	1531.914	0.000	100.000
26	0.669	0.386	0.917	55	34.255	0.575	99.856	84	1754.613	0.000	100.000
27	0.766	0.553	1.470	56	39.234	0.144	100.000	85	2000.000	0.000	100.000
28	0.877	0.784	2.254	57	44.938	0.000	100.000				
29	1.005	1.021	3.275	58	51.471	0.000	100.000				


[図2]

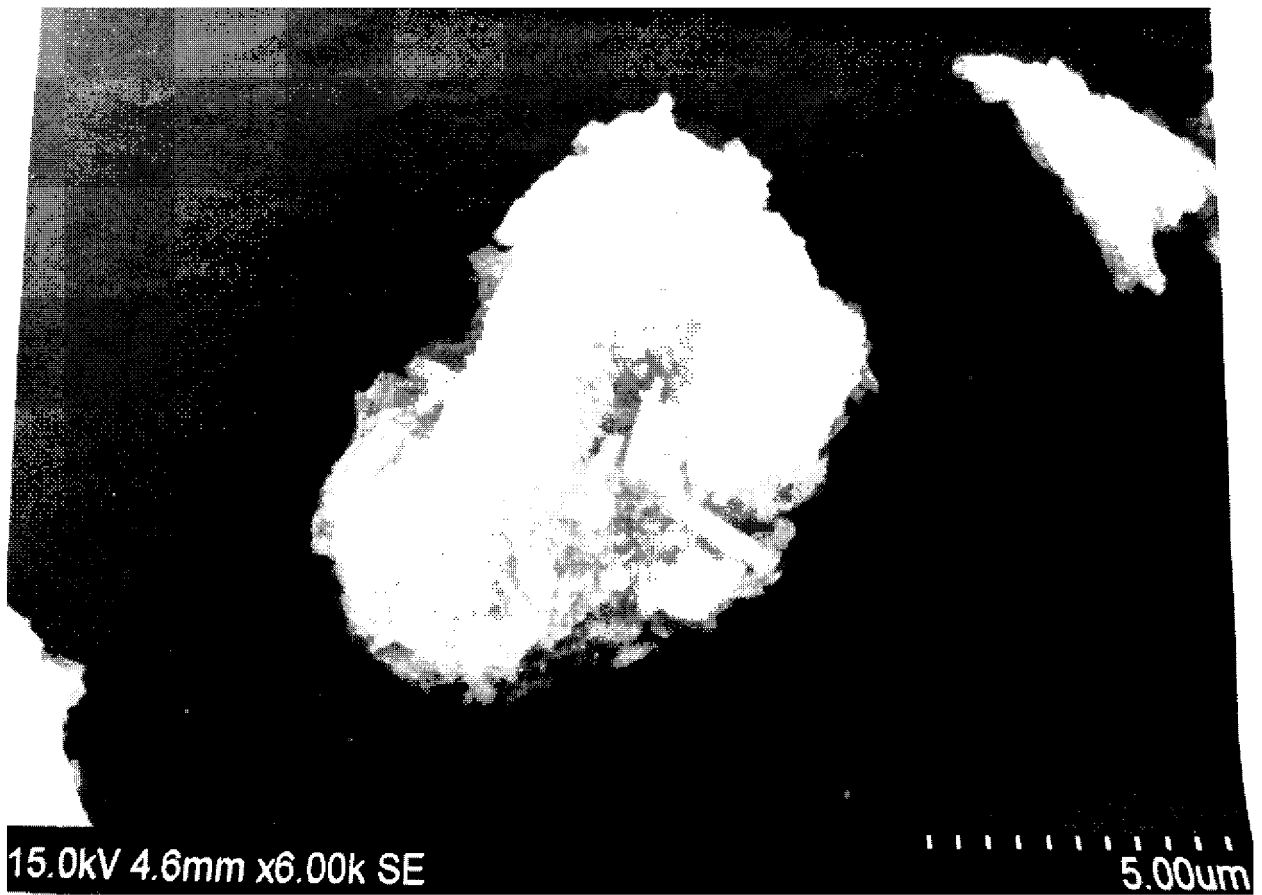


[図3]

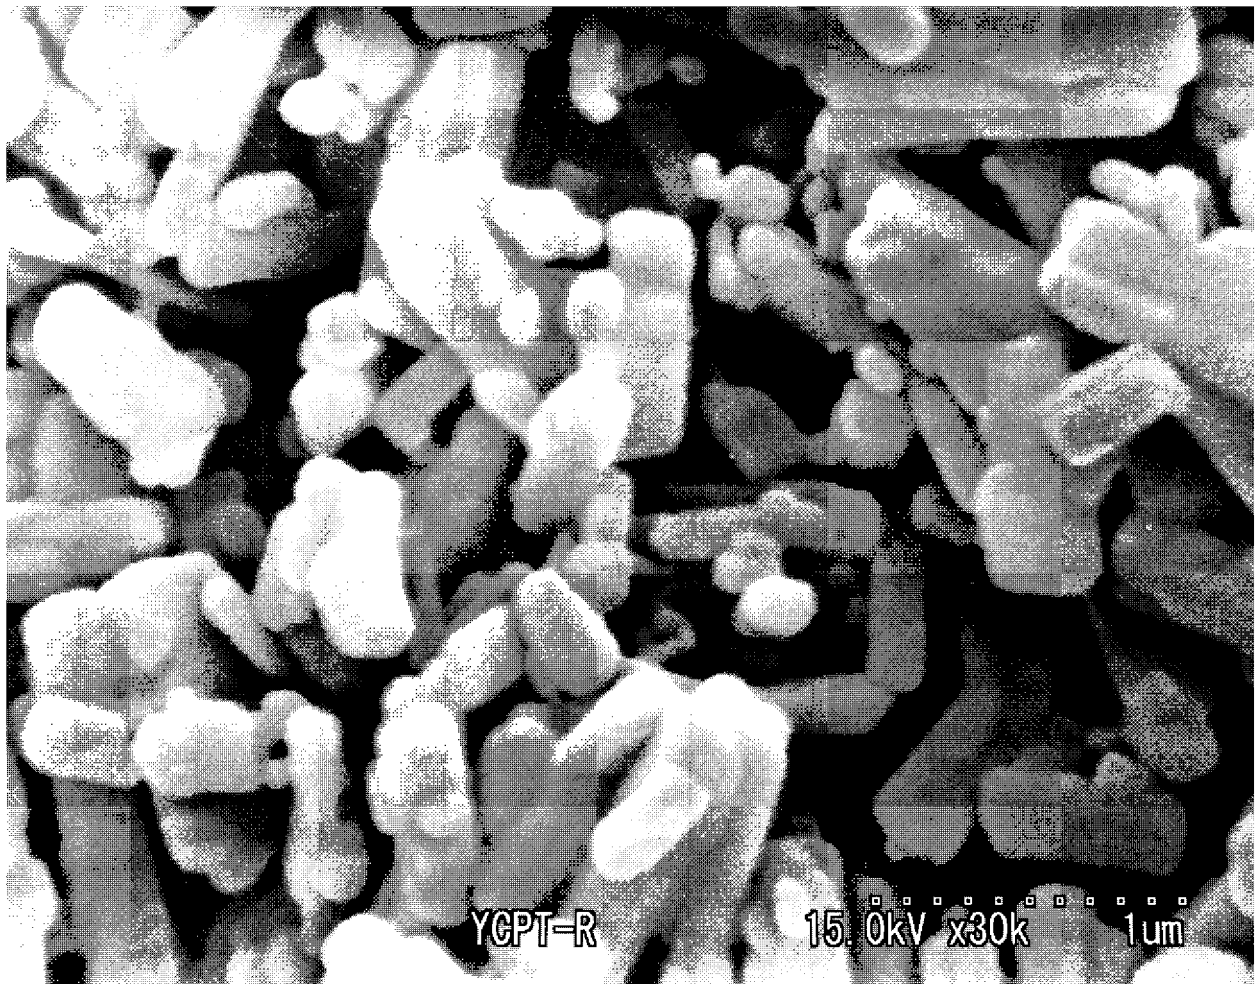

[図4]

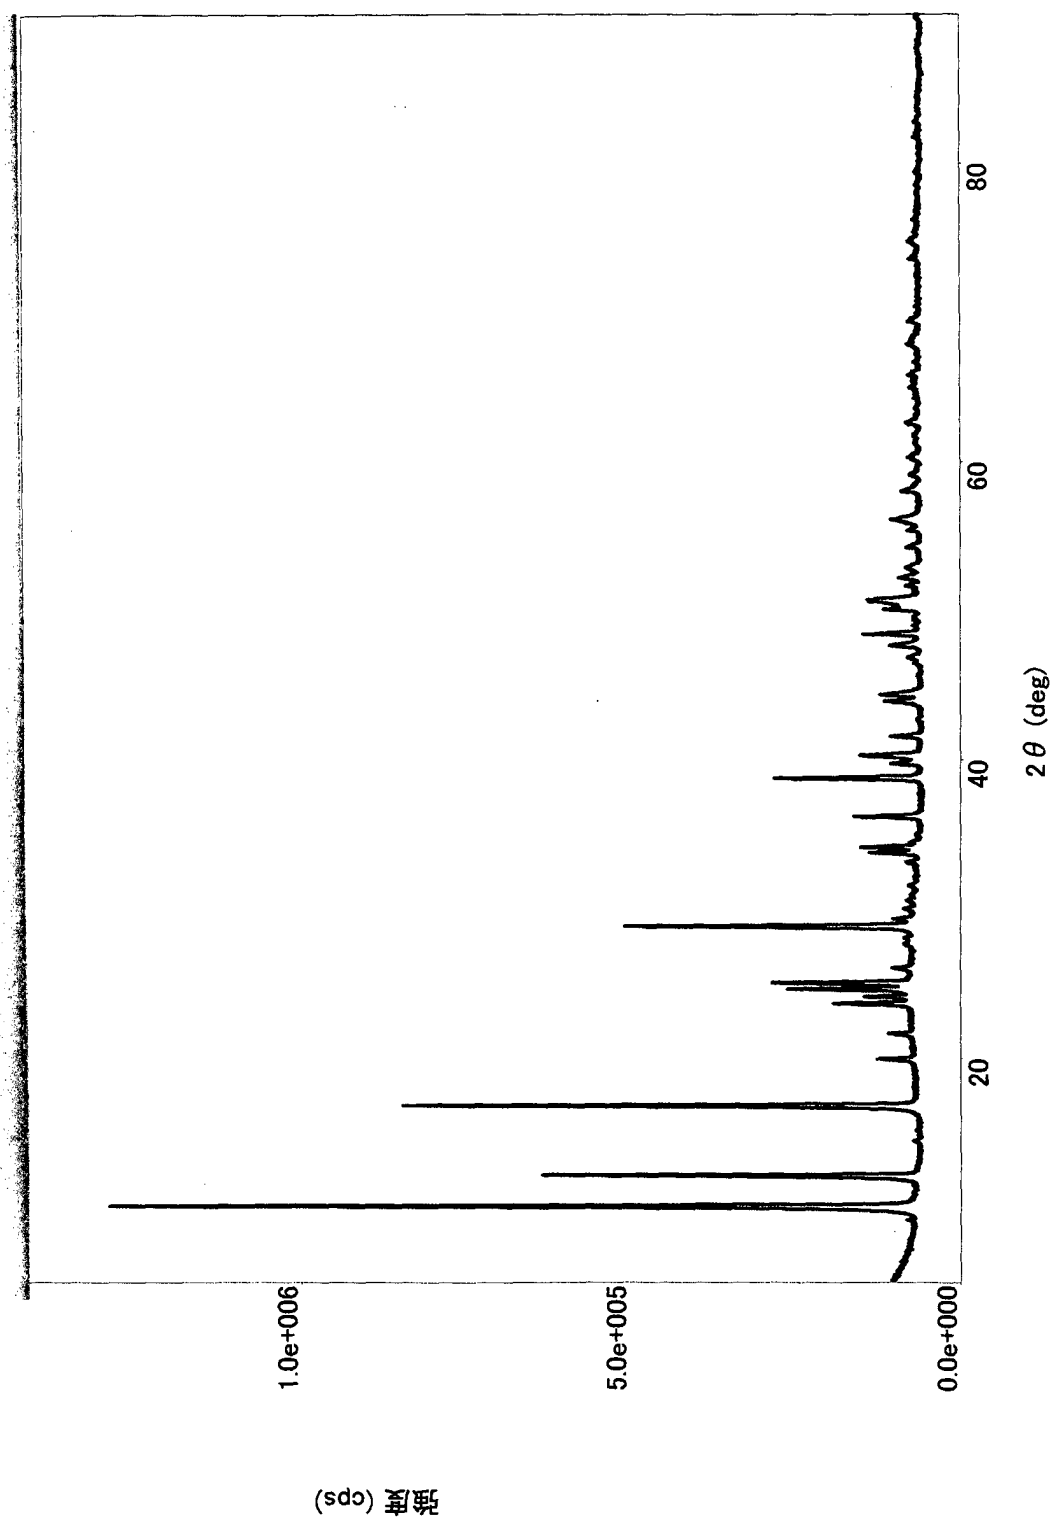

[図5]

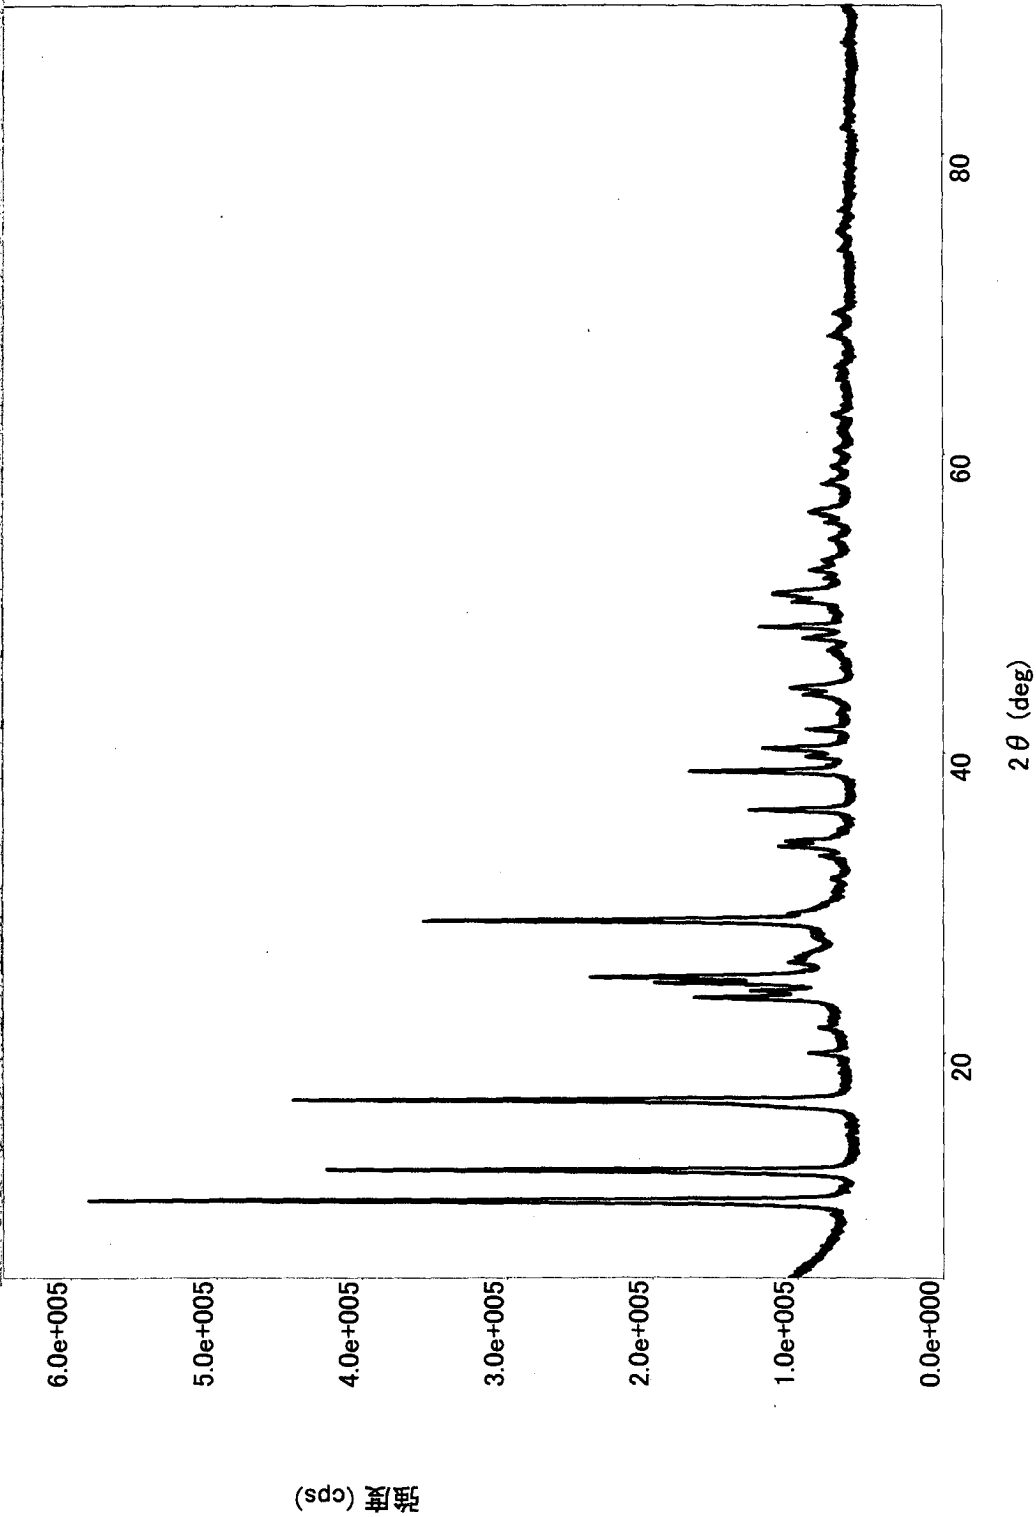


[図6]

HORIBA LA-920 for Windows(TM) [WET(LA-920)] Ver. 3.37
LA-920 system for Windows

試料名 : Y-CPT (13411)R

メジアン径 : 12.1168 (μm)

ファイル名	:	比表面積	:	19339 (cm ² /cm ³)
循環速度	:	メジアン径	:	12.1168 (μm)
超音波	:	%積算径	:	(1) 5.000 (%) - 0.5093 (μm)
透過率(L)	:		:	(2) 10.00 (%) - 1.2456 (μm)
透過率(H)	:		:	(9) 90.00 (%) - 27.7745 (μm)
粒子径基準	:		:	(10) 95.00 (%) - 32.6022 (μm)
相対屈折率	:	積算径%	:	100.0 (μm) - 100.000 (%)
物質名	:		:	10.00 (μm) - 41.188 (%)
ロット番号	:	算術平均径	:	13.7196 (μm)
分散媒	:	算術分散	:	98.661 (μm ²)
	:	算術標準偏差	:	9.9328 (μm)
	:	モード径	:	14.1769 (μm)

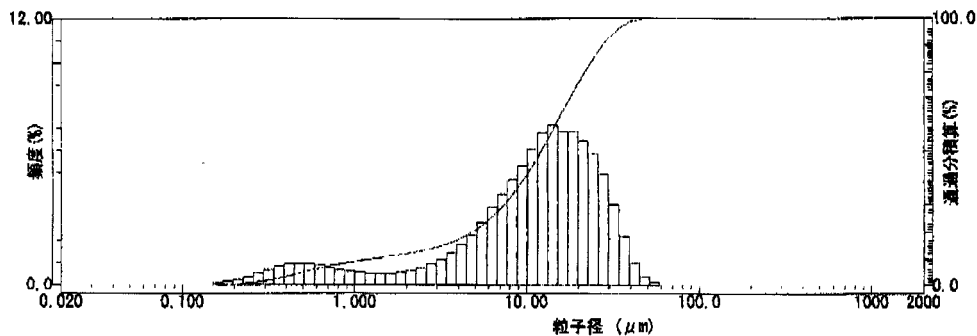

No.	粒子径 (μm)	頻度 (%)	積算 (%)	No.	粒子径 (μm)	頻度 (%)	積算 (%)	No.	粒子径 (μm)	頻度 (%)	積算 (%)
1	0.022	0.000	0.000	30	1.151	0.581	9.677	59	58.953	0.113	100.000
2	0.026	0.000	0.000	31	1.318	0.555	10.232	60	67.523	0.000	100.000
3	0.029	0.000	0.000	32	1.510	0.544	10.775	61	77.339	0.000	100.000
4	0.034	0.000	0.000	33	1.729	0.558	11.333	62	88.583	0.000	100.000
5	0.039	0.000	0.000	34	1.981	0.600	11.933	63	101.480	0.000	100.000
6	0.044	0.000	0.000	35	2.269	0.676	12.609	64	116.210	0.000	100.000
7	0.051	0.000	0.000	36	2.599	0.792	13.401	65	133.103	0.000	100.000
8	0.058	0.000	0.000	37	2.976	0.957	14.358	66	152.453	0.000	100.000
9	0.067	0.000	0.000	38	3.409	1.176	15.534	67	174.616	0.000	100.000
10	0.076	0.000	0.000	39	3.905	1.470	17.003	68	200.000	0.000	100.000
11	0.087	0.000	0.000	40	4.472	1.831	18.834	69	229.075	0.000	100.000
12	0.100	0.000	0.000	41	5.122	2.254	21.088	70	262.378	0.000	100.000
13	0.115	0.000	0.000	42	5.867	2.850	23.938	71	300.518	0.000	100.000
14	0.131	0.000	0.000	43	6.720	3.493	27.431	72	344.206	0.000	100.000
15	0.150	0.000	0.000	44	7.697	4.084	31.515	73	394.244	0.000	100.000
16	0.172	0.104	0.104	45	8.818	4.893	36.208	74	451.556	0.000	100.000
17	0.197	0.167	0.271	46	10.097	5.362	41.570	75	517.200	0.000	100.000
18	0.226	0.262	0.533	47	11.585	6.078	47.647	76	592.387	0.000	100.000
19	0.259	0.377	0.910	48	13.246	6.851	54.498	77	678.504	0.000	100.000
20	0.296	0.548	1.458	49	15.172	7.162	61.660	78	777.141	0.000	100.000
21	0.339	0.705	2.162	50	17.377	8.855	68.515	79	890.116	0.000	100.000
22	0.389	0.863	3.025	51	19.904	6.875	75.390	80	1019.515	0.000	100.000
23	0.445	0.972	3.998	52	22.797	6.479	81.869	81	1167.725	0.000	100.000
24	0.510	1.009	5.007	53	26.111	5.882	87.751	82	1337.481	0.000	100.000
25	0.584	1.012	6.019	54	29.907	4.942	92.693	83	1531.914	0.000	100.000
26	0.669	0.920	6.939	55	34.255	3.628	96.322	84	1754.613	0.000	100.000
27	0.766	0.804	7.743	56	39.234	2.187	98.509	85	2000.000	0.000	100.000
28	0.877	0.710	8.453	57	44.938	1.003	99.512				
29	1.005	0.643	9.095	58	51.471	0.375	99.887				