



- (51) International Patent Classification:
H04W 4/33 (2018.01) *G16H 50/20* (2018.01)
- (21) International Application Number:
PCT/US2023/012173
- (22) International Filing Date:
02 February 2023 (02.02.2023)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
63/306,279 03 February 2022 (03.02.2022) US
63/426,450 18 November 2022 (18.11.2022) US
63/428,074 27 November 2022 (27.11.2022) US
- (71) Applicant: **STRYKER CORPORATION** [US/US]; 2825
Airview Boulevard, Kalamazoo, Michigan 49002 (US).
- (72) Inventors: **THOTA, Madhu Sandeep**; 7375 Salerno
Circle, Portage, Michigan 49024 (US). **PAUL, Anish**;
7168 Bertland Drive, Portage, Michigan 49024 (US).
CHILDS, William Dwight; 11812 Lakeway Street, Plain-
well, Michigan 49080 (US). **BHIMAVARAPU, Krish-
na Sandeep**; 7068 Annandale Drive, Kalamazoo, Michi-
gan 49009 (US). **NEIHOUSER, Kirby M.**; 3007 French
Bay Drive, Portage, Michigan 49024 (US). **PEREIRA,
Celso Henrique Farnese Pires**; 1349 Auburn Woods
Trail, Portage, Michigan 49002 (US). **THOMAS, Mad-
hu**; 3206 Pomeroy Lane, London, Ontario N6P 1V7 (CA).
TREPANIER, Jerald A.; 7606 N. 46th Street, Augusta,
Michigan 49012 (US). **OTHMAN, Ramsey H.**; 7795 Ken-
mure Drive, Portage, Michigan 49024 (US).
- (74) Agent: **GOSKA, Matthew L.** et al.; WARNER NOR-
CROSS + JUDD LLP, 150 Ottawa Ave. NW, Ste. 1500,
Grand Rapids, Michigan 49503 (US).

(54) Title: COMMUNICATION SYSTEM FOR PATIENT SUPPORT APPARATUSES

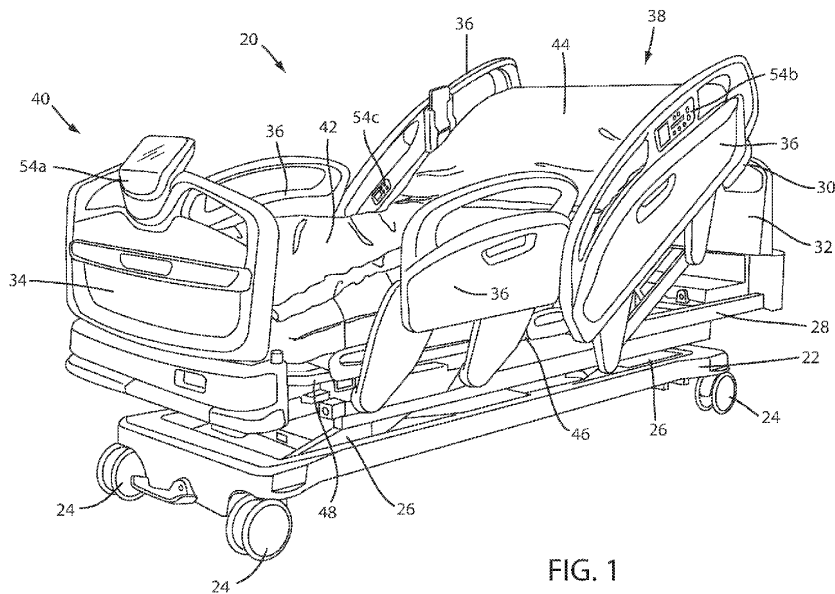


FIG. 1

(57) Abstract: A patient support apparatus for supporting a patient includes first, second, and third transceivers mounted at first, second, and third locations, respectively. A controller is adapted to use radio frequency communication between the first, second, and third transceivers and a first device—such as a display device, a fixed locator, and/or a vital sign sensor—to determine a position of the first device relative to the patient support apparatus. The controller is further adapted to send data to a display device if the first device is positioned inside a predetermined volume of space, and to not send the data to the display device if the first device is positioned outside of the predetermined volume of space. The patient support apparatus may also selectively accept and communicate with a removable cartridge that includes a vital sign port adapted to receive a plug of a cable from a vital sign sensor.

[Continued on next page]

(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CV, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IQ, IR, IS, IT, JM, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, WS, ZA, ZM, ZW.

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, CV, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, ME, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— *without international search report and to be republished upon receipt of that report (Rule 48.2(g))*