Figure-1: Comparative level of intensity of test lines recorded in HEV IgA POCT and HEV IgM rapid test.

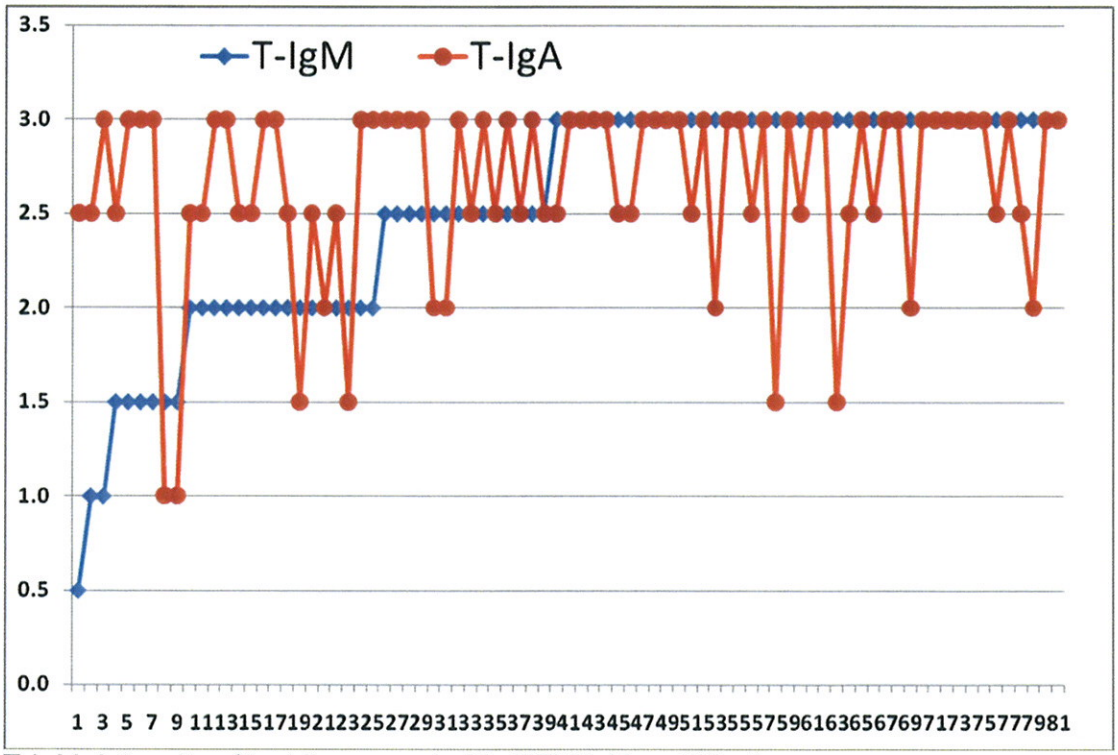

T-IgM: Intensity of test line recorded in HEV IgM rapid test
T-IgA: Intensity of test line recorded in HEV IgA POCT

Figure-2: Schematic diagram of HEV-IgA POCT device

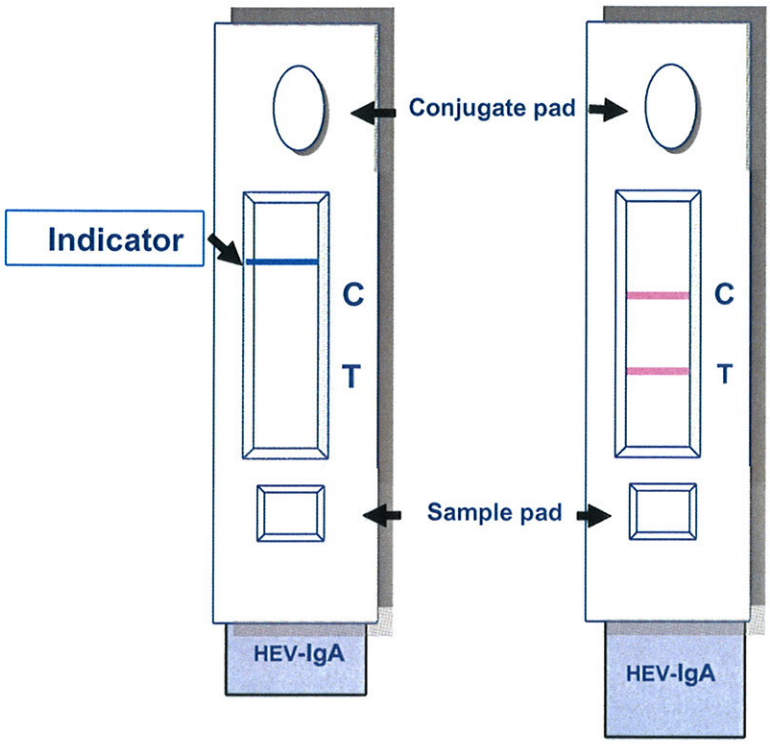

Reverse Flow Rapid Test