

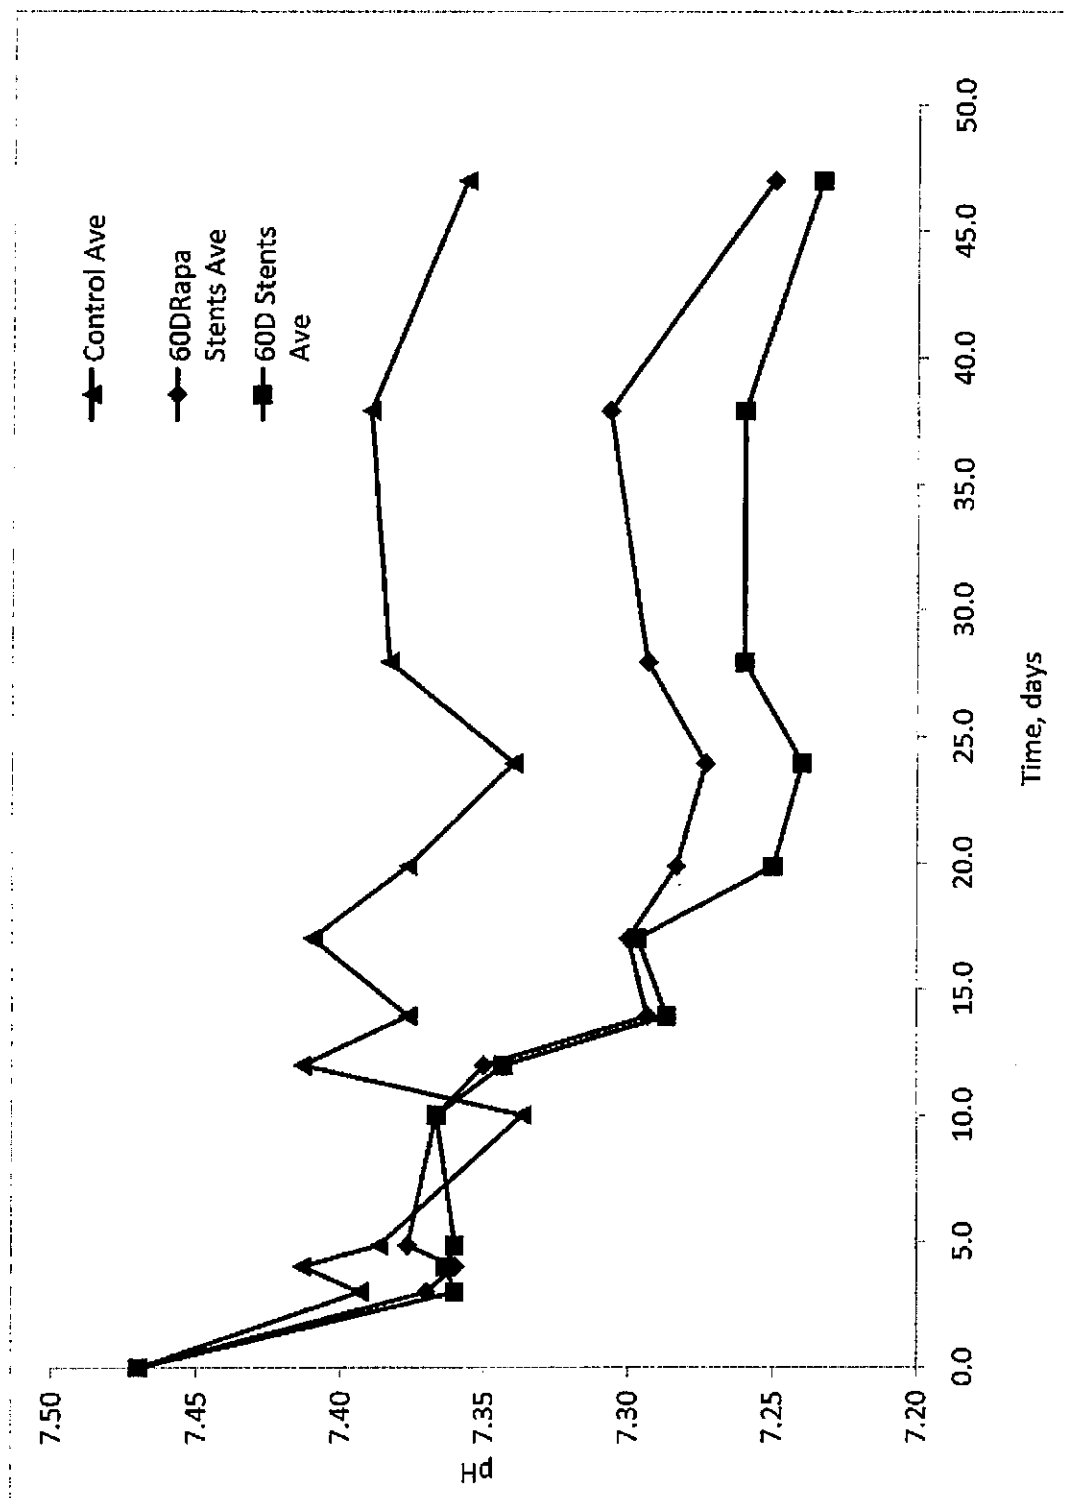
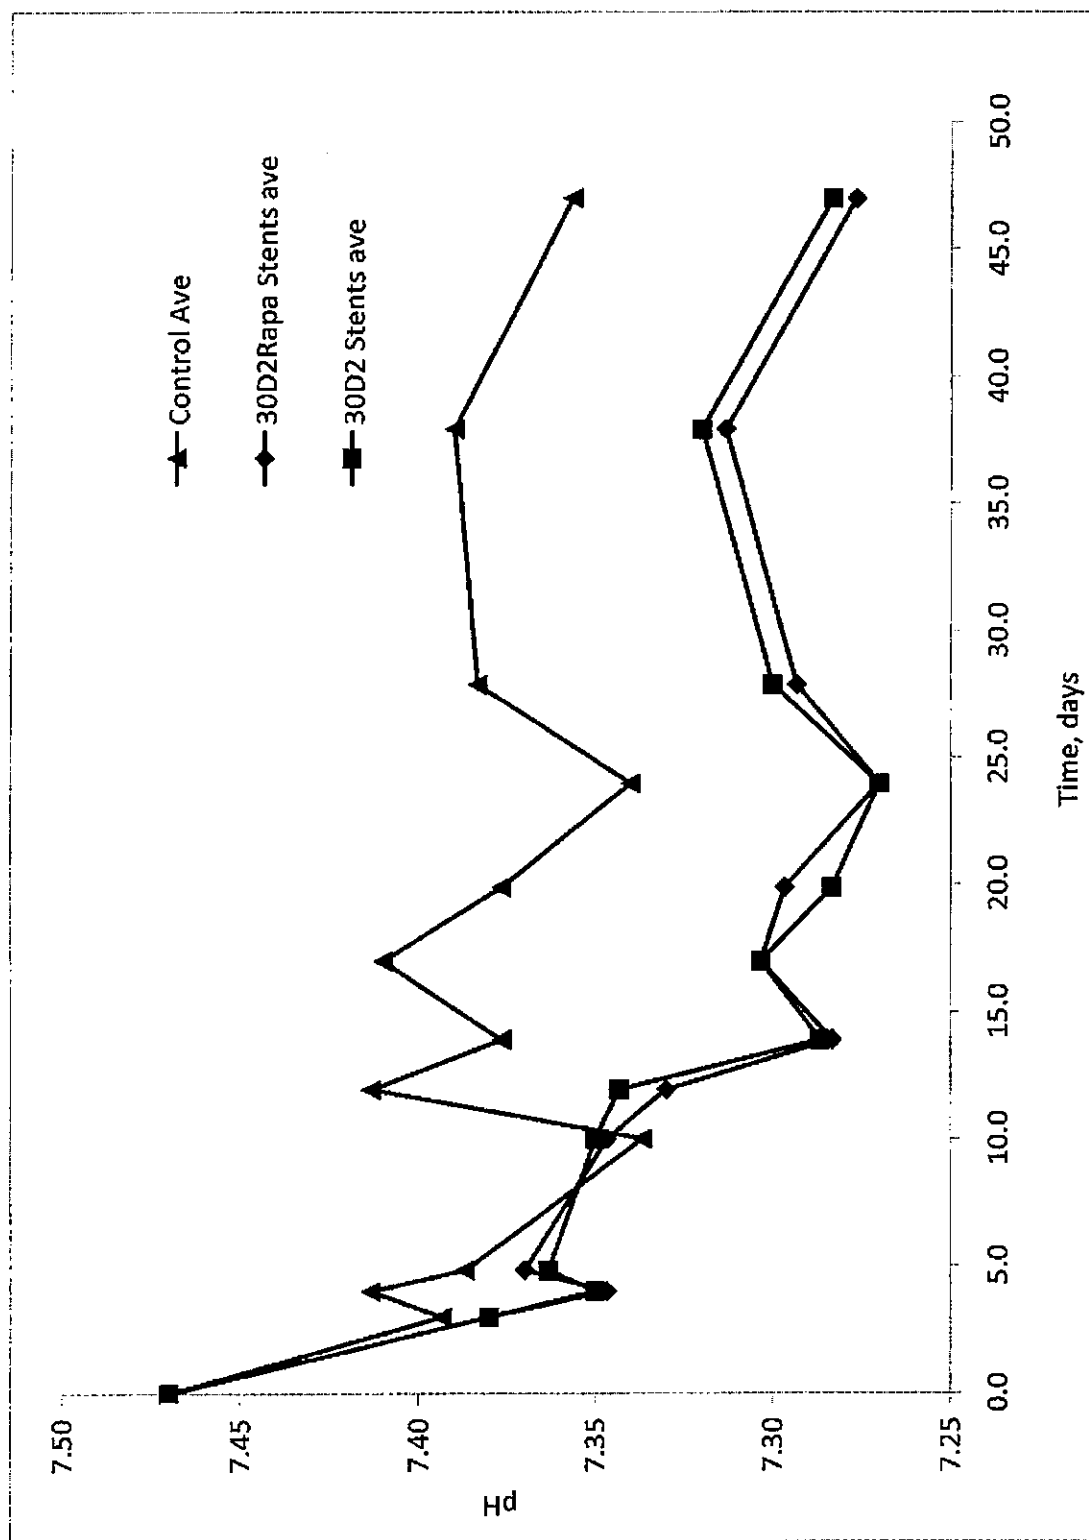


Figure 1

Figure 2



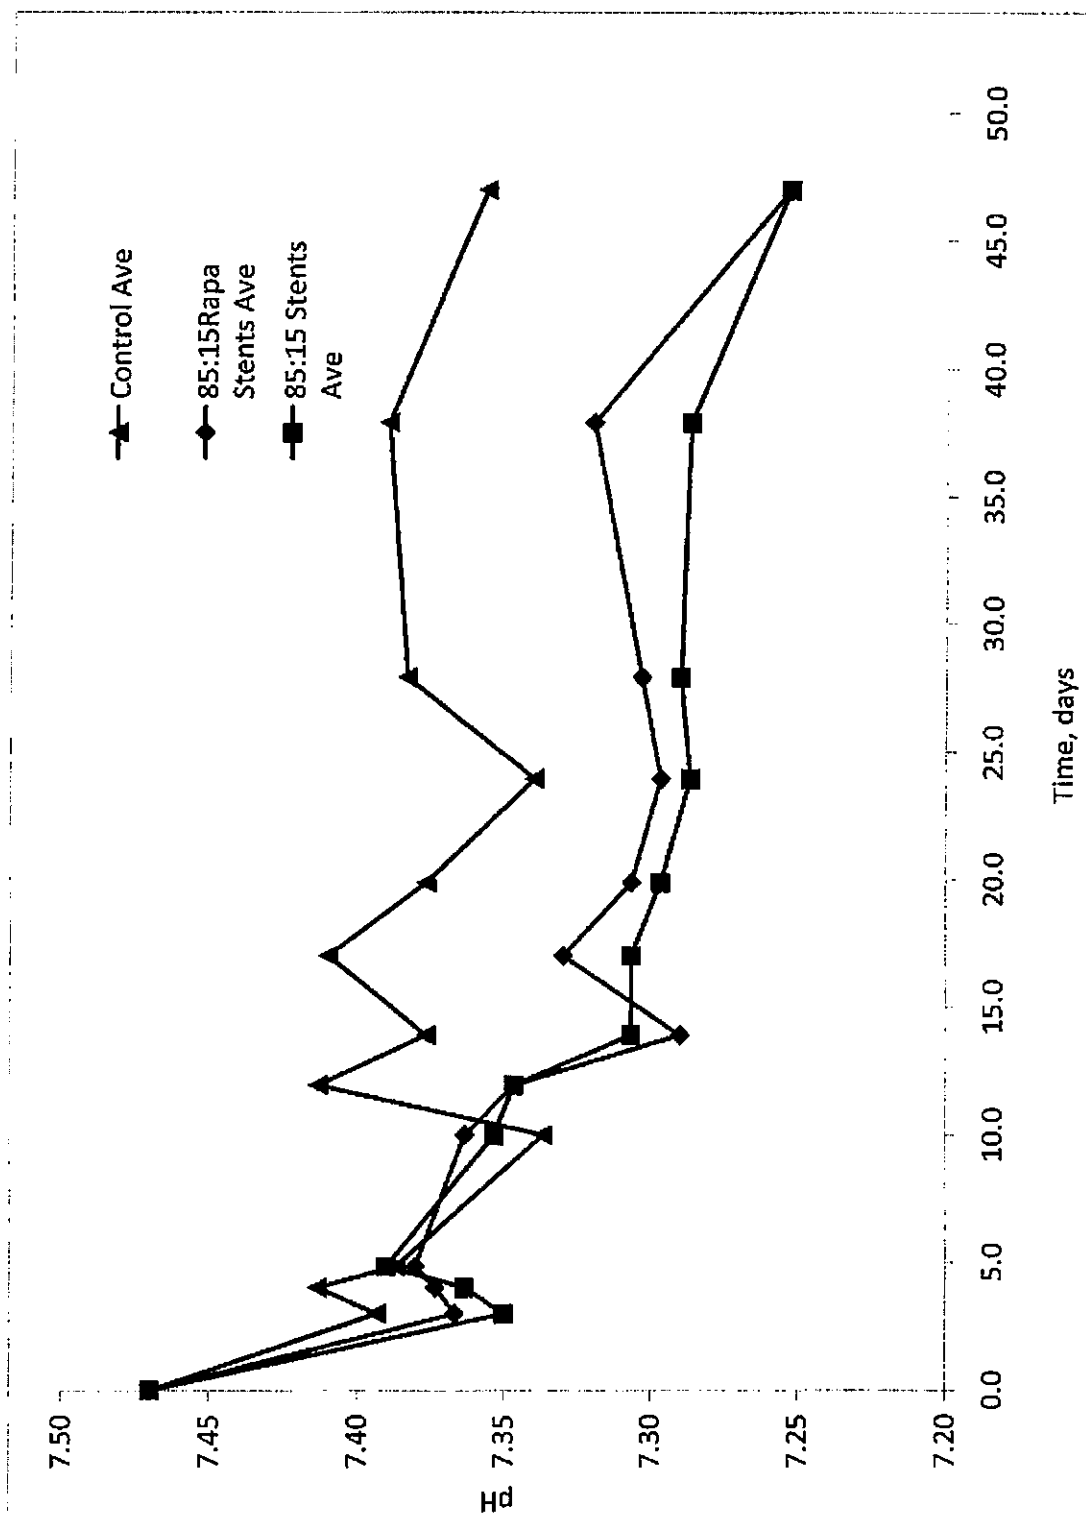


Figure 3

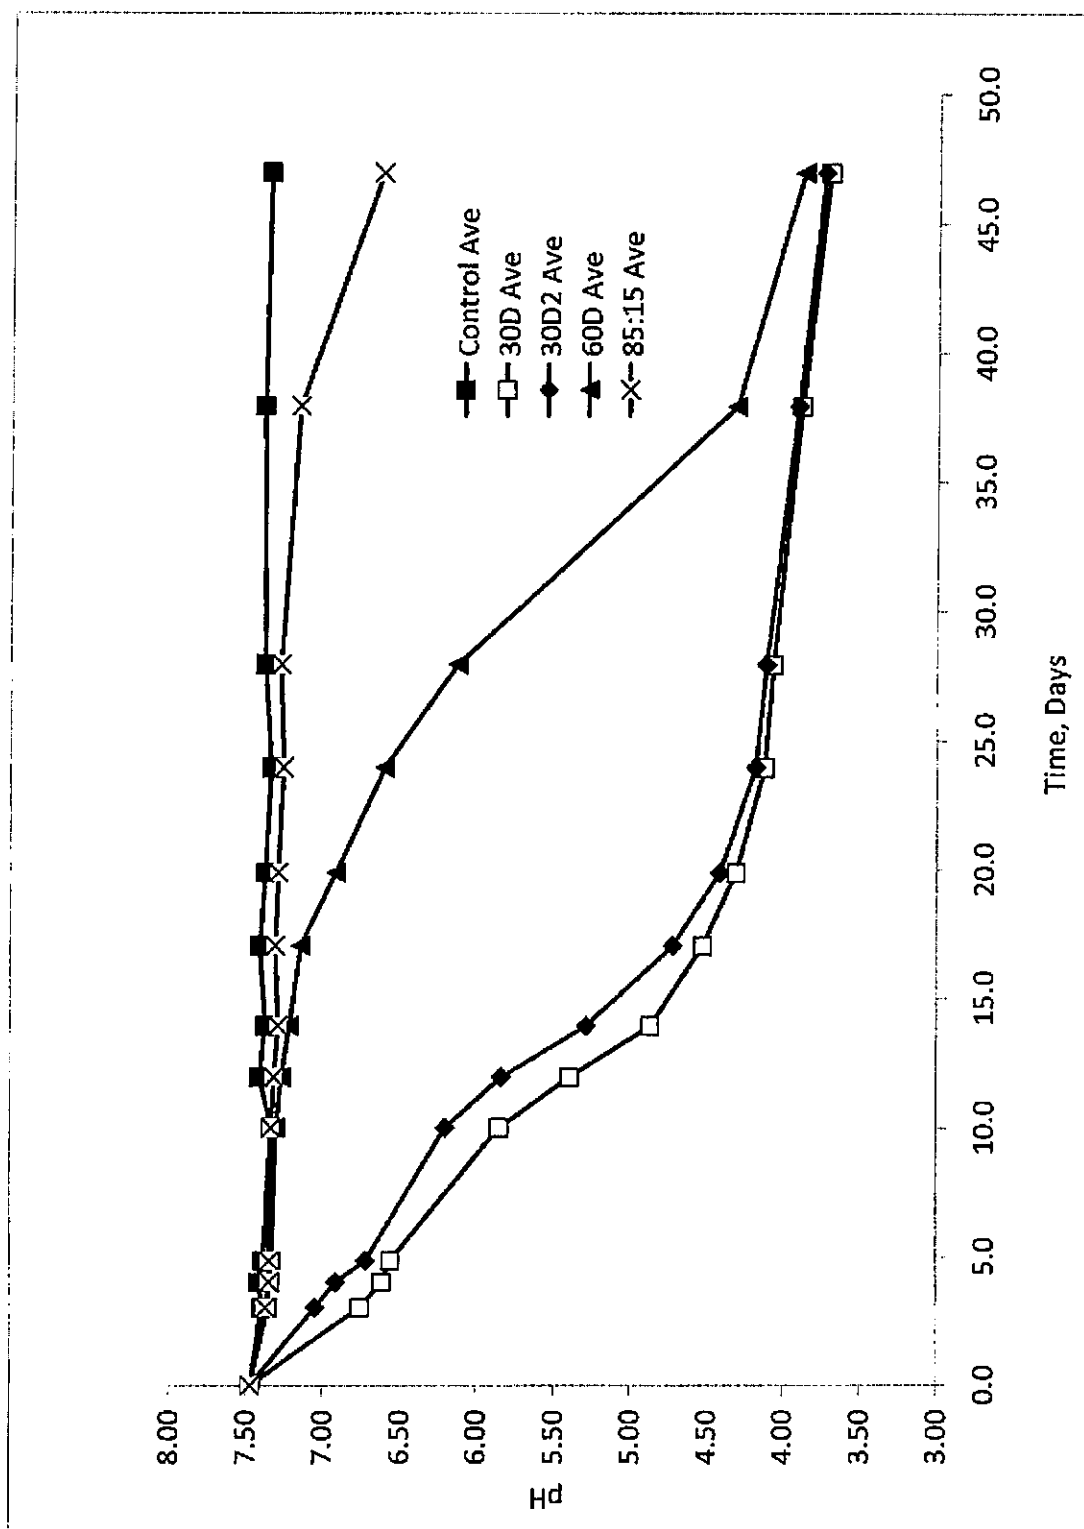


Figure 4:

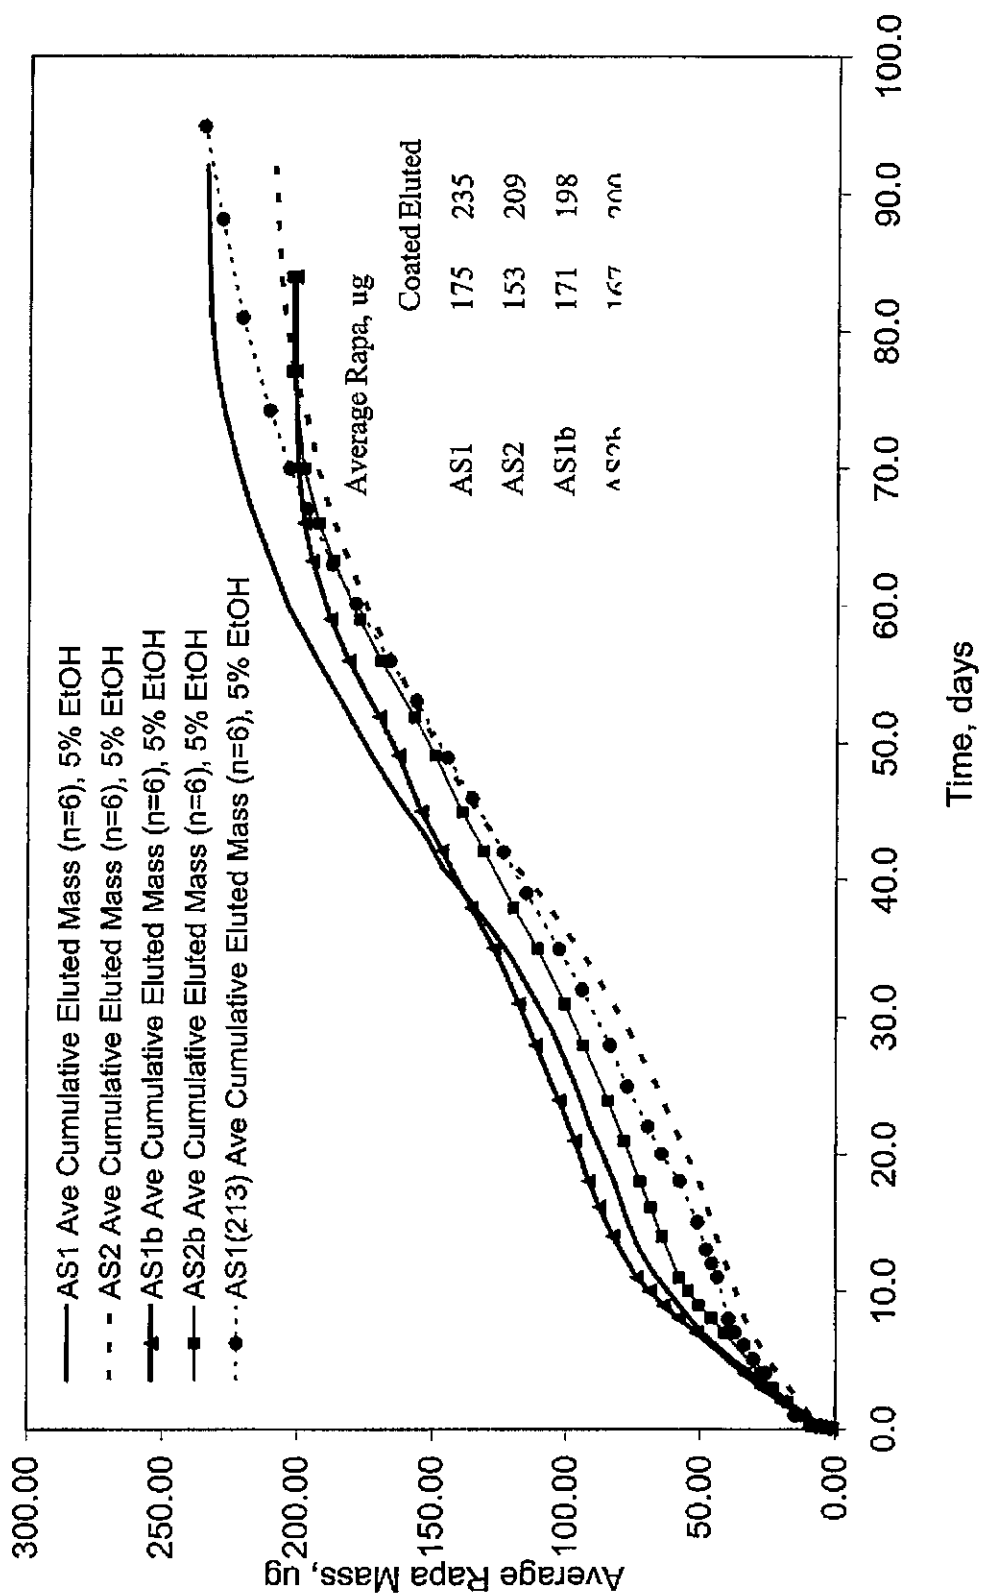
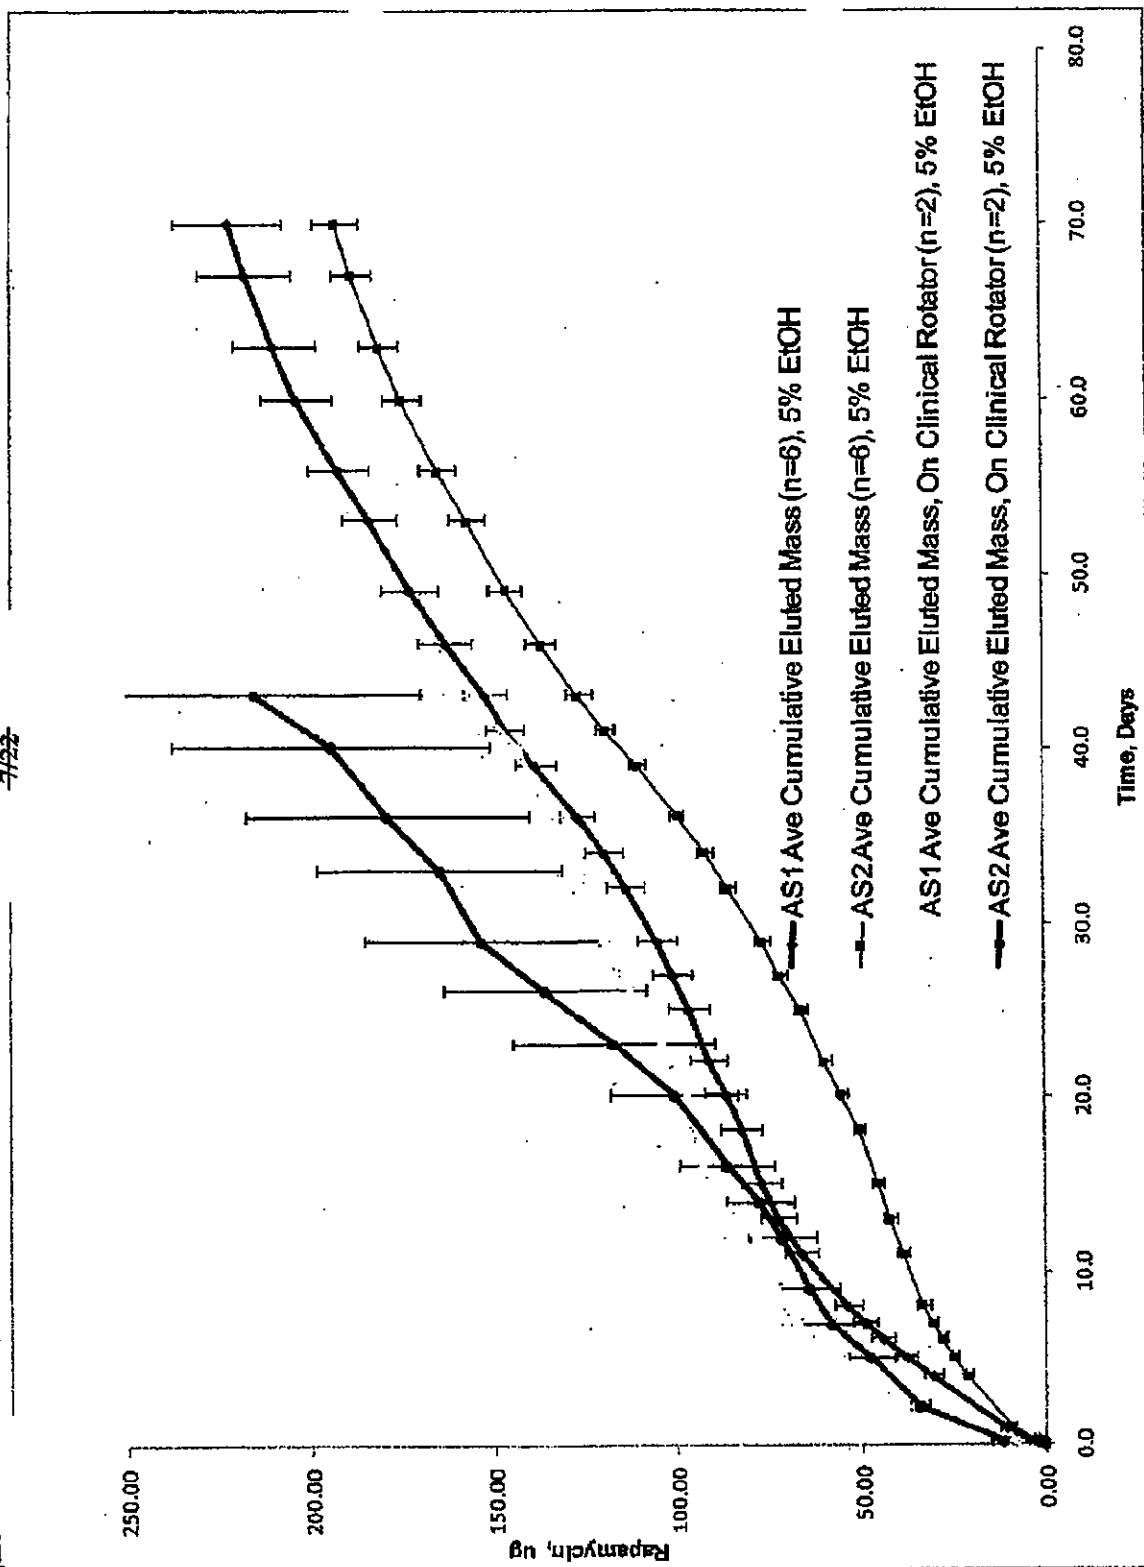


Figure 5:

7/22

Figure 7

7/22




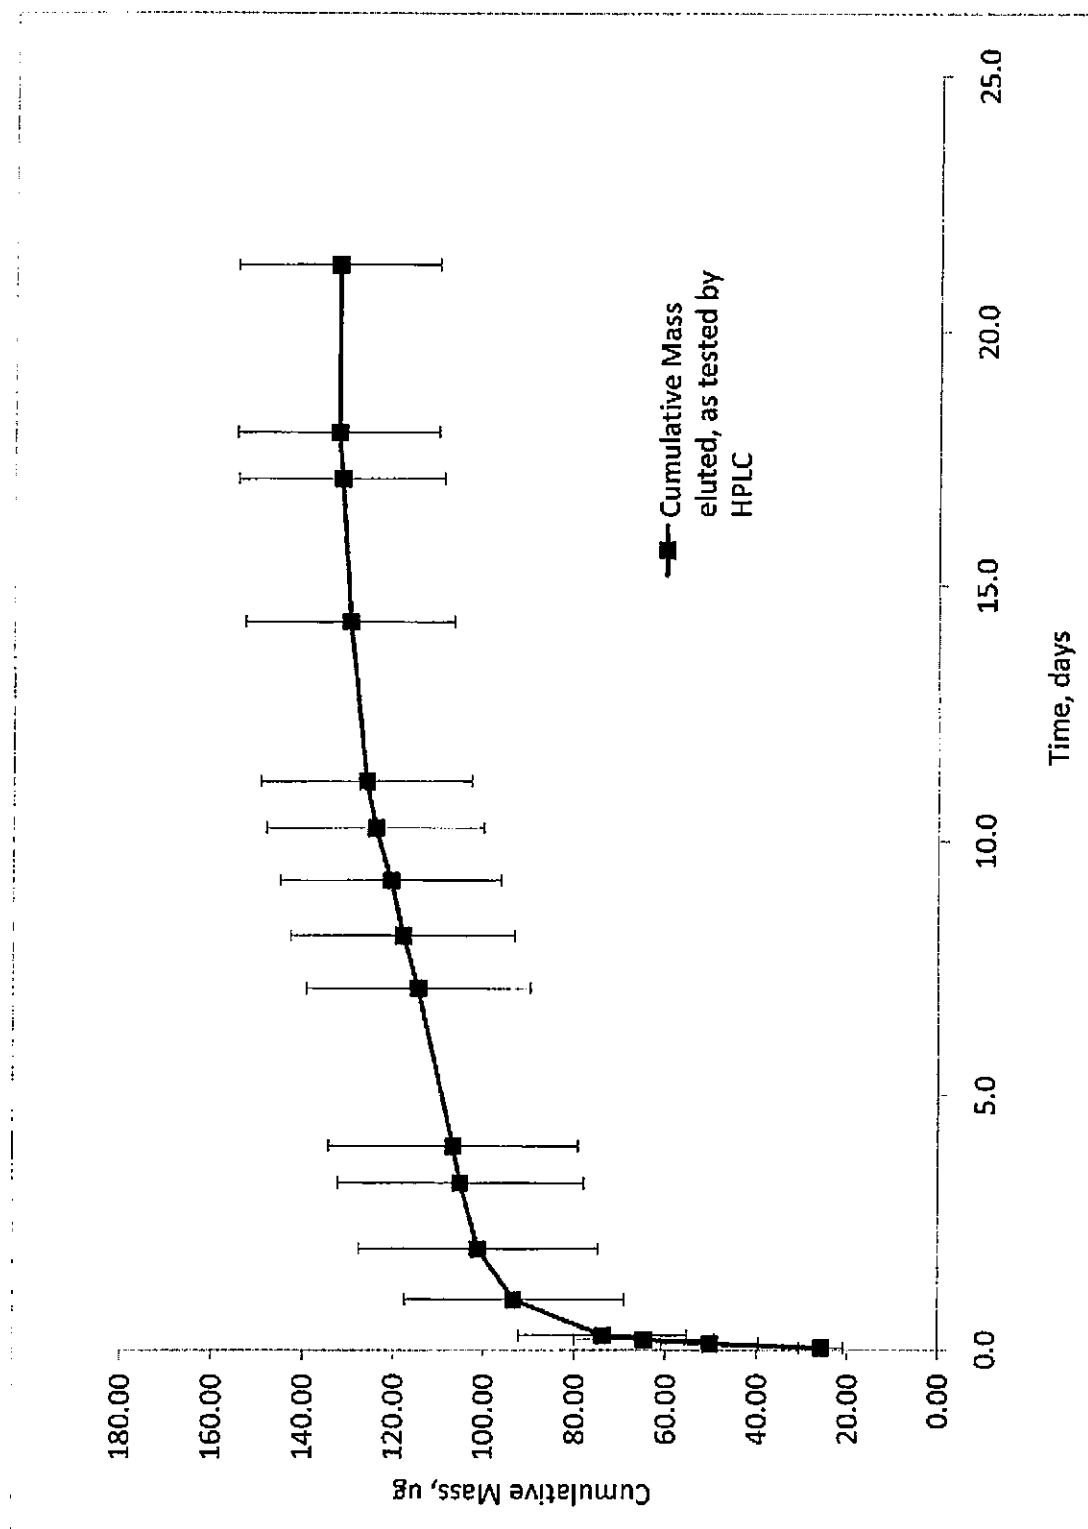


Figure 9:

10/22

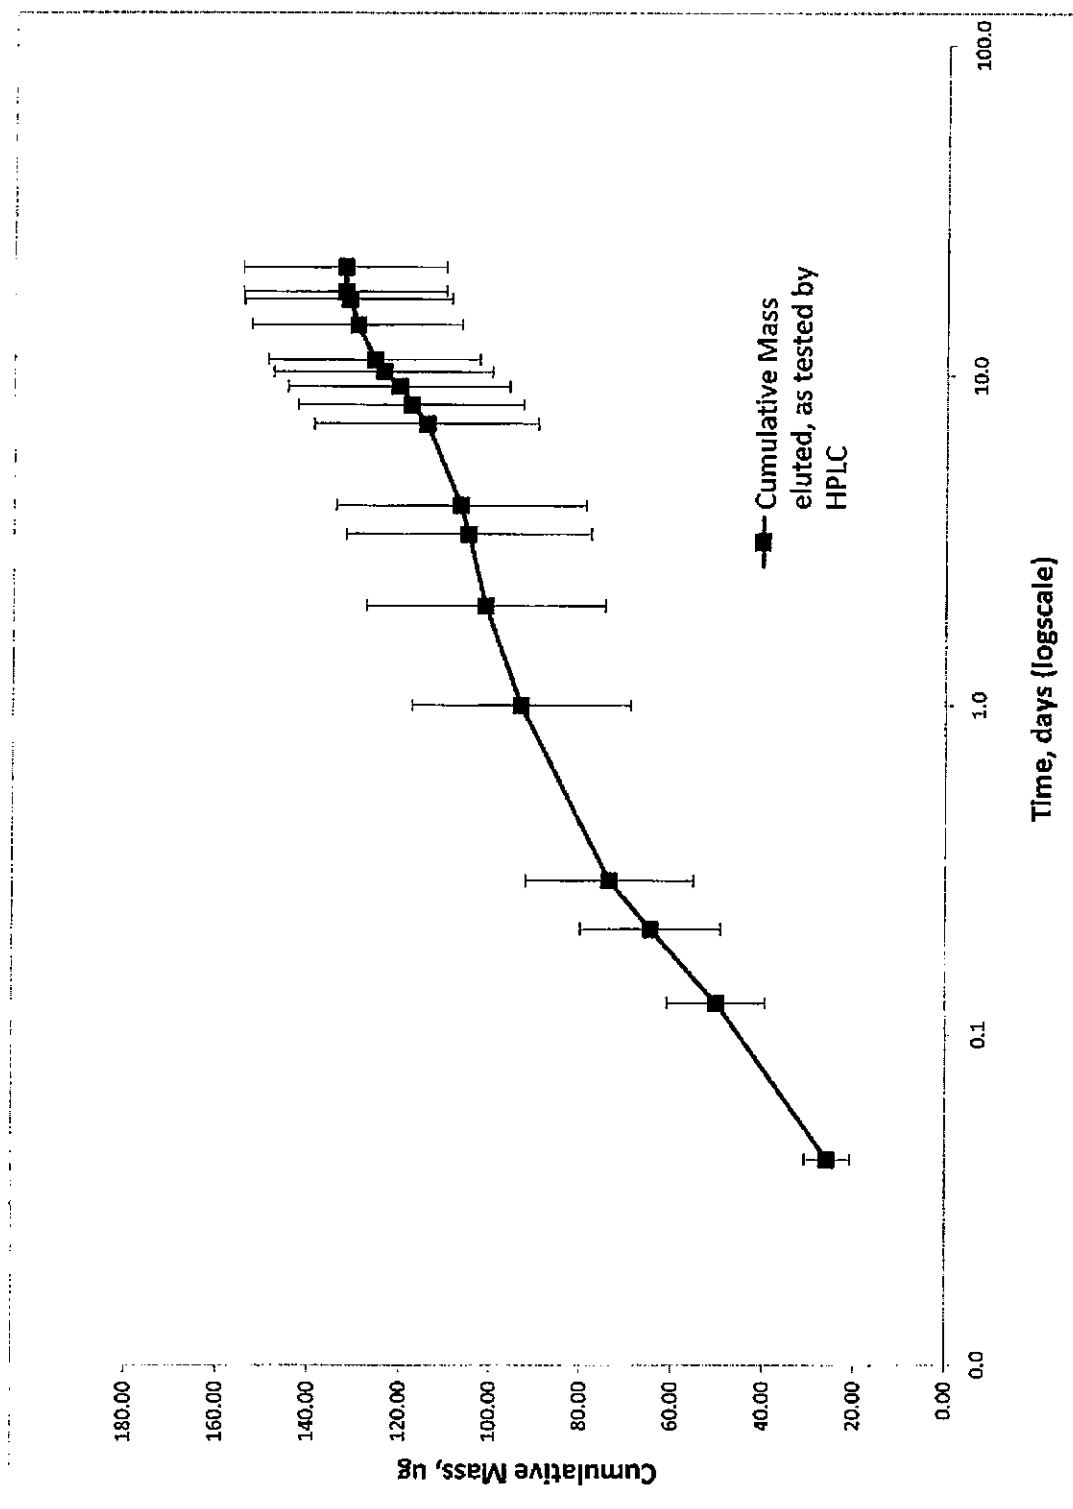


10

Figure 10:

11/22

Figure 11:

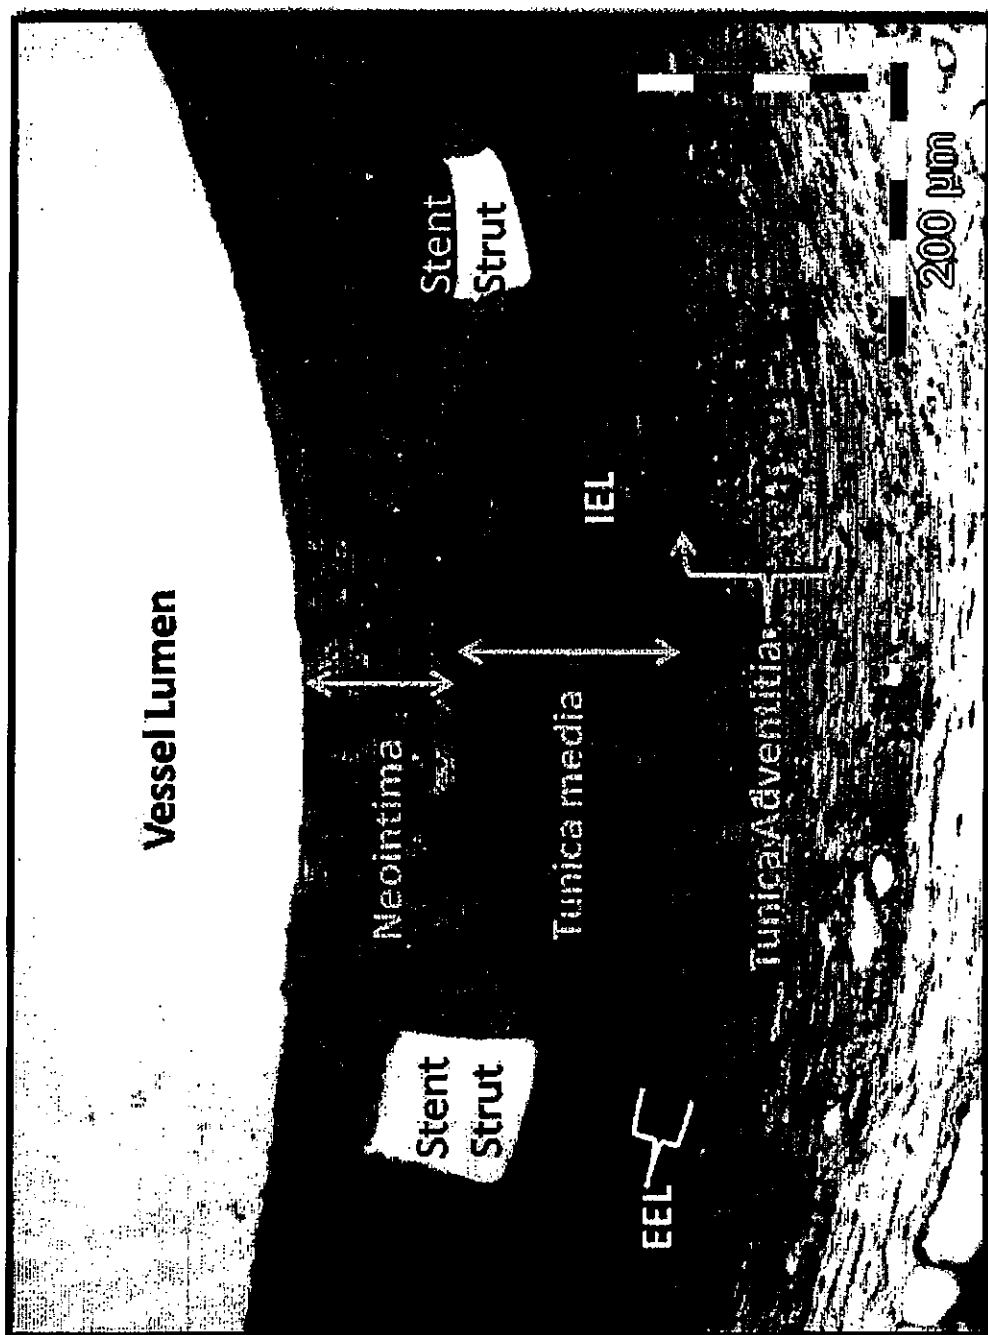

11

Figure 12

AS1



AS2



AS3 (BMS Control)



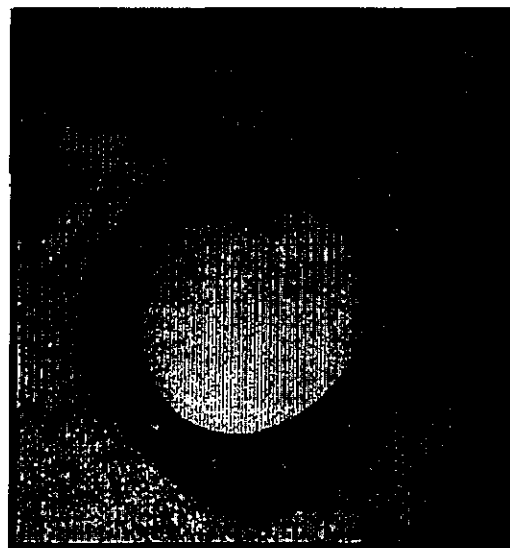


Figure 13:

AS1

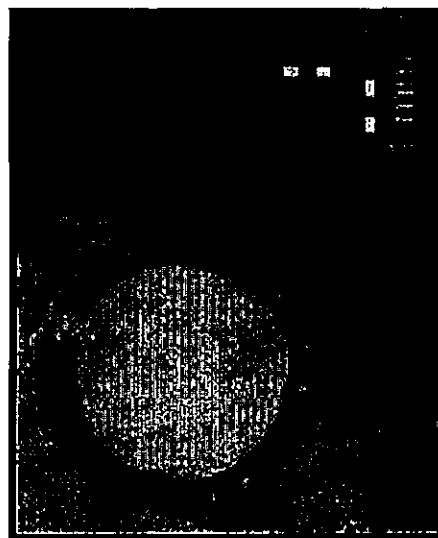

AS2

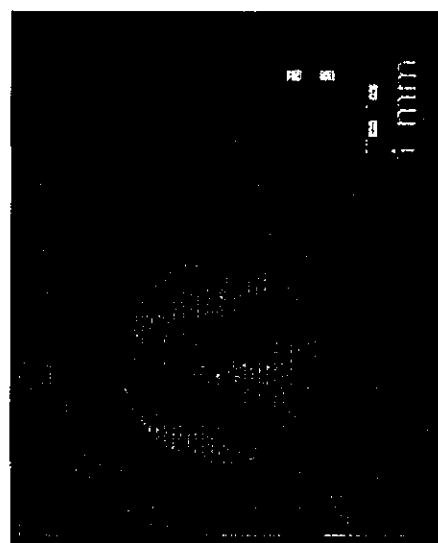

AS3 (BMS Control)



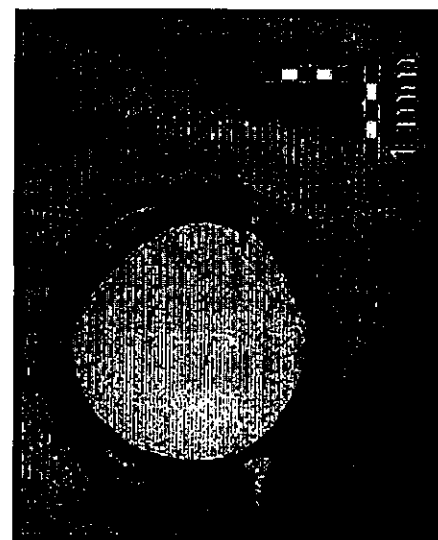


Figure 14

AS1

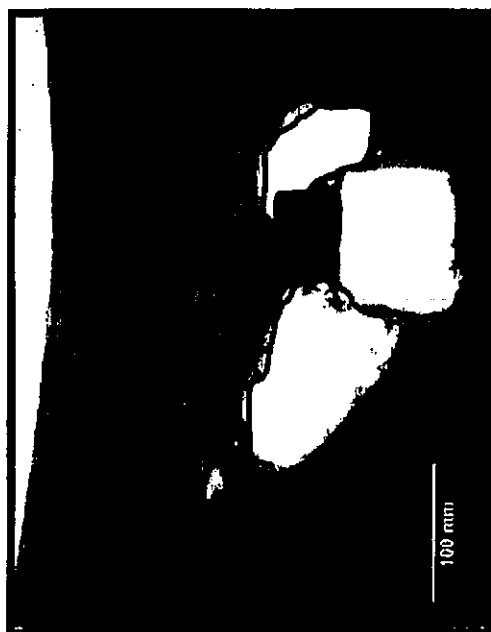


AS2

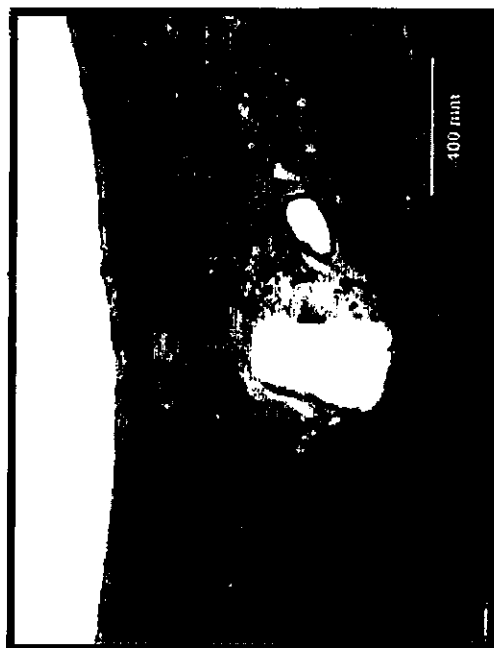


14/22

Figure 15

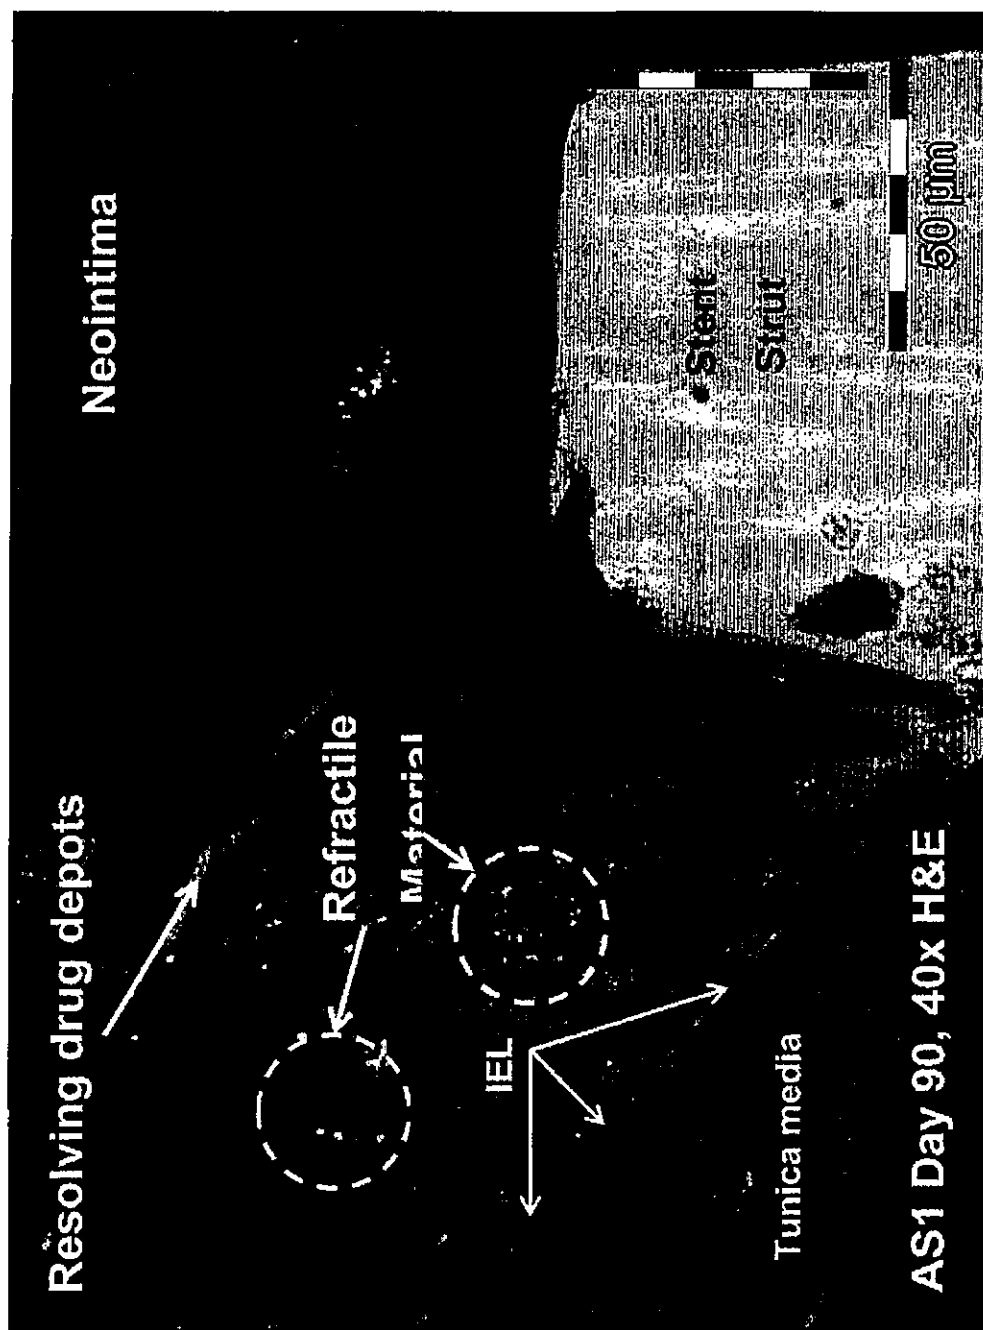

15/22

15/22

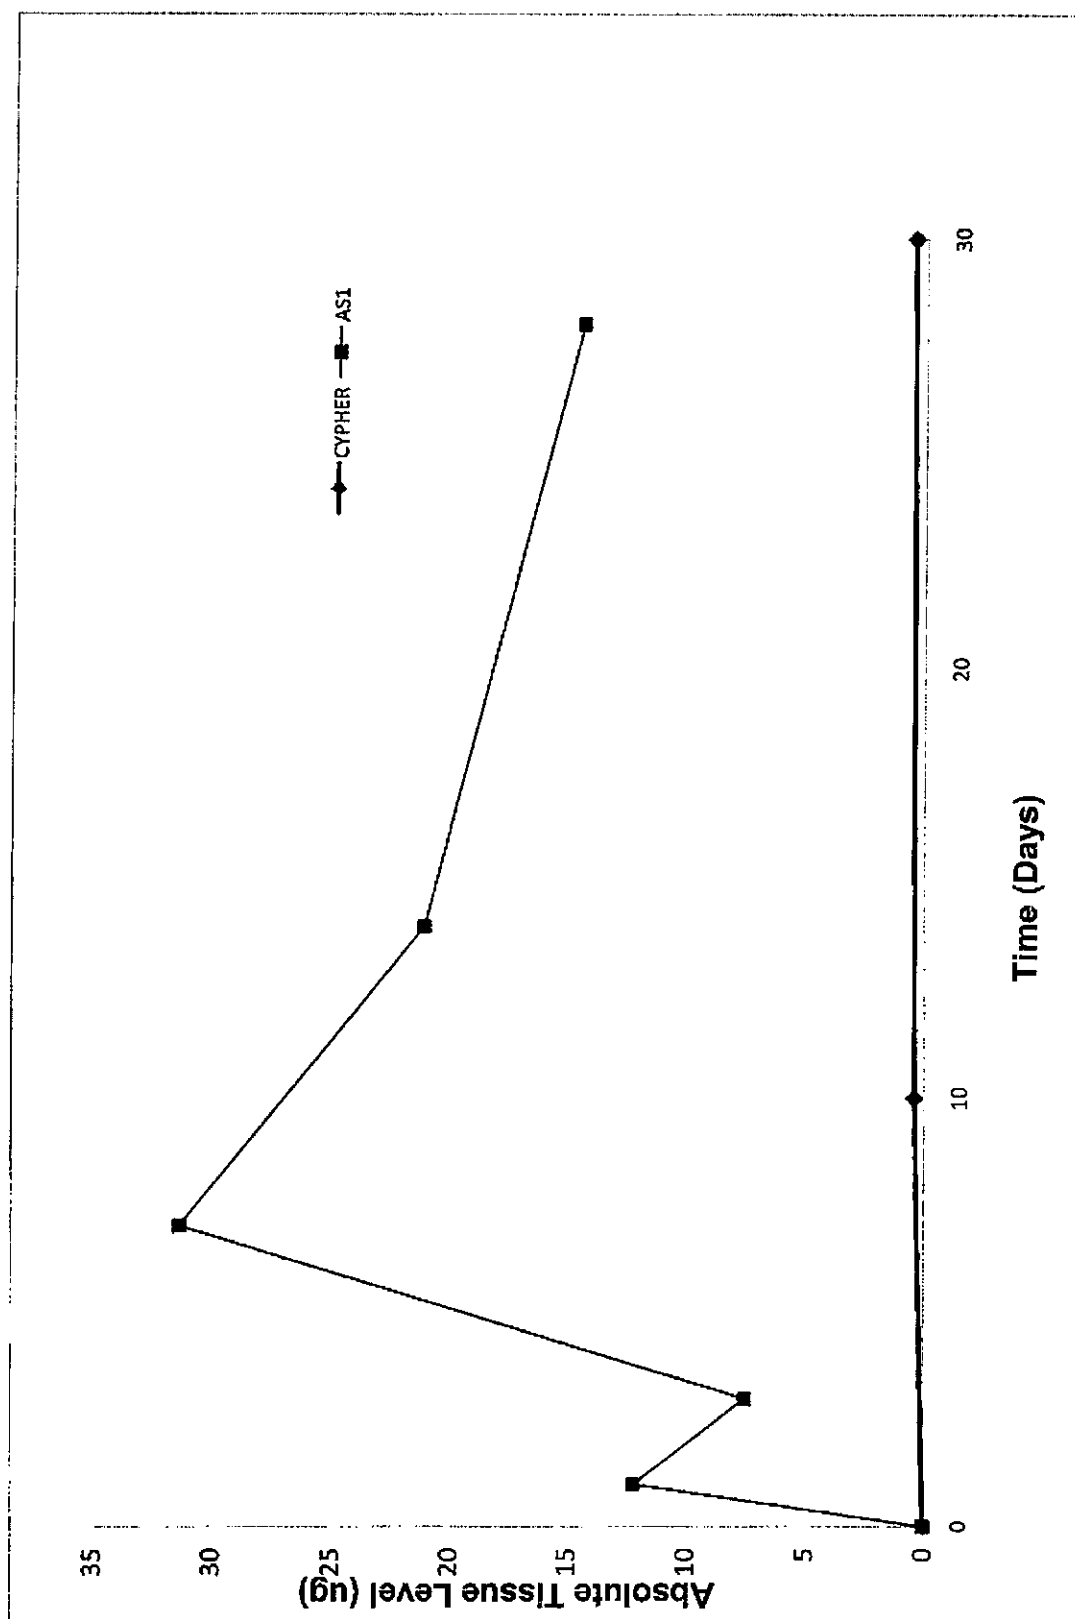


15

Figure 16

16/22

-16/22-

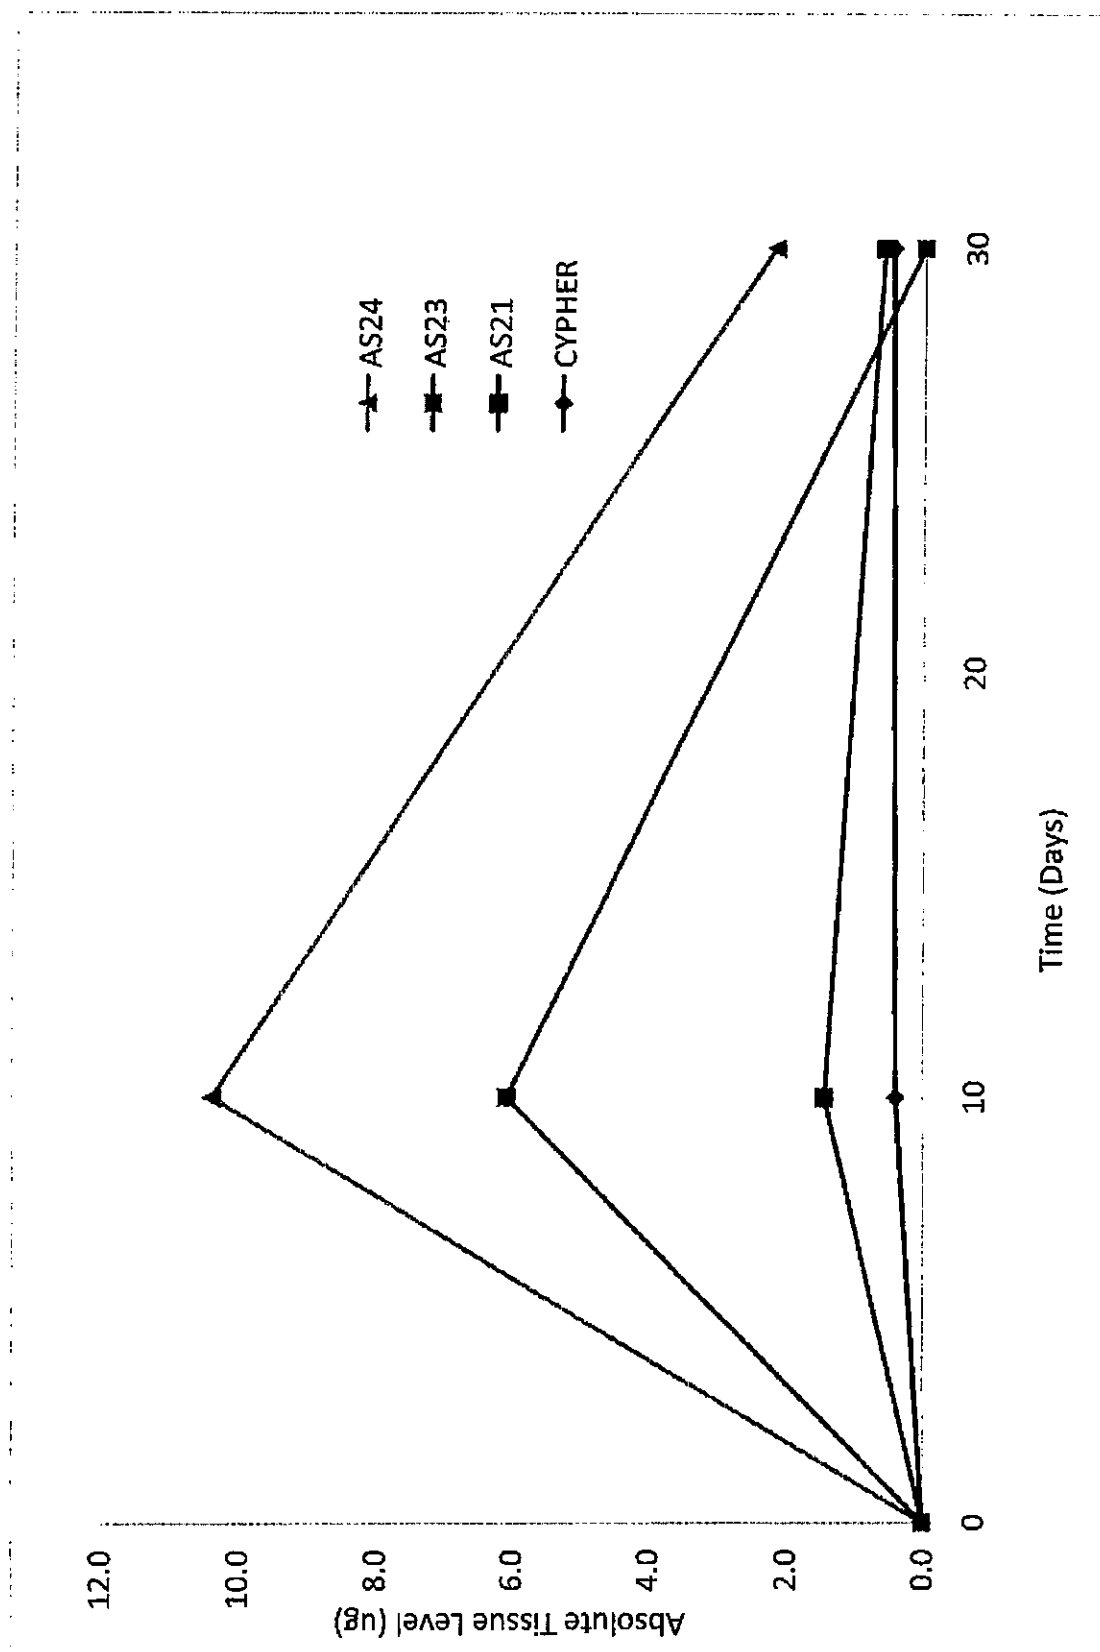

-16-

Figure 17

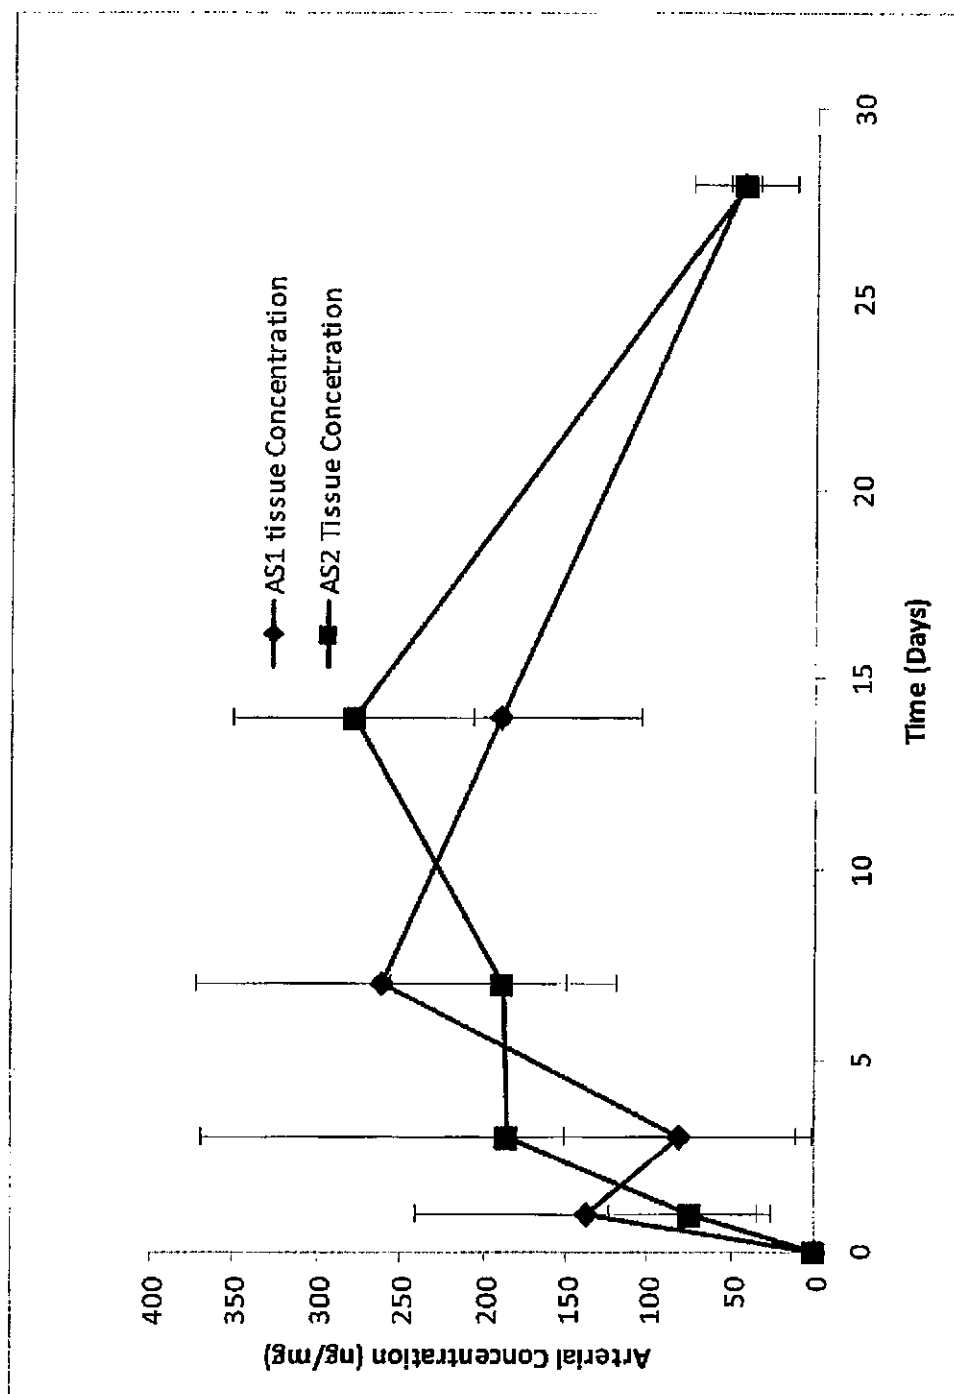


Figure 18

18/22

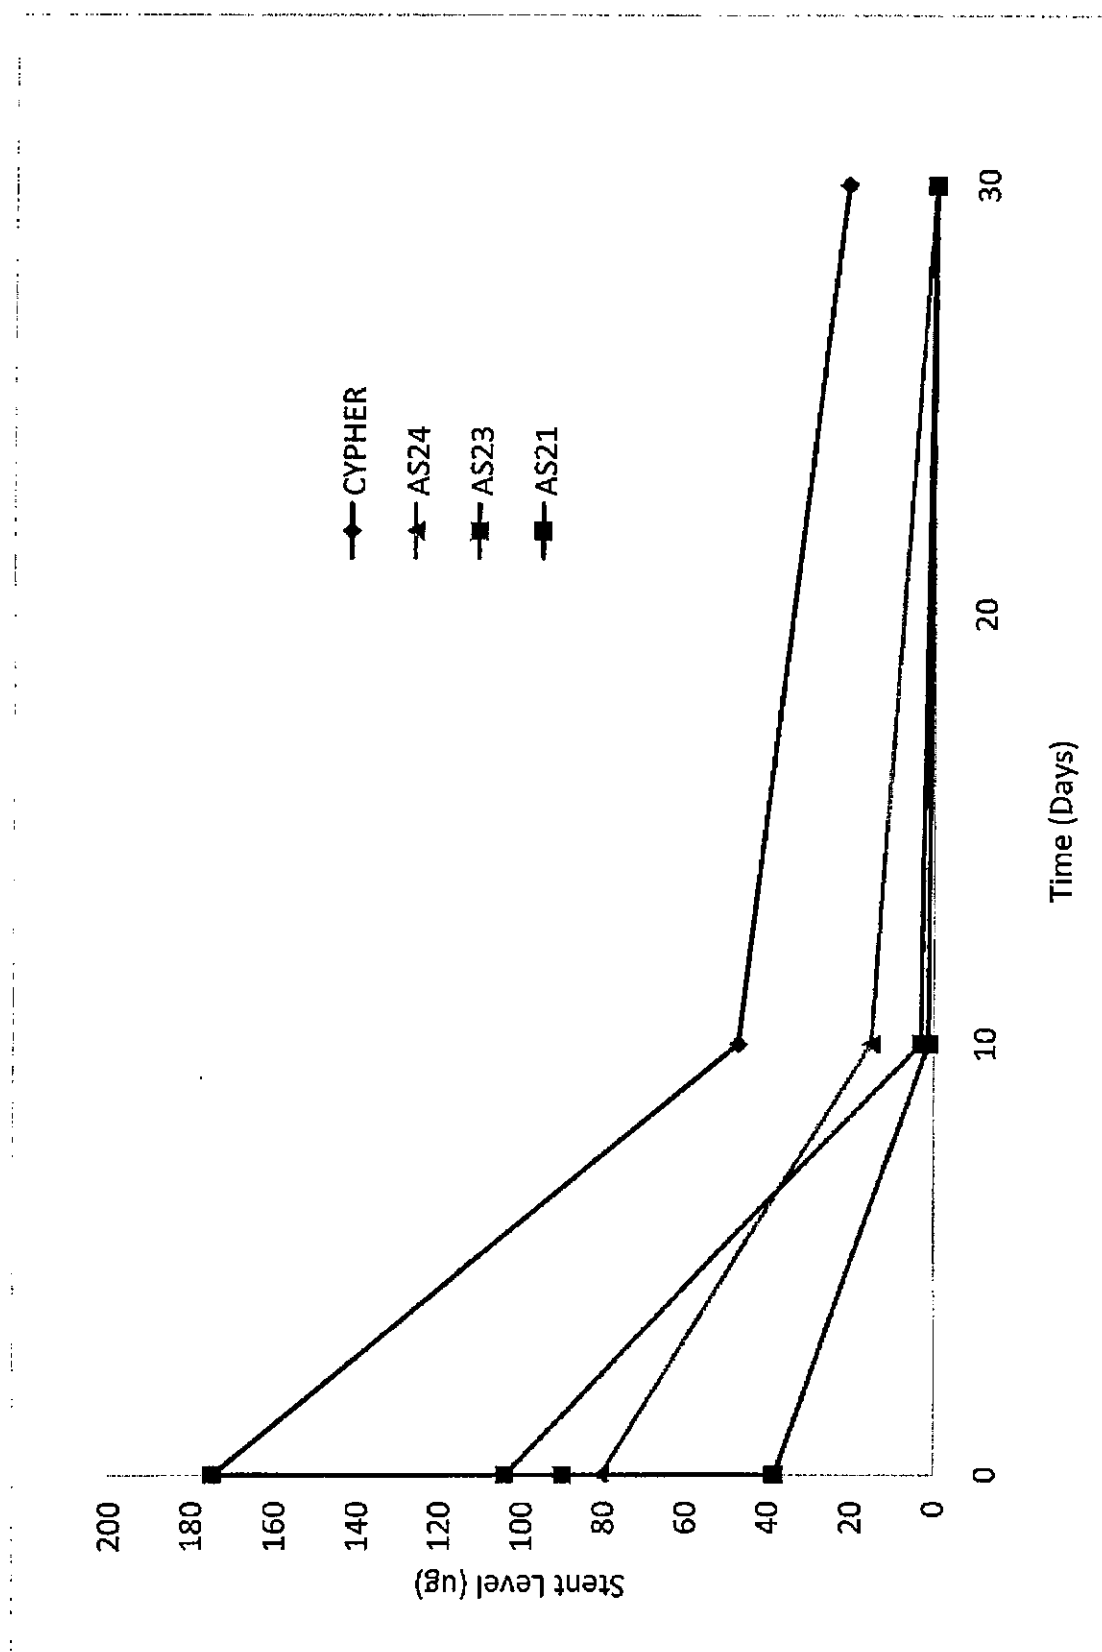


Figure 19

19/22



Figure 20

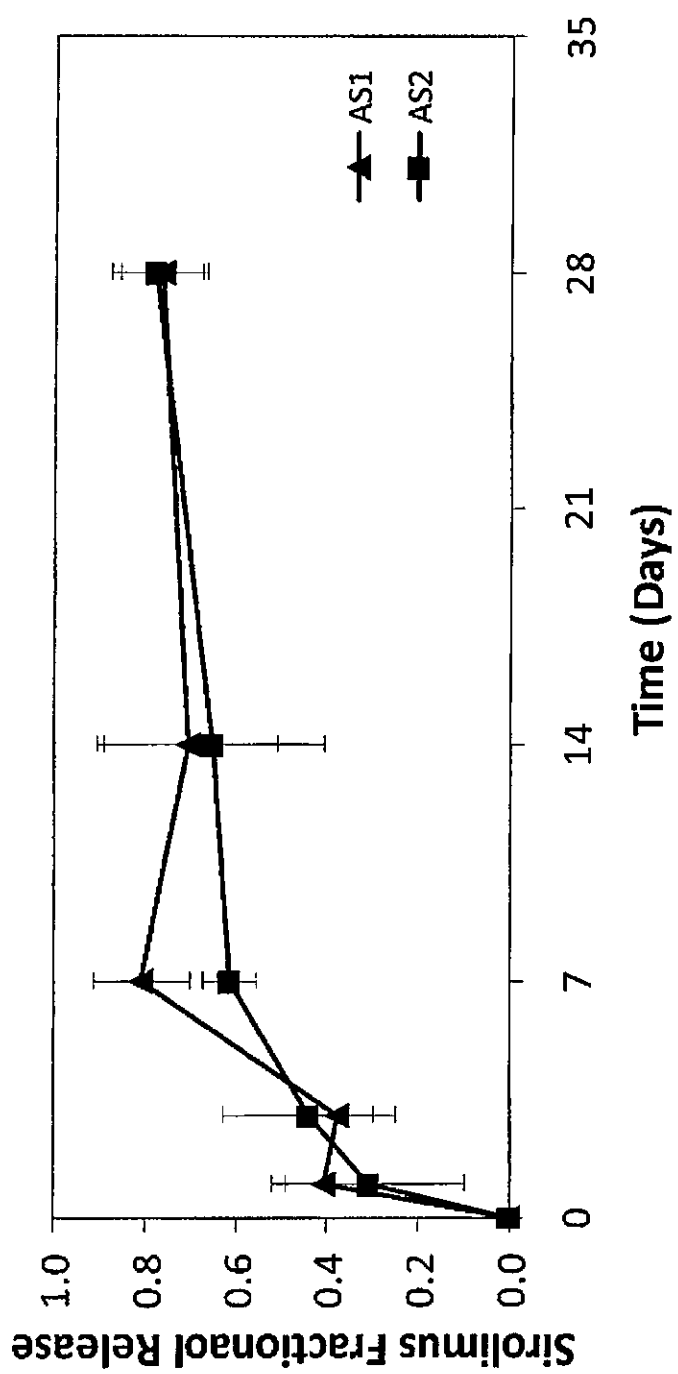


Figure 21

Sirolimus Blood Concentration Following Single Stent Implant


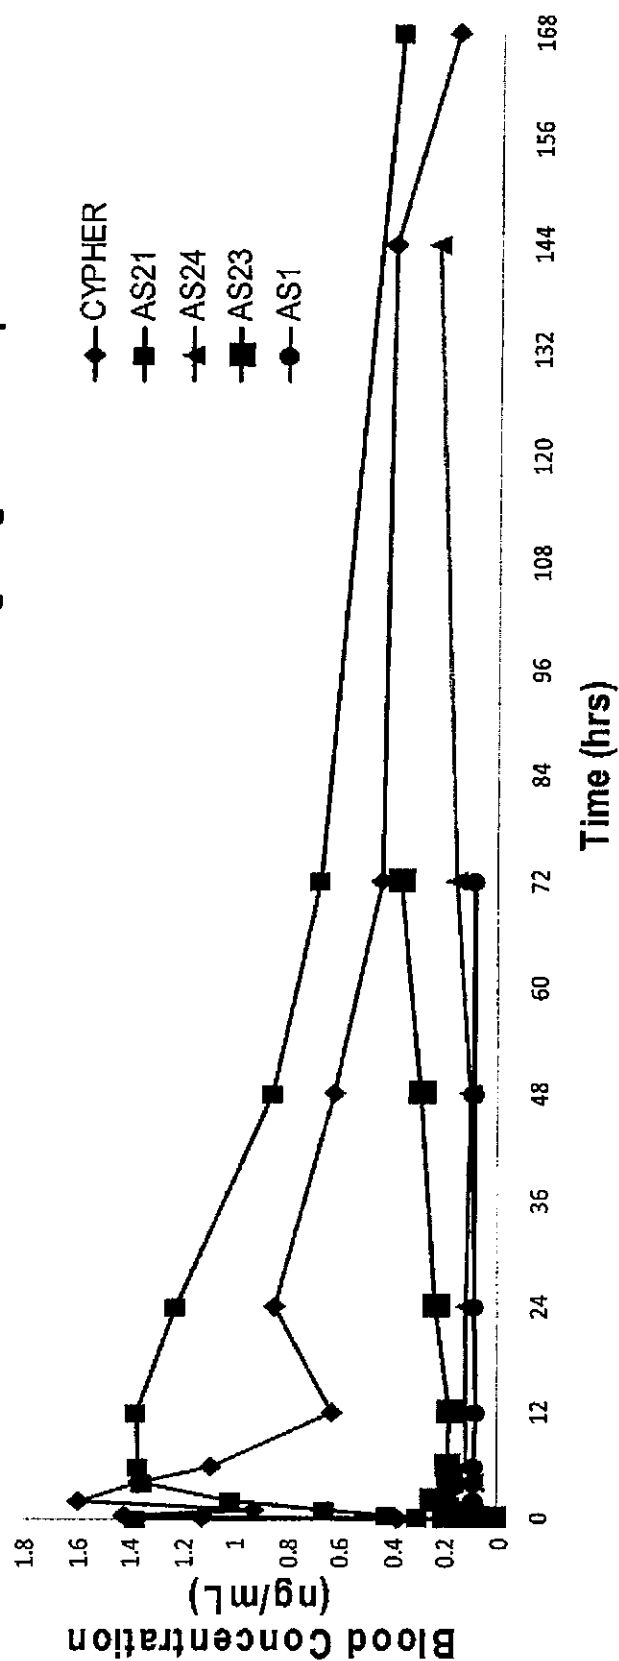


Figure 22

~~22/22~~

Figure 23

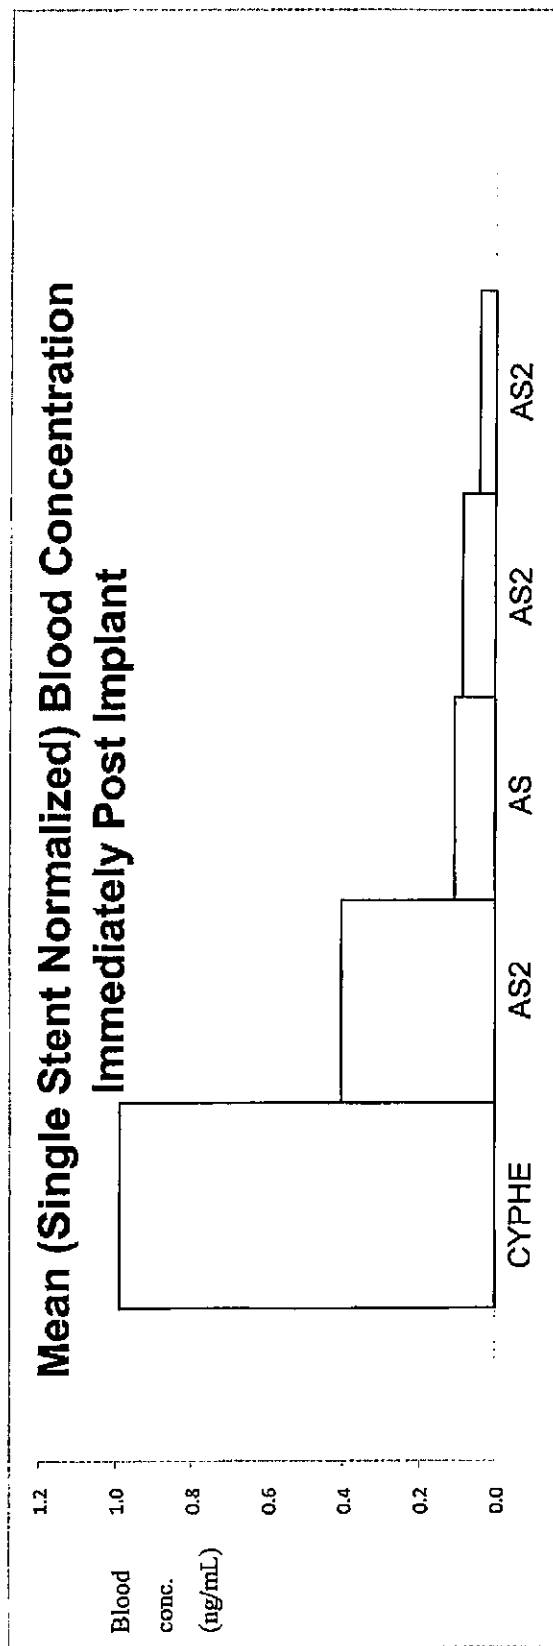

~~22~~