

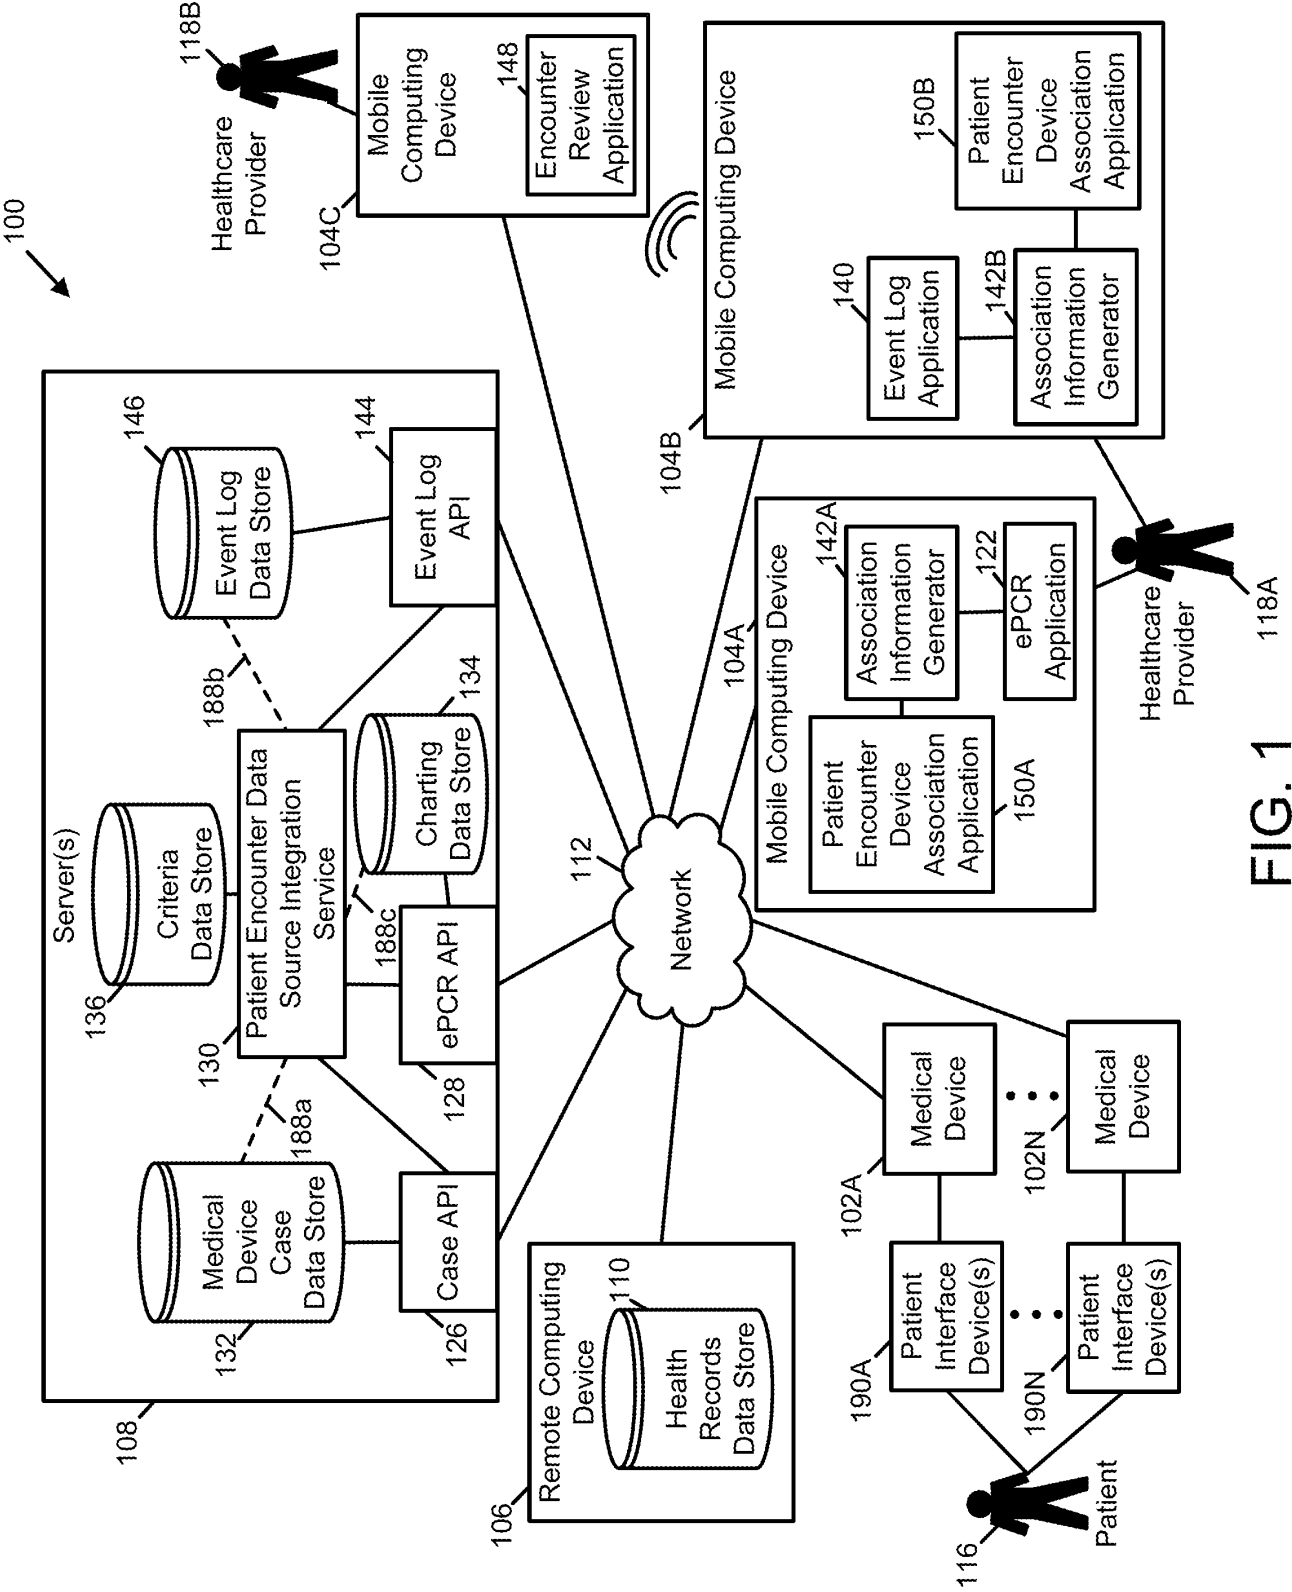


FIG. 1

200

| 202<br>Encounter ID                  | 204<br>Medical Device ID <sub>1</sub> | 206<br>Timestamp <sub>1</sub> | 208<br>Medical Device ID <sub>2</sub> | 210<br>Timestamp <sub>2</sub> |
|--------------------------------------|---------------------------------------|-------------------------------|---------------------------------------|-------------------------------|
| 128b2830-5014-11ea-b77f-2e728ce88125 | 839402938                             | 2019-05-01 11:20:34           | 839402967                             | 2019-05-01 11:22:15           |

FIG. 2

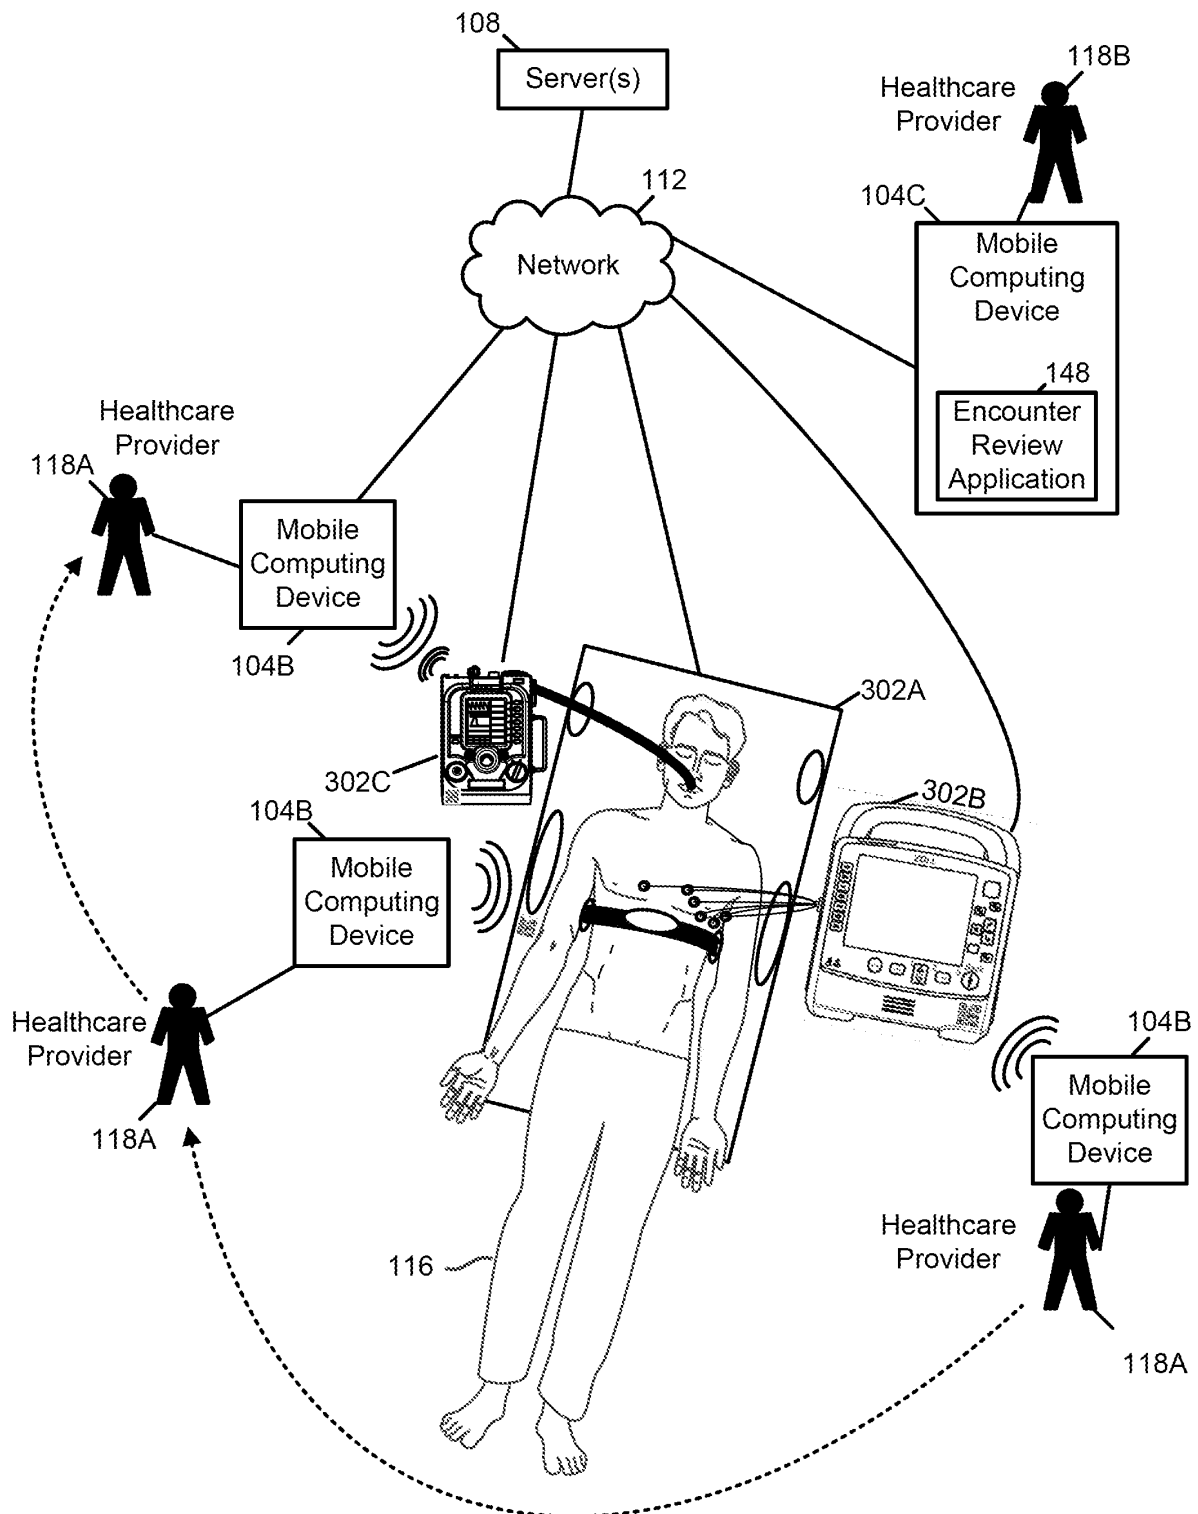
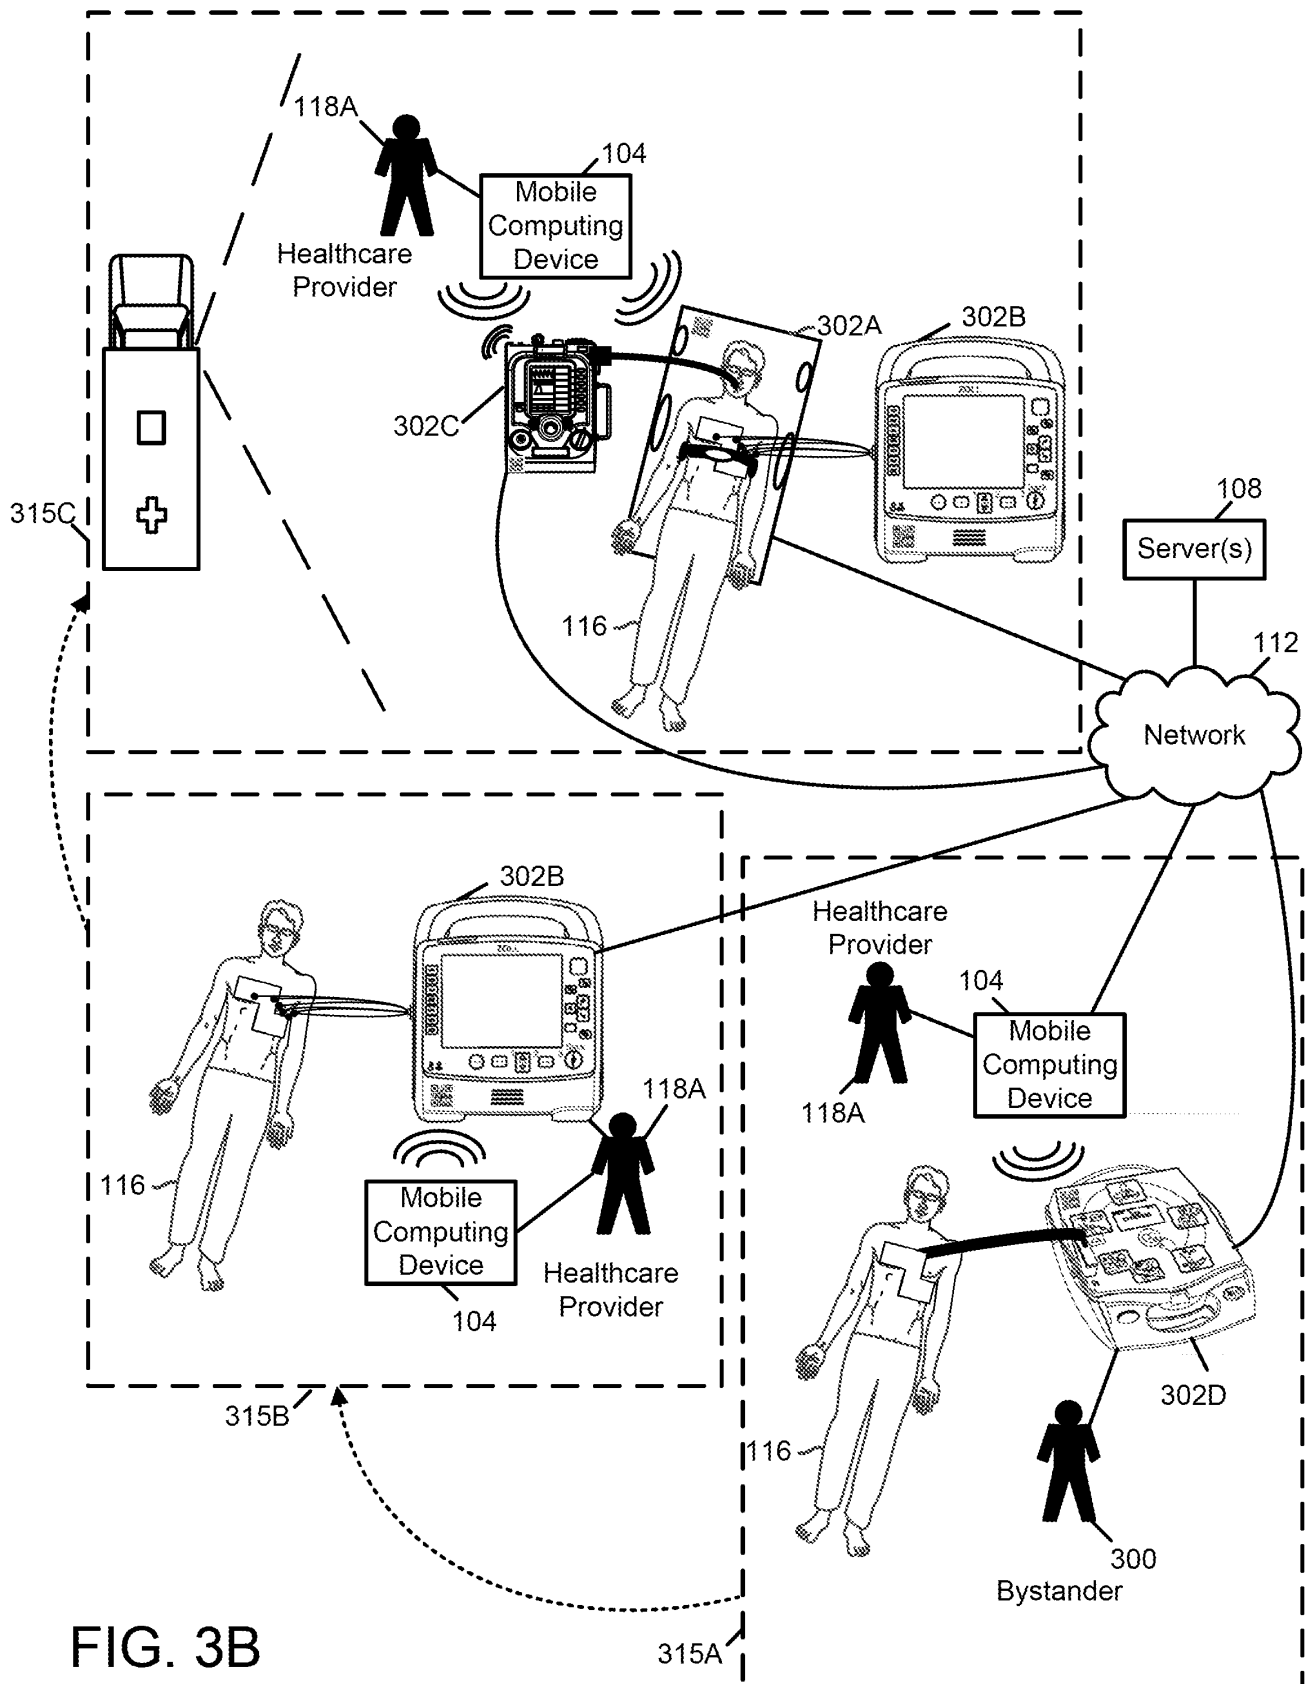


FIG. 3A



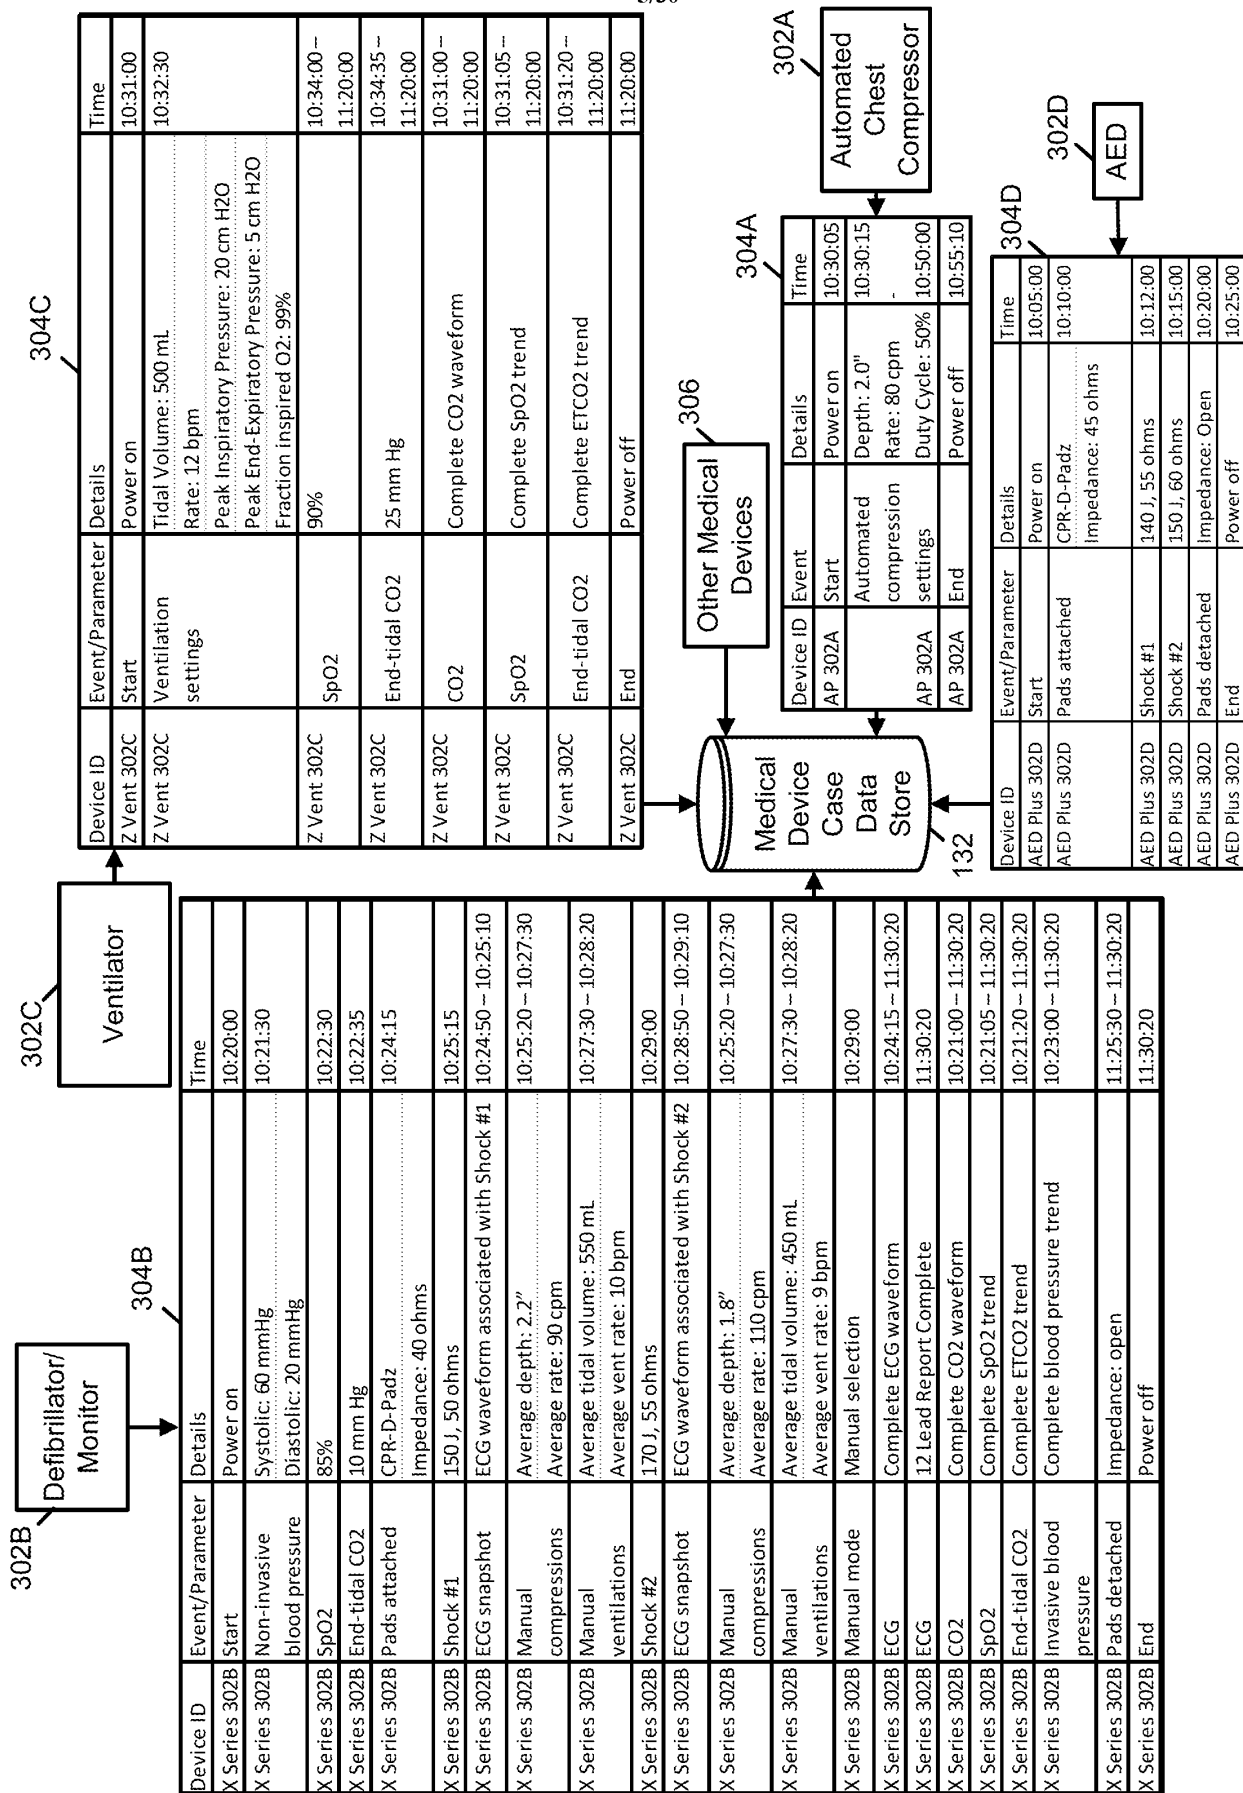


FIG. 3C

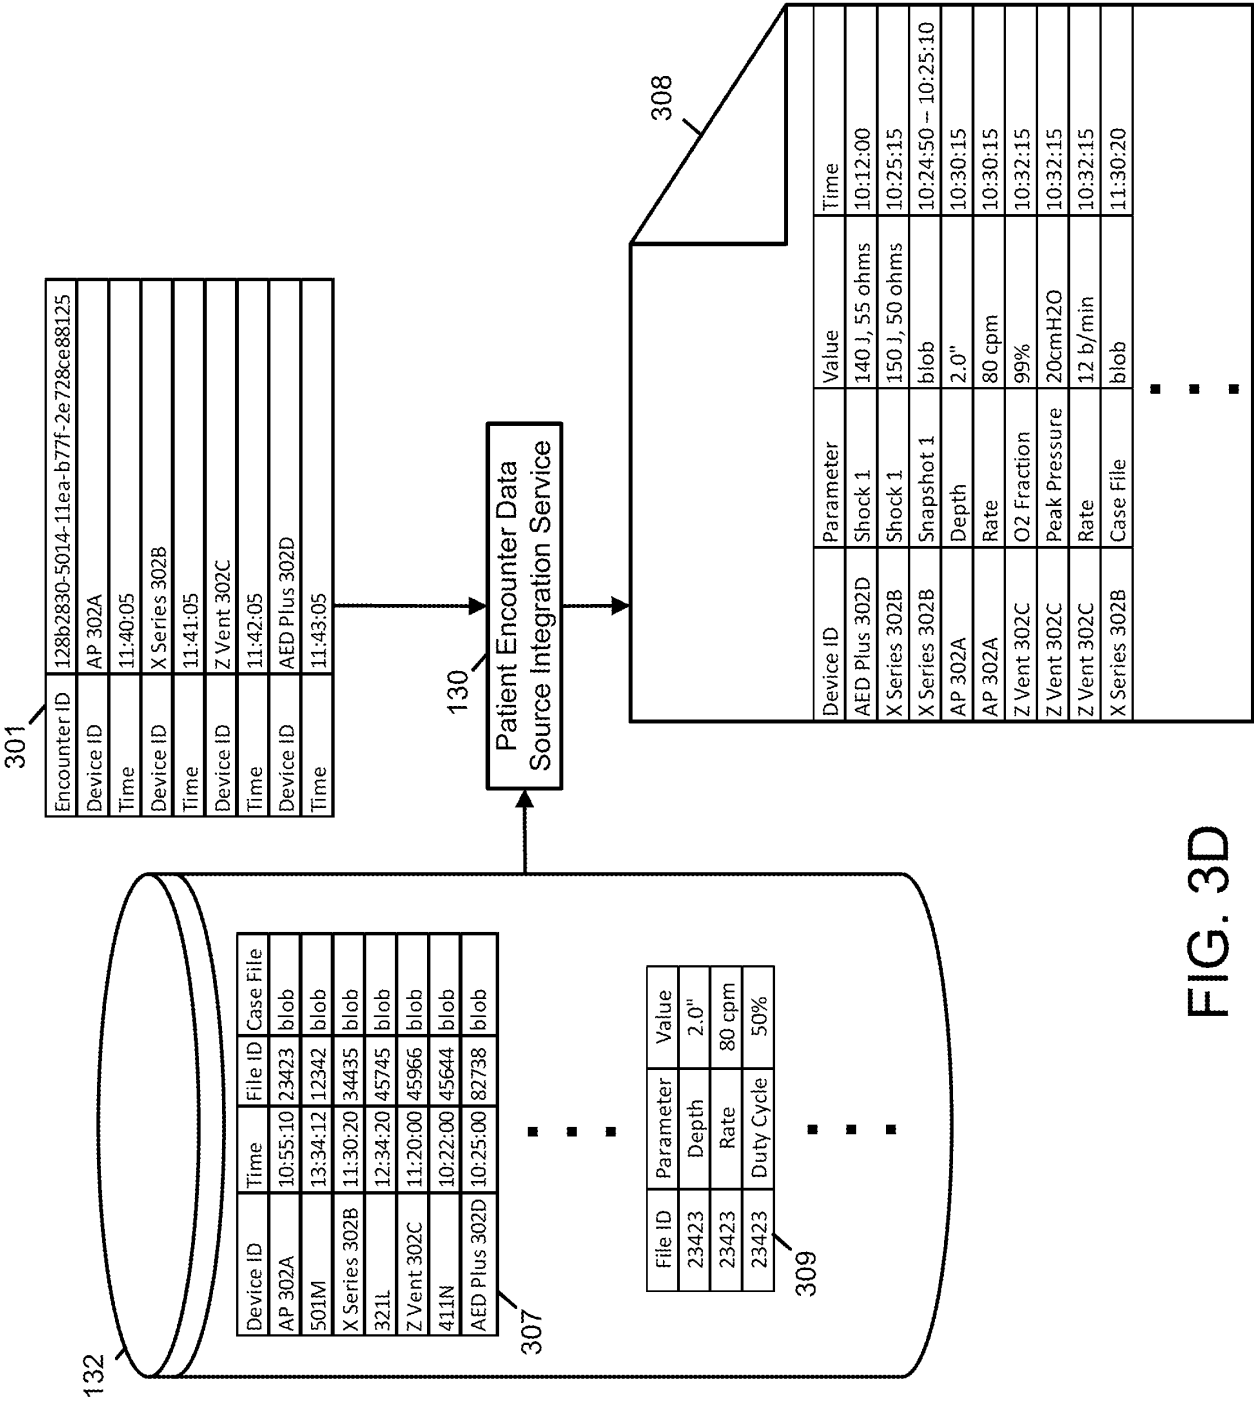
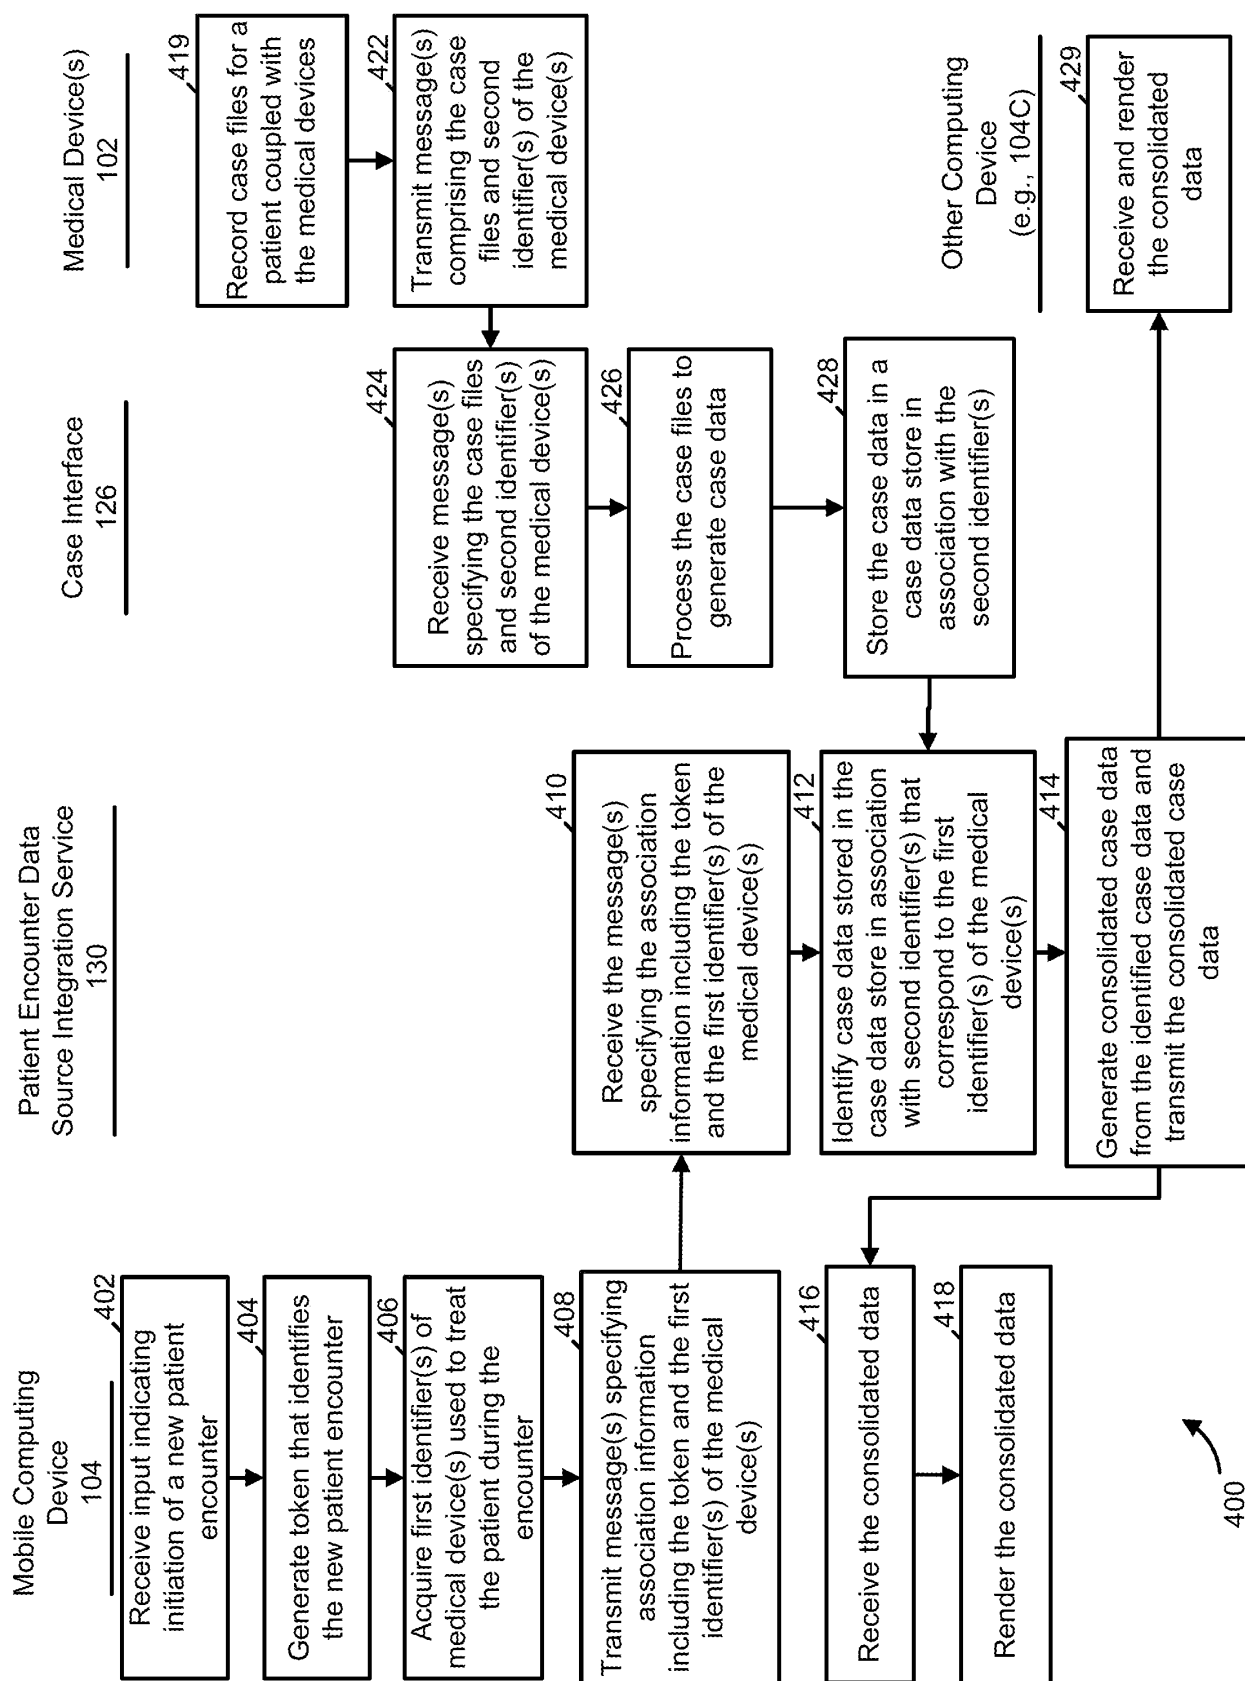


FIG. 3D



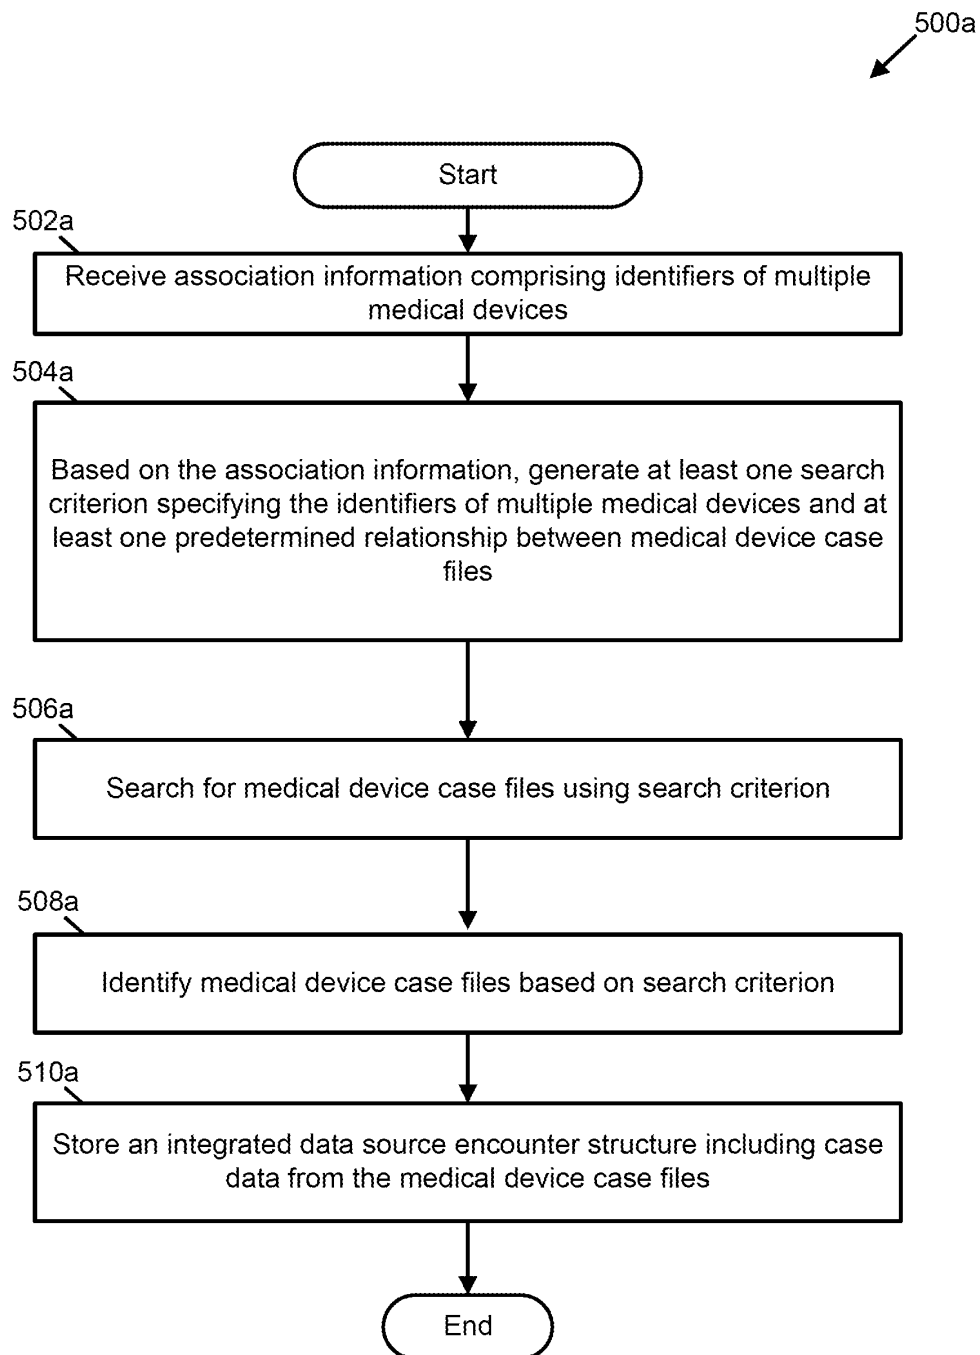


FIG. 5A

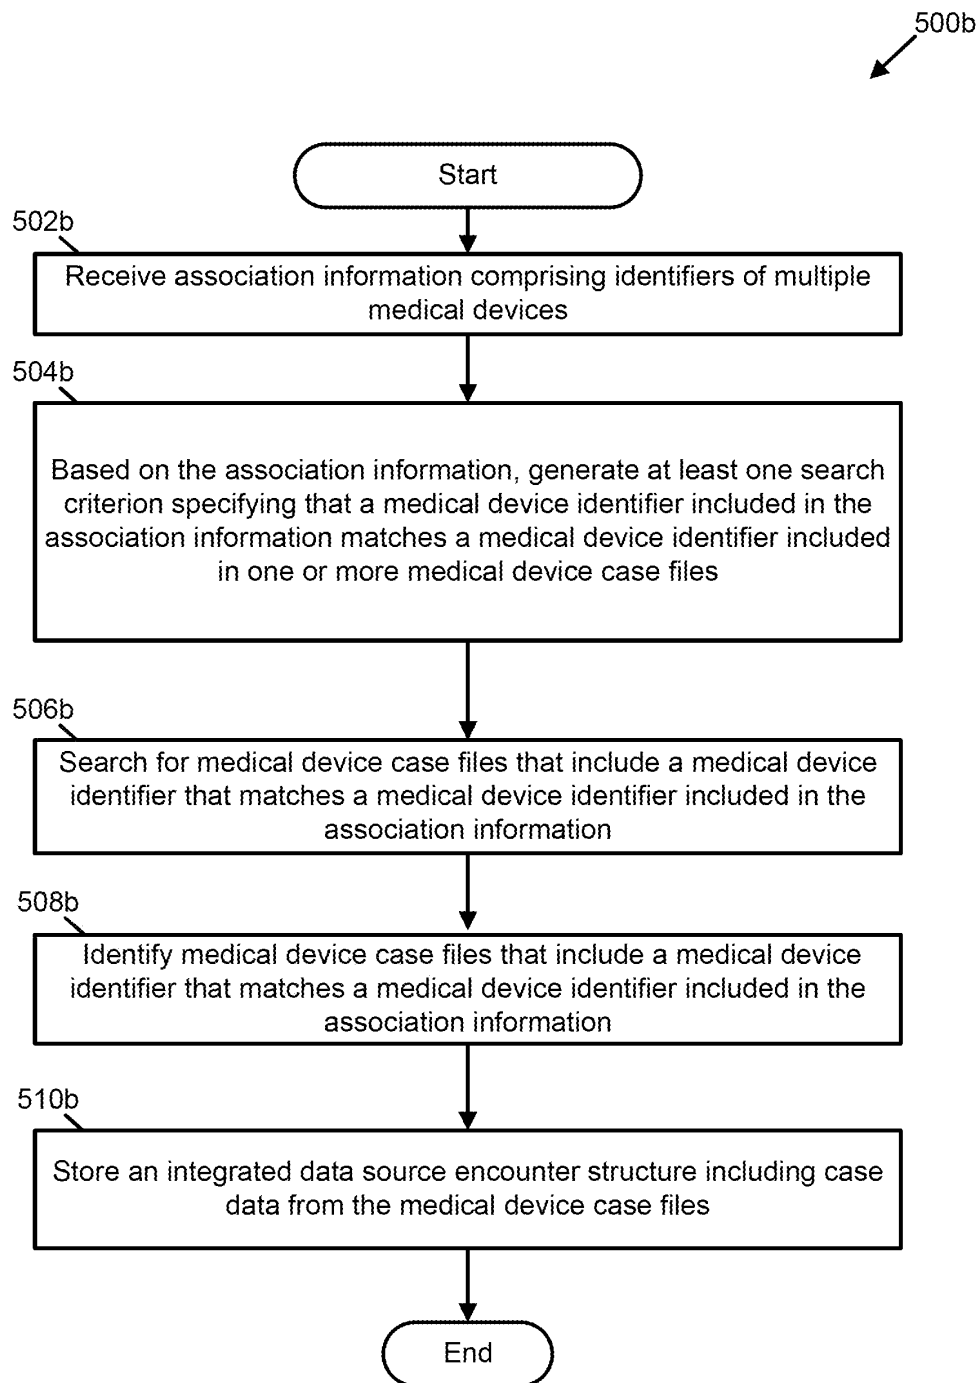


FIG. 5B

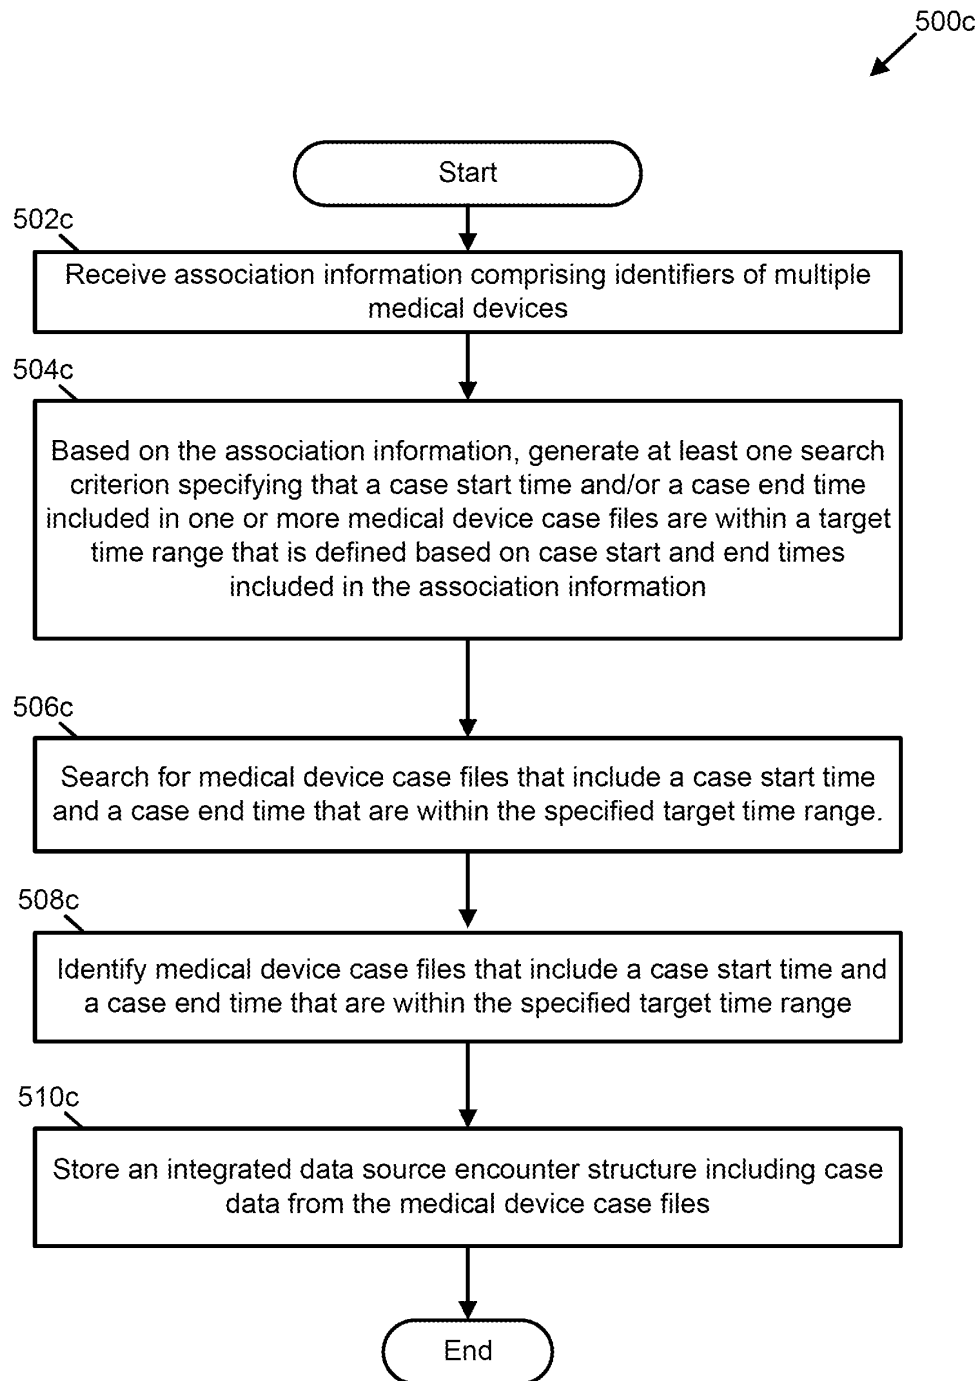


FIG. 5C

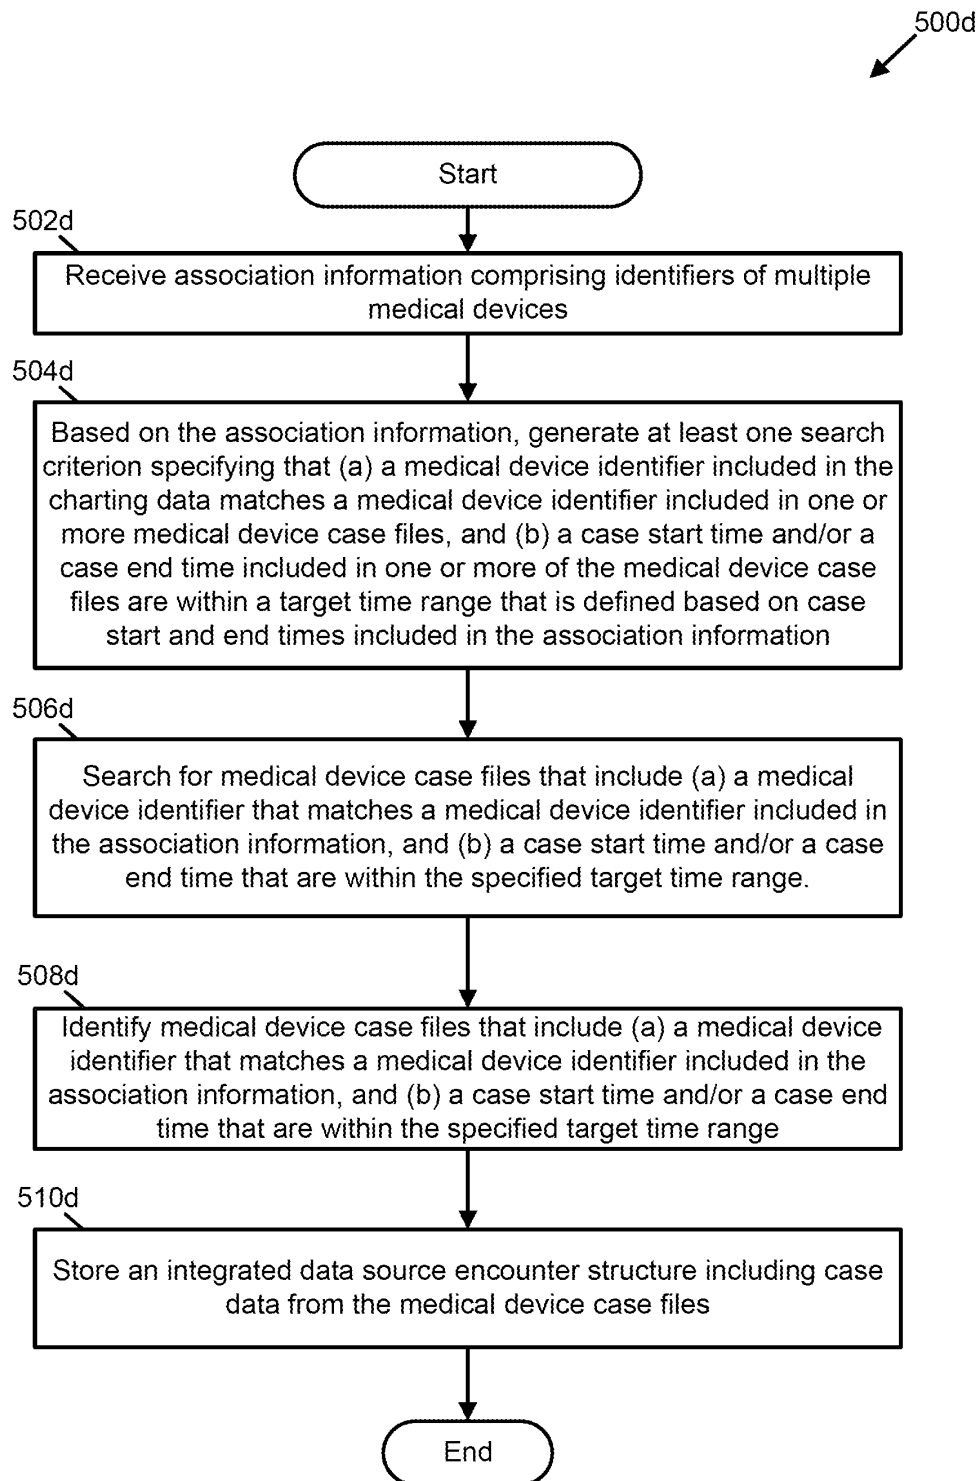


FIG. 5D

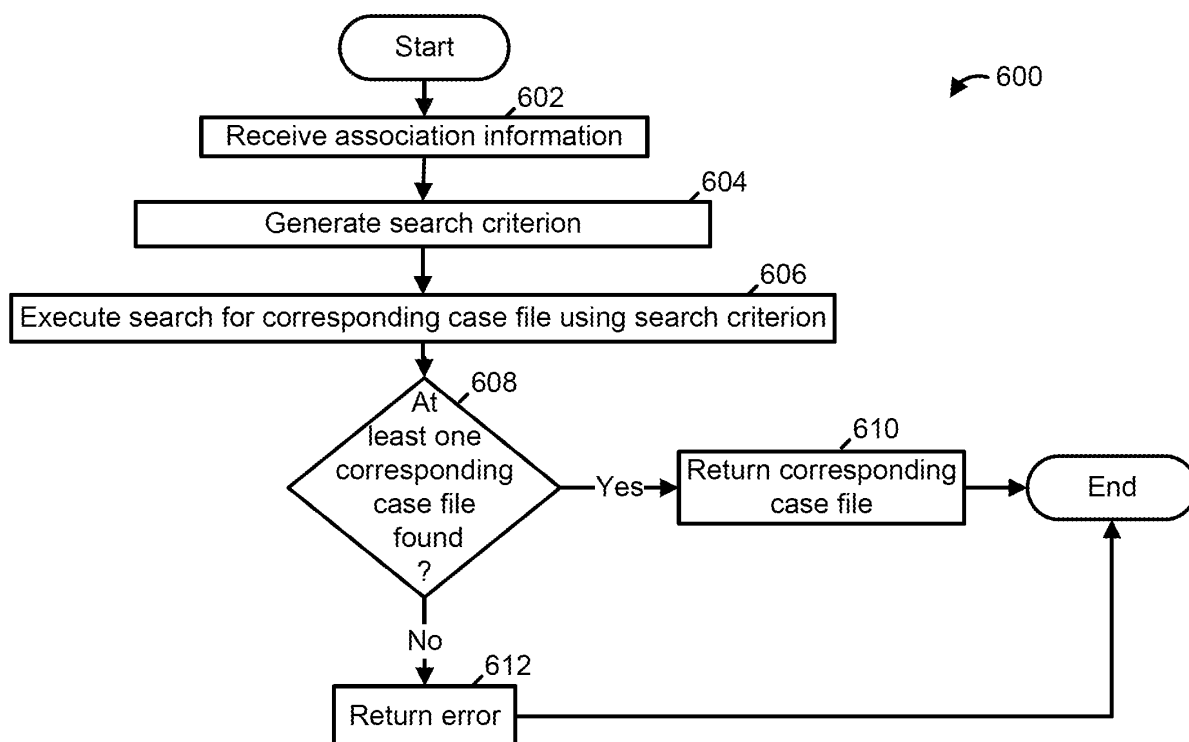


FIG. 6

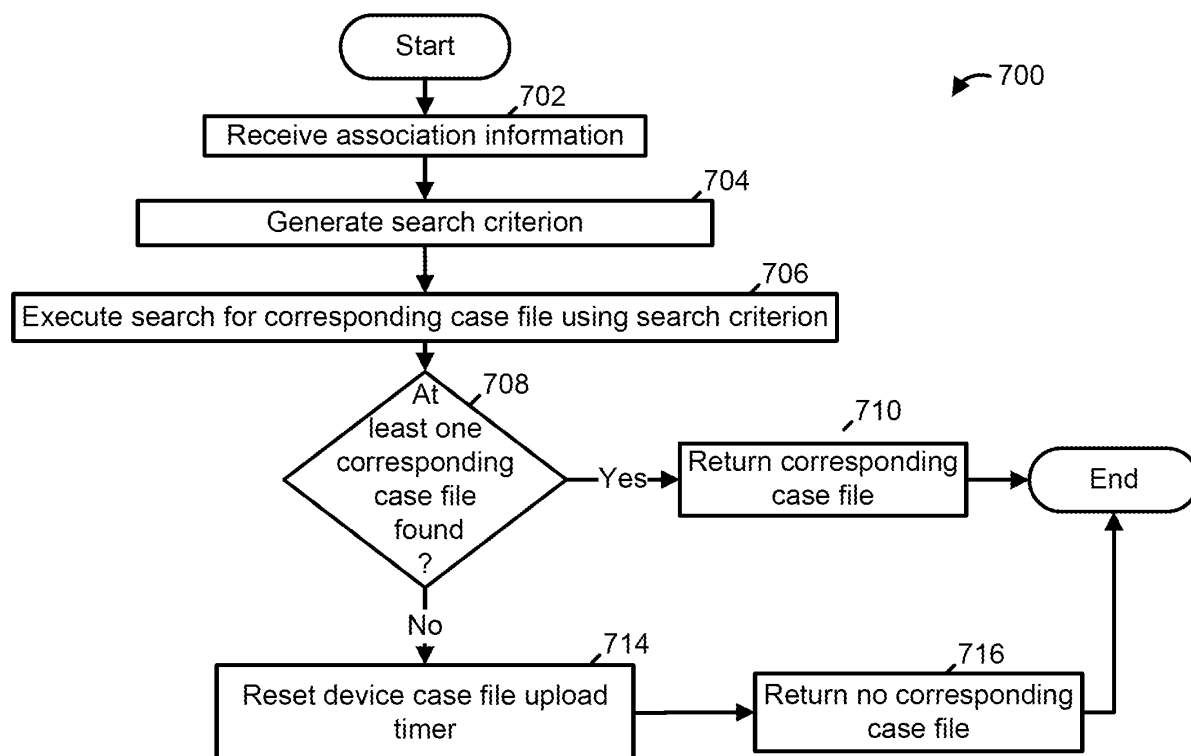


FIG. 7

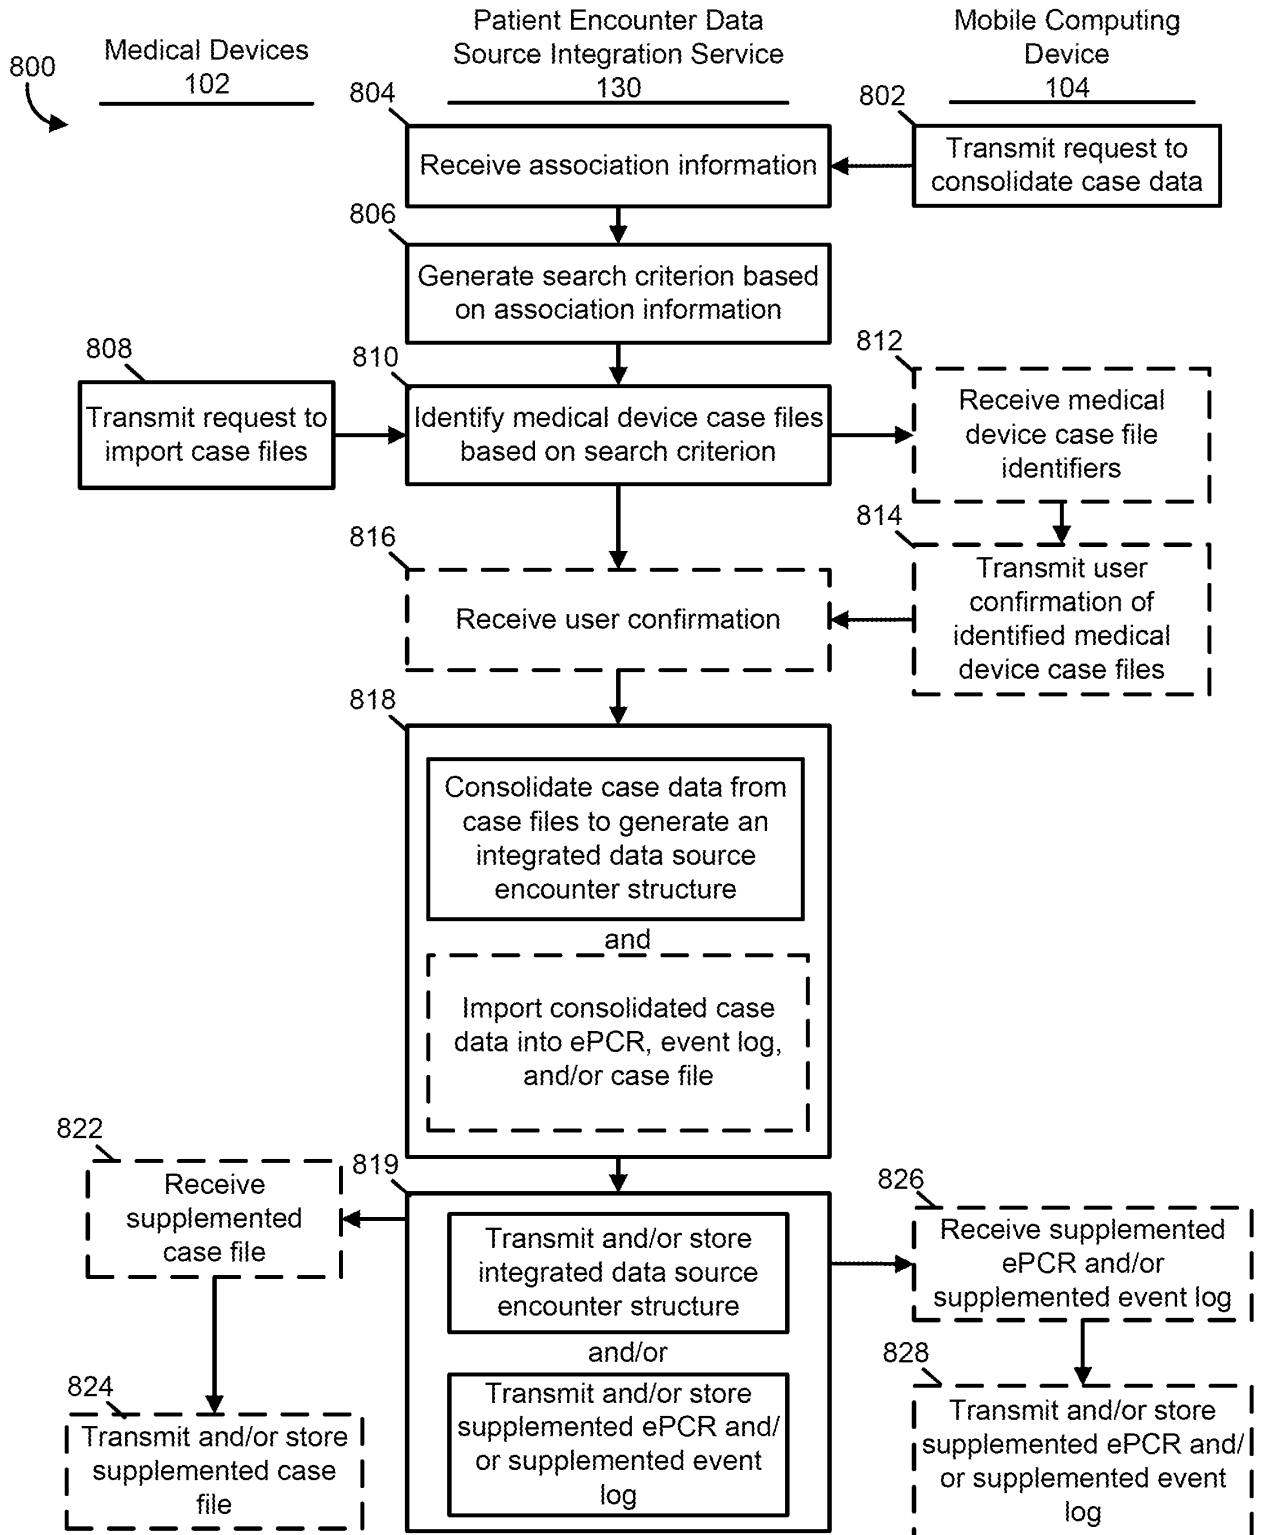


FIG. 8

900

902

904

906

| Case Start Time | Medical Device ID | Confirm?                            |
|-----------------|-------------------|-------------------------------------|
| 12:18 a.m.      | 839402938         | <input checked="" type="checkbox"/> |
| 12:20 a.m.      | 981820199         | <input type="checkbox"/>            |
| 12:27 a.m.      | 129348910         | <input checked="" type="checkbox"/> |

908

Submit

FIG. 9

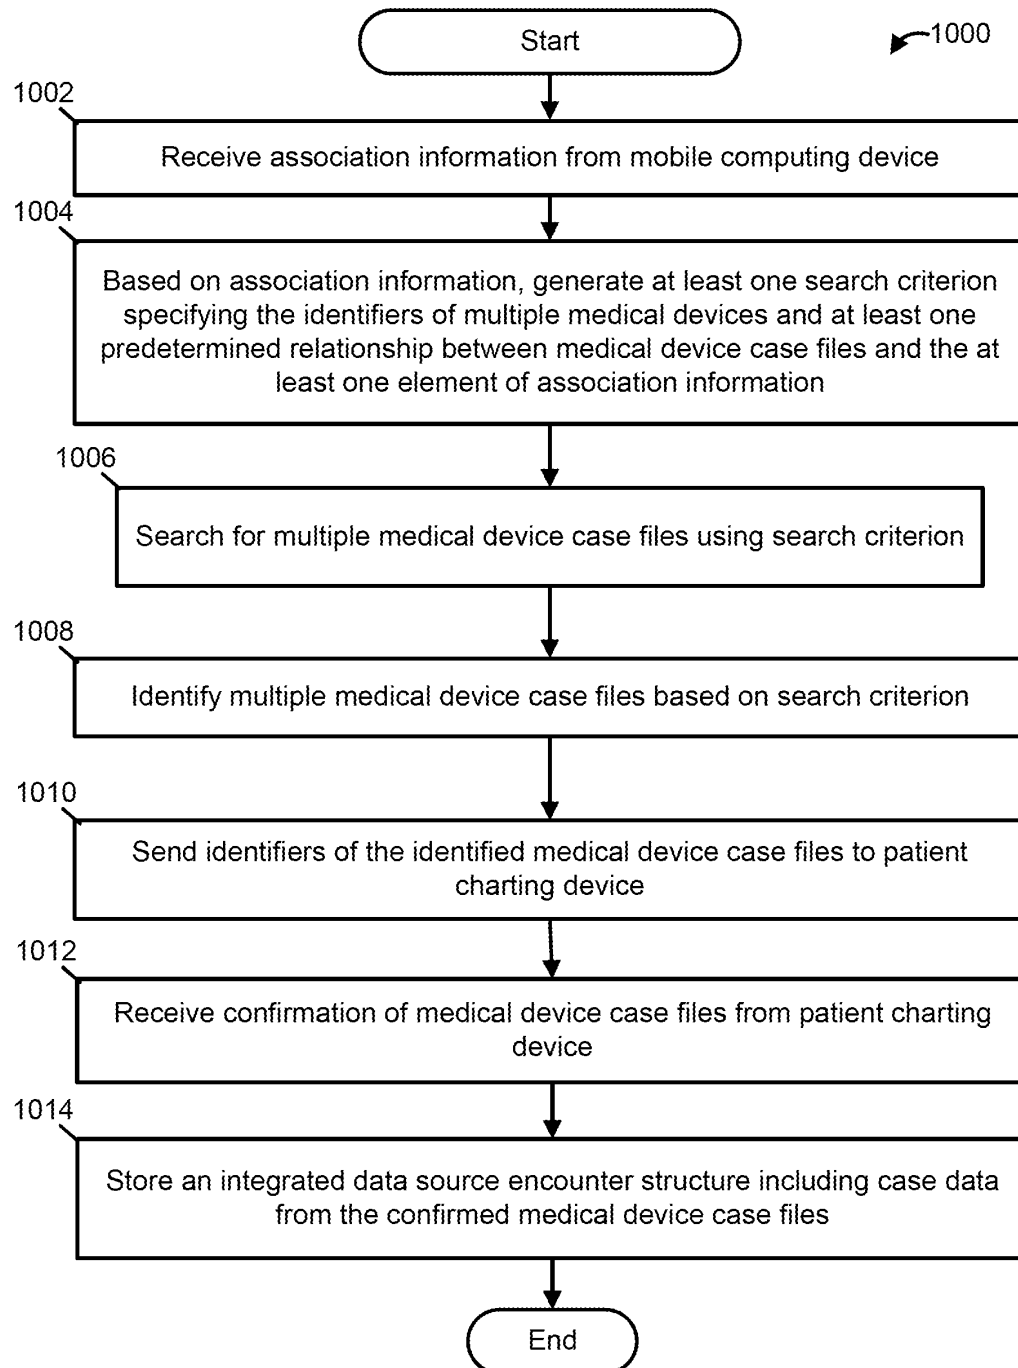


FIG. 10

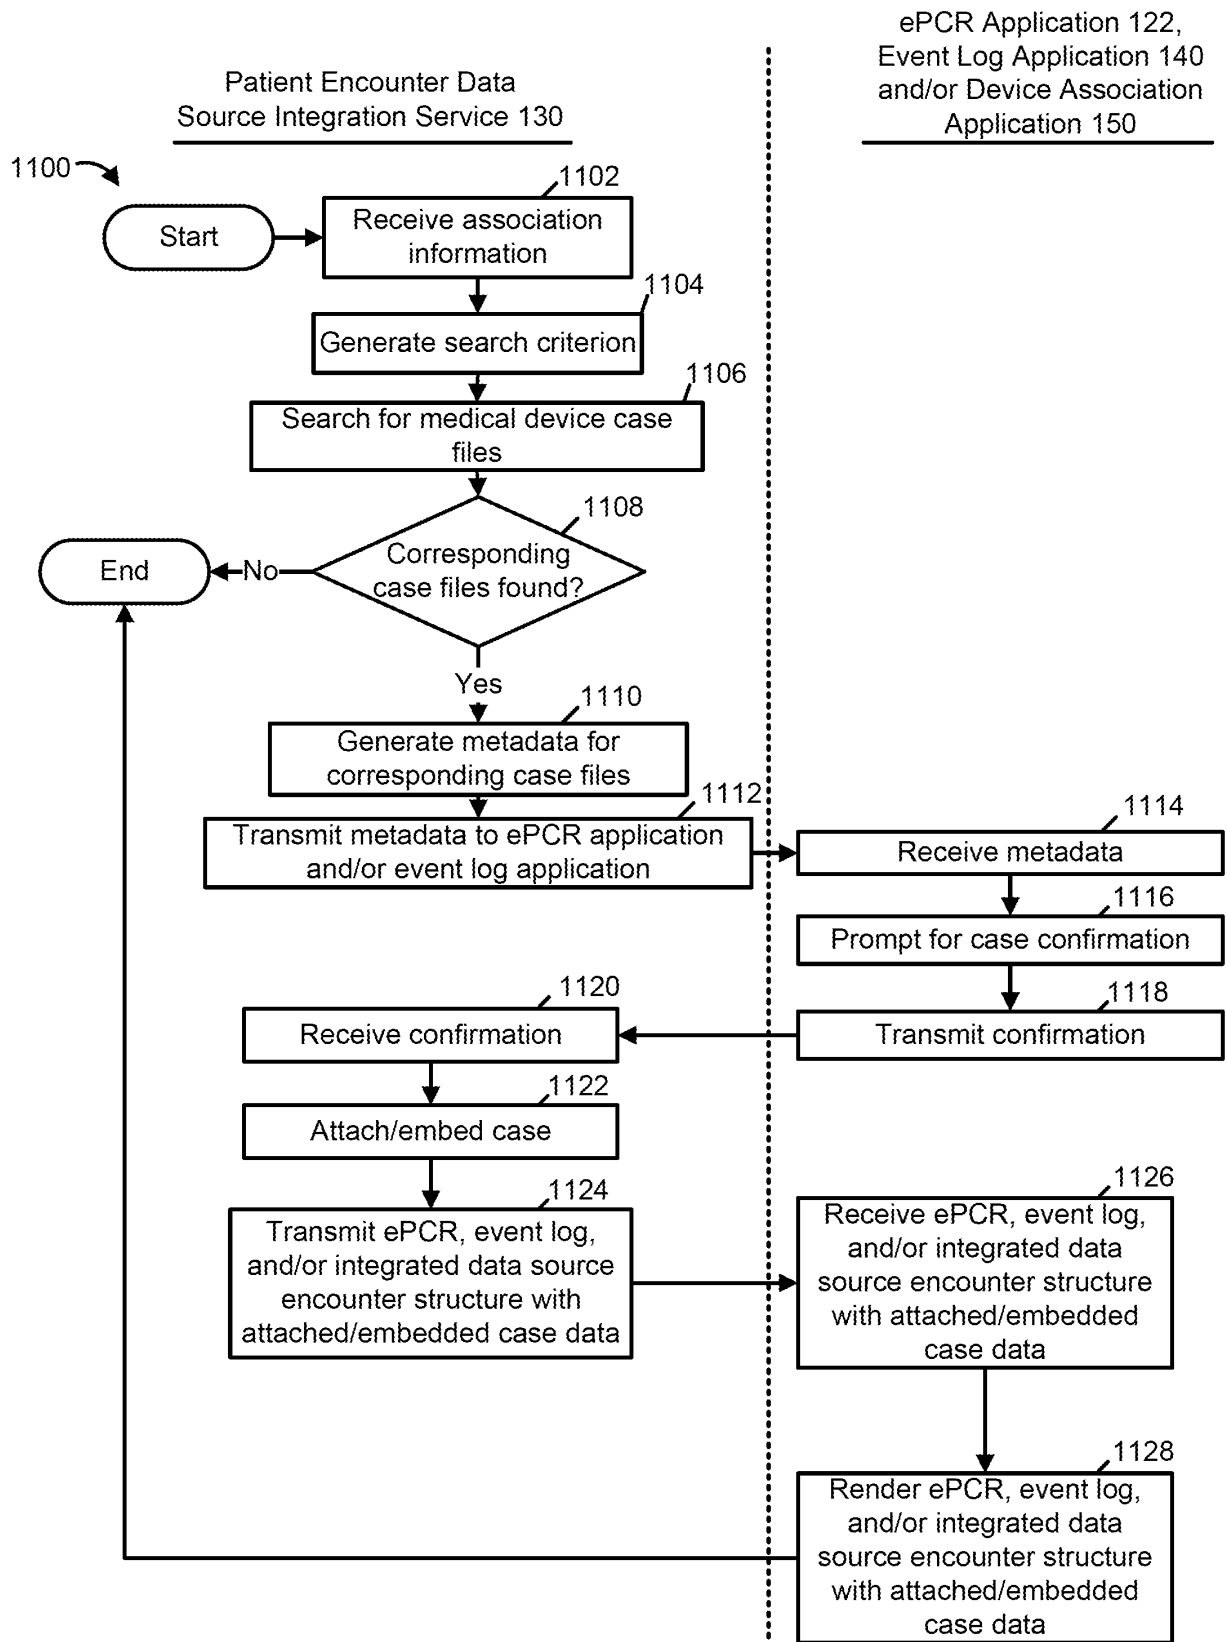


FIG. 11

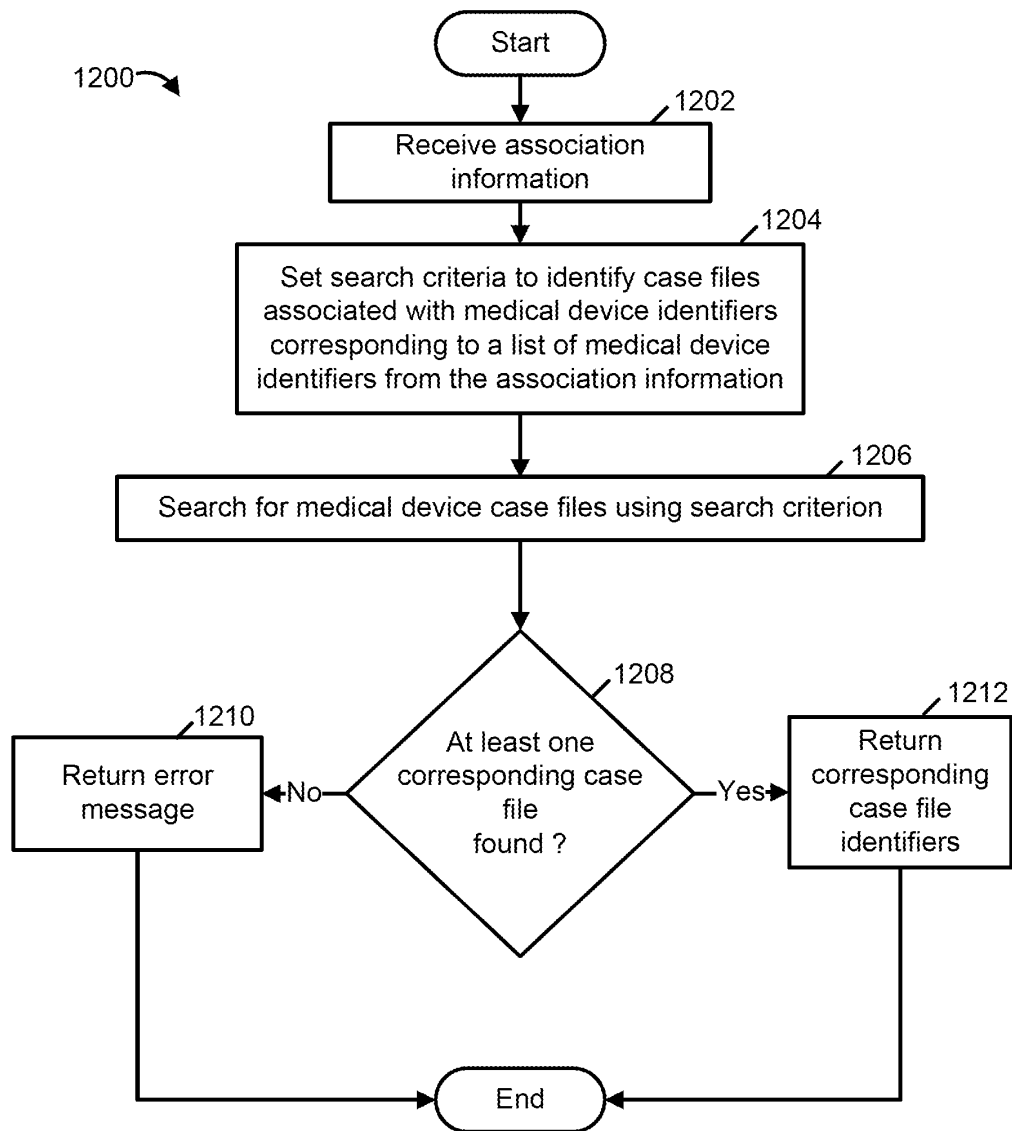


FIG. 12

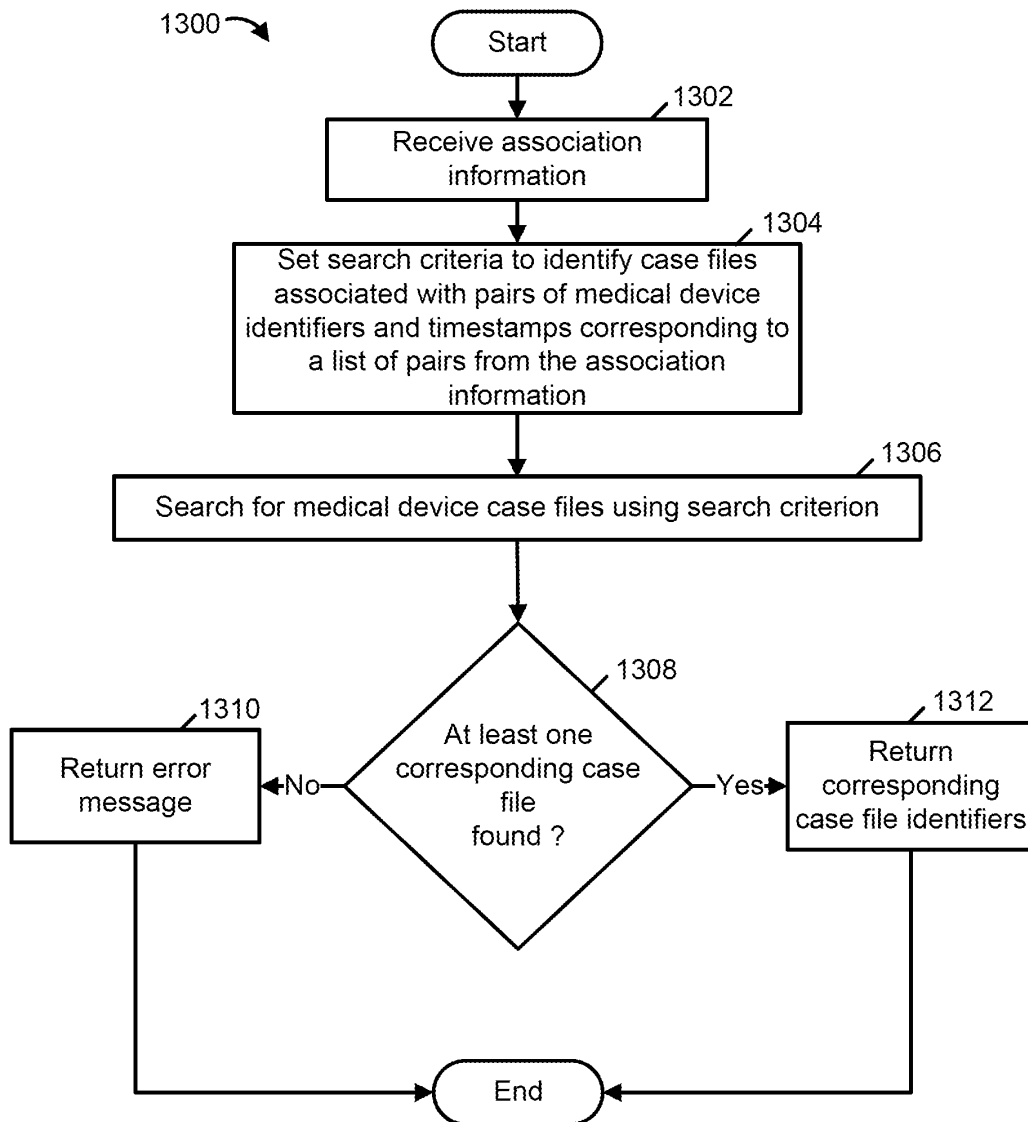


FIG. 13

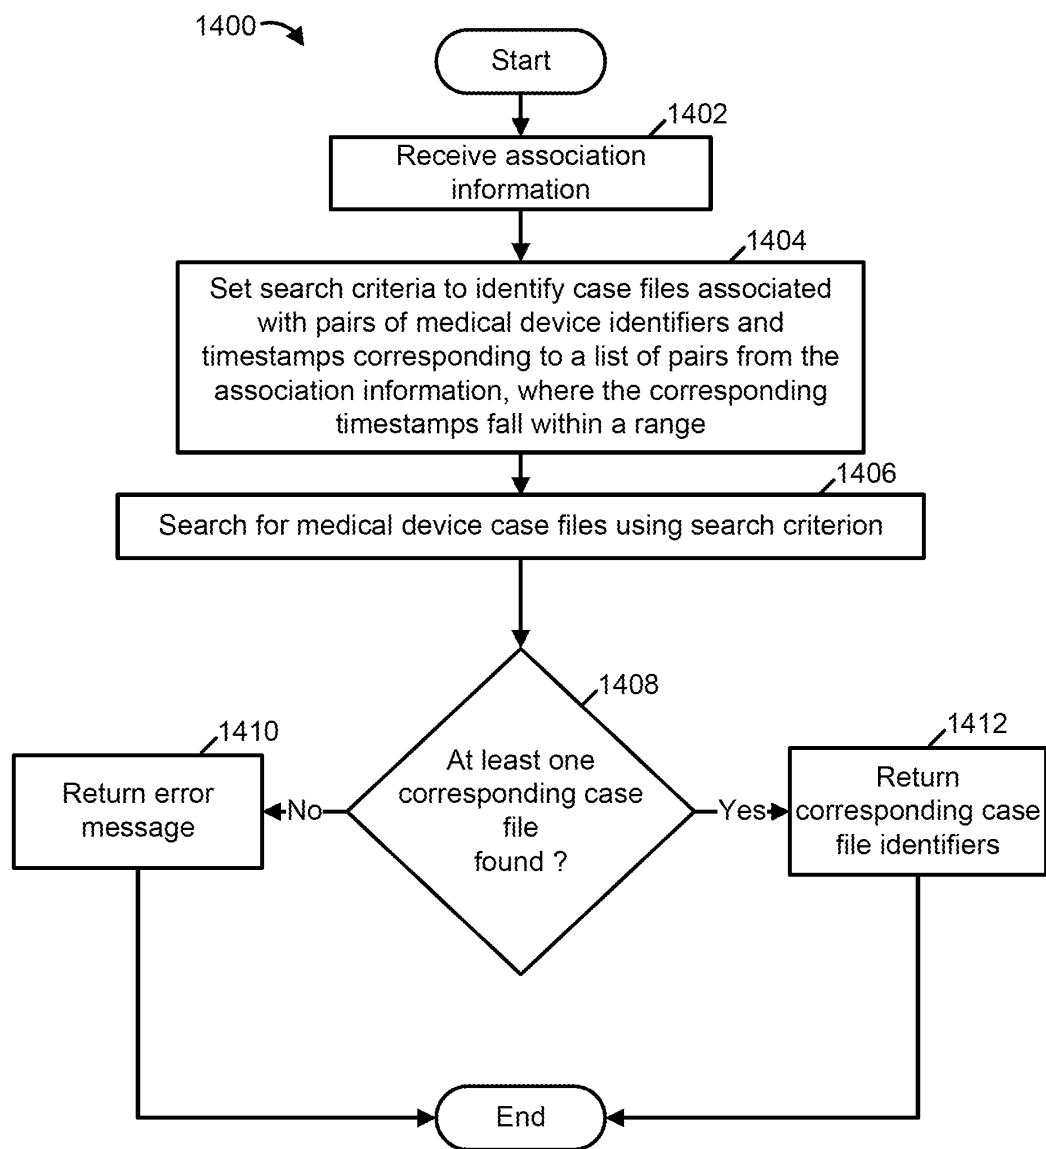


FIG. 14

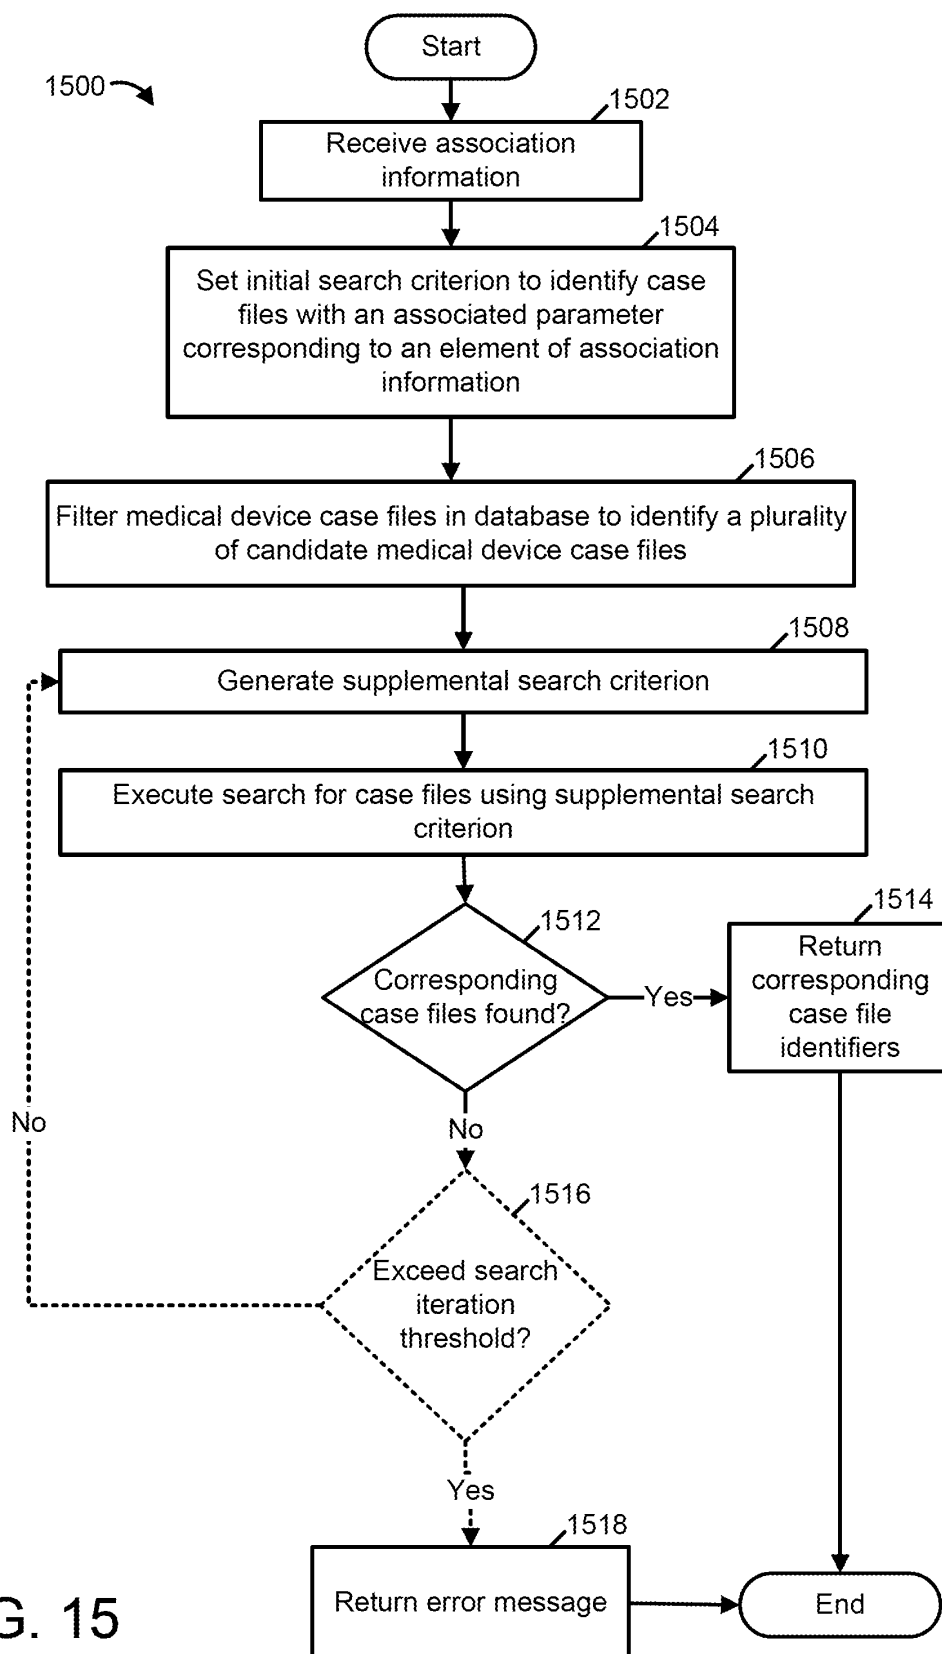


FIG. 15

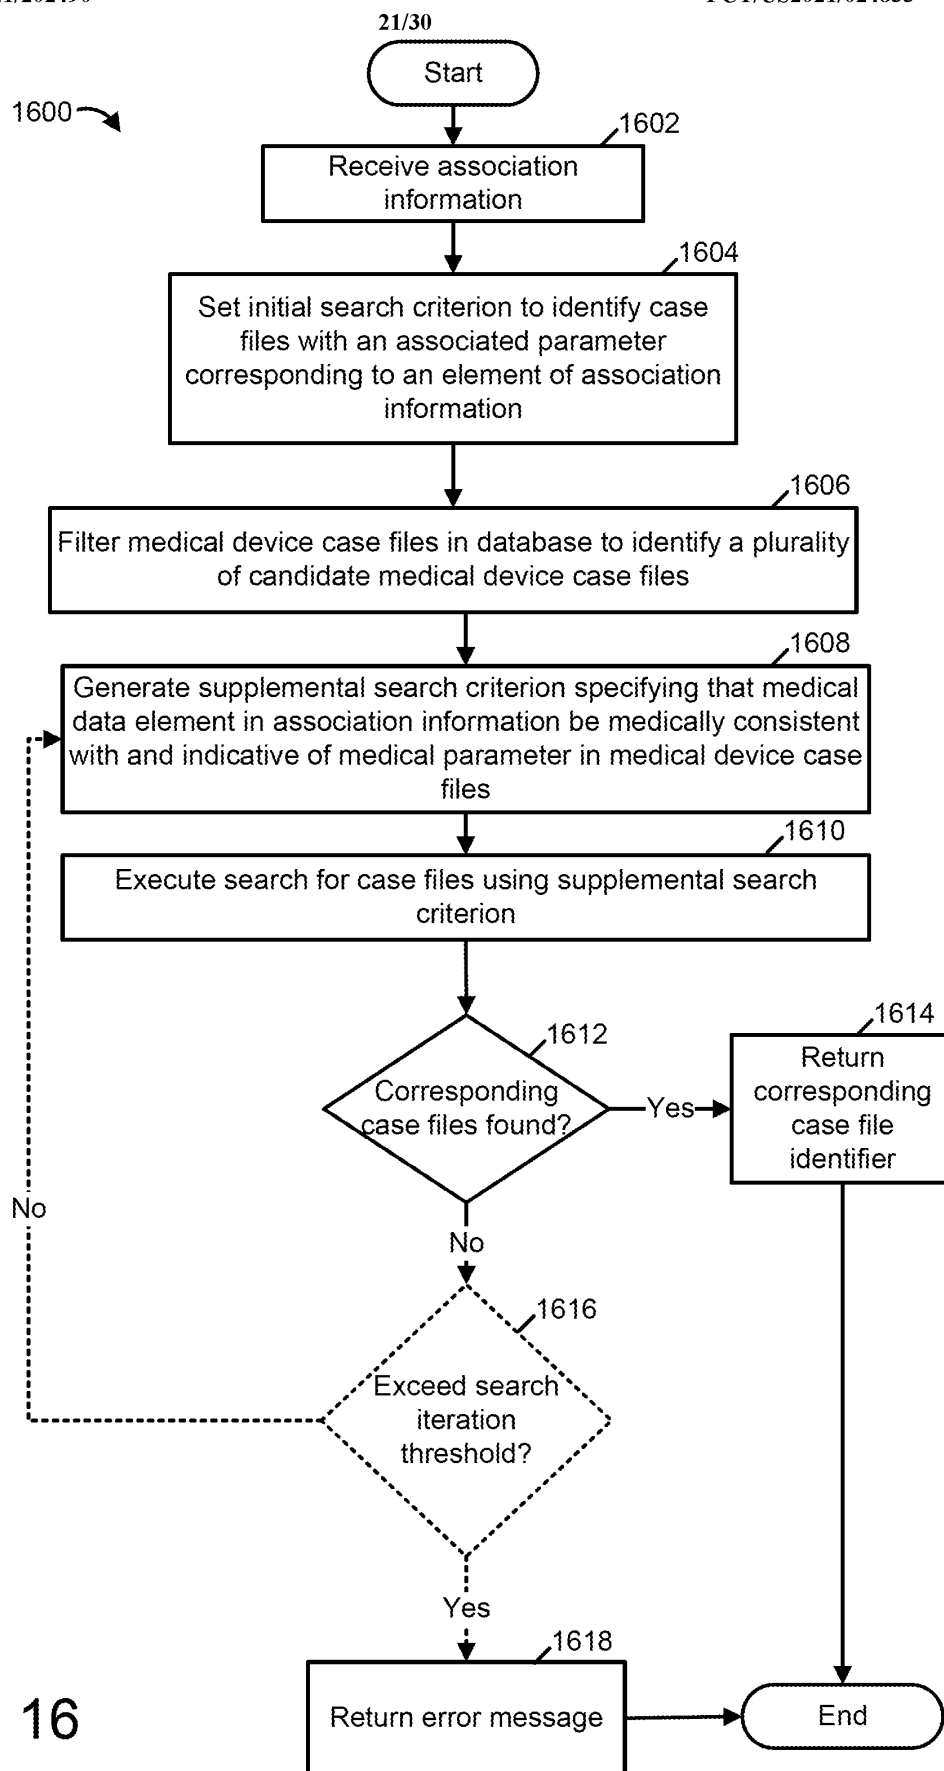


FIG. 16

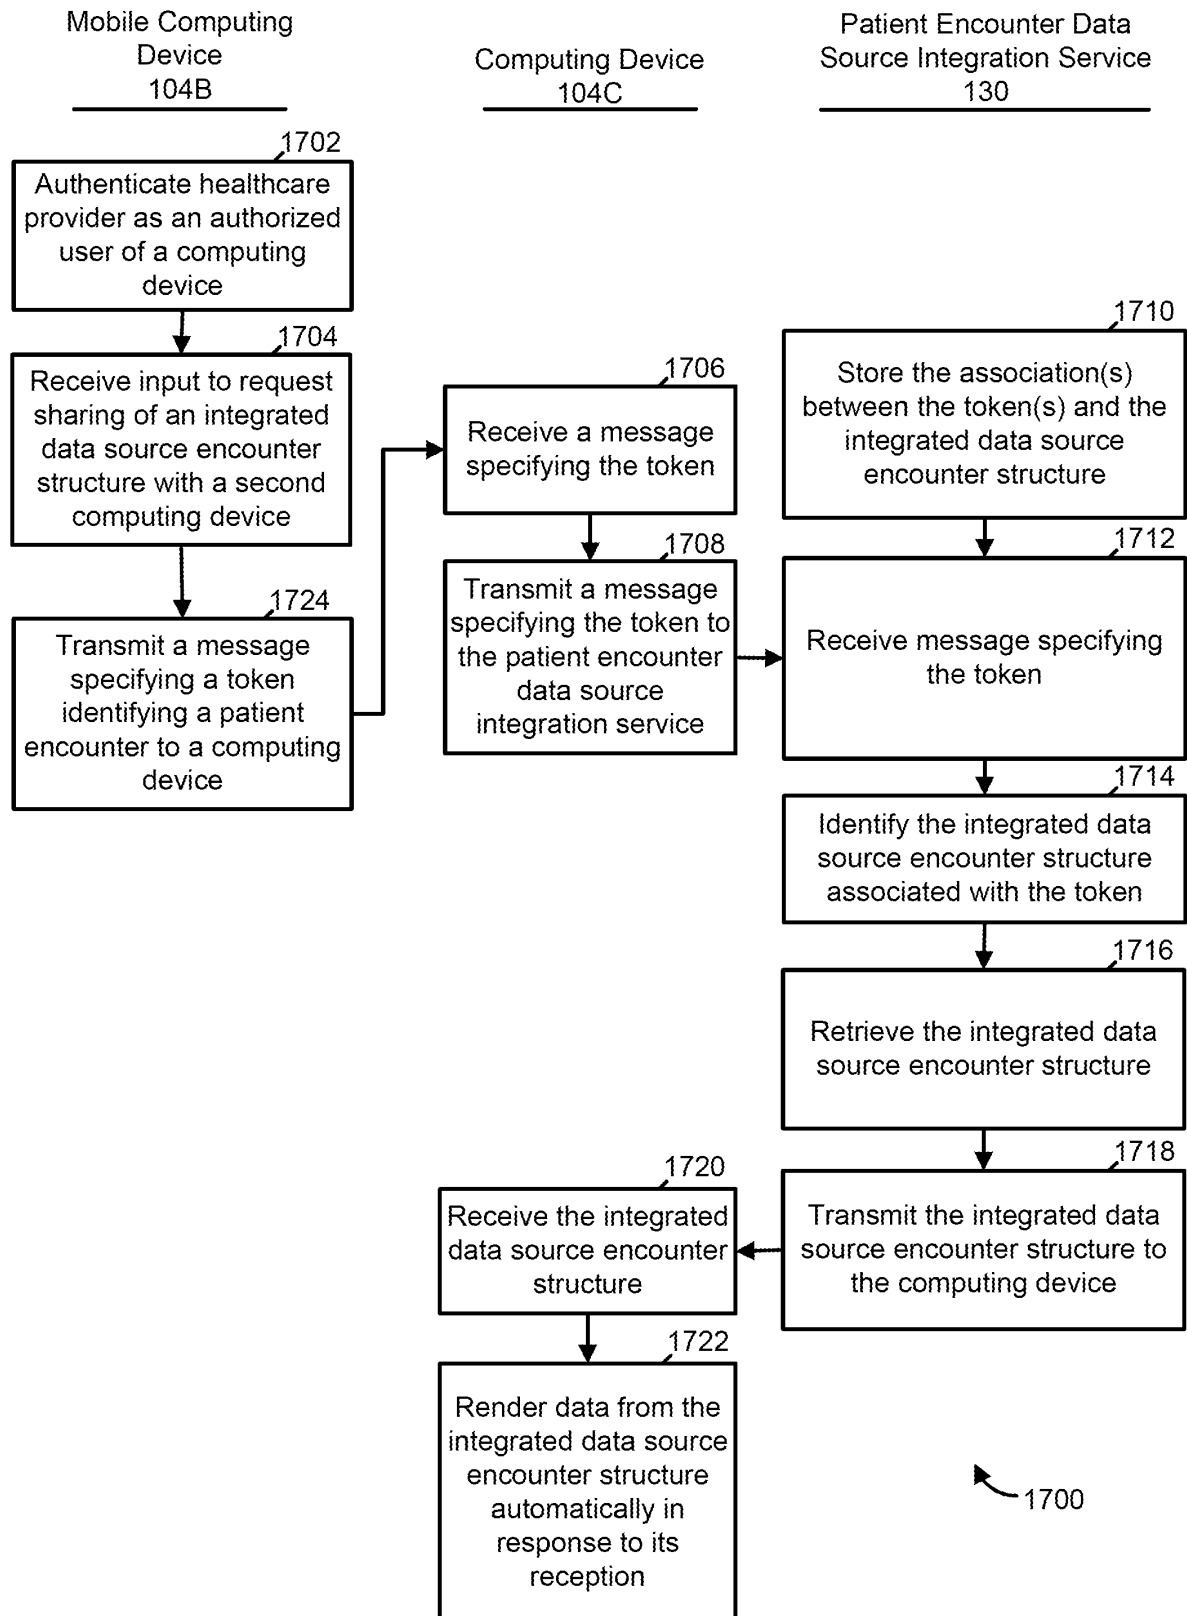


FIG. 17

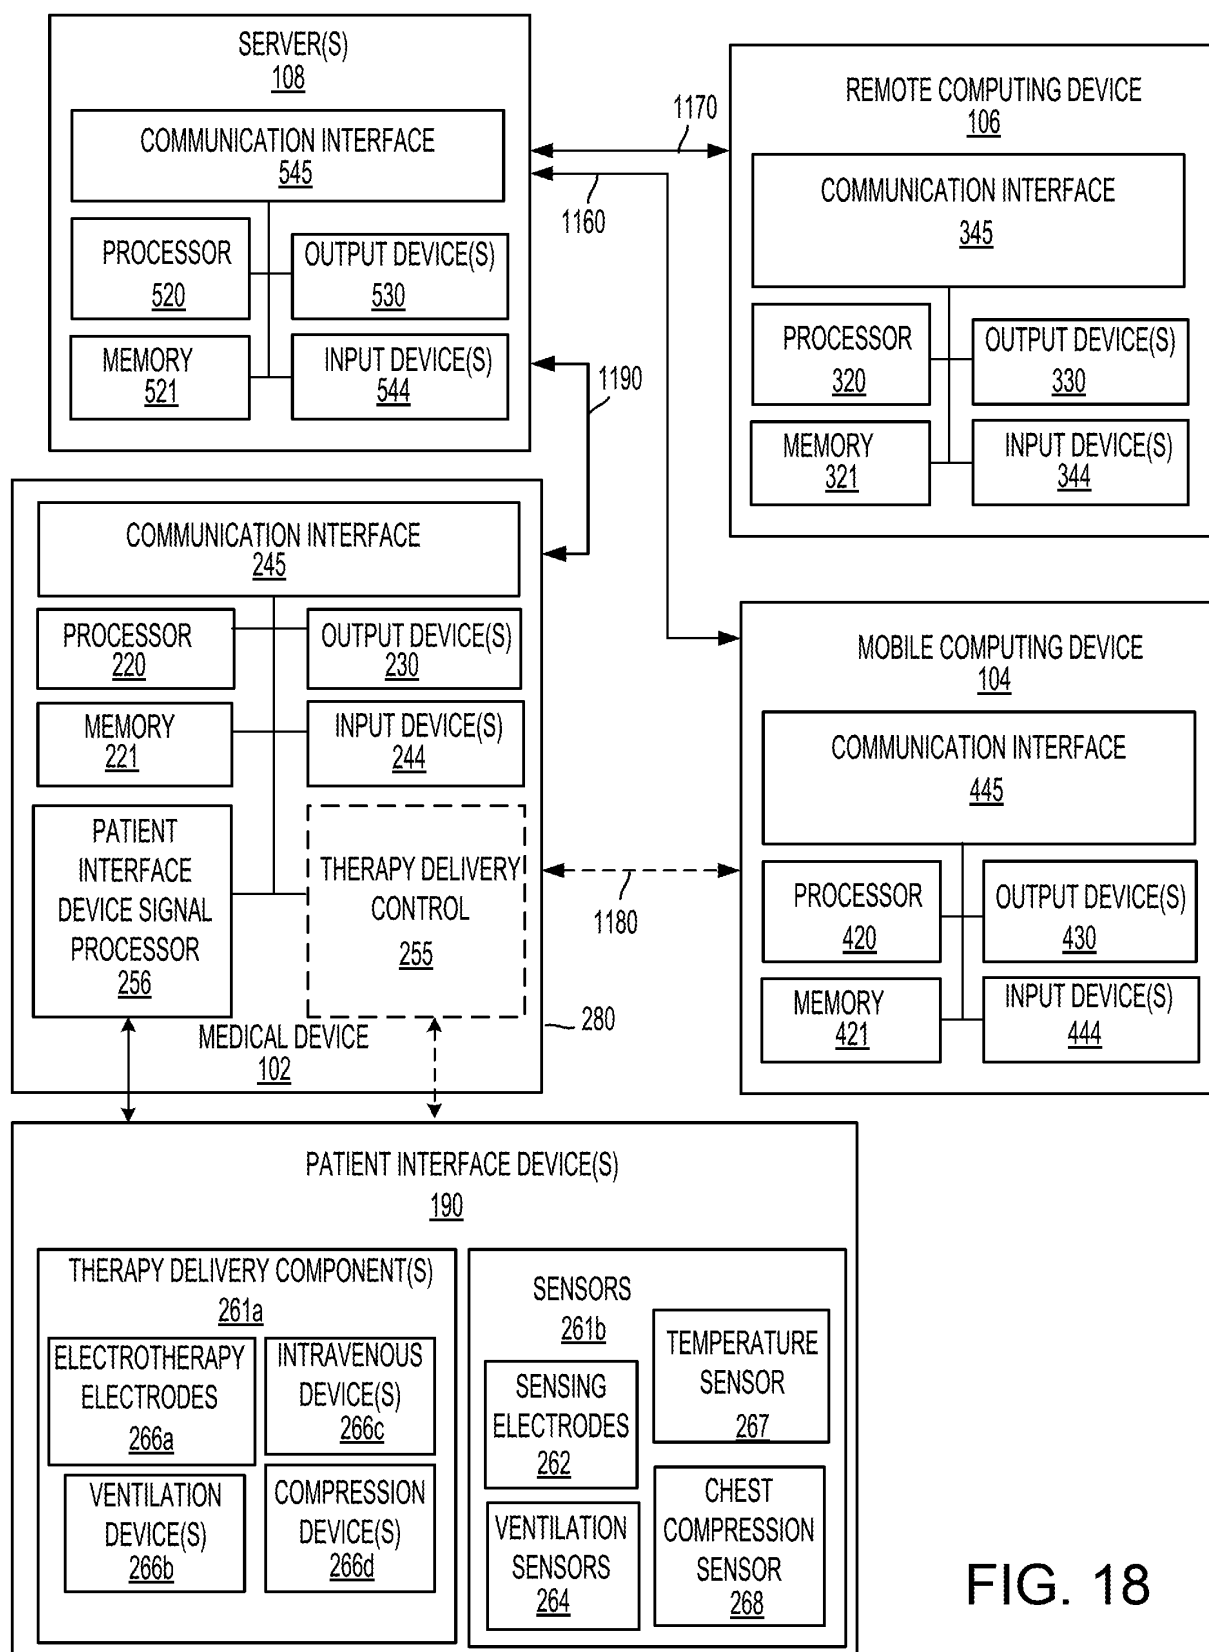


FIG. 18

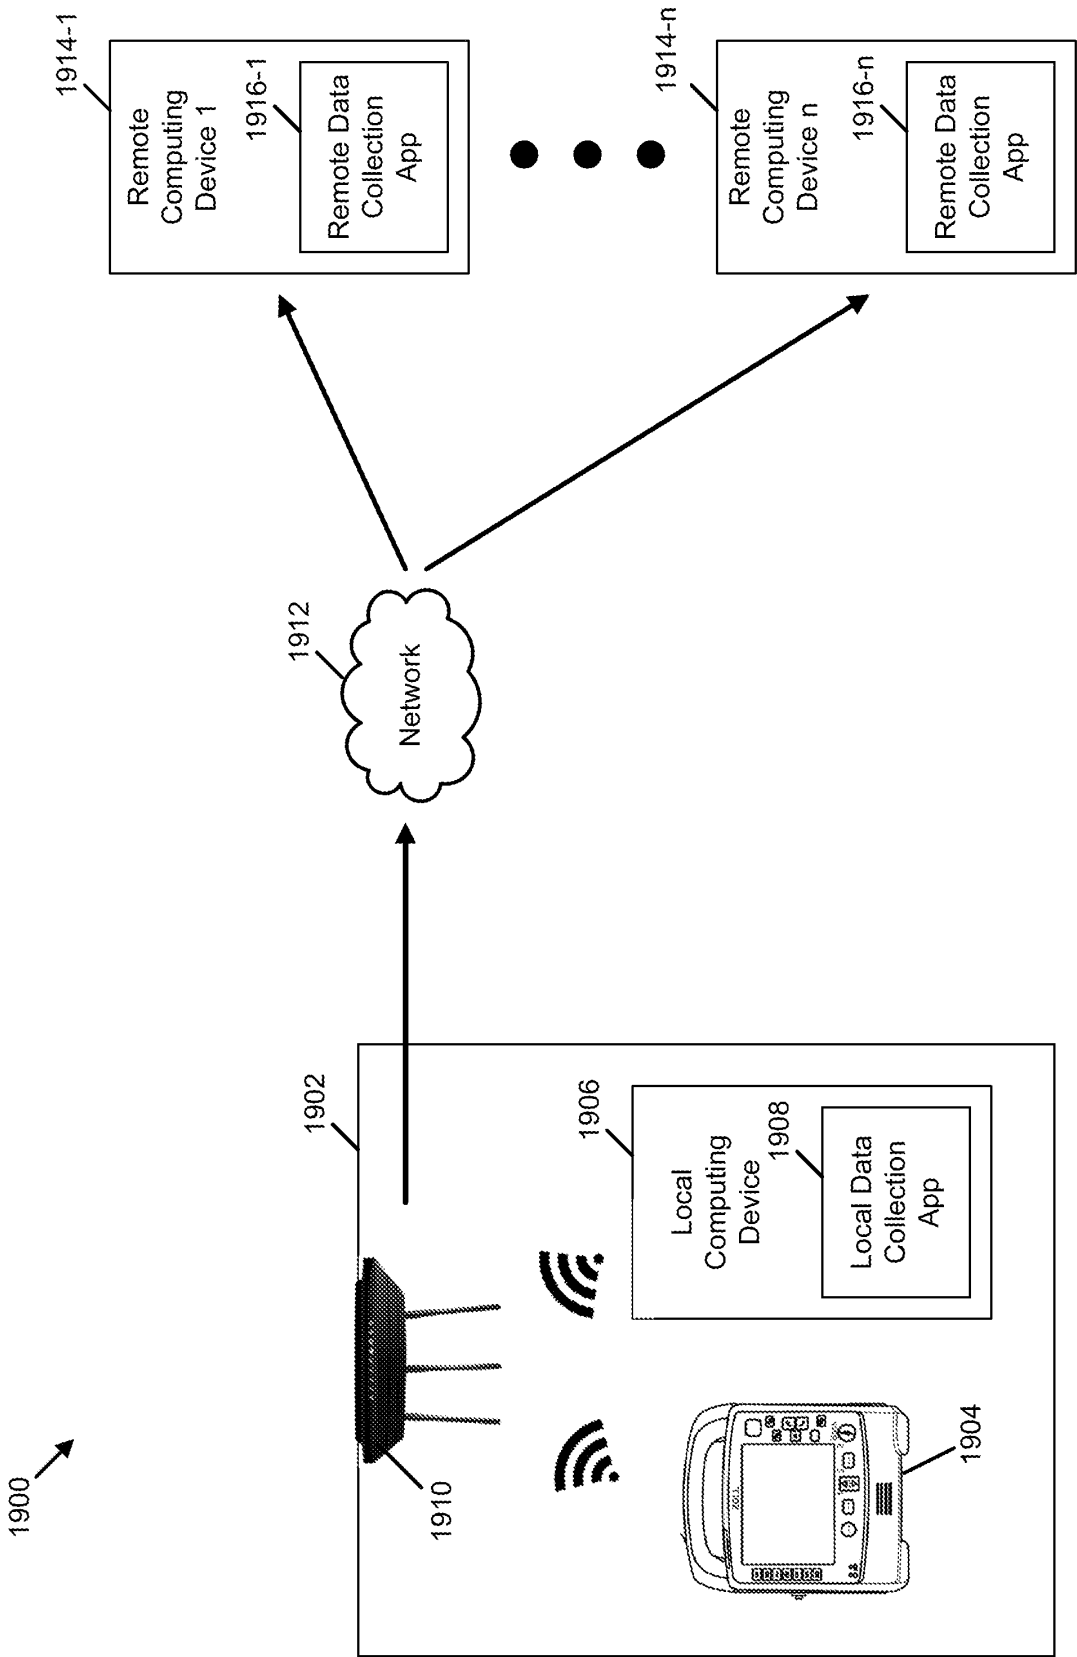


FIG. 19

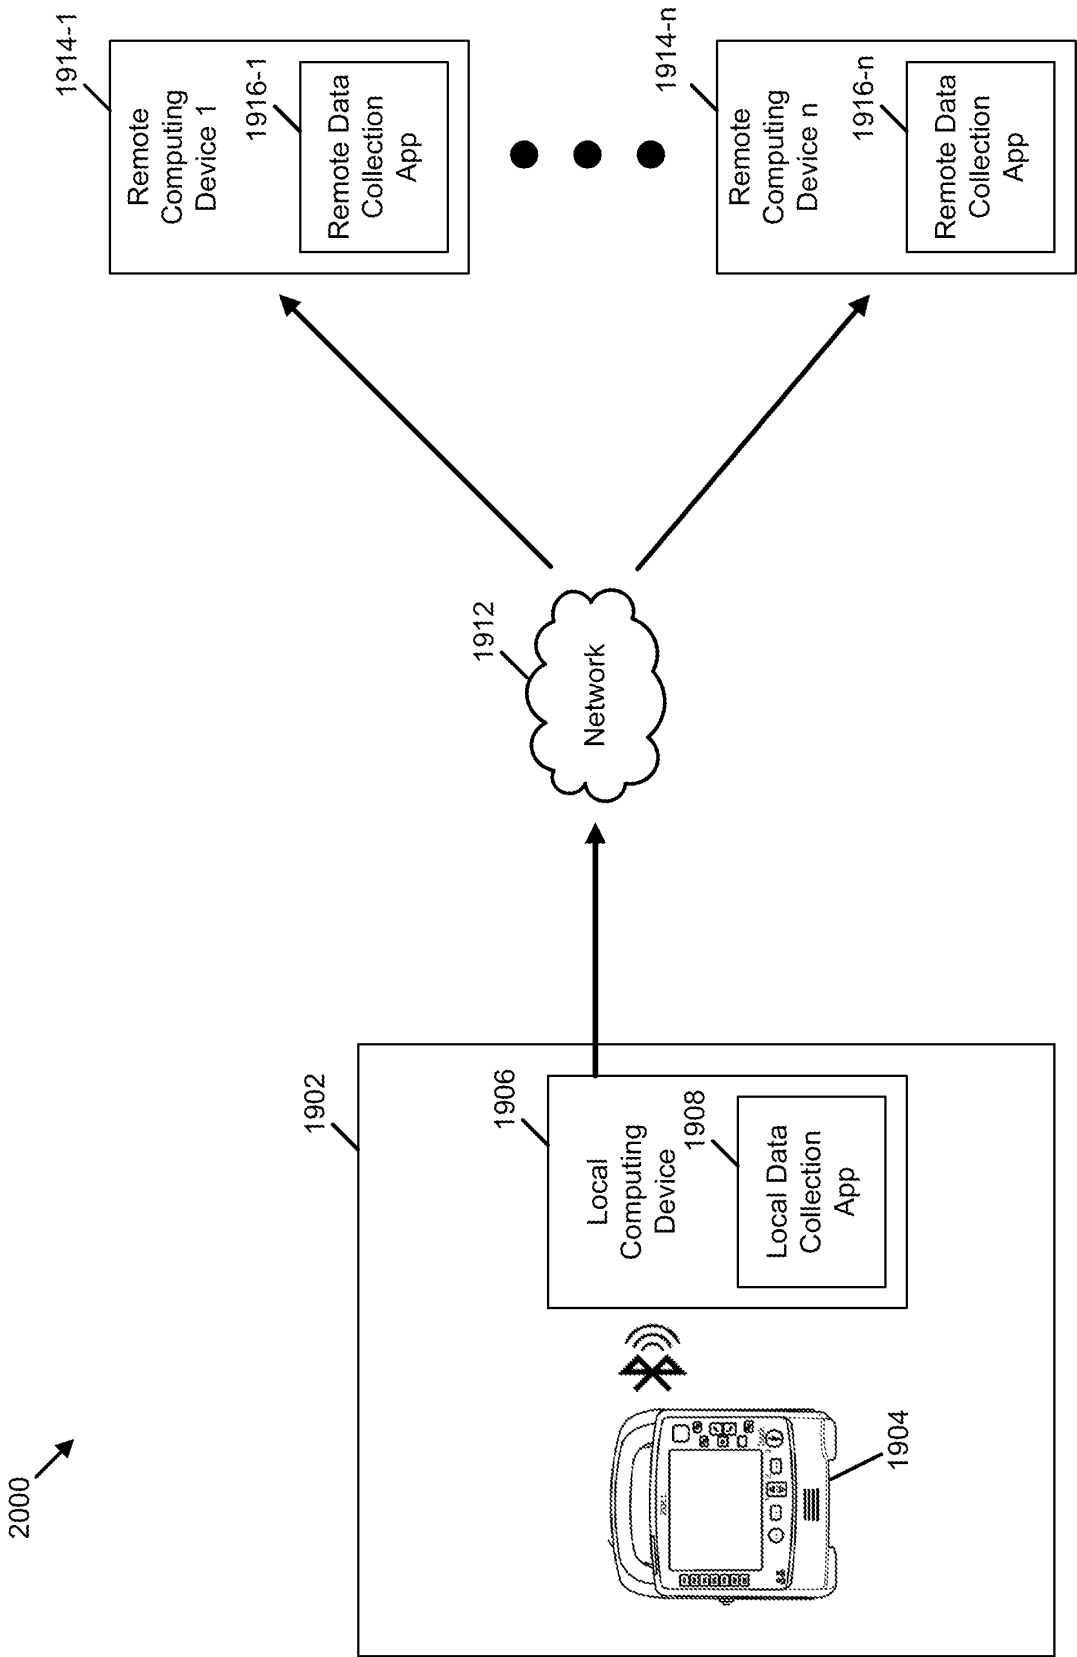


FIG. 20

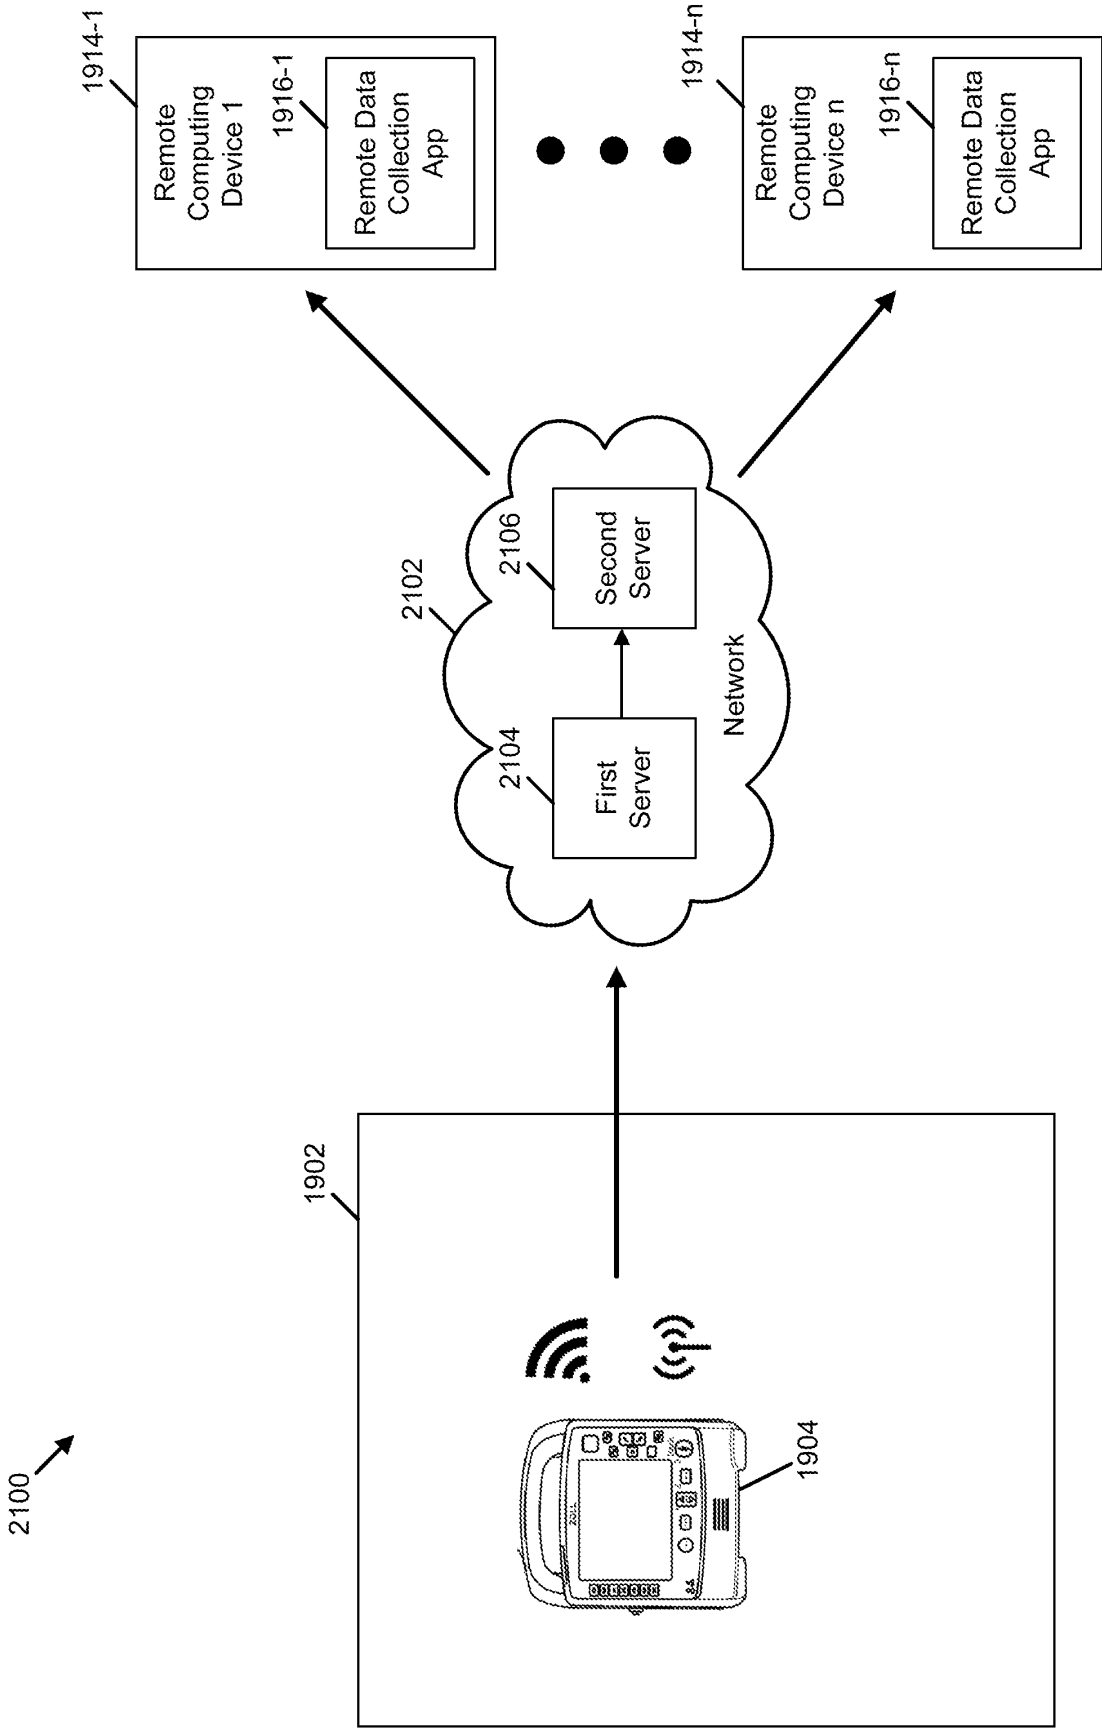


FIG. 21

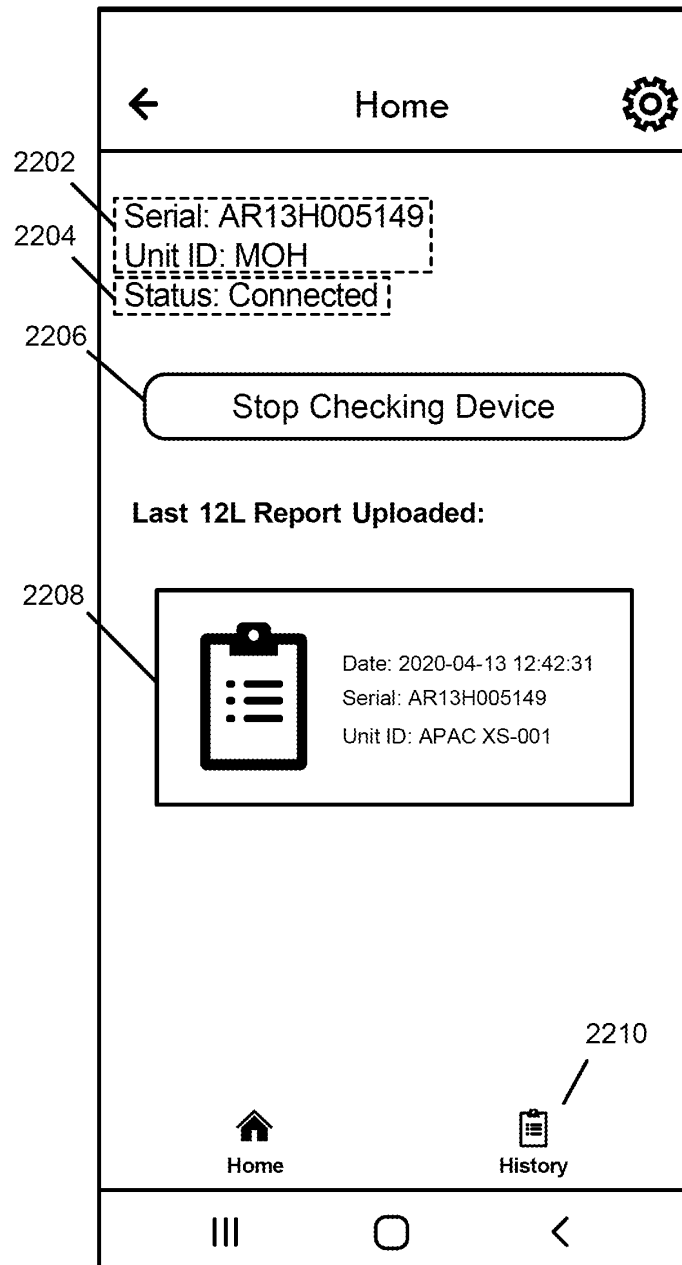
2200  
↓

FIG. 22

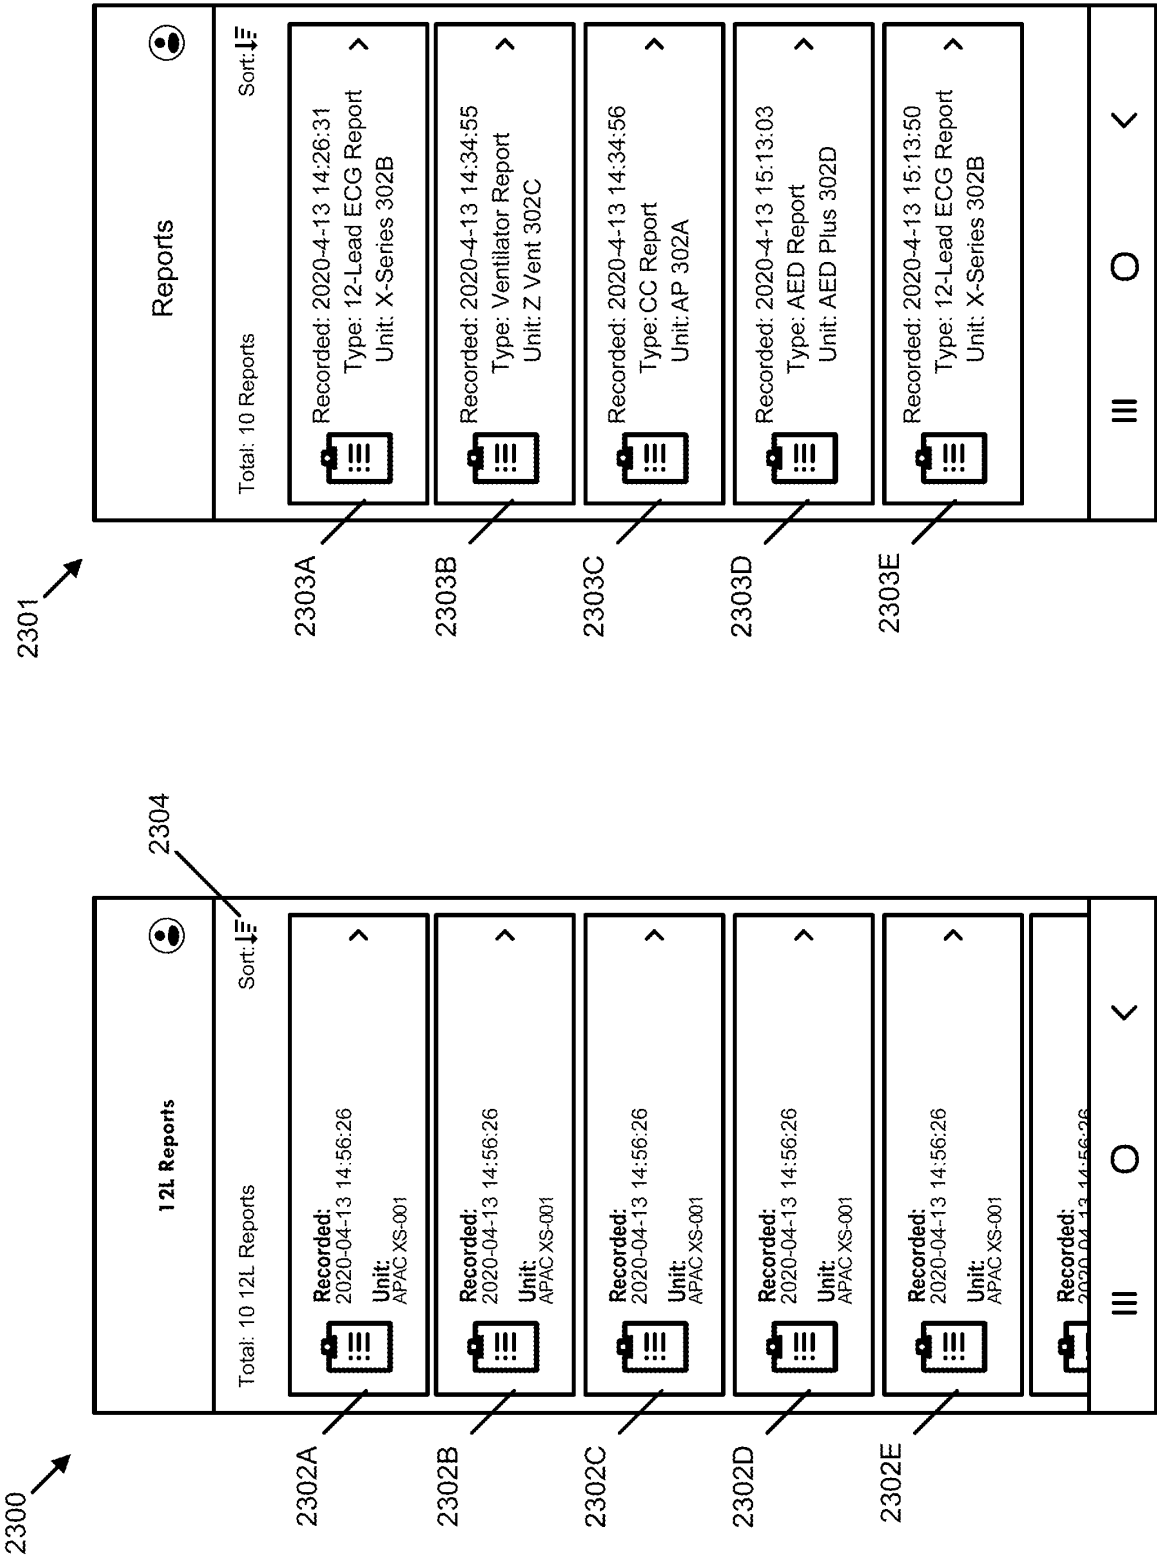


FIG. 23A

FIG. 23B

2400 ↗

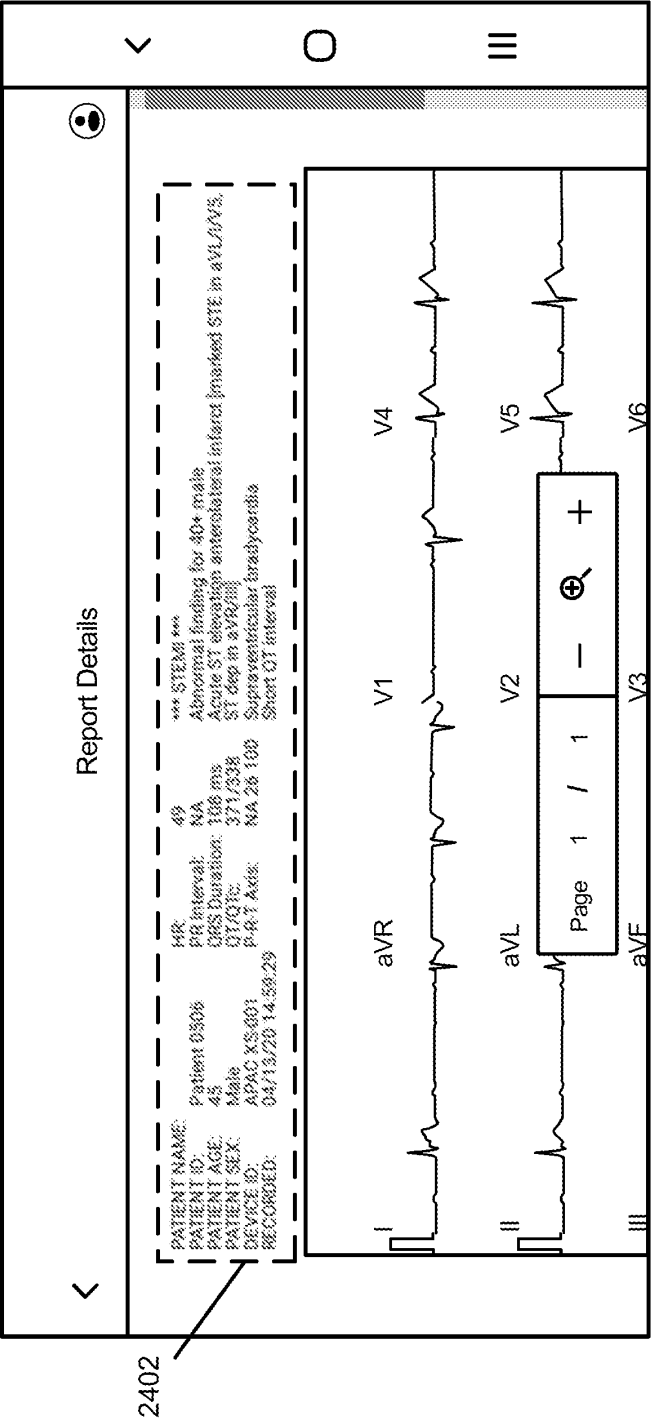


FIG. 24

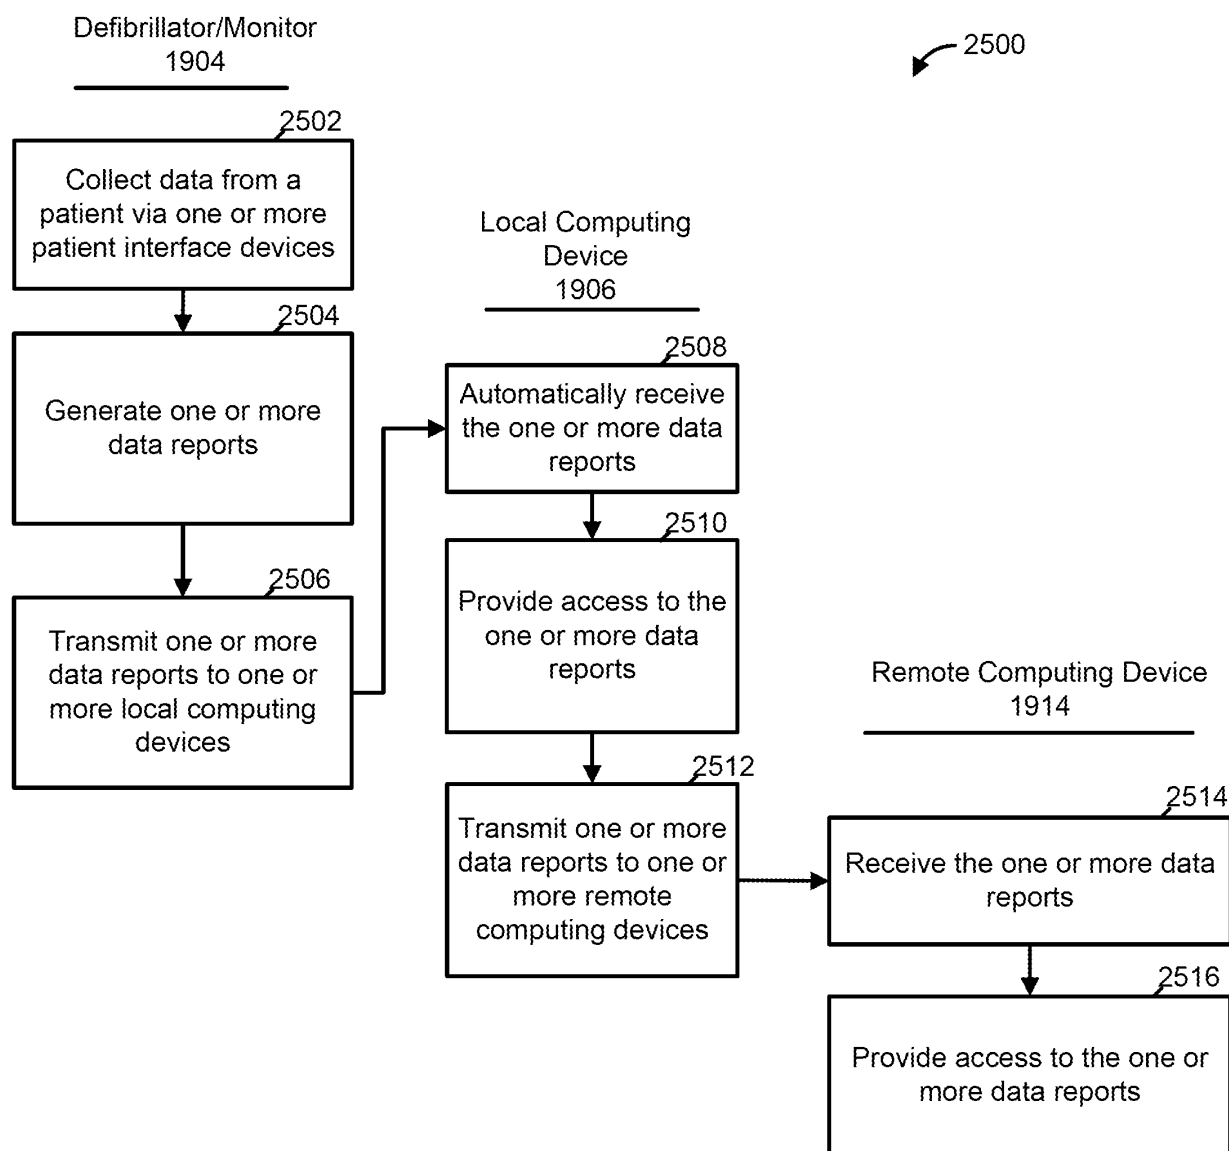


FIG. 25