

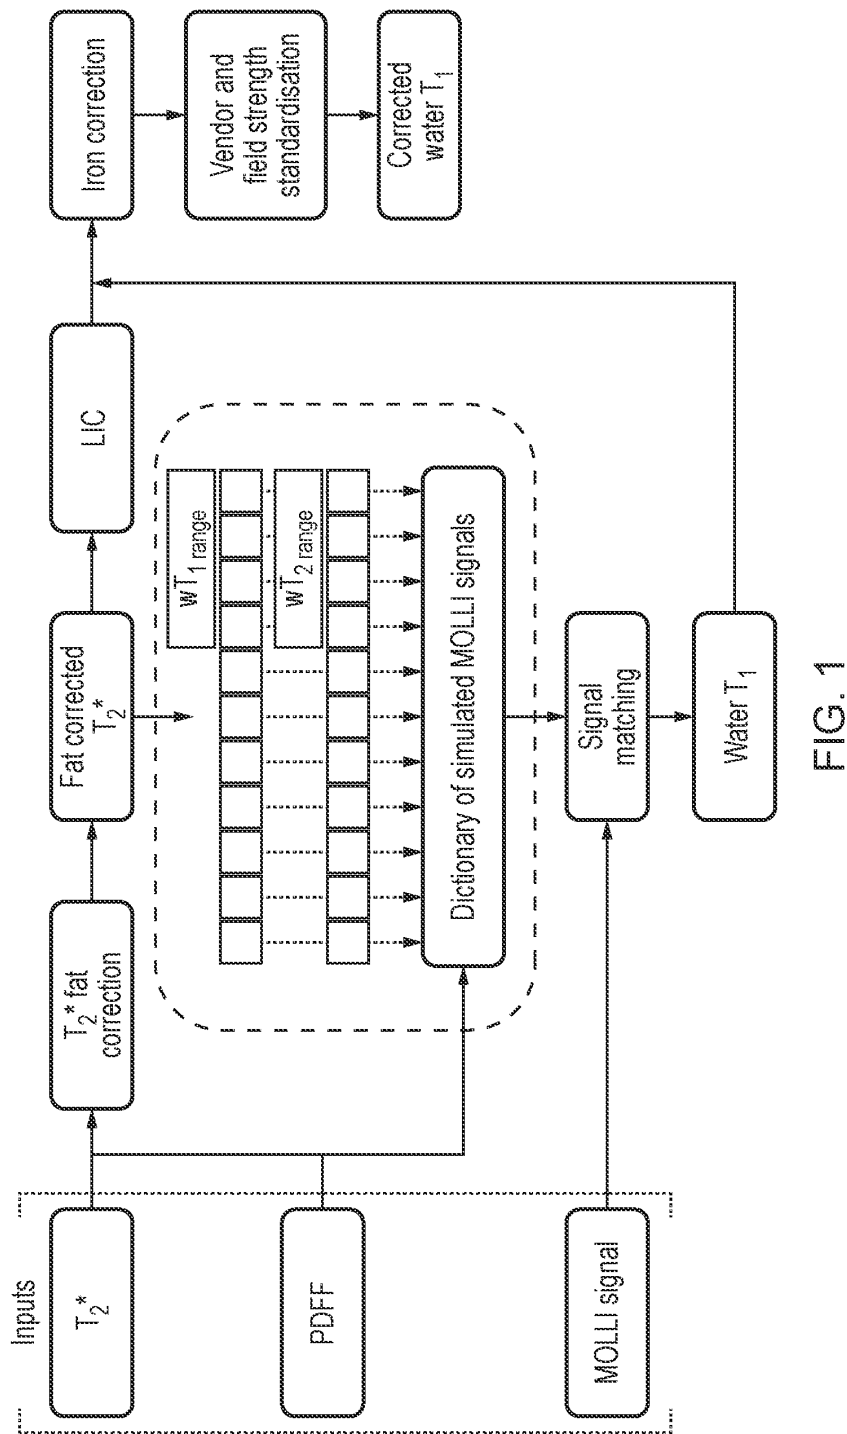


FIG. 1

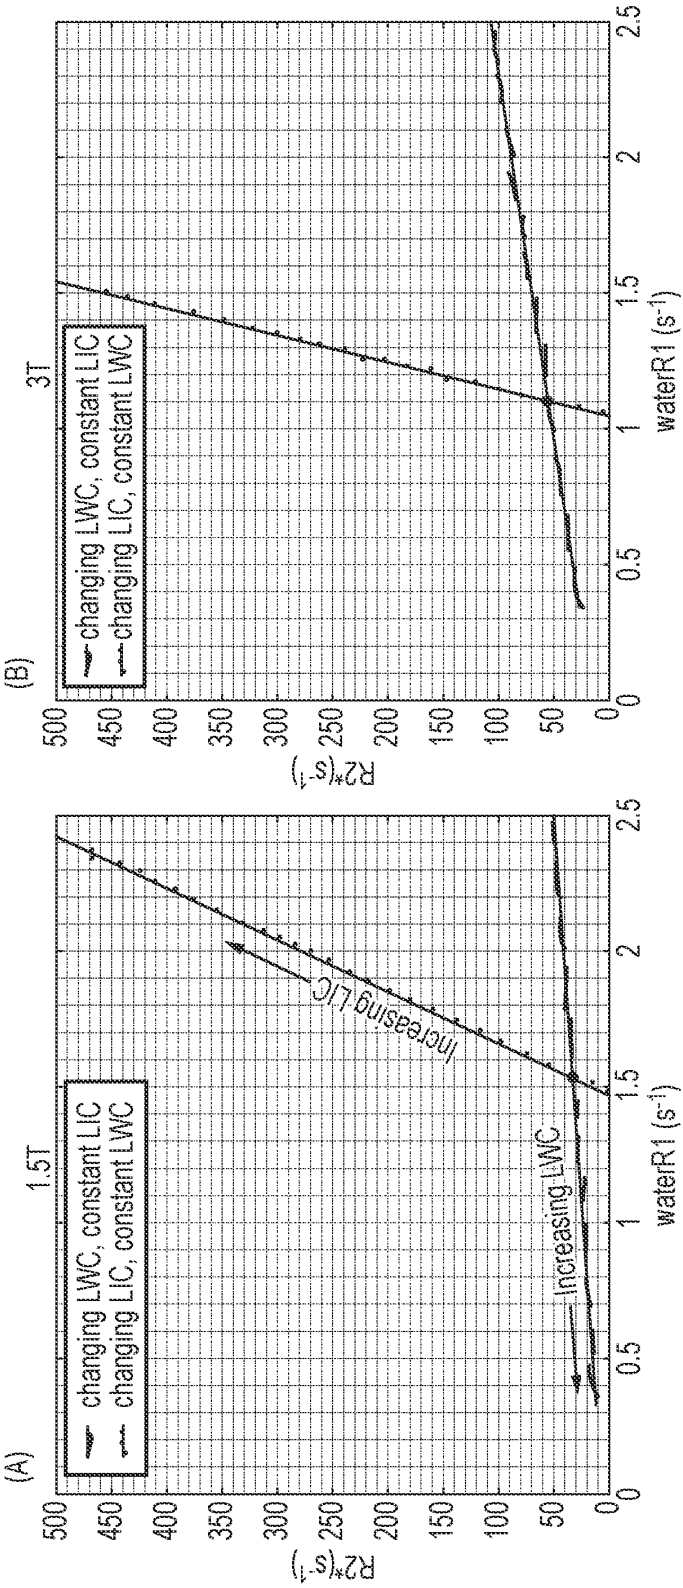


FIG. 2

3/4

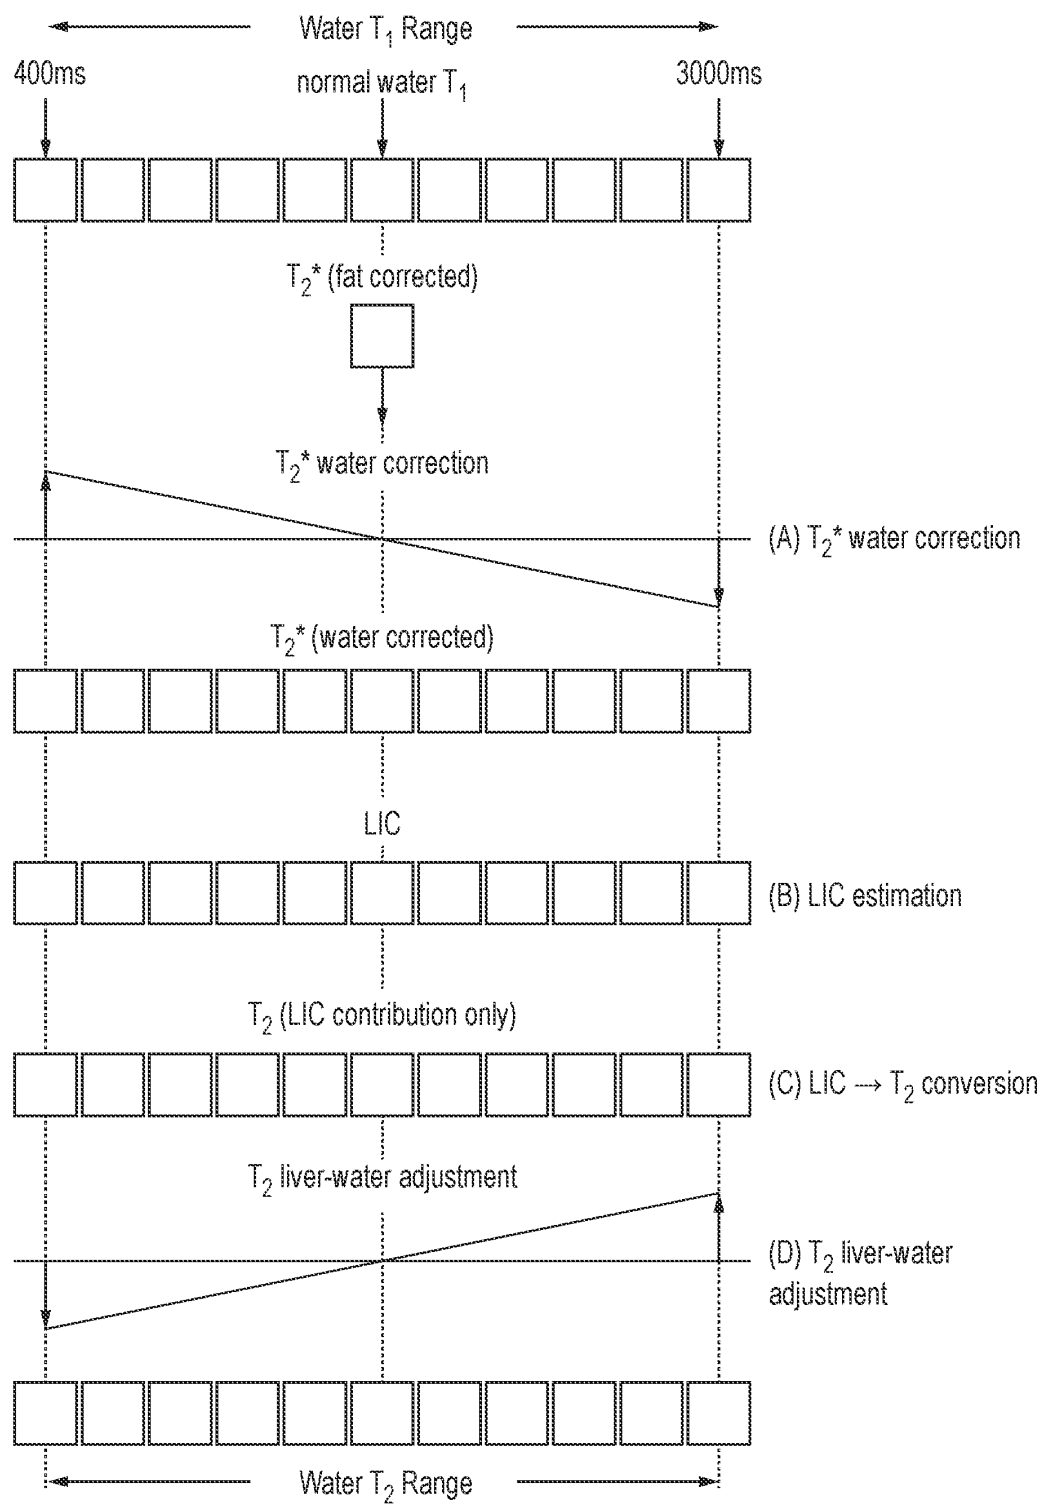


FIG. 3

SUBSTITUTE SHEET (RULE 26)

Scanner	$\Delta wT_{1\text{vendor}}$
Siemens 3T	0ms
Siemens 1.5T	5.2ms
GE 3T	-16.5ms
GE 1.5T	-76.2ms
Philips 3T	-54.7ms
Philips 1.5T	-69.3ms

Table 1 Values for the vendor-specific water T_1 correction terms ($\Delta wT_{1\text{vendor}}$).

FIG. 4