

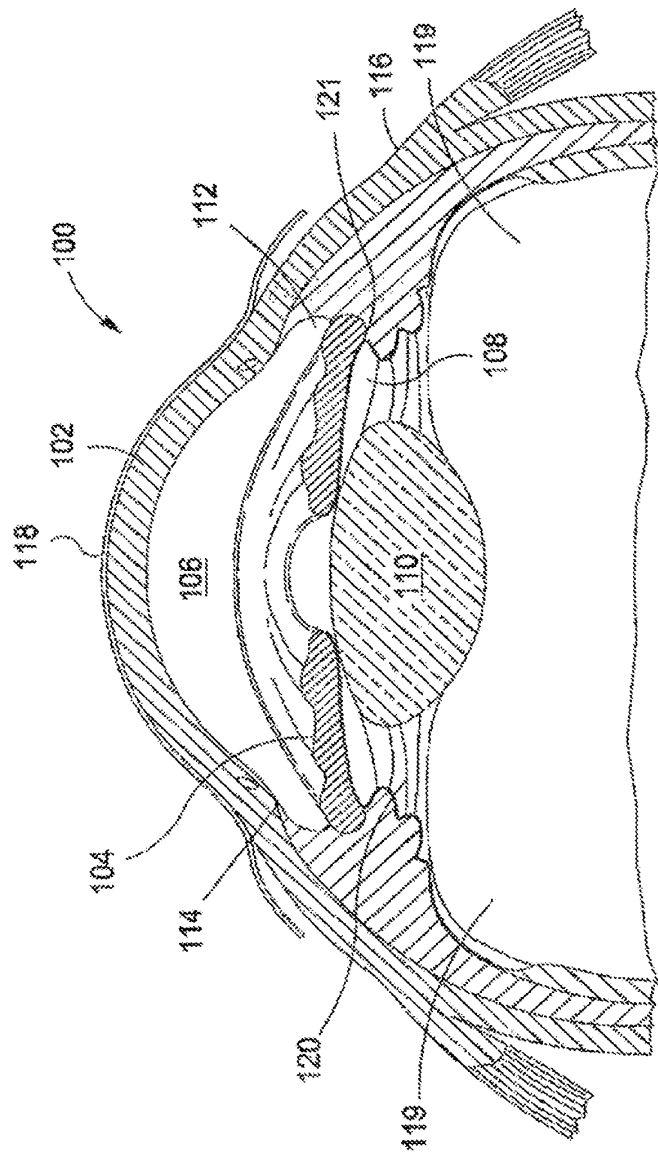


FIG. 1

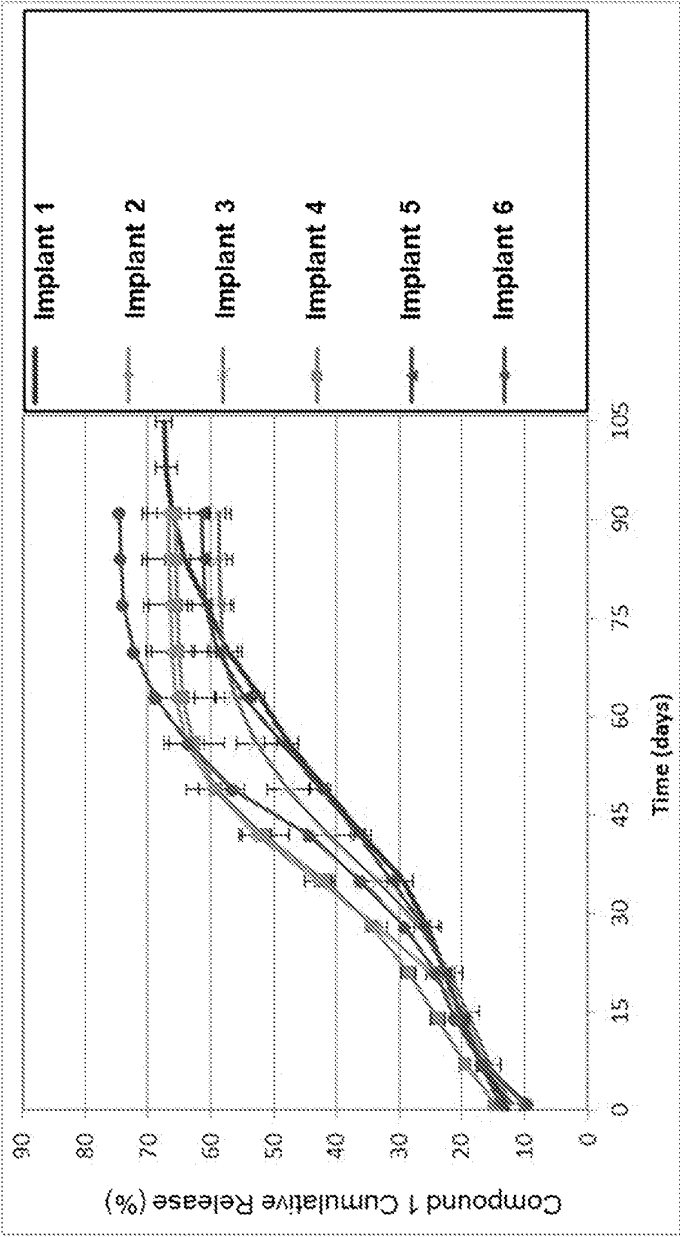


FIG. 2

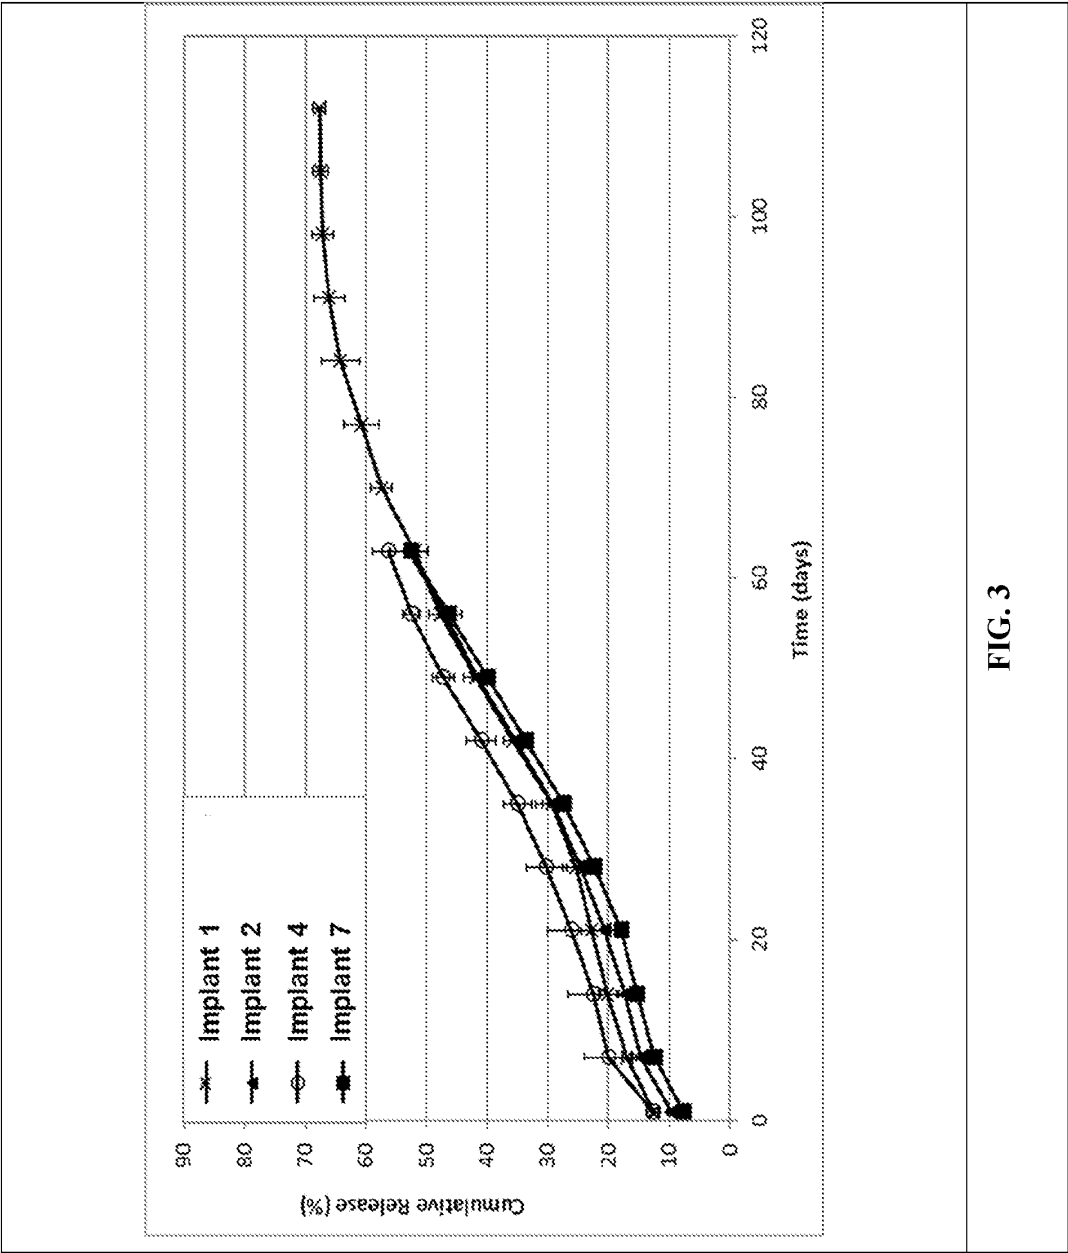


FIG. 3

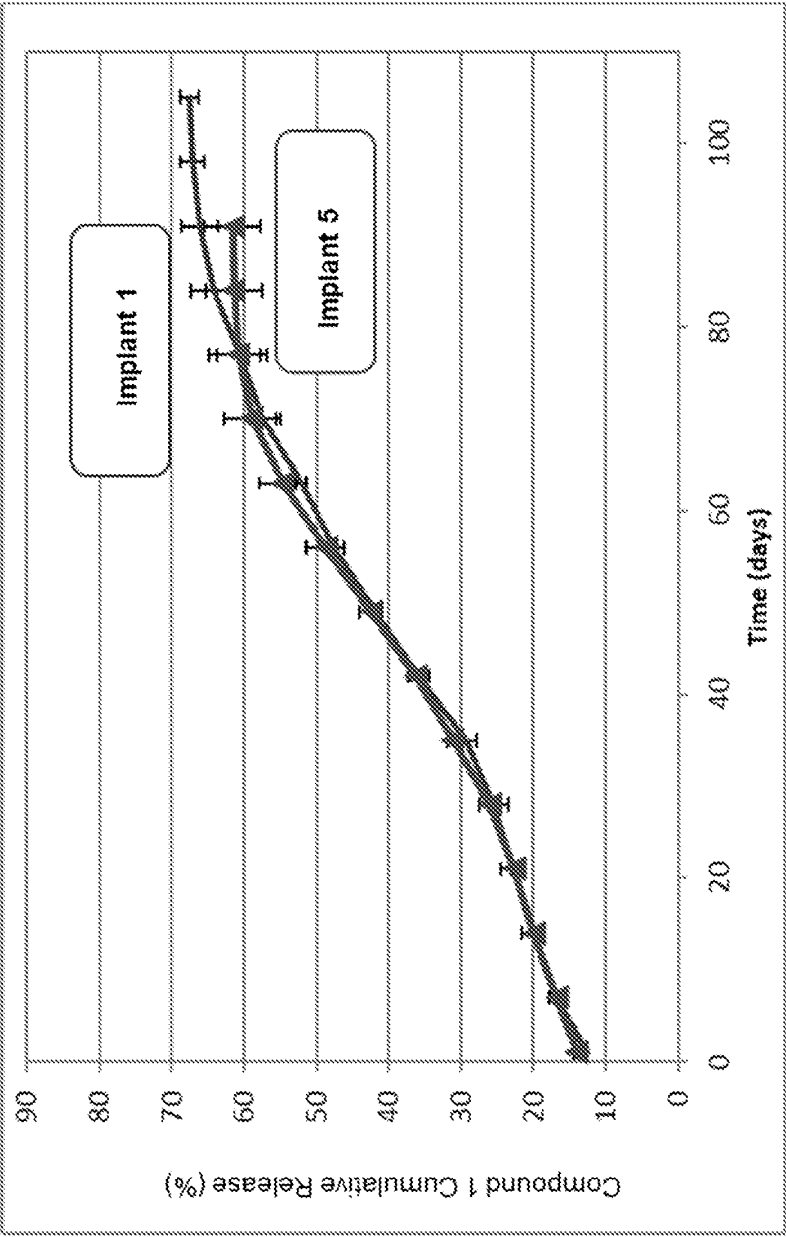


FIG. 4

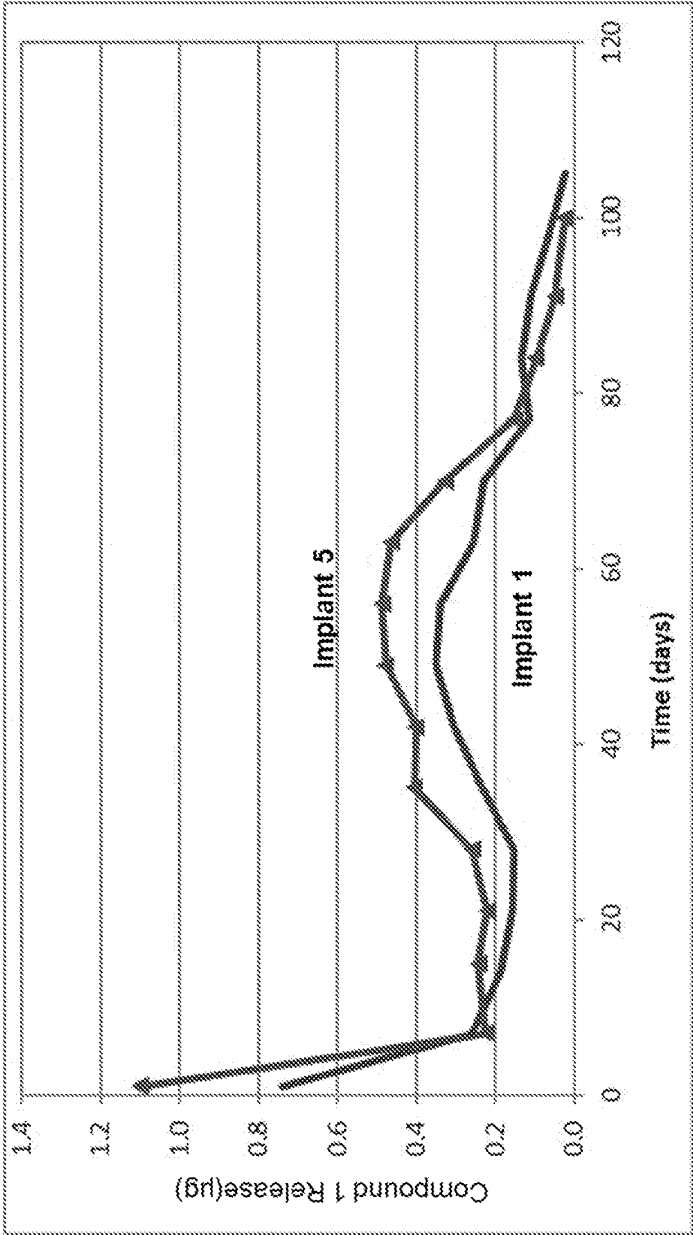


FIG. 5

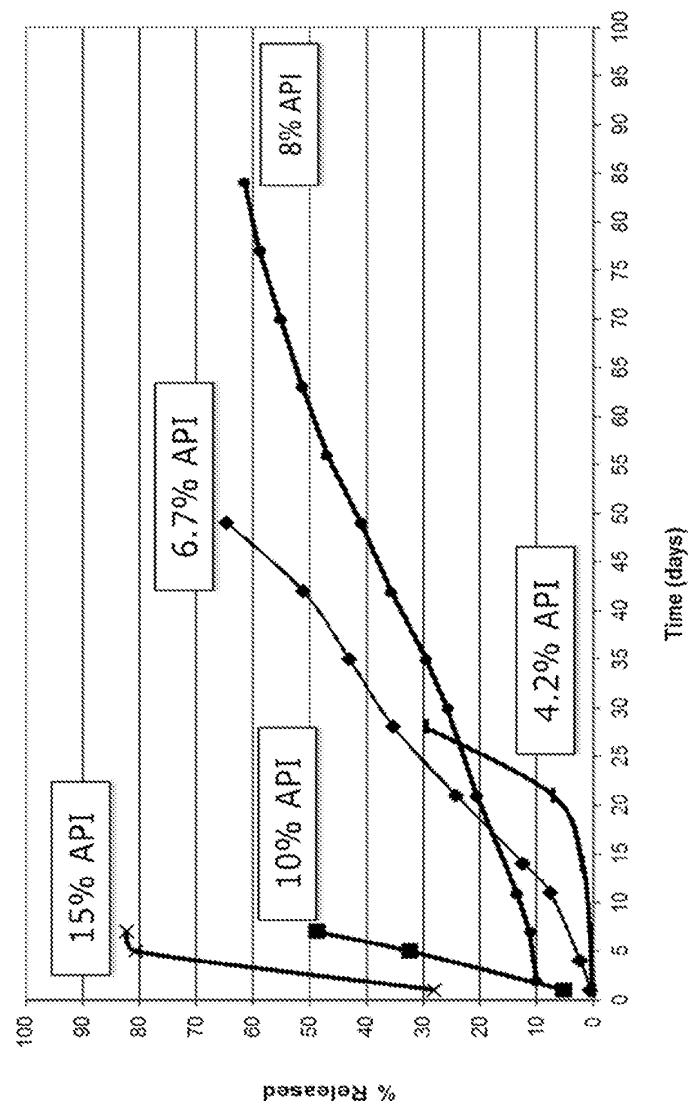


FIG. 6











Timepoint	3.8 µg/150 µm dia.		7.5 µg /150 µm dia.	
	Implant 1		Implant 5	
Day 0				
Day 91				
Day 127				
Day 196				
Day 280				
Day 415			N/A	

FIG. 7

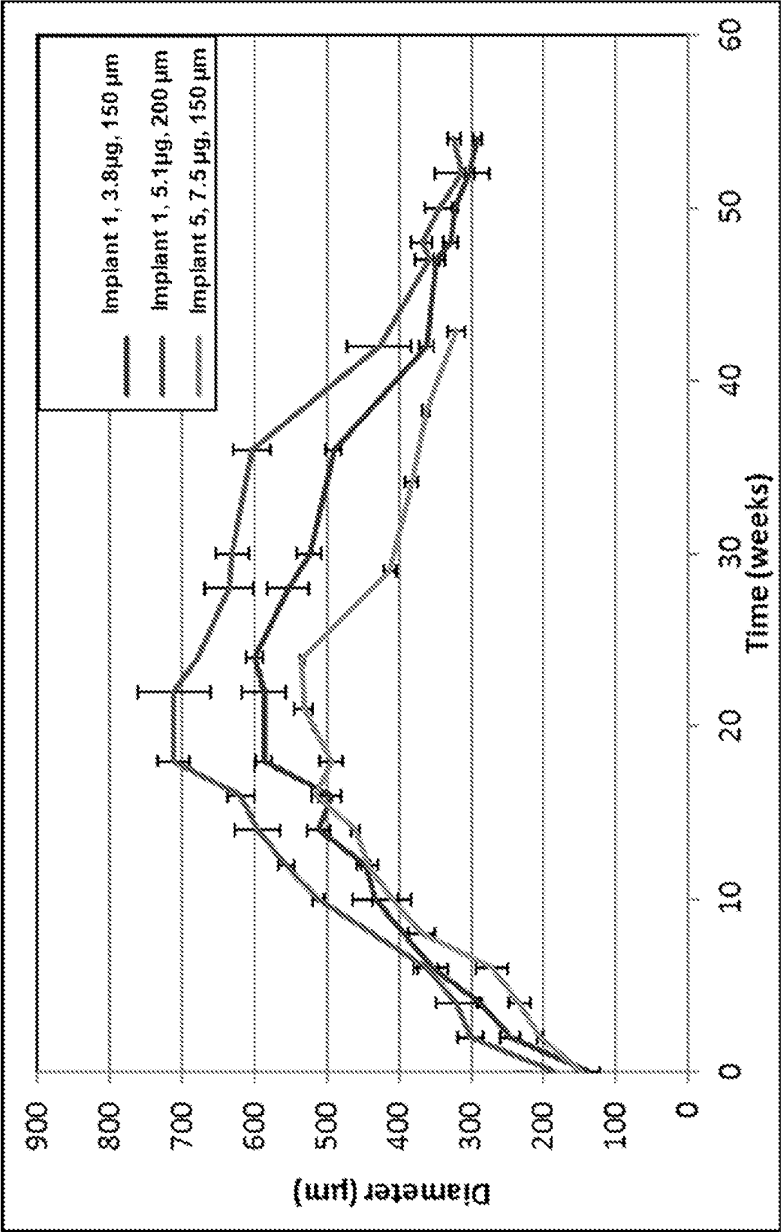


FIG. 8