

1 / 13

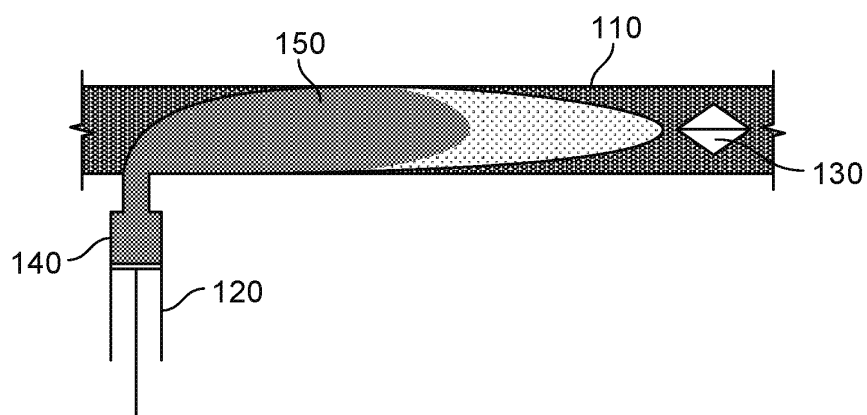


FIG. 1A

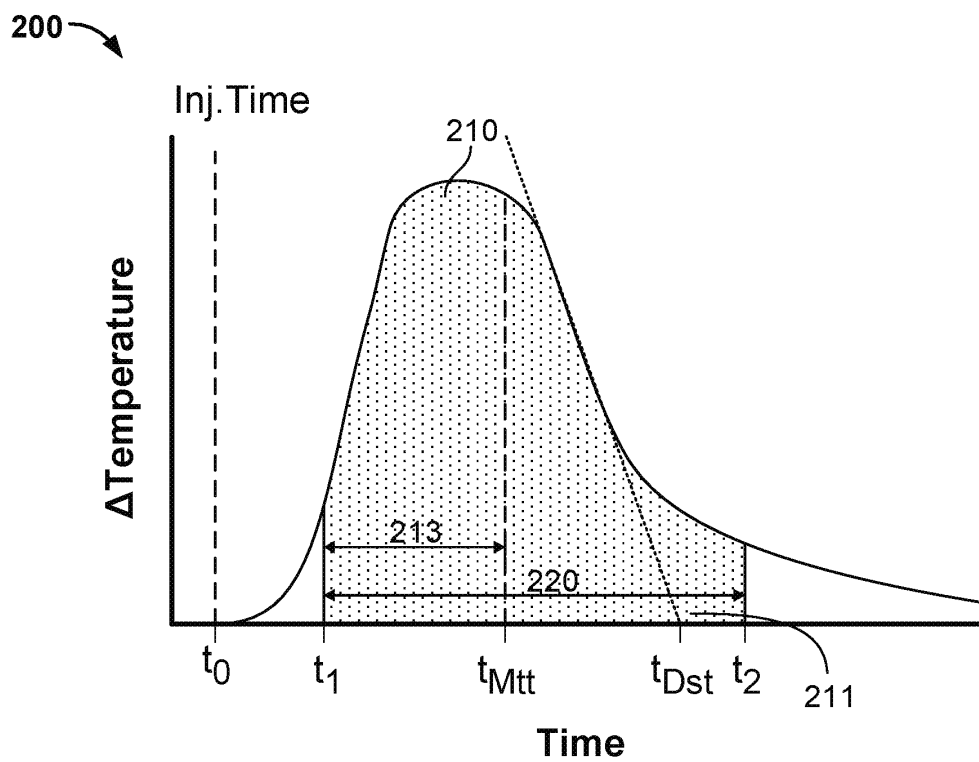


FIG. 1B

2 / 13

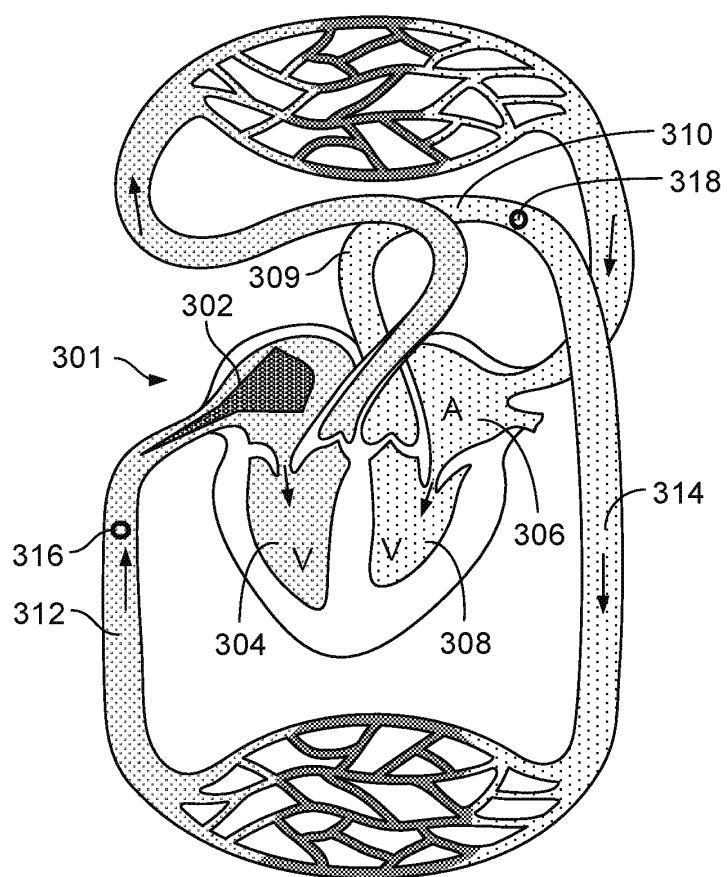


FIG. 2

405 →

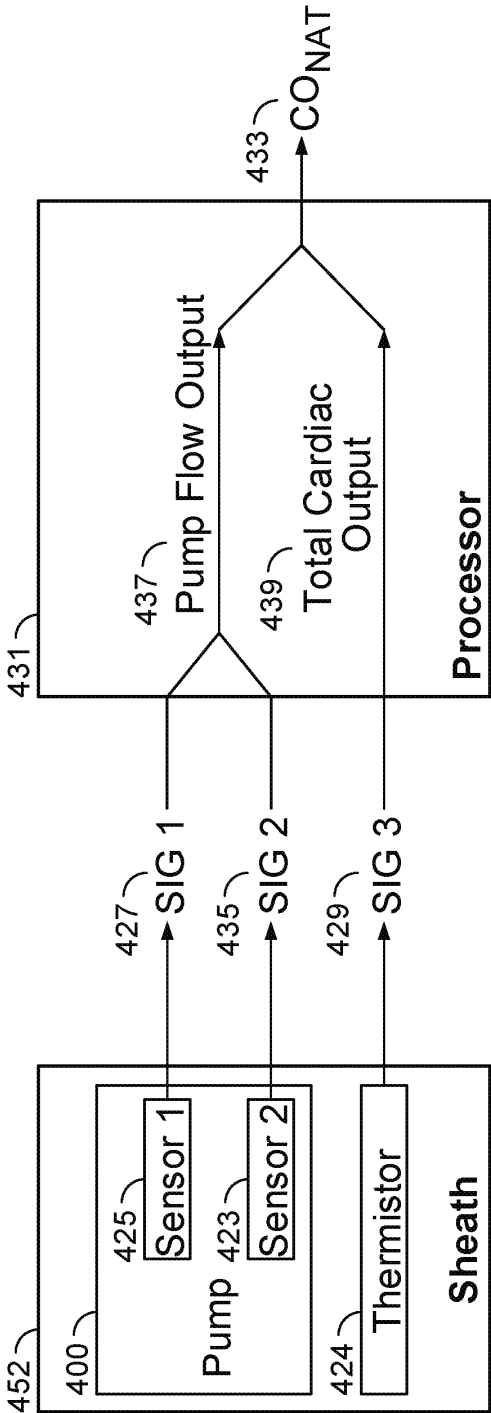
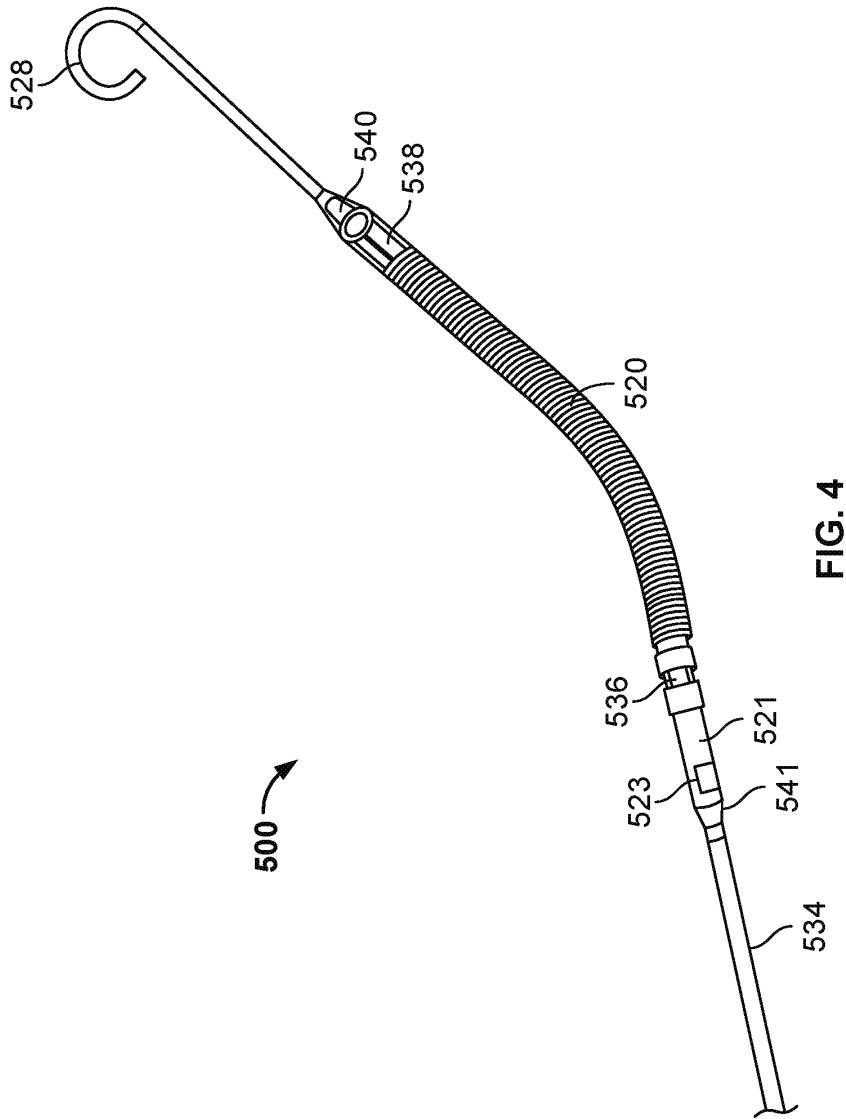


FIG. 3



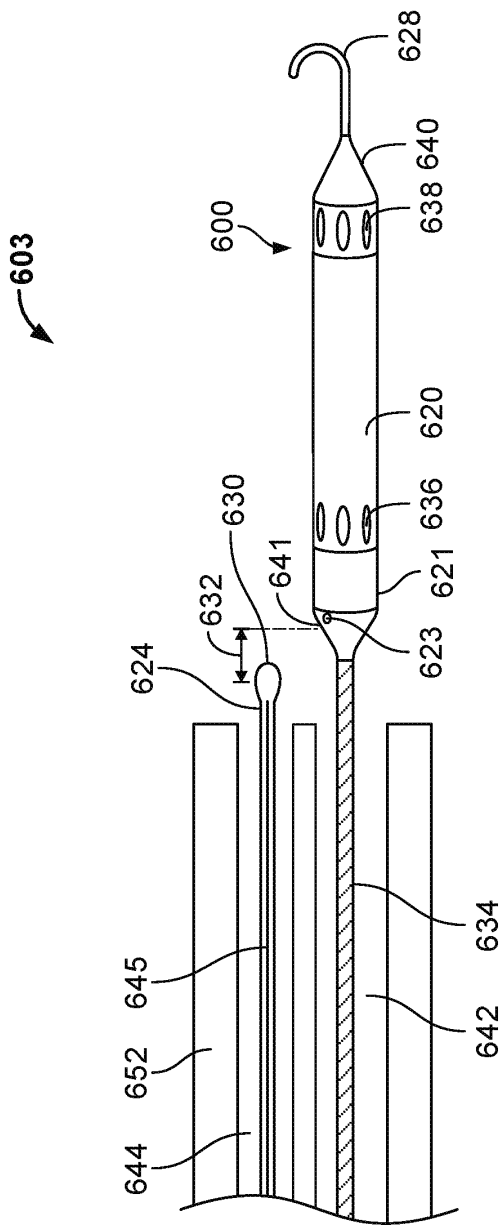


FIG. 5

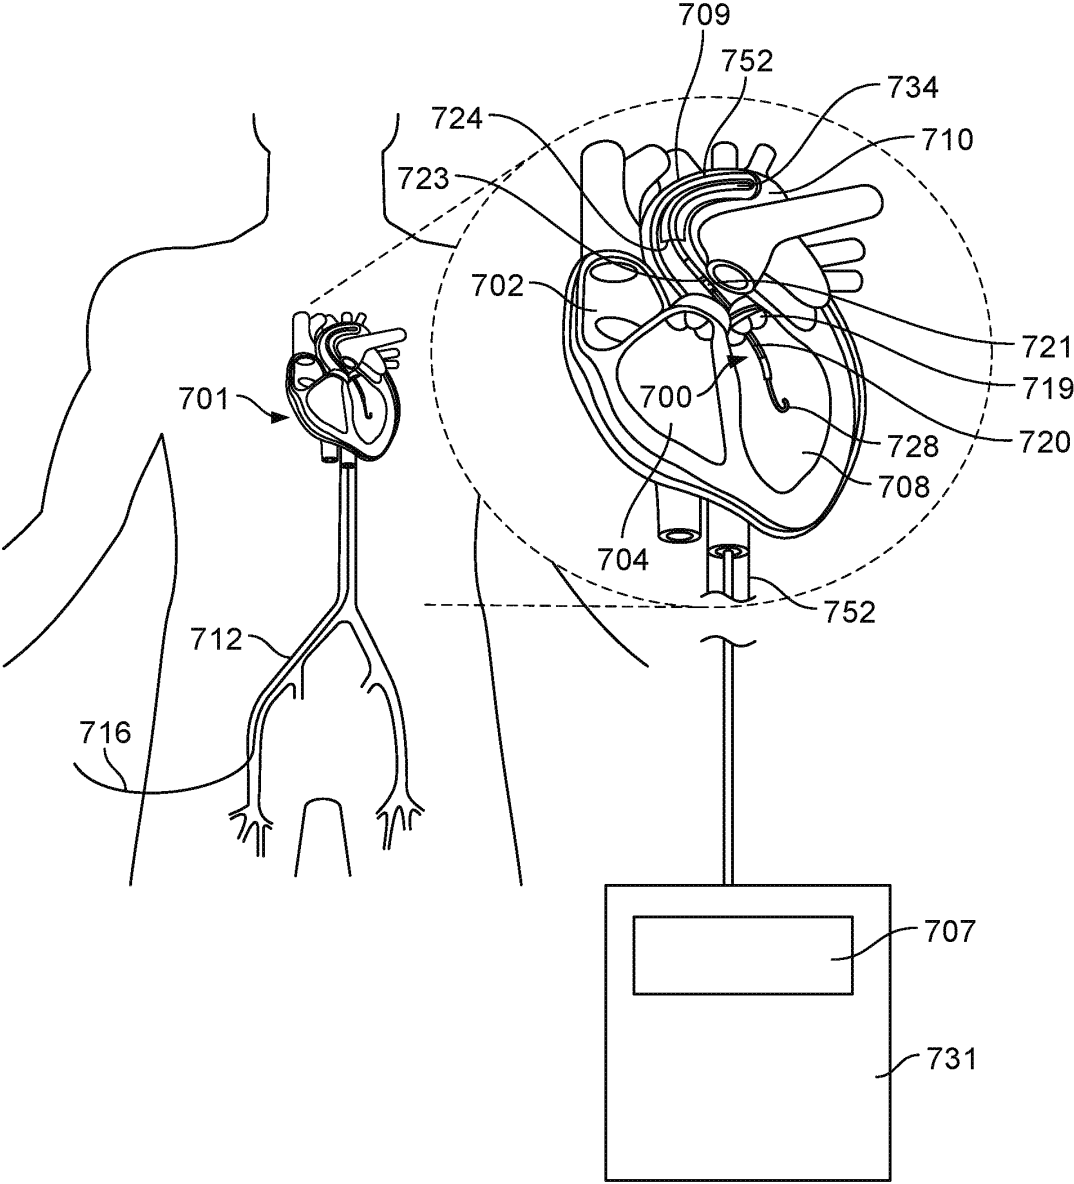


FIG. 6

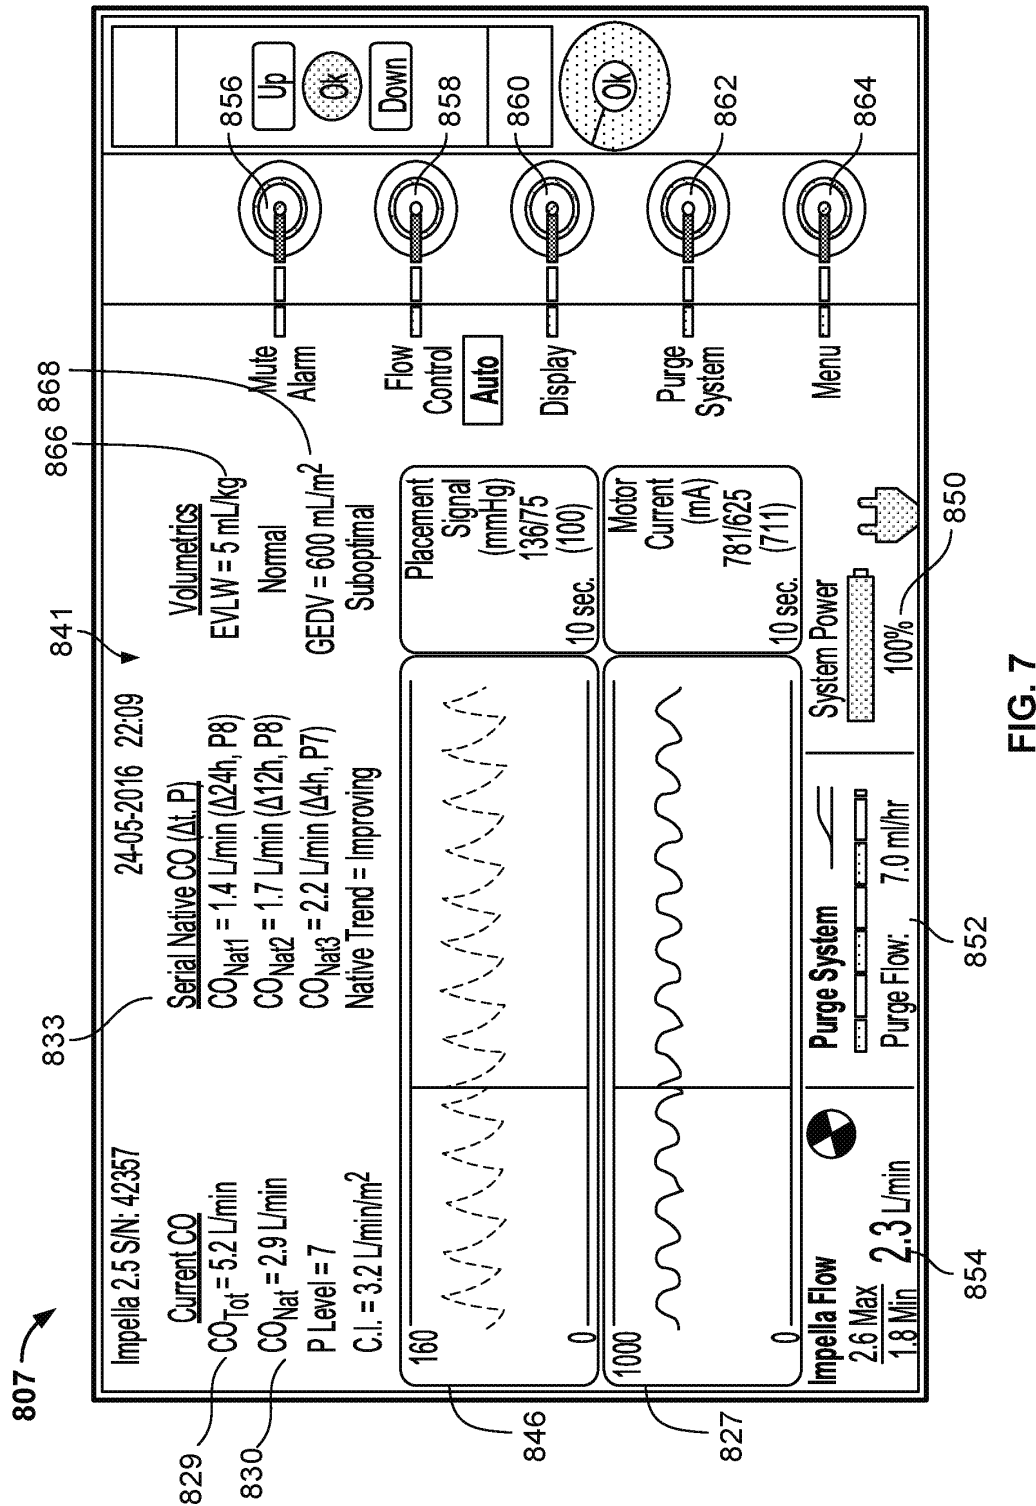


FIG. 7

8 / 13

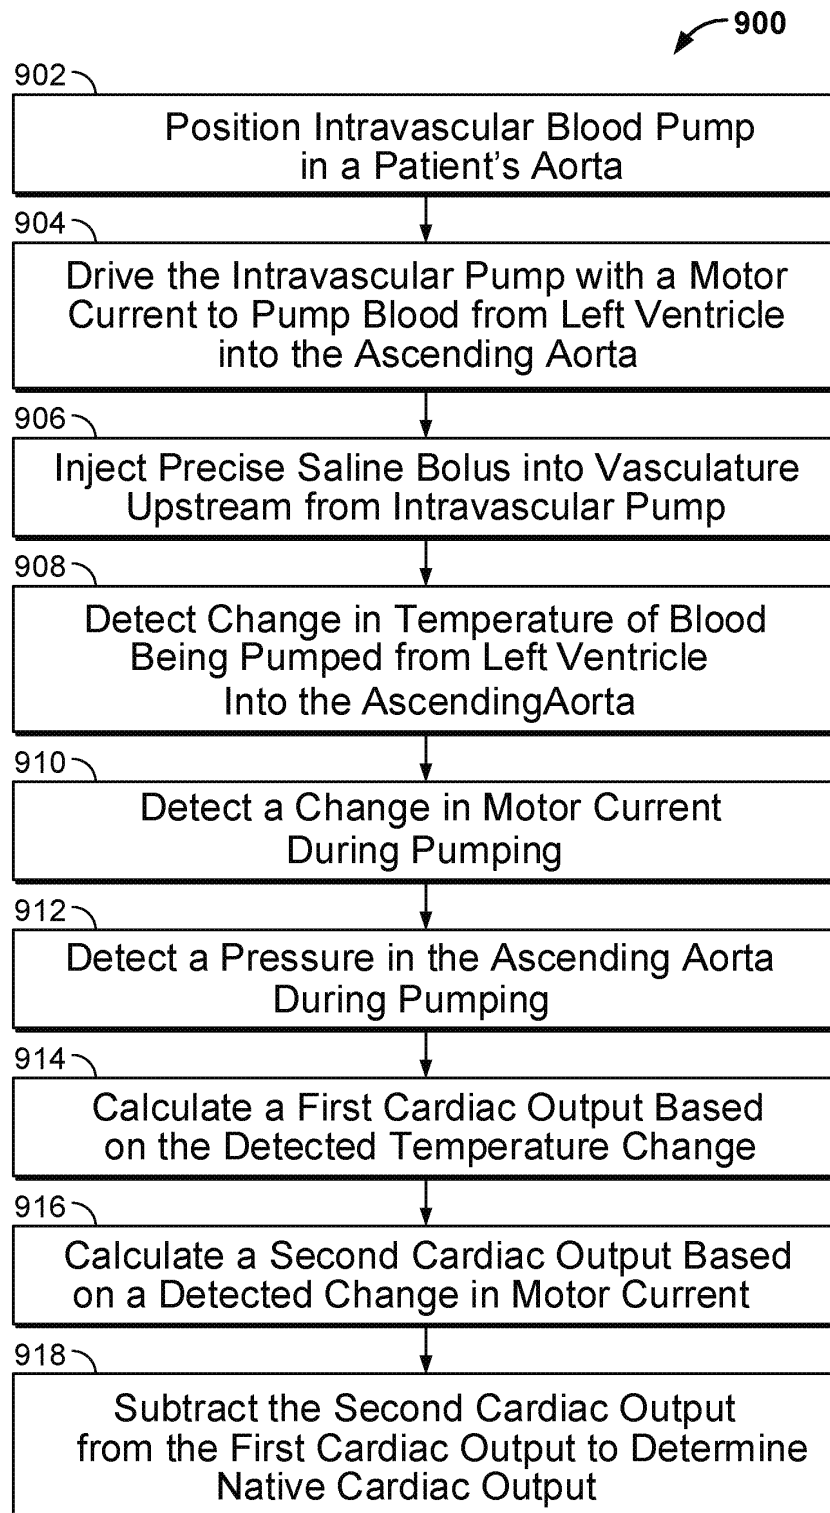


FIG. 8

9 / 13

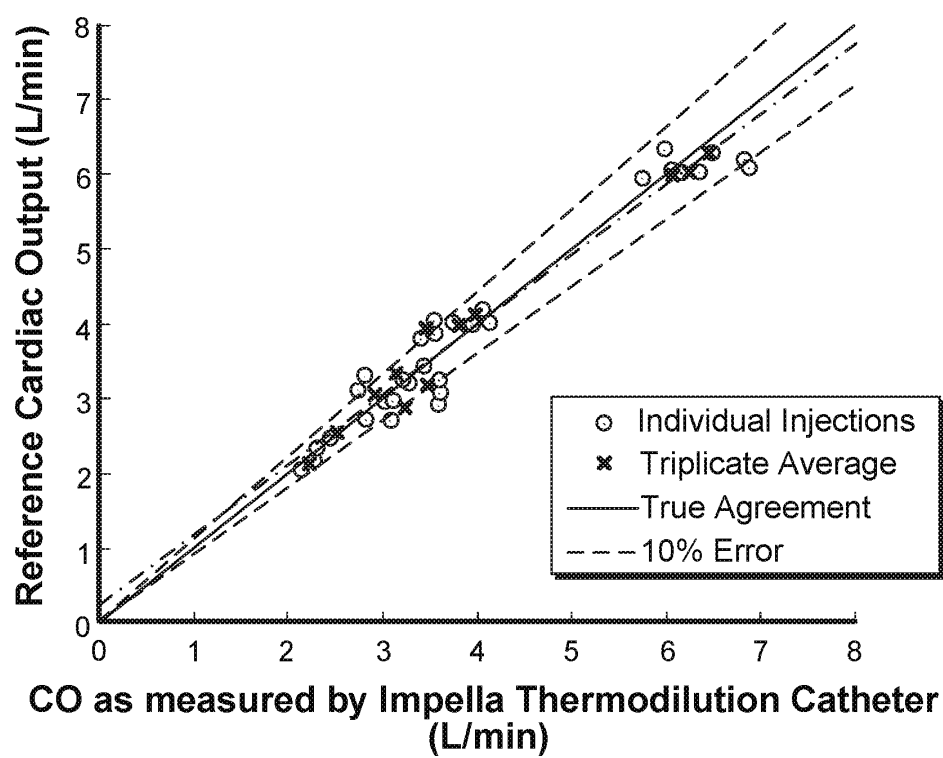


FIG. 9

10 / 13

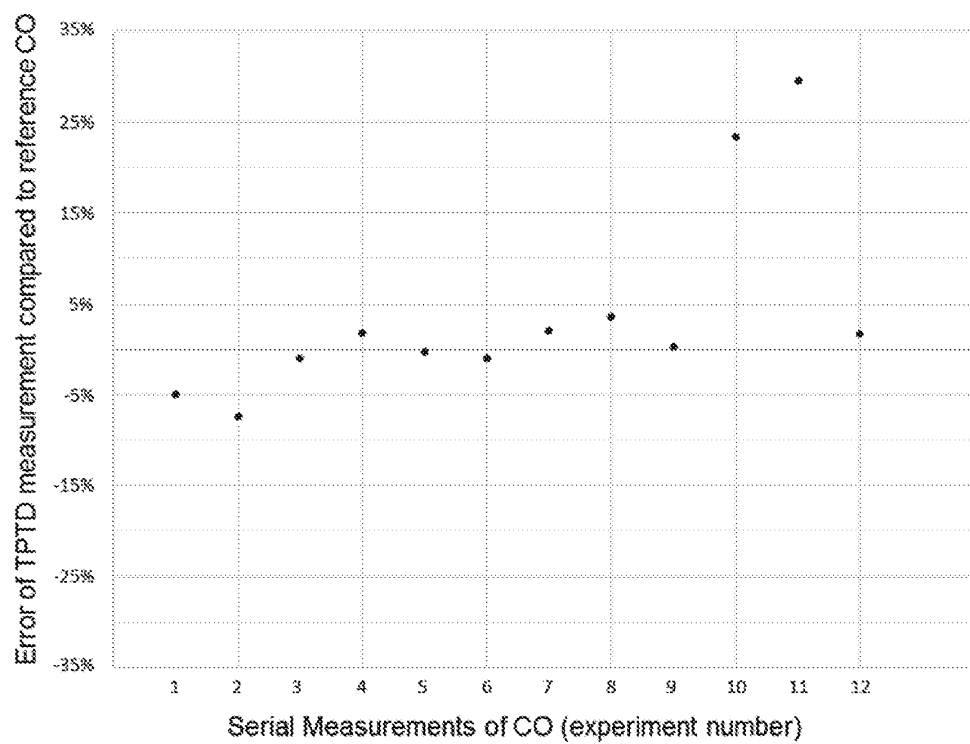


FIG. 10

11 / 13

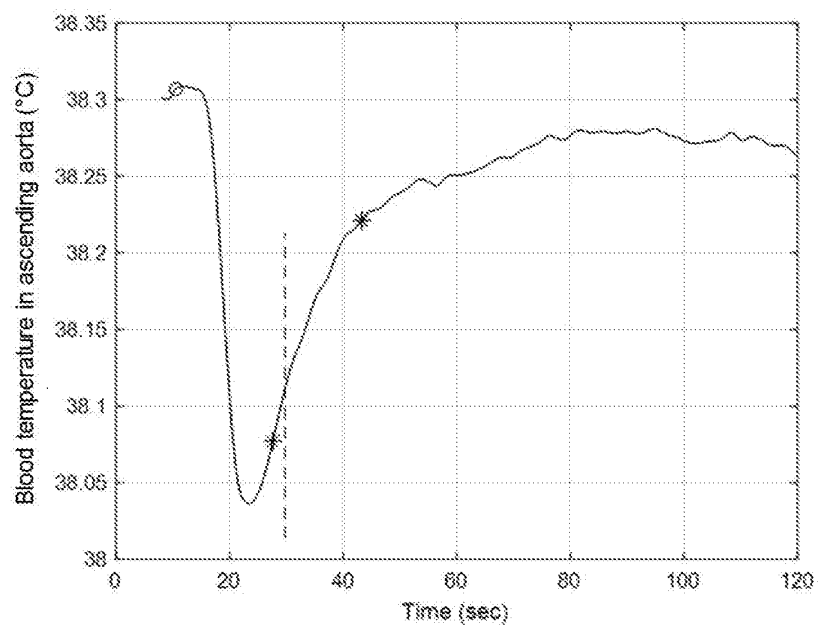


FIG. 11A

<u>Variable</u>	<u>Measured or calculated Value</u>
Reference CO (L/min)	2.32
Cardiac Output (L/min)	2.34
Mean Transit Time (sec)	19.32
Downslope Time (sec)	15.63
Intrathoracic Thermal Volume (mL)	754
Pulmonary Thermal Volume (mL)	610
Extravascular Lung Water (mL)	574
Cardiac Power Output (watts)	0.41

FIG. 11B

12 / 13

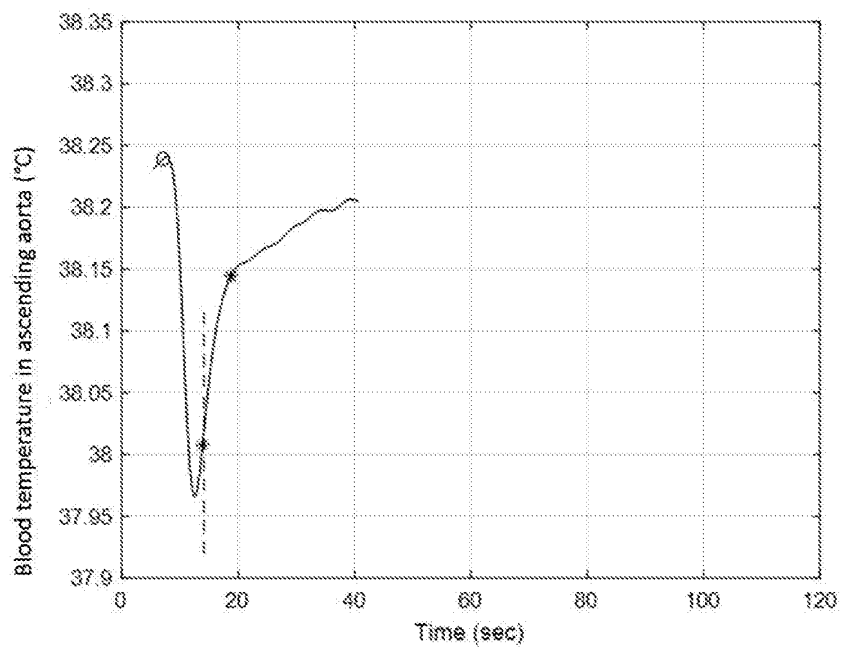


FIG. 12A

<u>Variable</u>	<u>Measured or calculated Value</u>
Reference CO (L/min)	6.04
Cardiac Output (L/min)	5.72
Mean Transit Time (sec)	7.04
Downslope Time (sec)	4.88
Intrathoracic Thermal Volume (mL)	671
Pulmonary Thermal Volume (mL)	465
Extravascular Lung Water (mL)	414
Cardiac Power Output (watts)	1.2

FIG. 12B

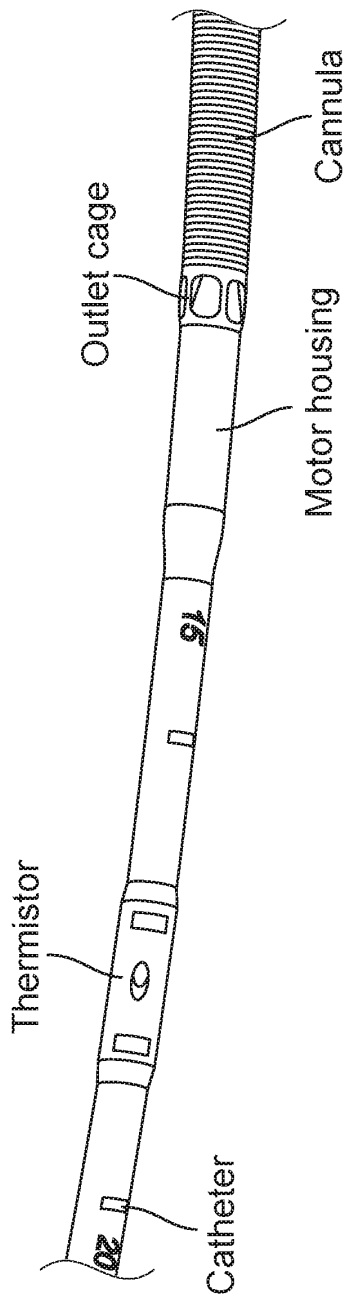


FIG. 13