



Fig. 1A


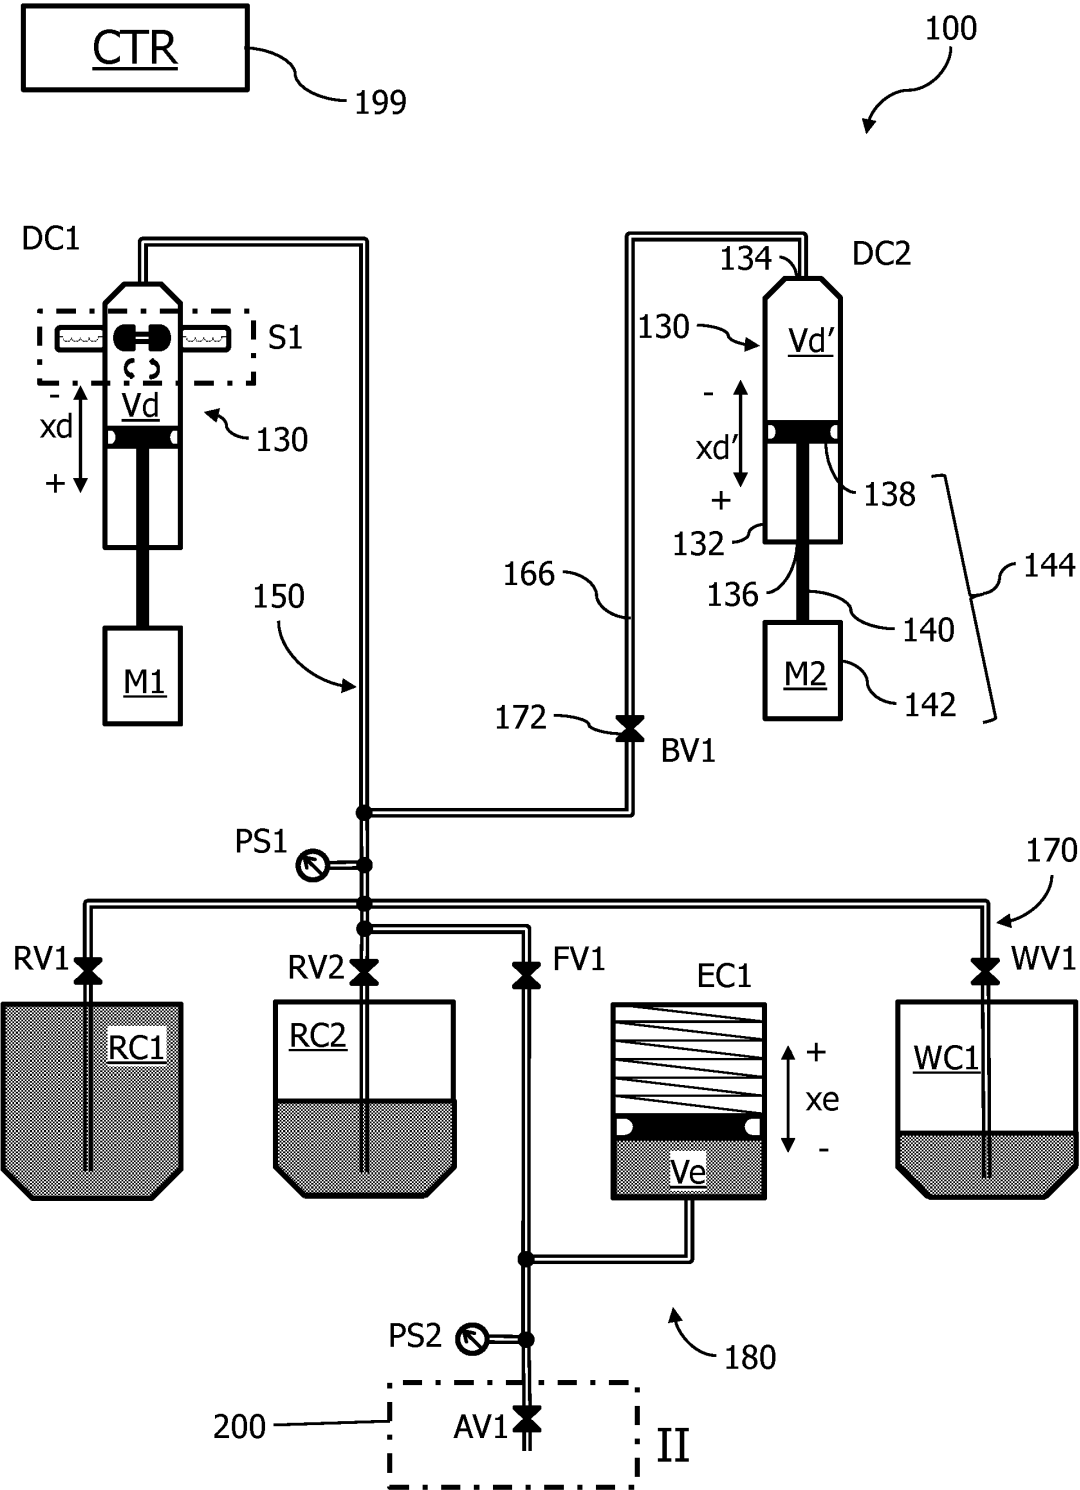


Fig. 1B

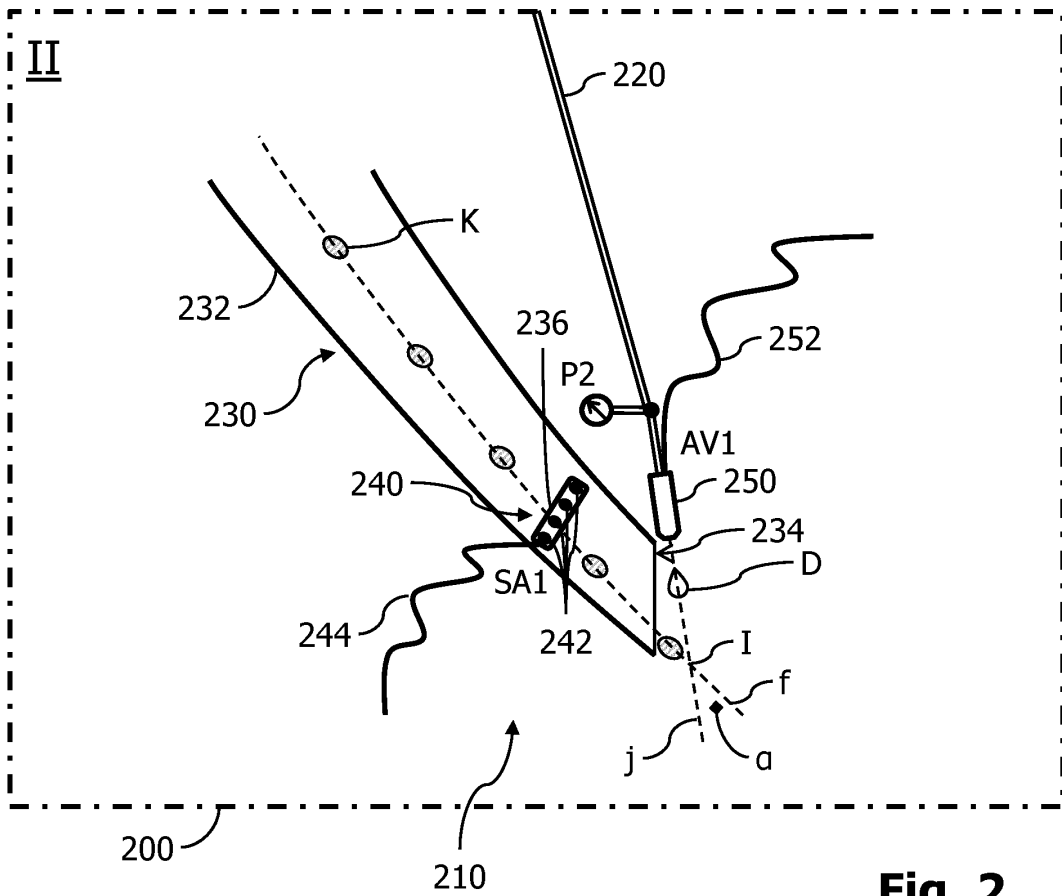

	Mode	DC1	S1	RV1	RV2	WV1	FV1	EC1	AV1
310	Single dose	+	0	O	C	C	C	-	T
320	Mixed dose	+	0	C/O	C/O	C	C	-	T
330	Blend		1	C	C	C	C	-	T
340	Feed	-	0	C	C	C	O	+	C
350	Dump	-	0	C	C	O	C		C
360	Flush	+/-	0	O/C	C	C	O/C	+/-	C

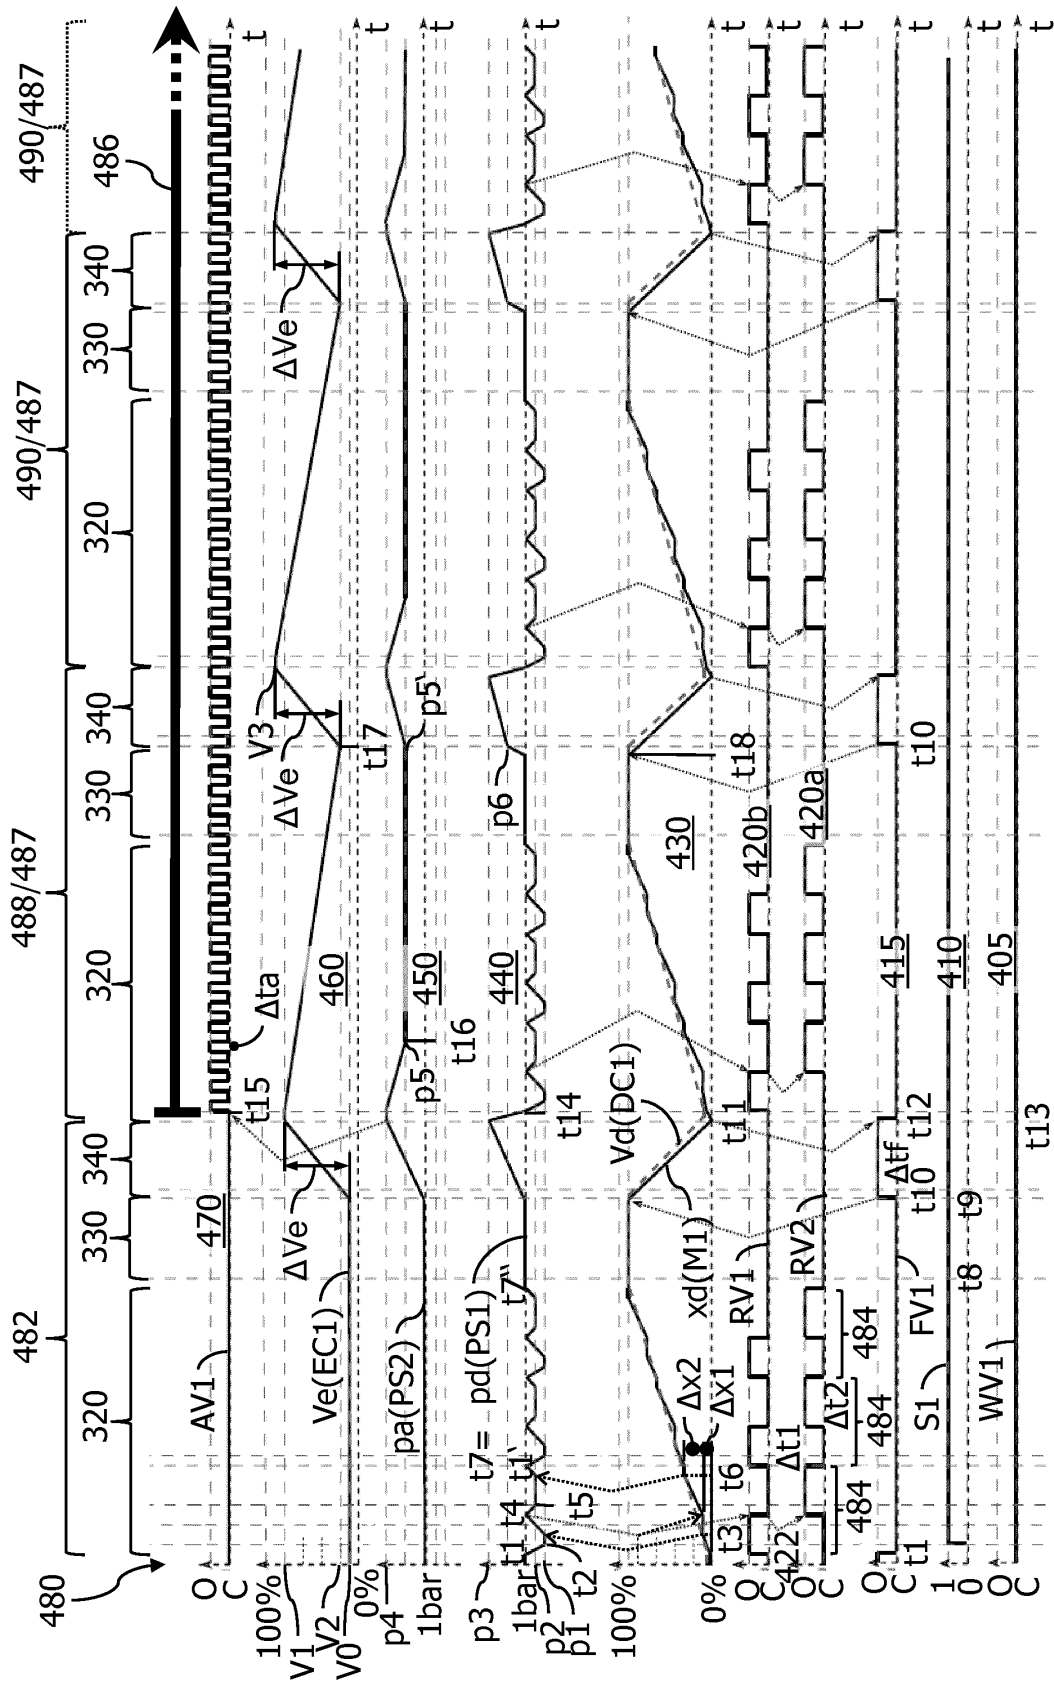


Fig. 4A

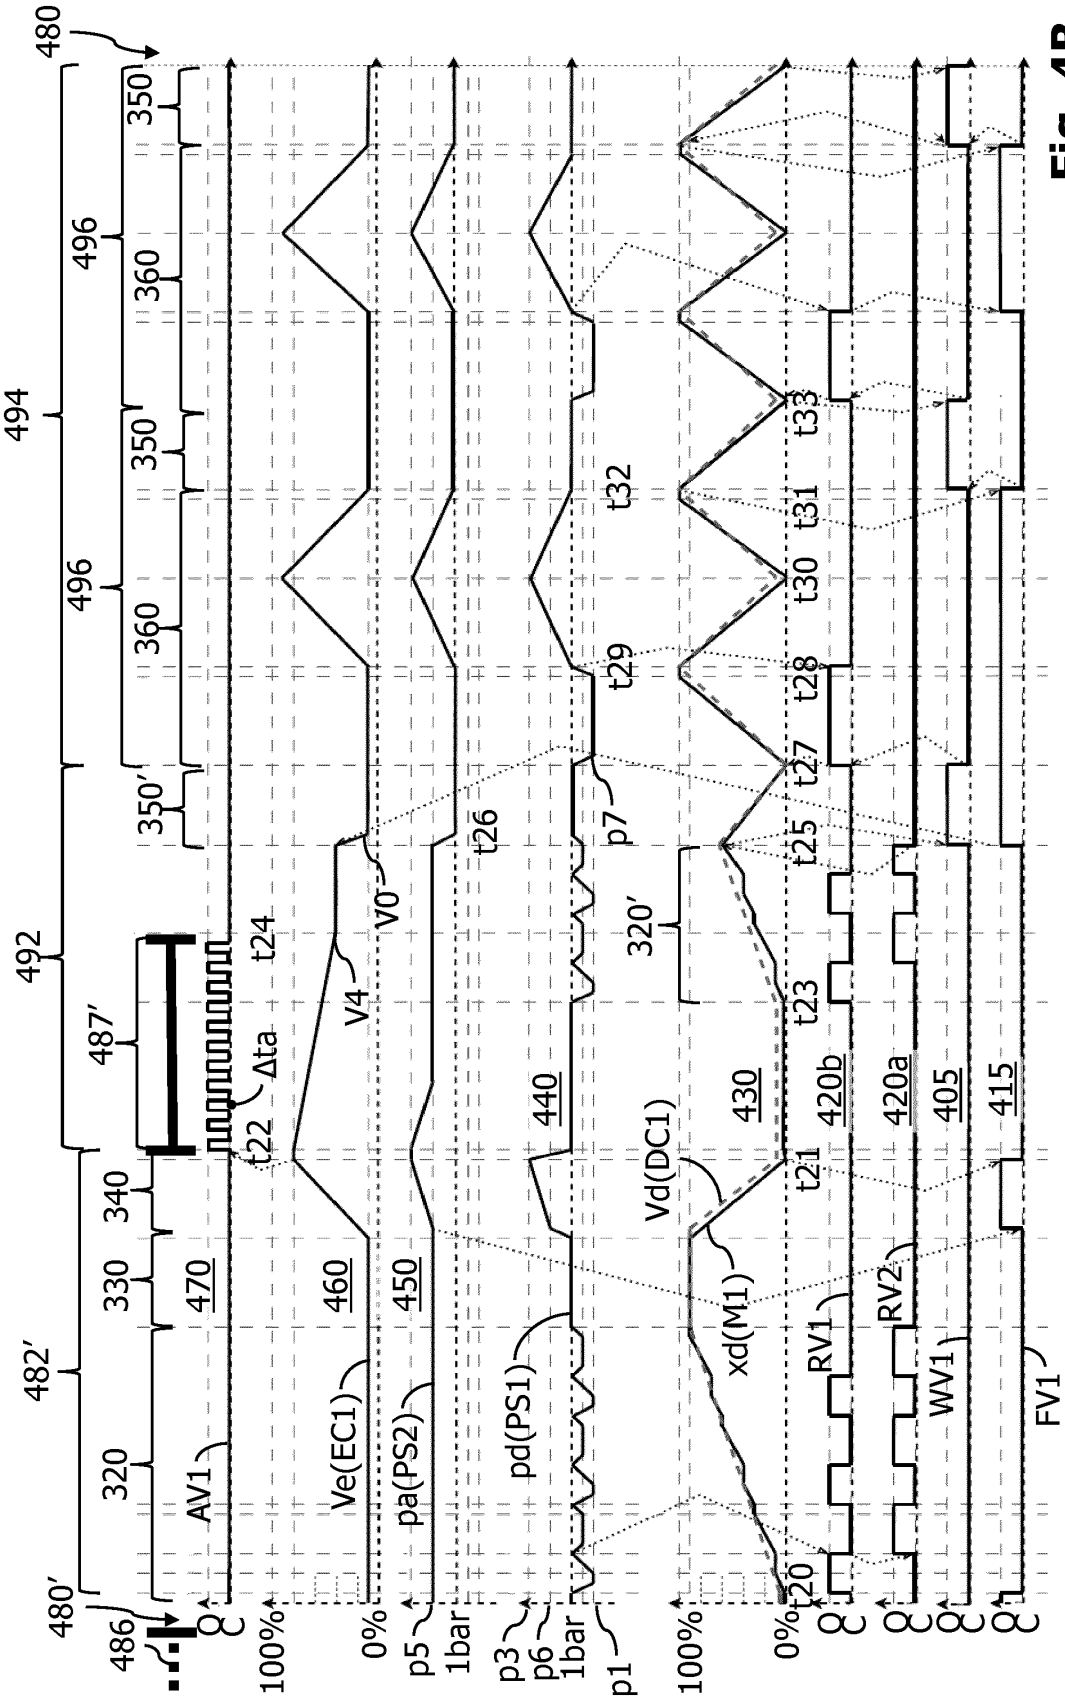


Fig. 4B

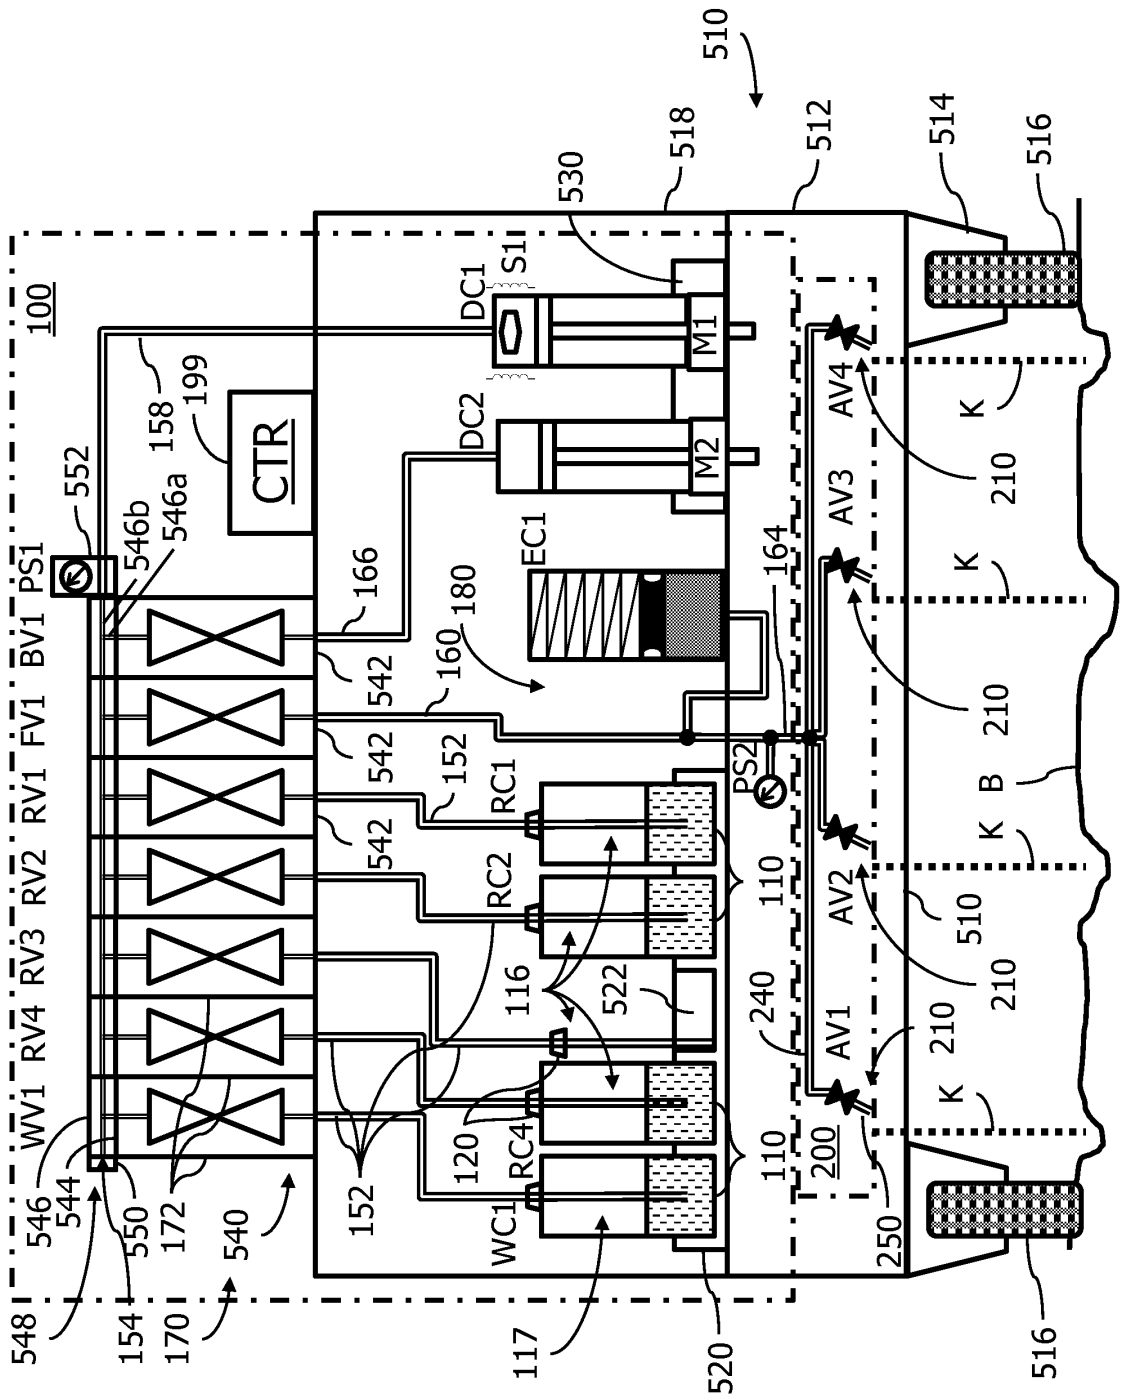
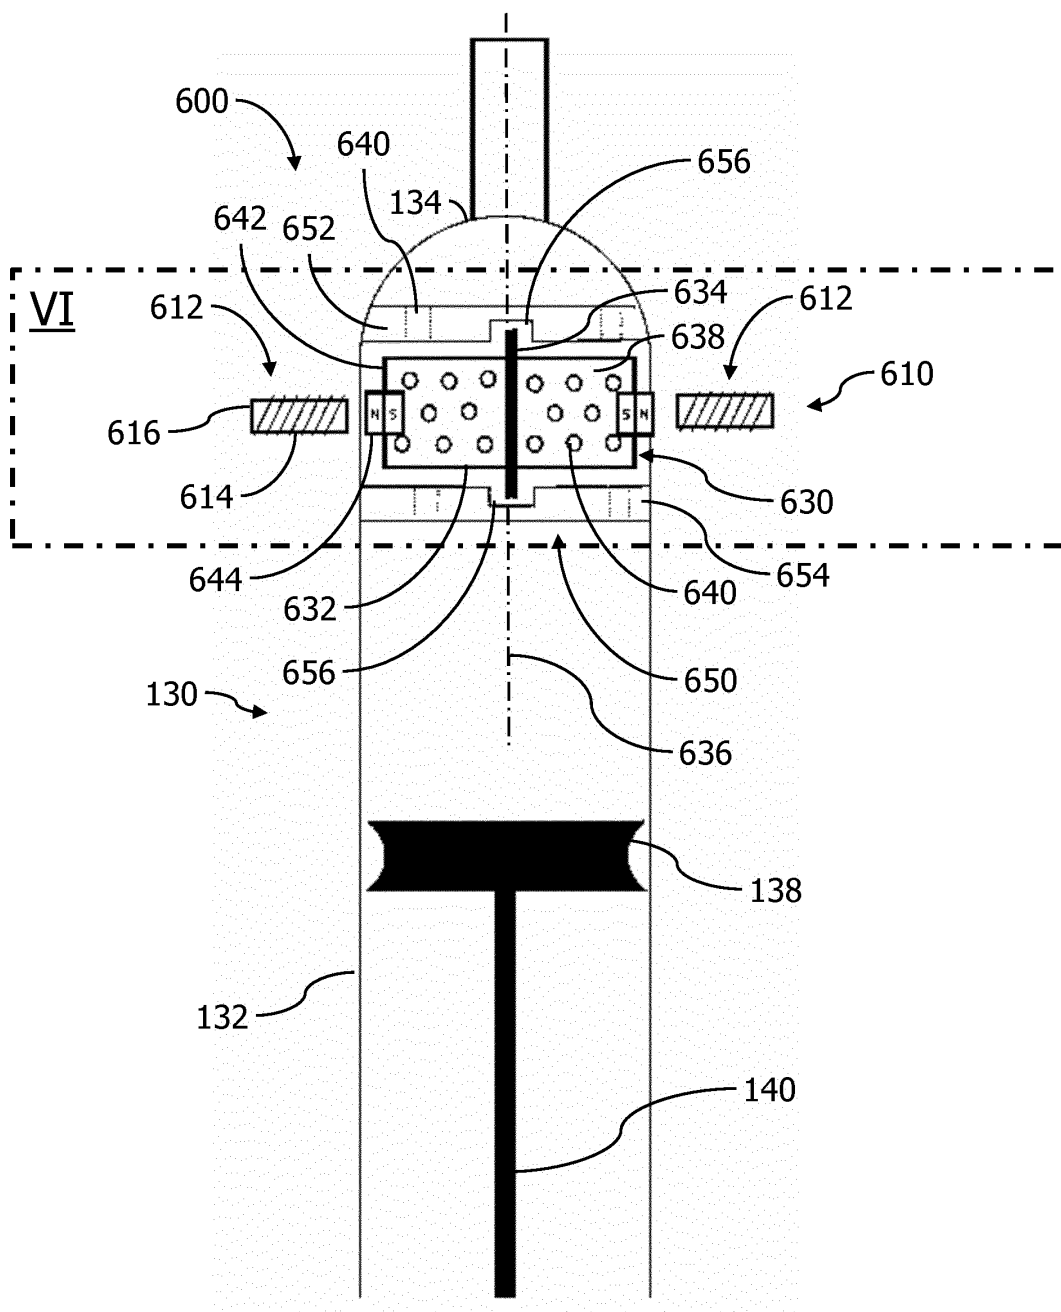


Fig. 5

**Fig. 6**