

Fig. 1

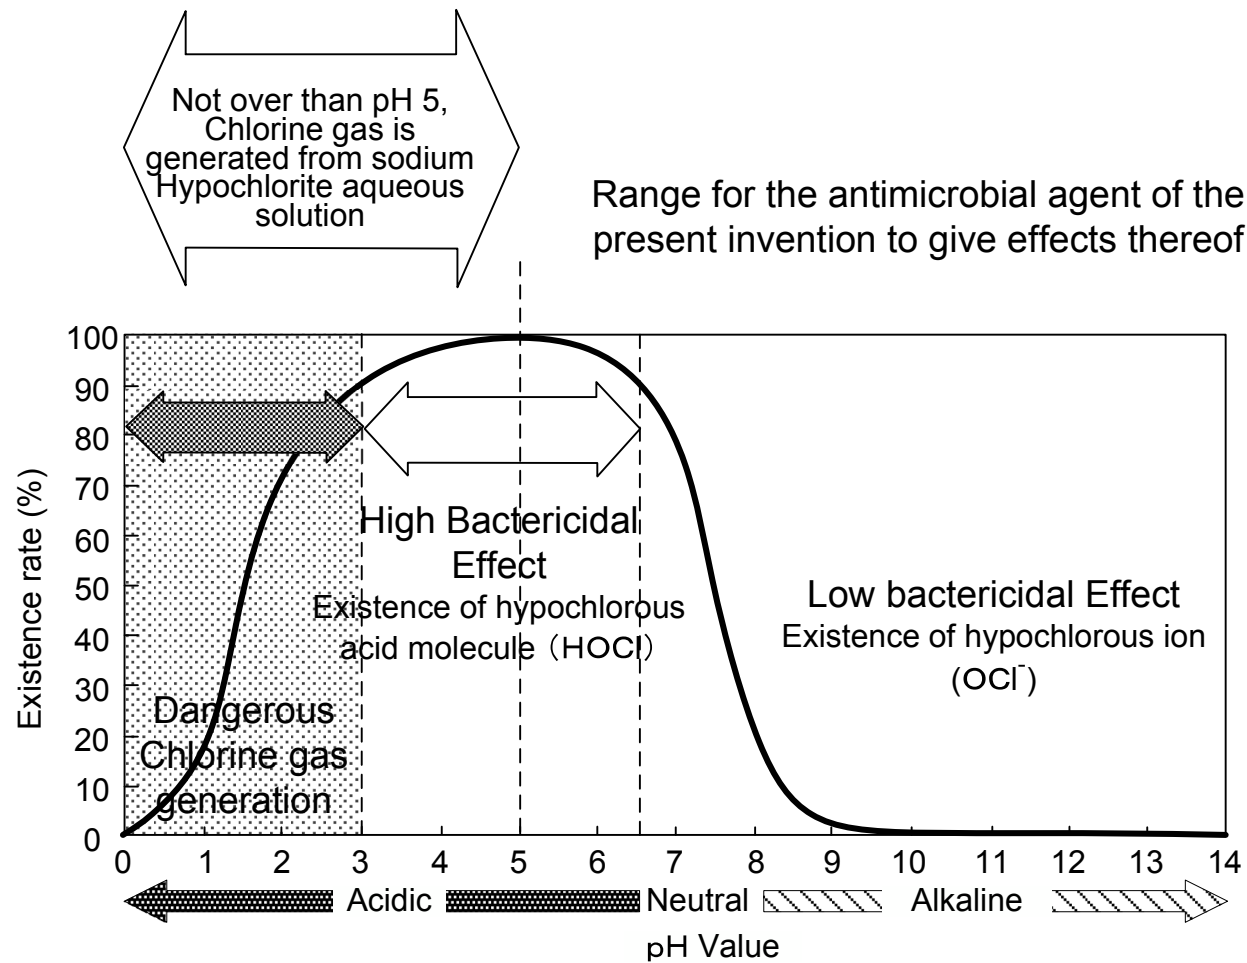


Fig. 2

<Clostridium butyricum NBRC13949>

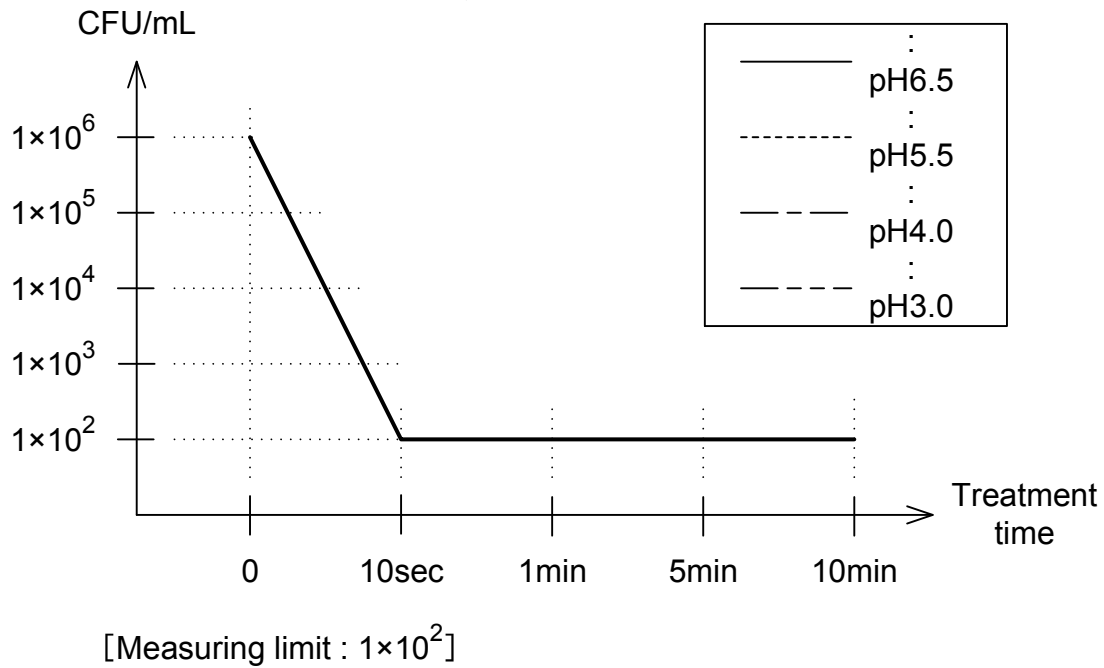


Fig. 3

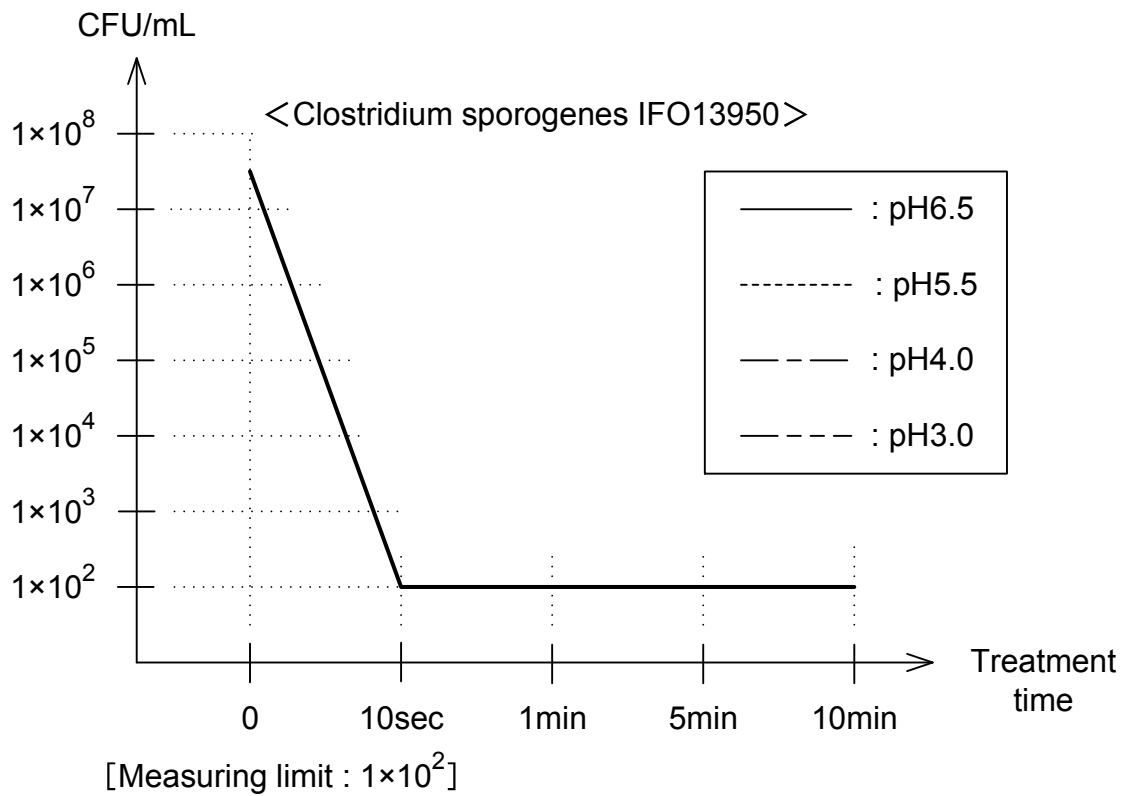


Fig. 4

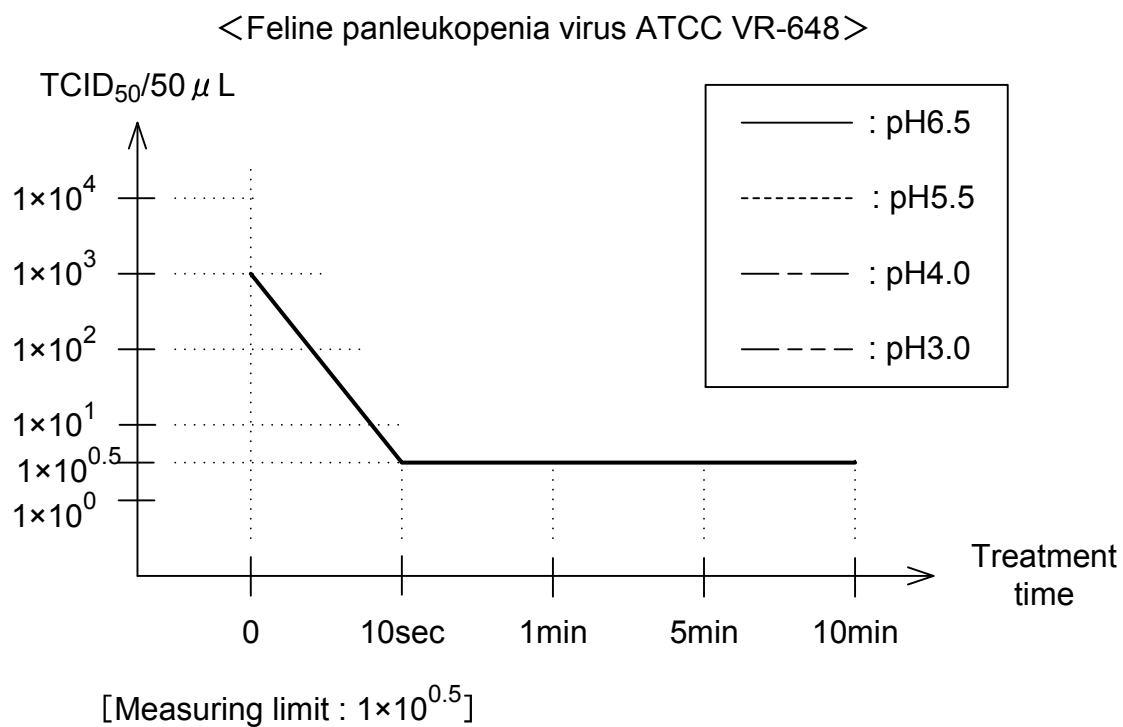


Fig. 5


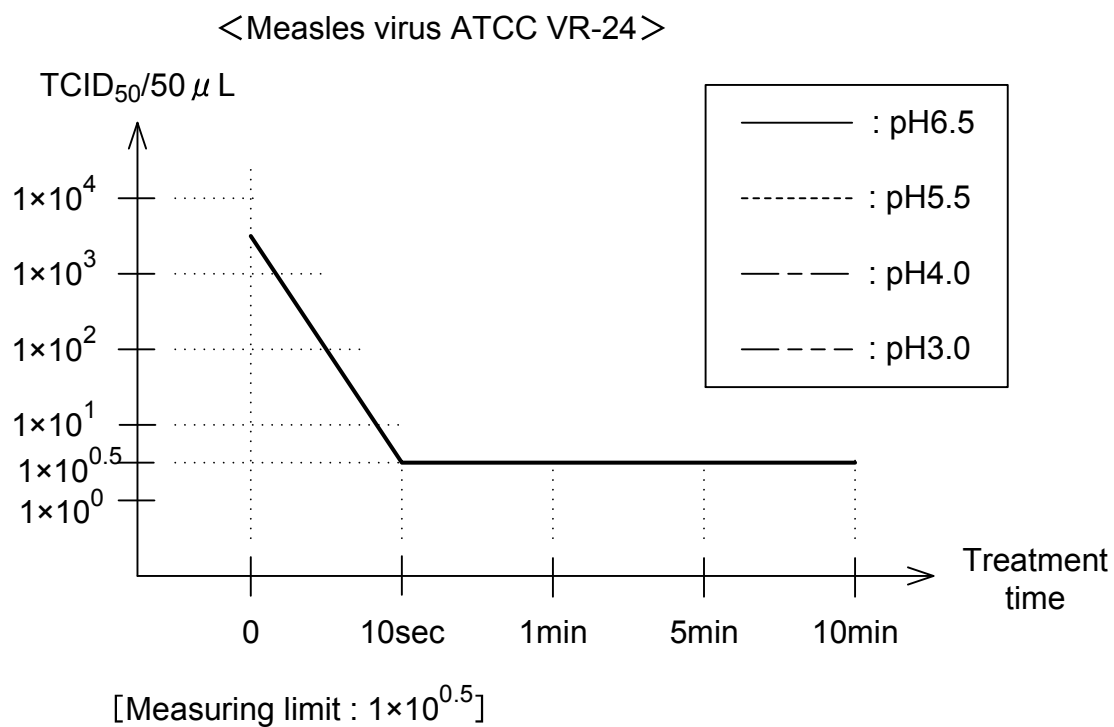


Fig. 6

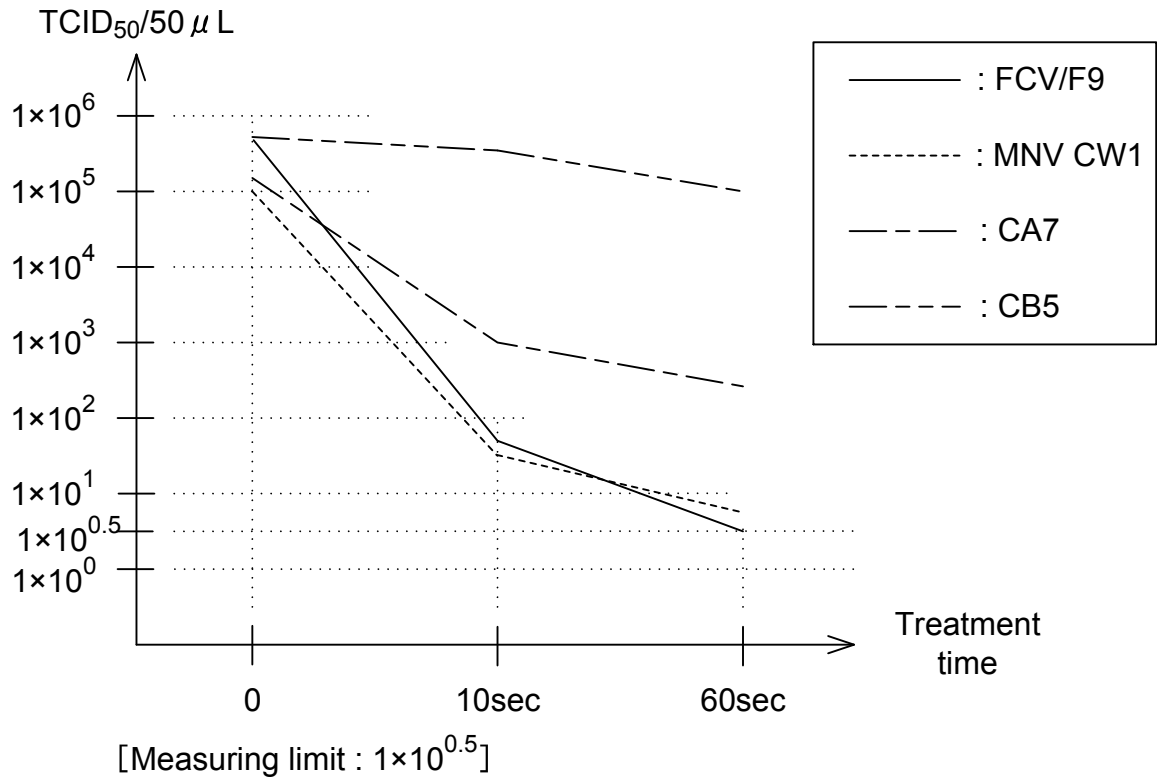

Measuring limit :

Fig. 7

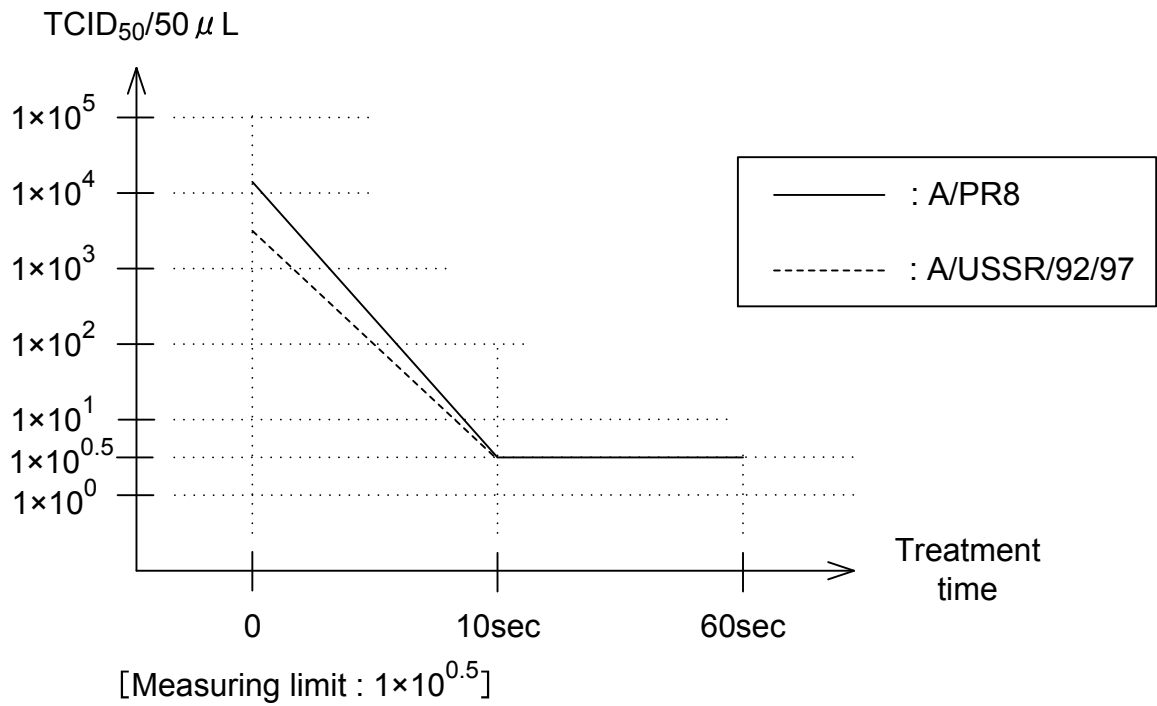


Fig. 8

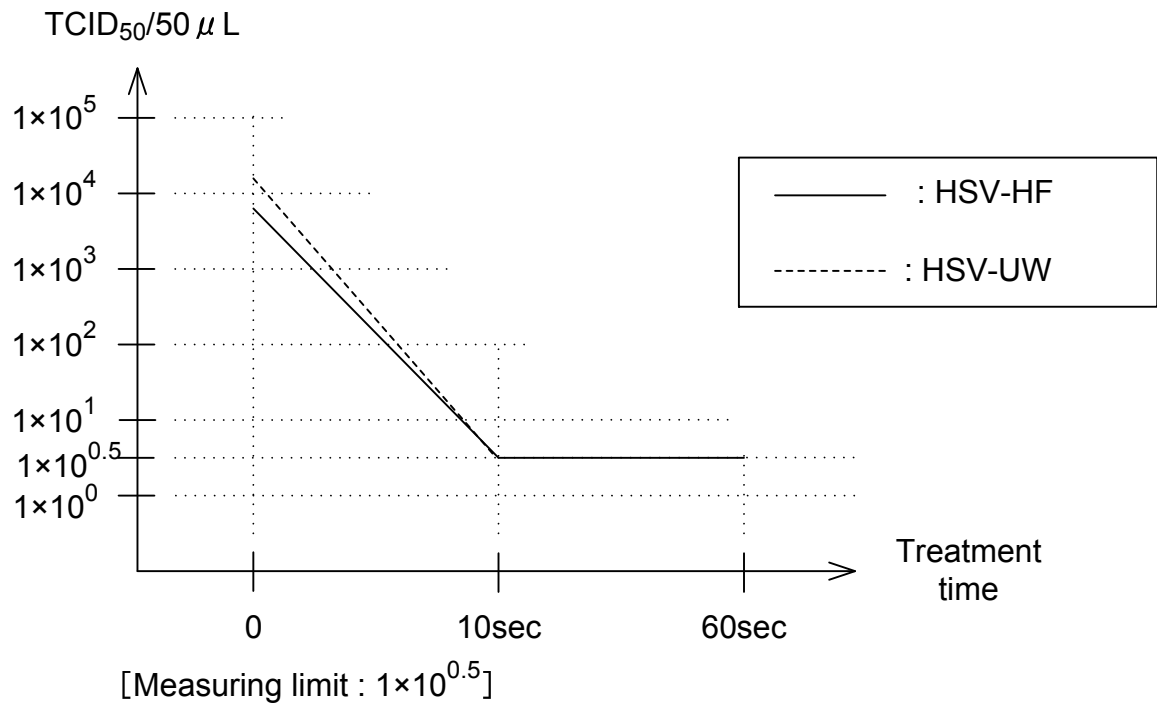


Fig. 9

