


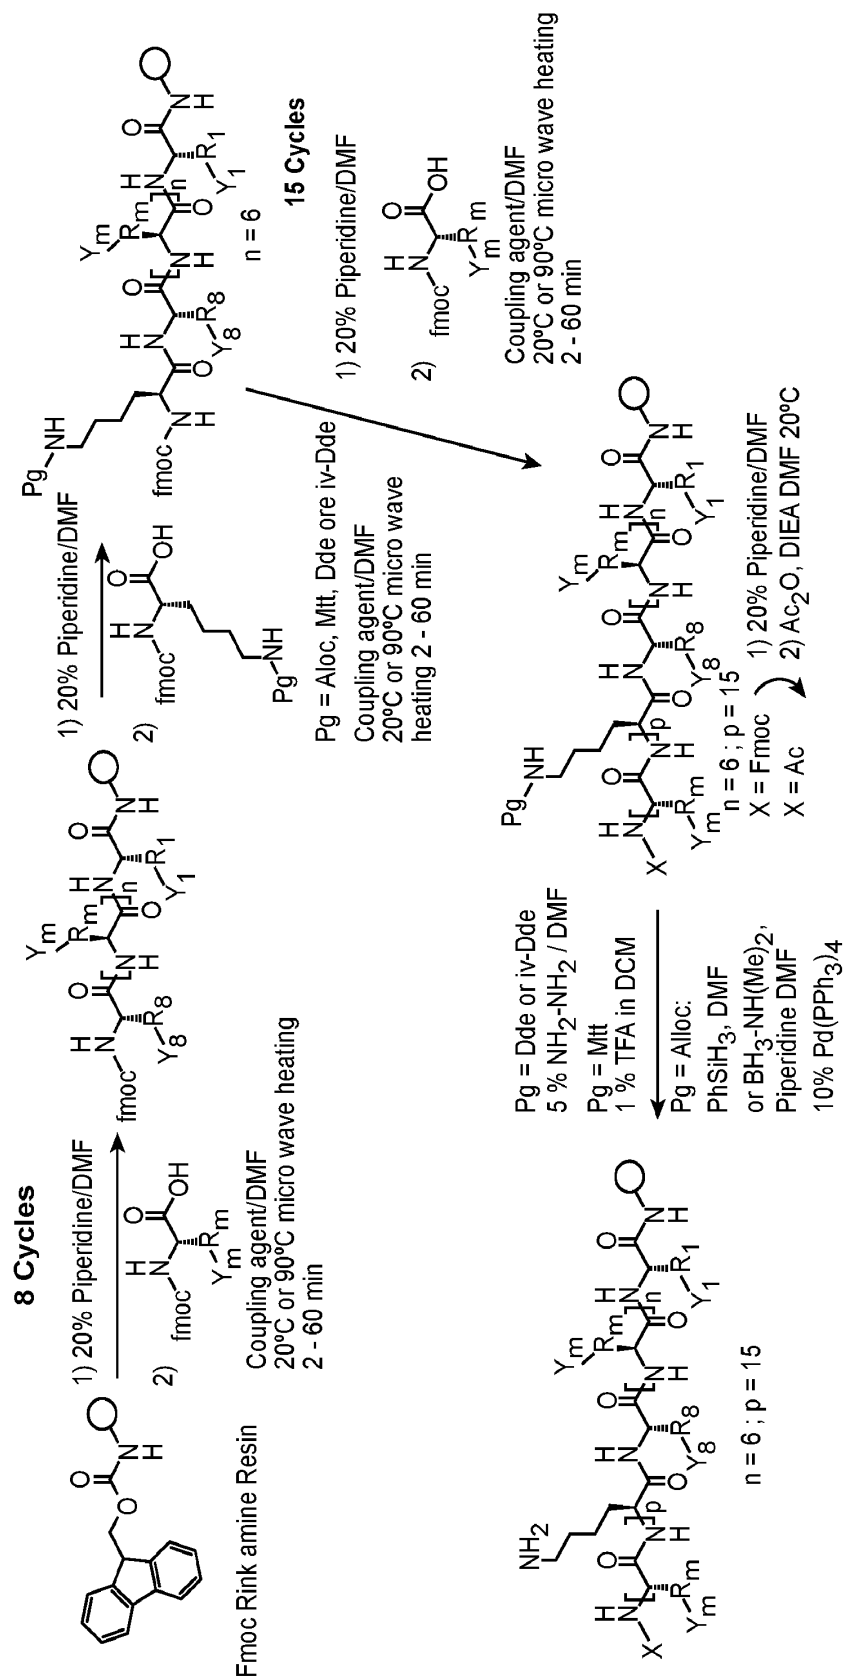

7
G
L

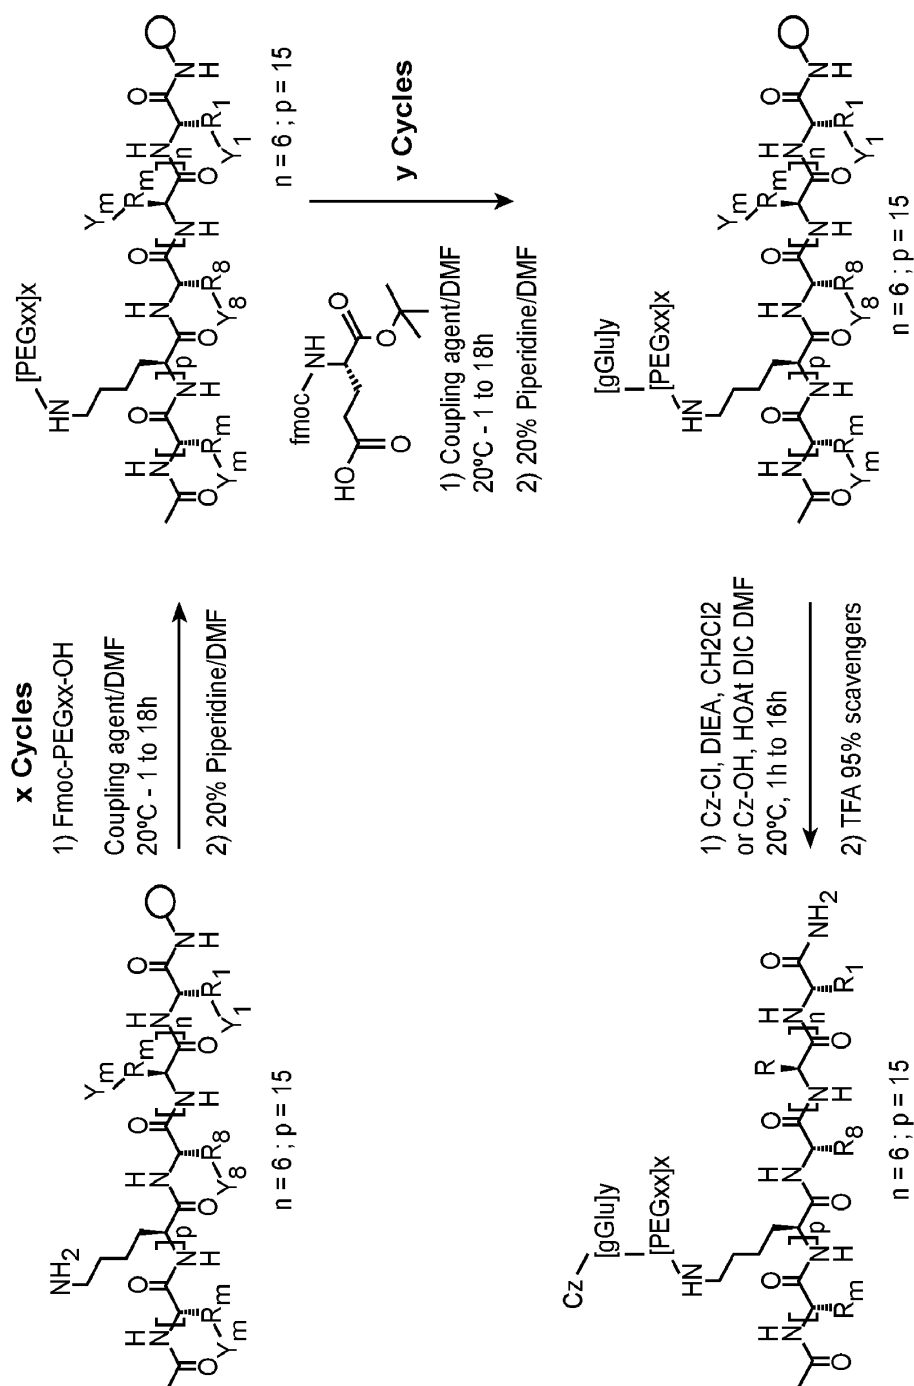


FIG. 2

Change from Baseline Effective Renal Plasma Flow (mL/min) - Day 13 (Pre)

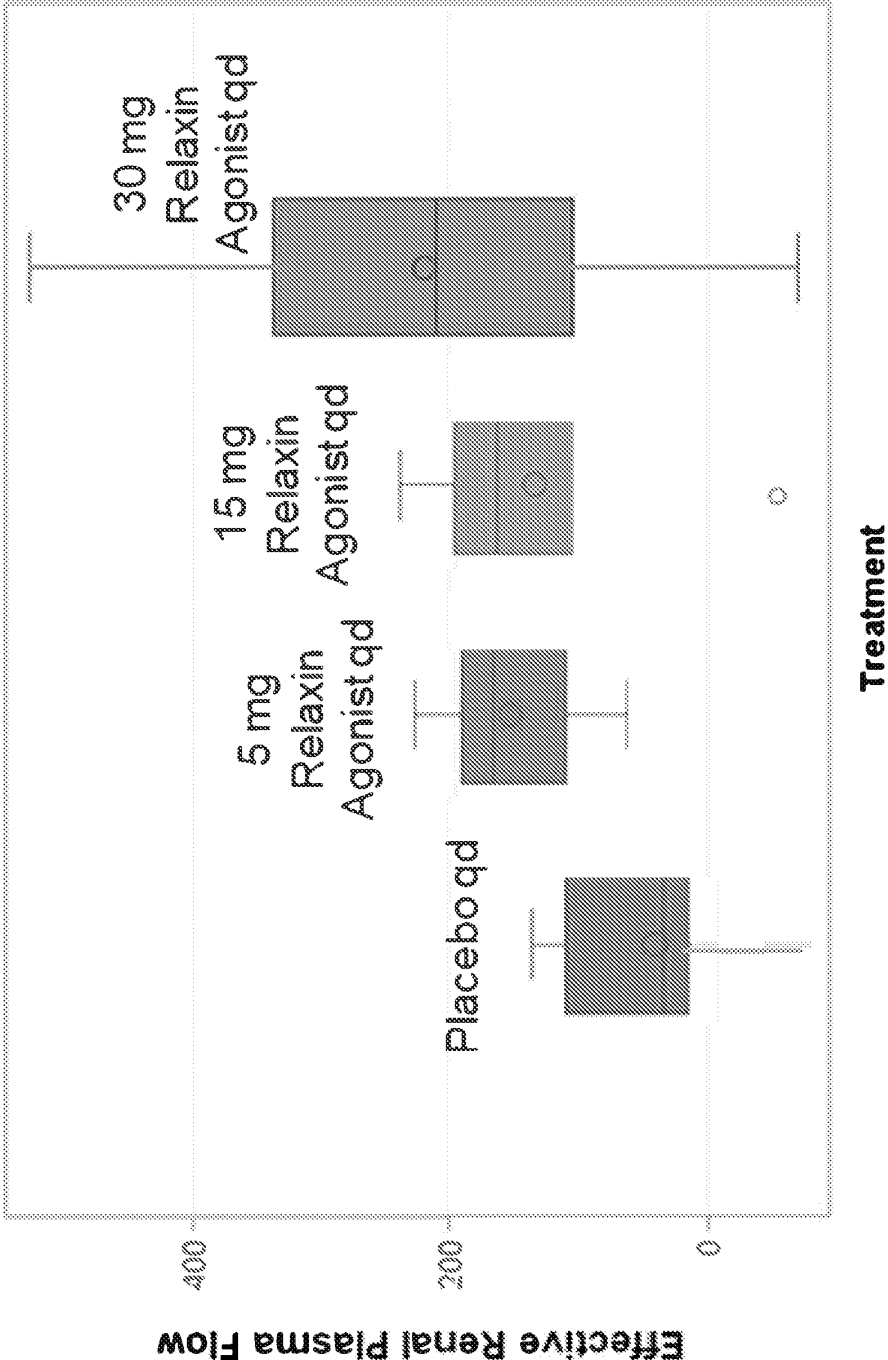


FIG. 3A

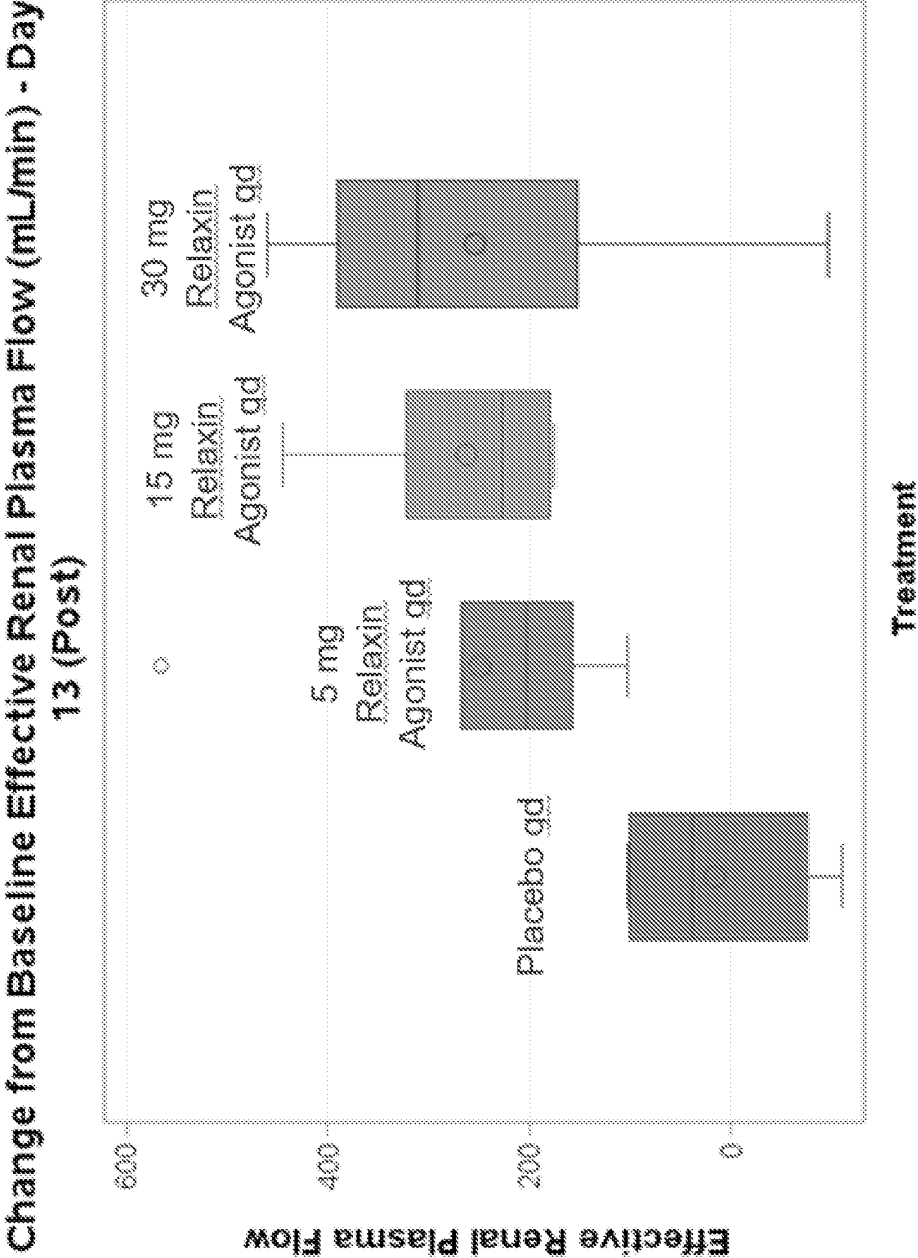


FIG. 3B

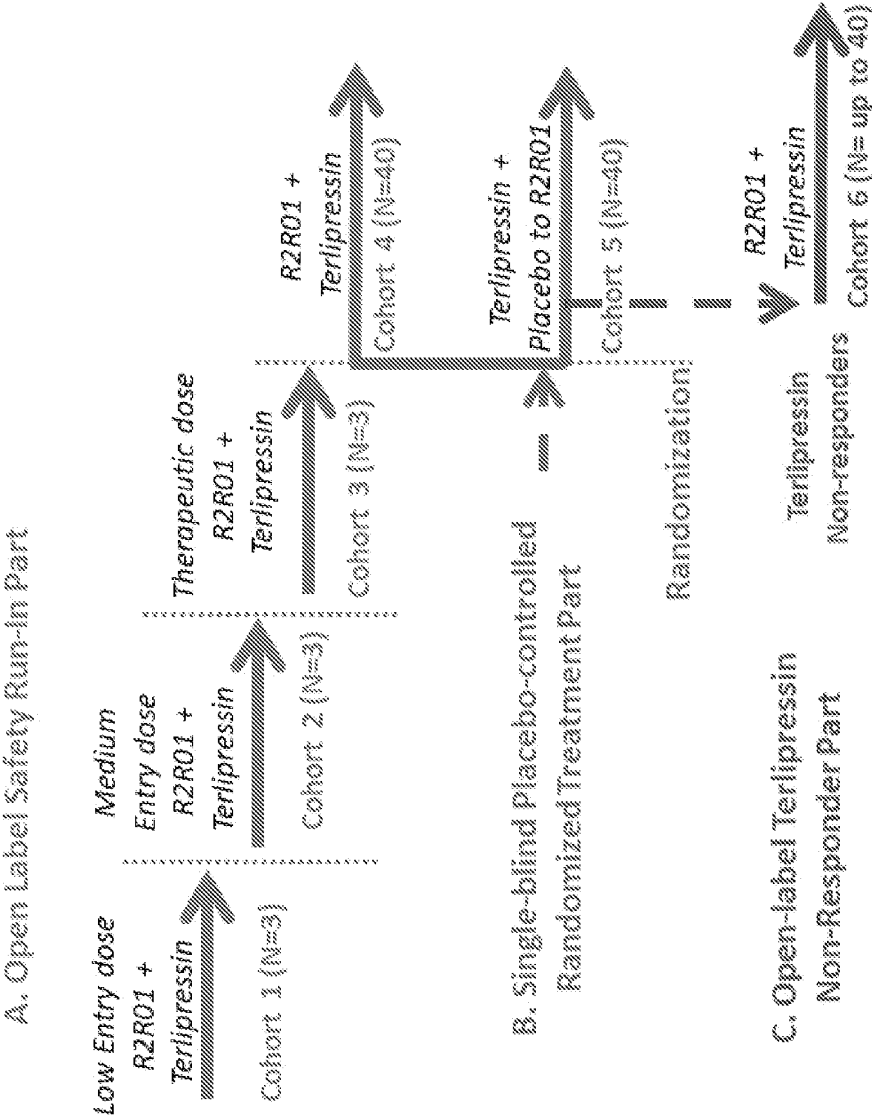


FIG. 4

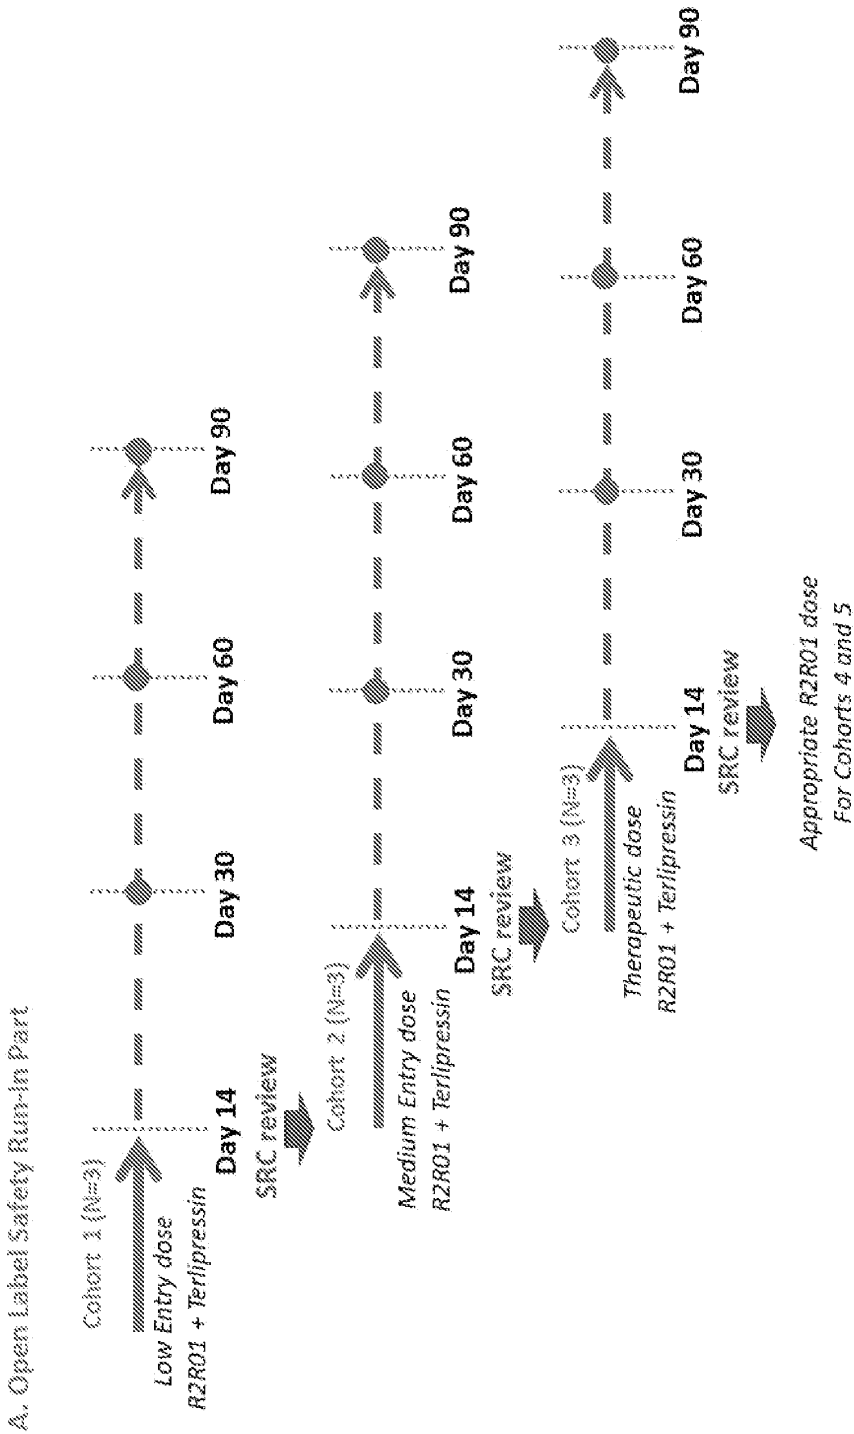


FIG. 5

B. Single-blind Placebo-controlled
Randomized Treatment Part

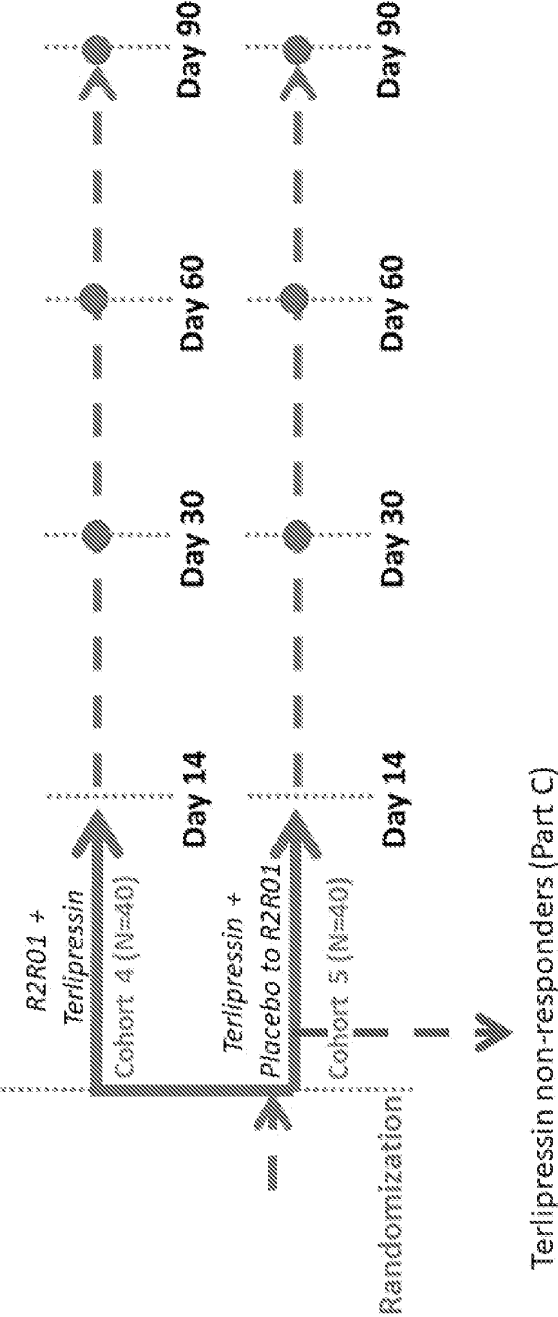


FIG. 6

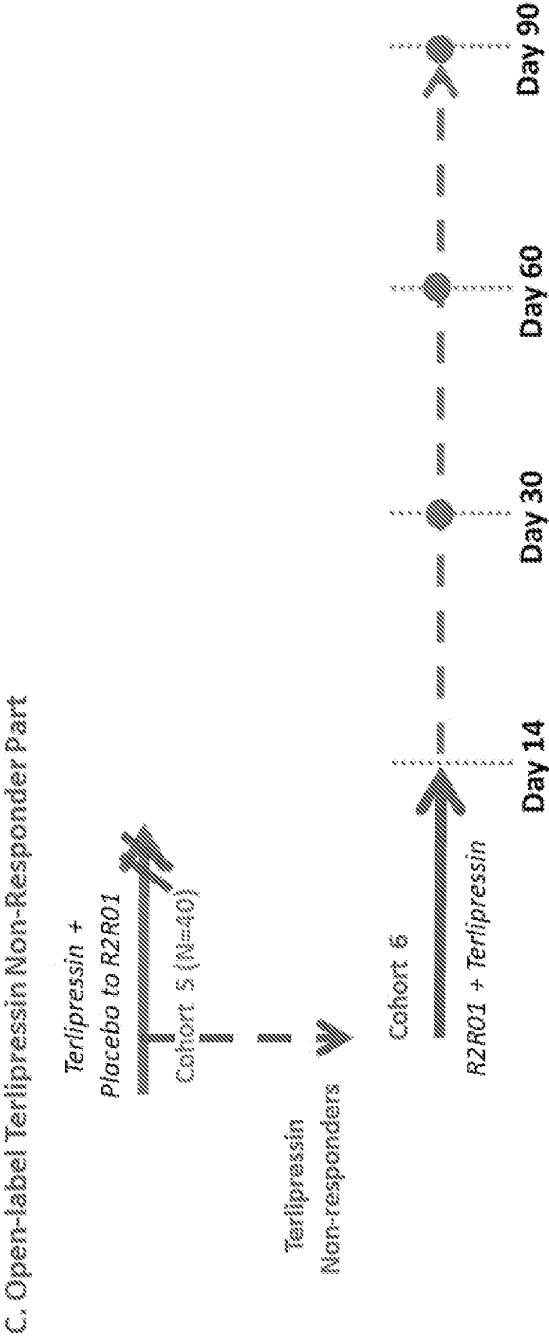


FIG. 7