



(51) International Patent Classification:

<i>A61B 34/20</i> (2016.01)	<i>G06T 7/13</i> (2017.01)
<i>A61B 5/055</i> (2006.01)	<i>G06T 7/70</i> (2017.01)
<i>A61B 8/08</i> (2006.01)	<i>G16H 30/20</i> (2018.01)
<i>A61B 34/30</i> (2016.01)	<i>G16H 50/20</i> (2018.01)
<i>A61N 7/02</i> (2006.01)	

(71) **Applicant: HISTOSONICS, INC.** [US/US]; 16305 36TH Avenue North, Suite 300, Plymouth, Minnesota 55446 (US).

(72) **Inventors: CANNATA, Jonathan M.;** 16305 36TH Avenue North, Suite 300, Plymouth, Minnesota 55446 (US). **DURYEA, Alexander P.;** 16305 36TH Avenue North, Suite 300, Plymouth, Minnesota 55446 (US). **MILLER, Ryan M.;** 16305 36TH Avenue North, Suite 300, Plymouth, Minnesota 55446 (US). **MLADENOVIC, Zeljko;** 16305 36TH Avenue North, Suite 300, Plymouth, Minnesota 55446 (US). **STOPEK, Joshua;** 16305 36TH Avenue North, Suite 300, Plymouth, Minnesota 55446 (US). **LEMIEUX, Erin-Anne;** 16305 36TH Avenue North, Suite 300, Plymouth, Minnesota 55446 (US). **TURNER, Carolyn M.;** 16305 36TH Avenue North, Suite 300, Plymouth, Minnesota 55446 (US). **SHAFFER, Carol L.;** 16305 36TH Avenue North, Suite 300, Plymouth, Minnesota 55446 (US).

(21) International Application Number:

PCT/US2024/025730

(22) International Filing Date:

22 April 2024 (22.04.2024)

(25) **Filing Language:** English

(26) **Publication Language:** English

(30) Priority Data:

63/497,277 20 April 2023 (20.04.2023) US

(54) Title: HISTOTRIPSY SYSTEMS AND ASSOCIATED METHODS INCLUDING USER INTERFACES AND WORKFLOWS FOR TREATMENT PLANNING AND THERAPY

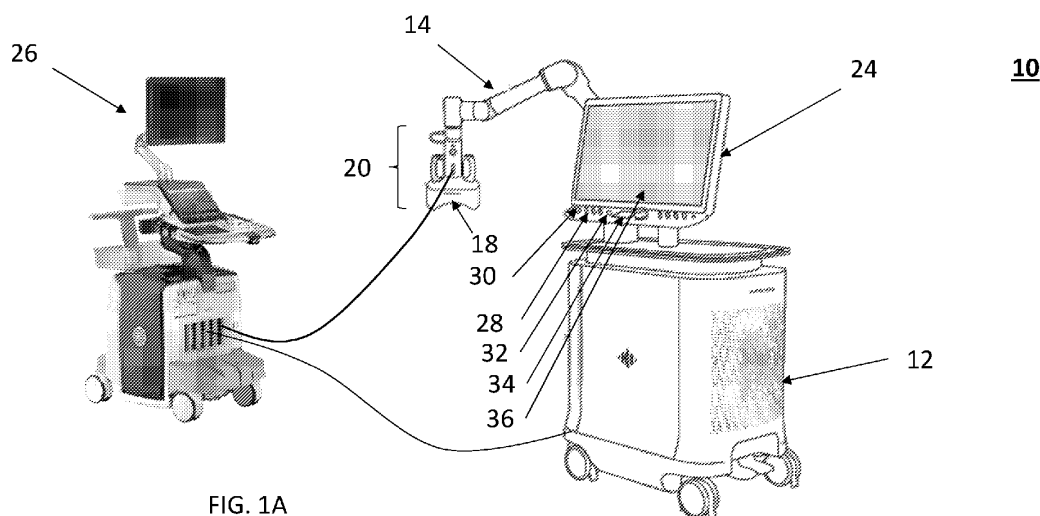


FIG. 1A

(57) **Abstract:** A system and method, including an ultrasound imaging transducer, an ultrasound therapy transducer, a robotic arm configured to orient the ultrasound imaging transducer and the ultrasound therapy transducer about a patient, a display connected to imaging transducer, and a memory, storing instructions that when executed by a processor receive ultrasound images from the imaging transducer, present ultrasound images, receive an input to alter a shape of a contour line, present the contour line, receive an input of a size of a margin around the treatment area, present the margin, determine end points at locations where X, Y, and Z axes bisect the contour line in an XZ plane and a YZ plane, drive the ultrasound therapy transducer to a location where a focal point of the ultrasound therapy transducer is at the end point, and determining whether a resistance to movement exceeds a threshold.

(74) **Agent: THOMAS, Justin**; Shay Glenn LLP, 155 Bovet Road, Suite 710, SAN MATEO, California 94402 (US).

(81) **Designated States** (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CV, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IQ, IR, IS, IT, JM, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, MG, MK, MN, MU, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, WS, ZA, ZM, ZW.

(84) **Designated States** (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, CV, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SC, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, ME, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(88) **Date of publication of the international search report:**

03 April 2025 (03.04.2025)