

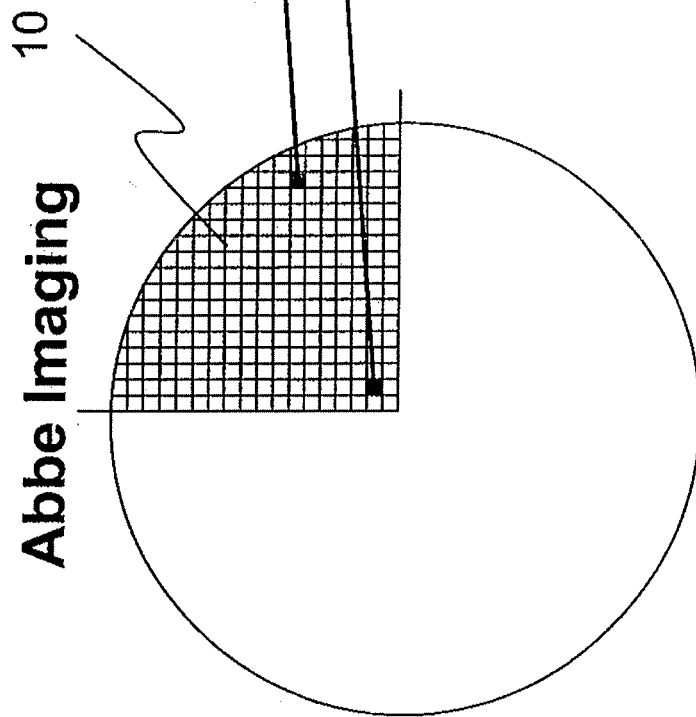


FIG. 1A

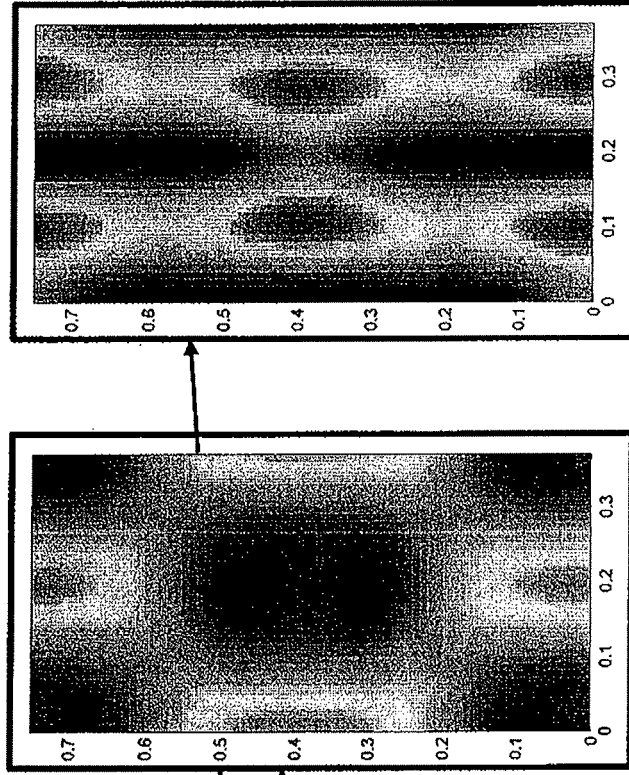


FIG. 1B

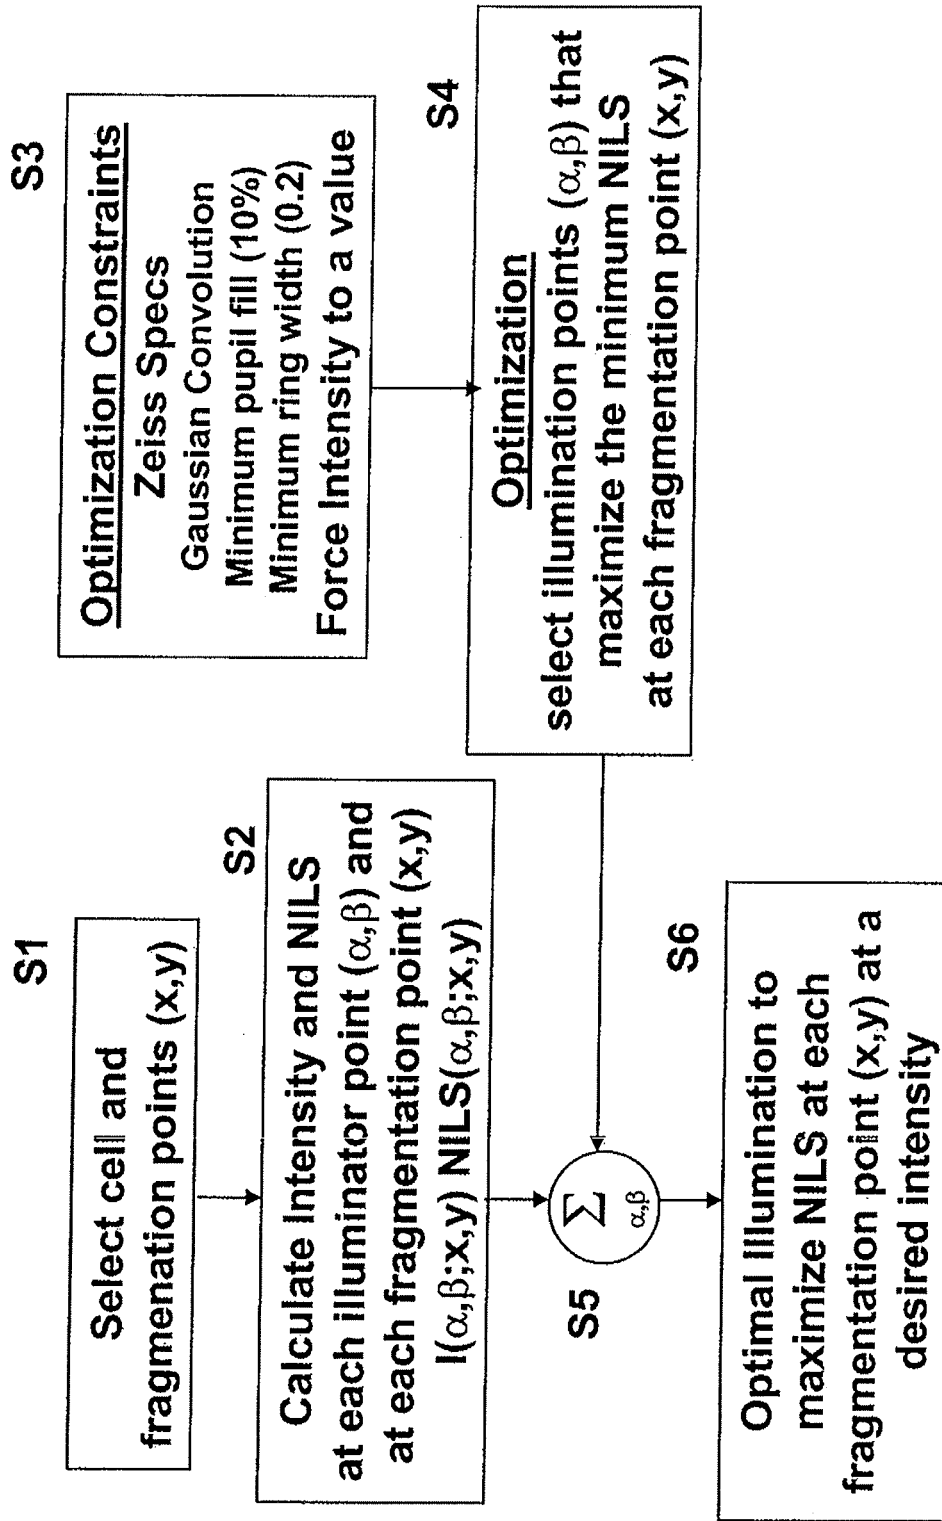


FIG. 2

Hopkins Imaging

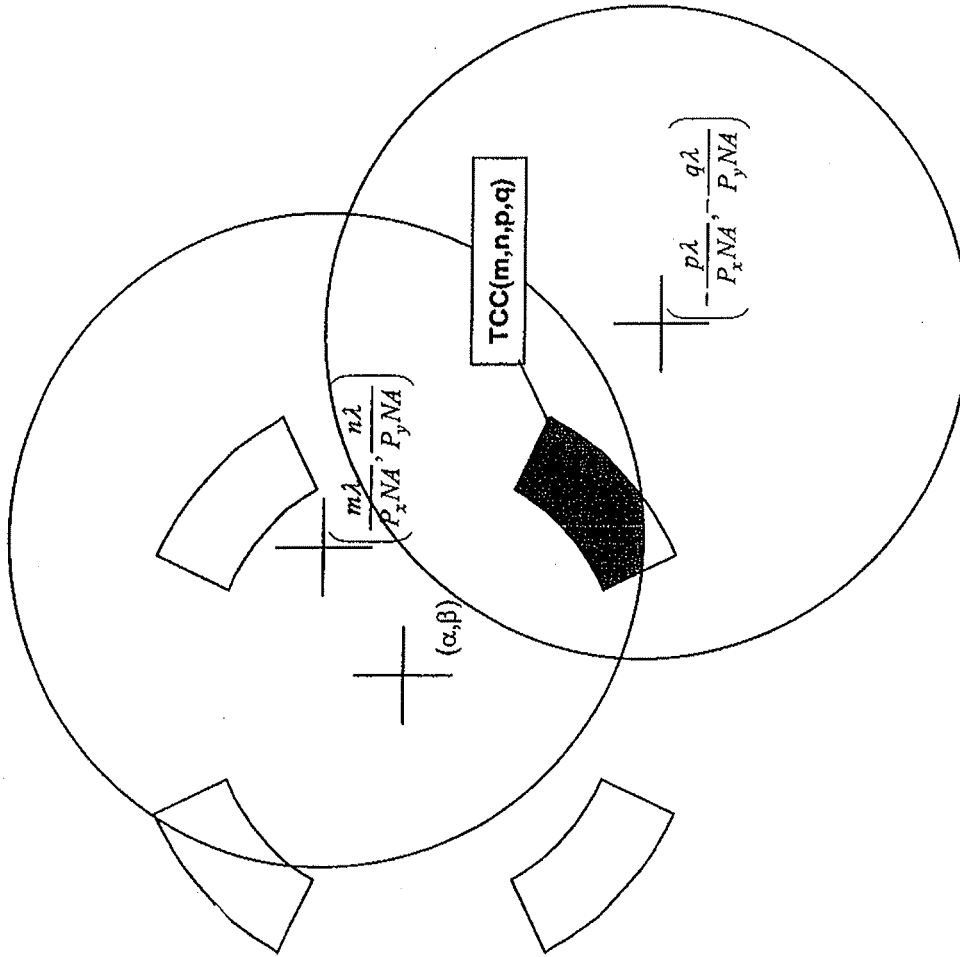


FIG. 3

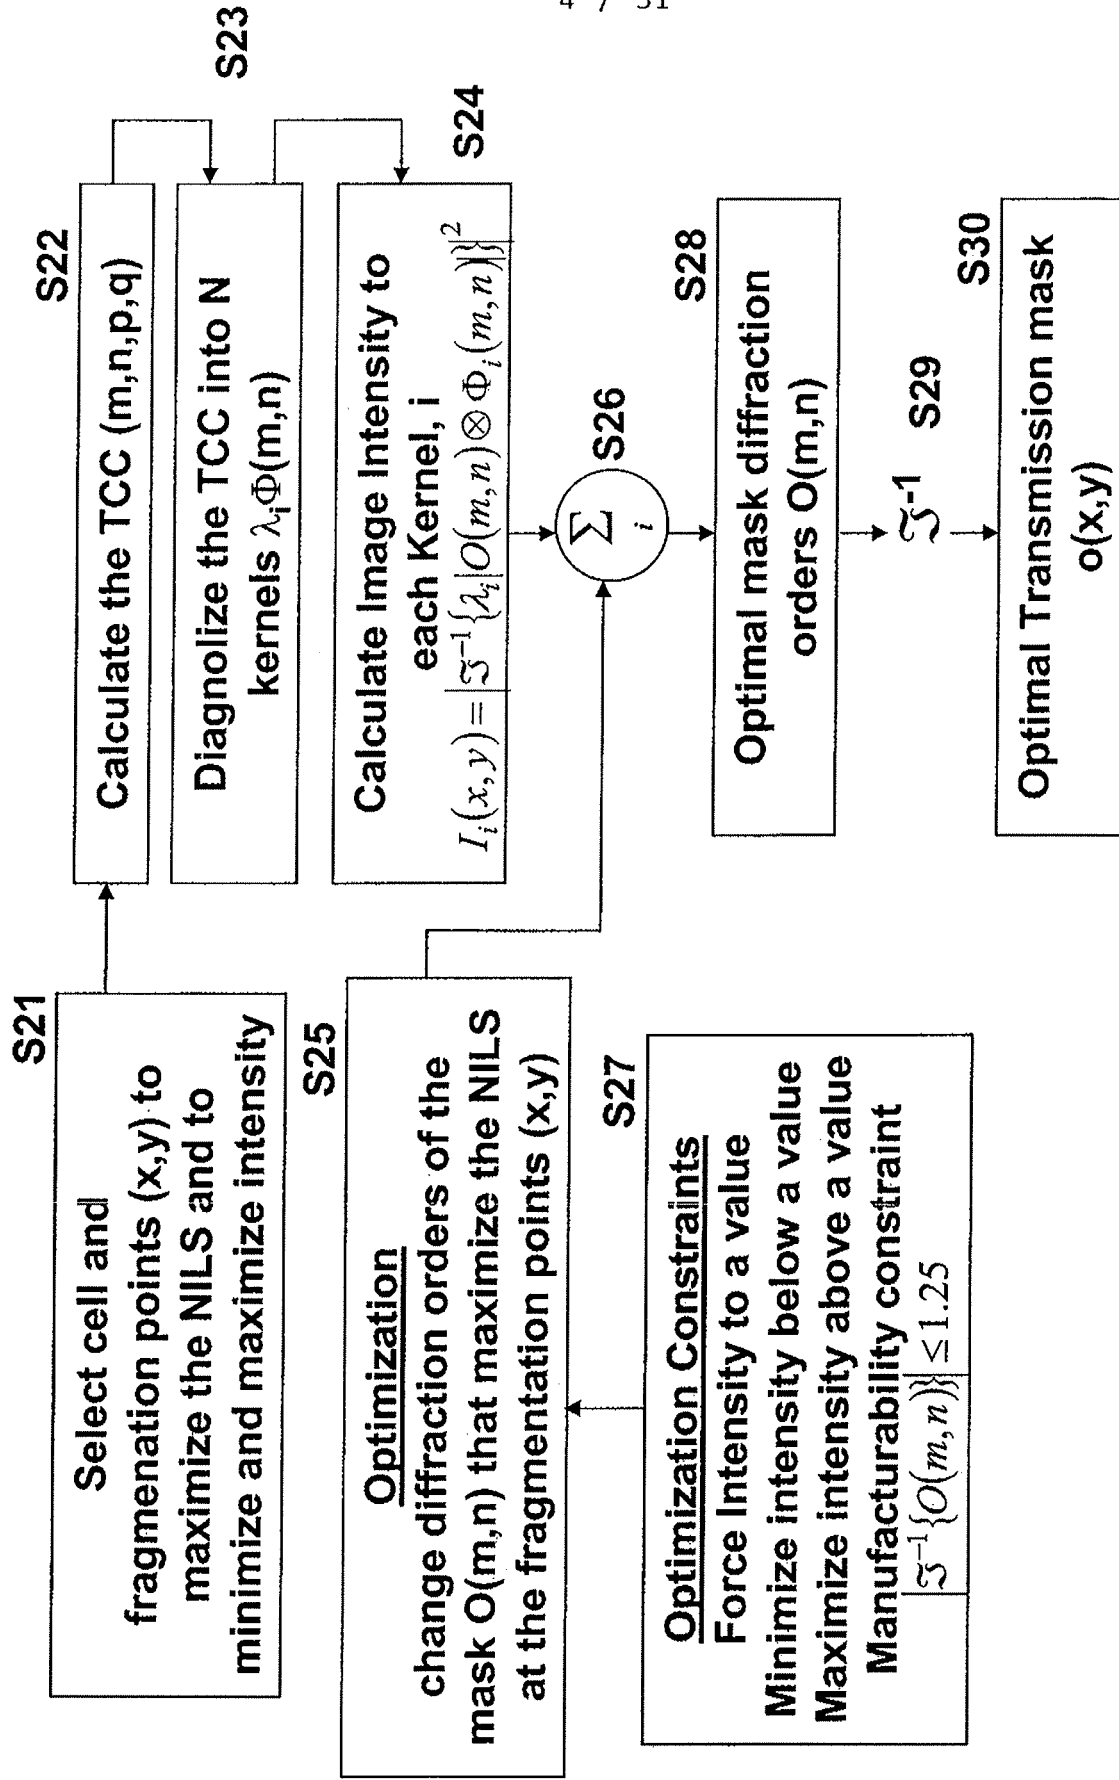


FIG. 4

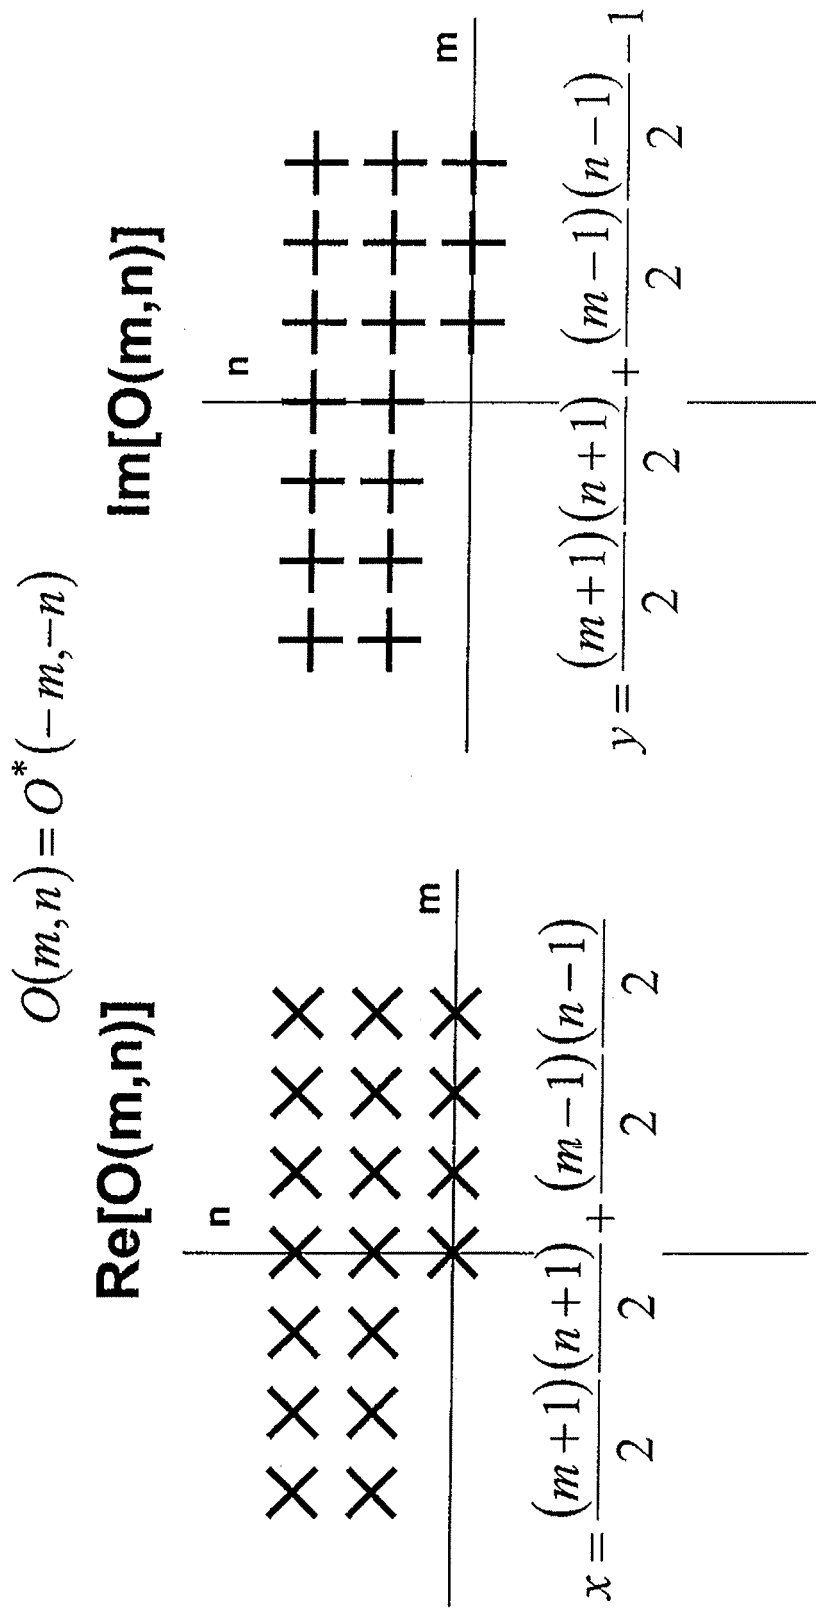


FIG. 5A

FIG. 5B

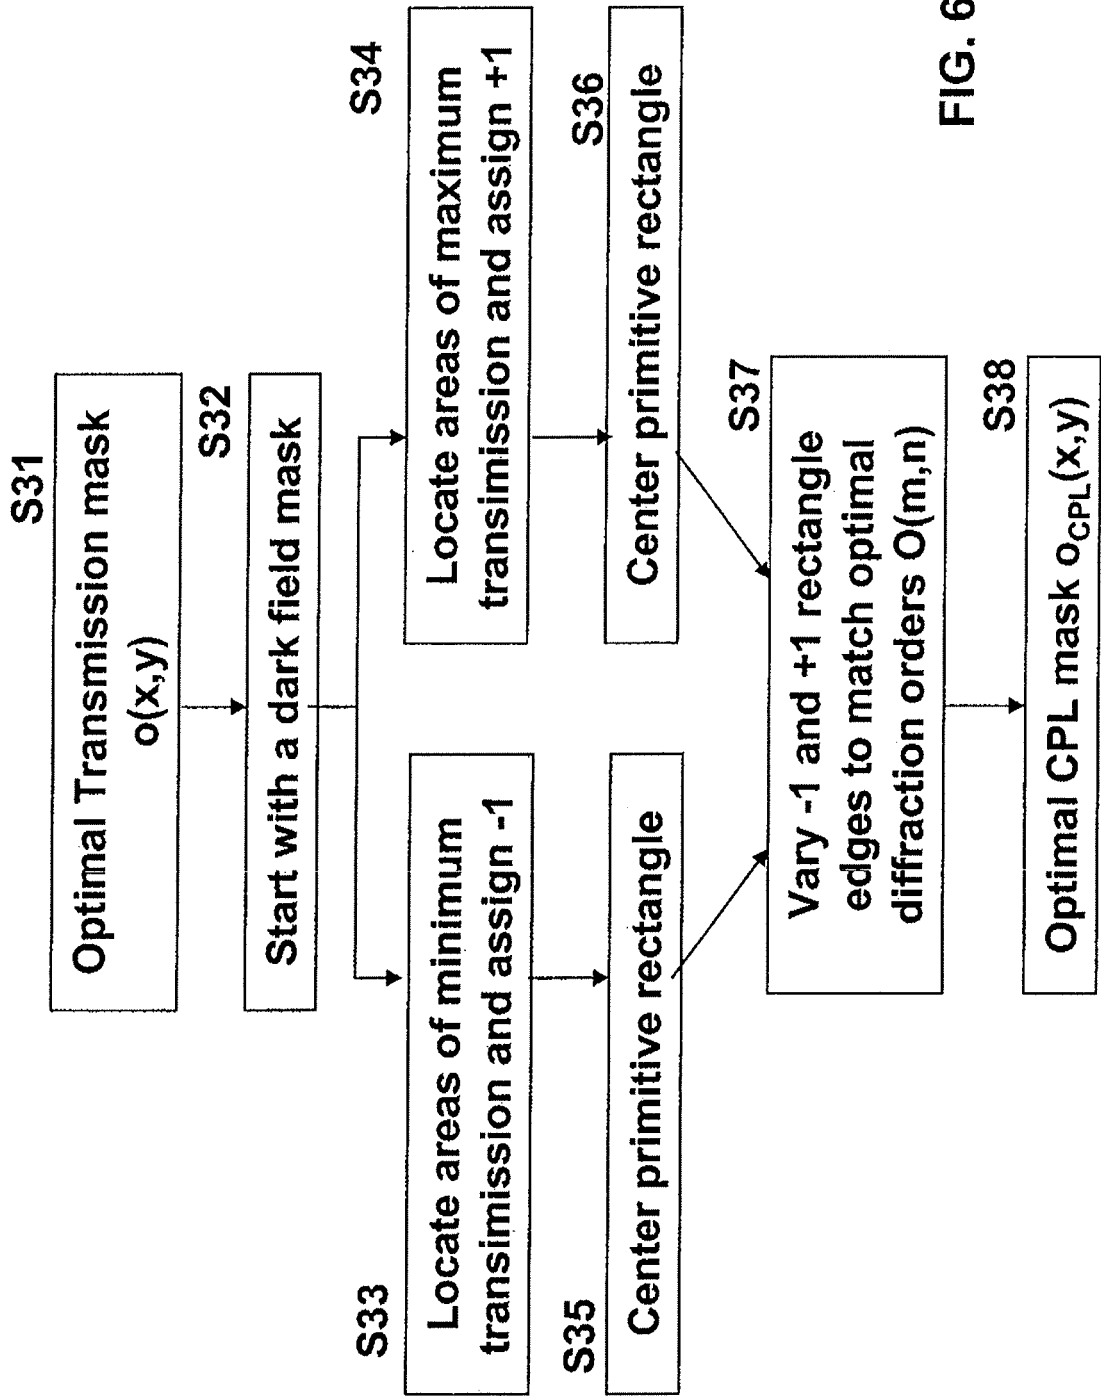


FIG. 6

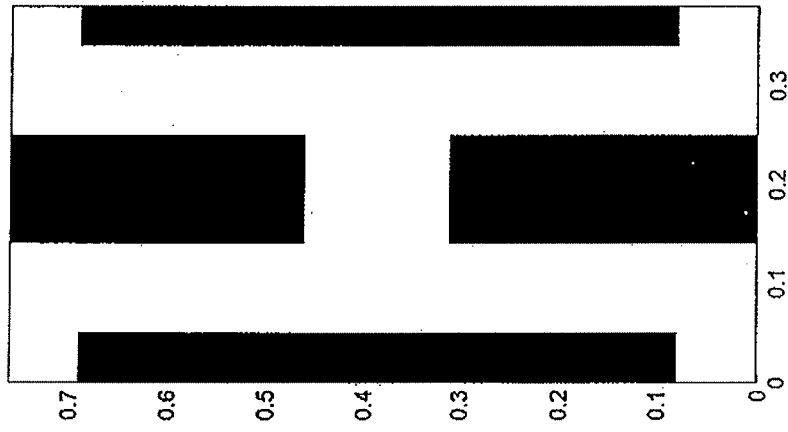


FIG. 7A

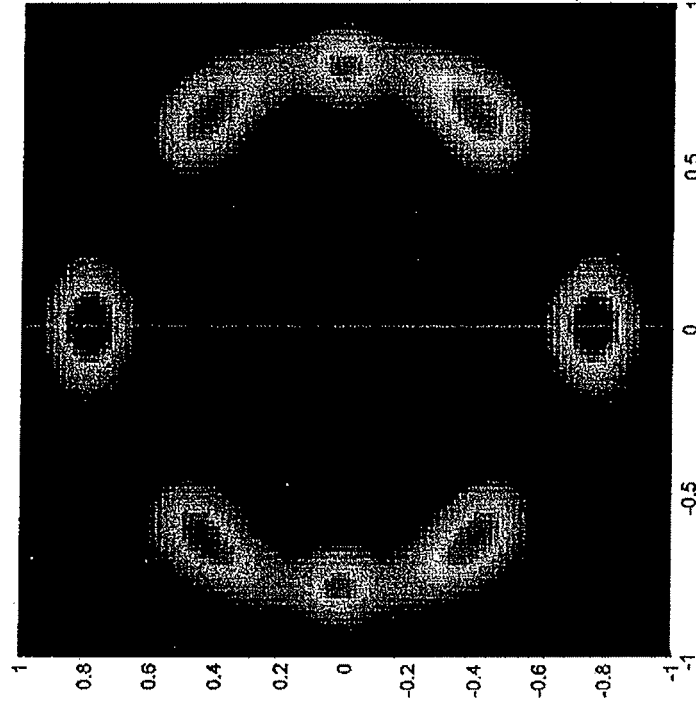


FIG. 7B

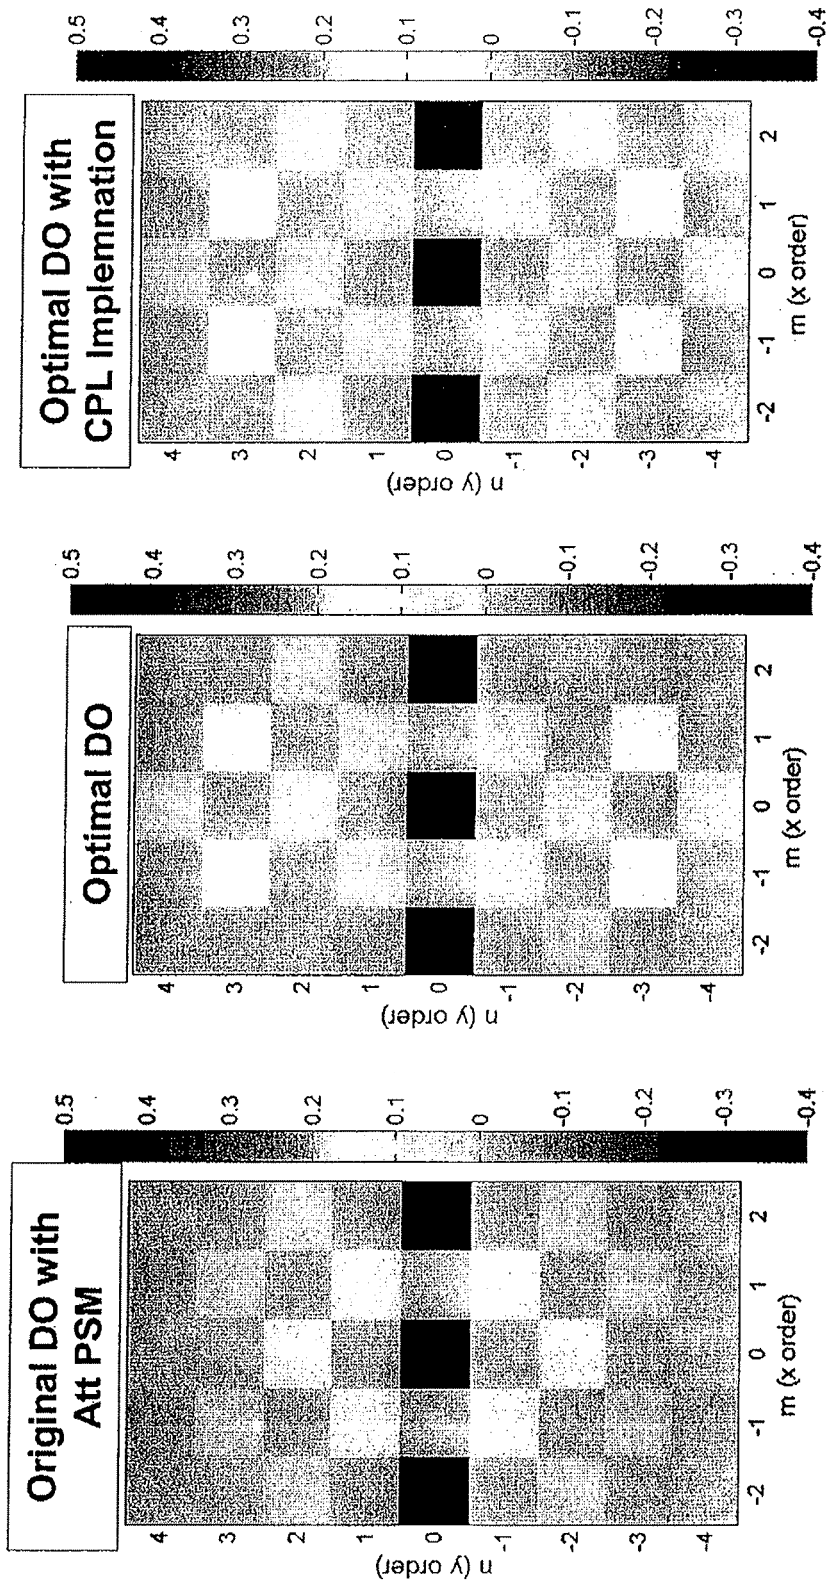


FIG. 8A

FIG. 8B

FIG. 8C

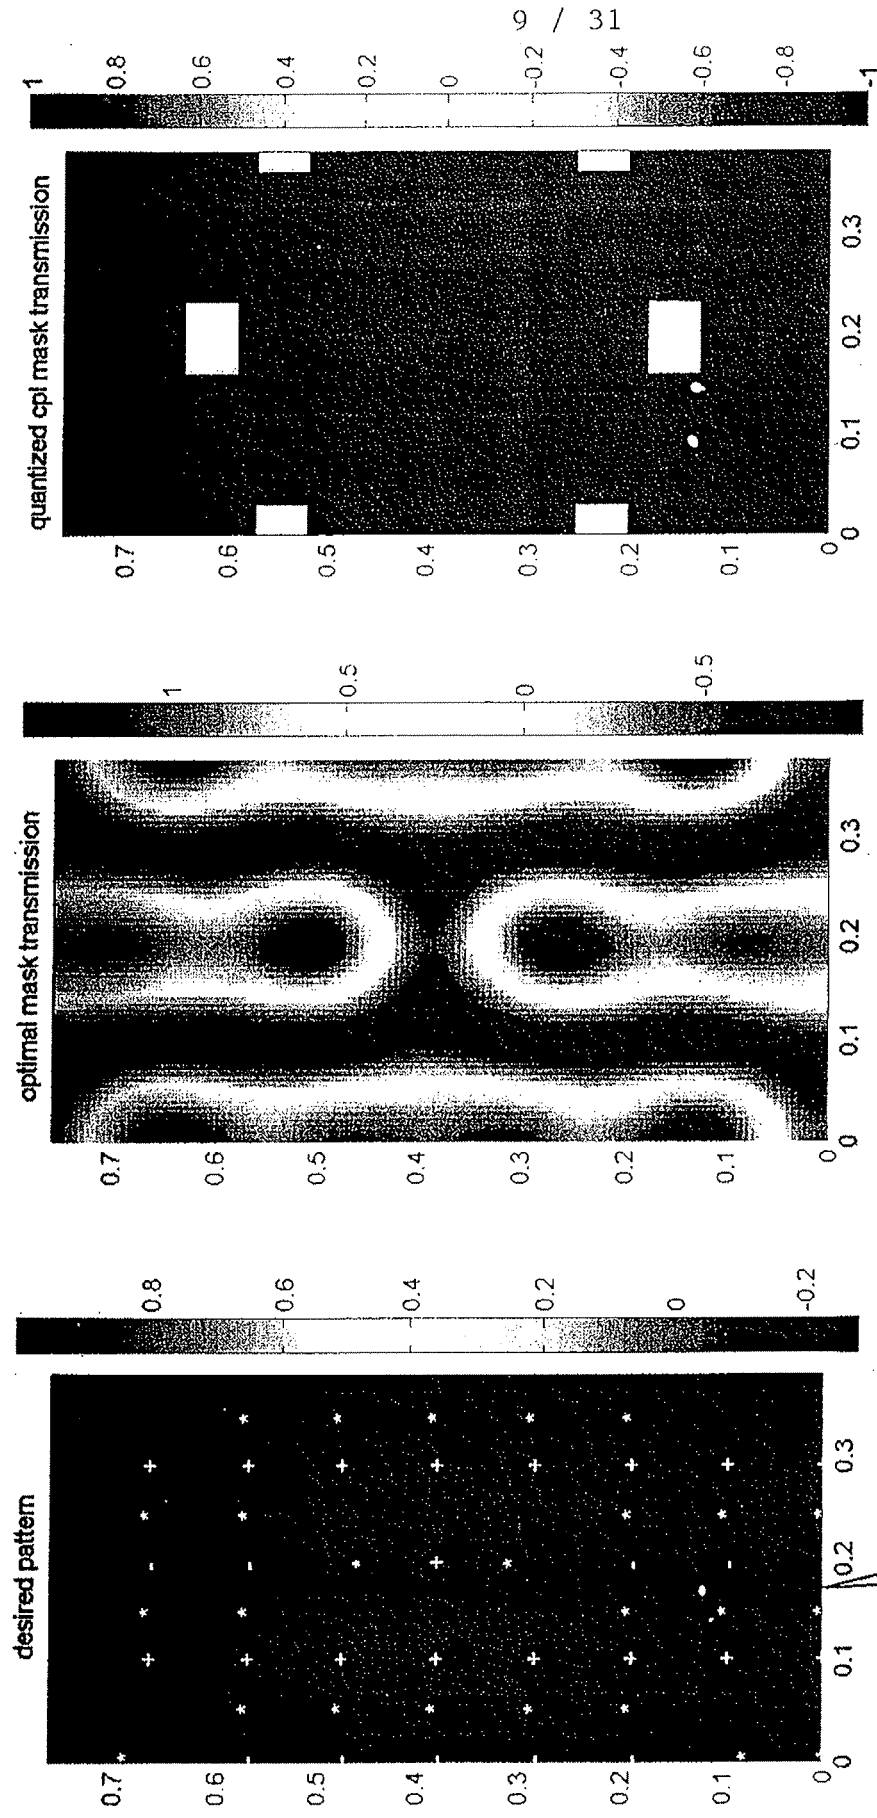
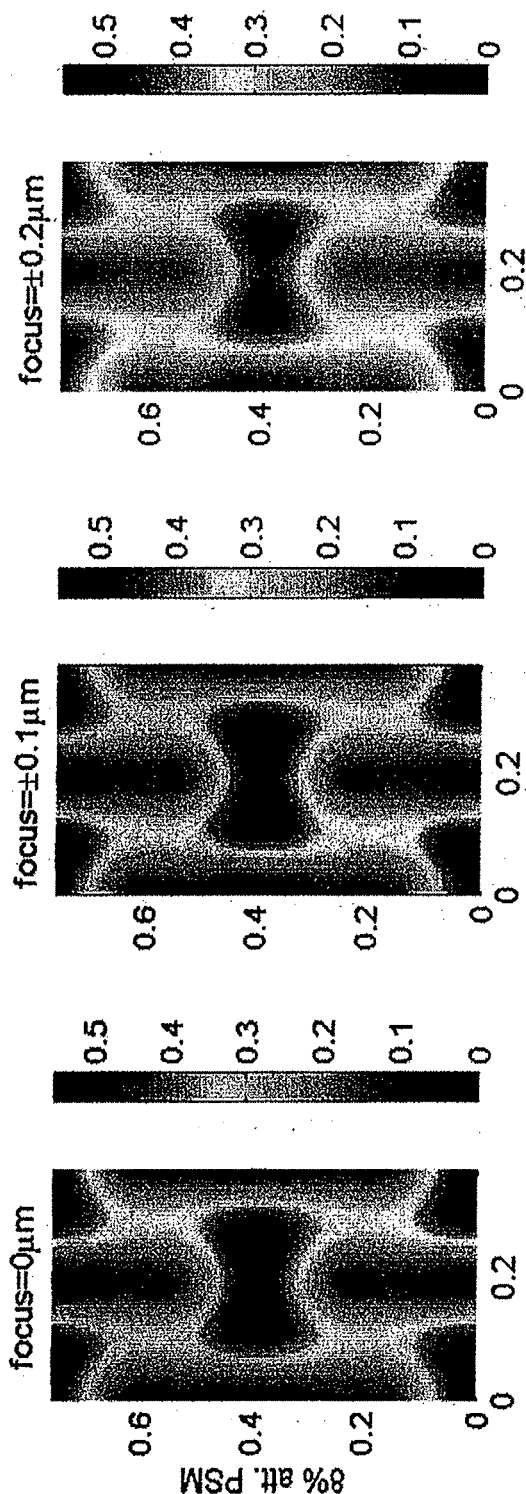
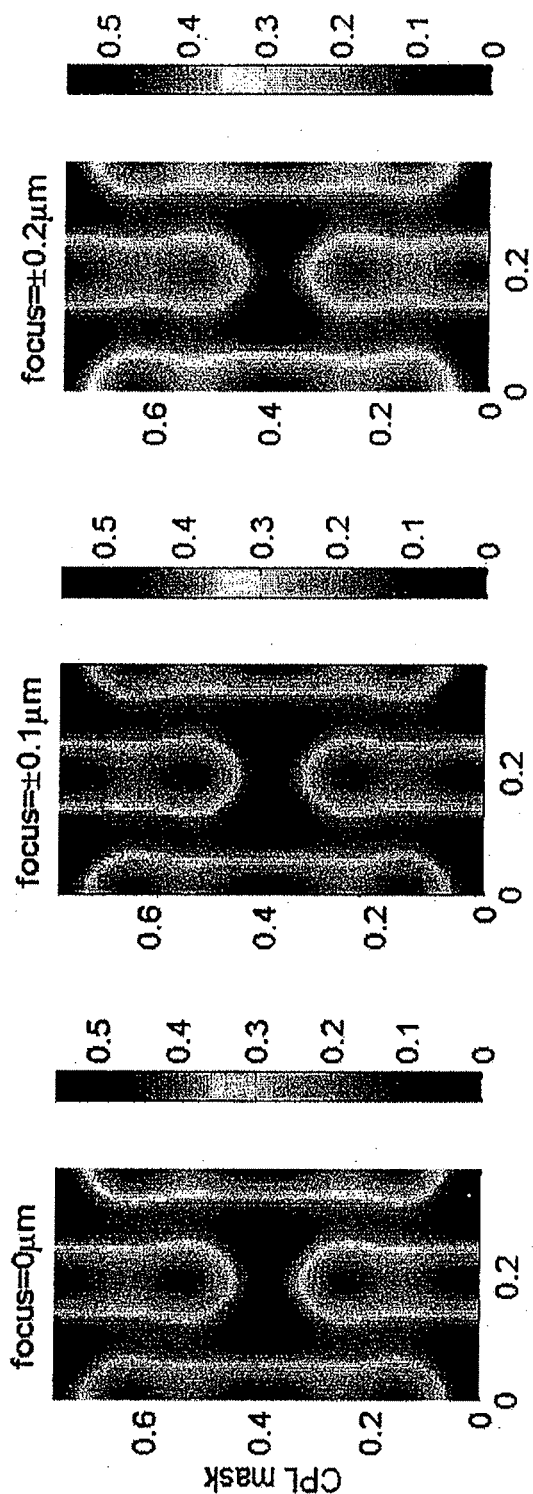


FIG. 9B

FIG. 9C

FIG. 9A



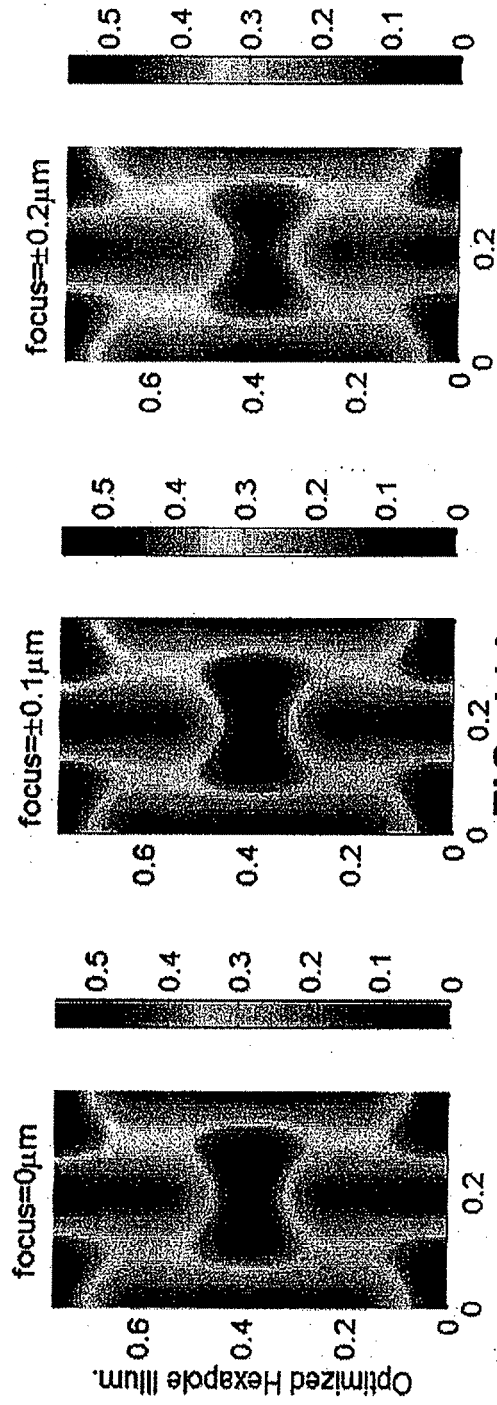


FIG. 11A

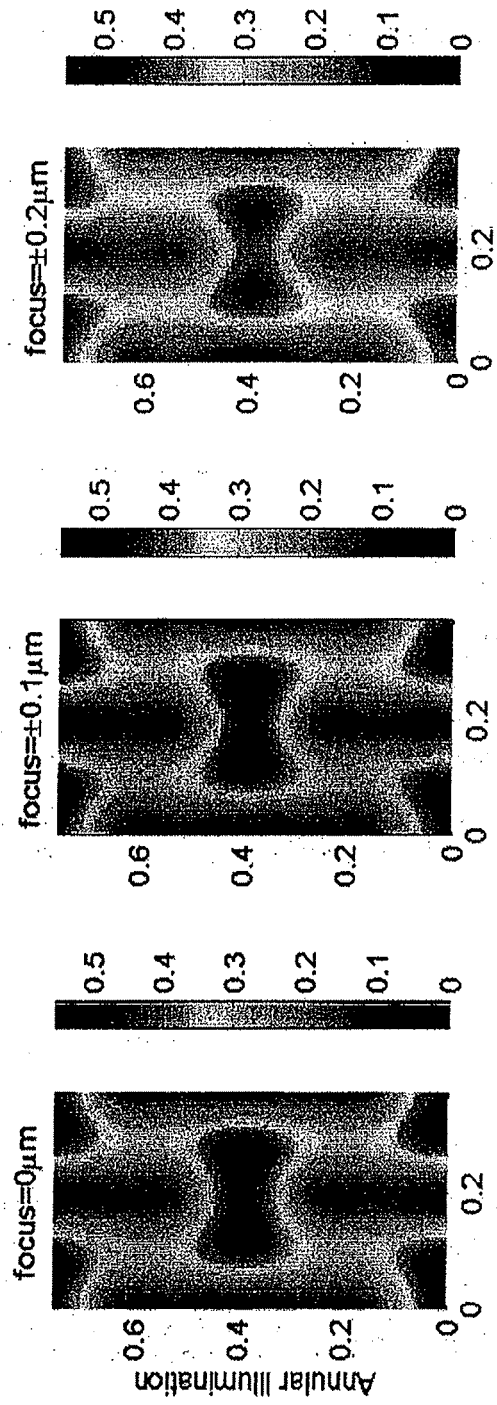


FIG. 11B

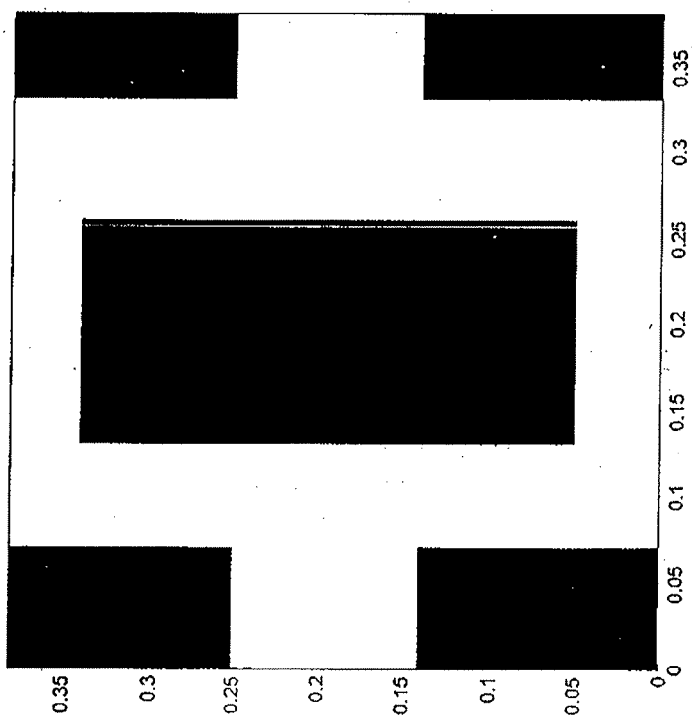


FIG. 12A

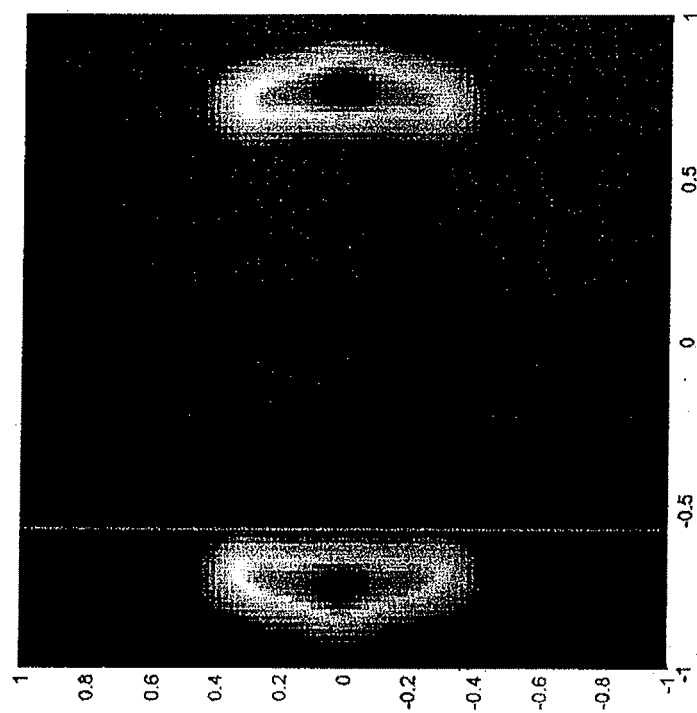


FIG. 12B

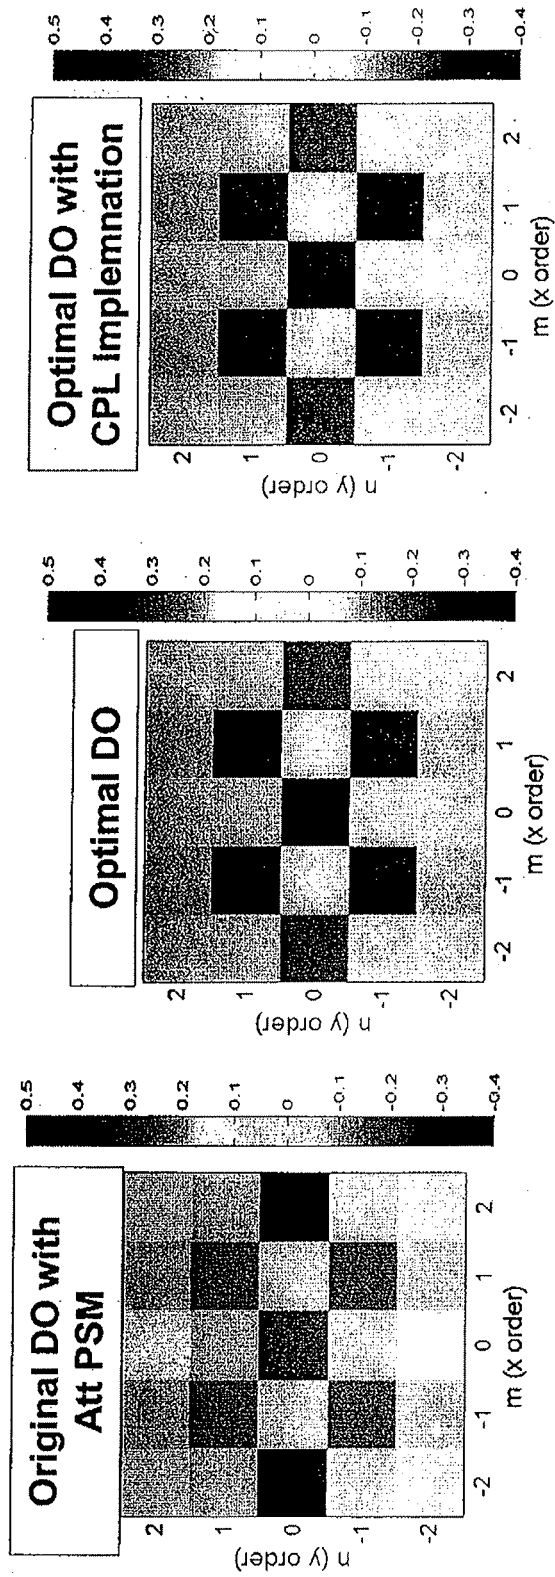


FIG. 13A

FIG. 13B

FIG. 13C

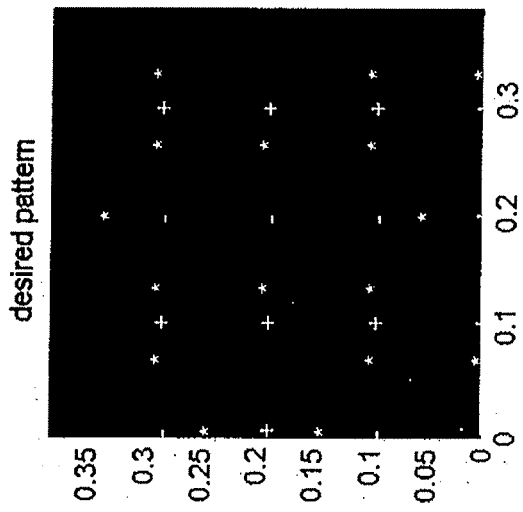


FIG. 14A

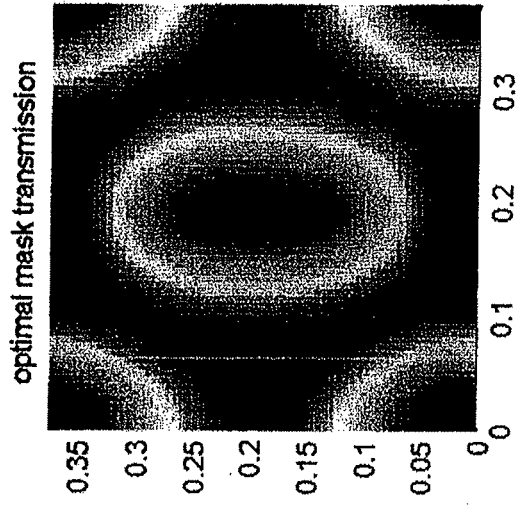


FIG. 14B

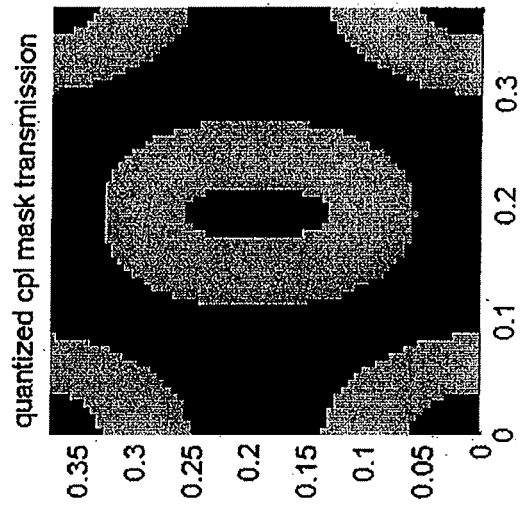


FIG. 14C

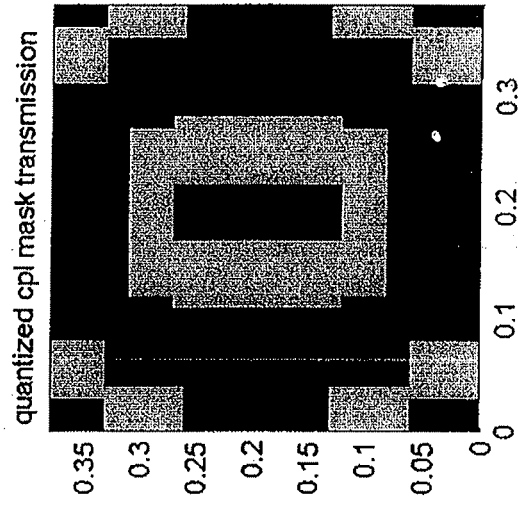


FIG. 14D

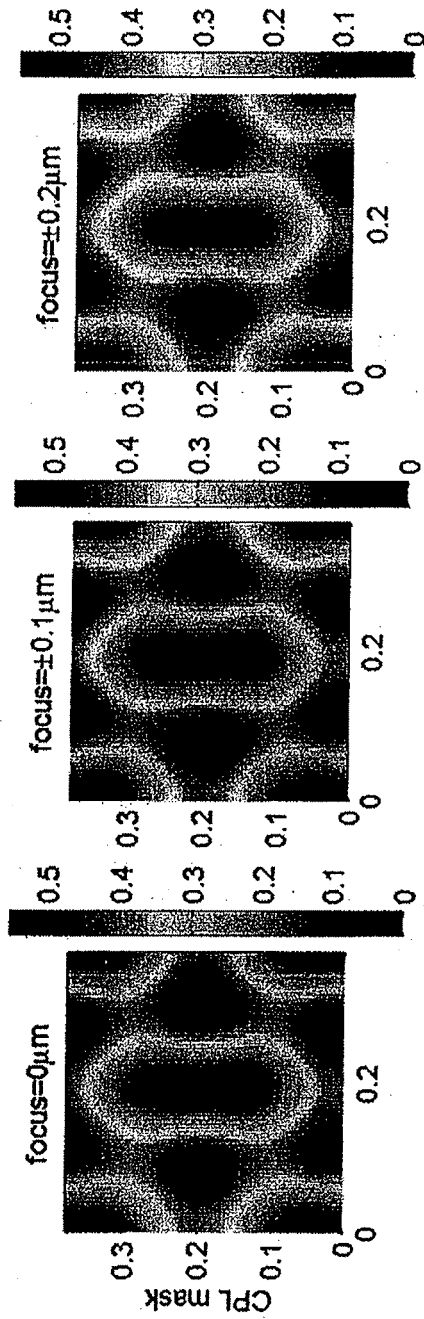


FIG. 15A

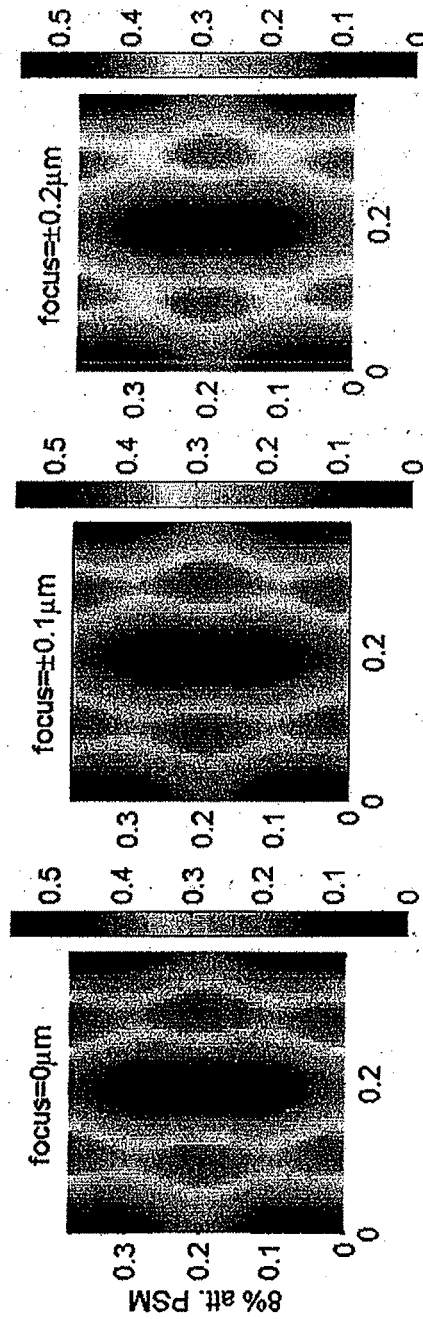


FIG. 15B

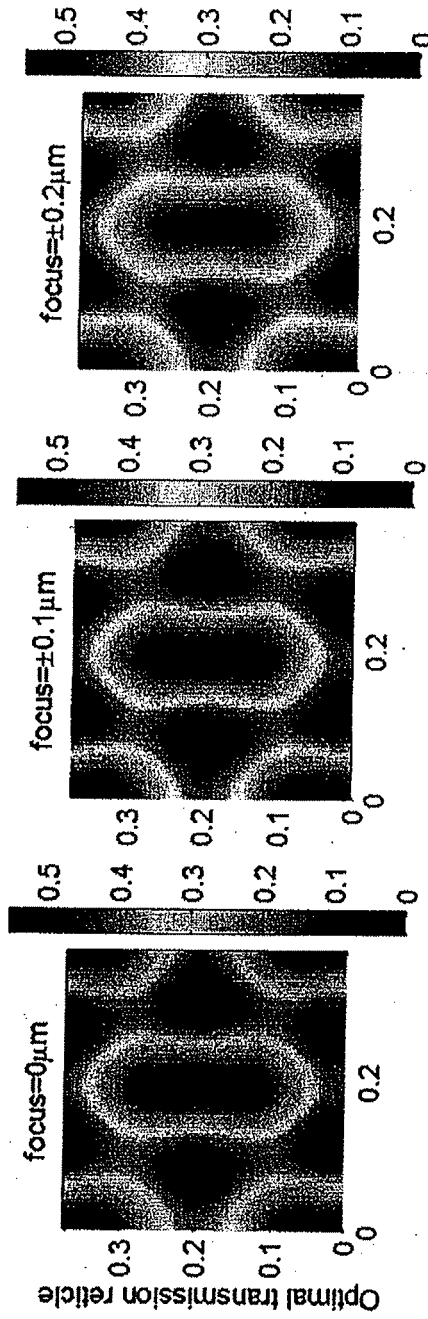


FIG. 16A

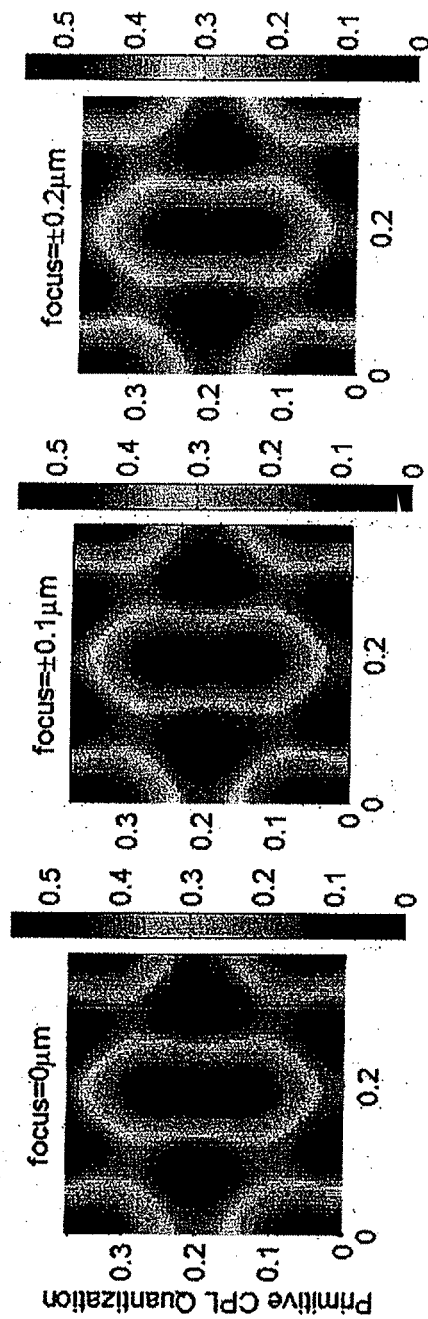


FIG. 16B

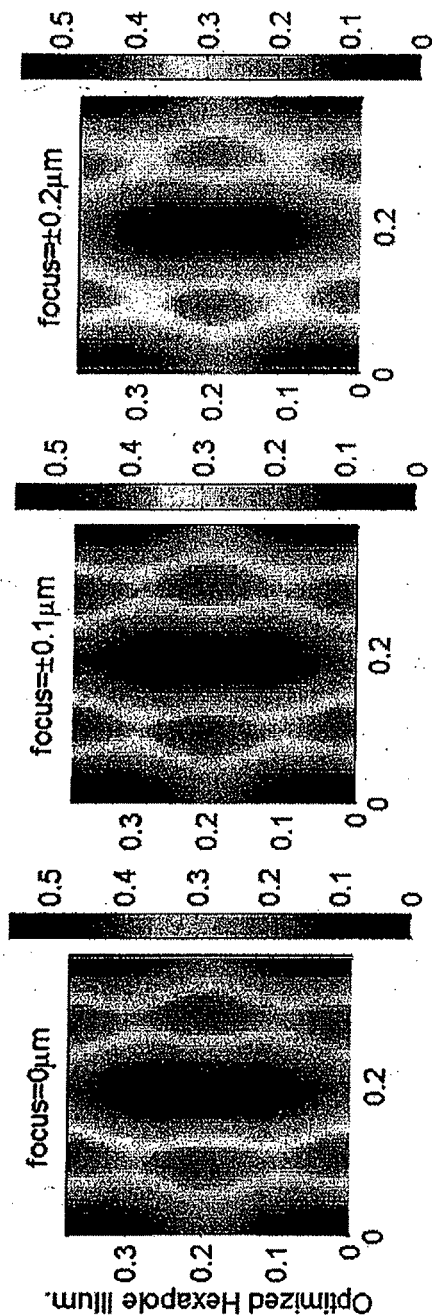


FIG. 17A

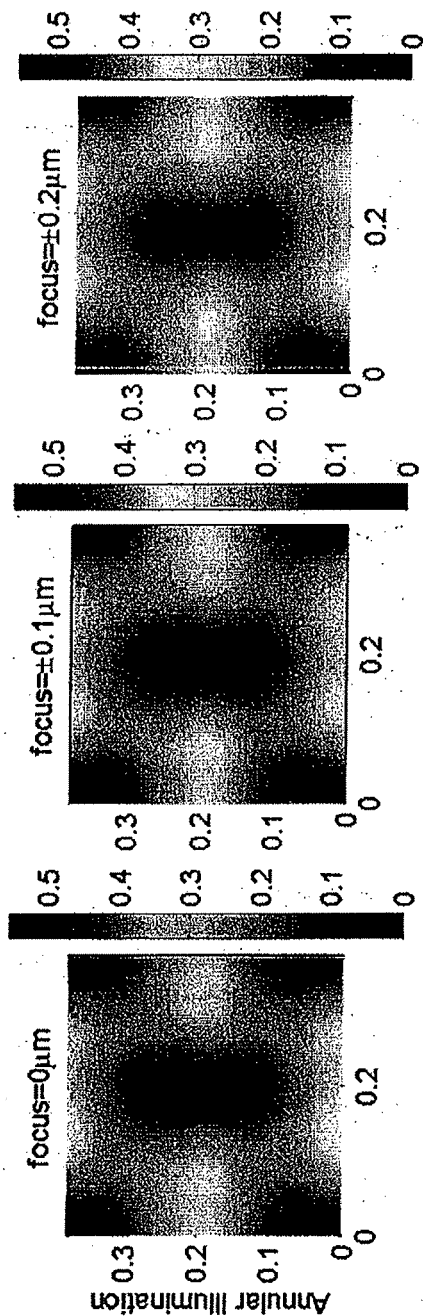


FIG. 17B



FIG. 18B

FIG. 18A

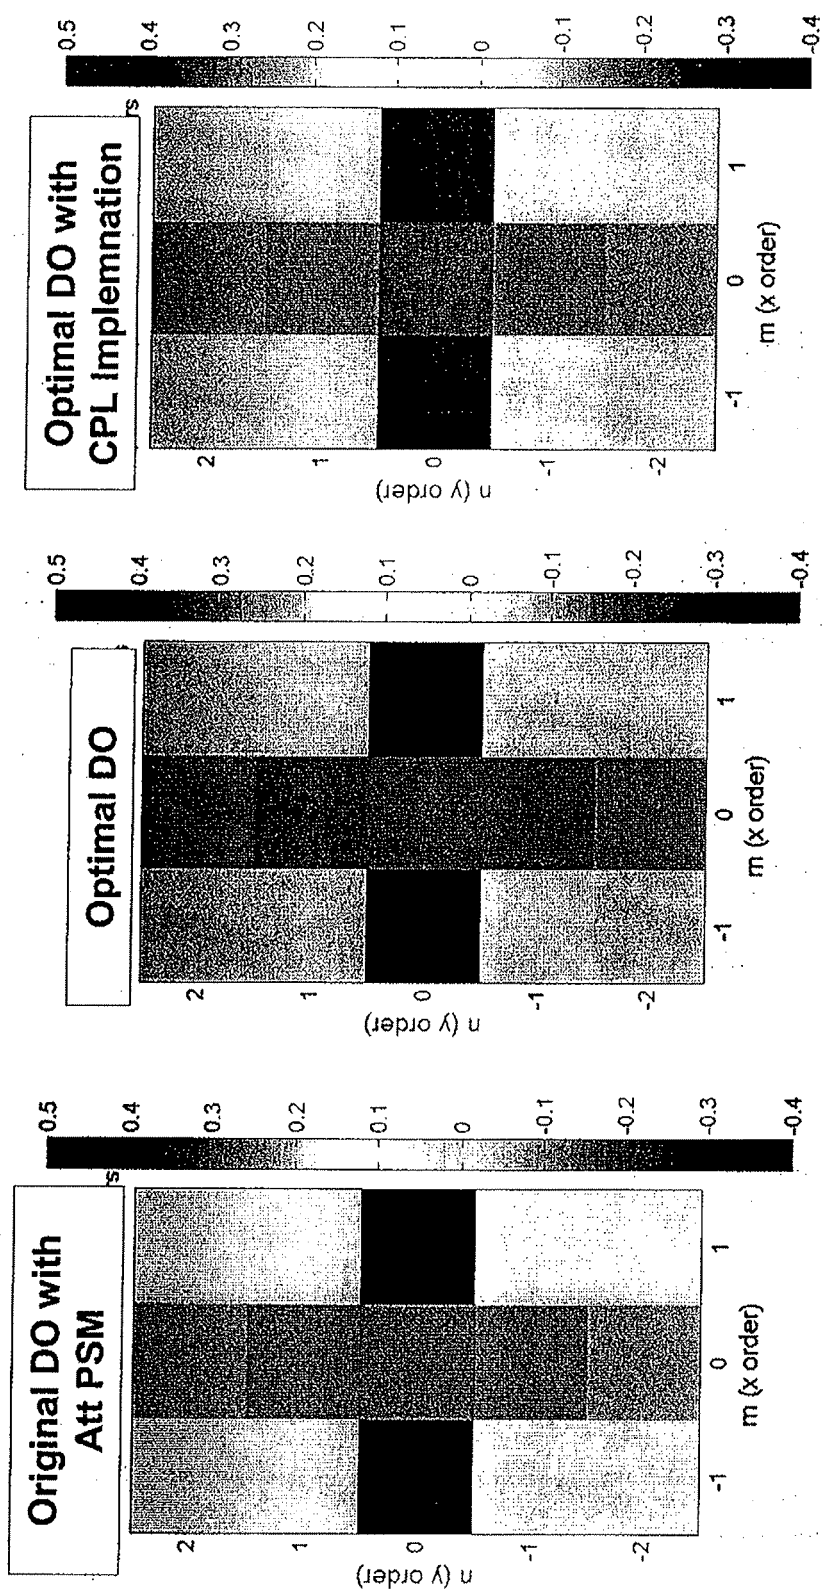


FIG. 19A

FIG. 19B

FIG. 19C

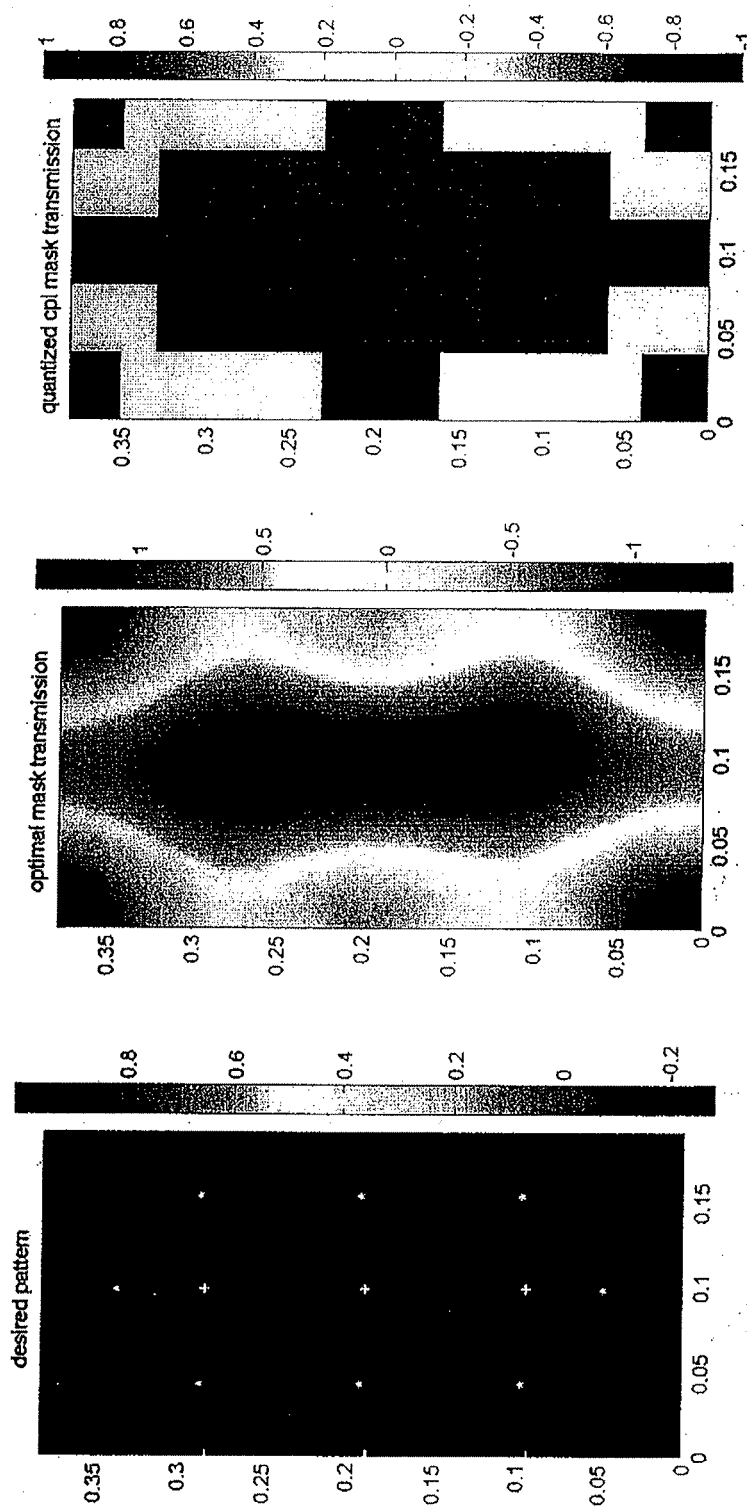


FIG. 20A

FIG. 20B

FIG. 20C

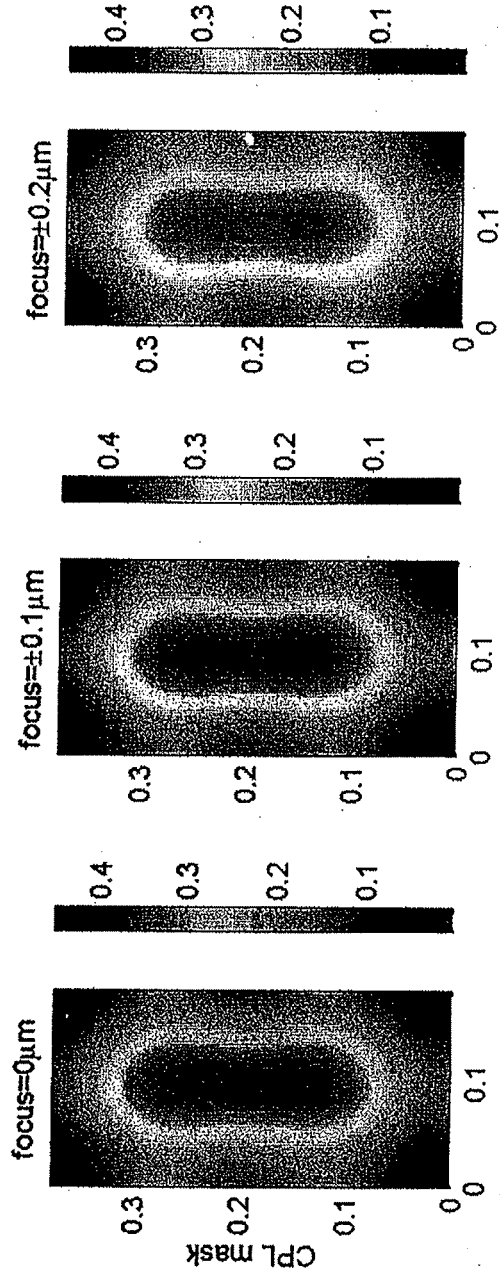


FIG. 21A

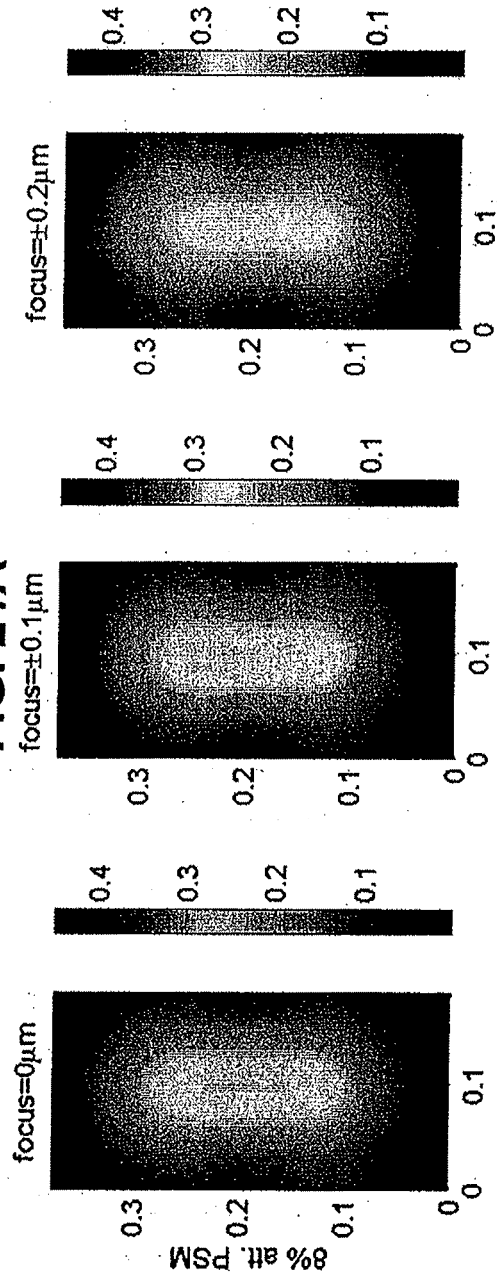


FIG. 21B

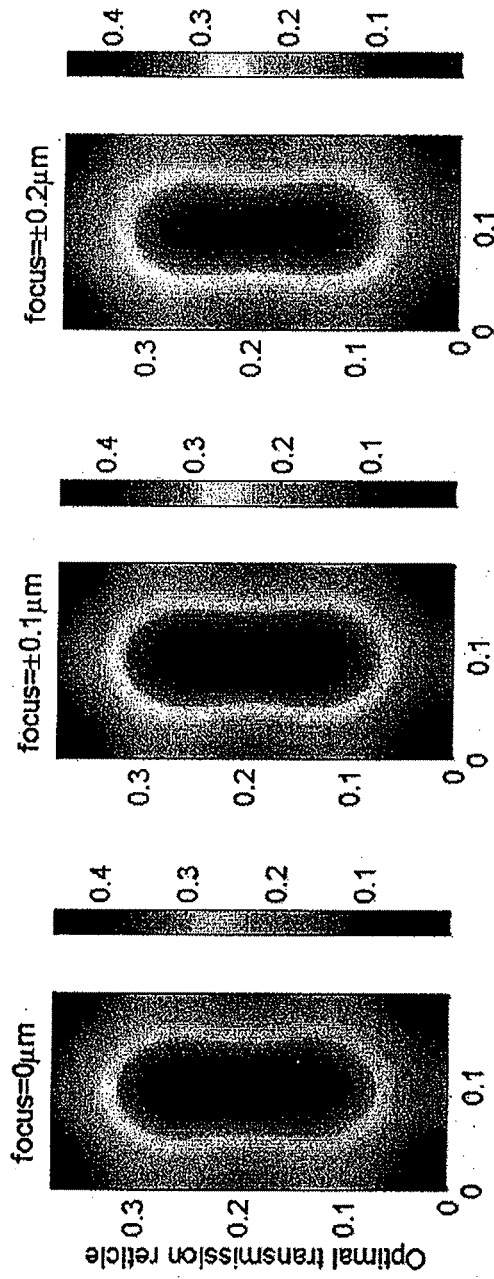


FIG. 22A

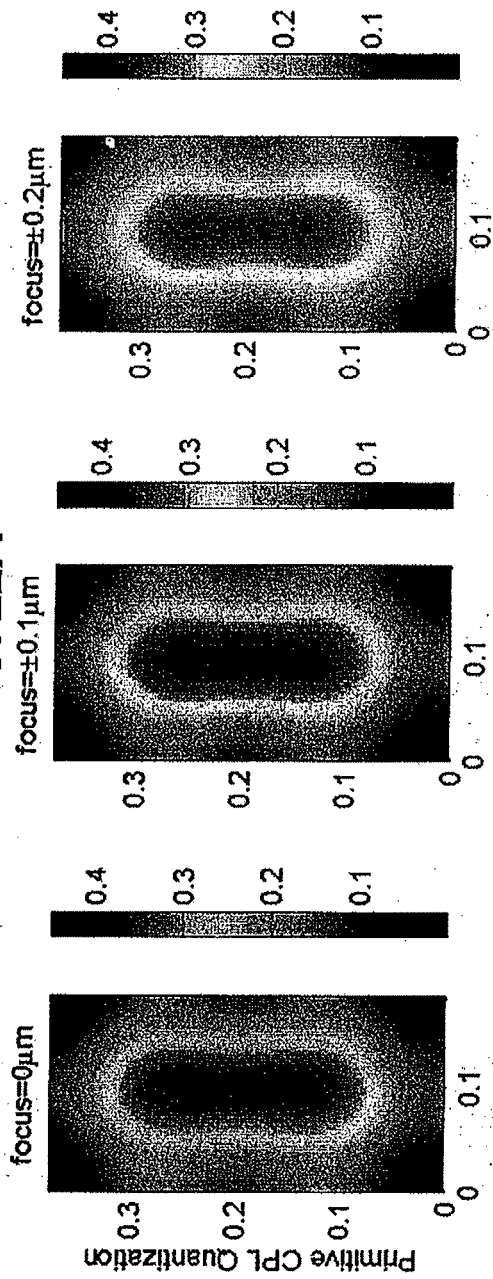


FIG. 22B

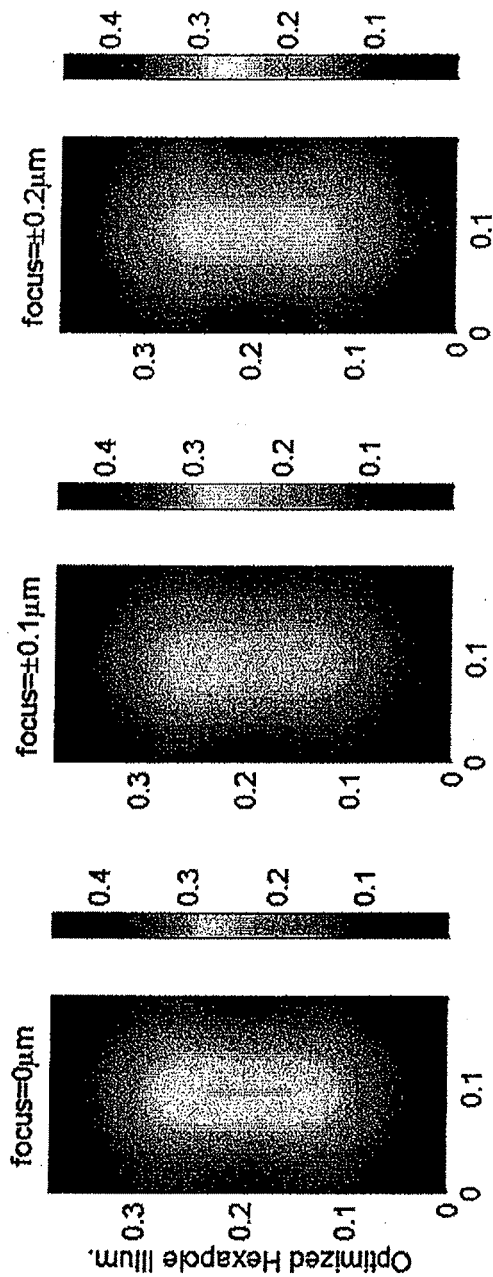


FIG. 23A

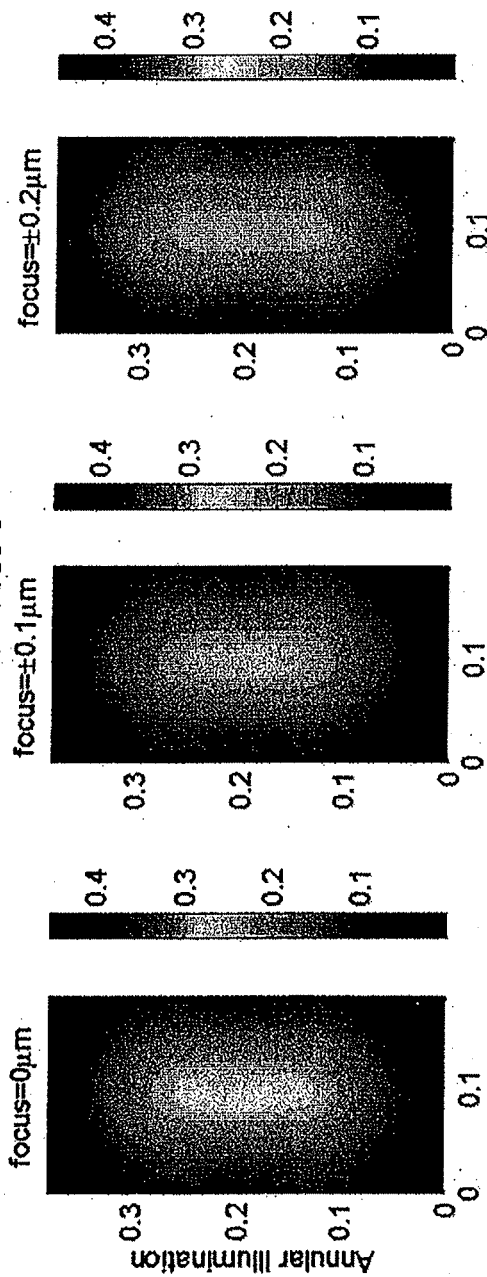


FIG. 23B

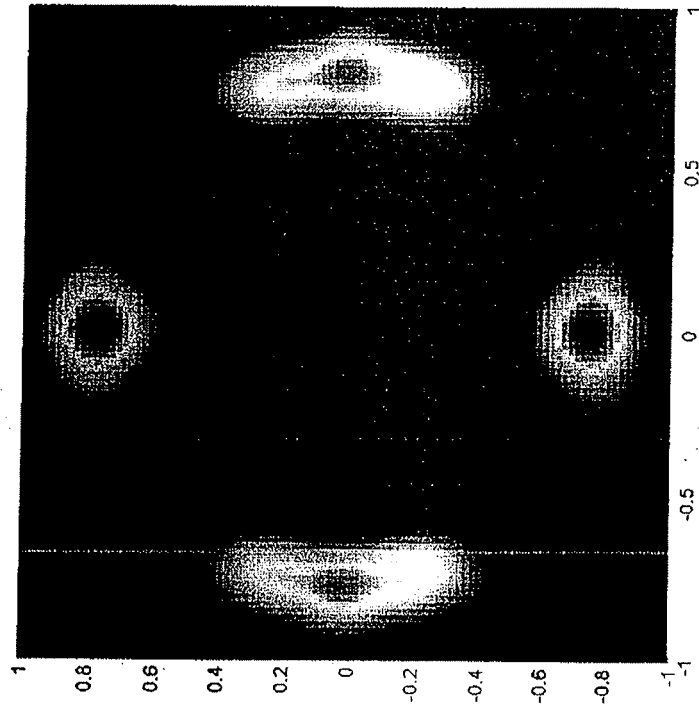


FIG. 24B

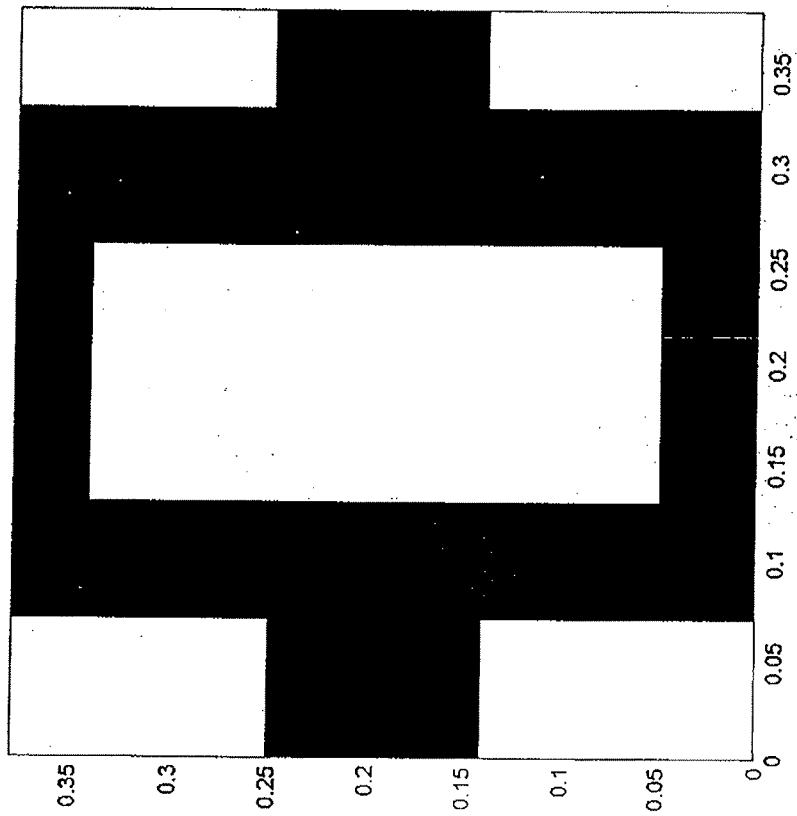


FIG. 24A

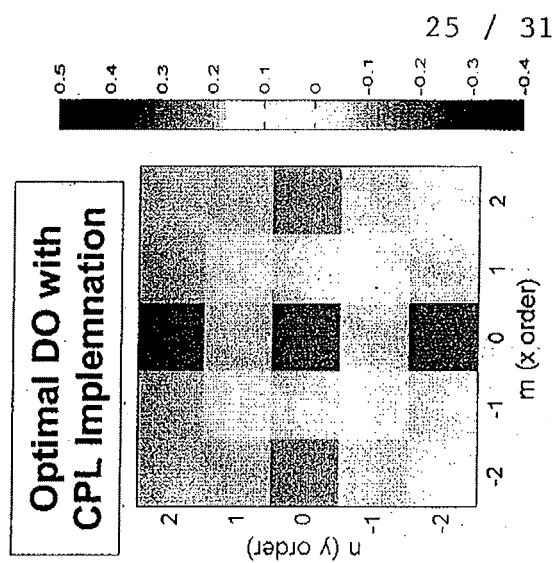
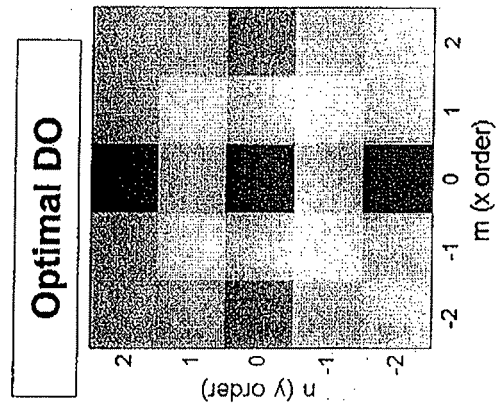
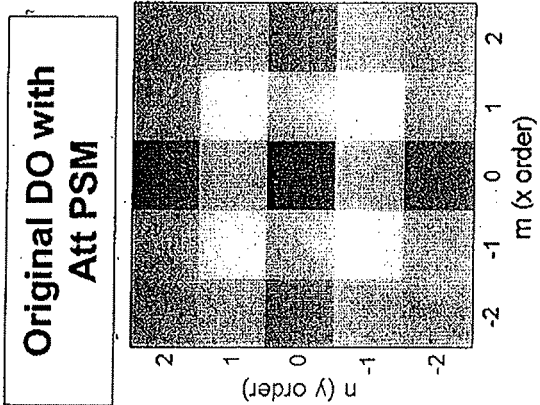


FIG. 25A

FIG. 25B

FIG. 25C

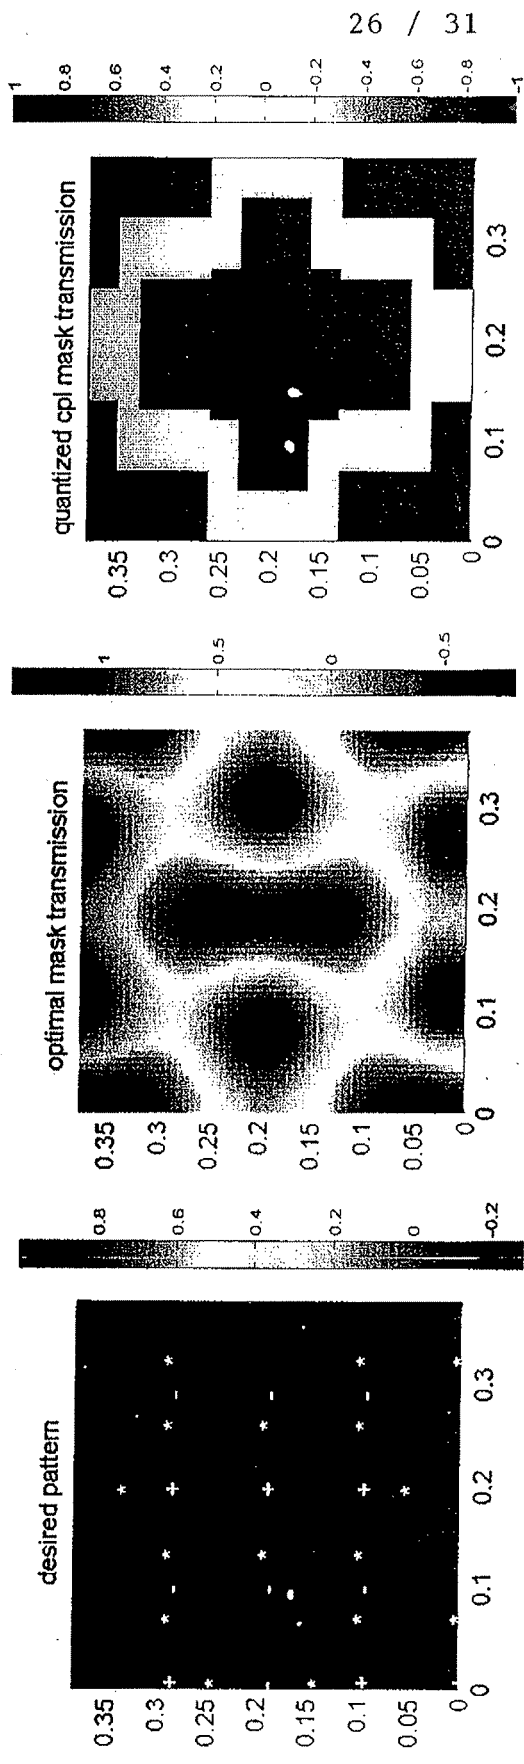


FIG. 26A

FIG. 26B

FIG. 26C

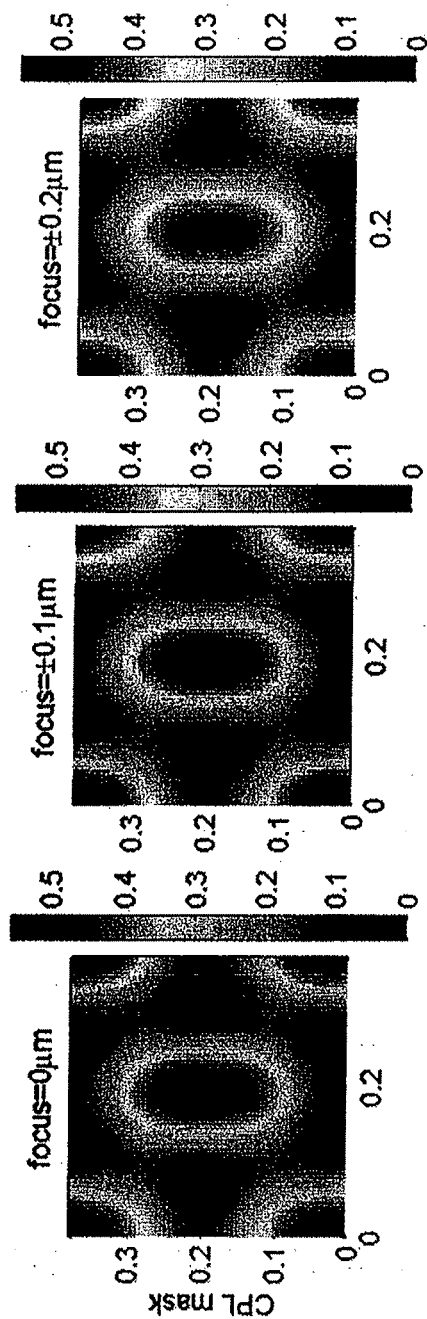


FIG. 27A

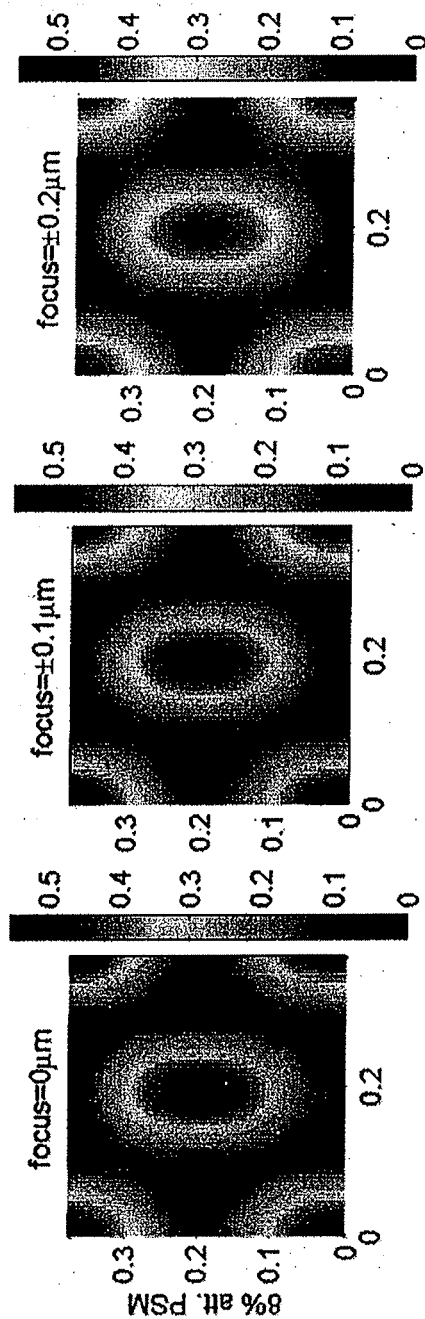


FIG. 27B

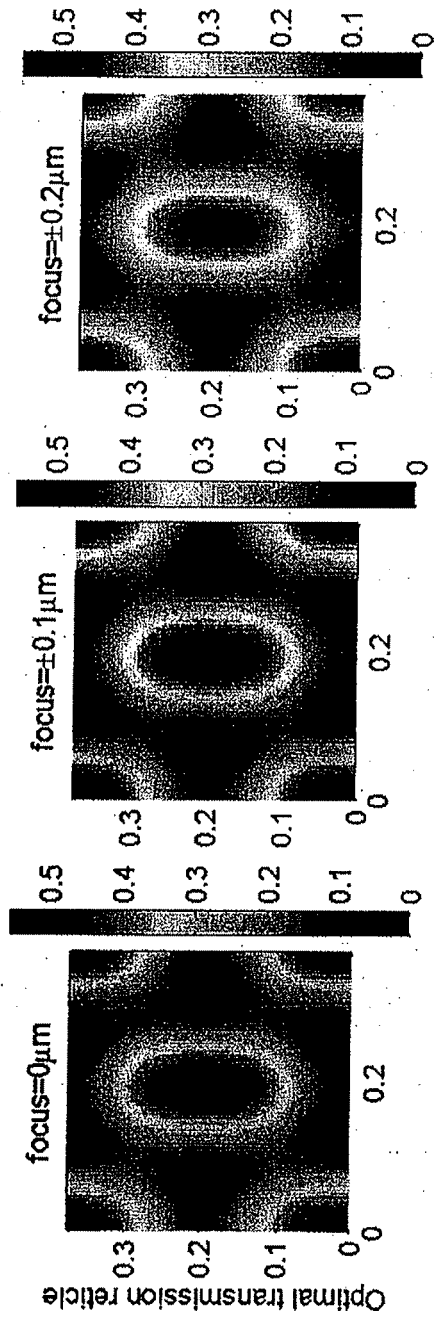


FIG. 28A

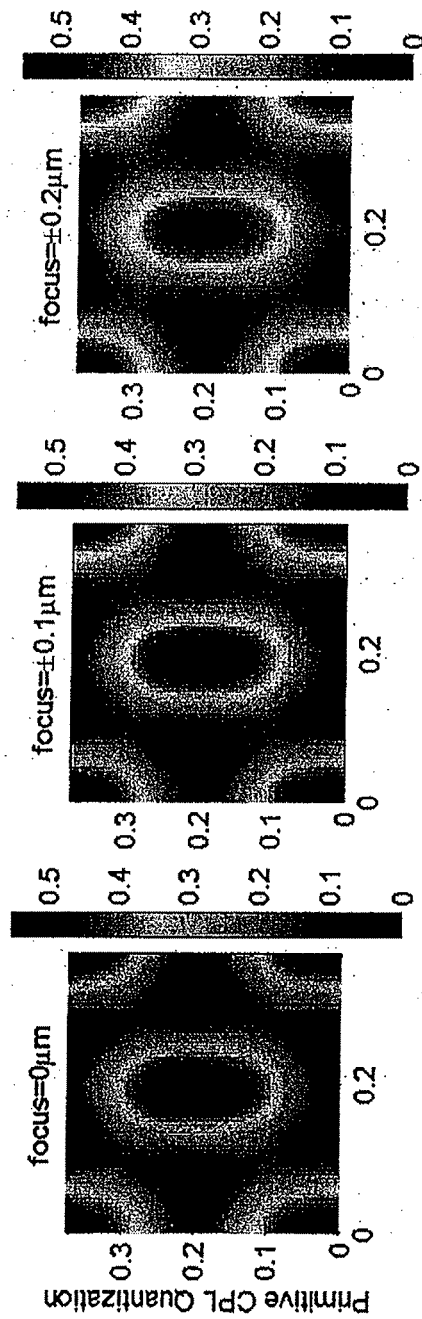


FIG. 28B

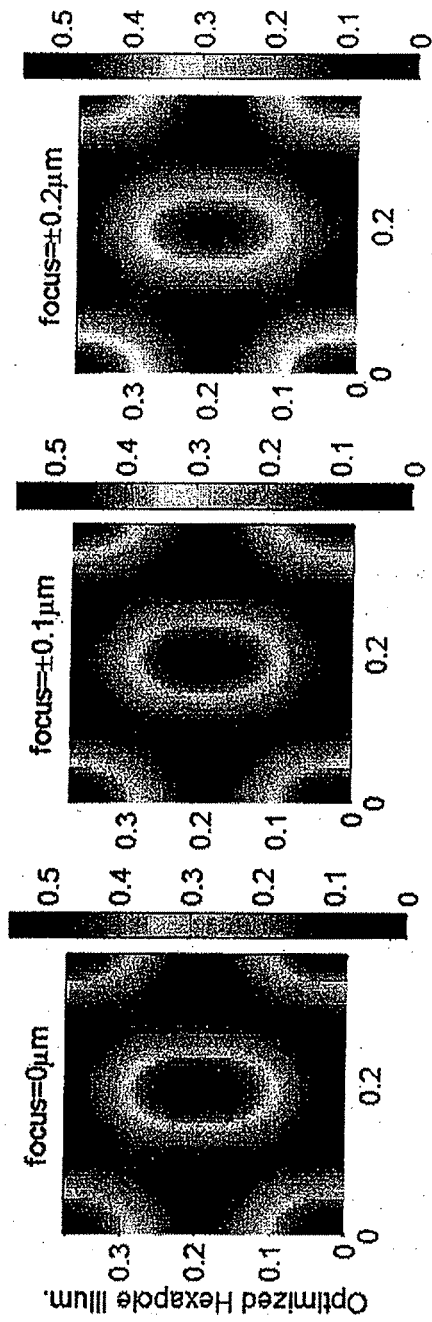


FIG. 29A

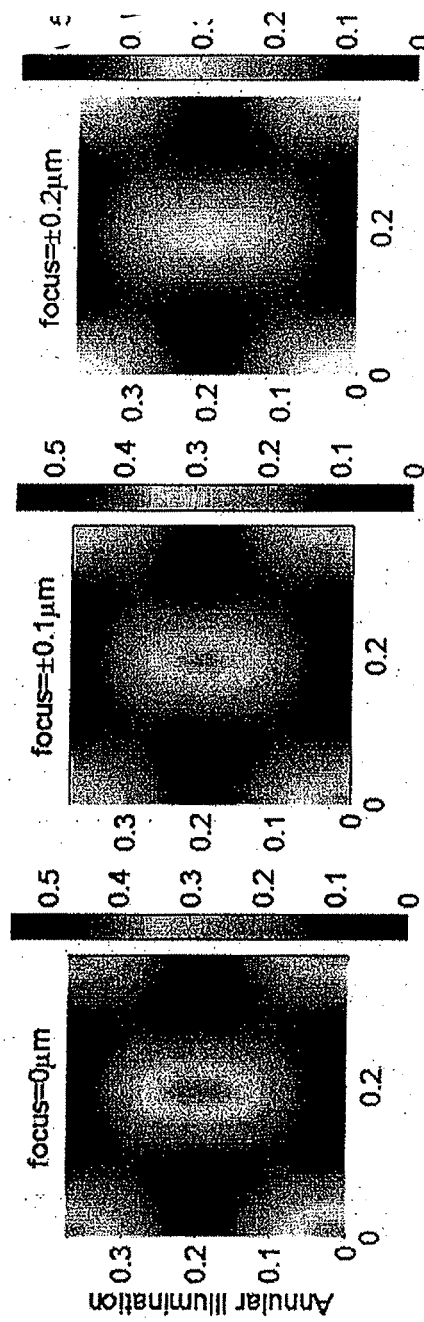


FIG. 29B

FIG. 30

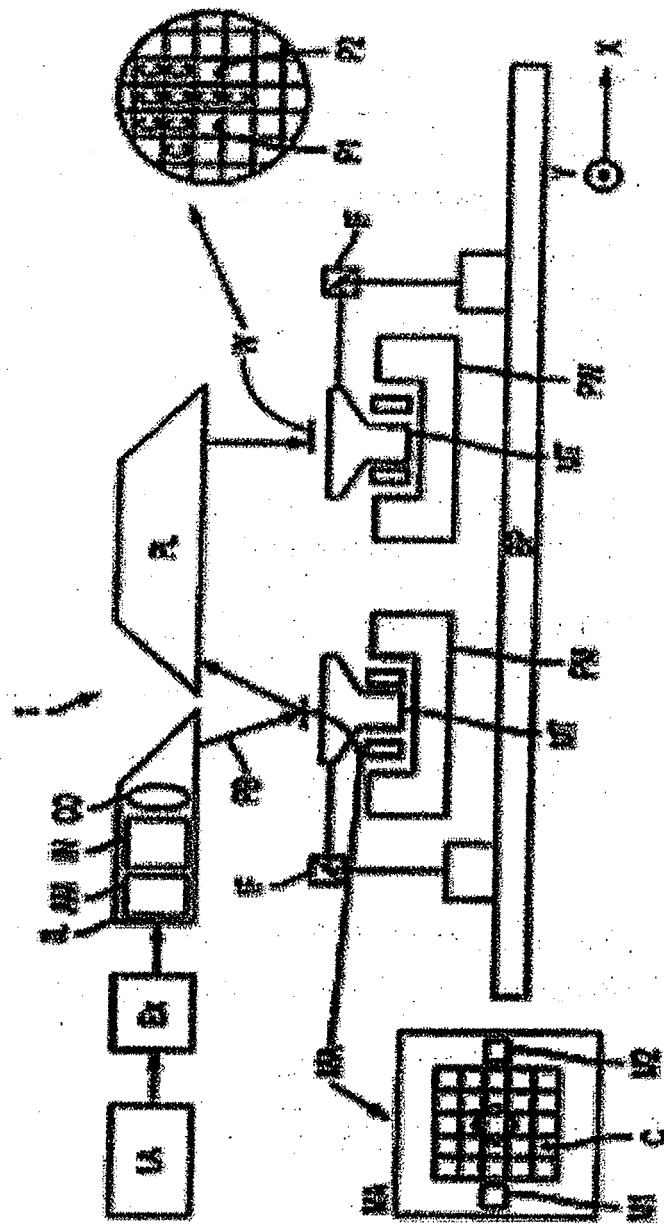


FIG. 31