

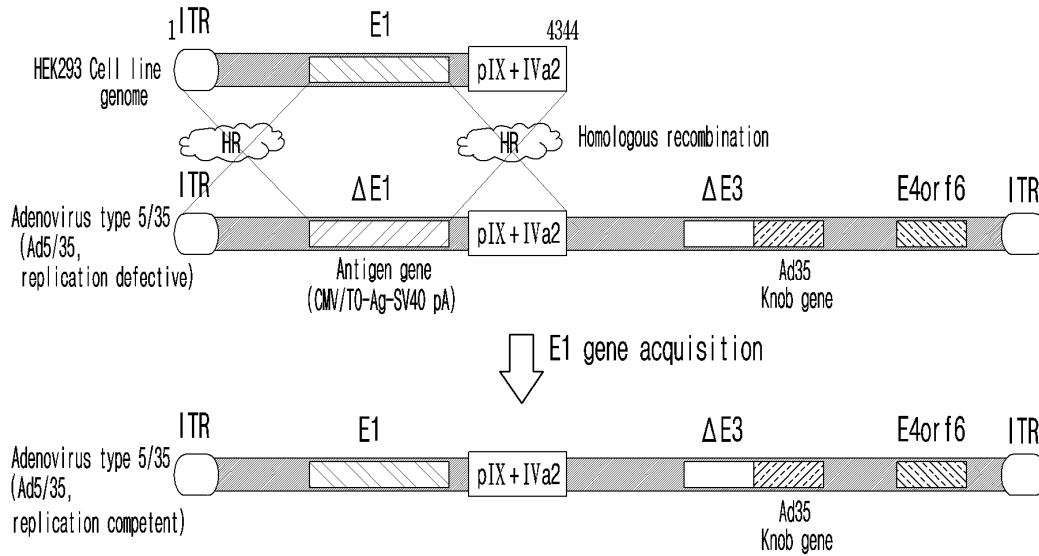
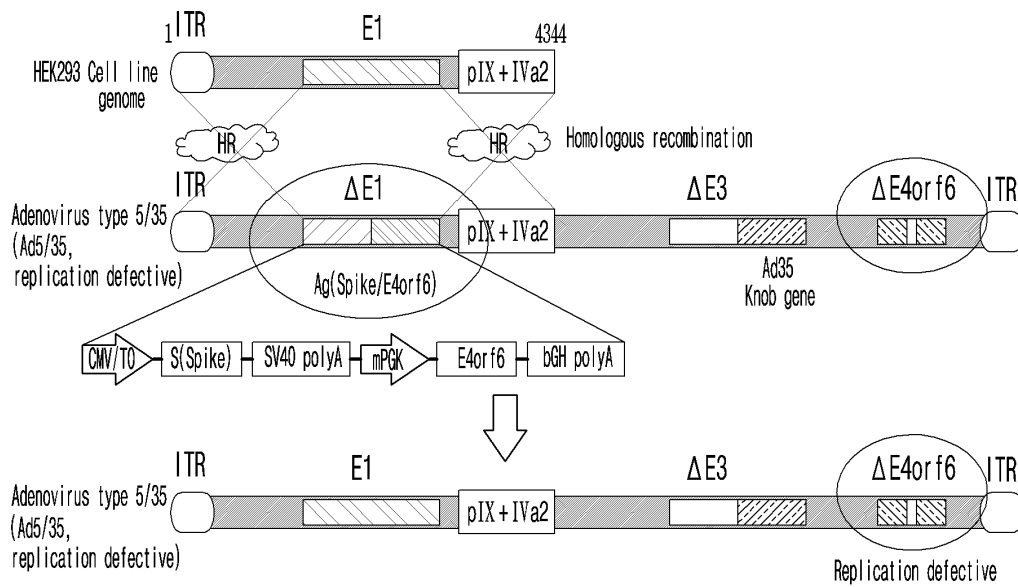
Fig. 1**Fig. 2**

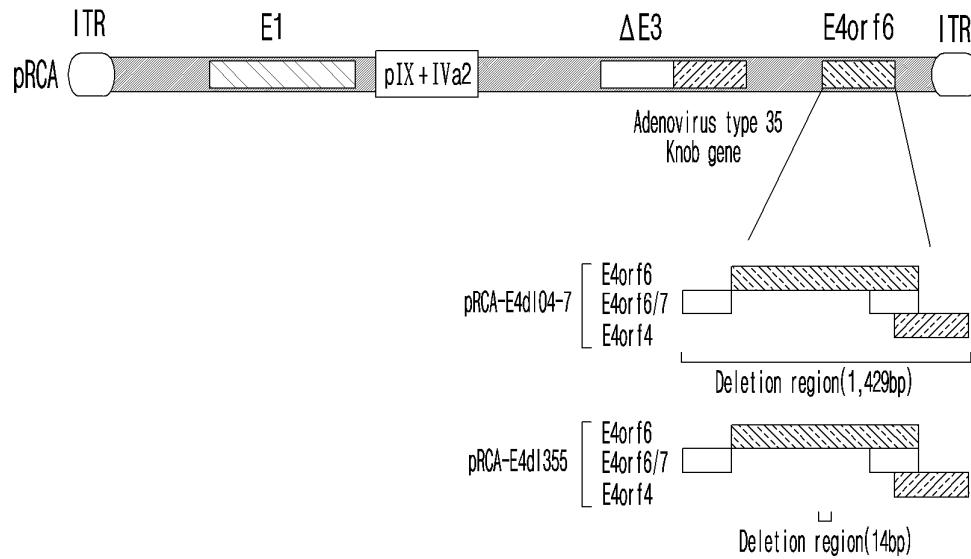
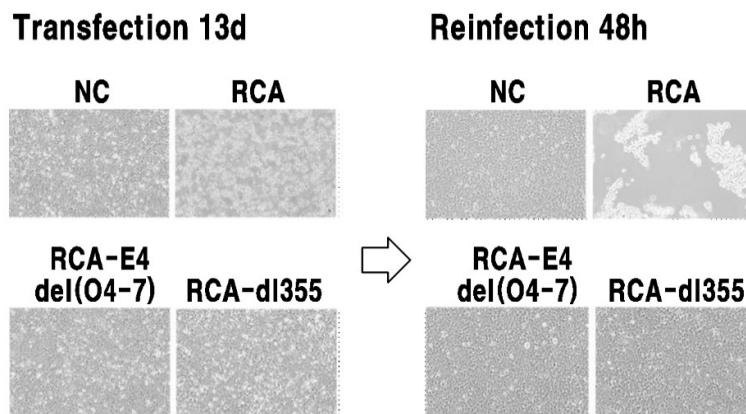
Fig. 3**Fig. 4**

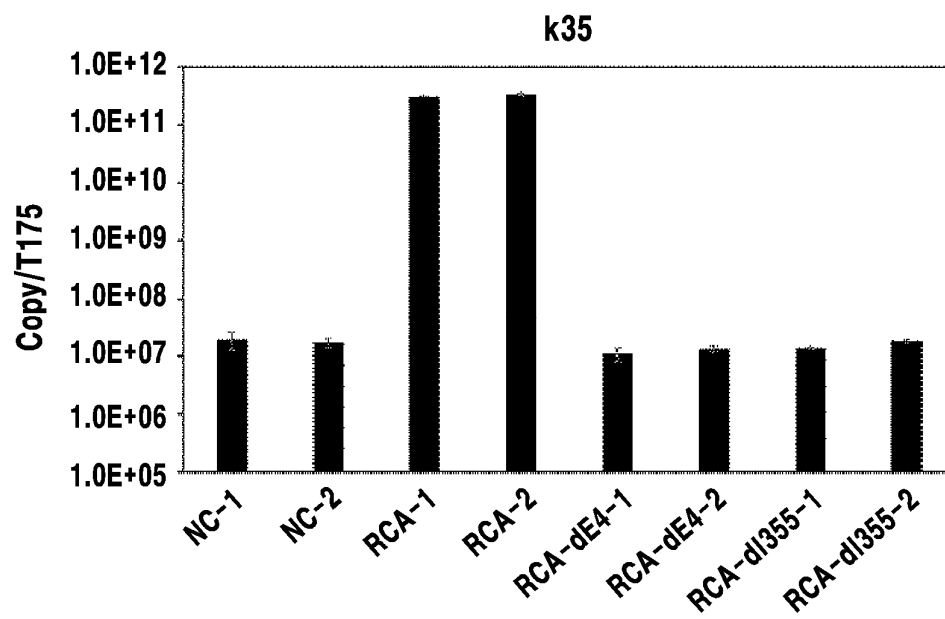
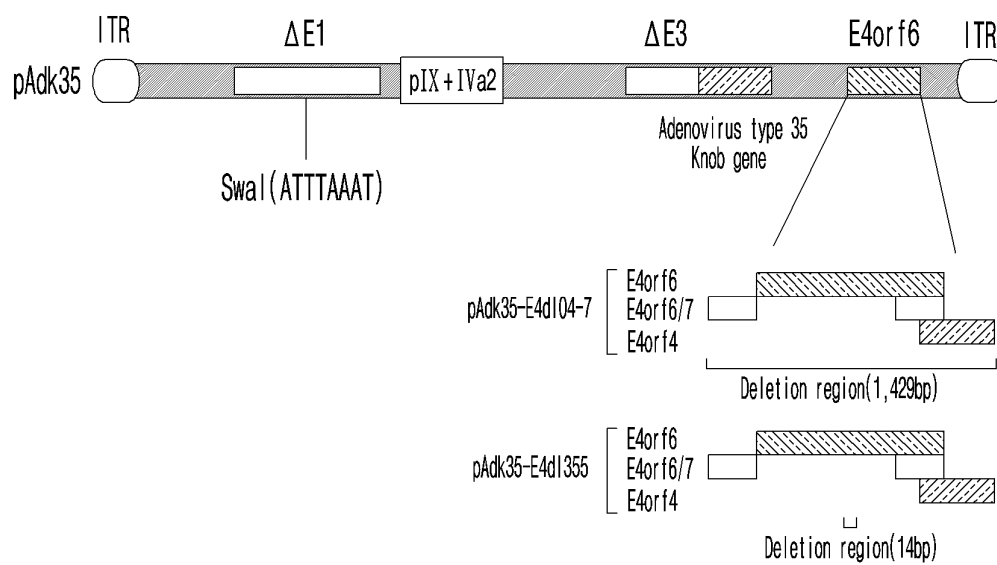
Fig. 5**Fig. 6**

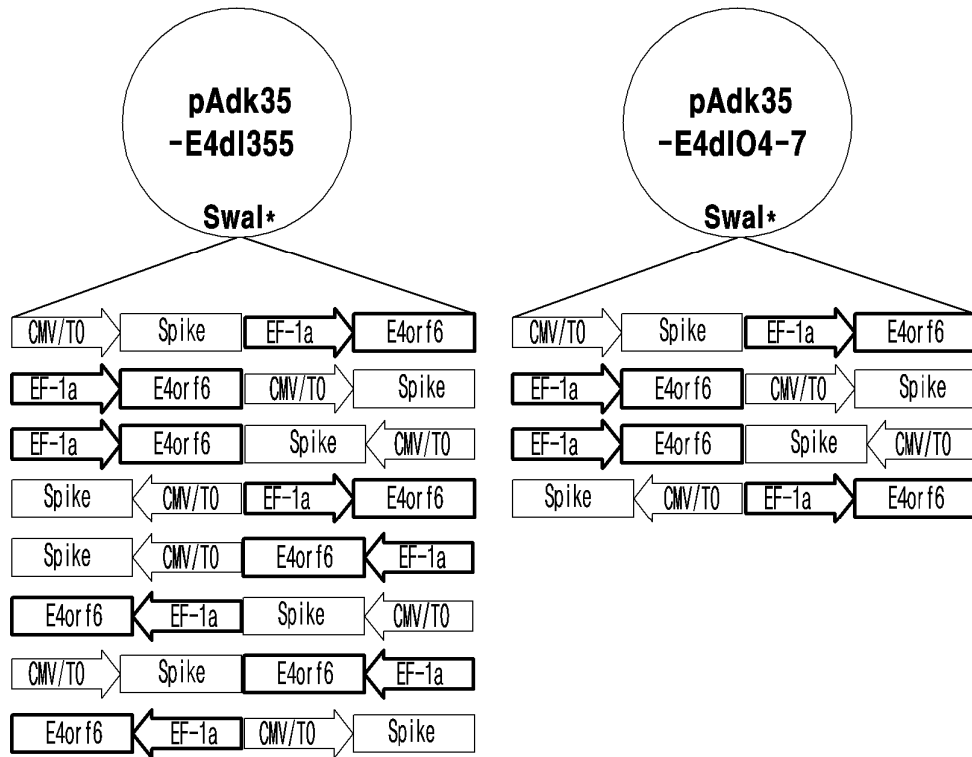
Fig. 7

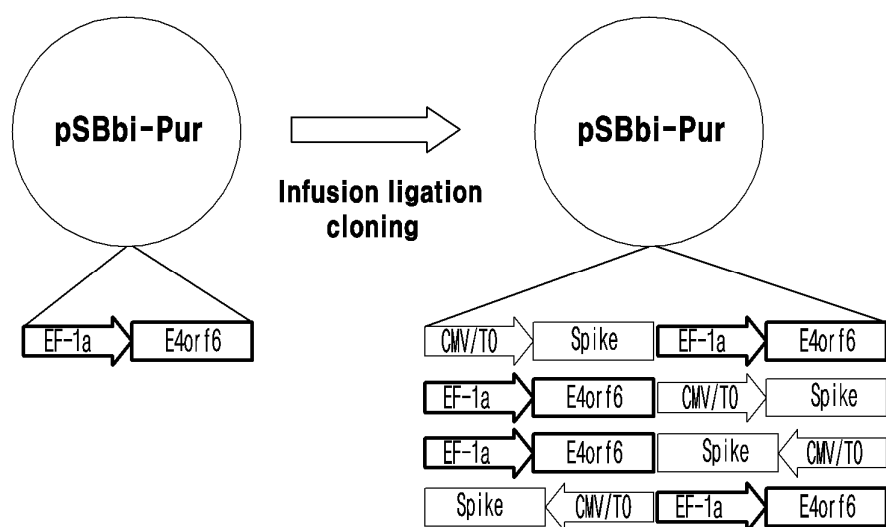
Fig. 8

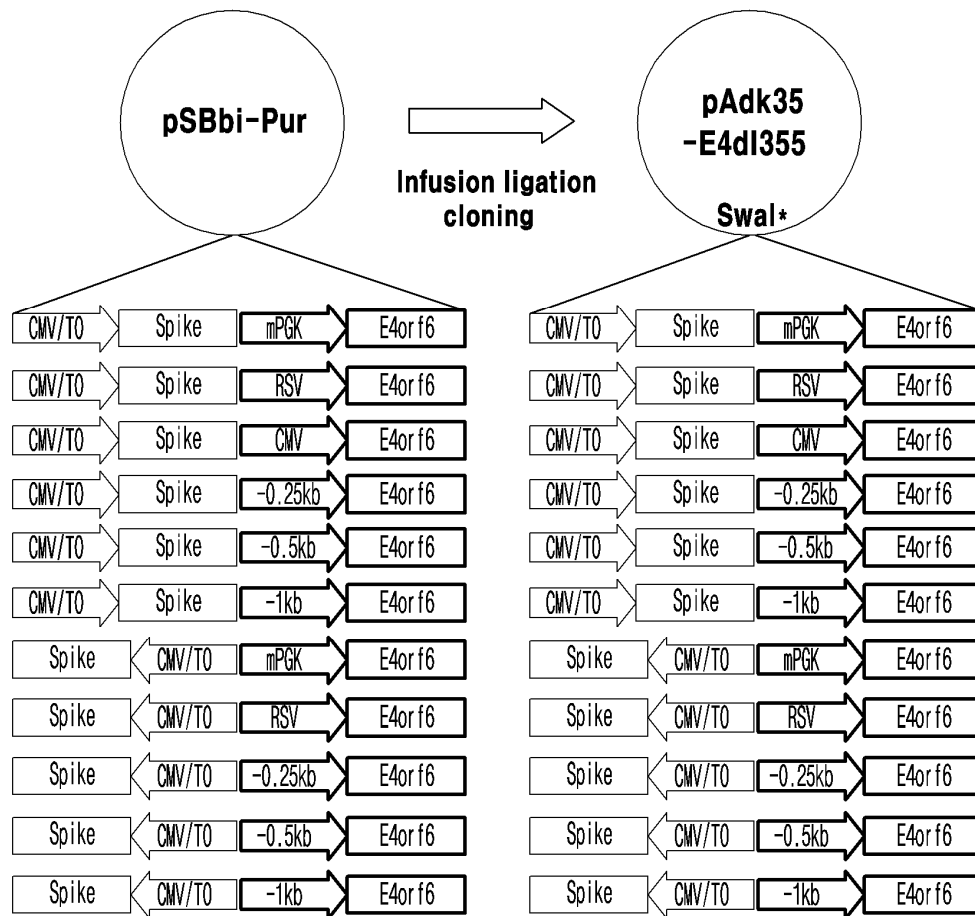
Fig. 9

Fig. 10

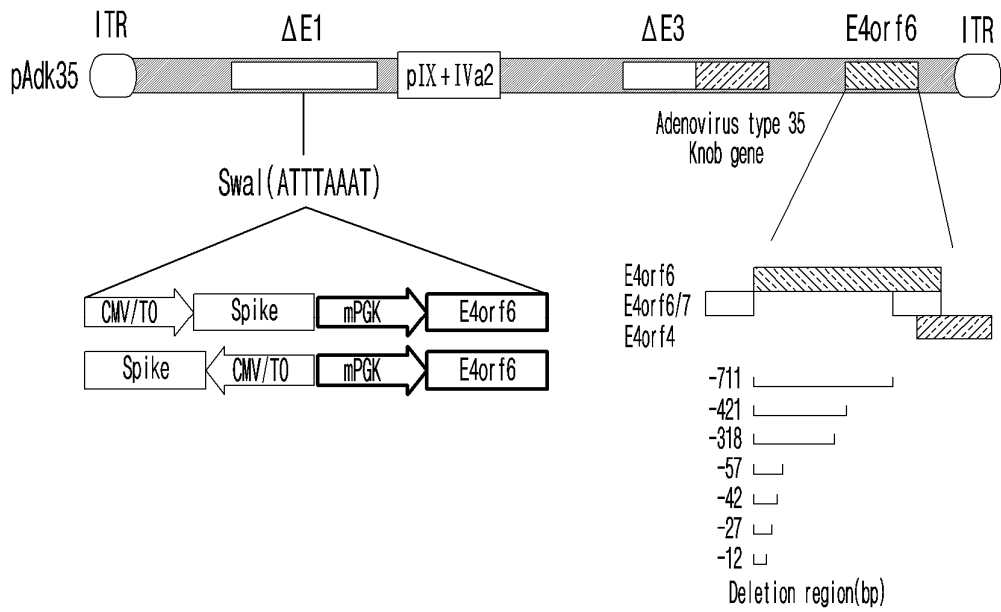


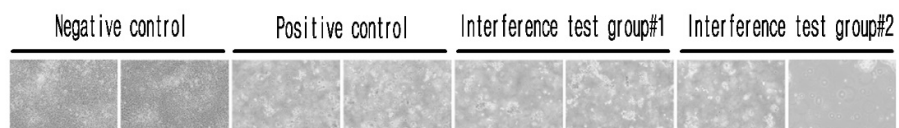
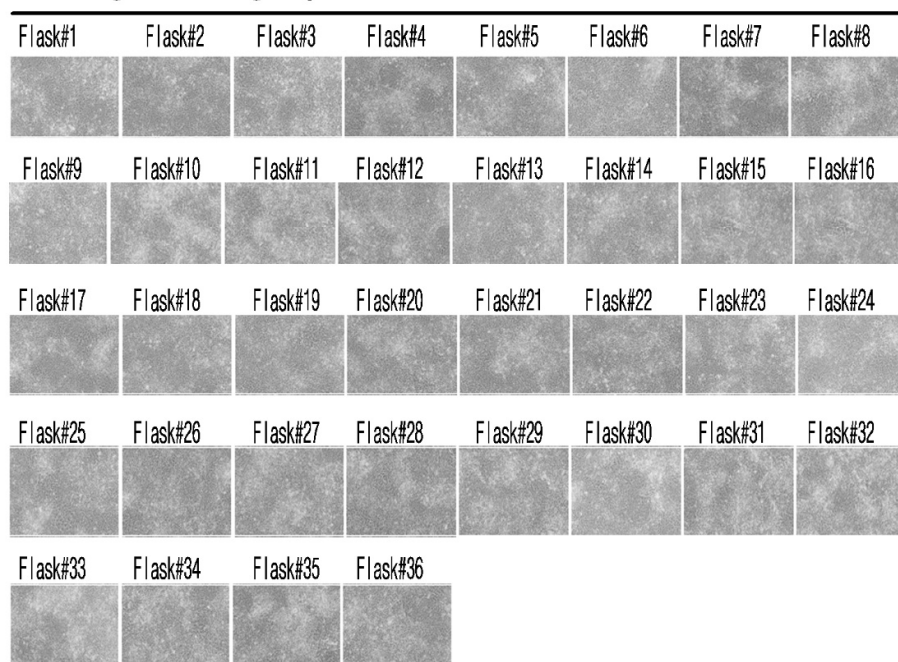
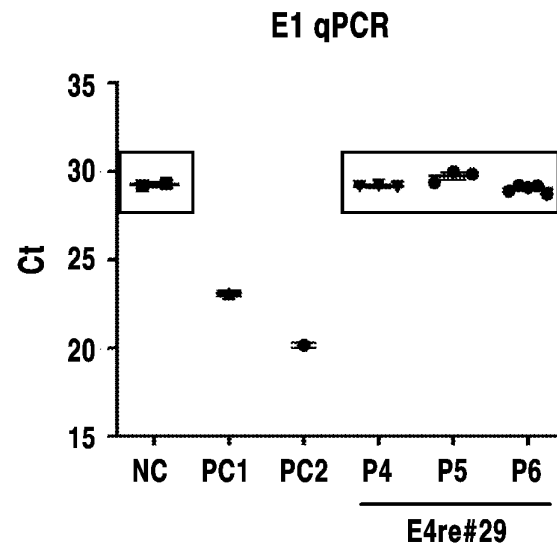
Fig. 11**RCA Negative test group: 4.14×10^{10} VP**

Fig. 12

NC : Negative control

PC1 : Adenovirus standard 1PFU

PC2 : Adenovirus standard 1PFU

P4 : E4re#29 virus passage4

P5 : E4re#29 virus passage5

P5 : E4re#29 virus passage6

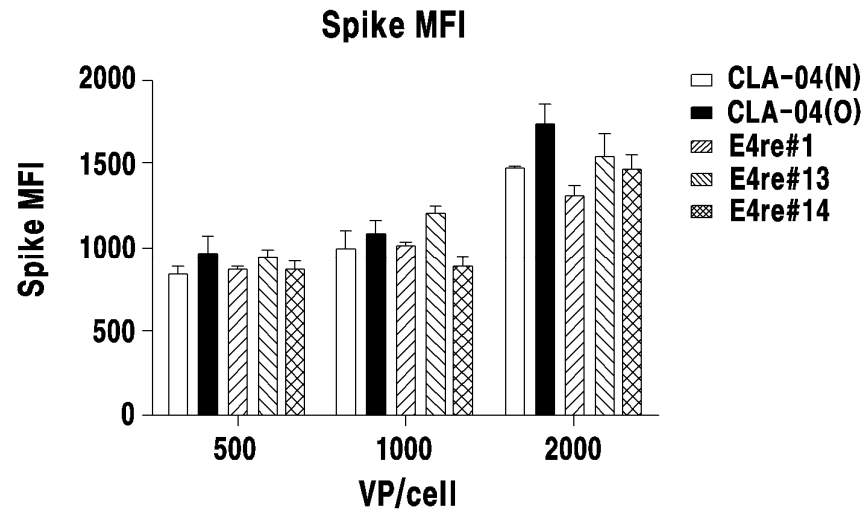
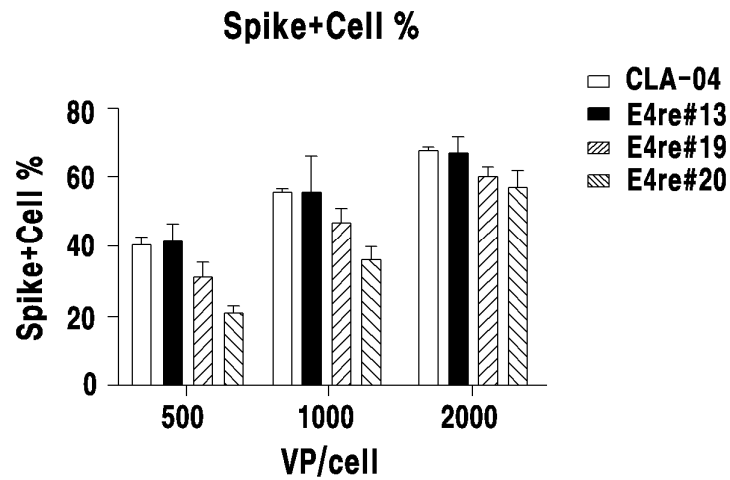
Fig. 13A**Fig. 13B**

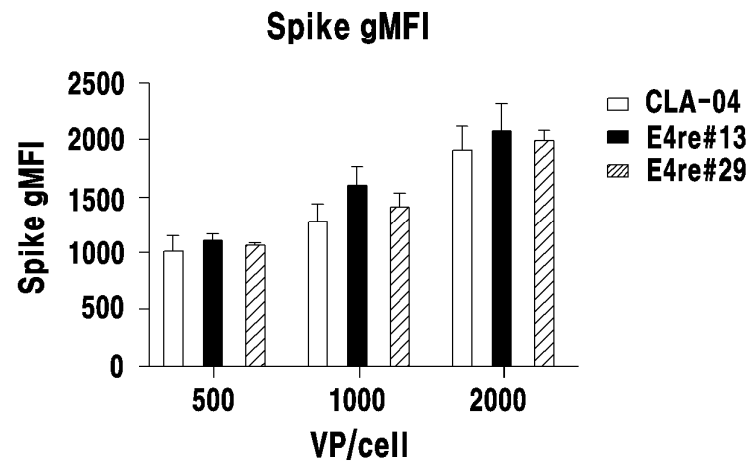
Fig. 13C

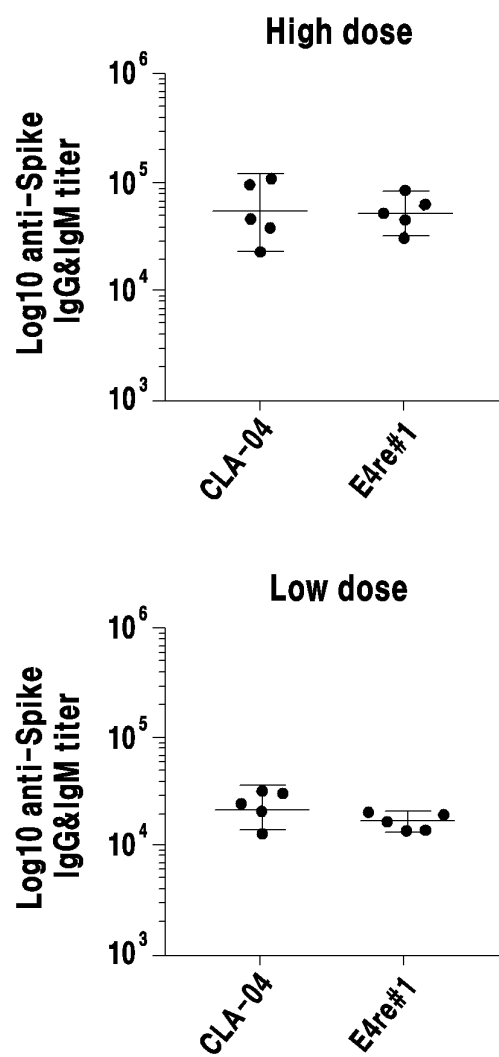
Fig. 14A

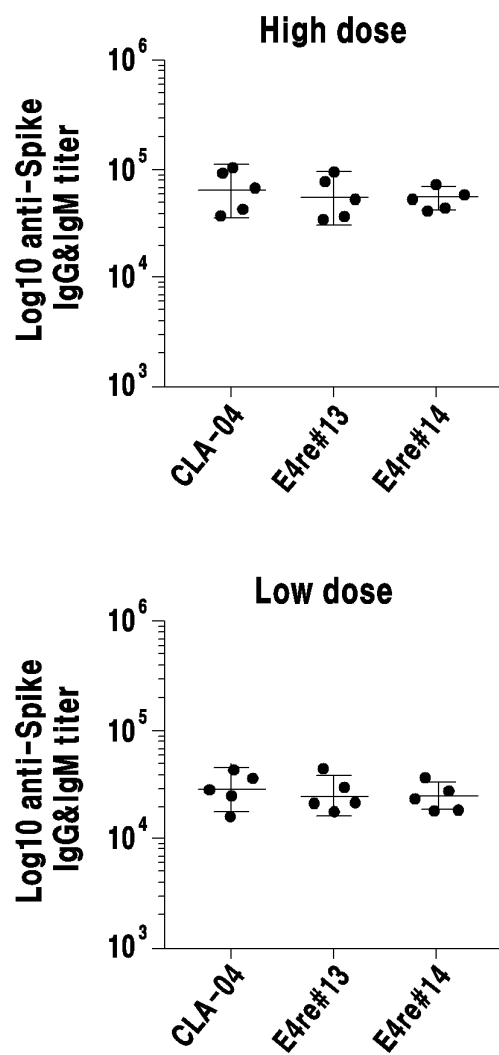
Fig. 14B

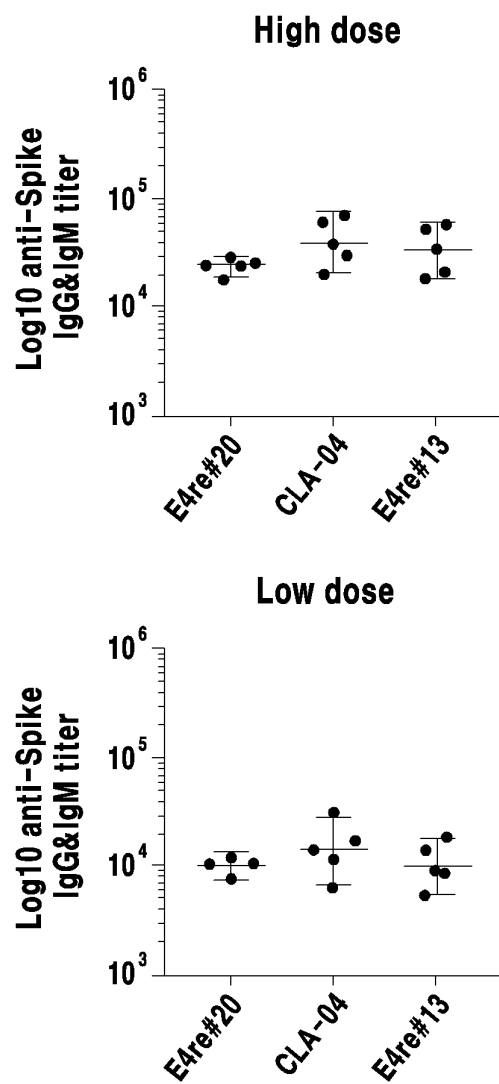
Fig. 14C

Fig. 14D

