

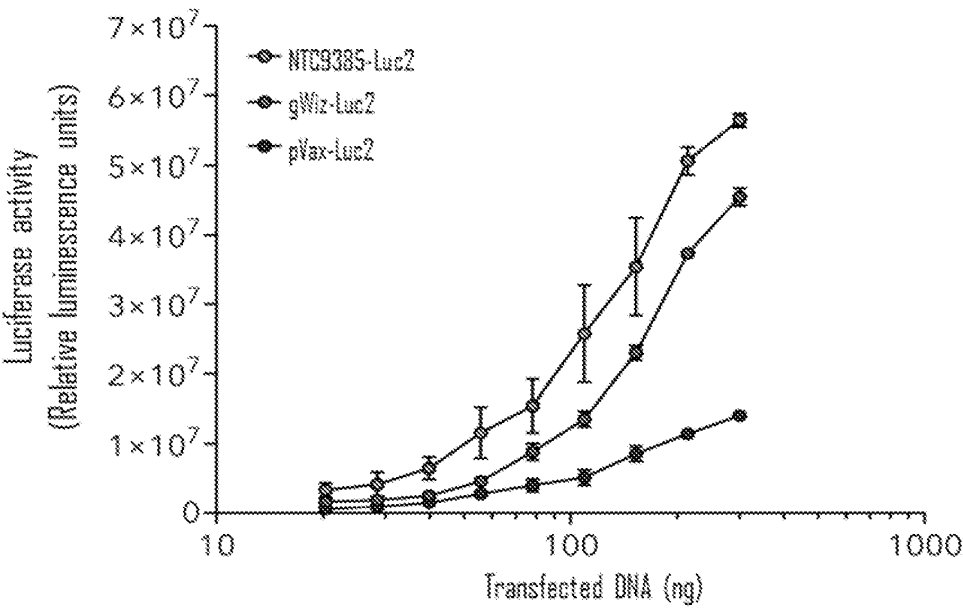


Fig. 1

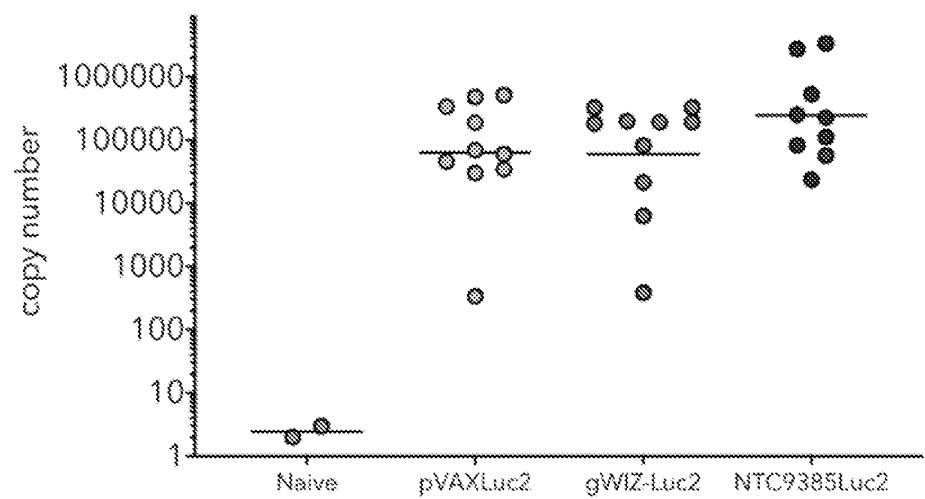


Fig. 2A

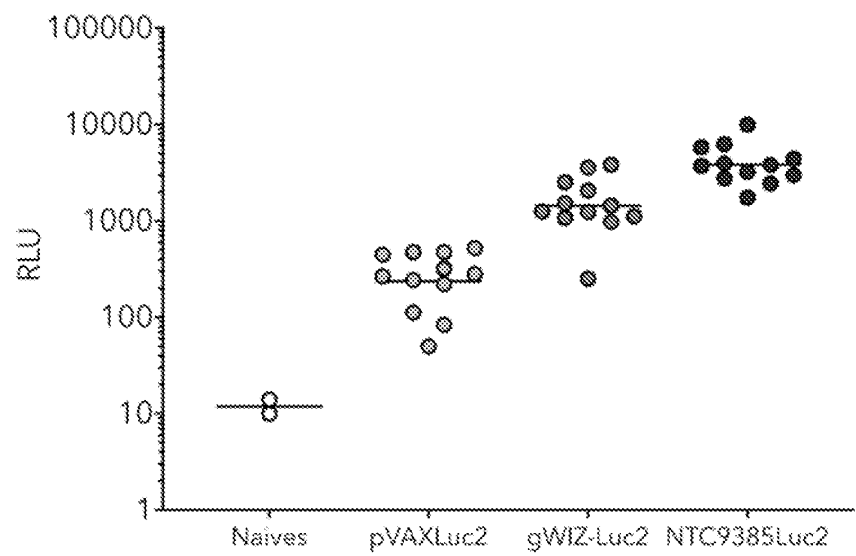


Fig. 2B

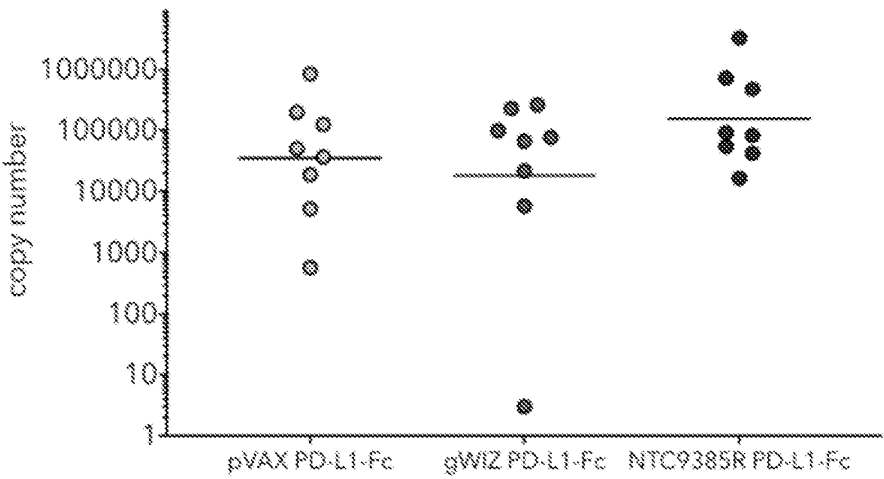


Fig. 2C

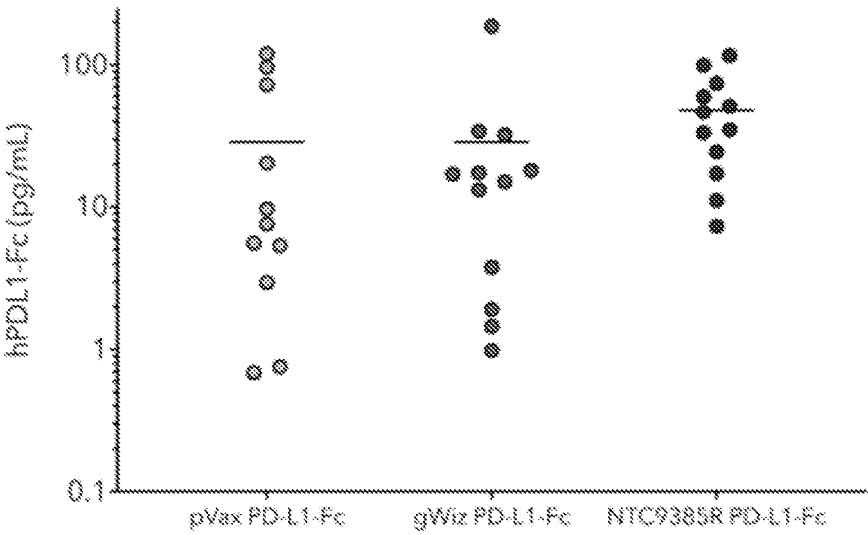


Fig. 2D

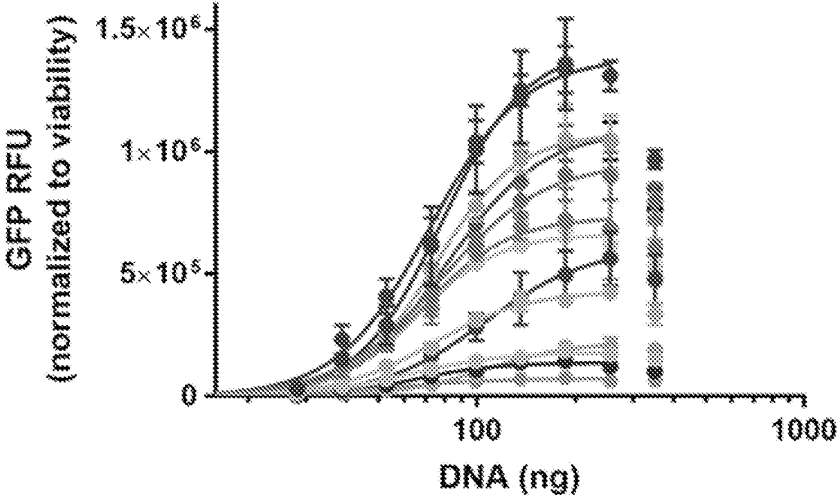


Fig. 3A

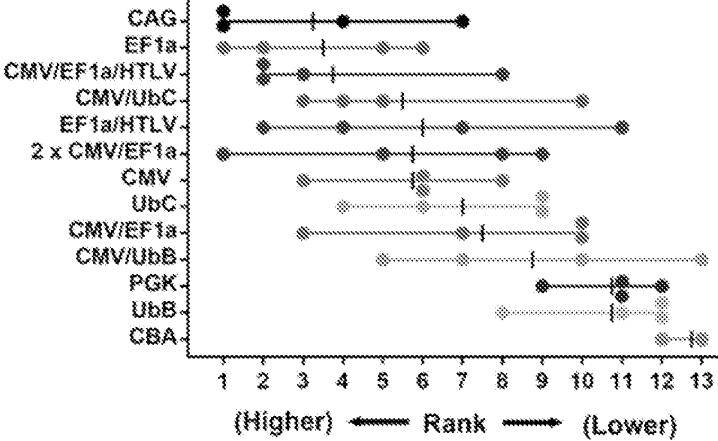


Fig. 3B

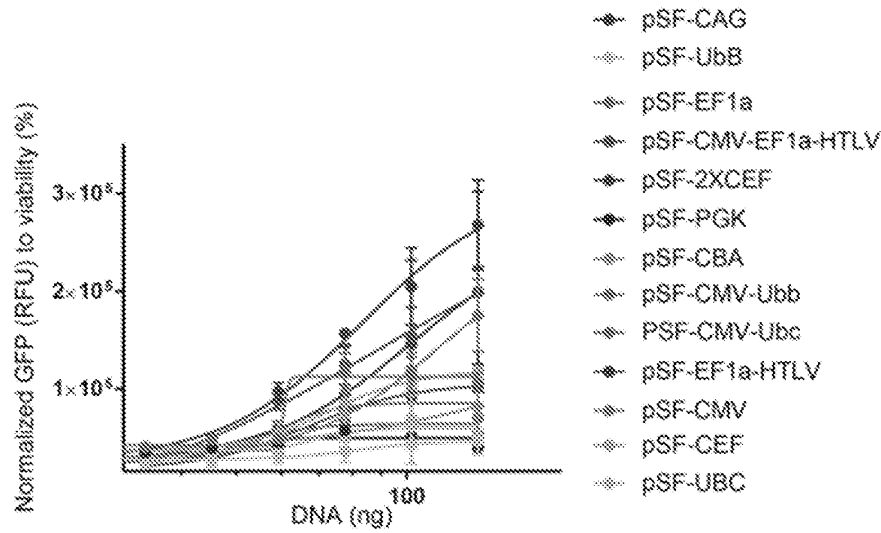


Fig. 4A

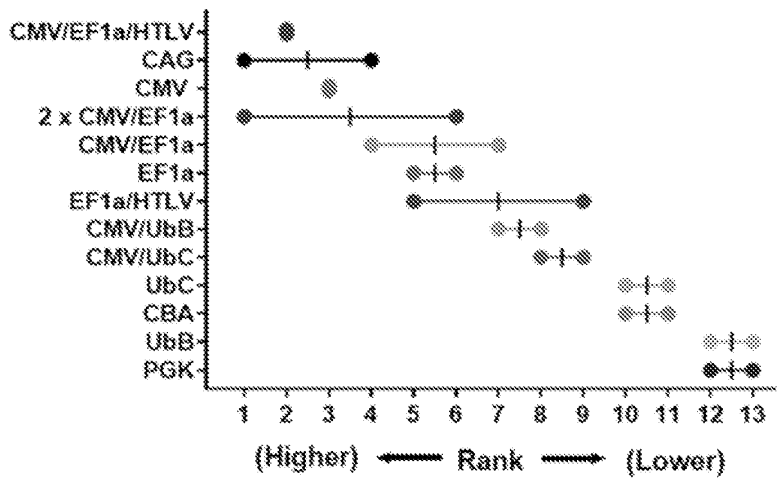


Fig. 4B

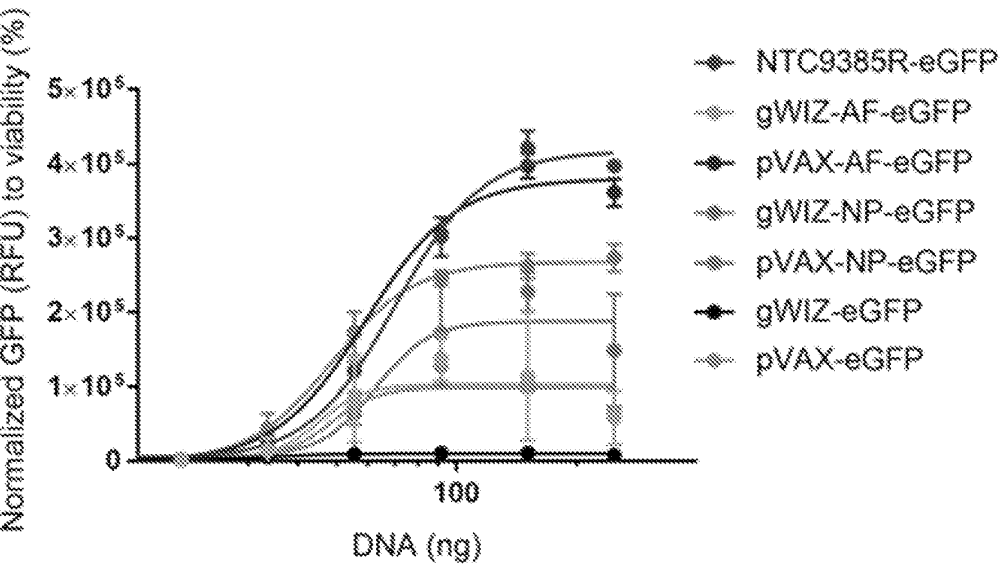


Fig. 5A

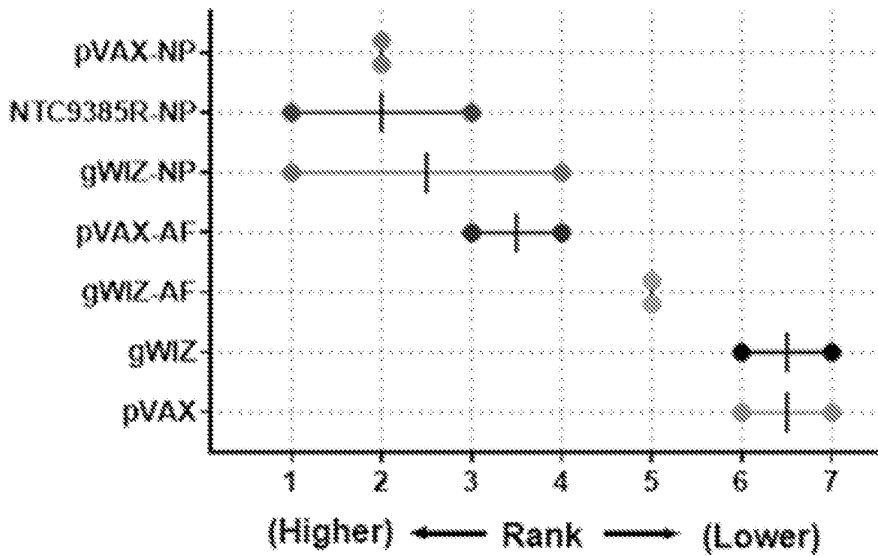


Fig. 5B

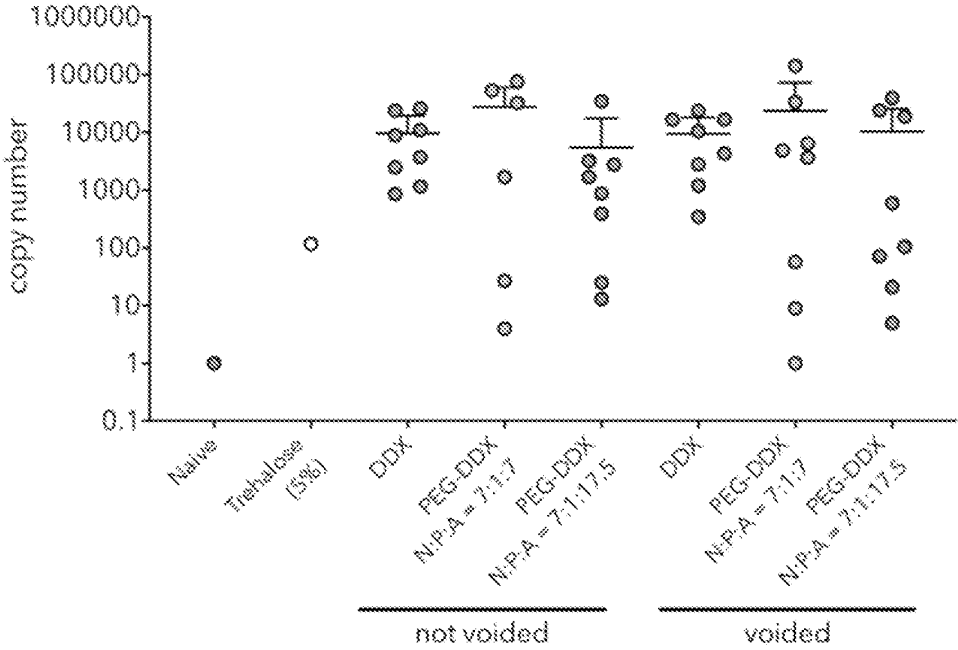


Fig. 6

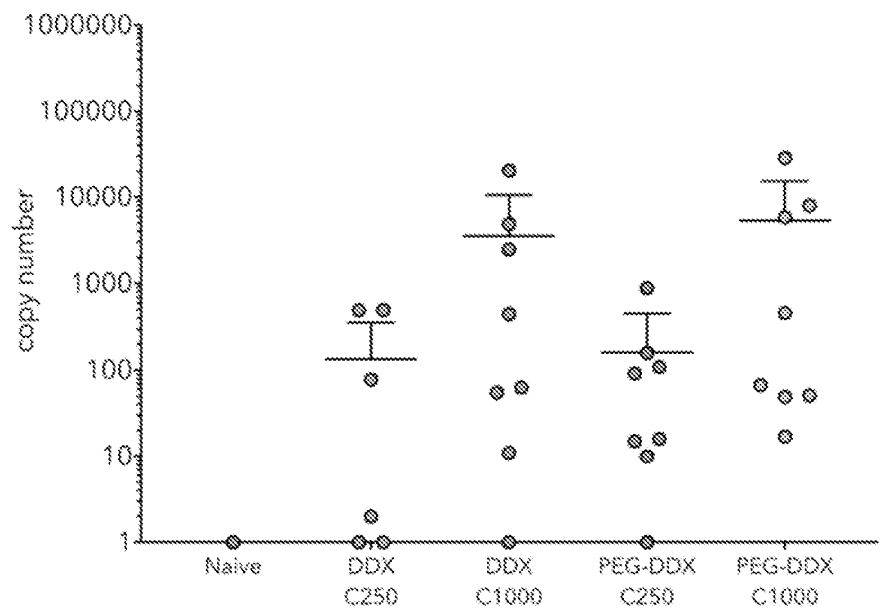


Fig. 7A

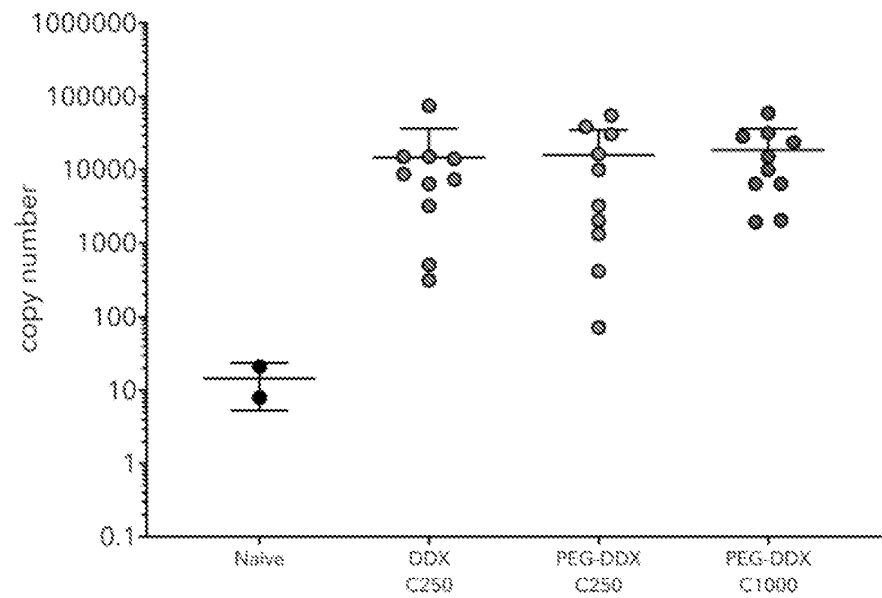


Fig. 7B

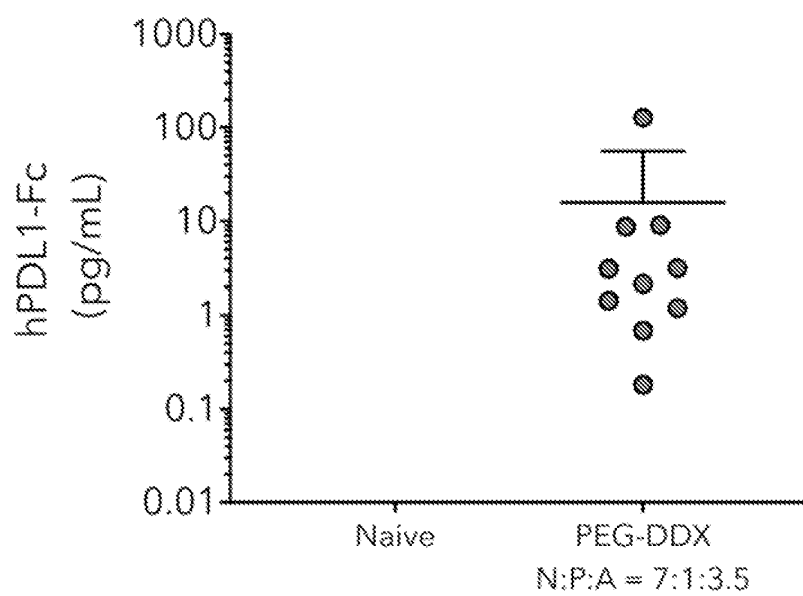


Fig. 8

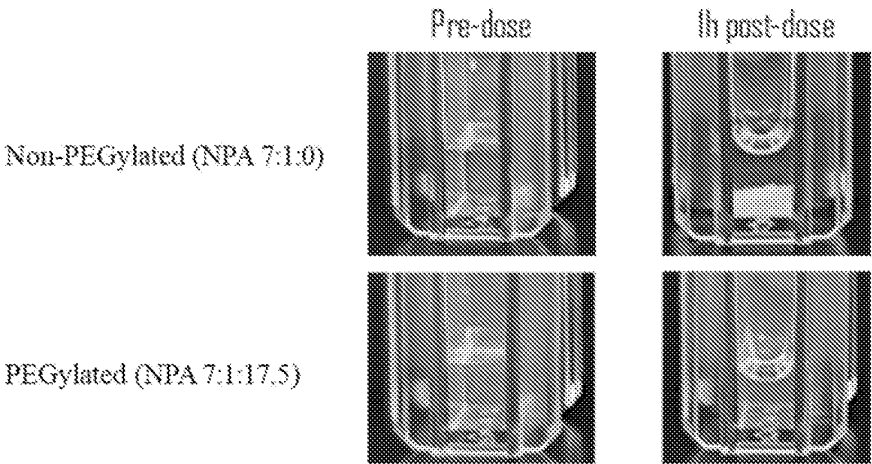


Fig. 9A

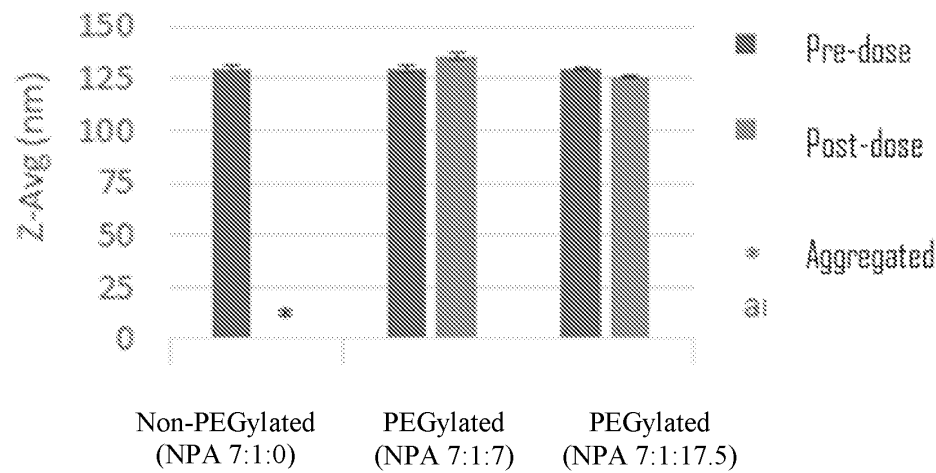


Fig. 9B

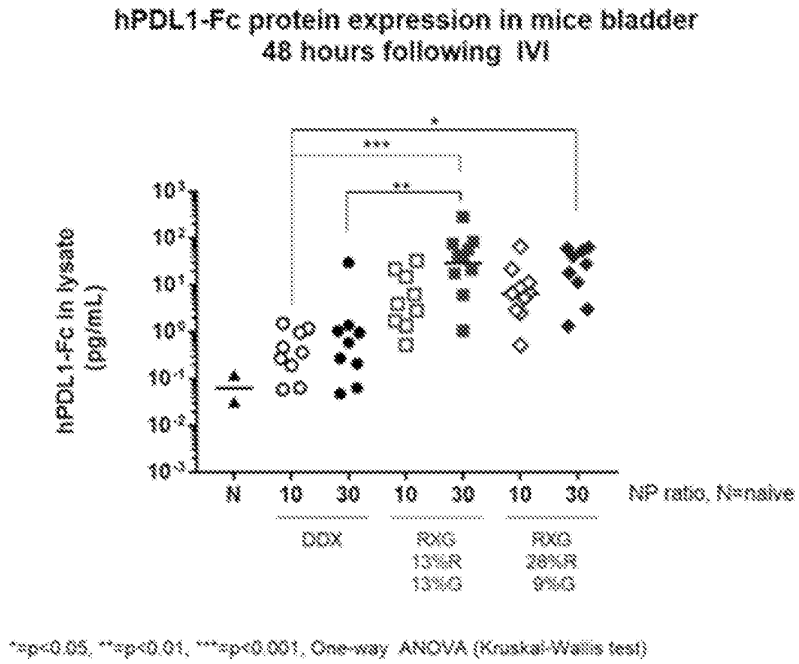
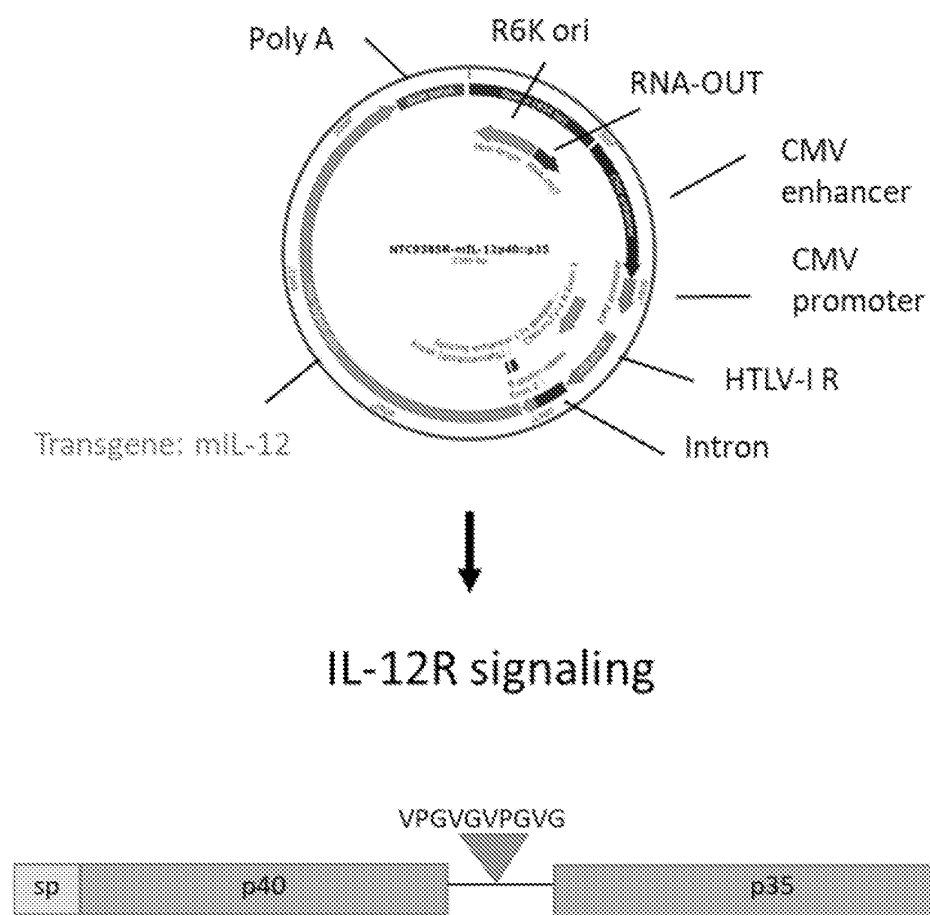


Fig. 10

**Fig. 12A**

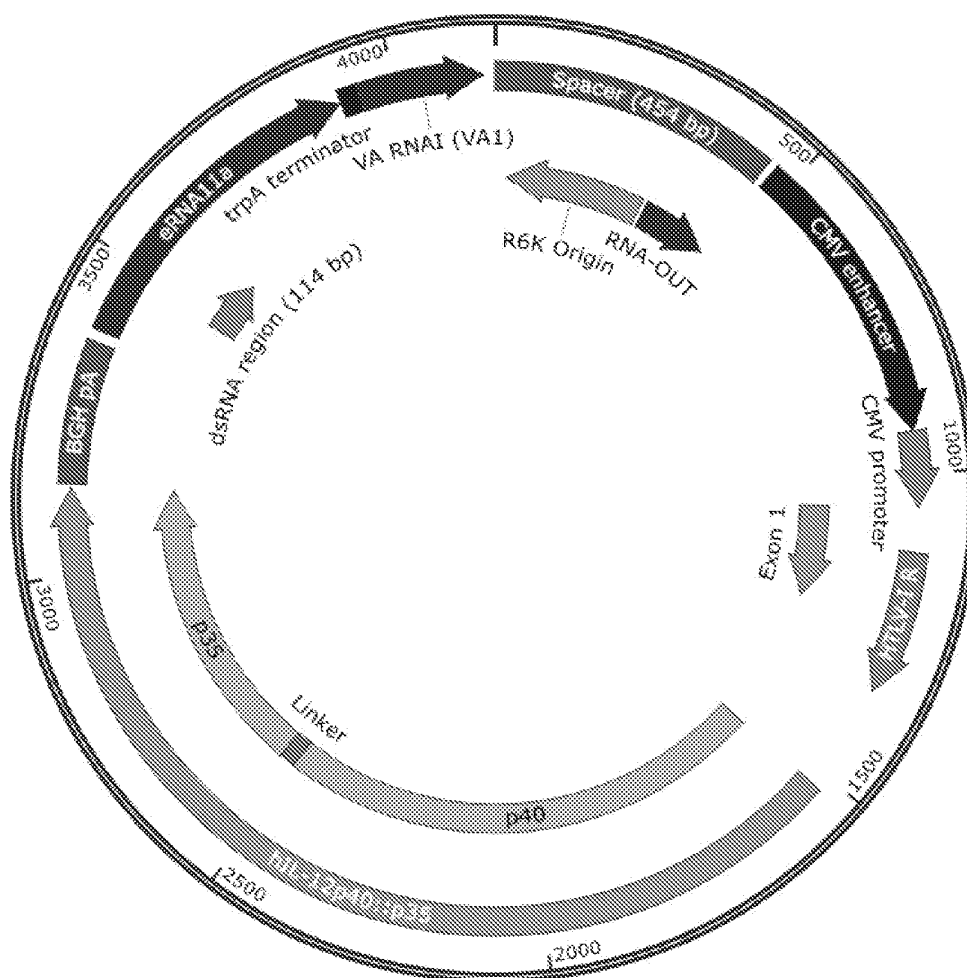


Fig. 12B

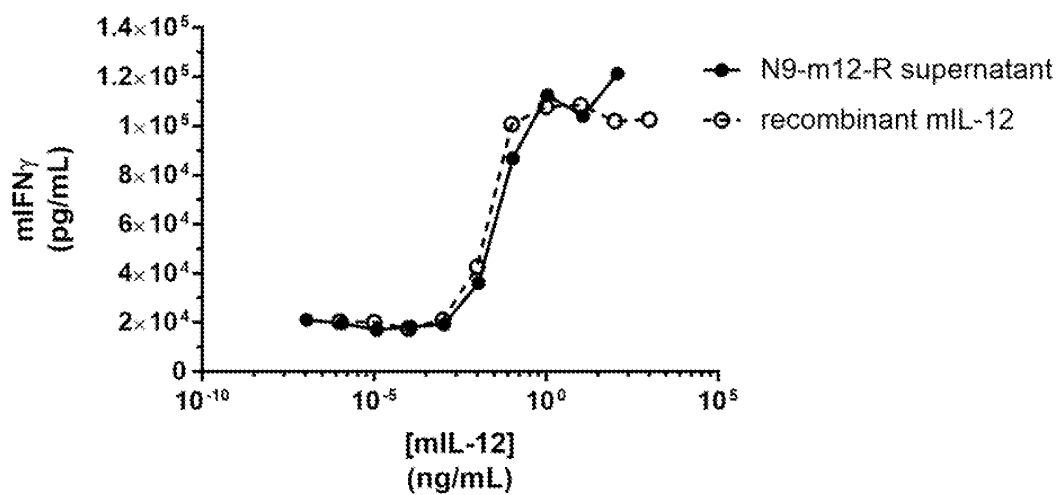


Fig. 13A

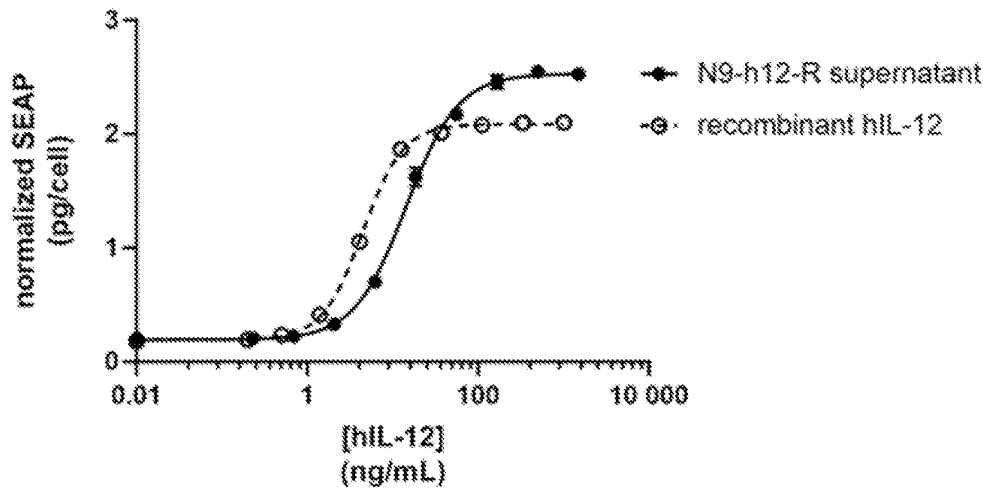


Fig. 13B

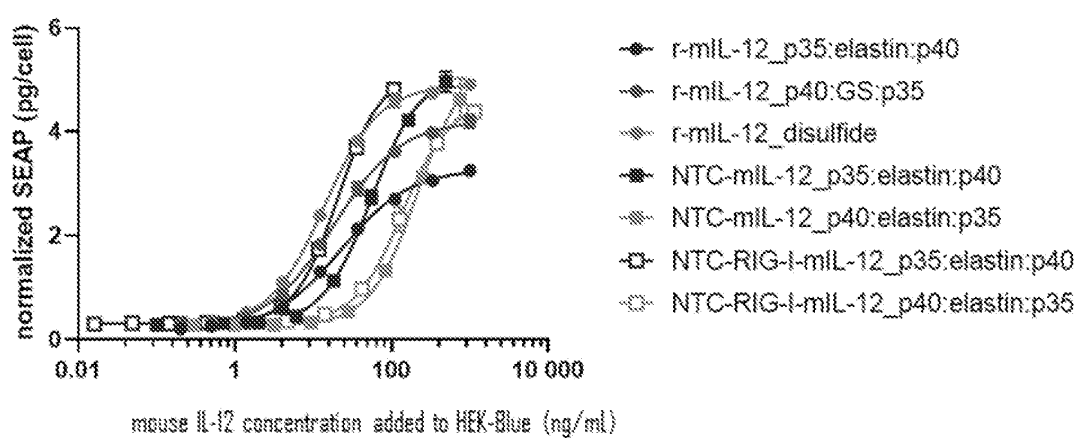


Fig. 13C

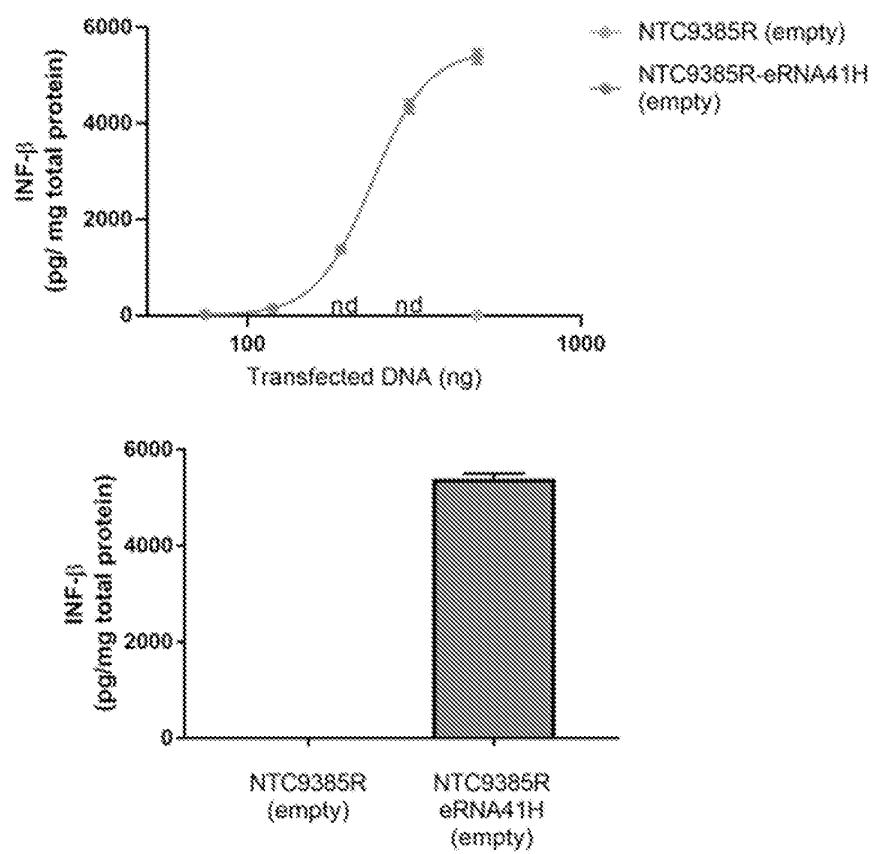


Fig. 14A

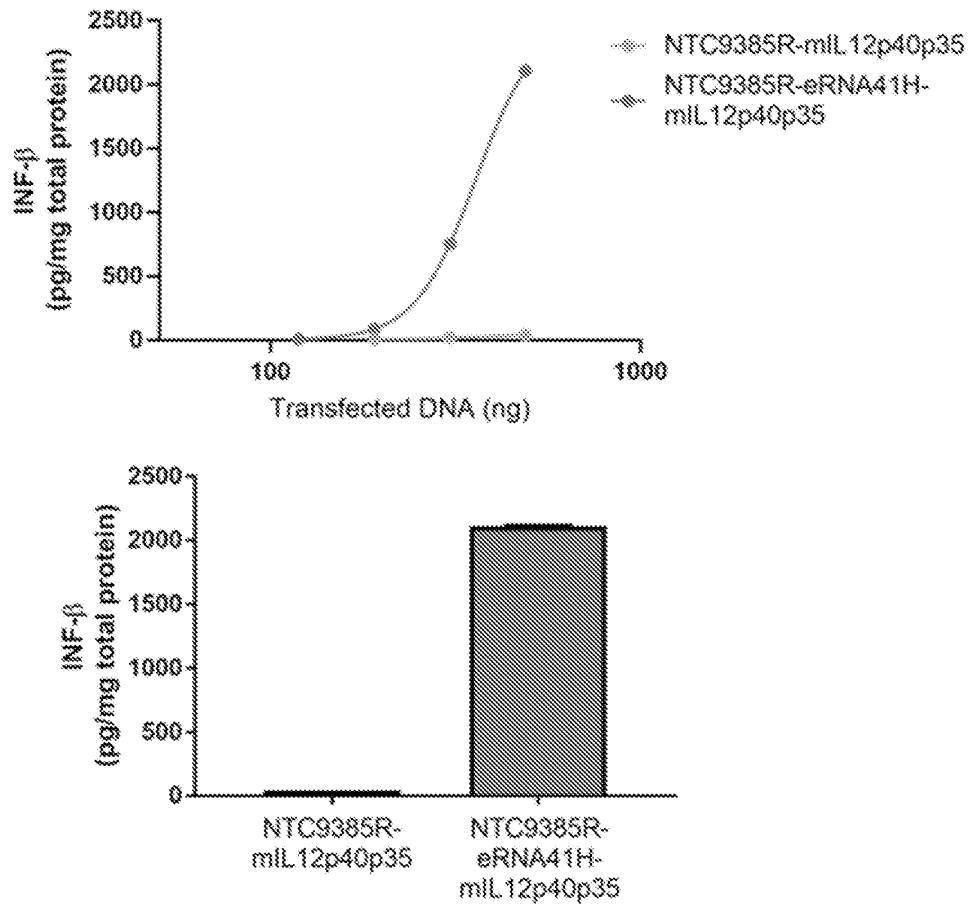


Fig. 14B


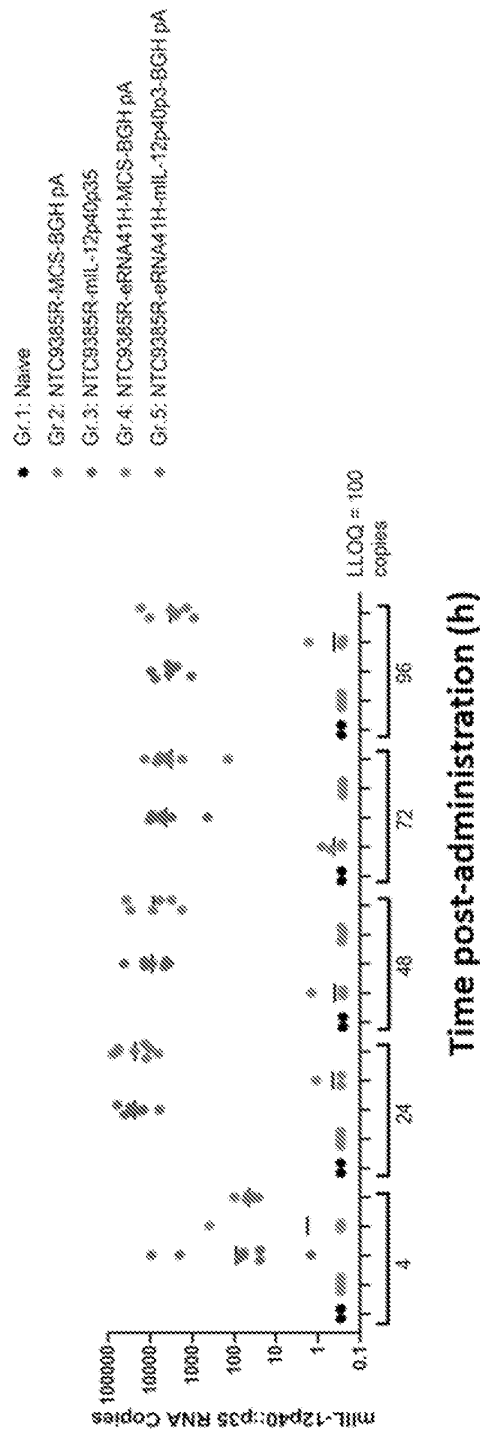


Fig. 15

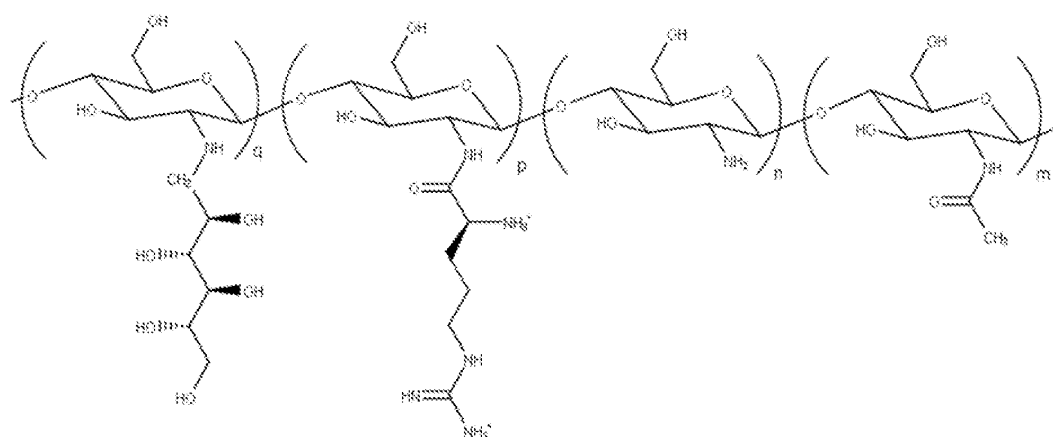

Sub-units: $q \sim 0.10$, $p \sim 0.28$, $n \sim 0.61$, $m \sim 0.01$

Fig. 16A

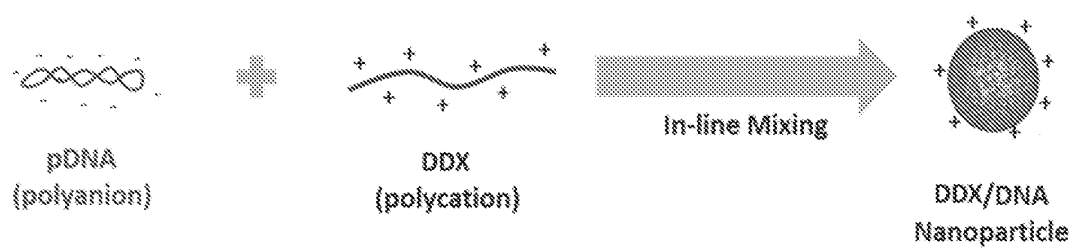


Fig. 16B

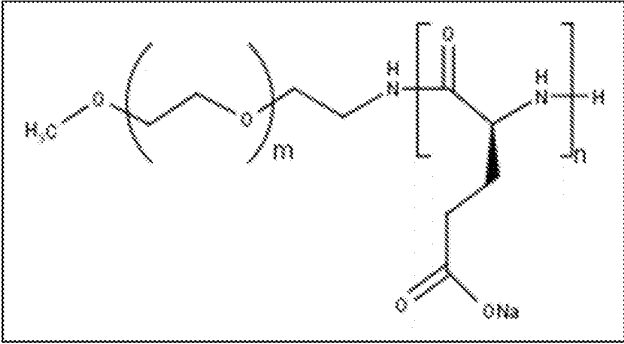


Fig. 16C

Z-average diameter	90 -135 nm
Polydispersity Index (PDI)	0.11 - 0.23
DNA capture	For all DDX, no DNA smearing for N:P ≥ 10
Supercoil DNA	> 80%

Fig. 17A

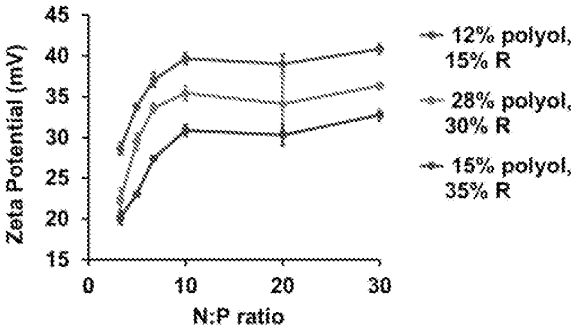


Fig. 17B

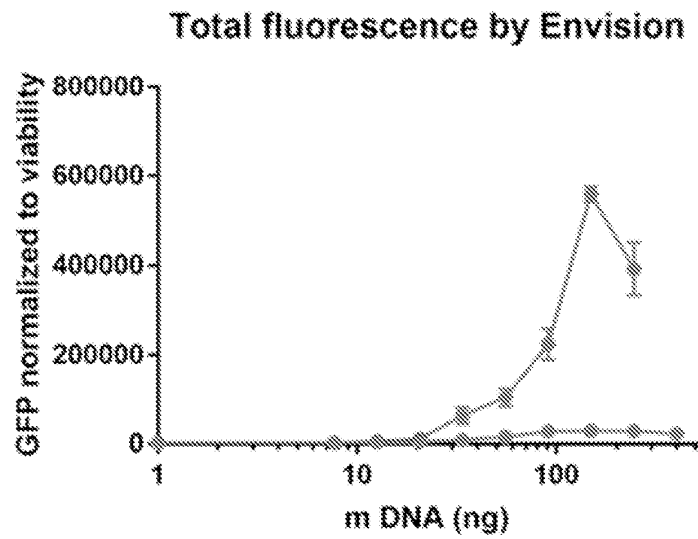


Fig. 18A

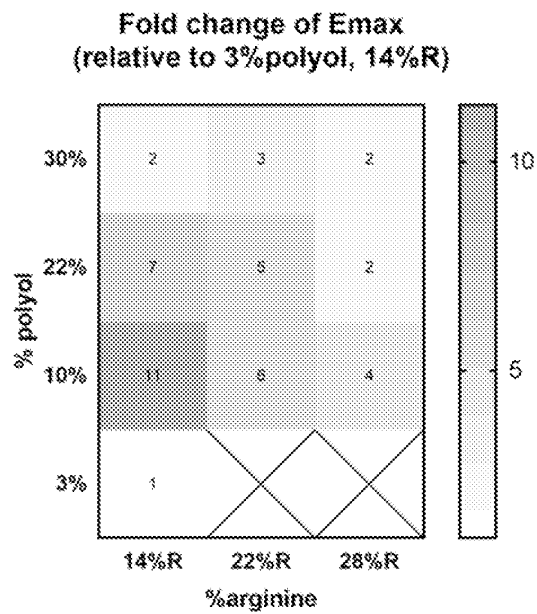


Fig. 18B

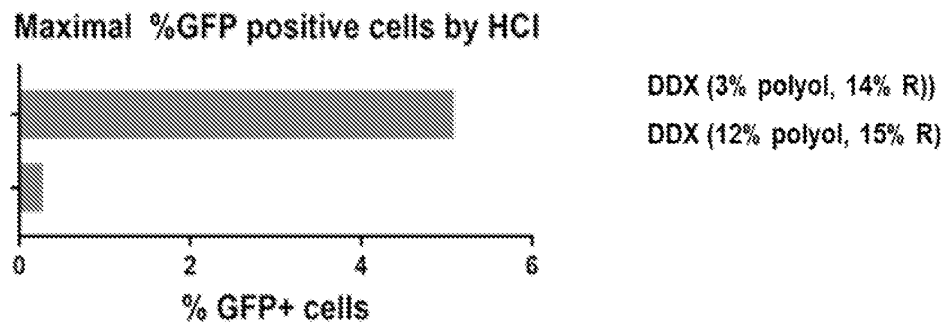


Fig. 18C

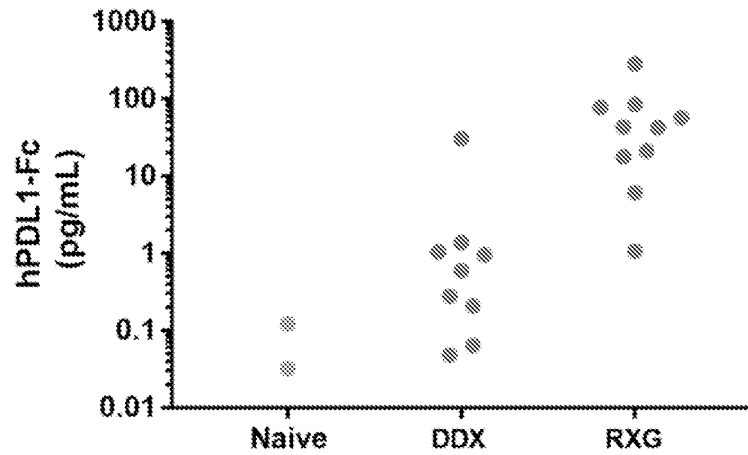


Fig. 19

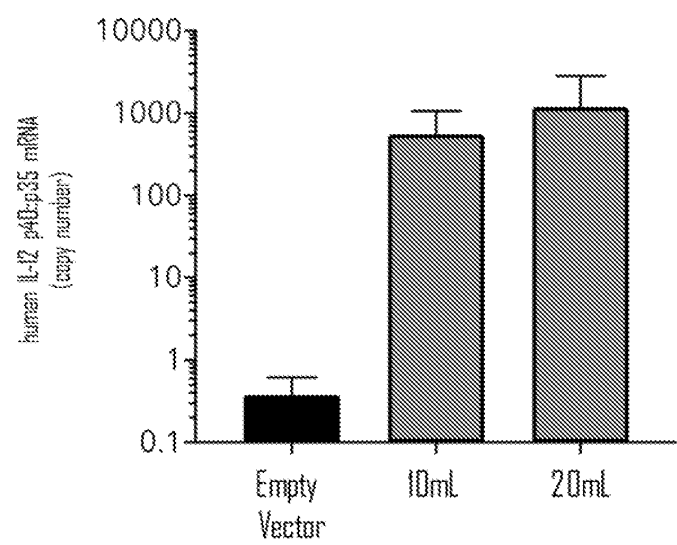


Figure 20A

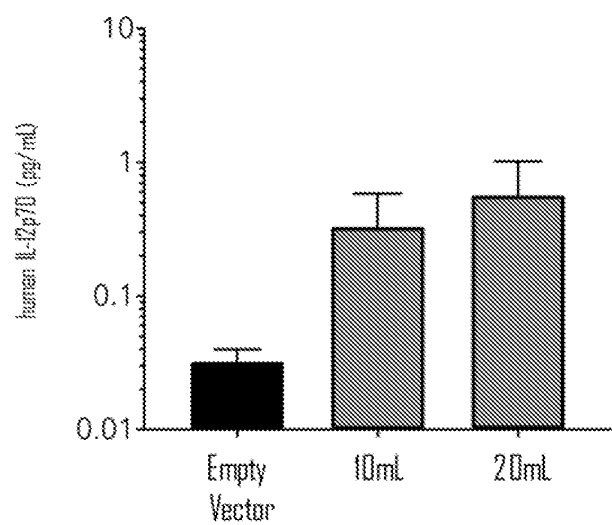


Fig. 20B

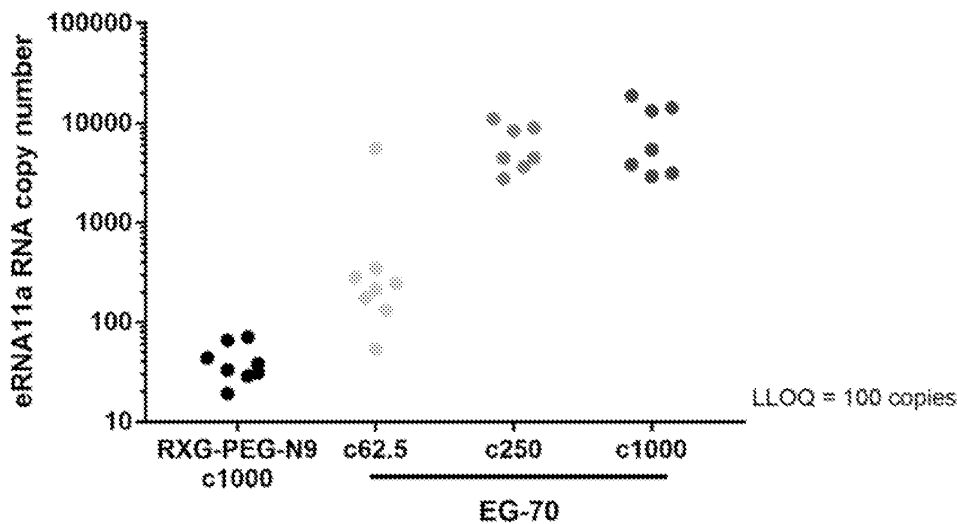


Fig. 21

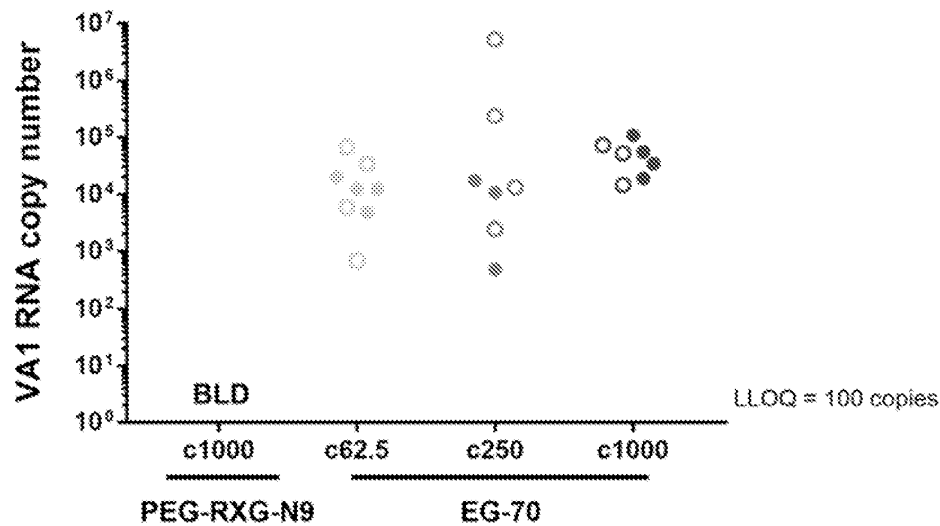


Fig. 22

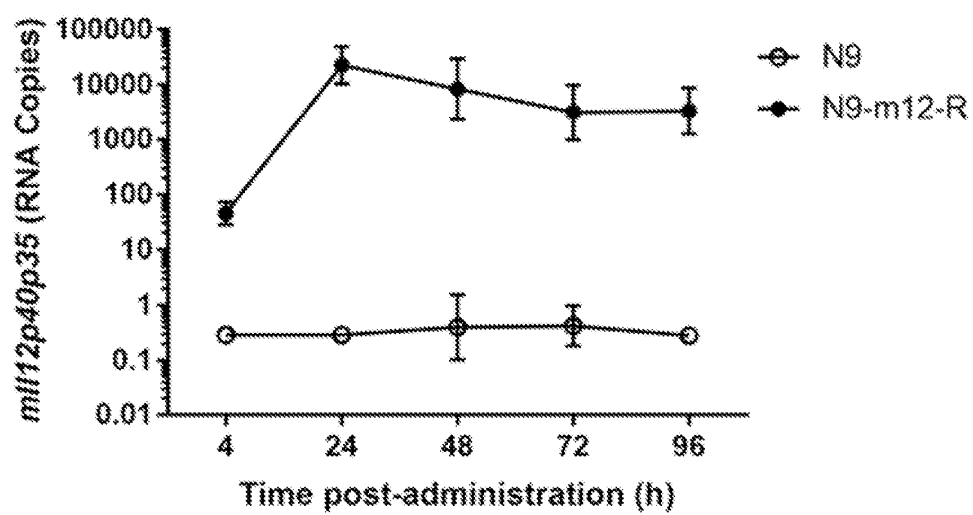


Fig. 23

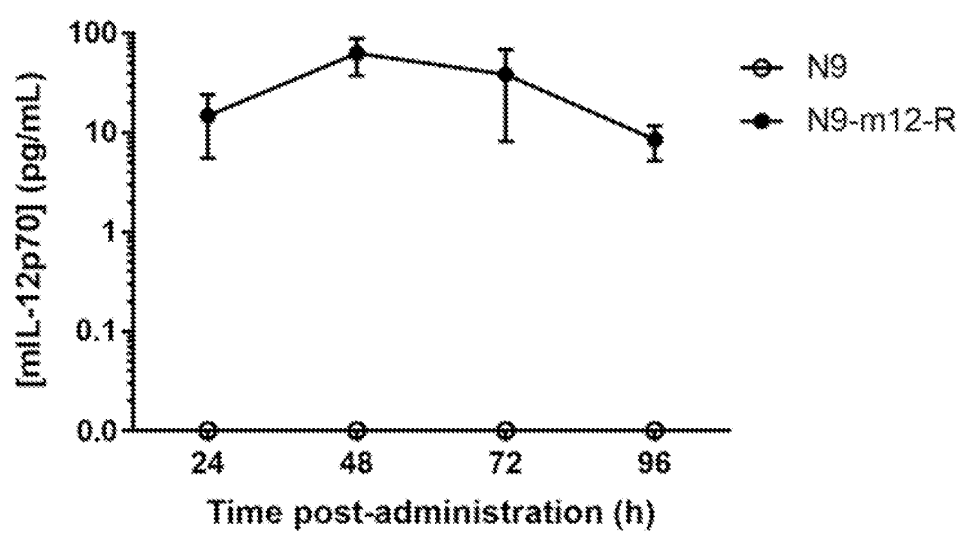


Fig. 24

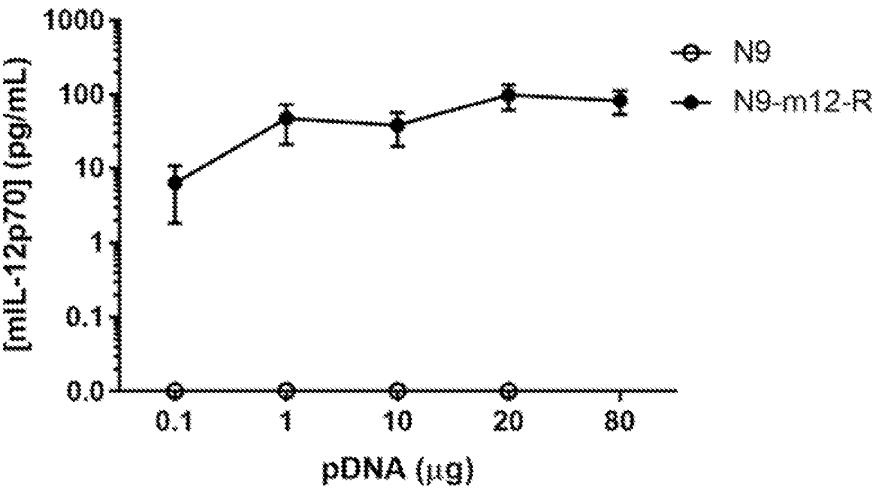


Fig. 25

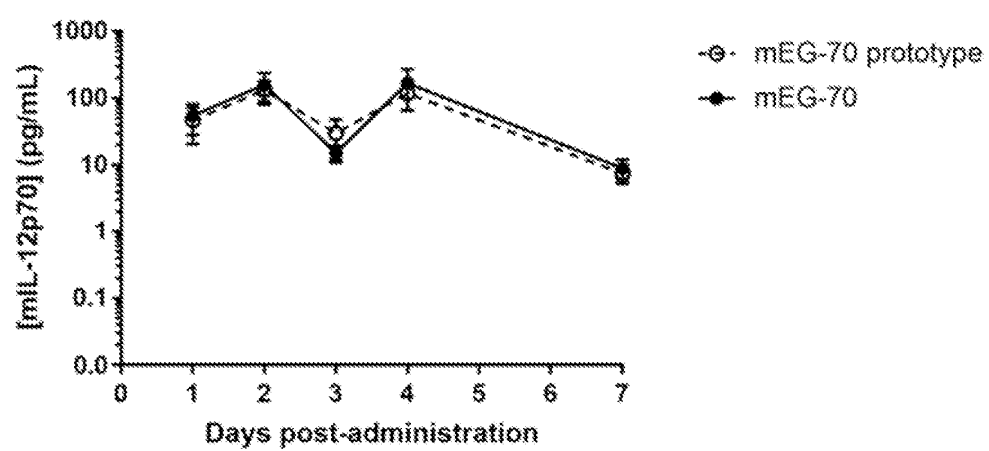


Fig. 26

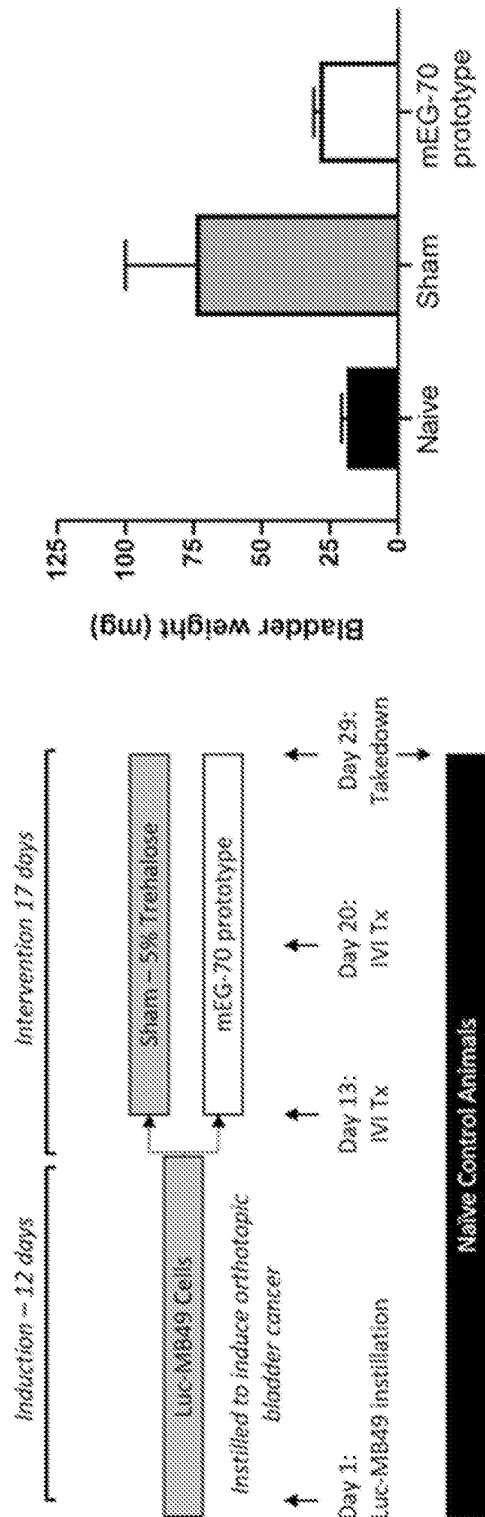


Fig. 27B

Fig. 27A