

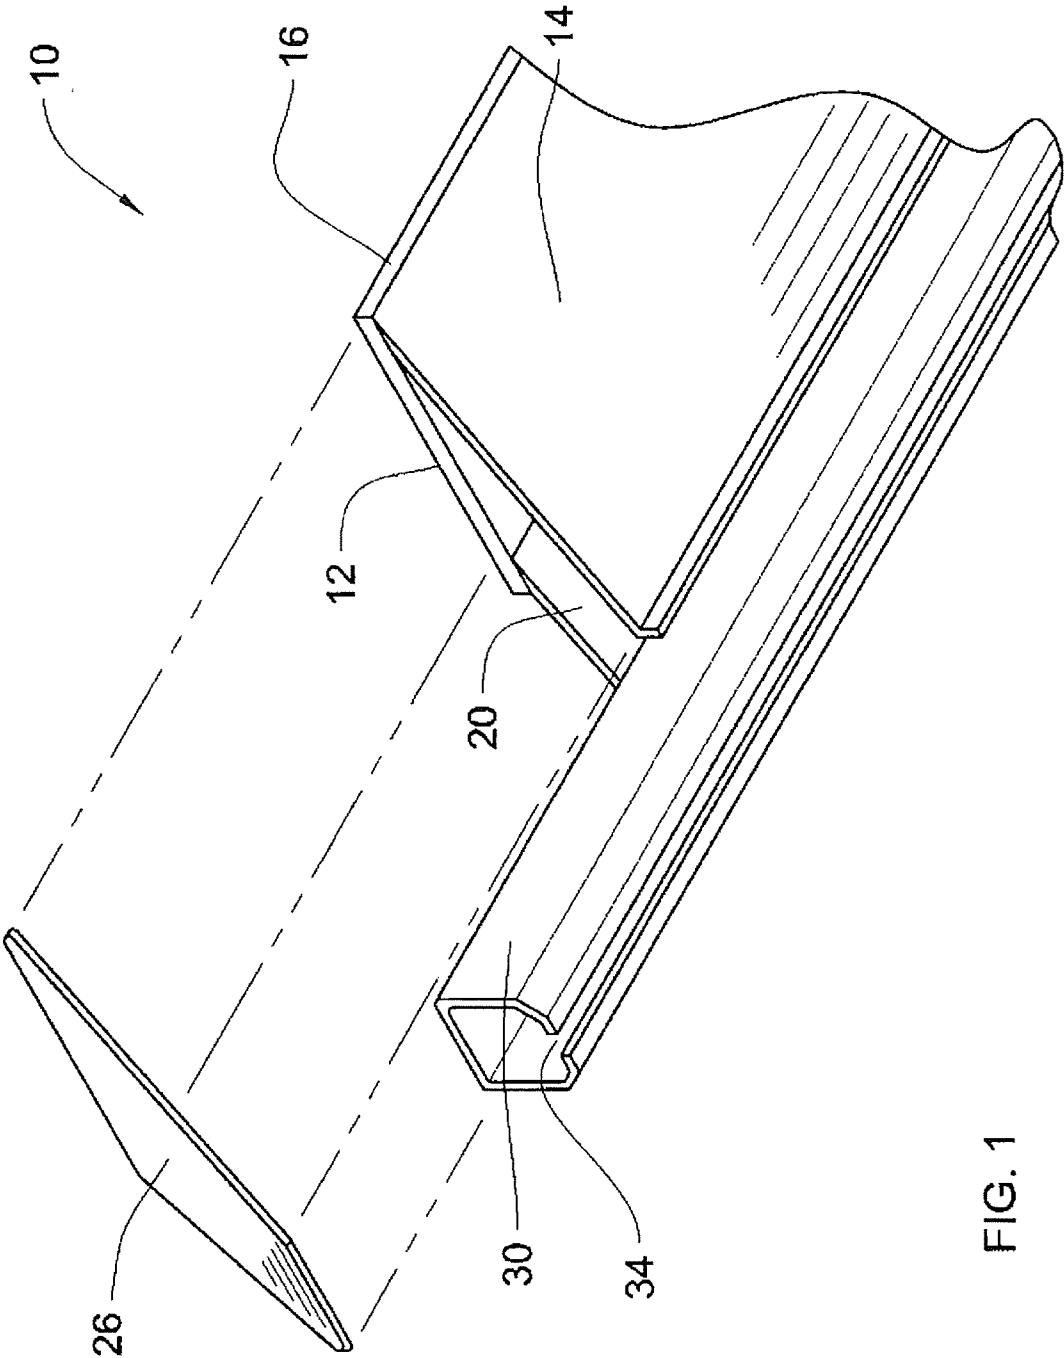
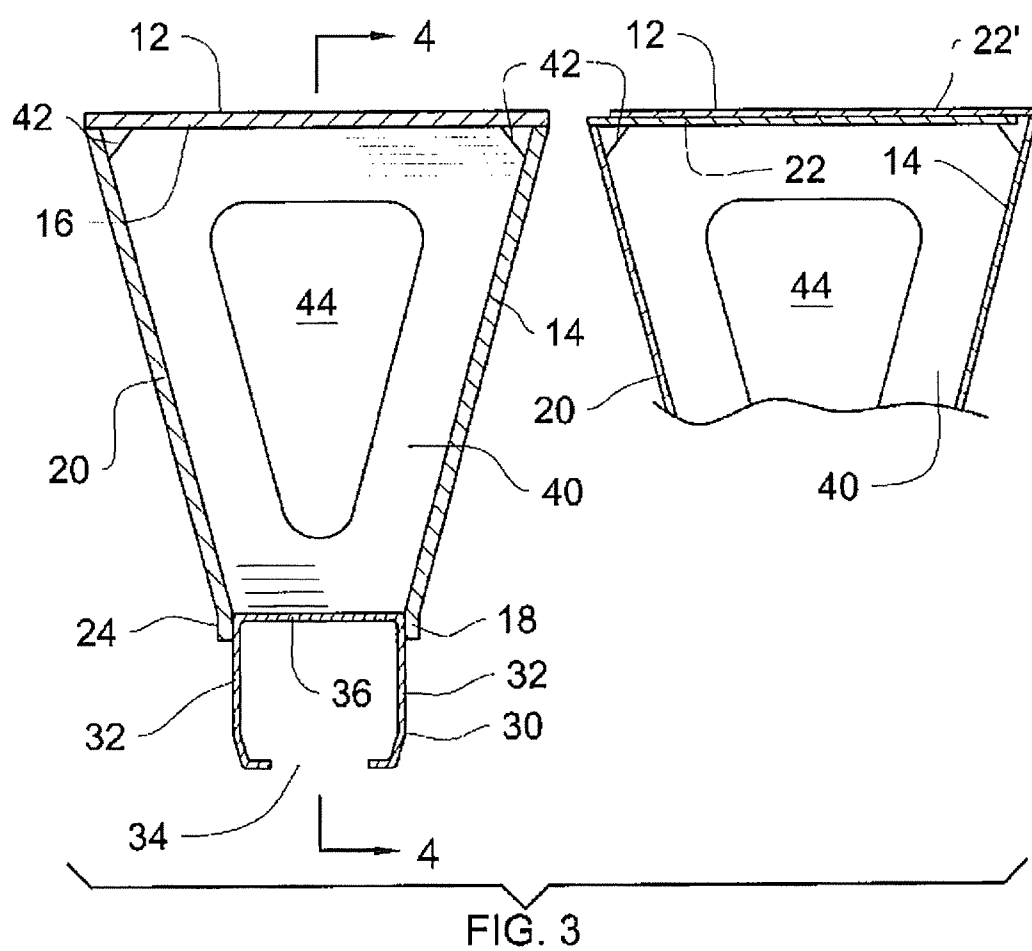
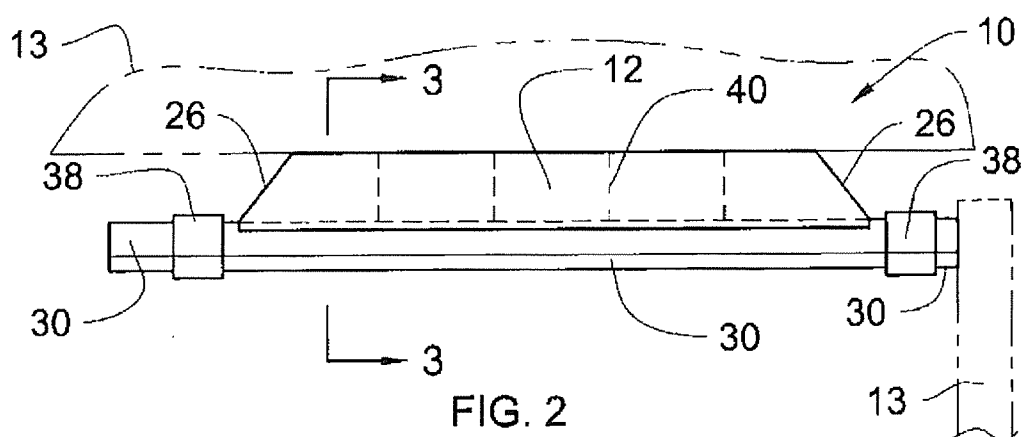


FIG. 1

2 / 21



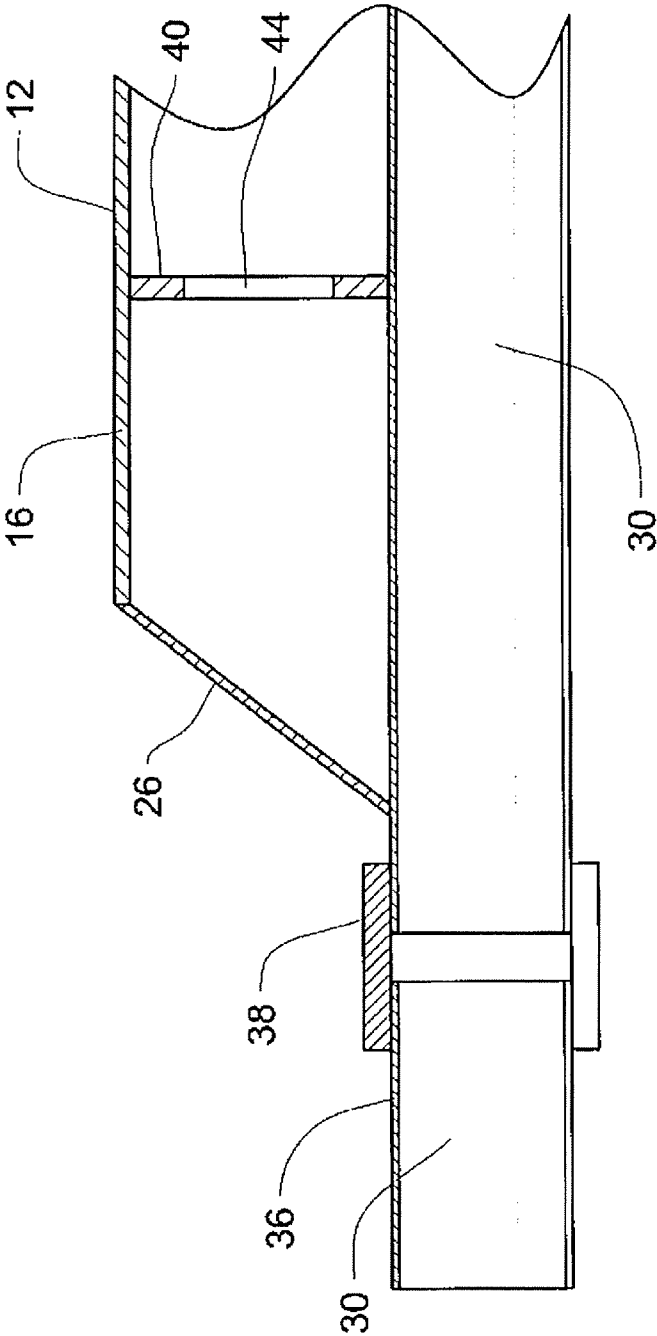
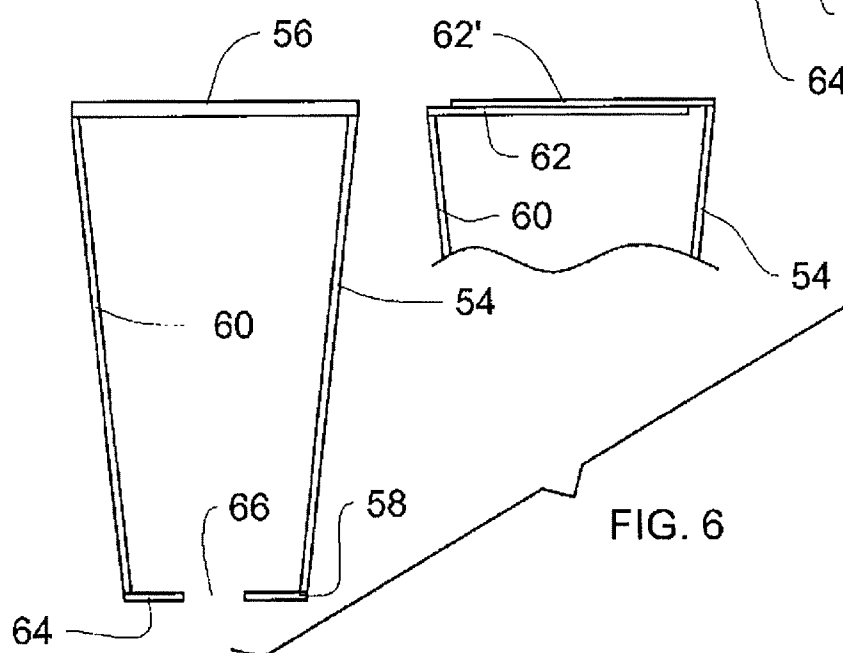
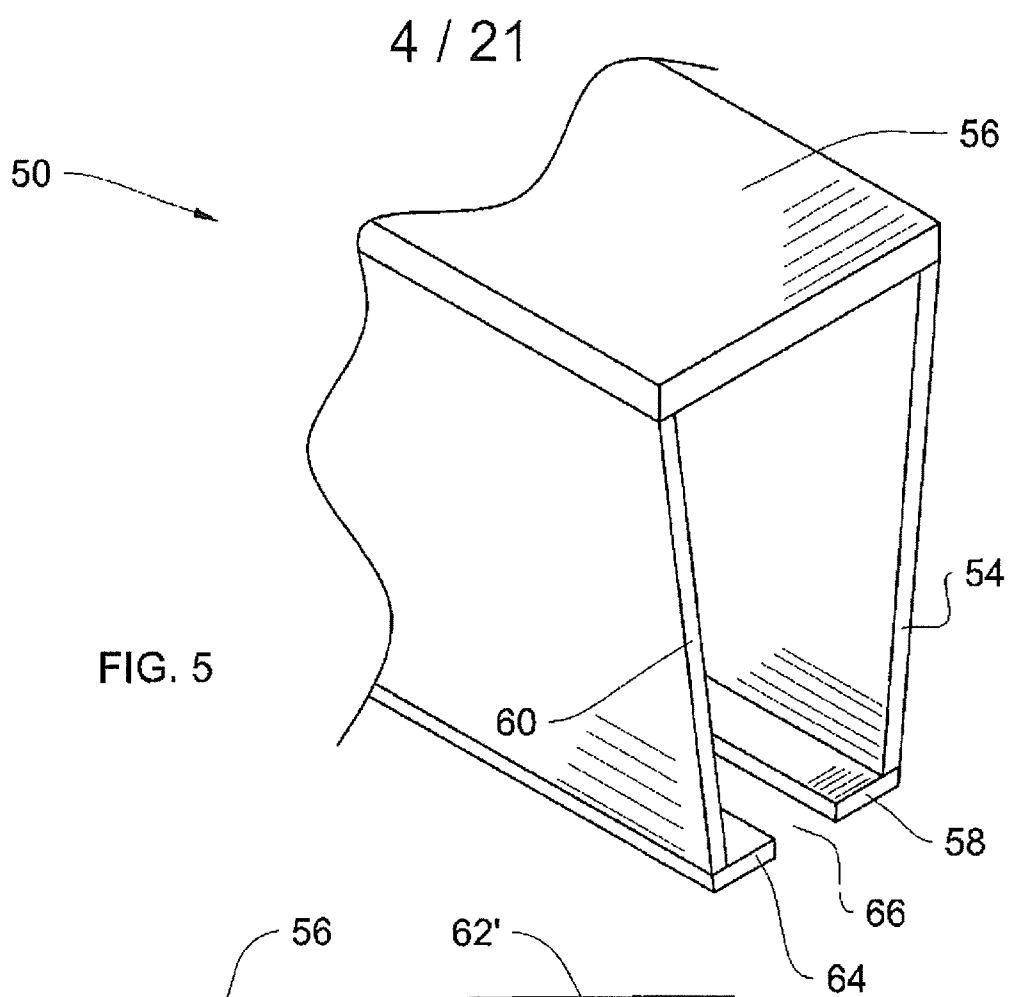


FIG. 4



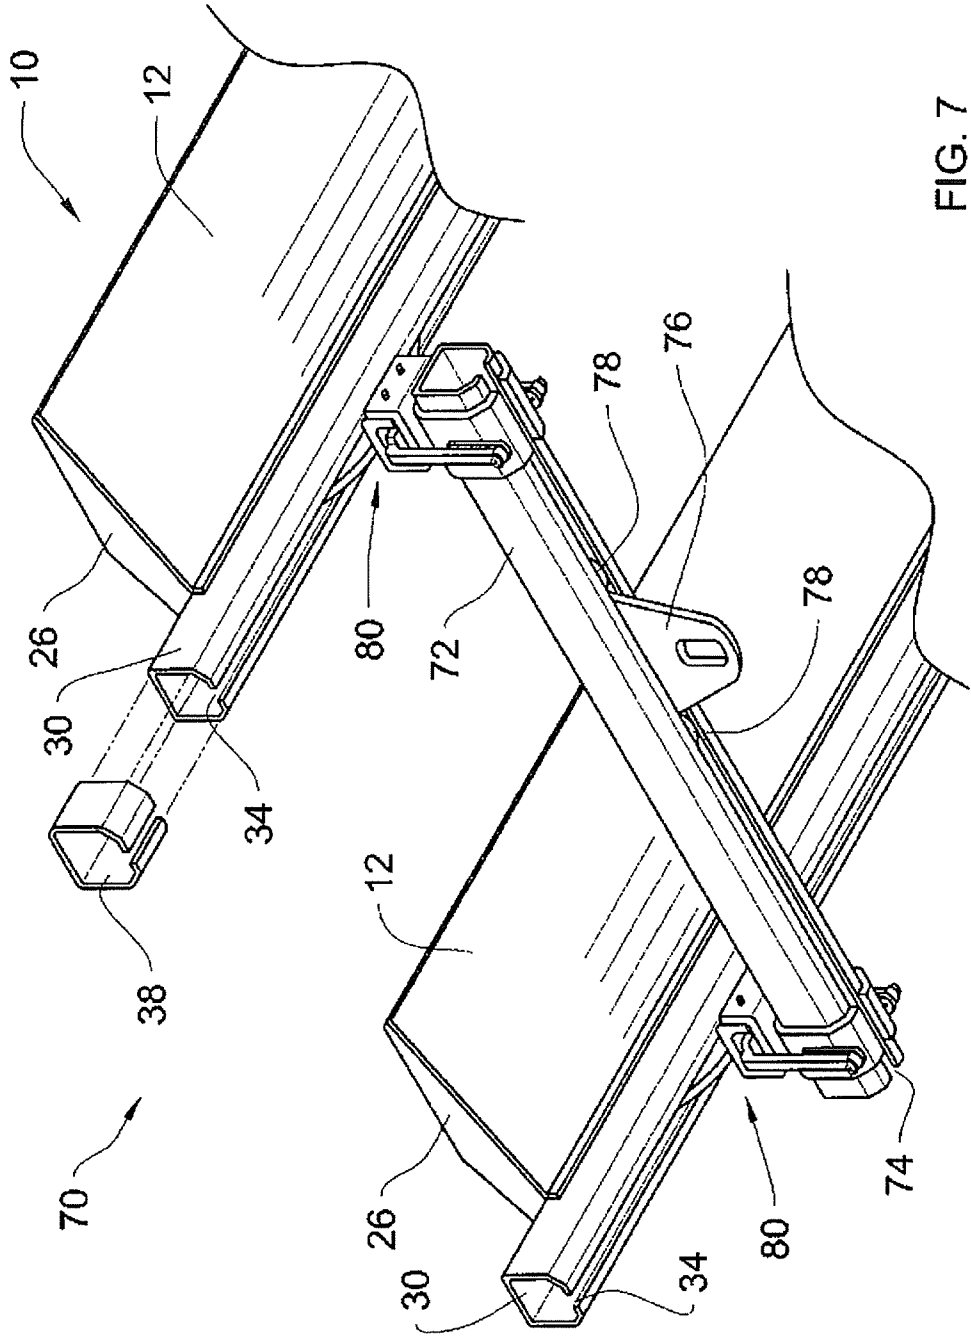


FIG. 7



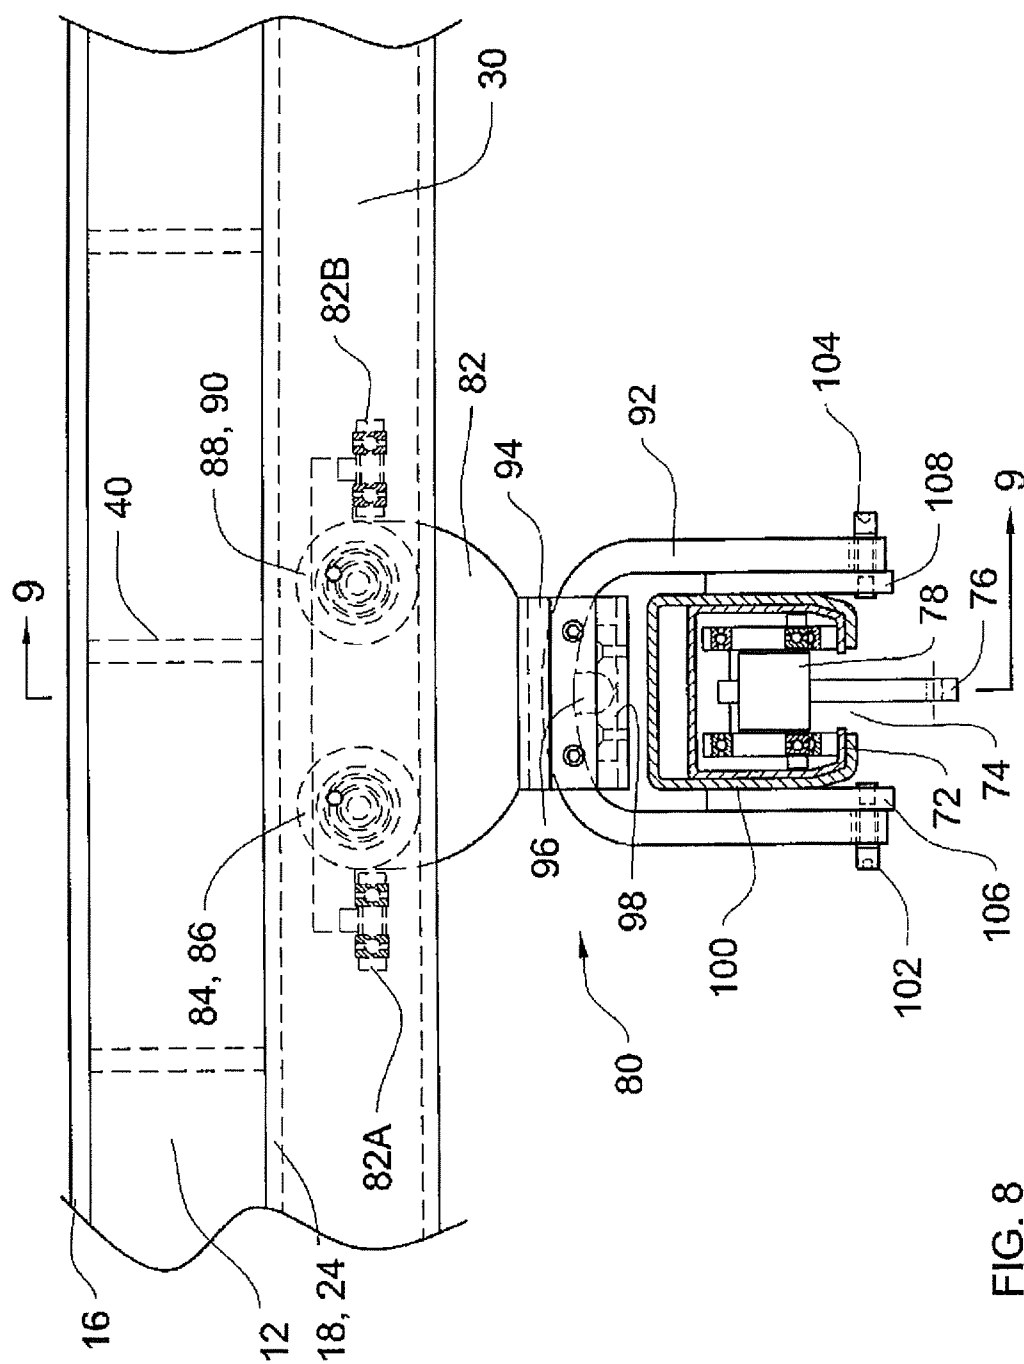


FIG. 8

7 / 21

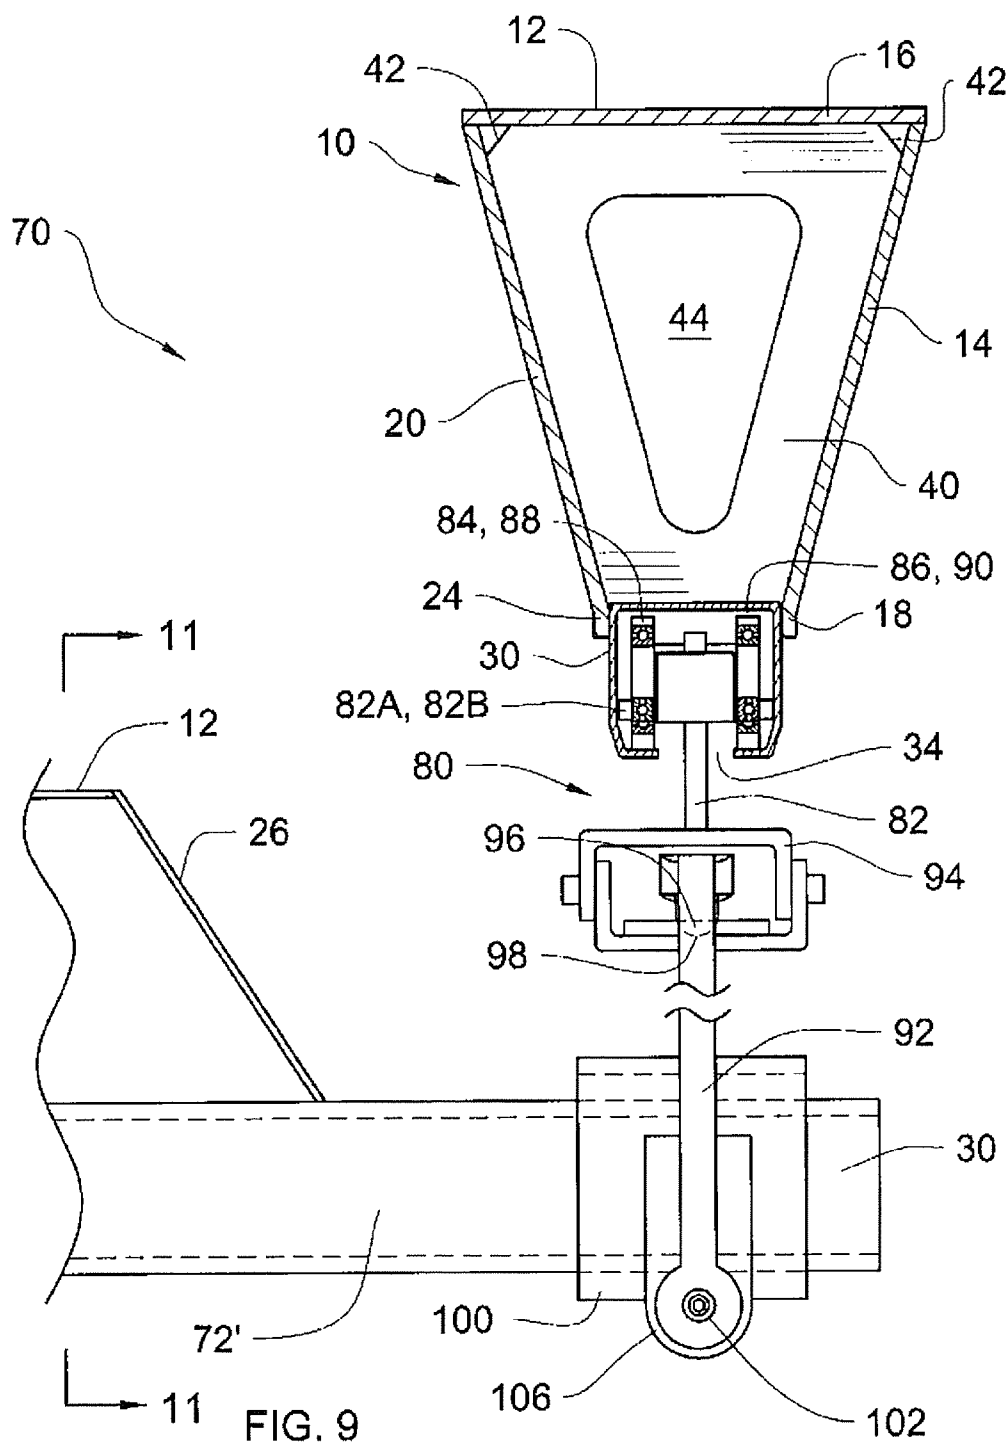

8 / 21

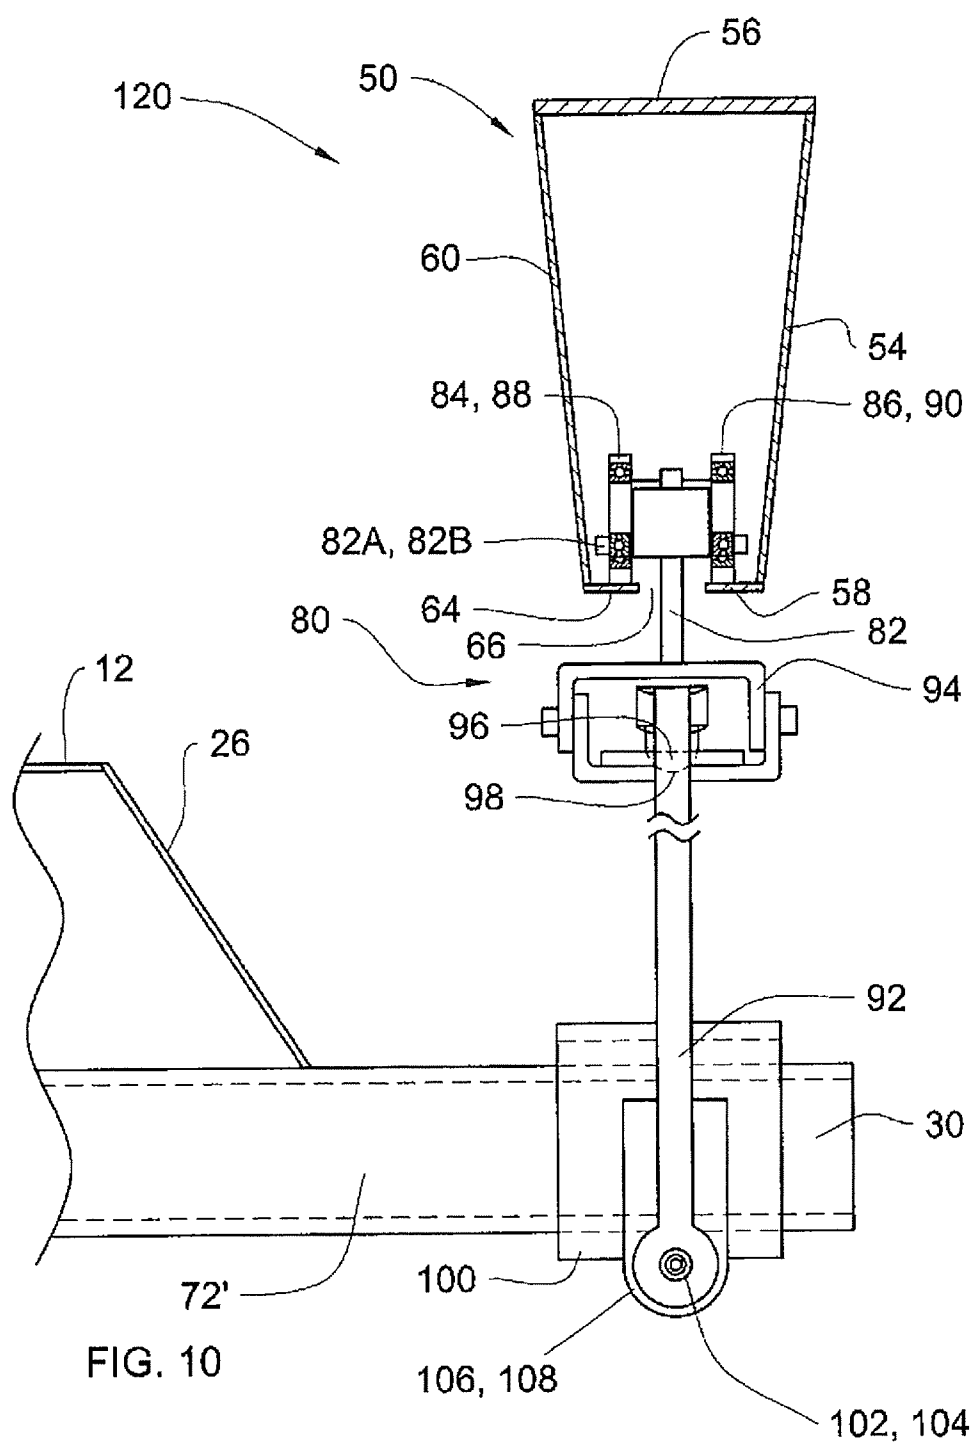

9 / 21

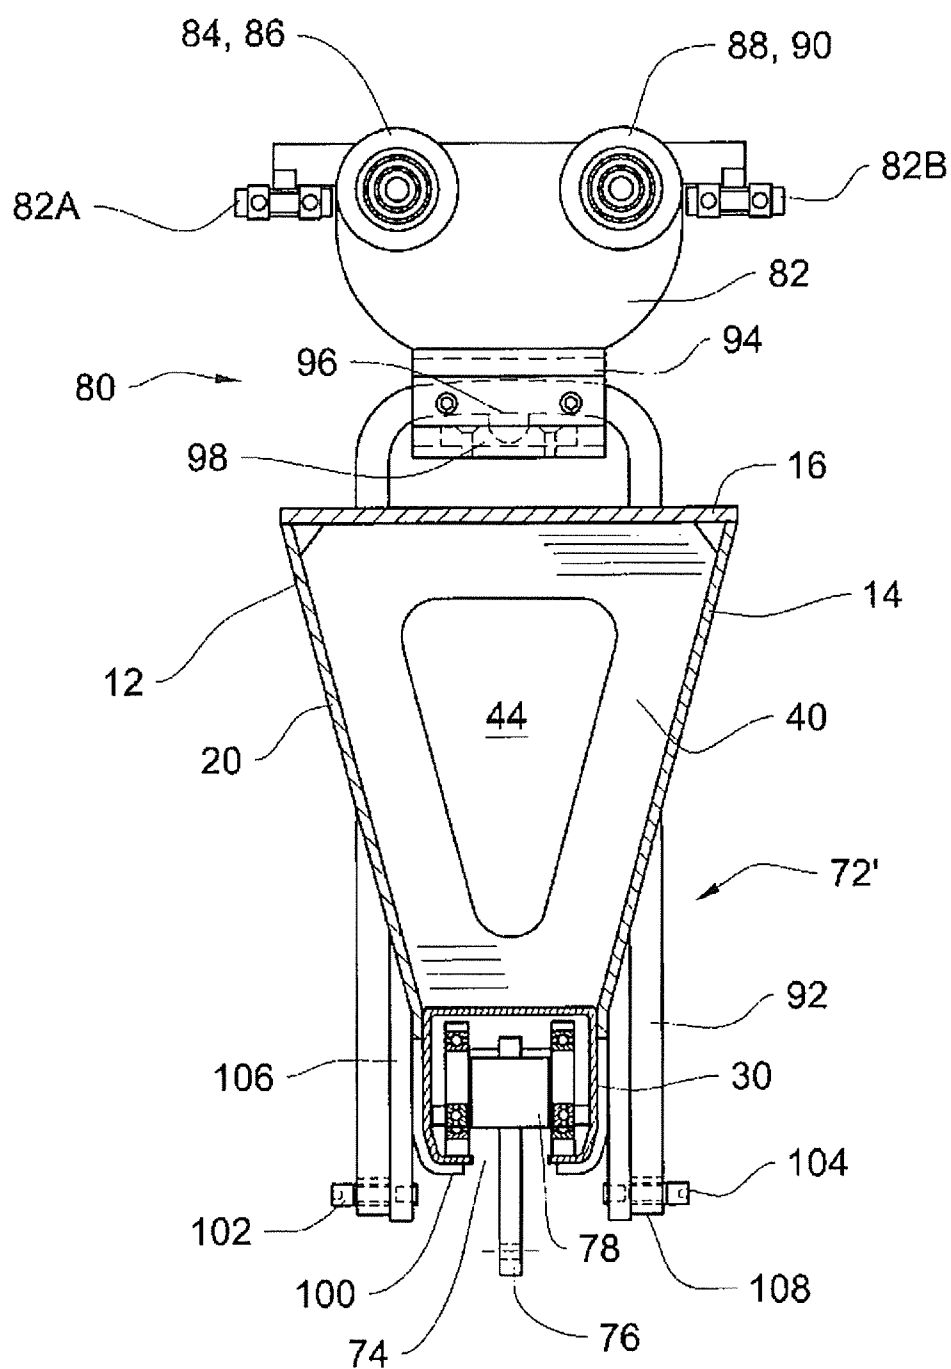


FIG. 11



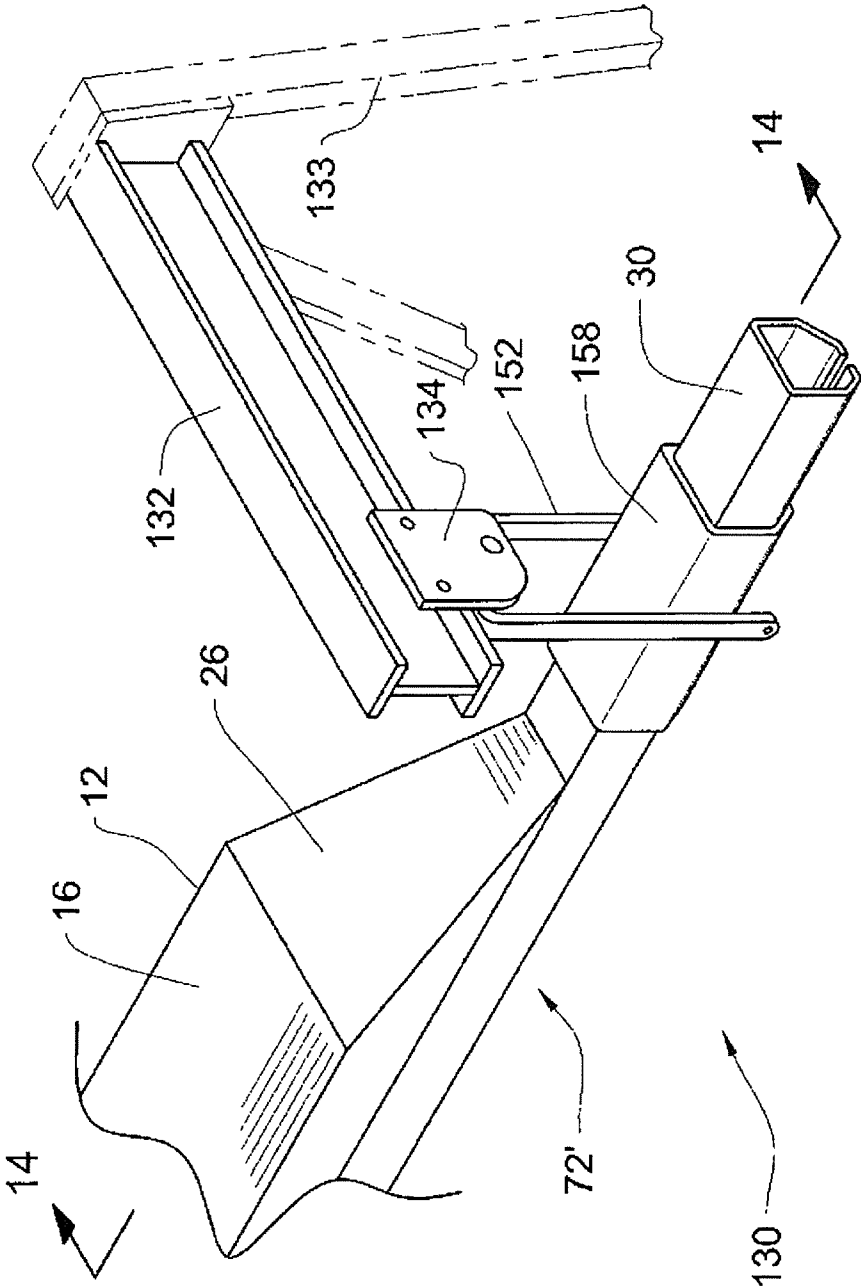


FIG. 13

12 / 21

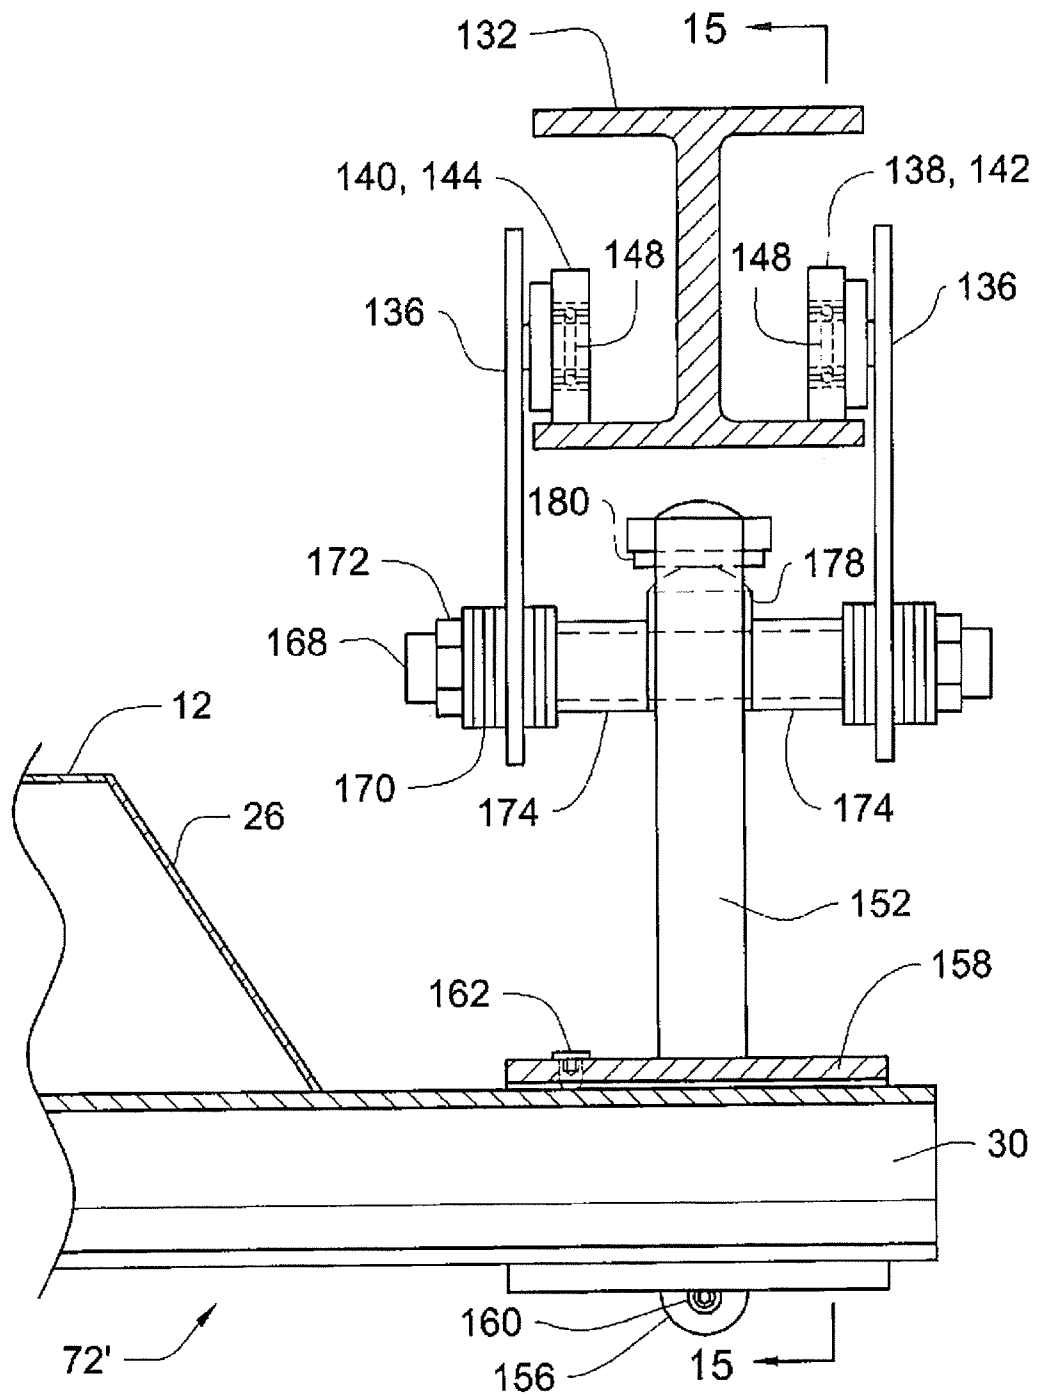


FIG. 14

13 / 21


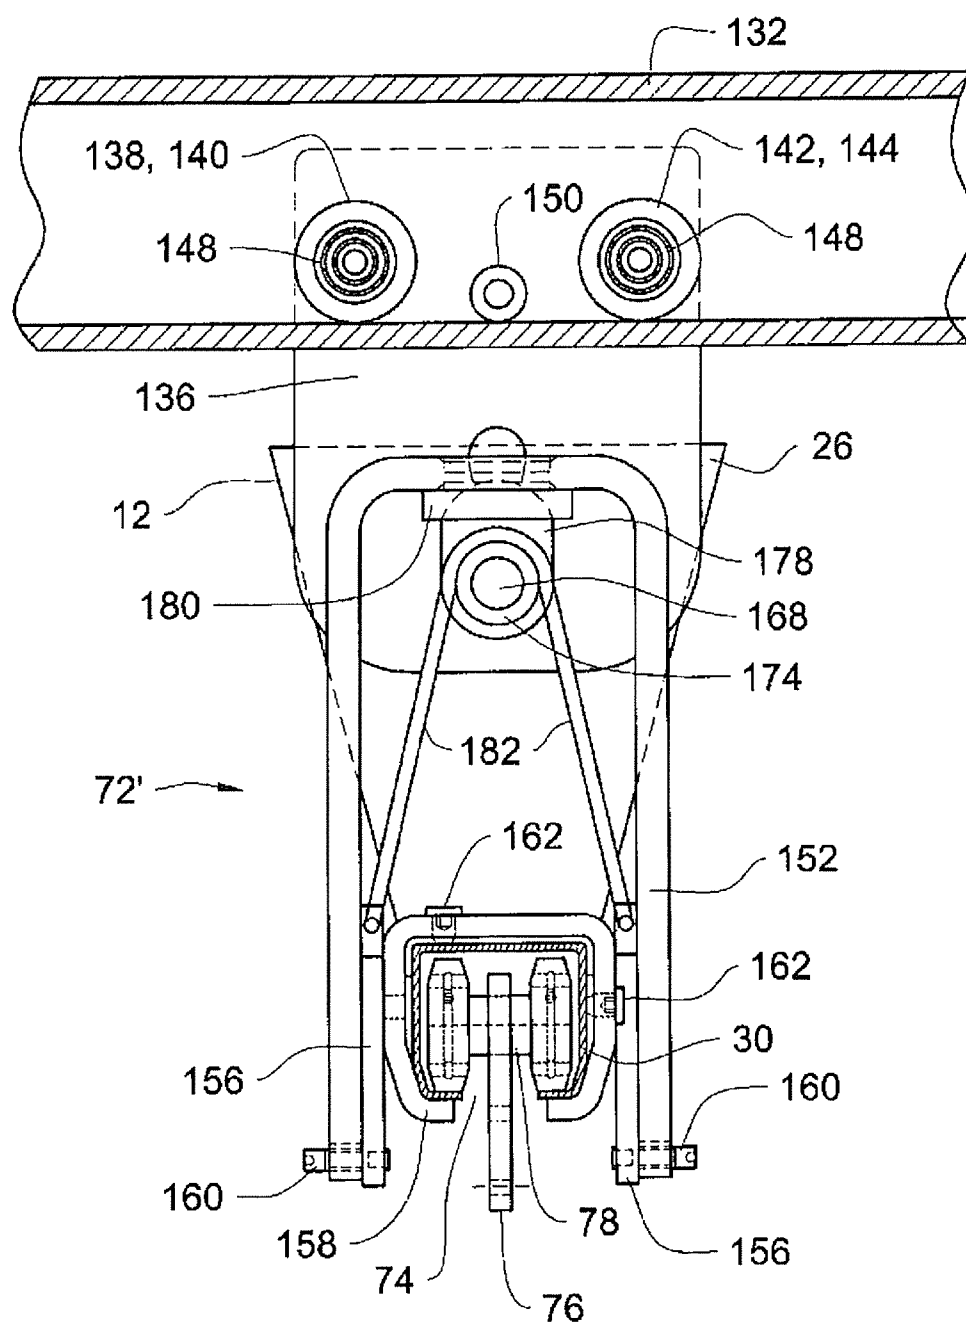


FIG. 15

14/21

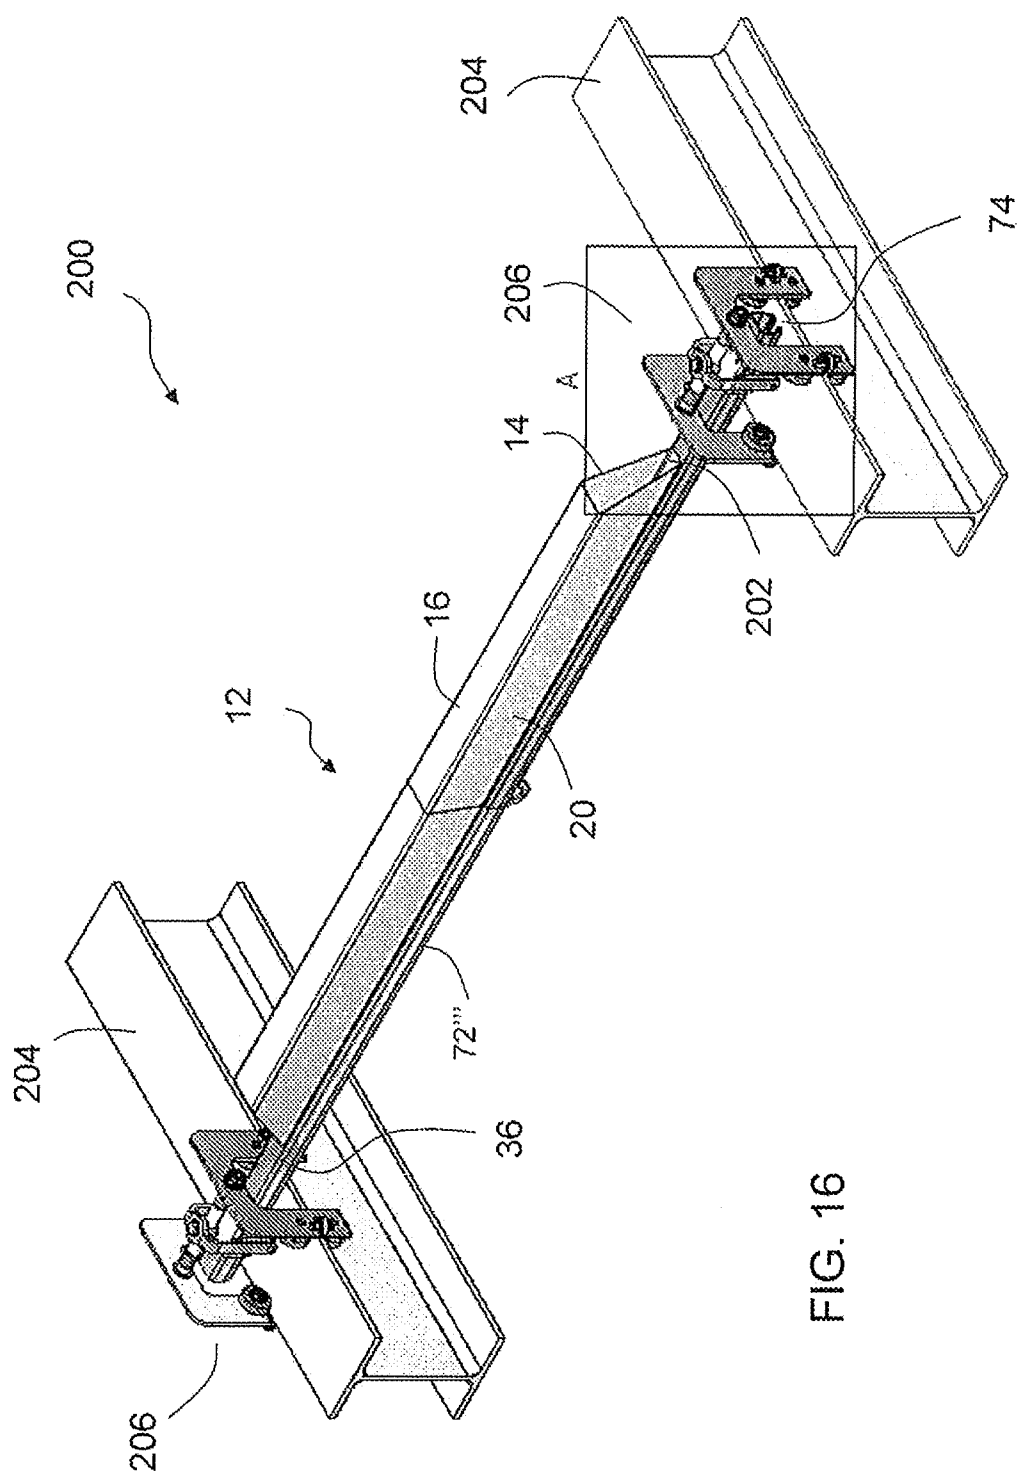

15/21

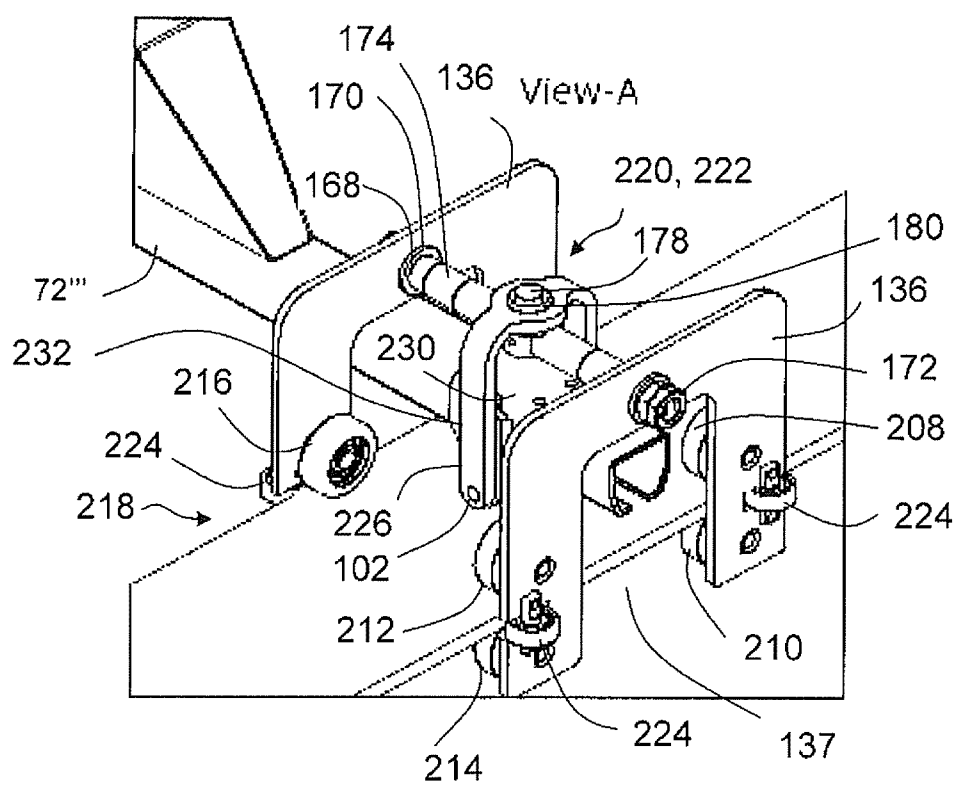


FIG. 17

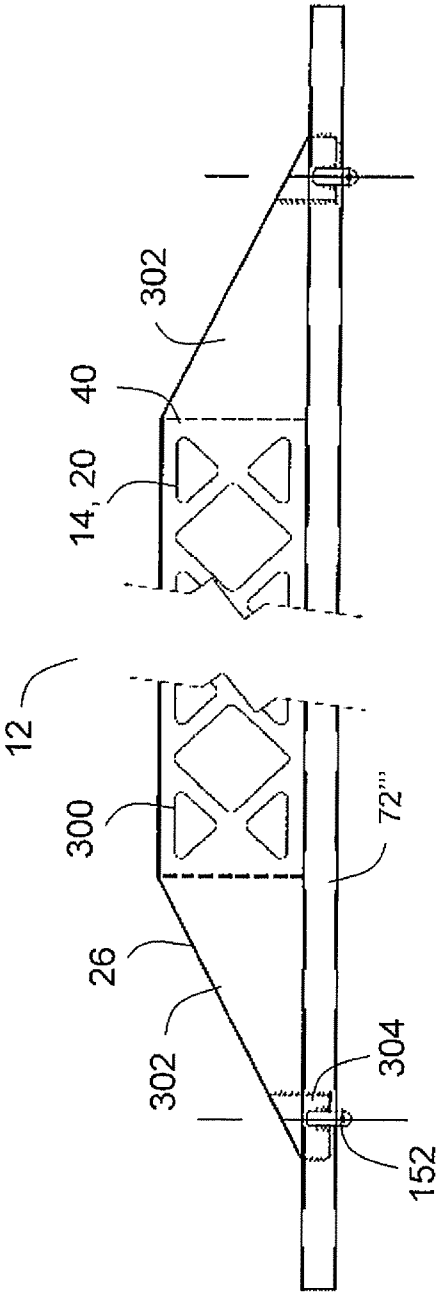


FIG. 18

17/21

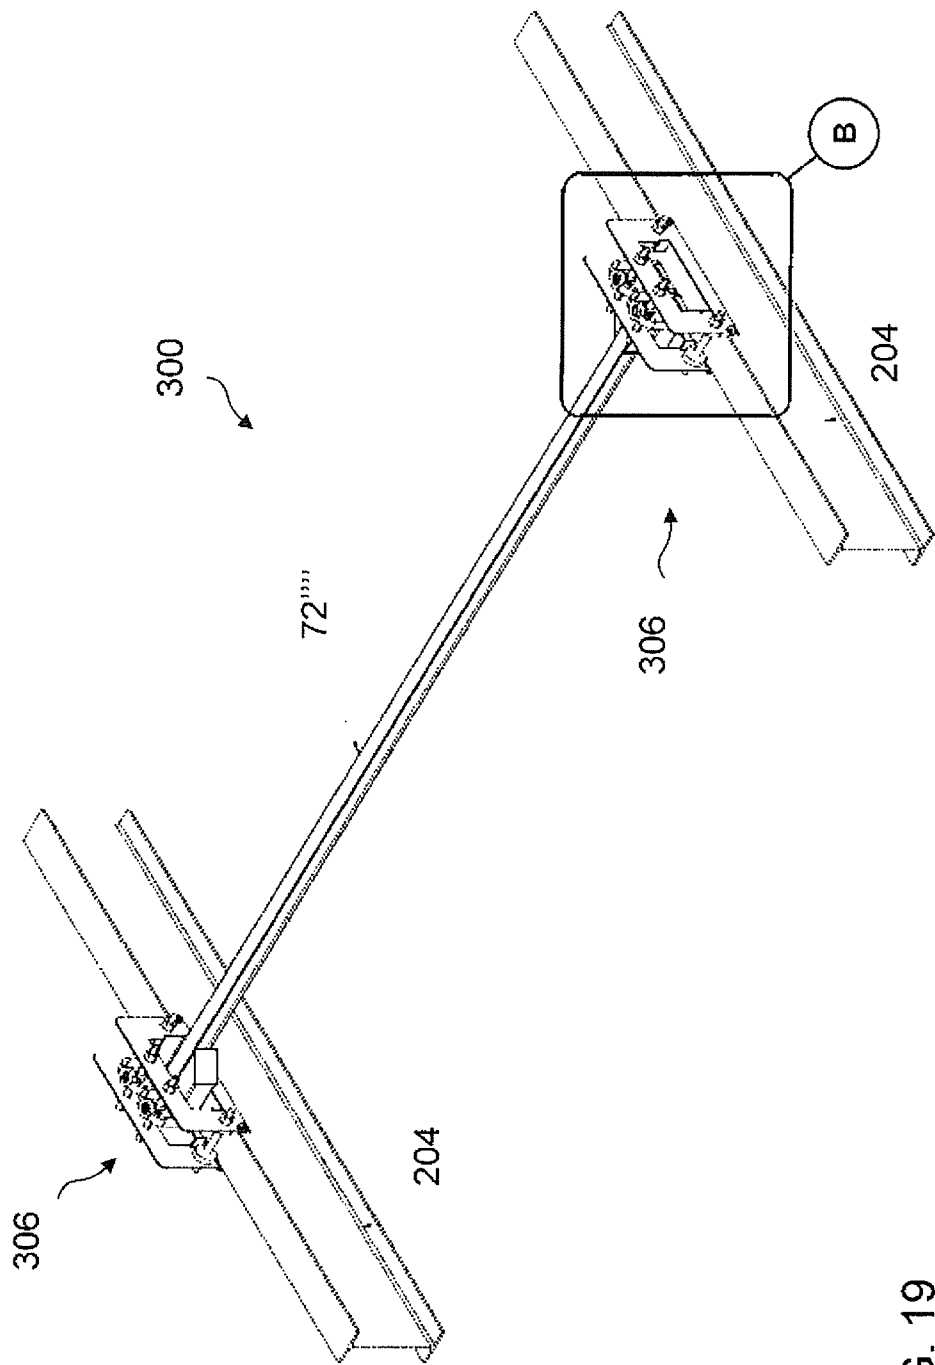


FIG. 19

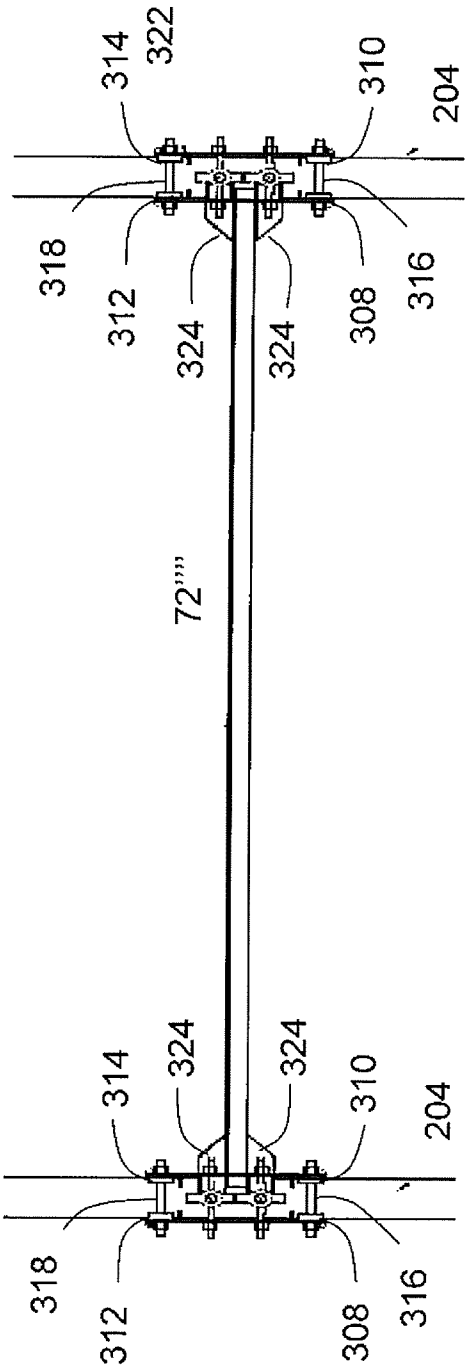


FIG. 20

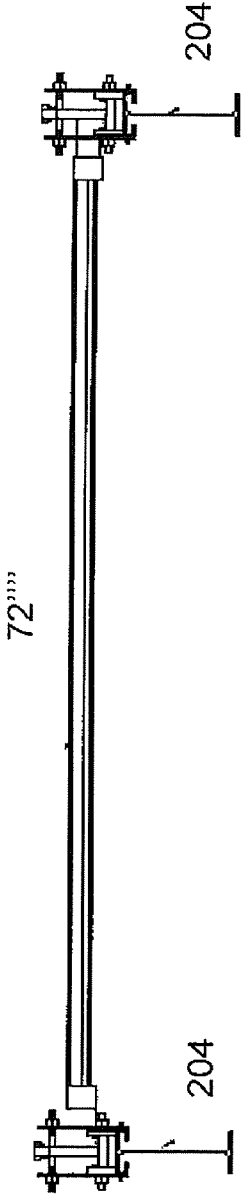


FIG. 21

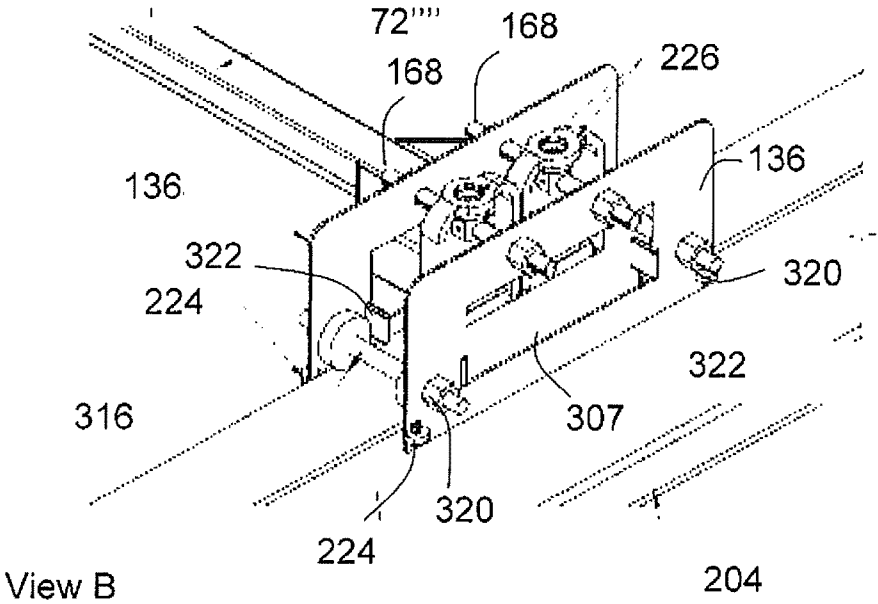


FIG. 22

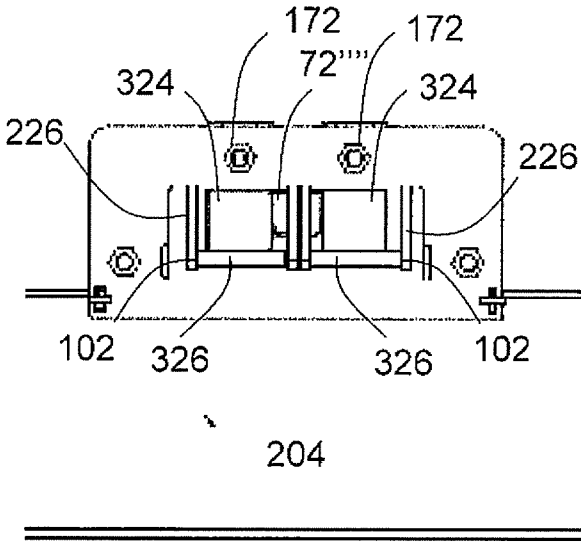


FIG. 23

20/21

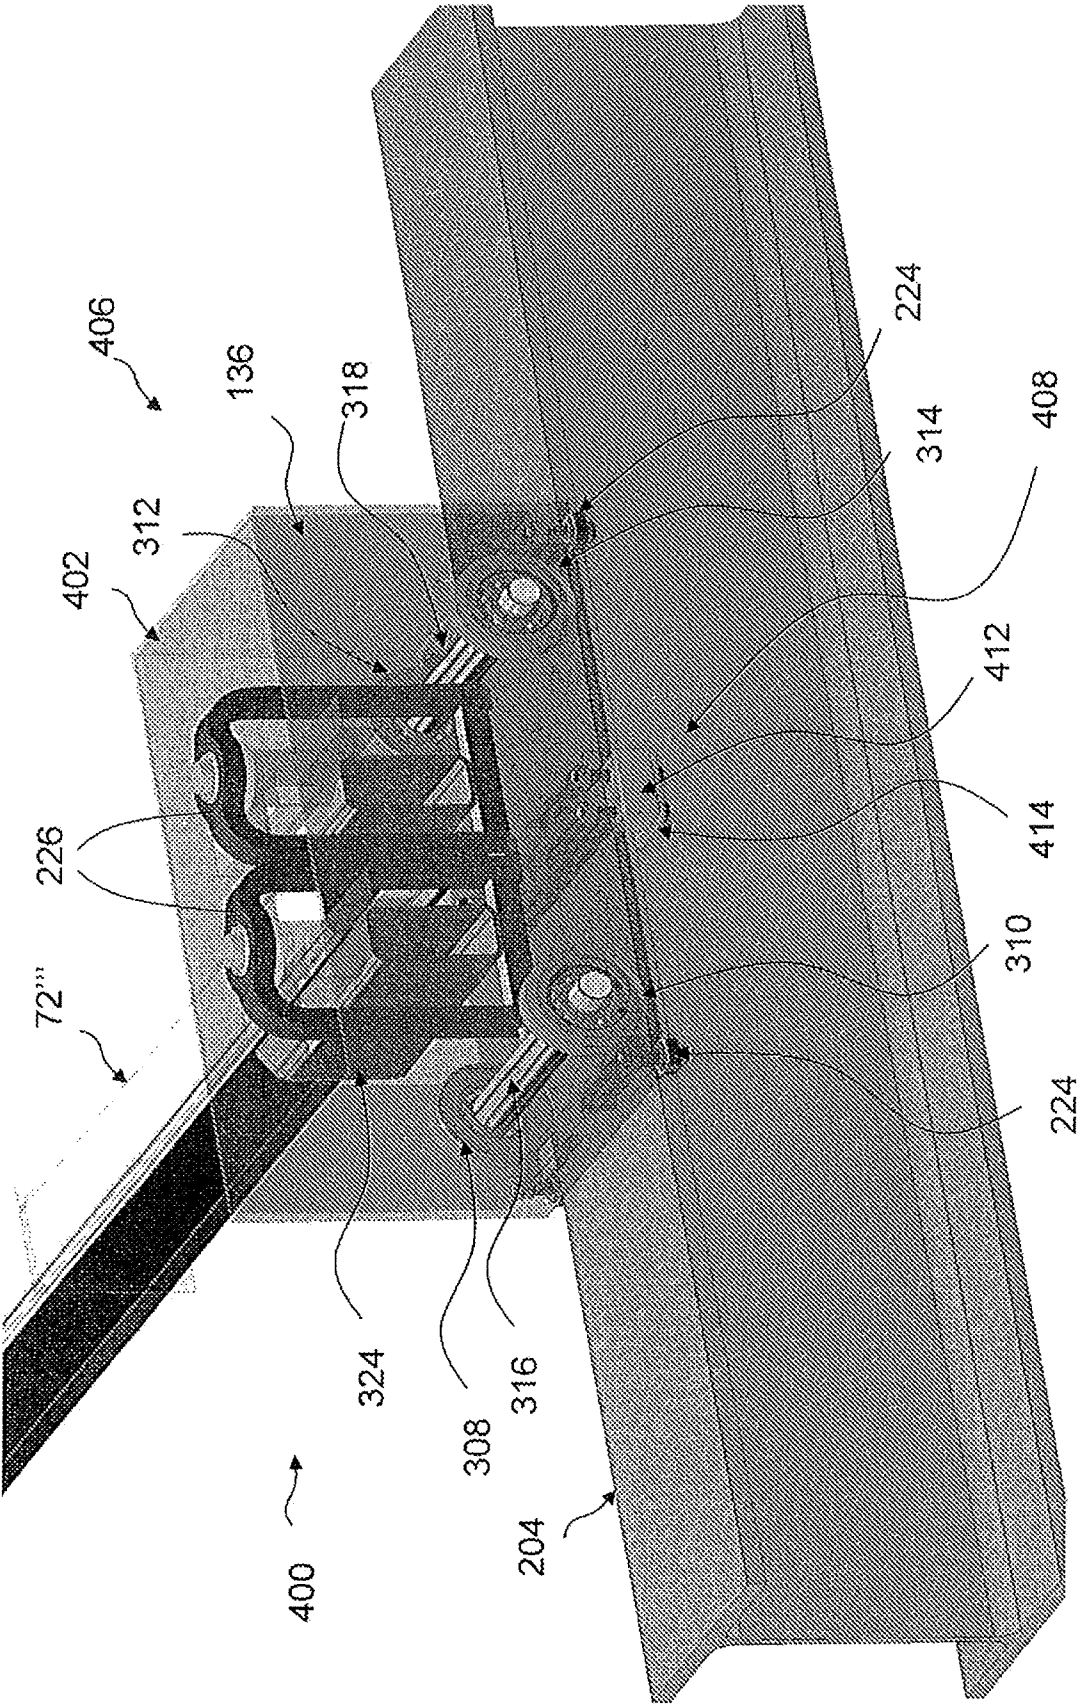


FIG. 24

21/21

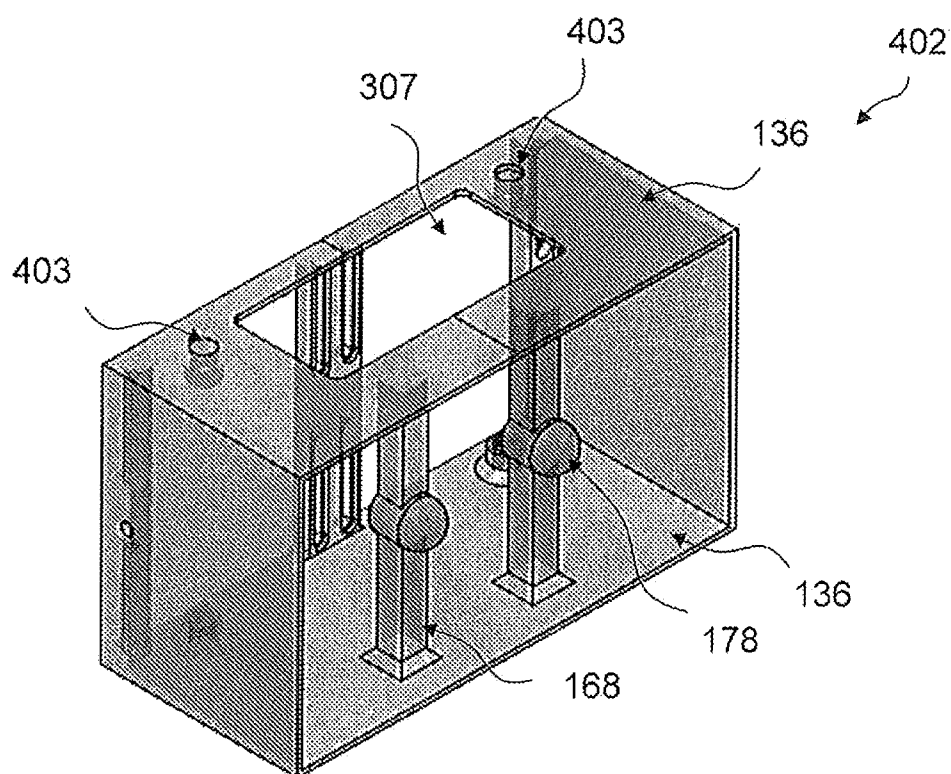


FIG. 25

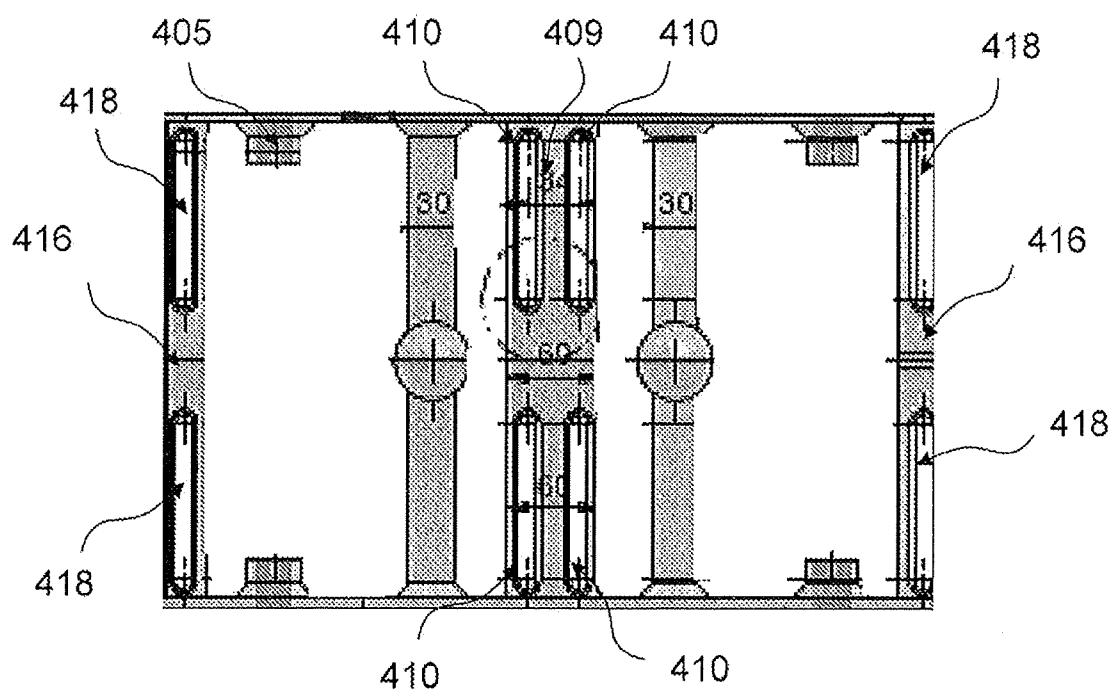


FIG. 26