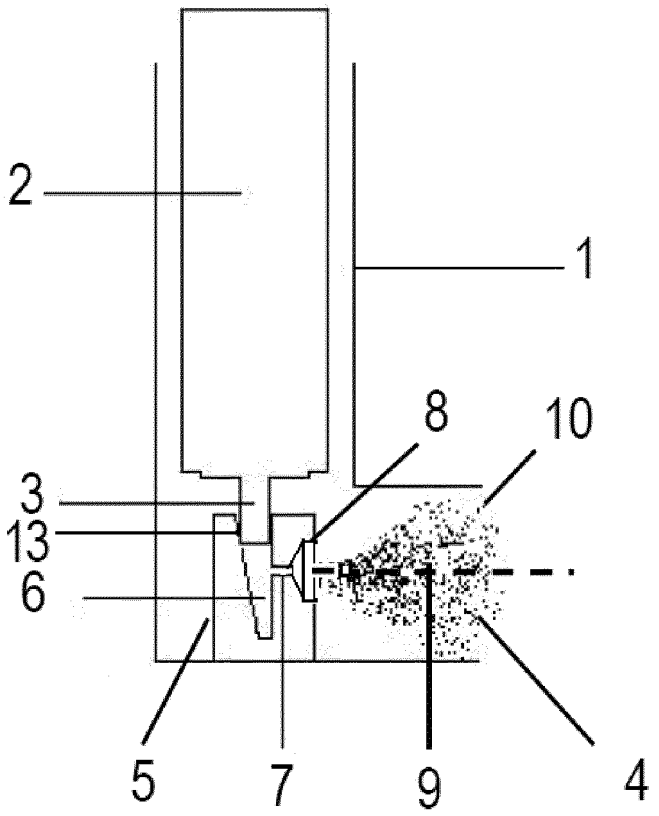


Figure 1

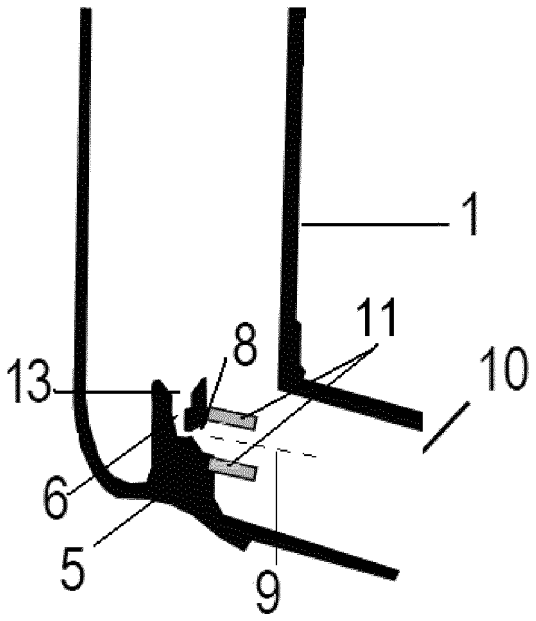


Figure 2

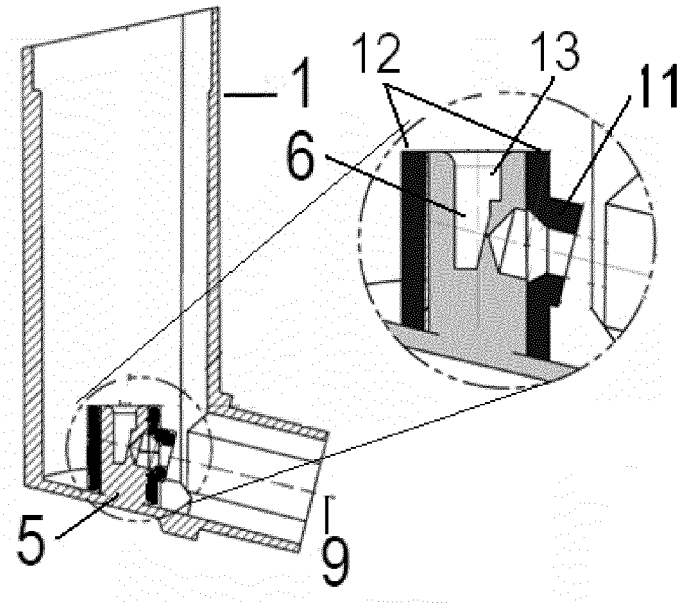


Figure 3A

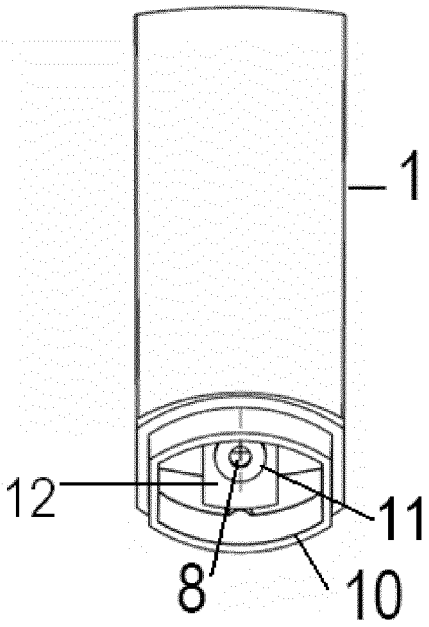


Figure 3B

Figure 3C

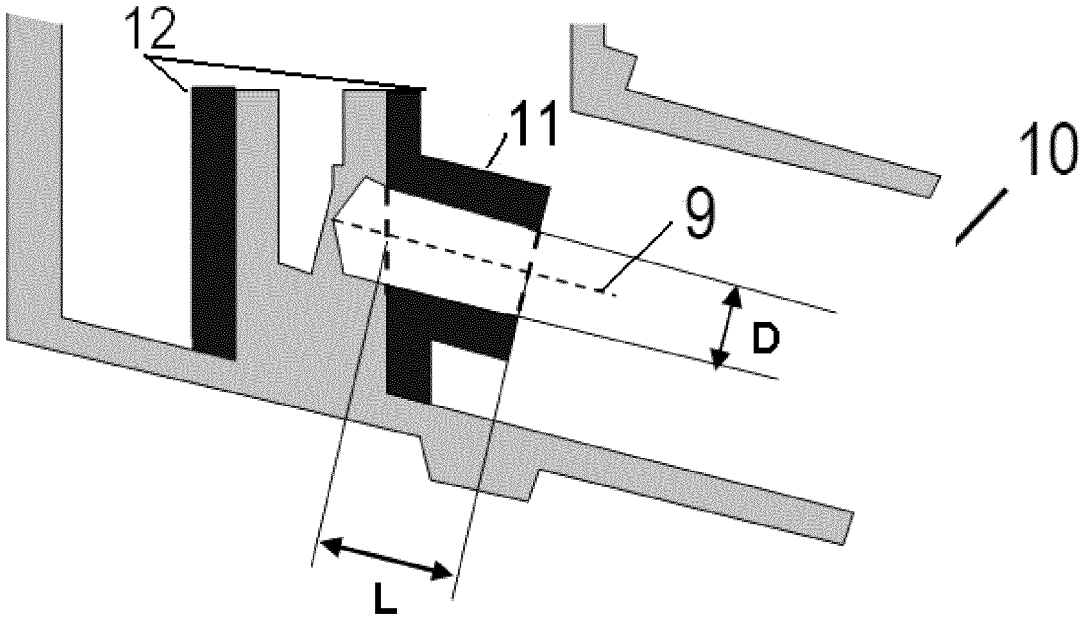


Figure 4

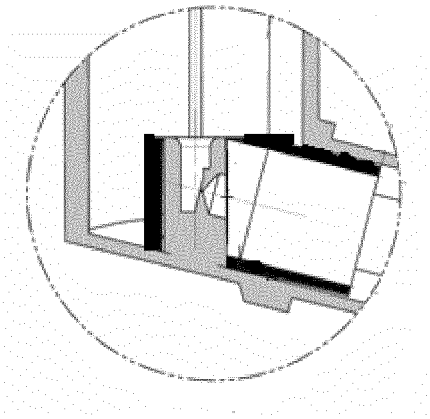


Figure 5

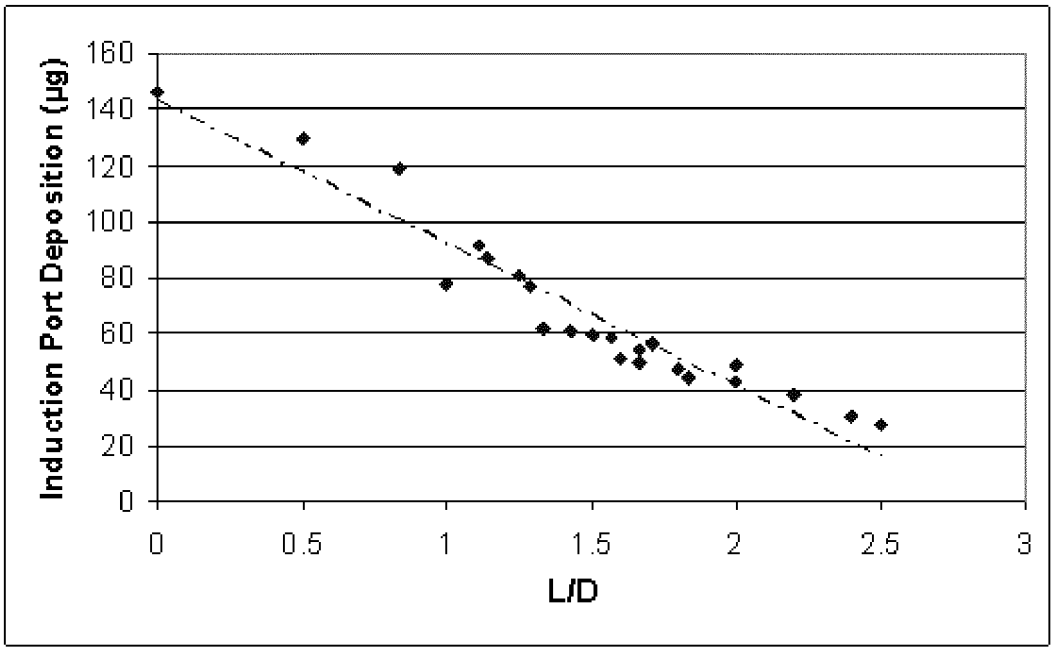


Figure 6

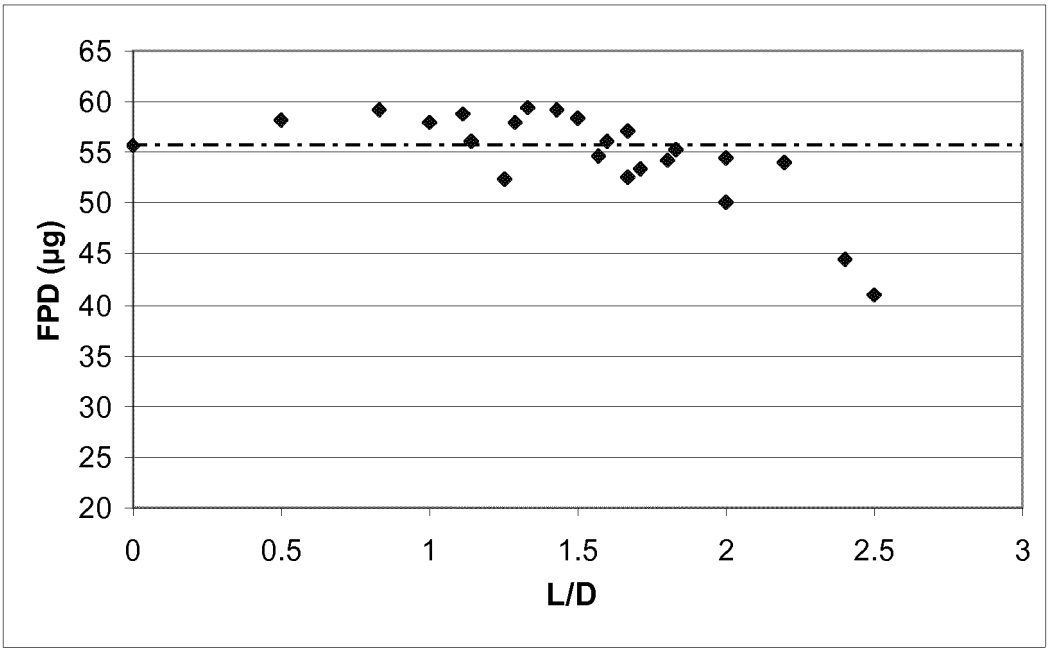


Figure 7

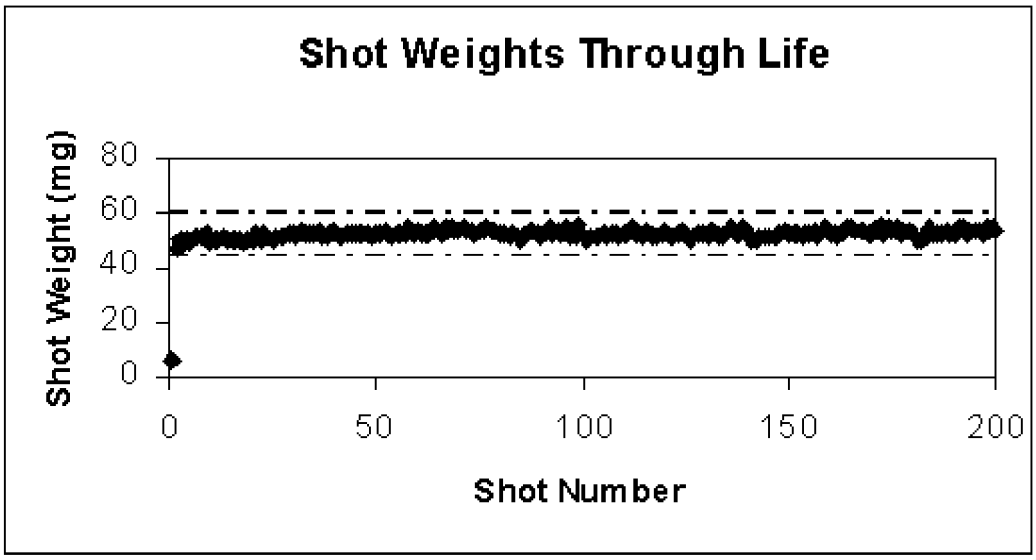


Figure 8

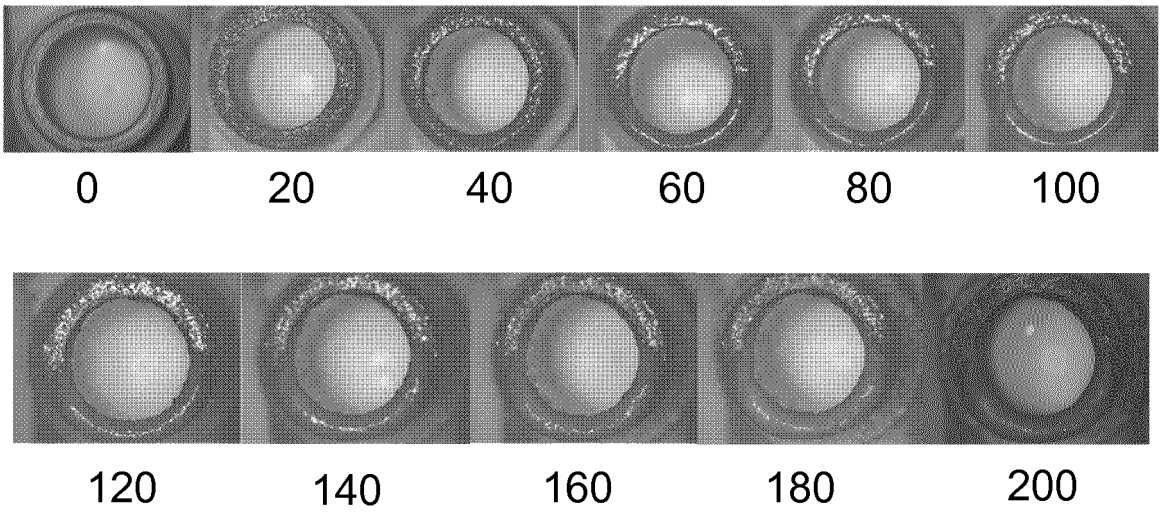


Figure 9

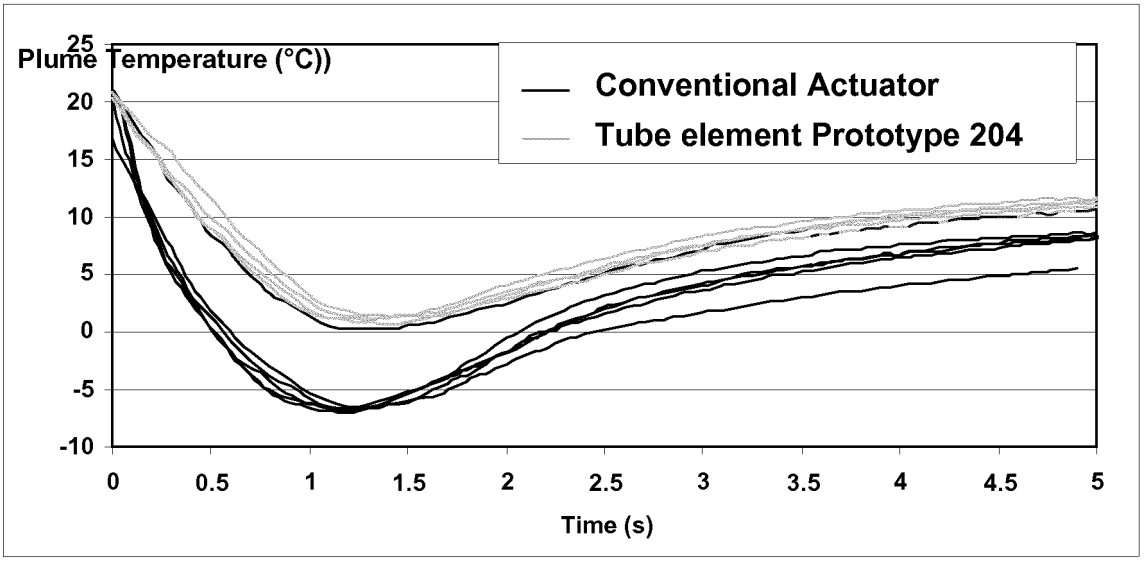


Figure 10

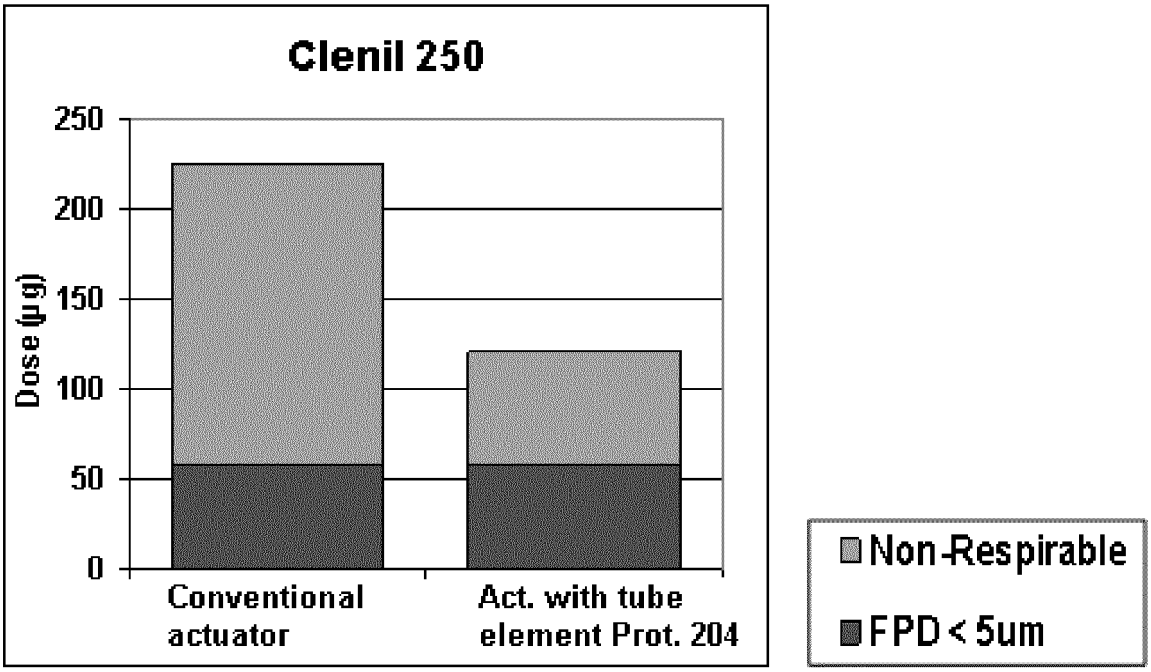


Figure 11

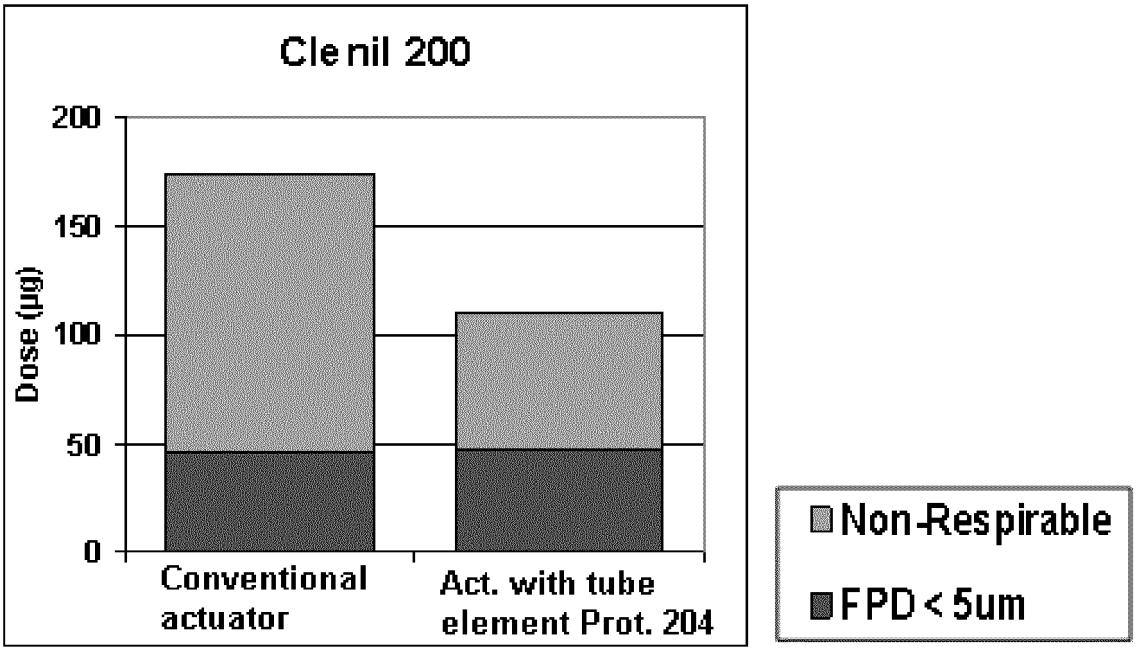


Figure 12

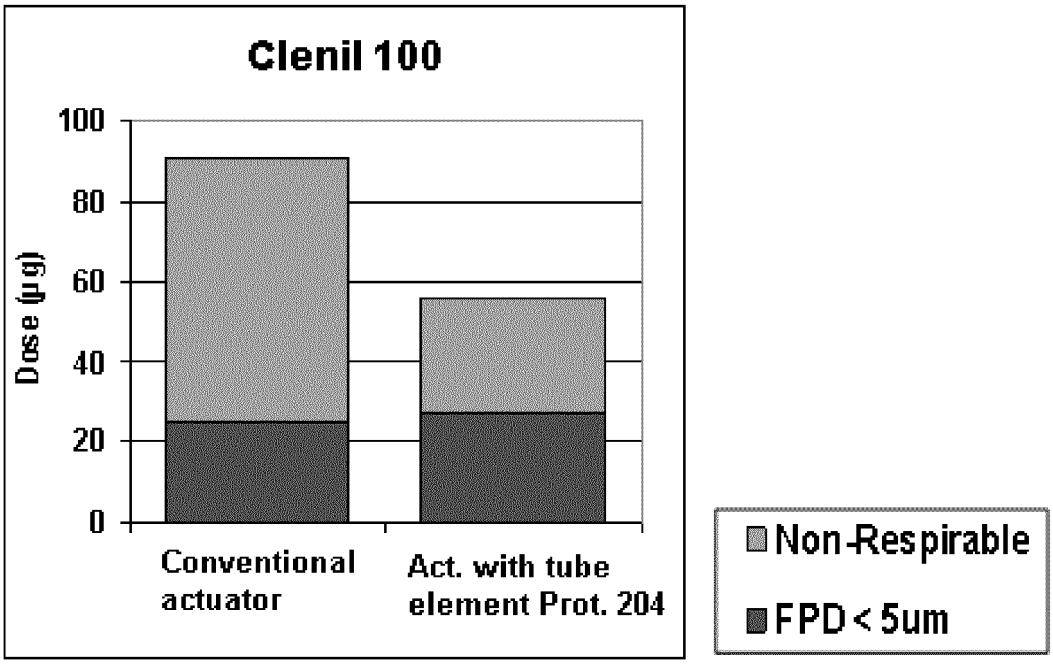


Figure 13

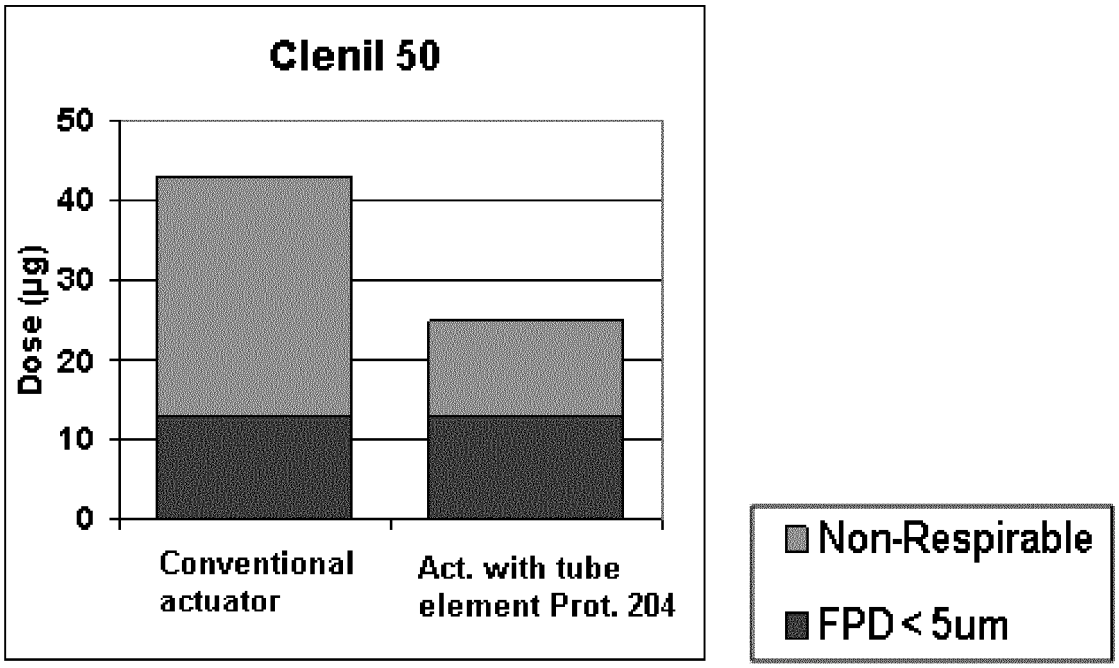


Figure 14

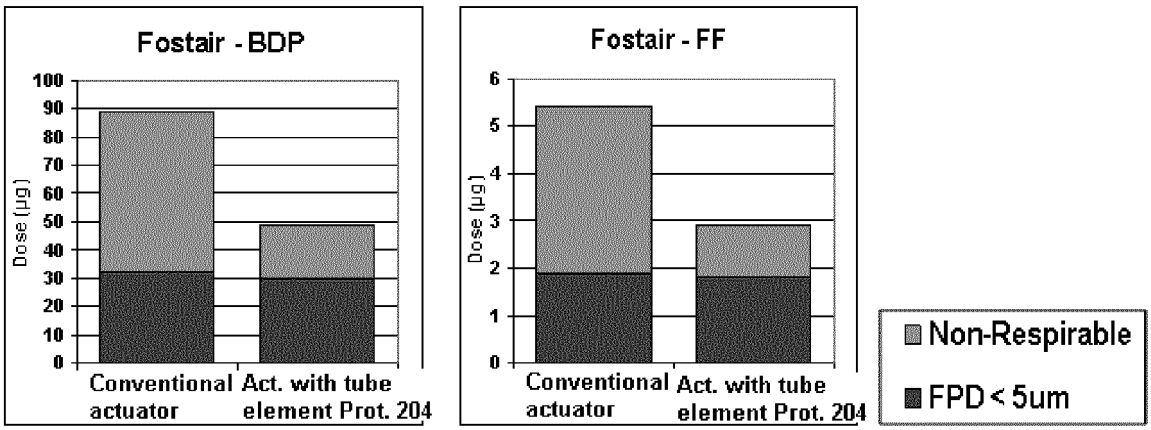

Fostair - BDP
Dose (µg)
100
90
80
70
60
50
40
30
20
10
0
Conventional actuator
Act. with tube element Prot. 204
Fostair - FF
Dose (µg)
6
5
4
3
2
1
0
Conventional actuator
Act. with tube element Prot. 204
Non-Respirable
FPD < 5um

Figure 15

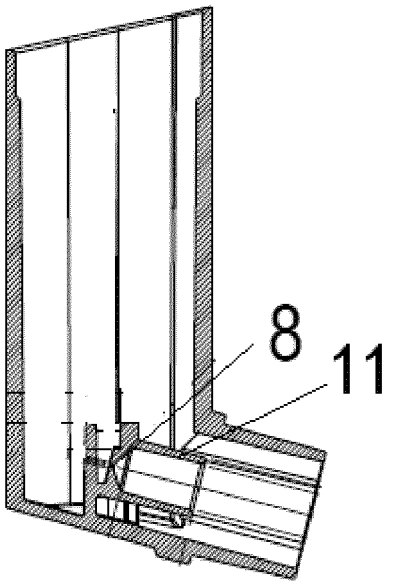


Figure 16A

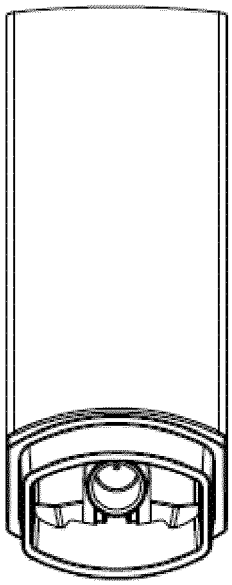


Figure 16B

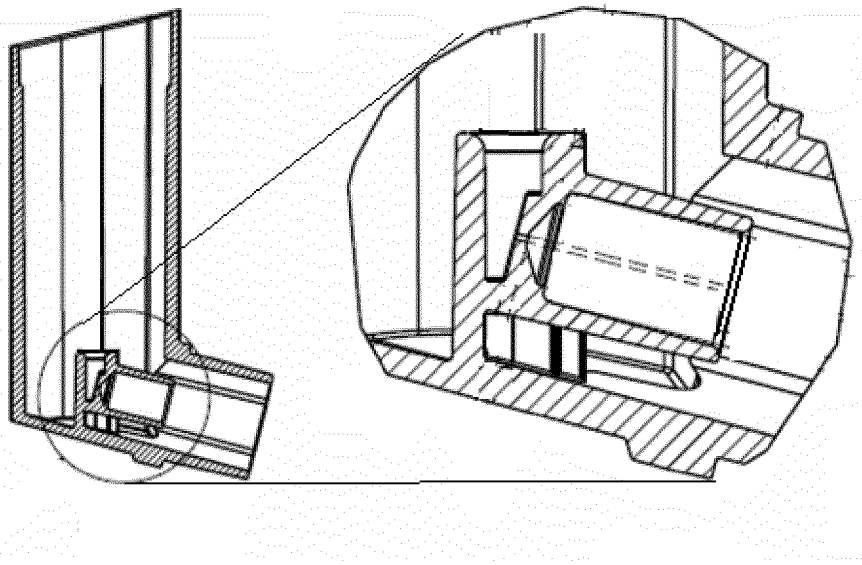


Figure 17A

Figure 17B

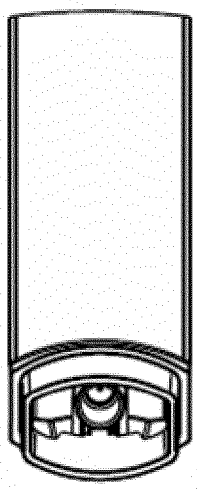


Figure 17C

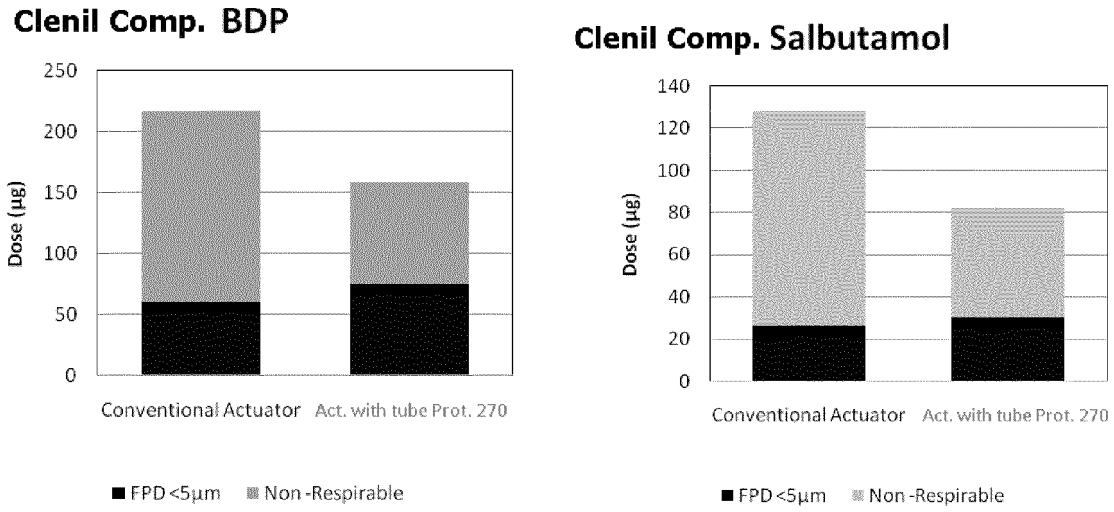


Figure 18

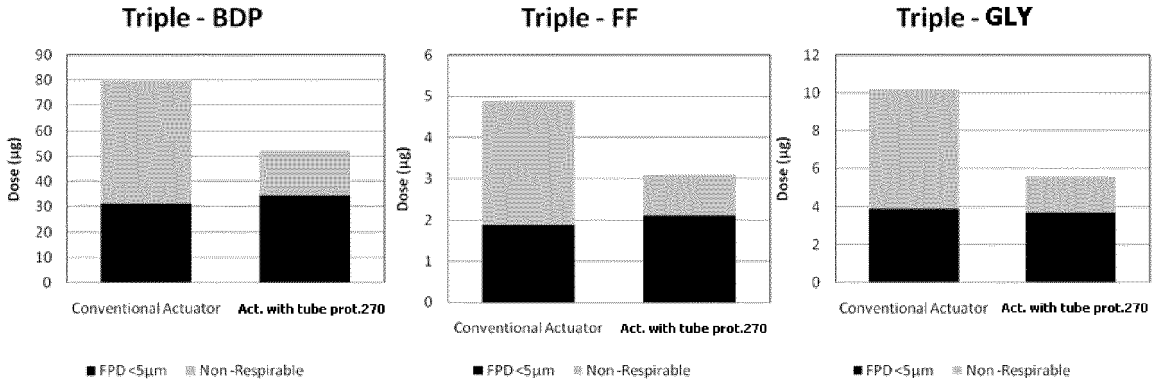


Figure 19

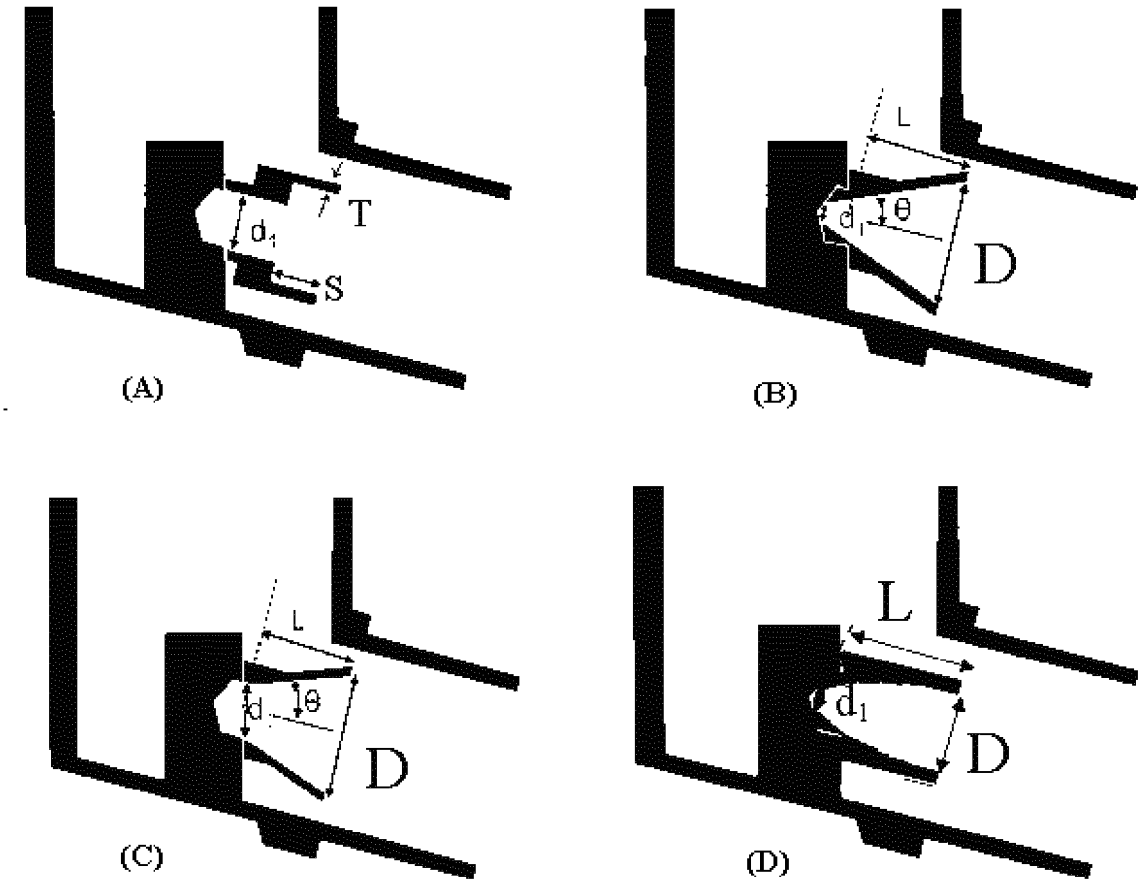


Figure 20