

1/2

INSTRUMENT BROADENING APPLIED:
PSEUDO-VOIGT 0.1 -0.036 0.040 0.6

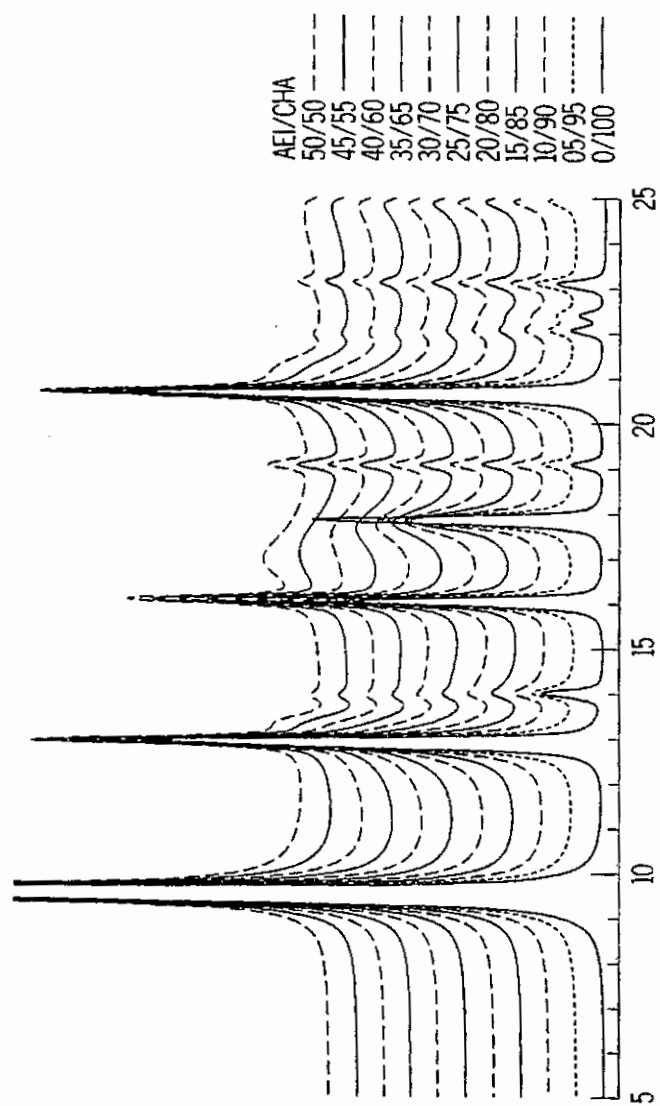


FIG. 1a

2/2

INSTRUMENT BROADENING APPLIED:
PSEUDO-VOIGT 0.1 -0.036 0.040 0.6

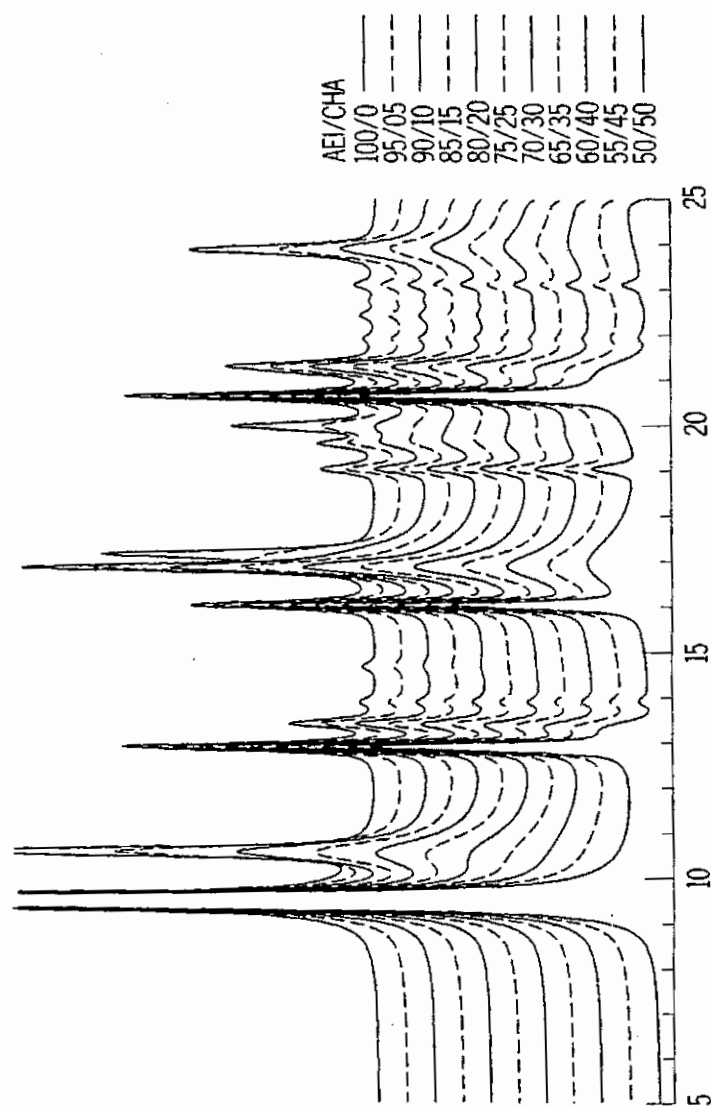


FIG. 1b