

1/8

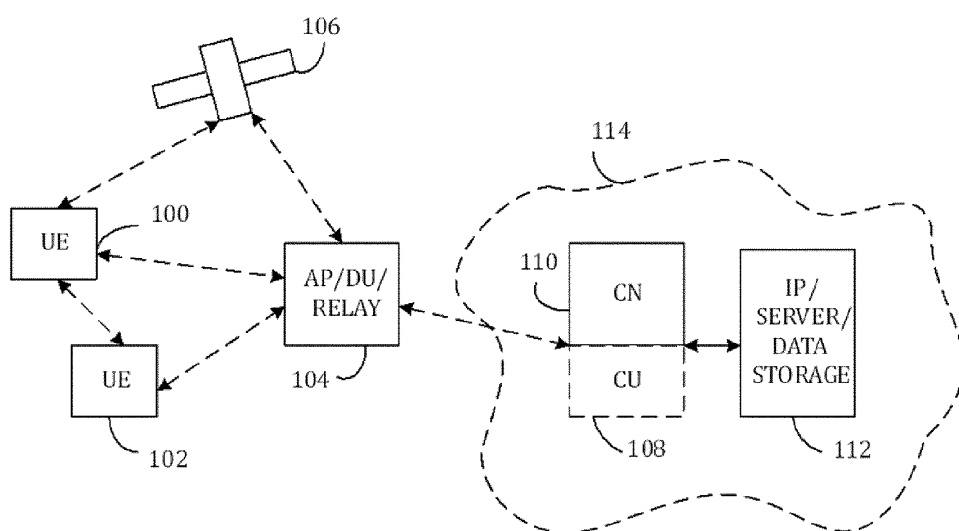


FIG. 1

2/8

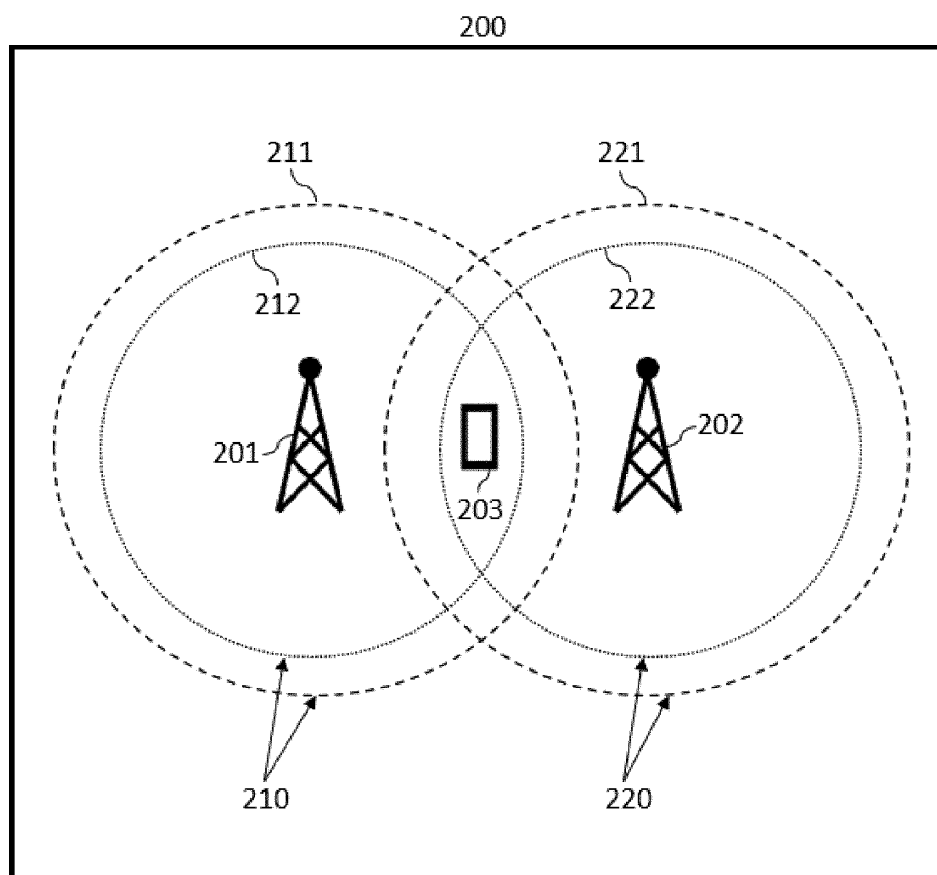


FIG. 2

3/8

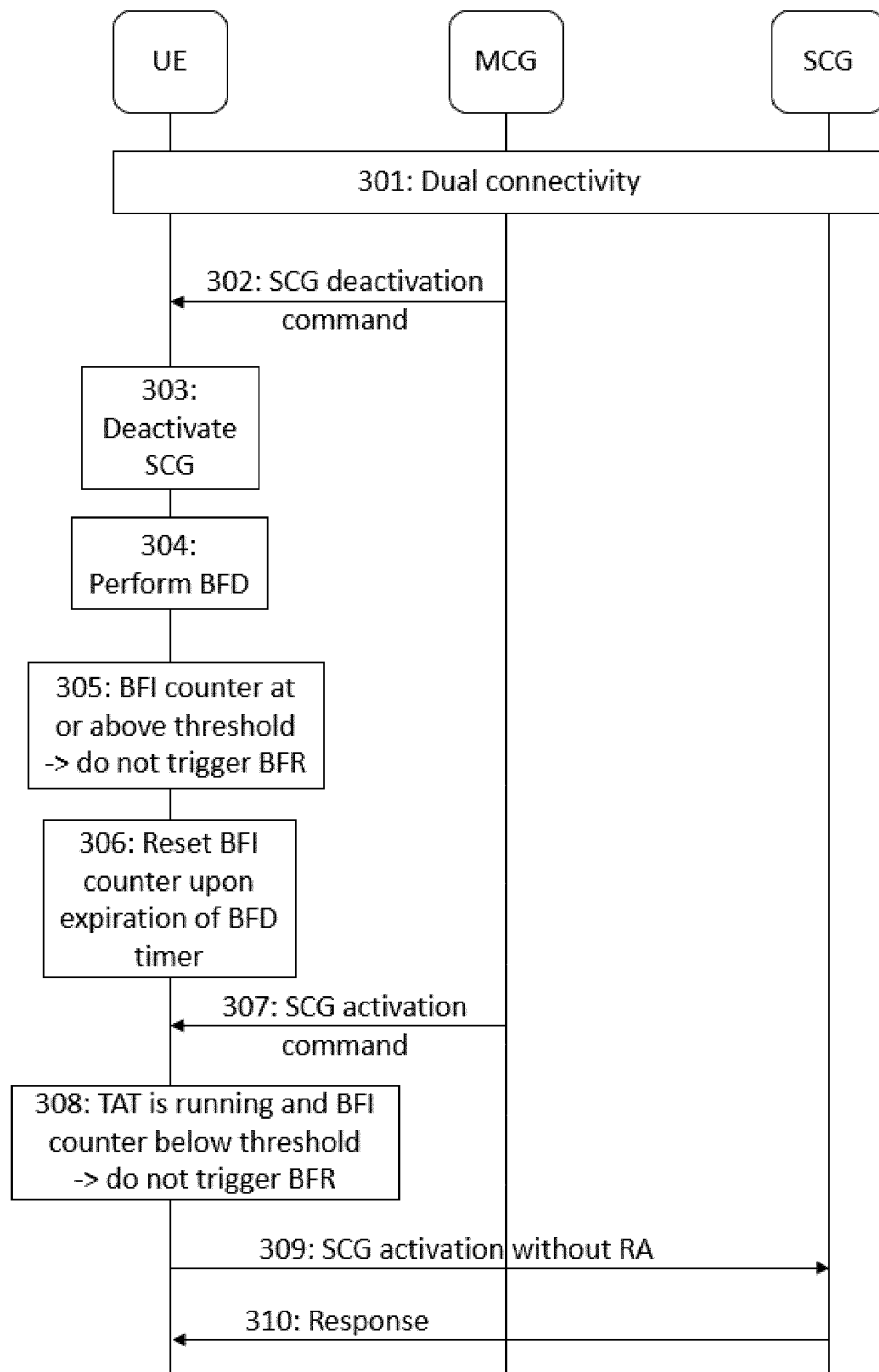


FIG. 3

4/8

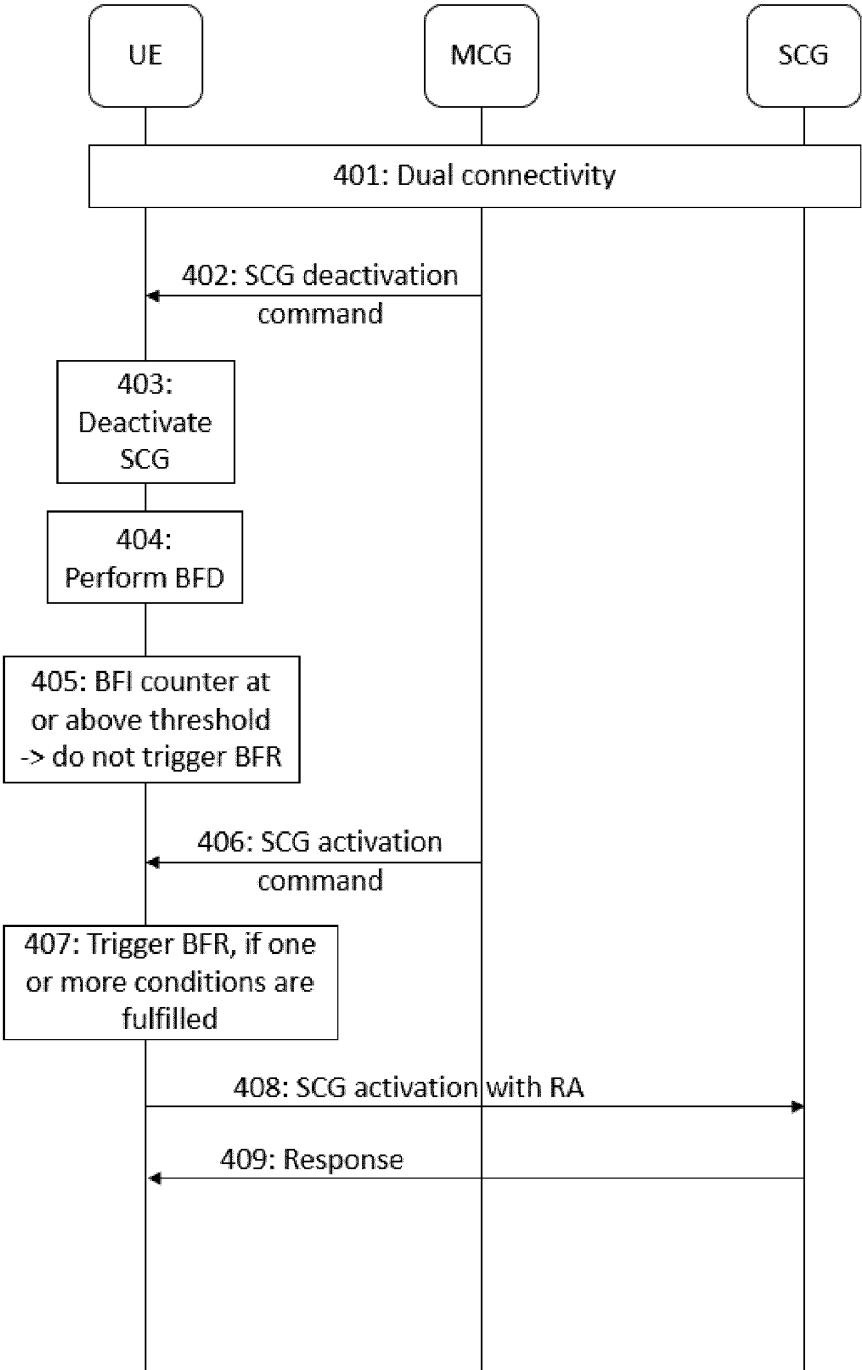


FIG. 4

5/8




FIG. 5

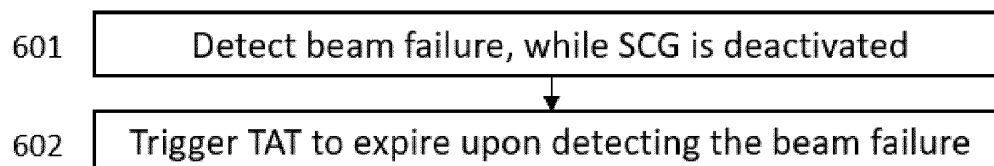


FIG. 6

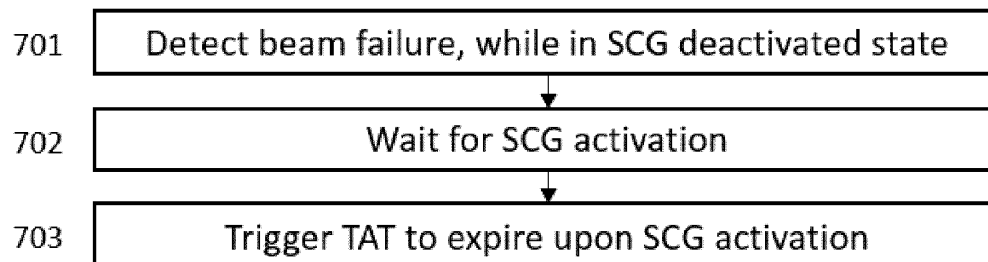


FIG. 7

6/8

801 Stop performing BFD when TAT expires

FIG. 8

901 Indicate detected beam failure on deactivated SCG via MCG

FIG. 9

1001 Transmit message indicative of configuration

FIG. 10

1101 Transmit first set of parameters for activated SCG



1102 Transmit second set of parameters for deactivated SCG

FIG. 11

7/8

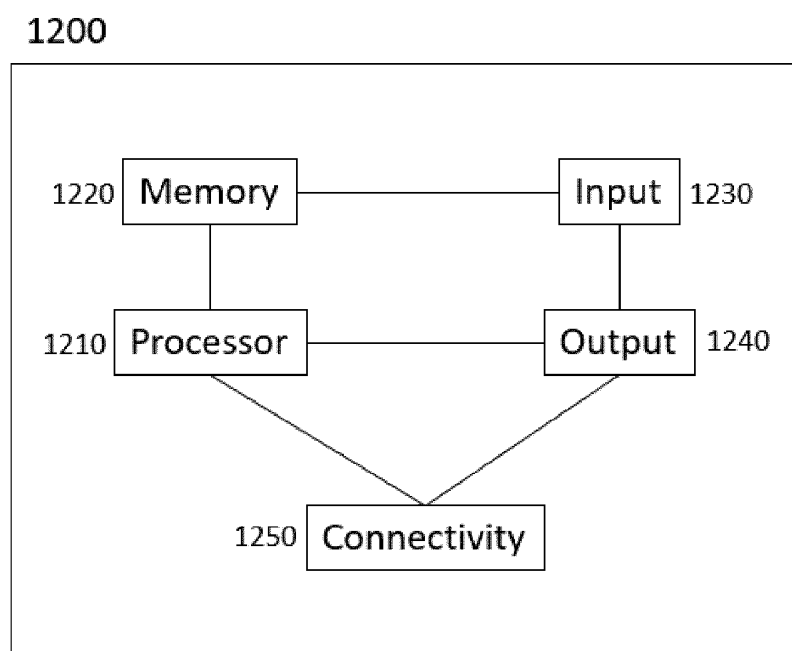


FIG. 12

8/8

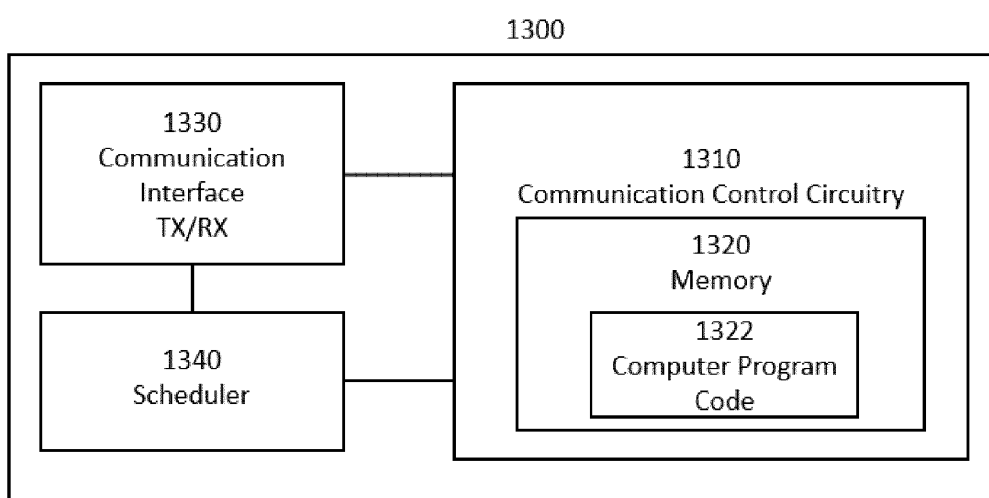


FIG. 13