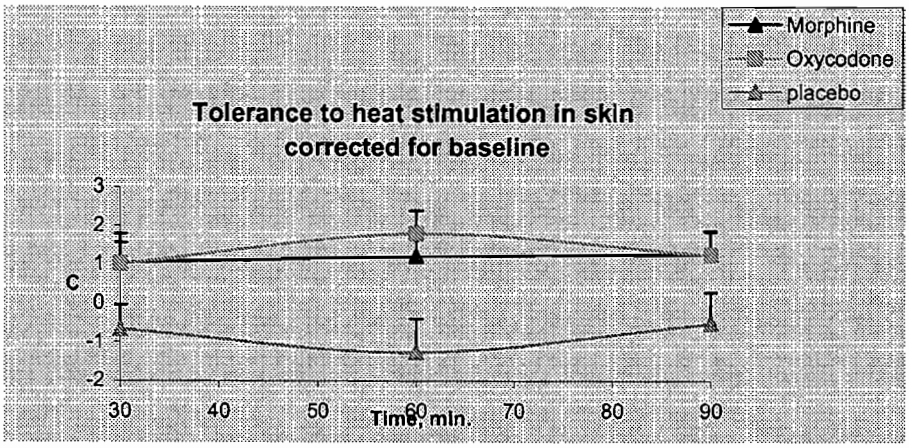
Figure 1


Morphine
Oxycodone
placebo
Tolerance to heat stimulation in skin
corrected for baseline
C
3
2
1
0
-1
-2
30
40
50
60
70
80
90
Time, min.

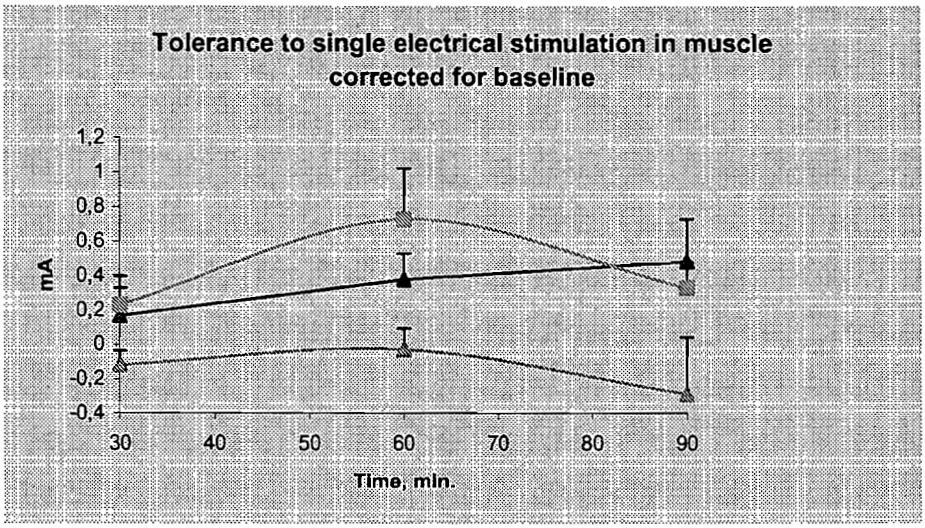
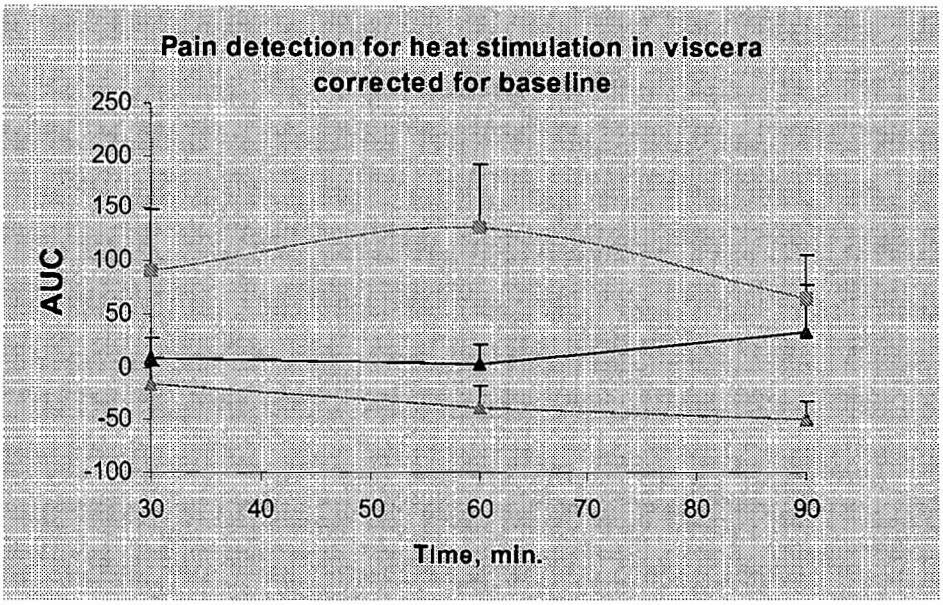
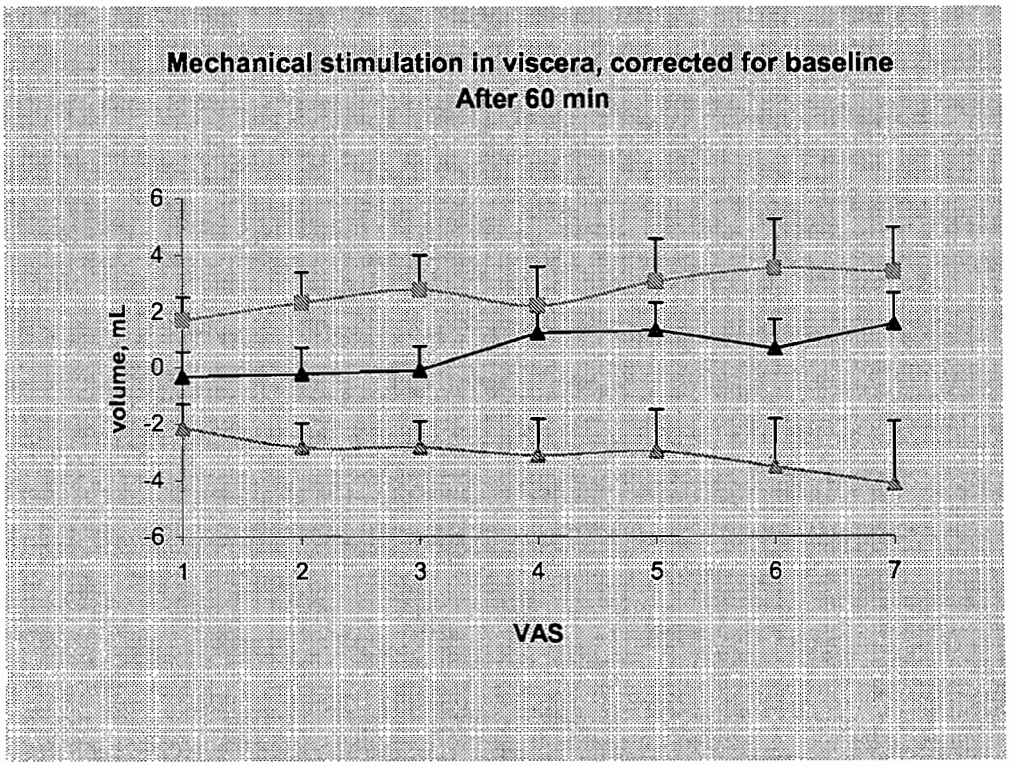

Tolerance to single electrical stimulation in muscle
corrected for baseline
mA
1,2
1
0,8
0,6
0,4
0,2
0
-0,2
-0,4
30
40
50
60
70
80
90
Time, min.

Figure 2


Pain detection for heat stimulation in viscera
corrected for baseline
AUC
250
200
150
100
50
0
-50
-100
30
40
50
60
70
80
90
Time, min.


Mechanical stimulation in viscera, corrected for baseline
After 60 min
volume, mL
6
4
2
0
-2
-4
-6
1
2
3
4
5
6
7
VAS