

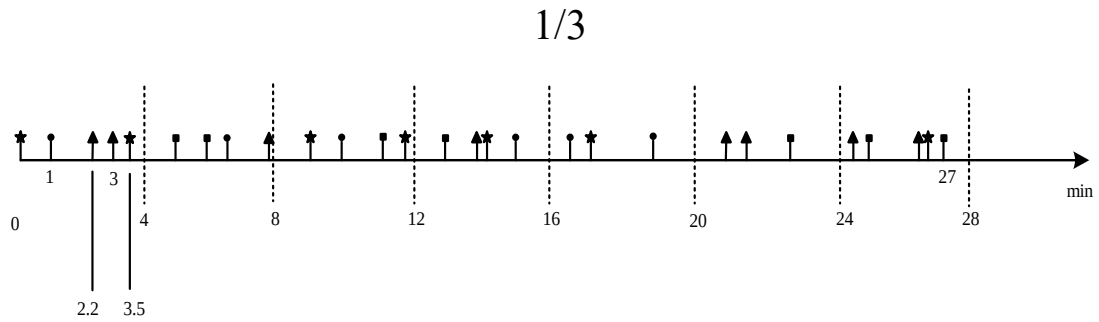


FIG. 1

Method 200

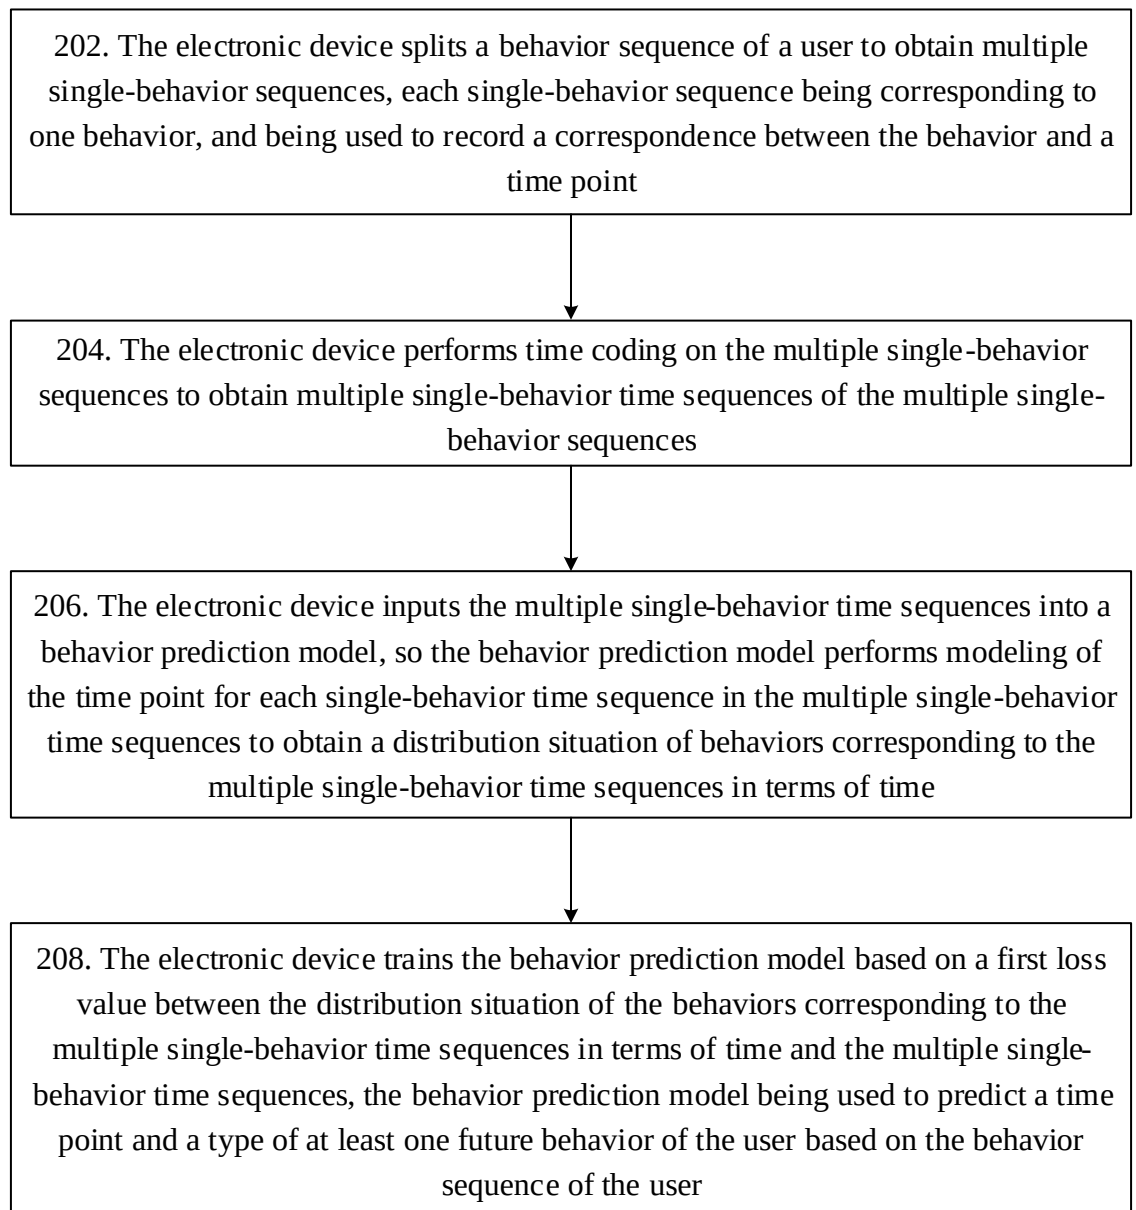


FIG. 2

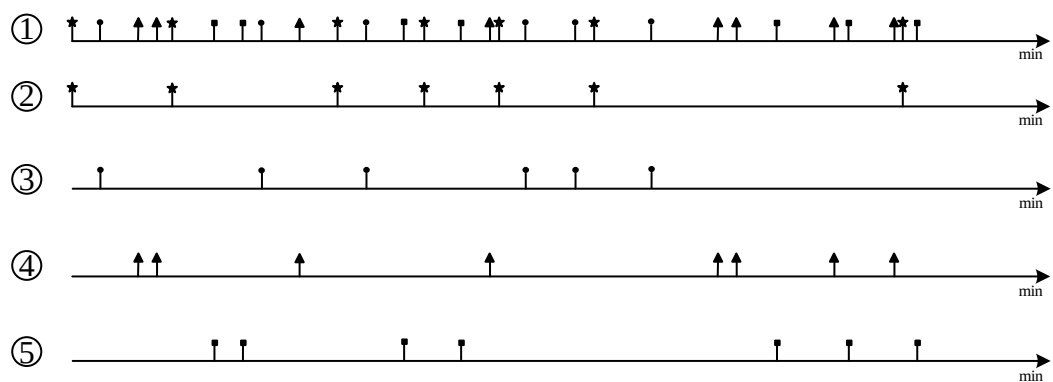


FIG. 3

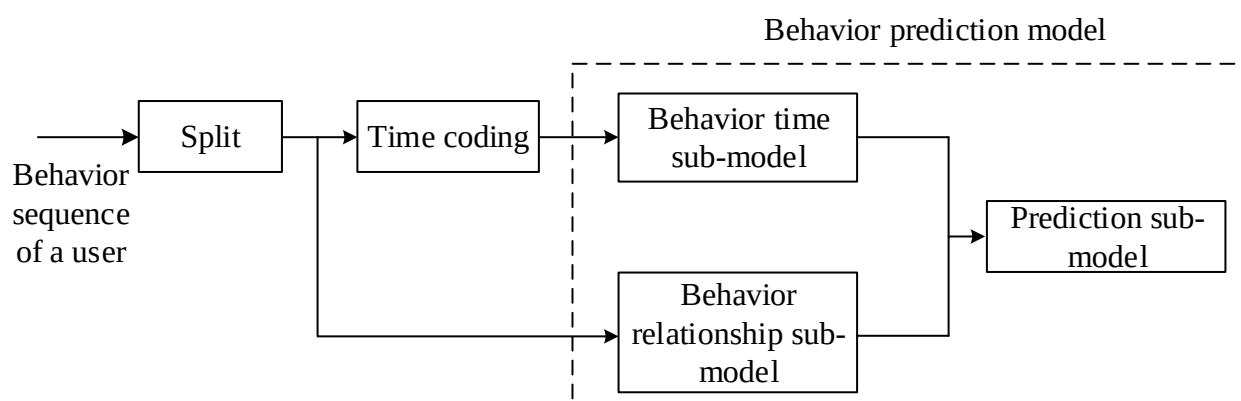


FIG. 4

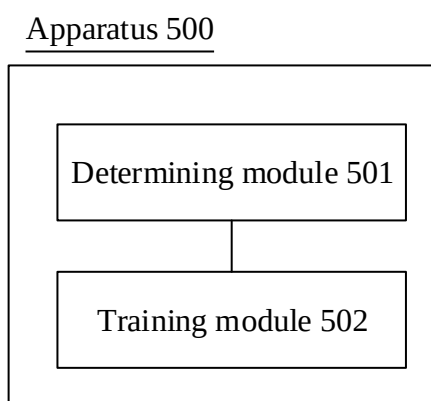


FIG. 5

Device 600

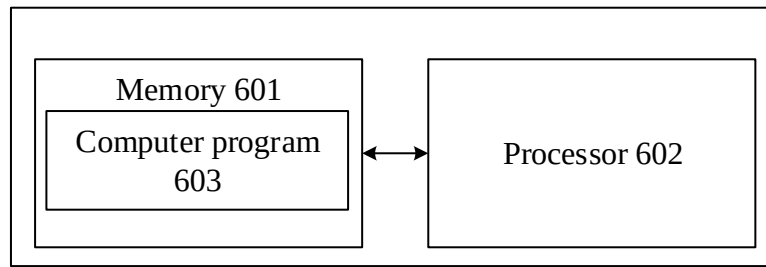


FIG. 6