

Figure 1

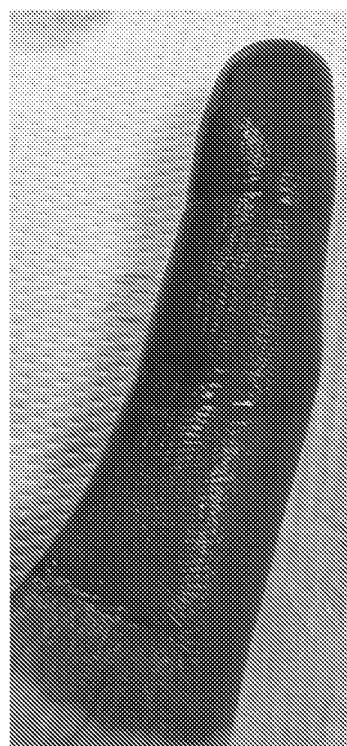


Figure 3


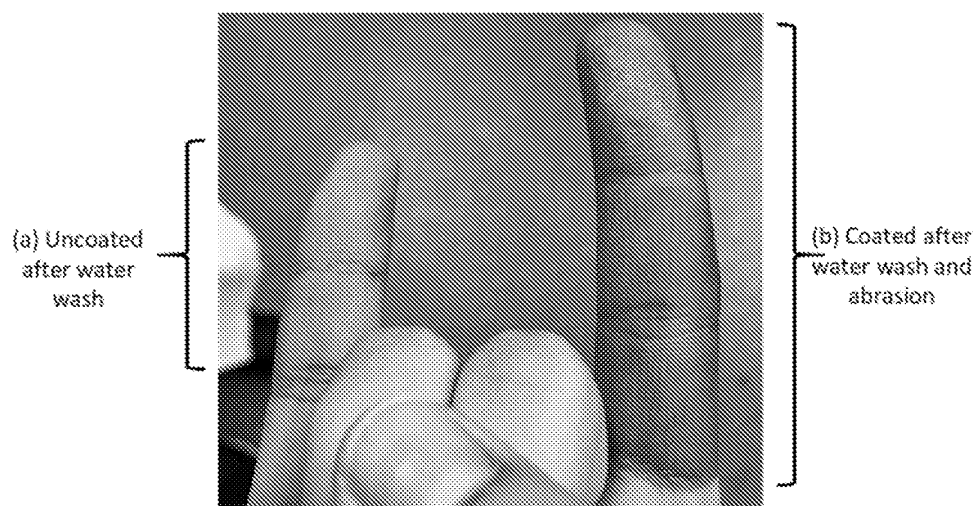


Figure 2



Coated after 18 hours with glove and
before washing

Figure 4

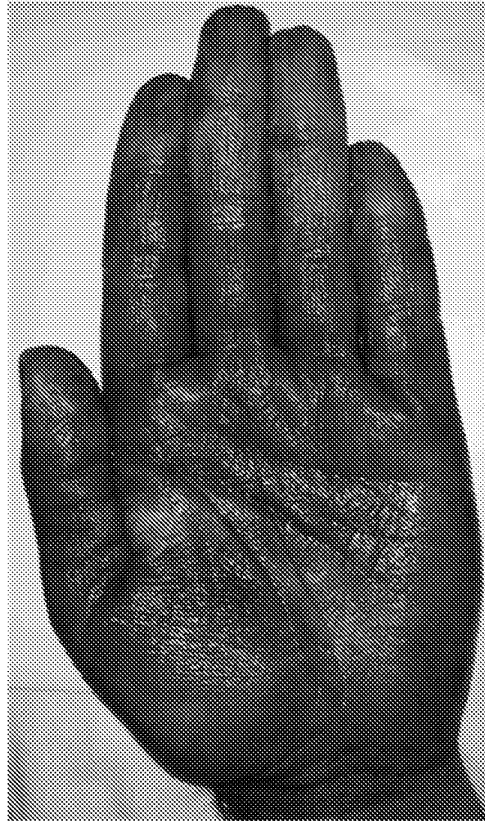

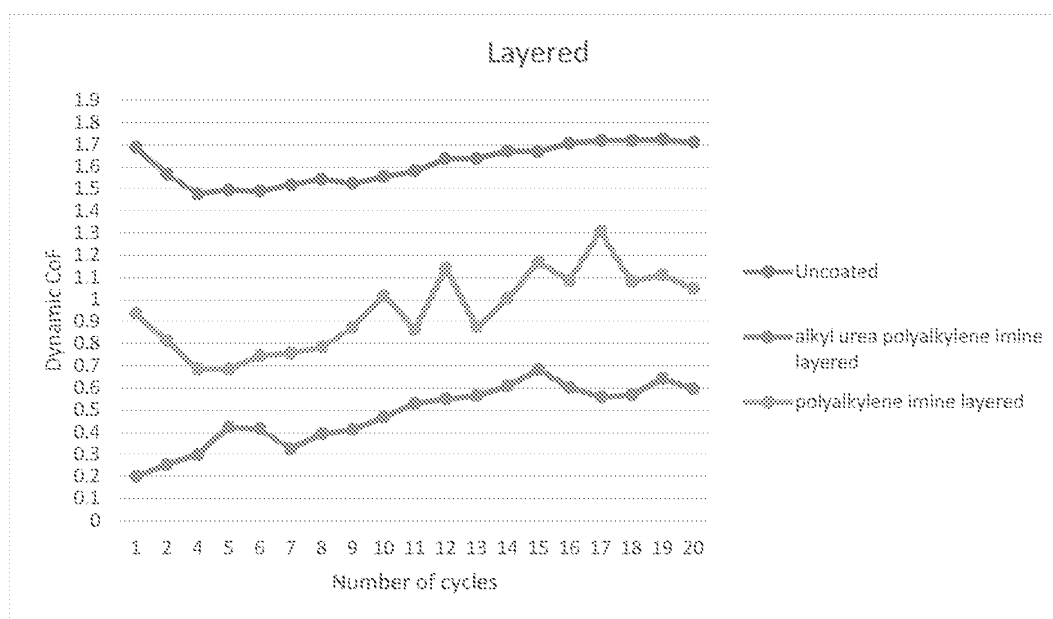
Coated with 18 hours in glove,
after washing and abrasion


Figure 5





Coated with 18 hours in glove, after washing
with soap and warm water

Figure 6

**Figure 7**

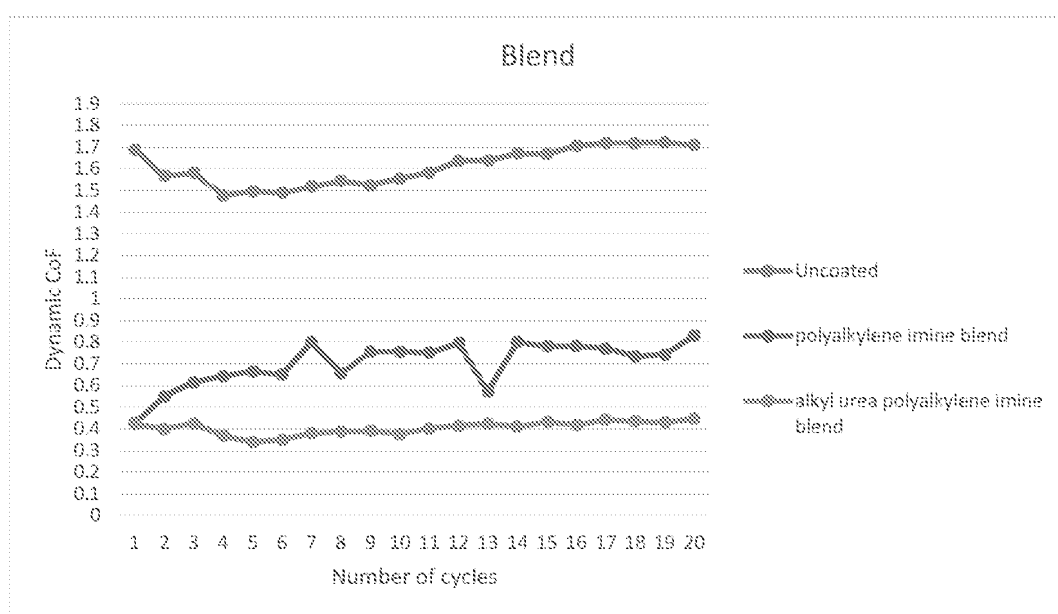**Figure 8**

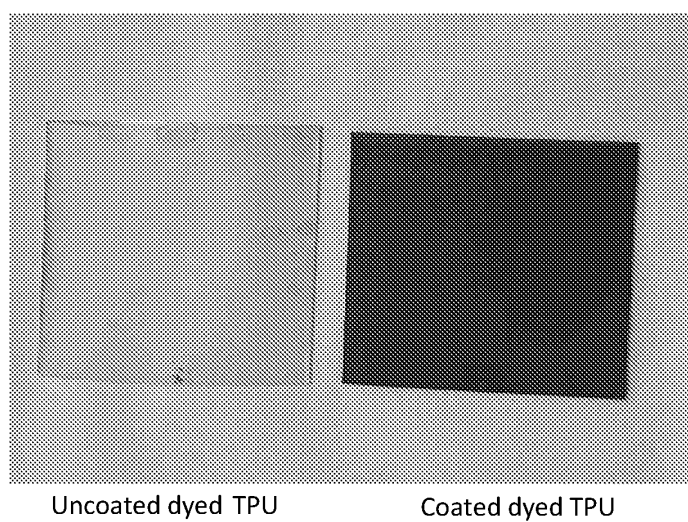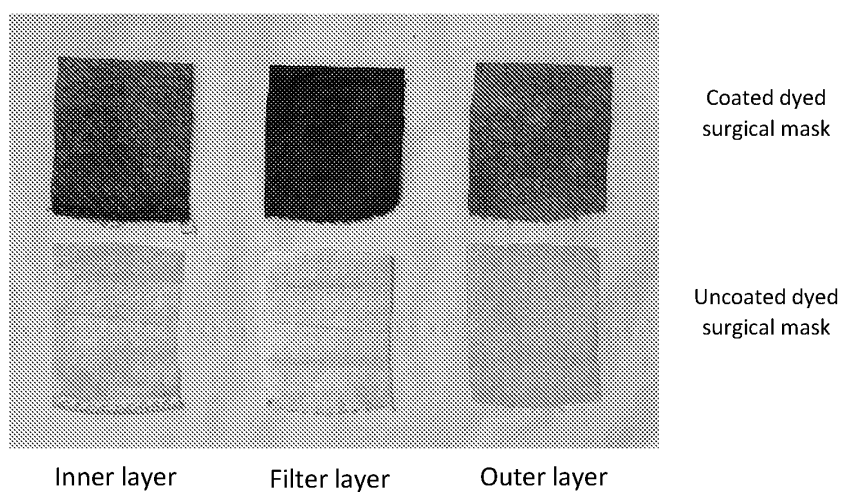**Figure 9(a)****Figure 9(b)**

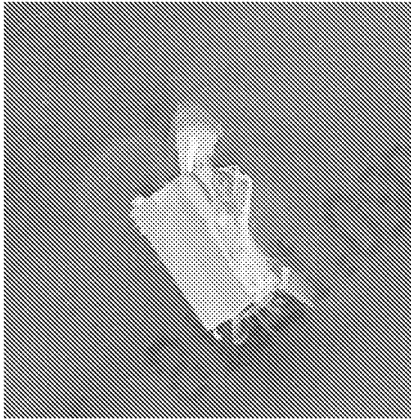


Figure 10(a) No zone of Inhibition from
TPU coated with D1 formulation

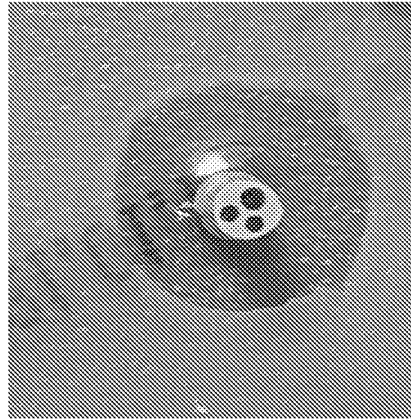


Figure 10(b) Positive control
catheter (chlorhexidine/silver)

Figure 10