



(43) International Publication Date
11 April 2013 (11.04.2013)

- (51) International Patent Classification:
A61M 1/28 (2006.01) *G06F 19/00* (2011.01)
- (21) International Application Number:
PCT/MY2012/000260
- (22) International Filing Date:
2 October 2012 (02.10.2012)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
PI2011004753 4 October 2011 (04.10.2011) MY
- (72) Inventor; and
- (71) Applicant : **LOW, Chin Guan** [MY/MY]; 41, Jalan Langgak Tunku, Bukit Tunku, 50480 Kuala Lumpur (MY).
- (74) Agents: **BOEY, Weng Choong** et al.; Henry Goh & Co. Sdn. Bhd., 217 Jalan Imbi, 55100, Kuala Lumpur (MY).
- (81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP,

KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

- (84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).


Declarations under Rule 4.17:

— of inventorship (Rule 4.17(iv))

Published:

- with international search report (Art. 21(3))
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

(54) Title: PERITONEAL DIALYSIS MACHINE

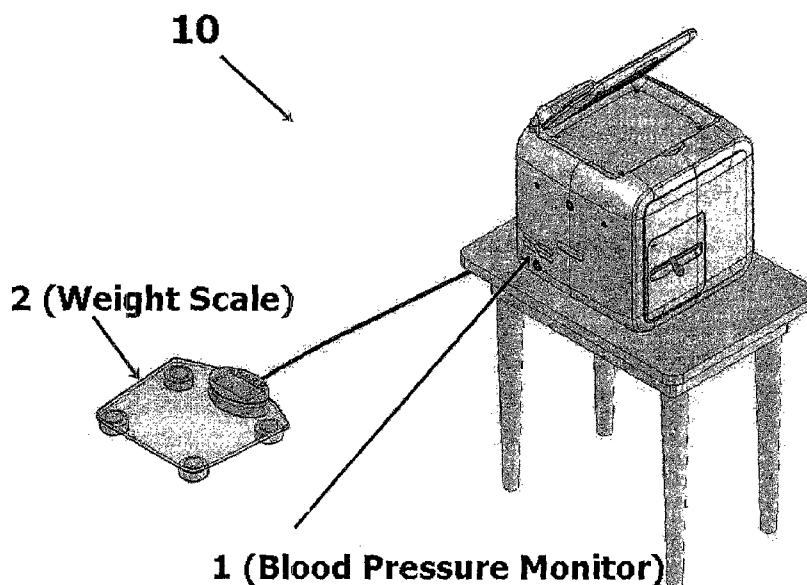

(57) Abstract: A peritoneal dialysis (PD) machine (10) comprising a blood pressure monitor (1) and a weight scale (2) which are powered by the dialysis machine. The peritoneal dialysis machine records and stores the measurements in the machine of a patient's blood pressure and weight that are taken using the blood pressure monitor and scale. The frequency with which such measurements are recorded is also monitored by the PD machine. If the frequency of recording the measurements does not comply with a predetermined schedule, a local and/or remote alert is generated.