

FIG. 1A

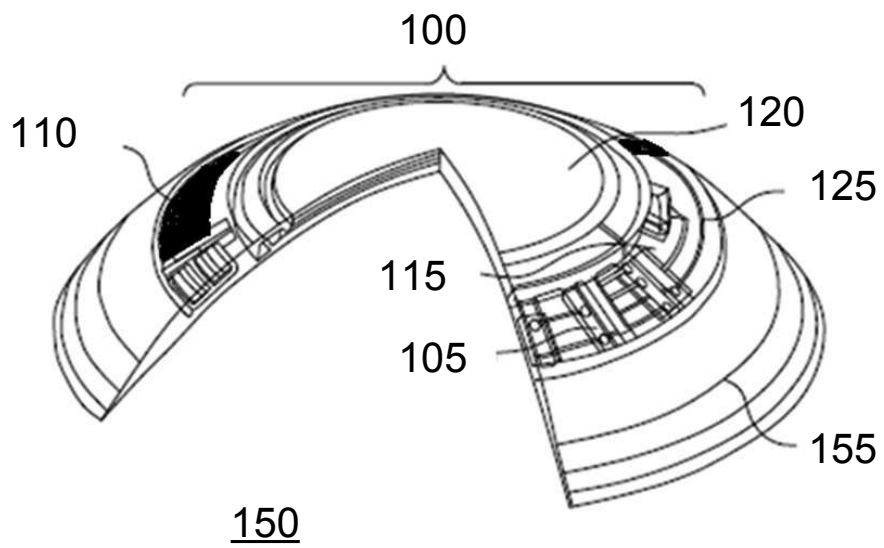
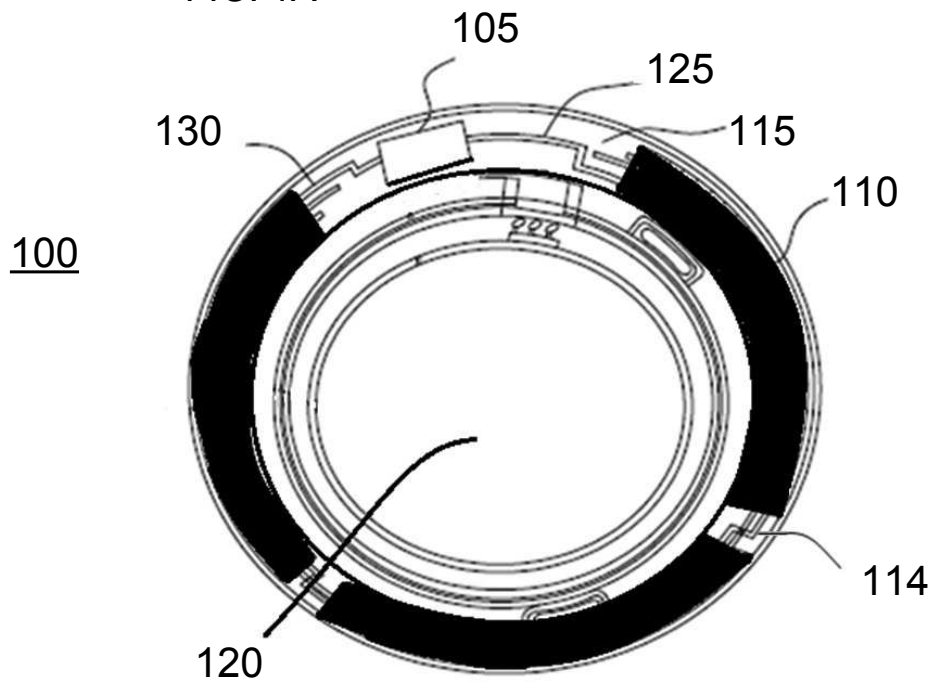


FIG. 1B

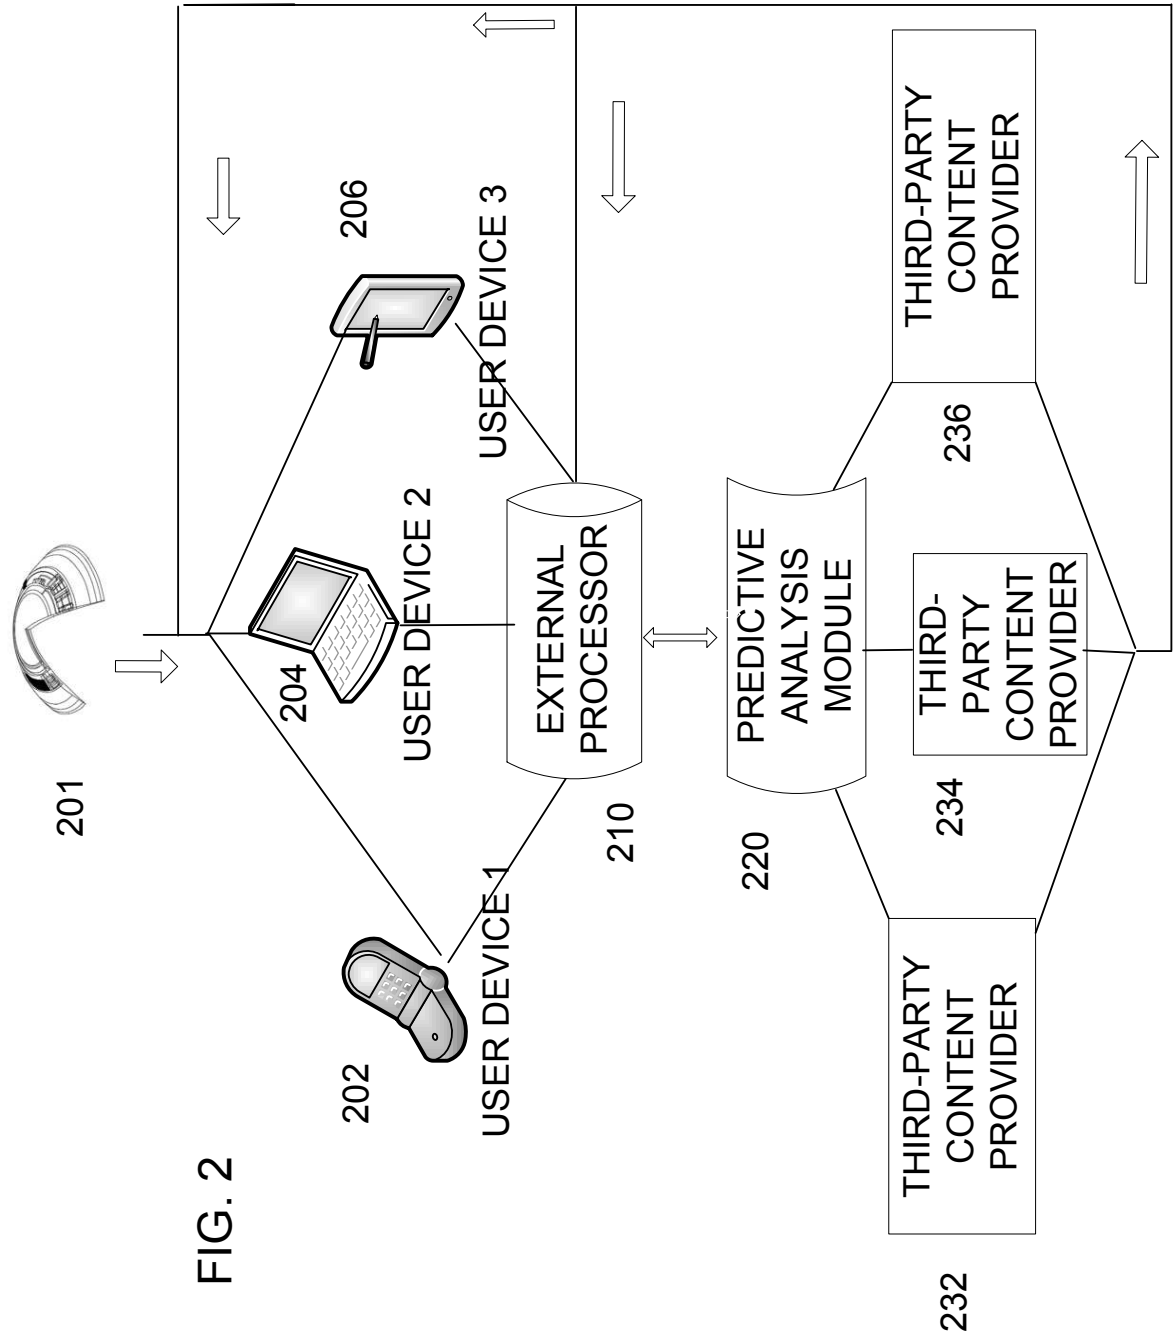


FIG. 3

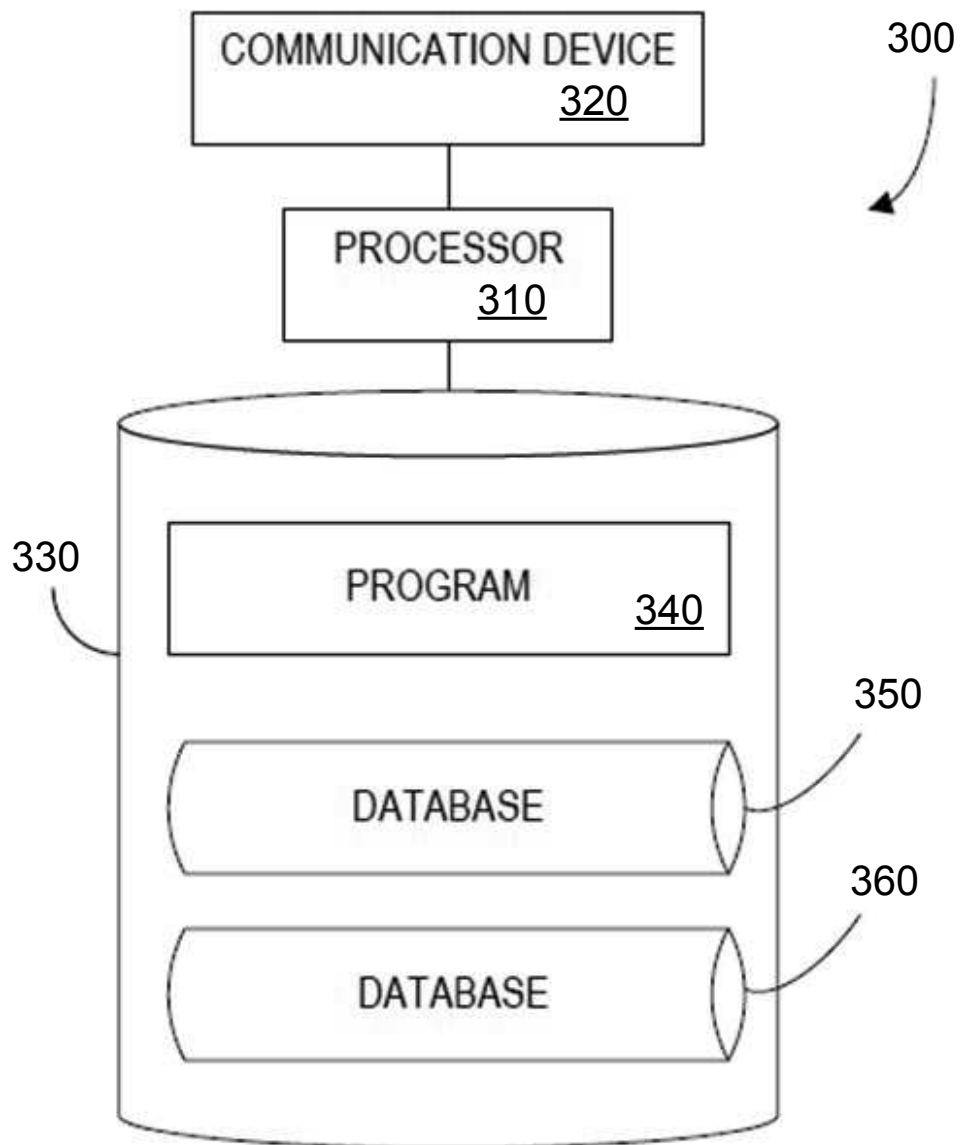


FIG. 4

410

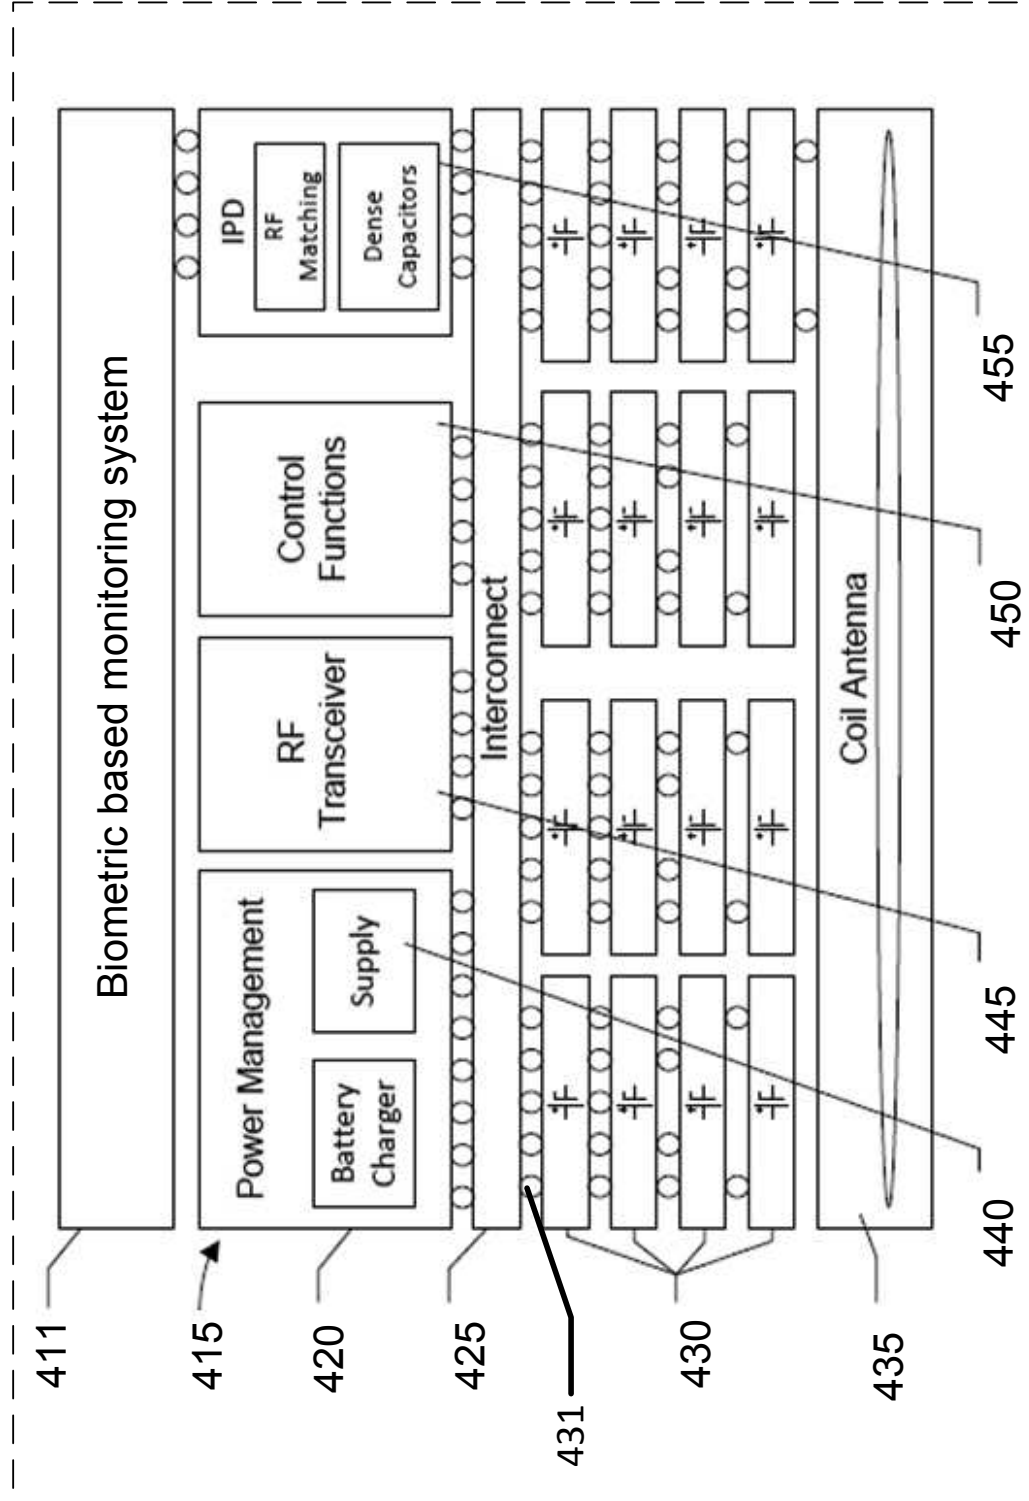


FIG. 5

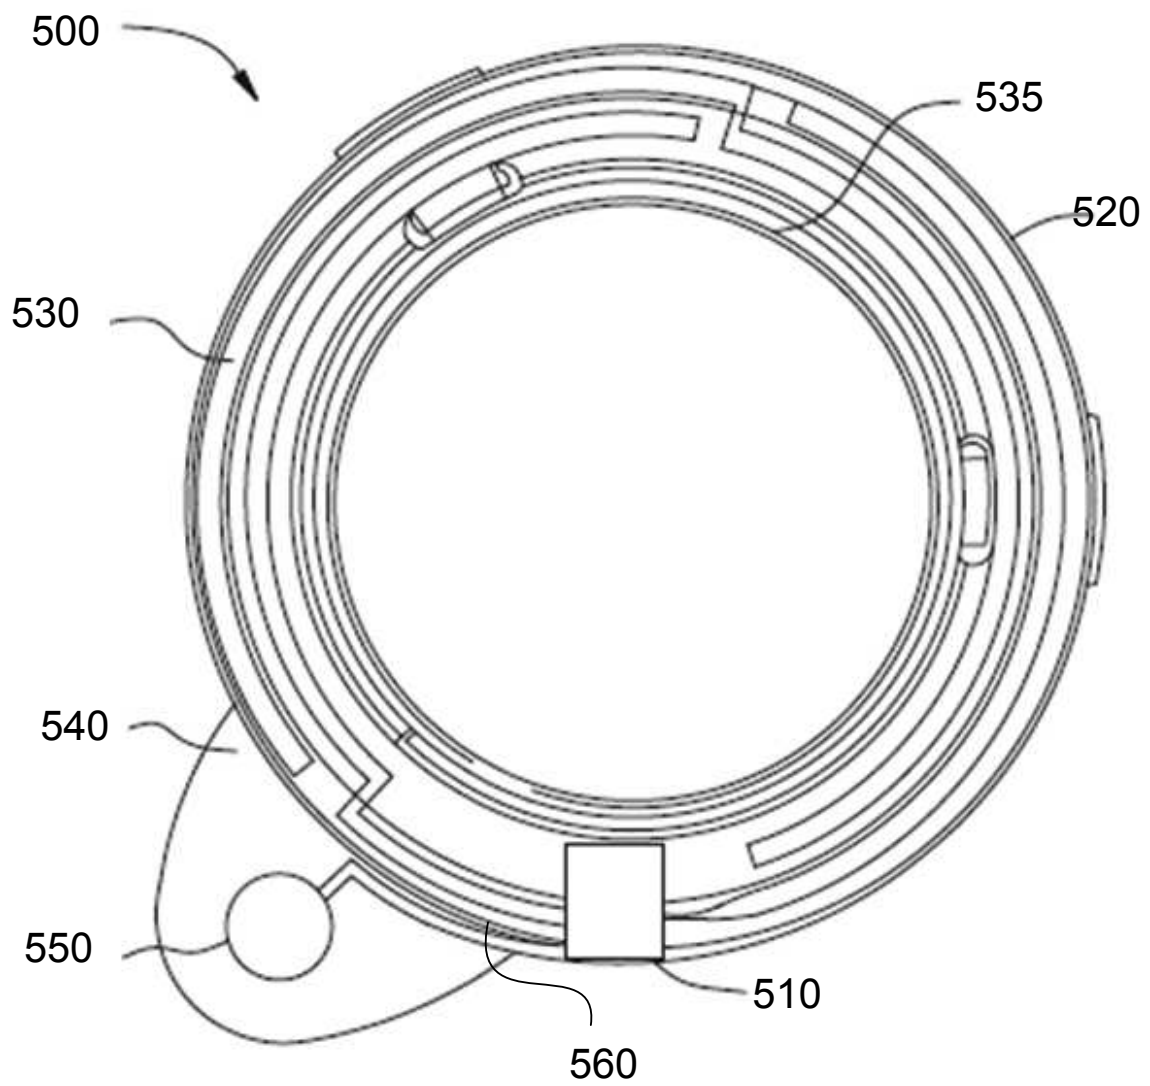


FIG. 6A

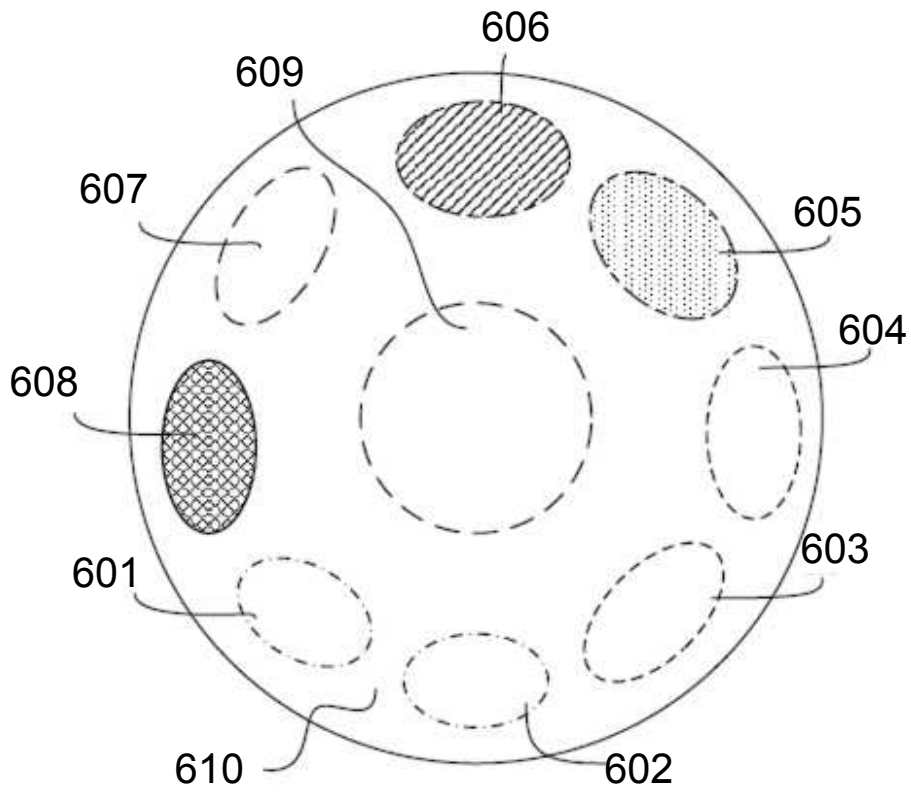


FIG. 6B

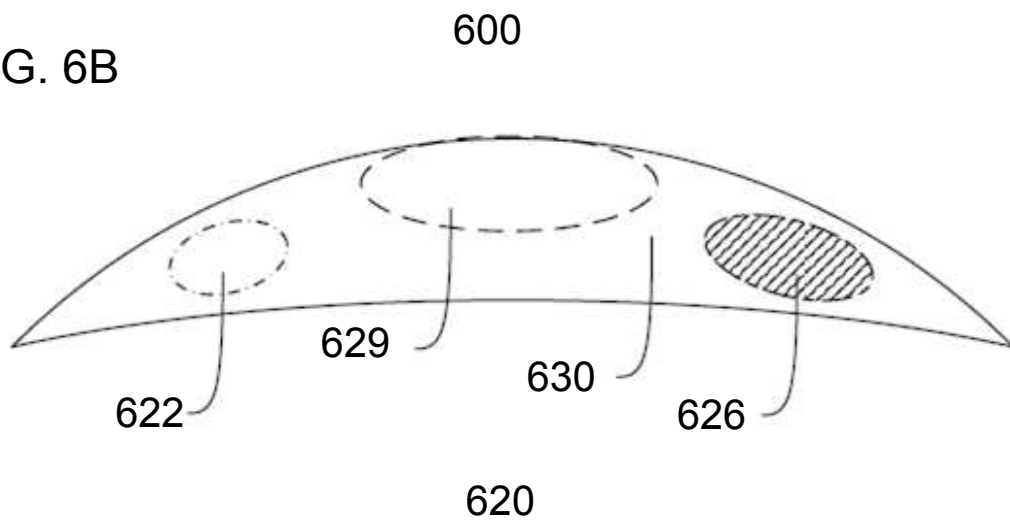


Fig. 7A

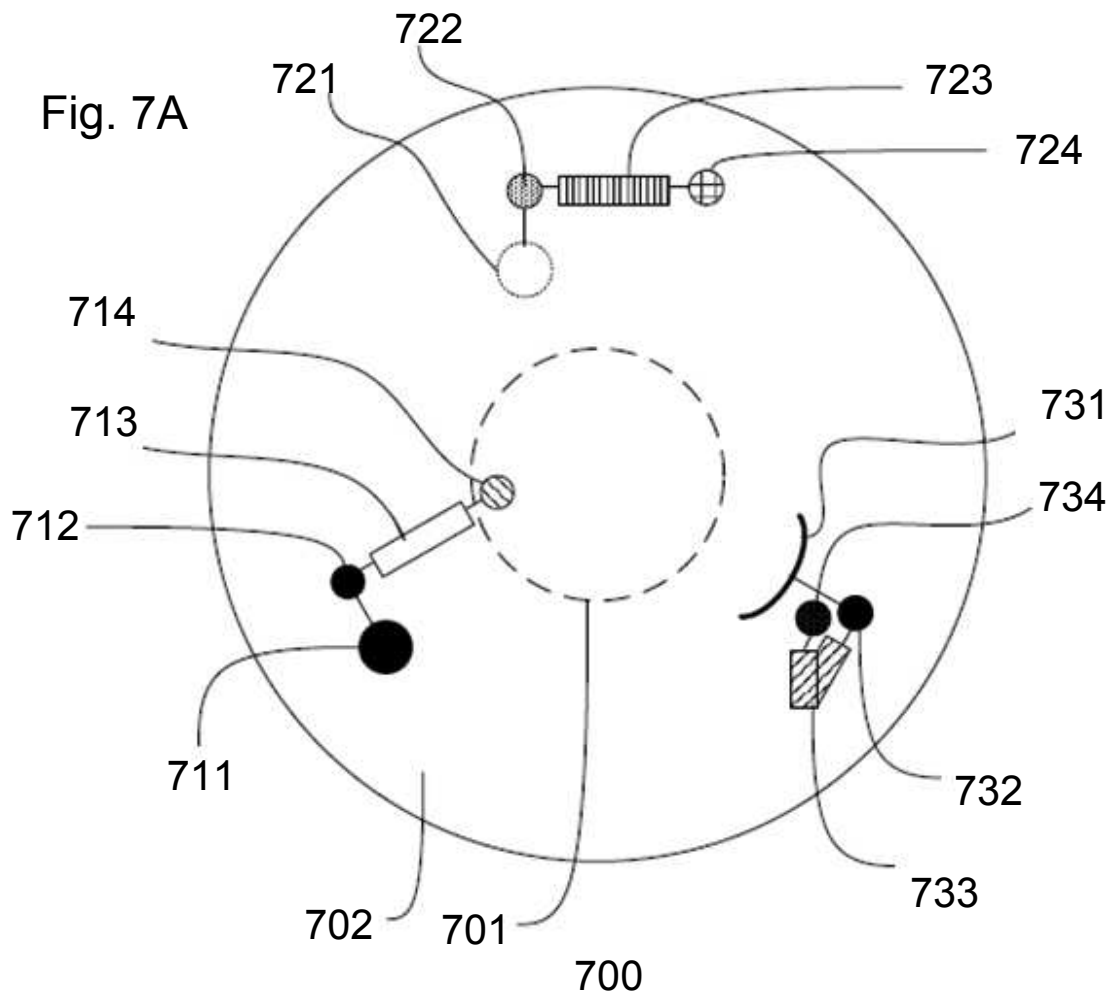


Fig. 7B

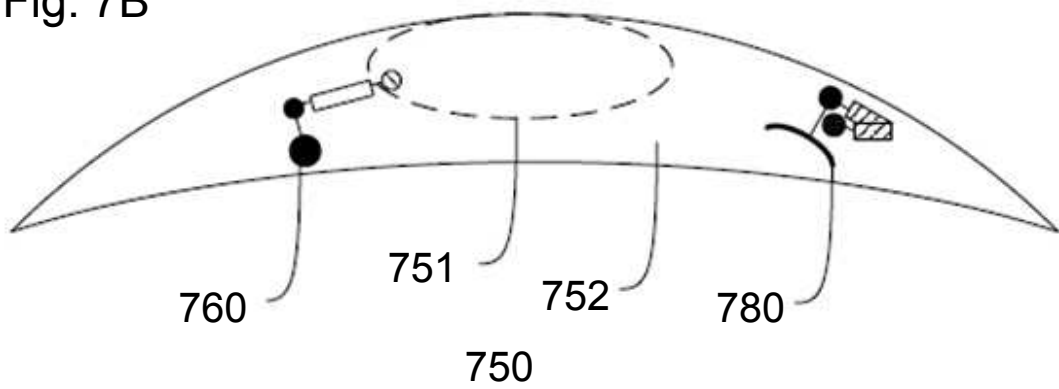
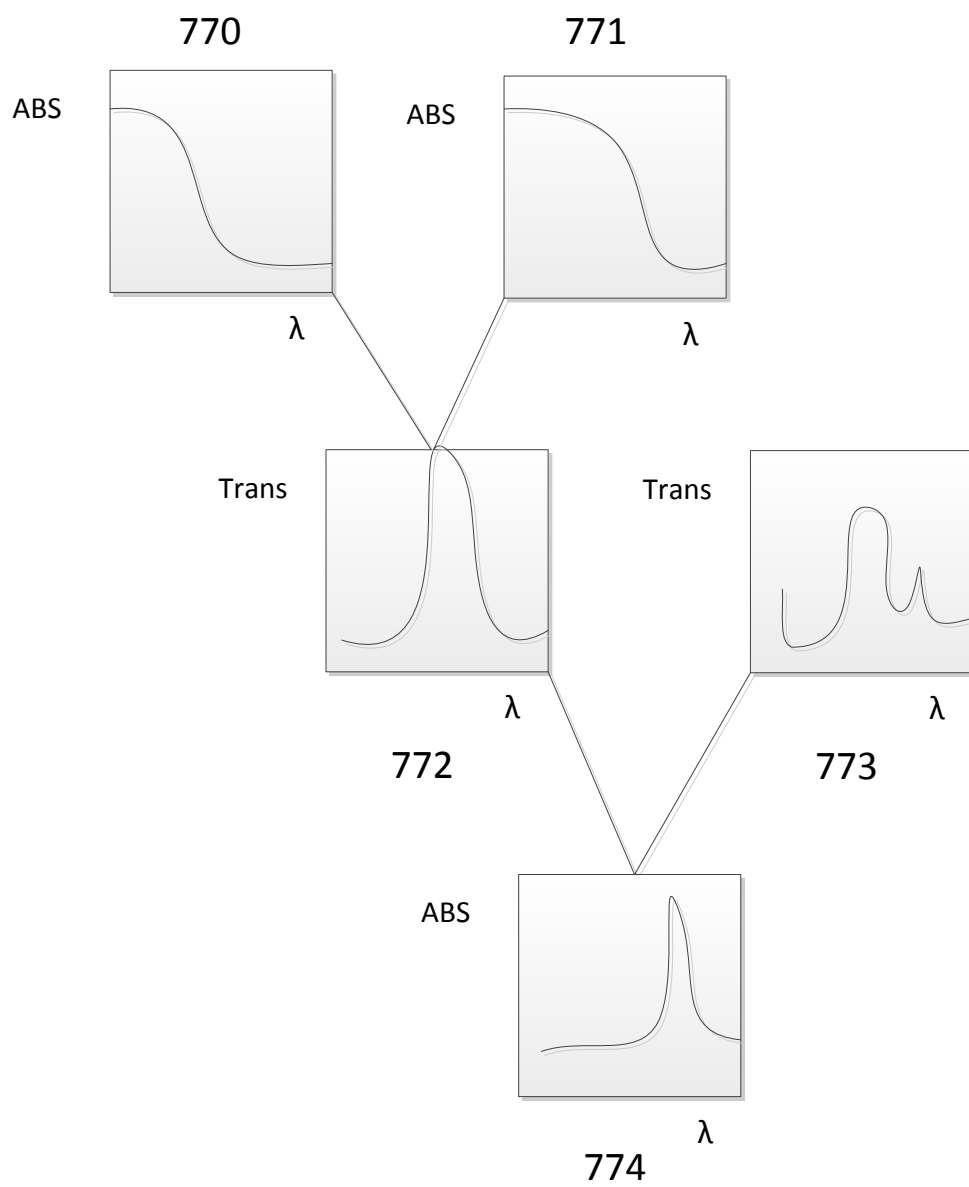


Fig. 7C



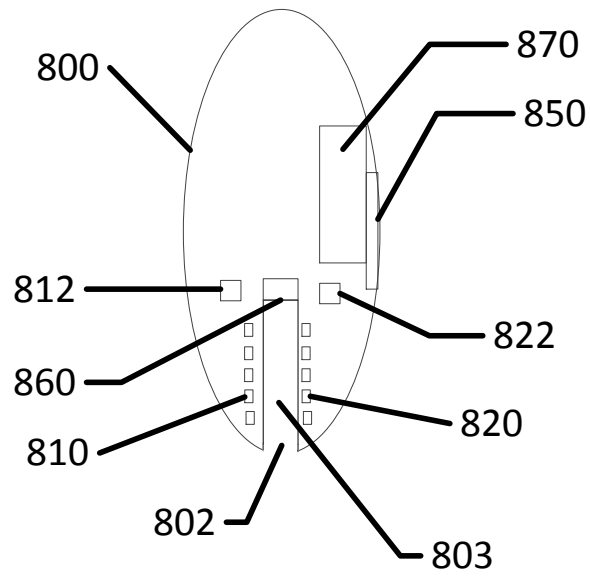


FIG. 8A

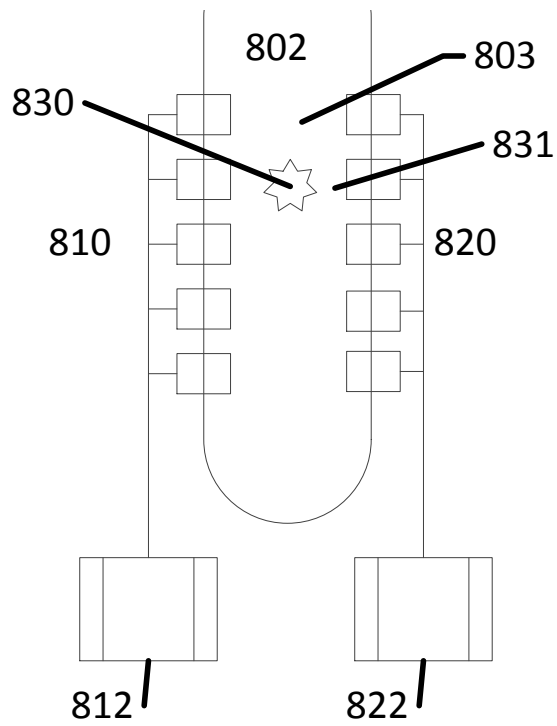


FIG. 8B

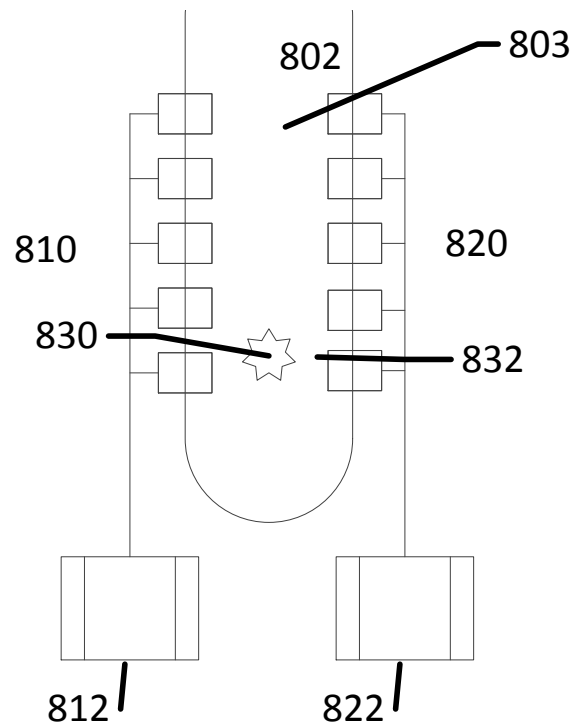


FIG. 8C

FIG. 9A

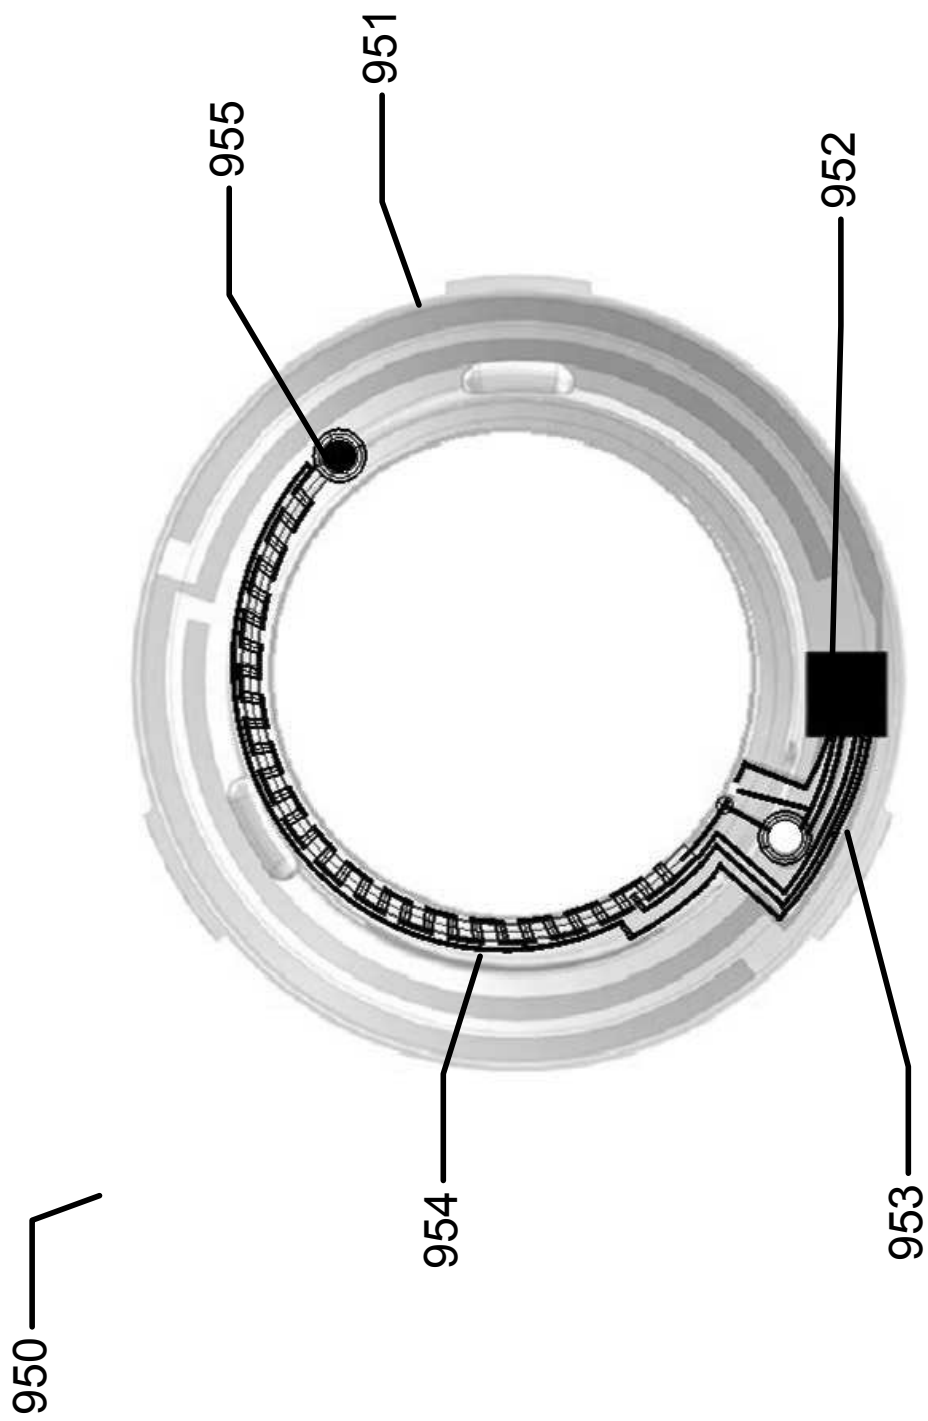
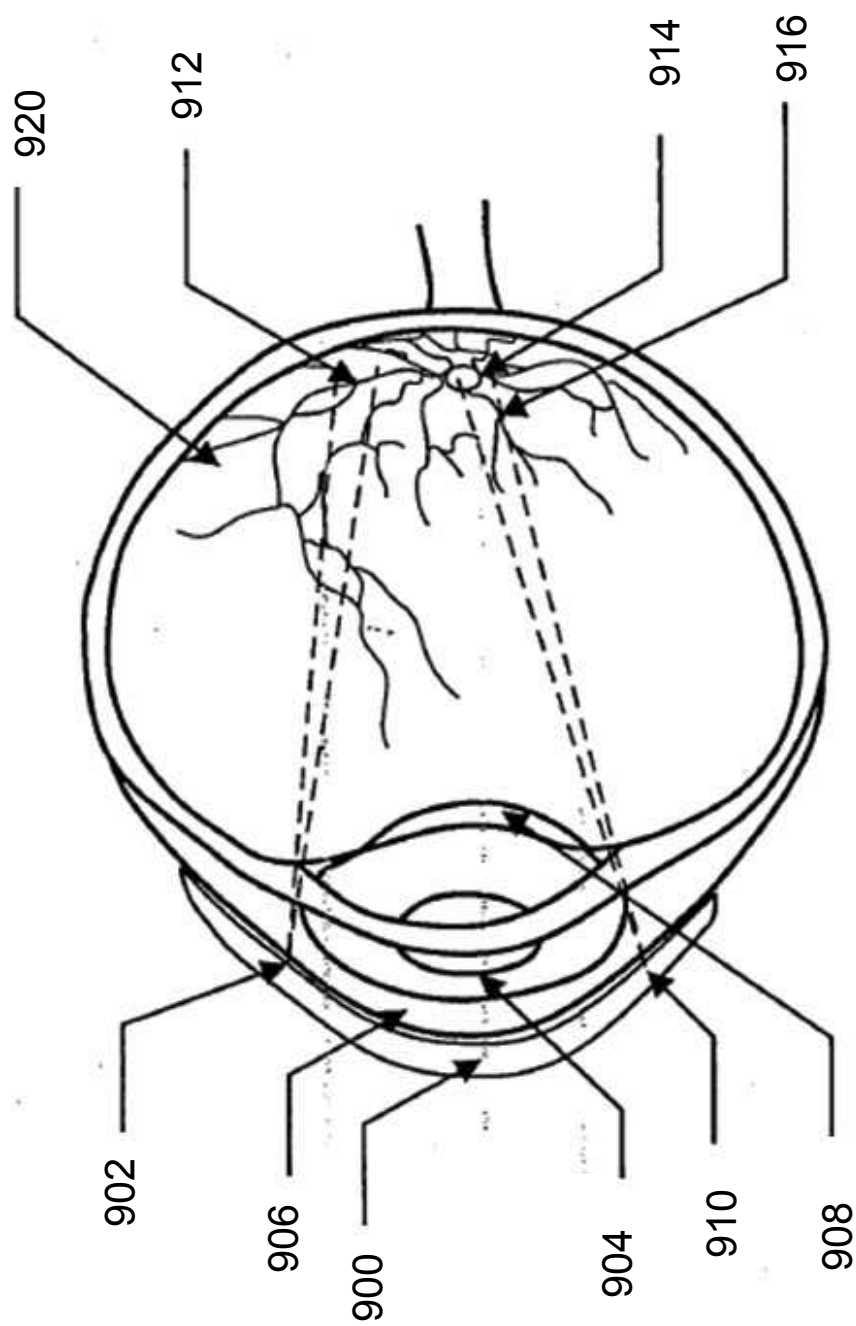
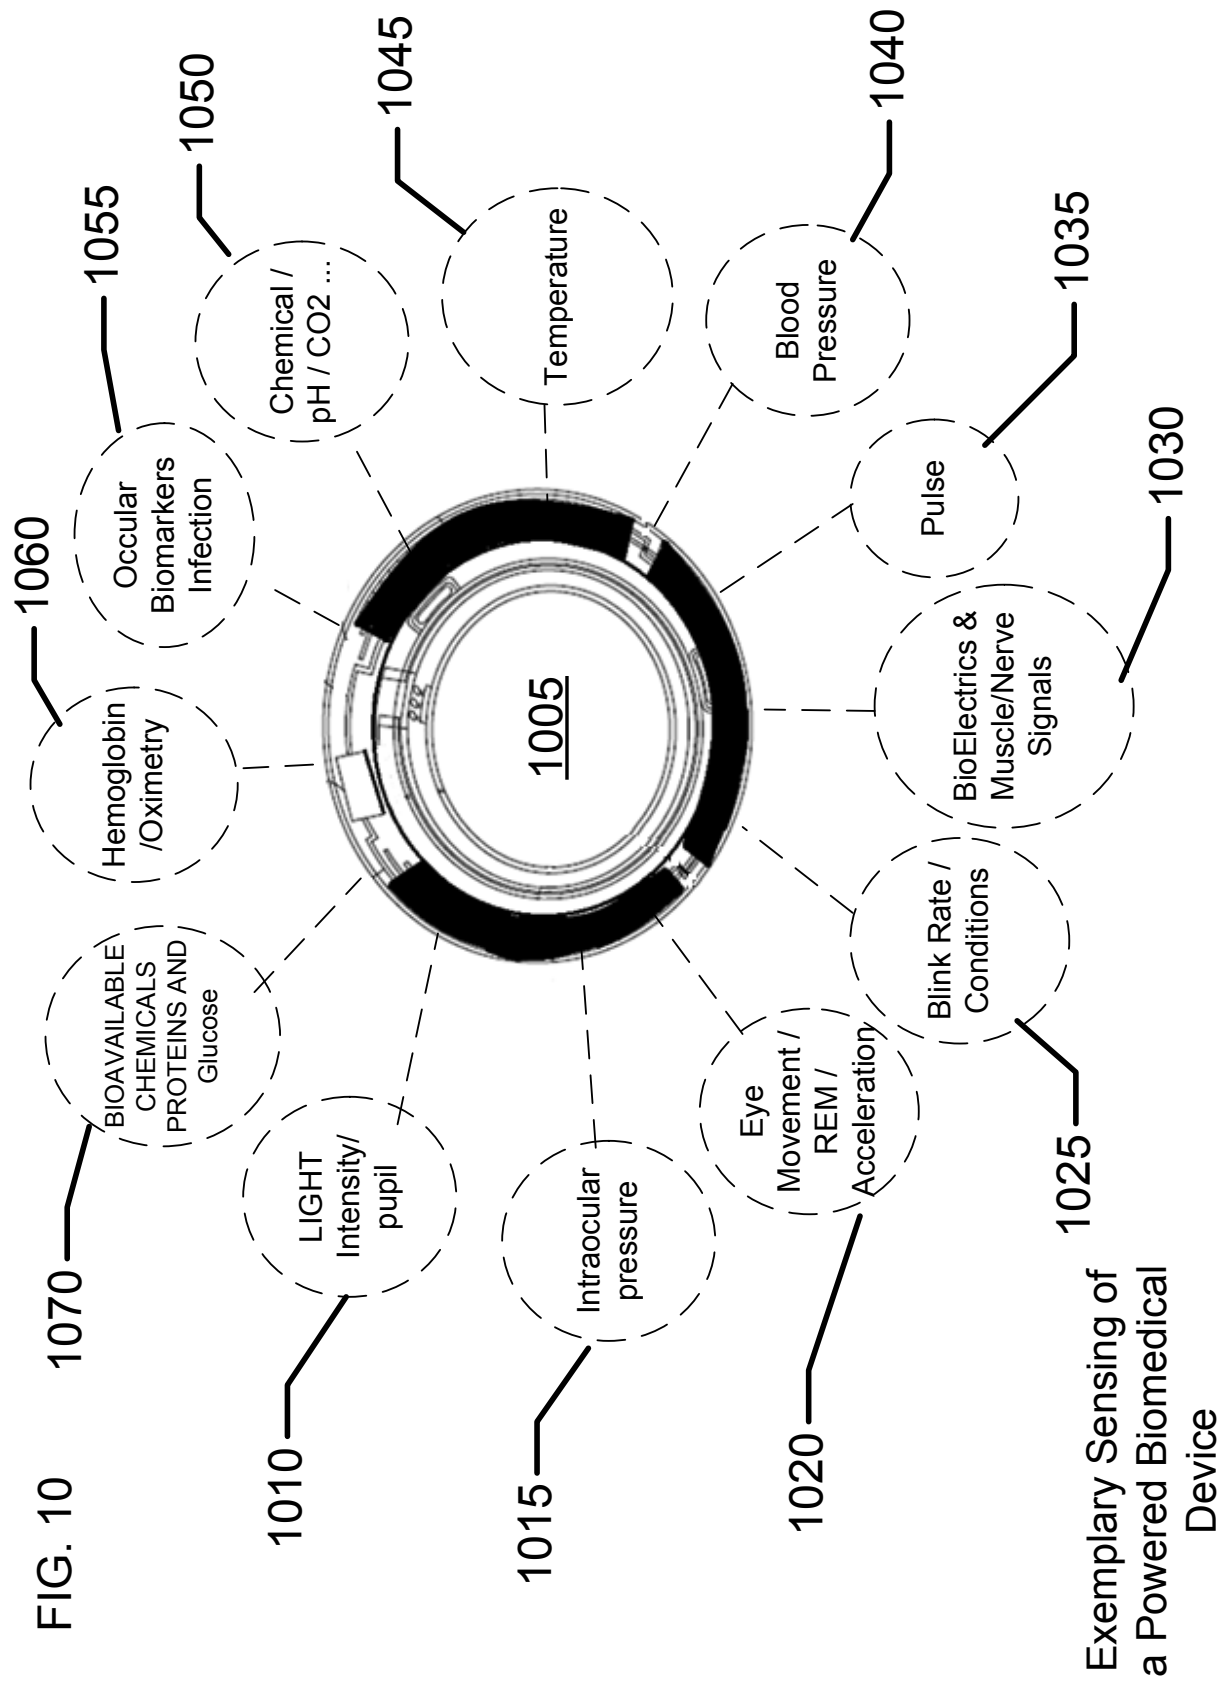


FIG. 9B





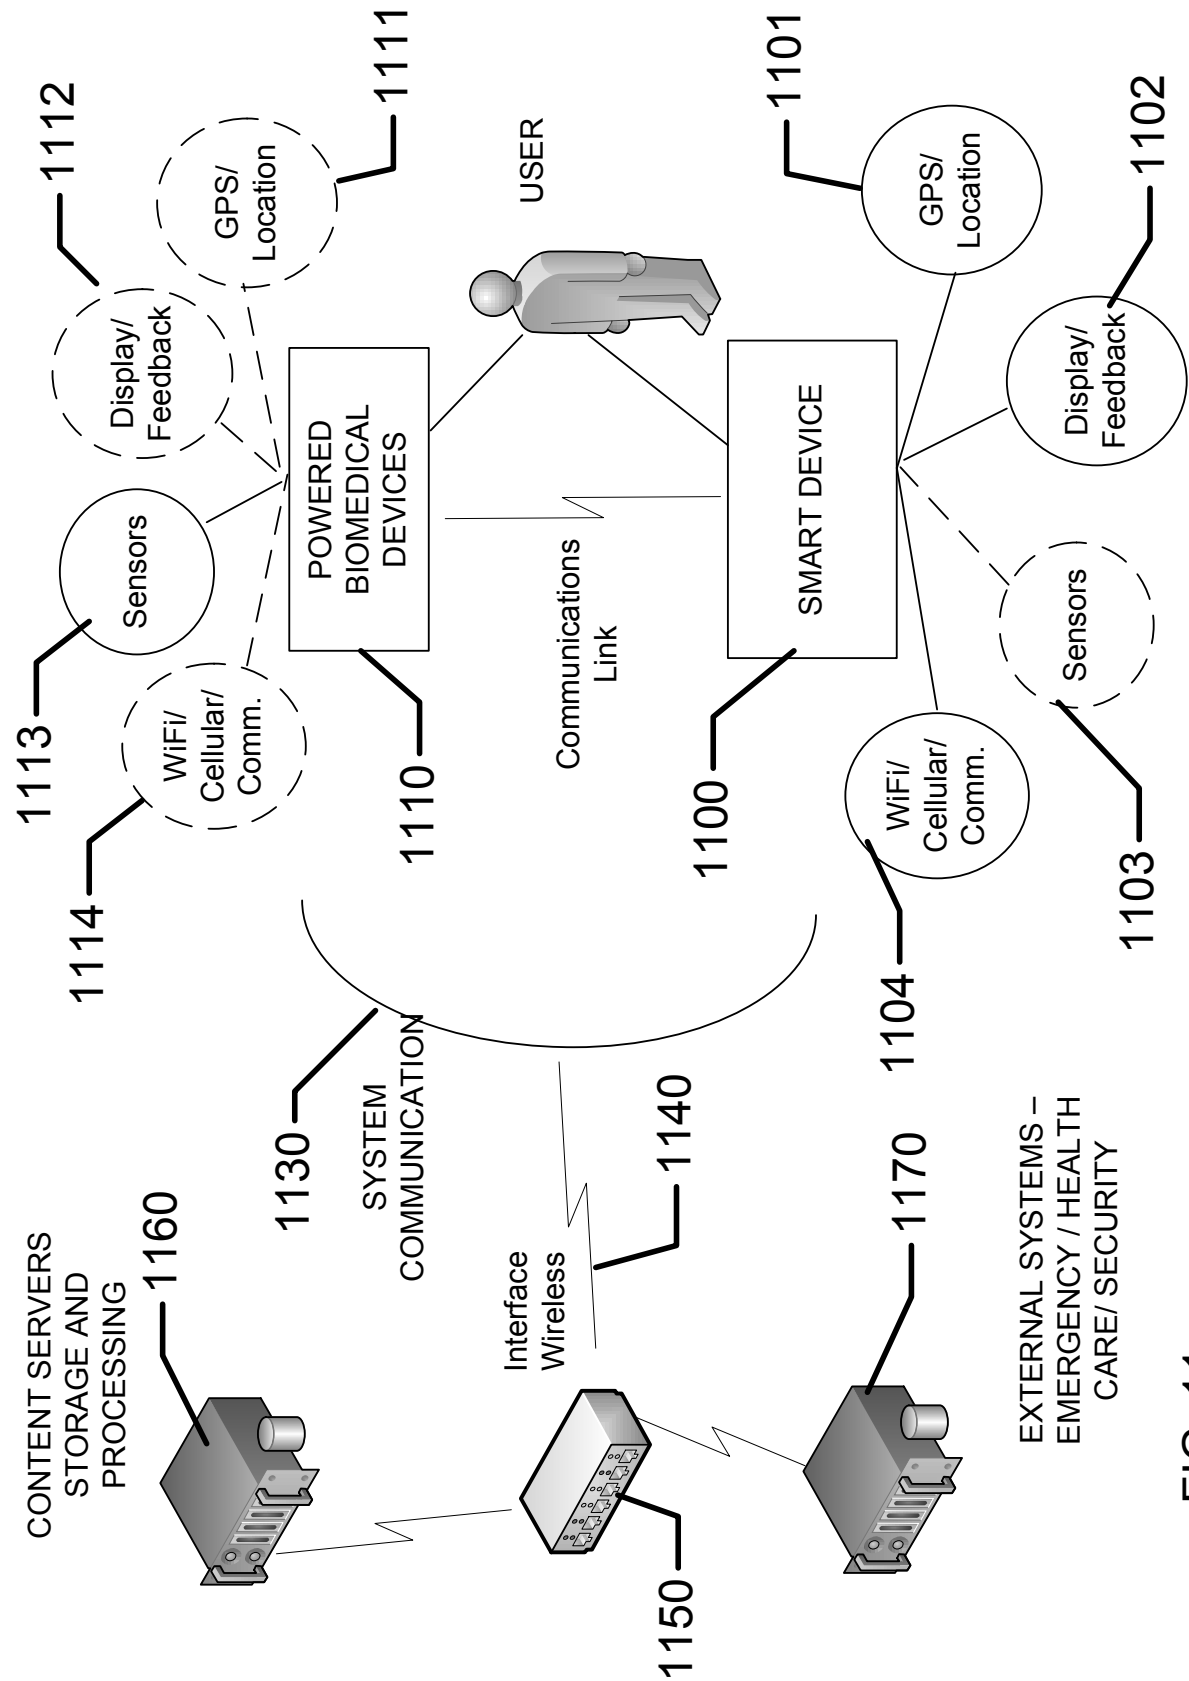


FIG. 11

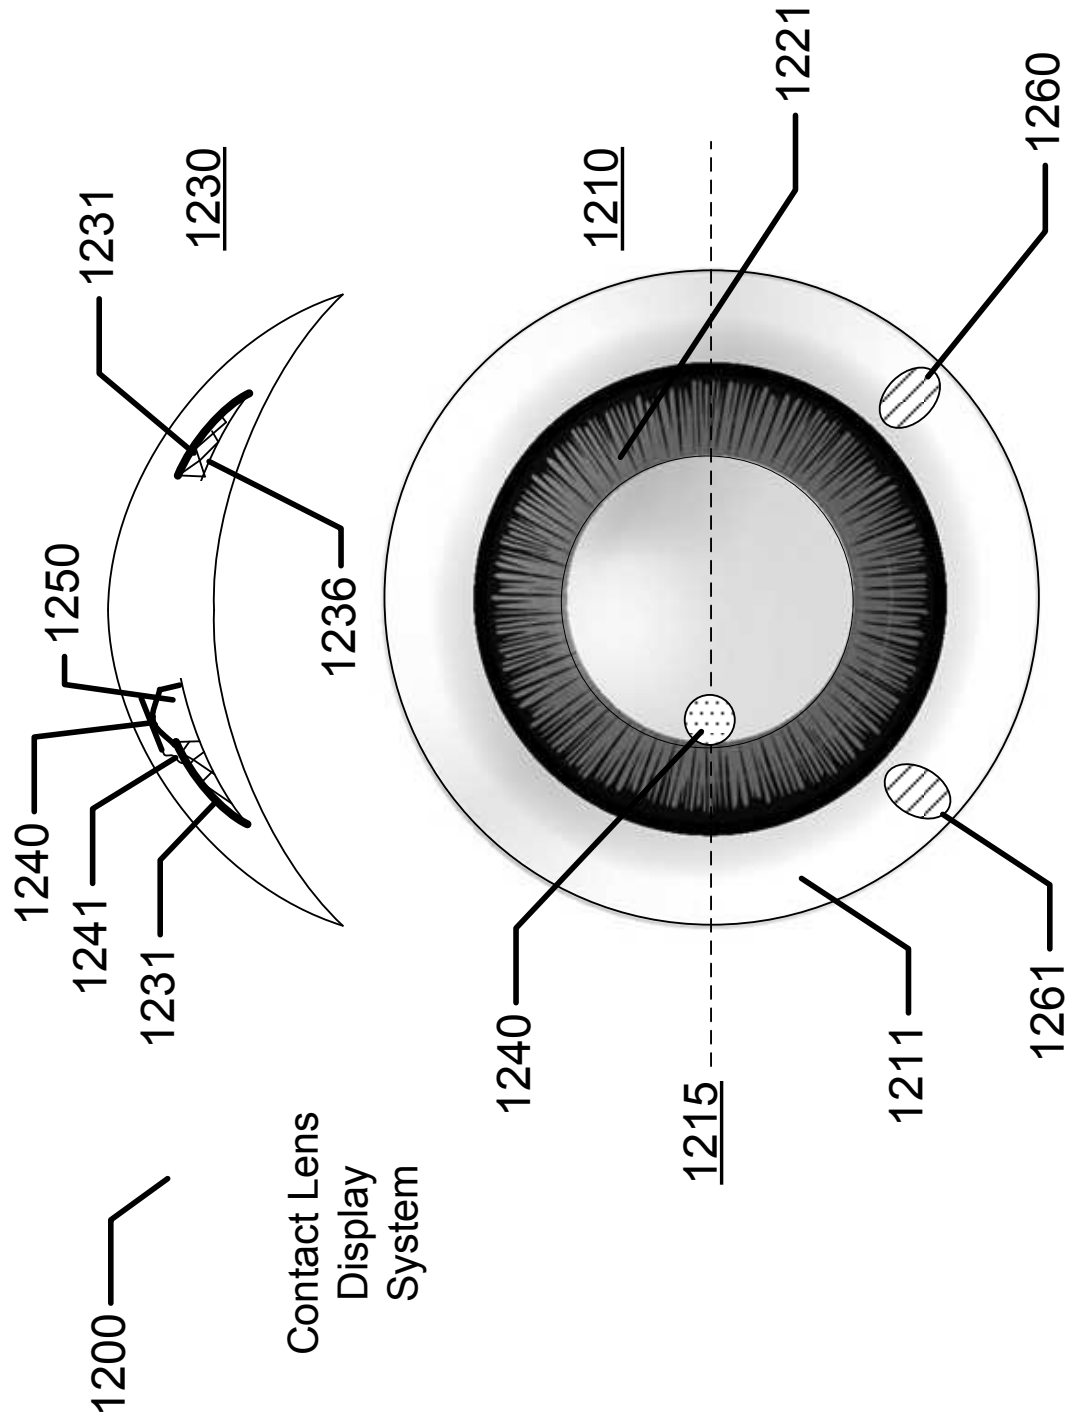


FIG. 12

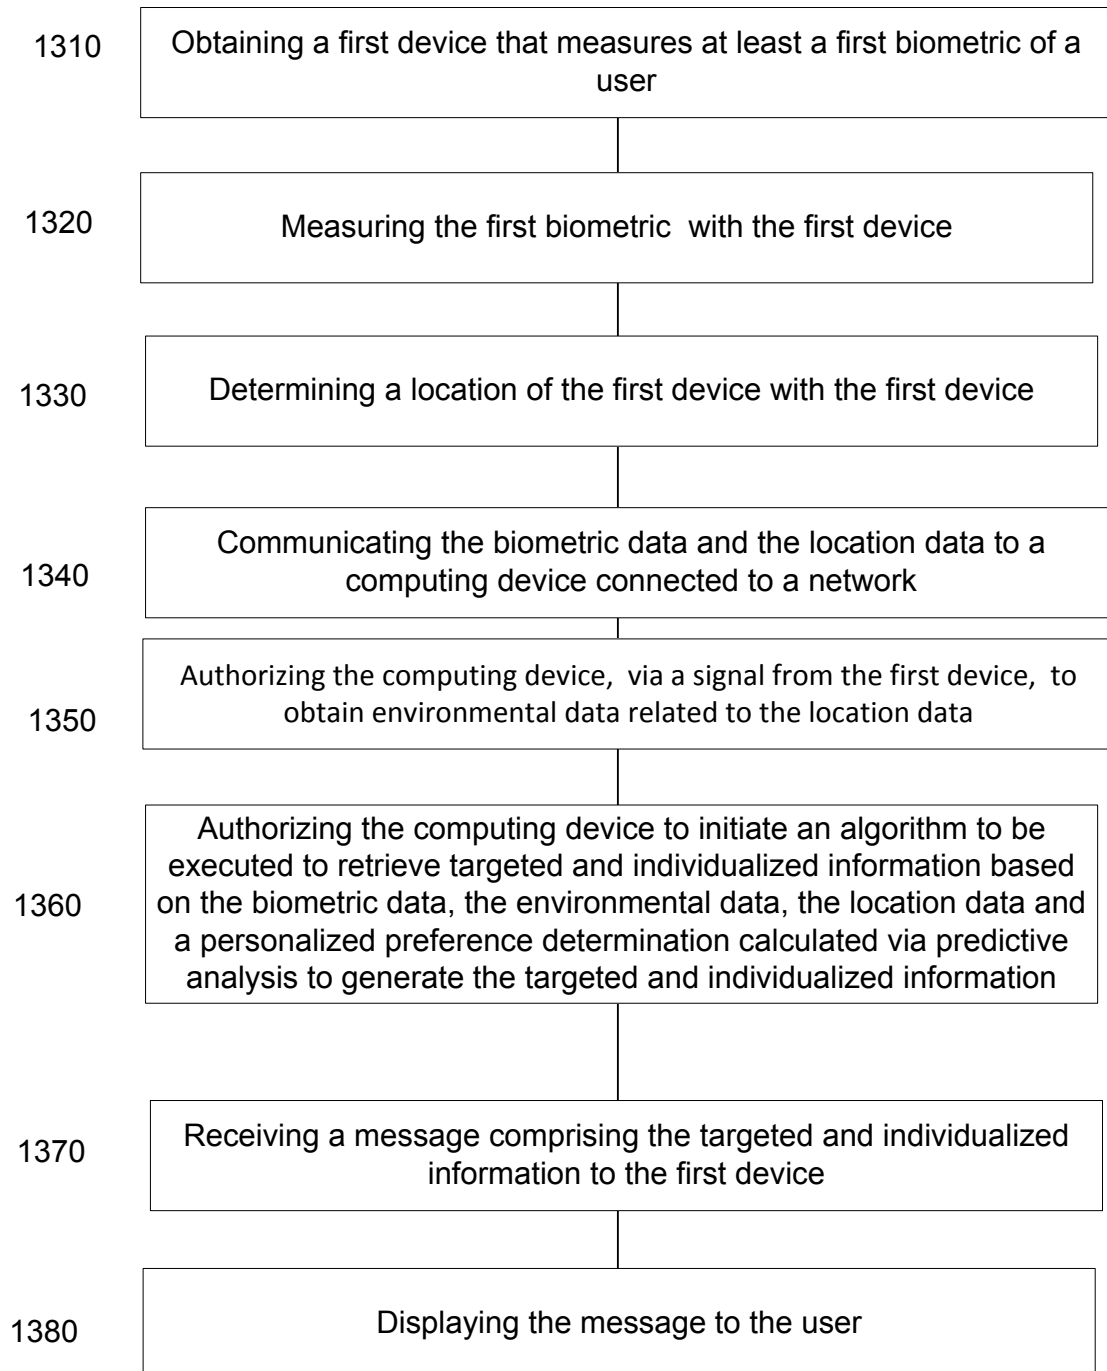


FIG. 13

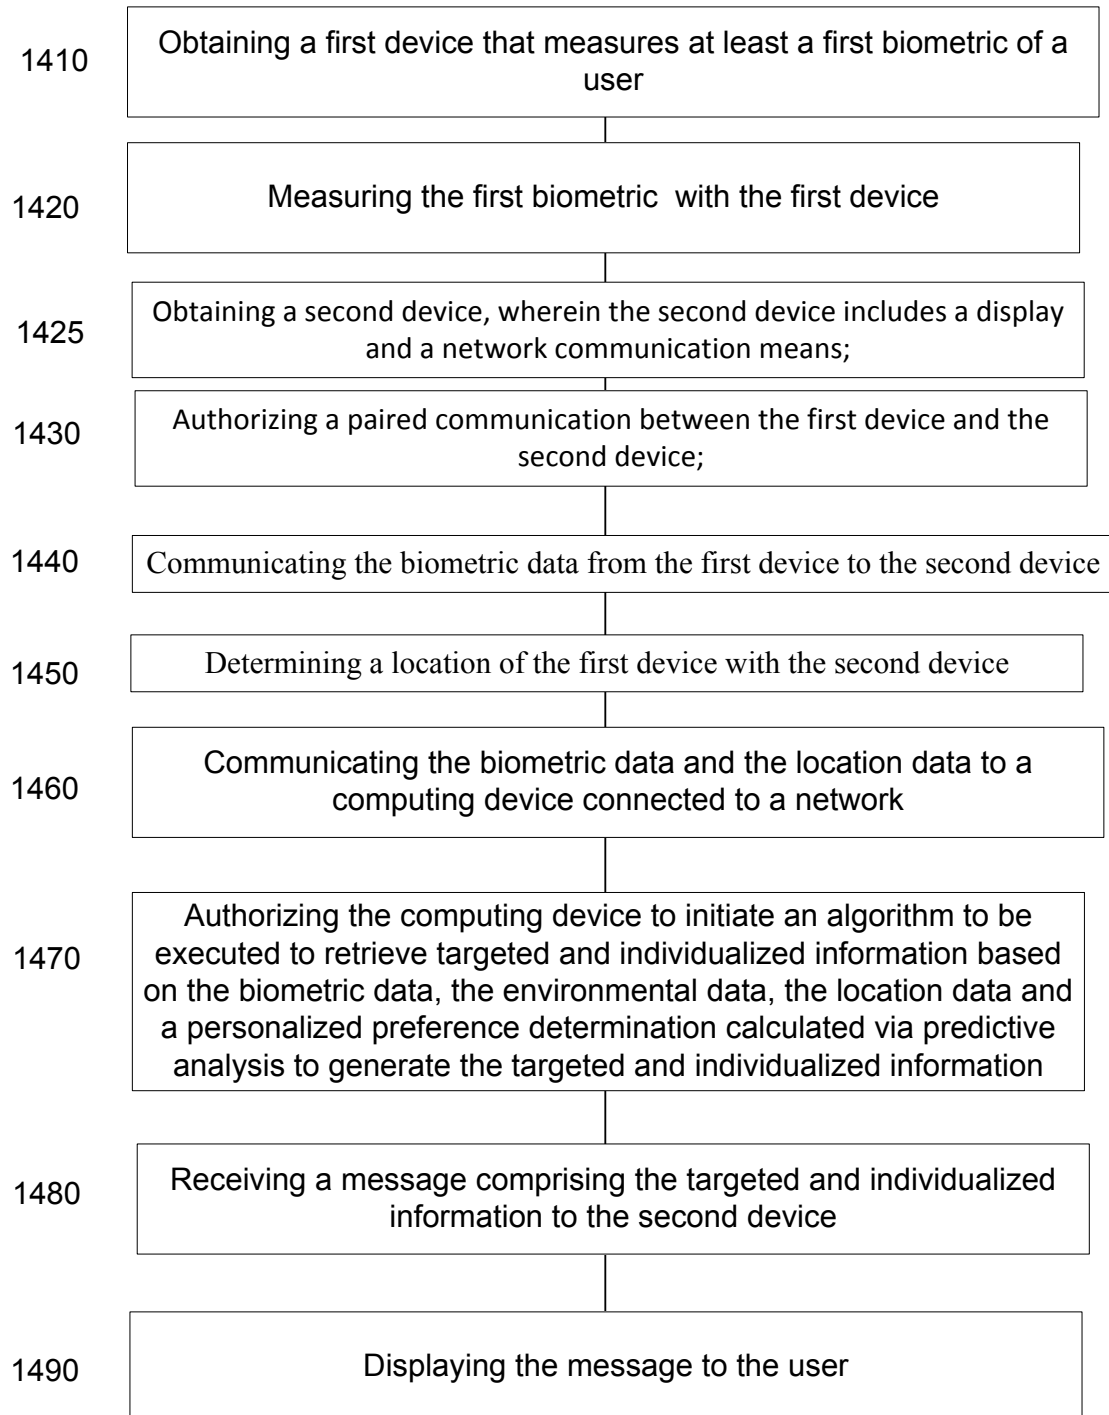


FIG. 14

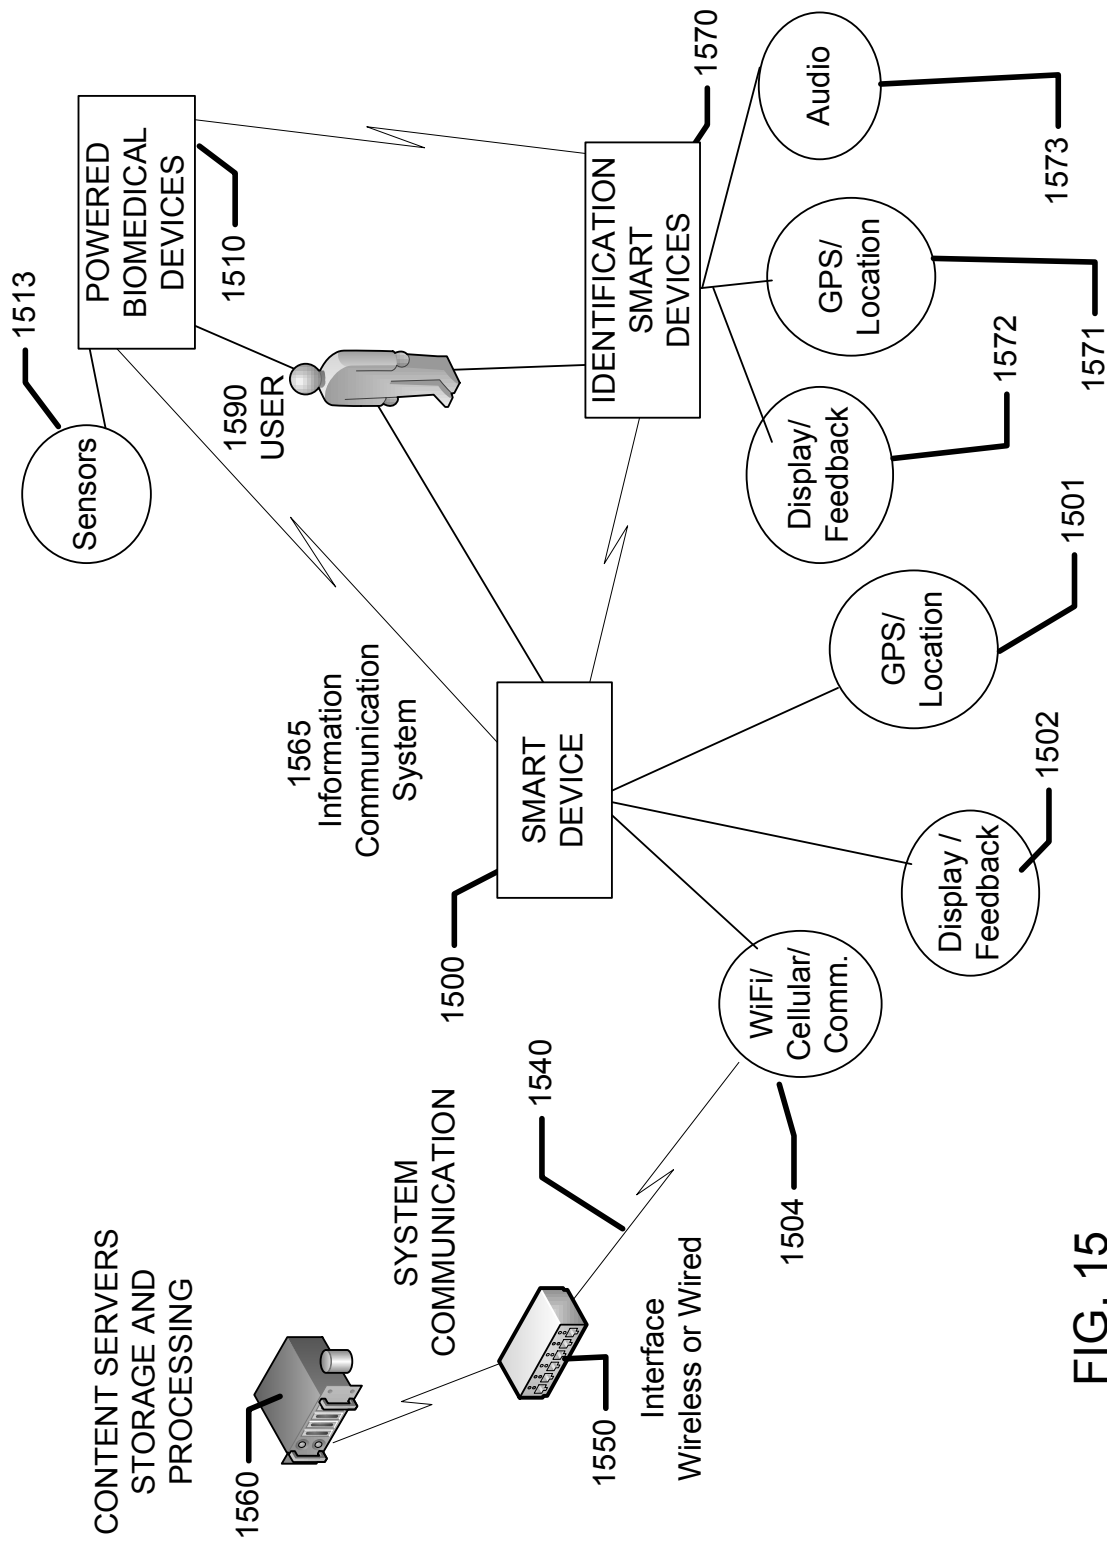


FIG. 15

POWERED  
BIOMEDICAL  
DEVICES FOR  
IDENTIFICATION  
1600

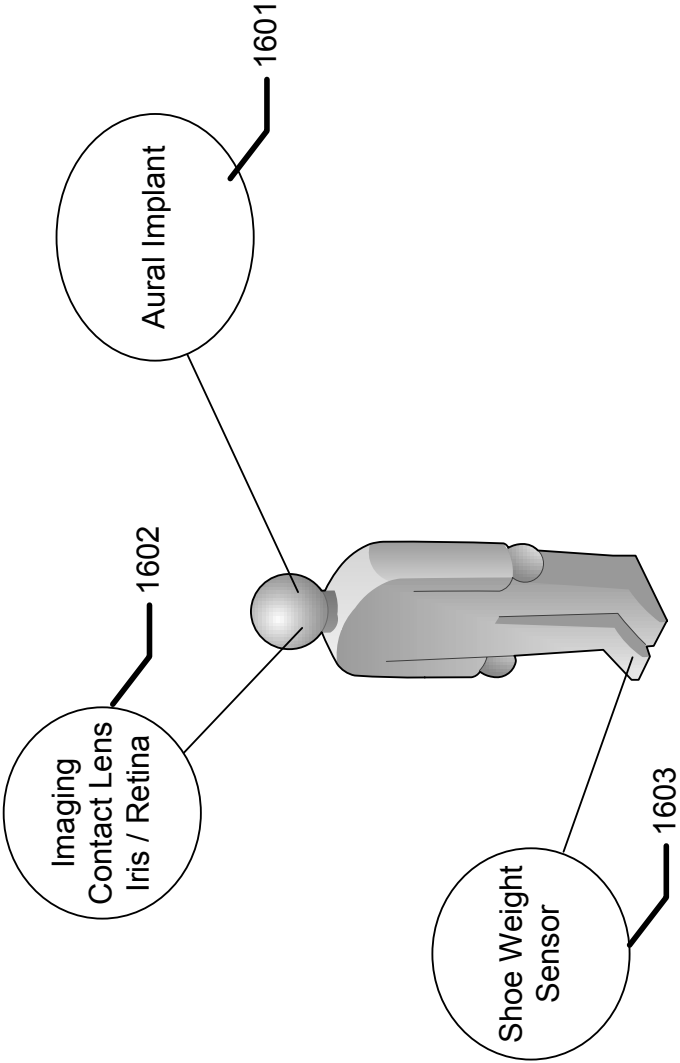


FIG. 16A

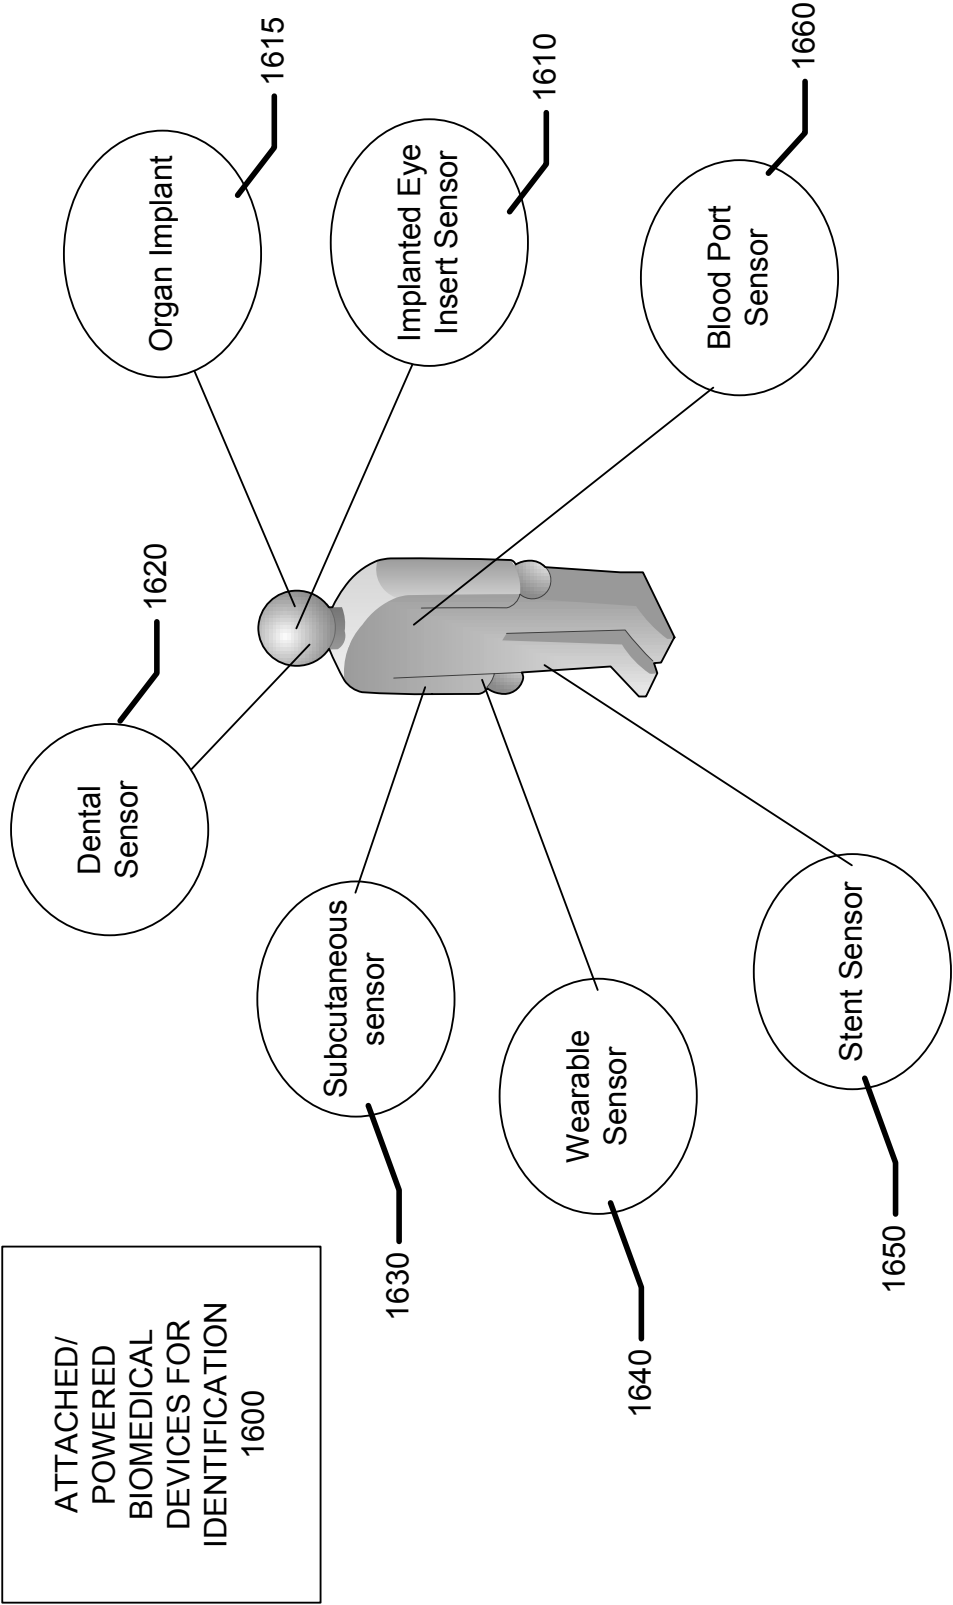


FIG. 16B

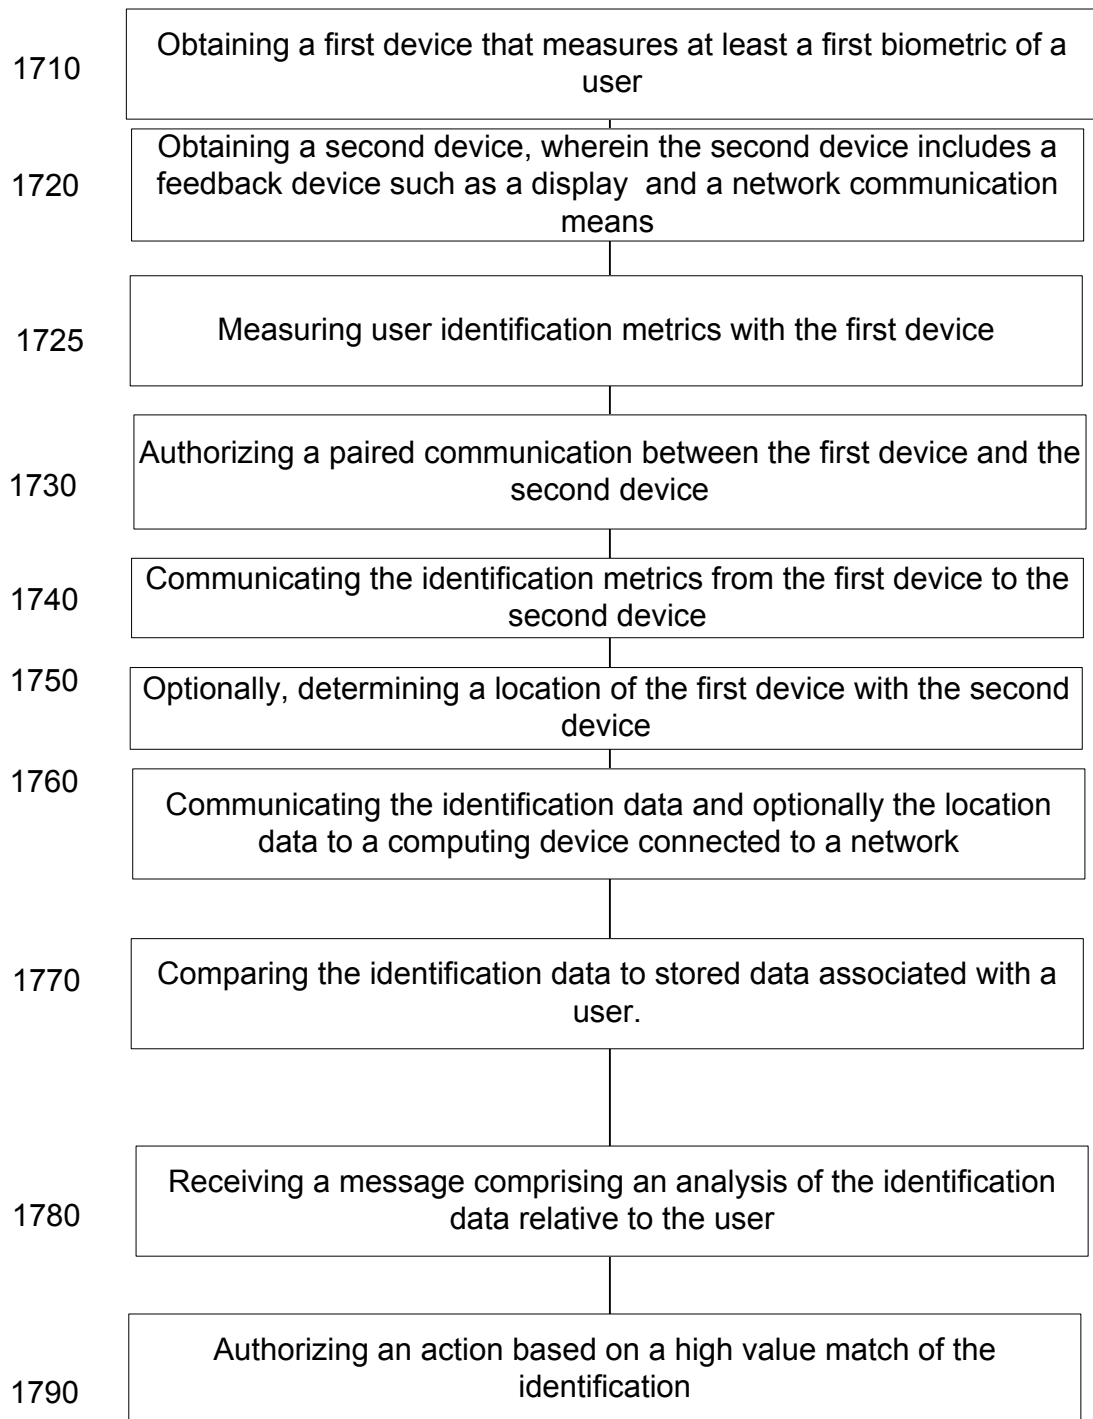


FIG. 17

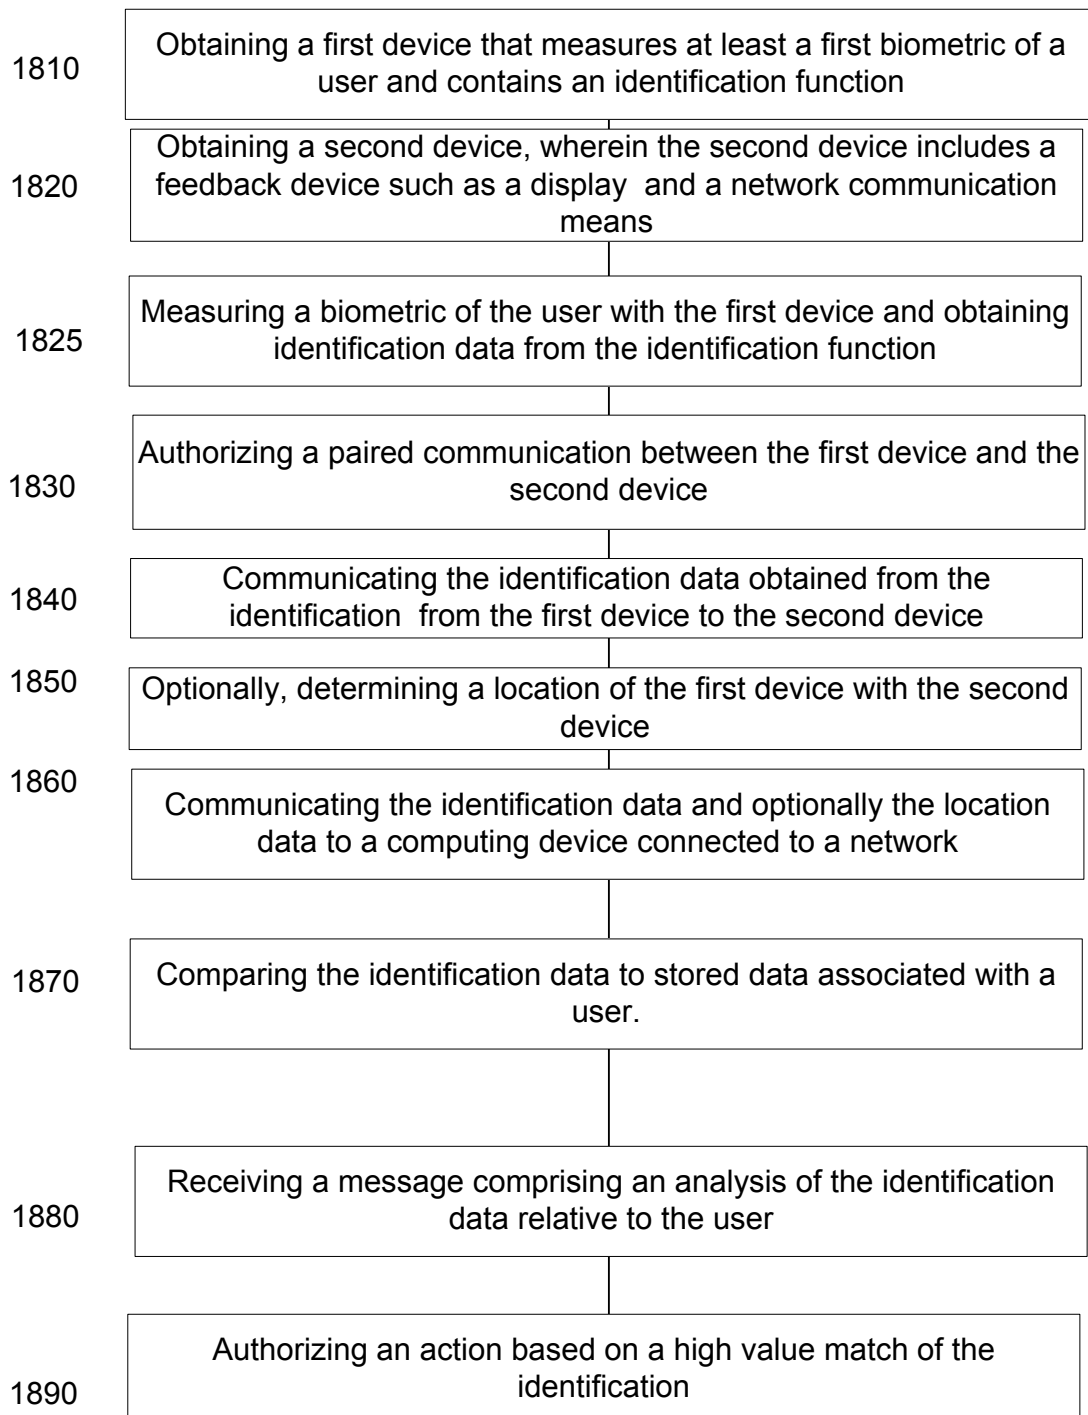


FIG. 18

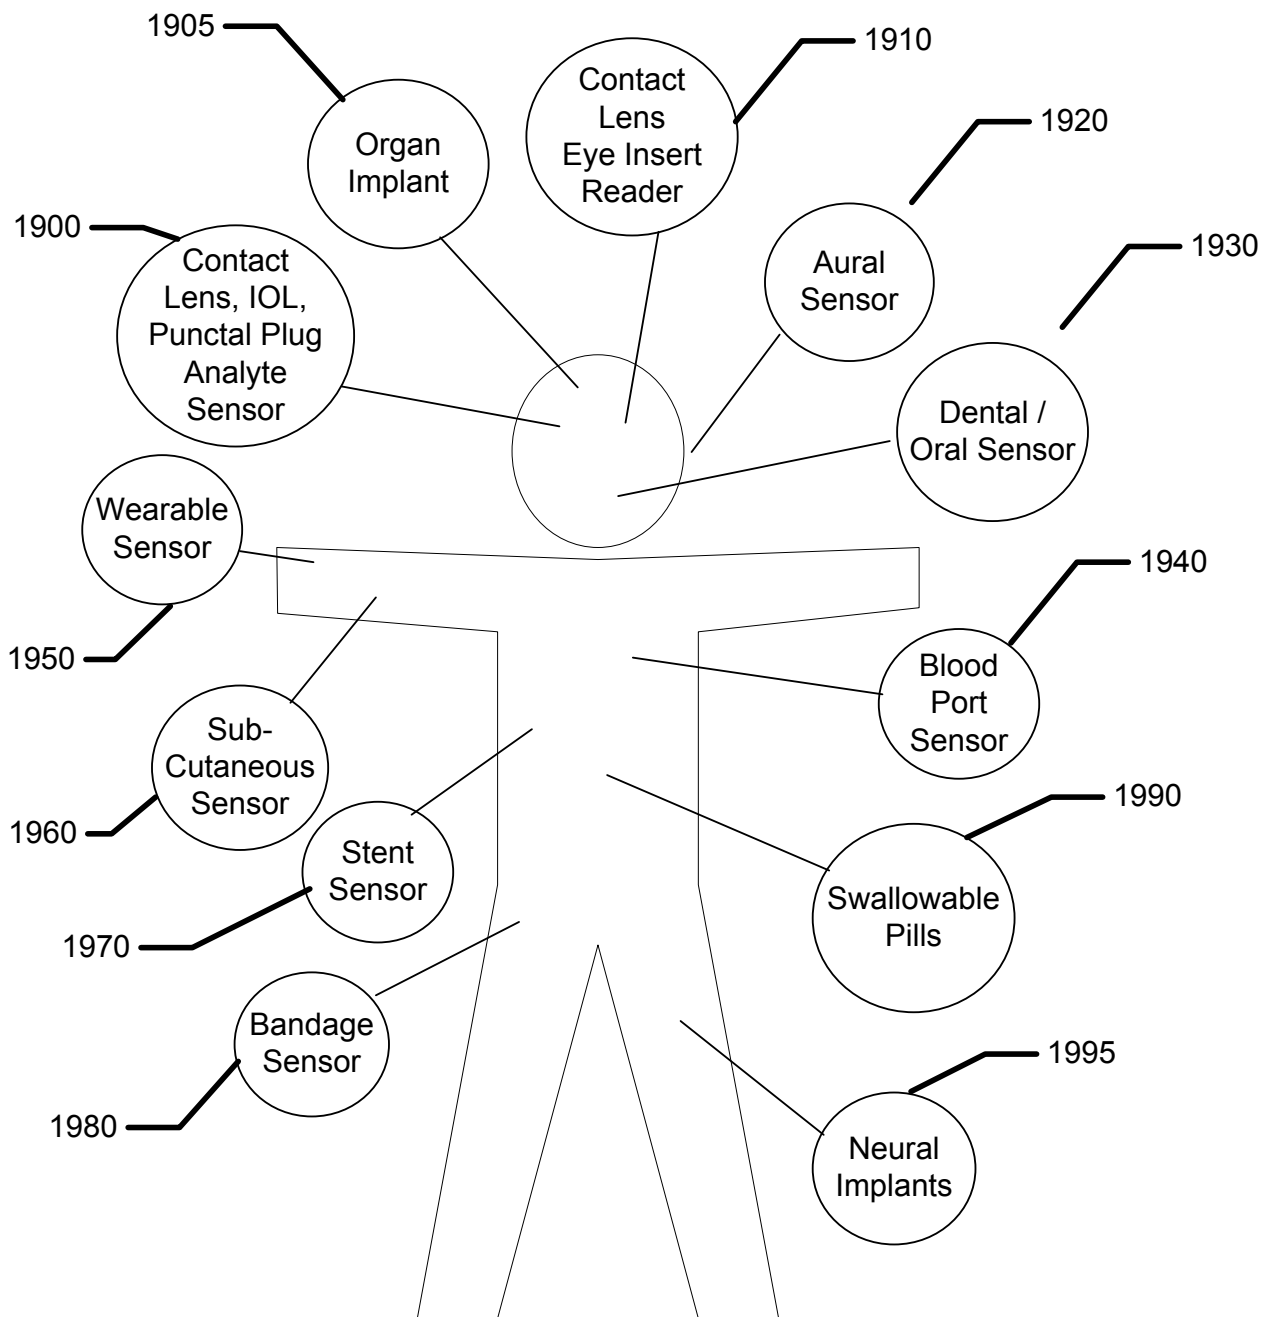


FIG. 19