

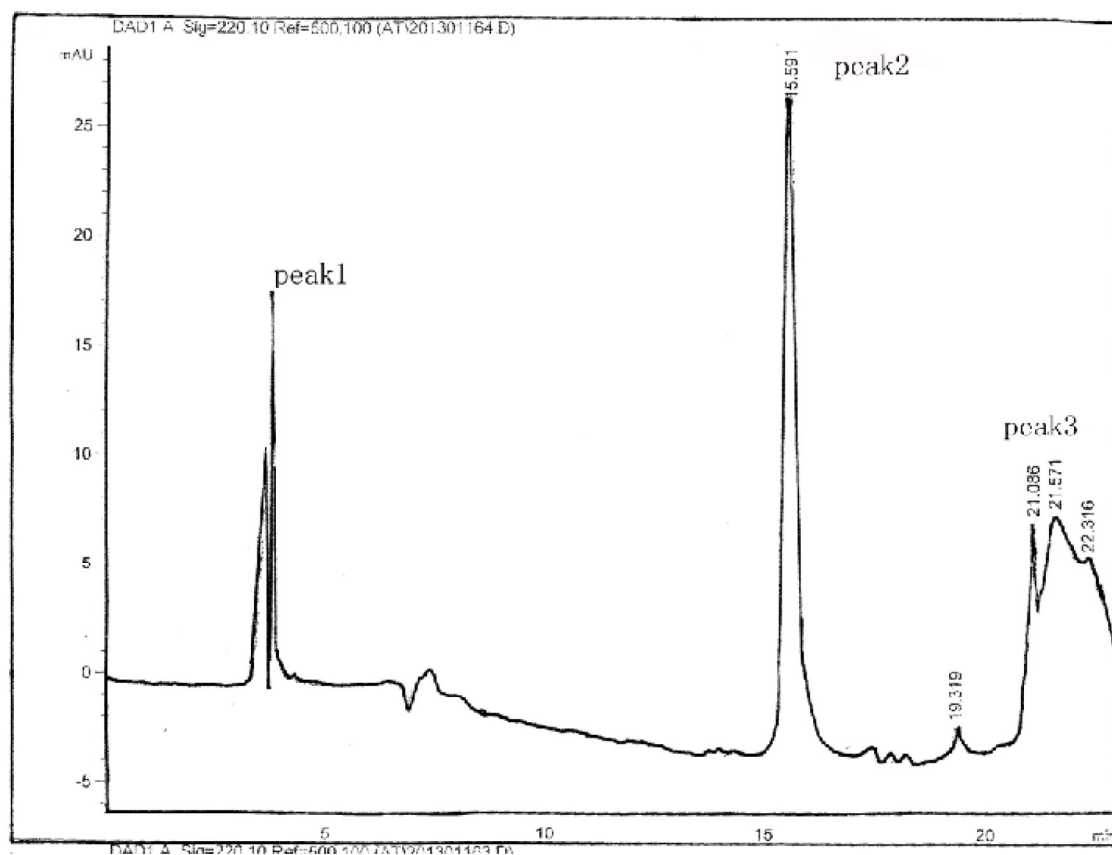


Fig.1 HPLC C₁₈ reversed-phase column separation pattern of α_1 -antitrypsin obtain 3 peaks.

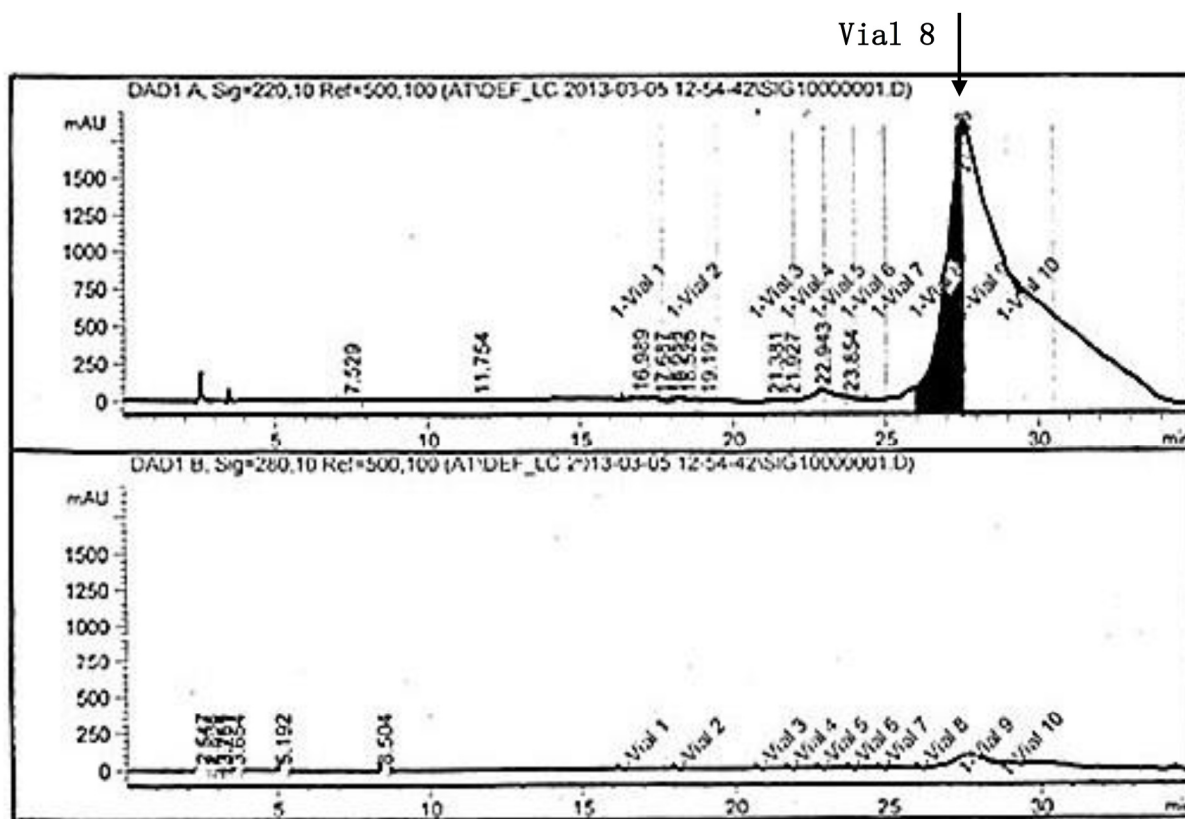


Fig 2 HPLC C_{18} reversed-phase column separation pattern with an increasing eluting gradient of peak 3 obtained 10 peaks

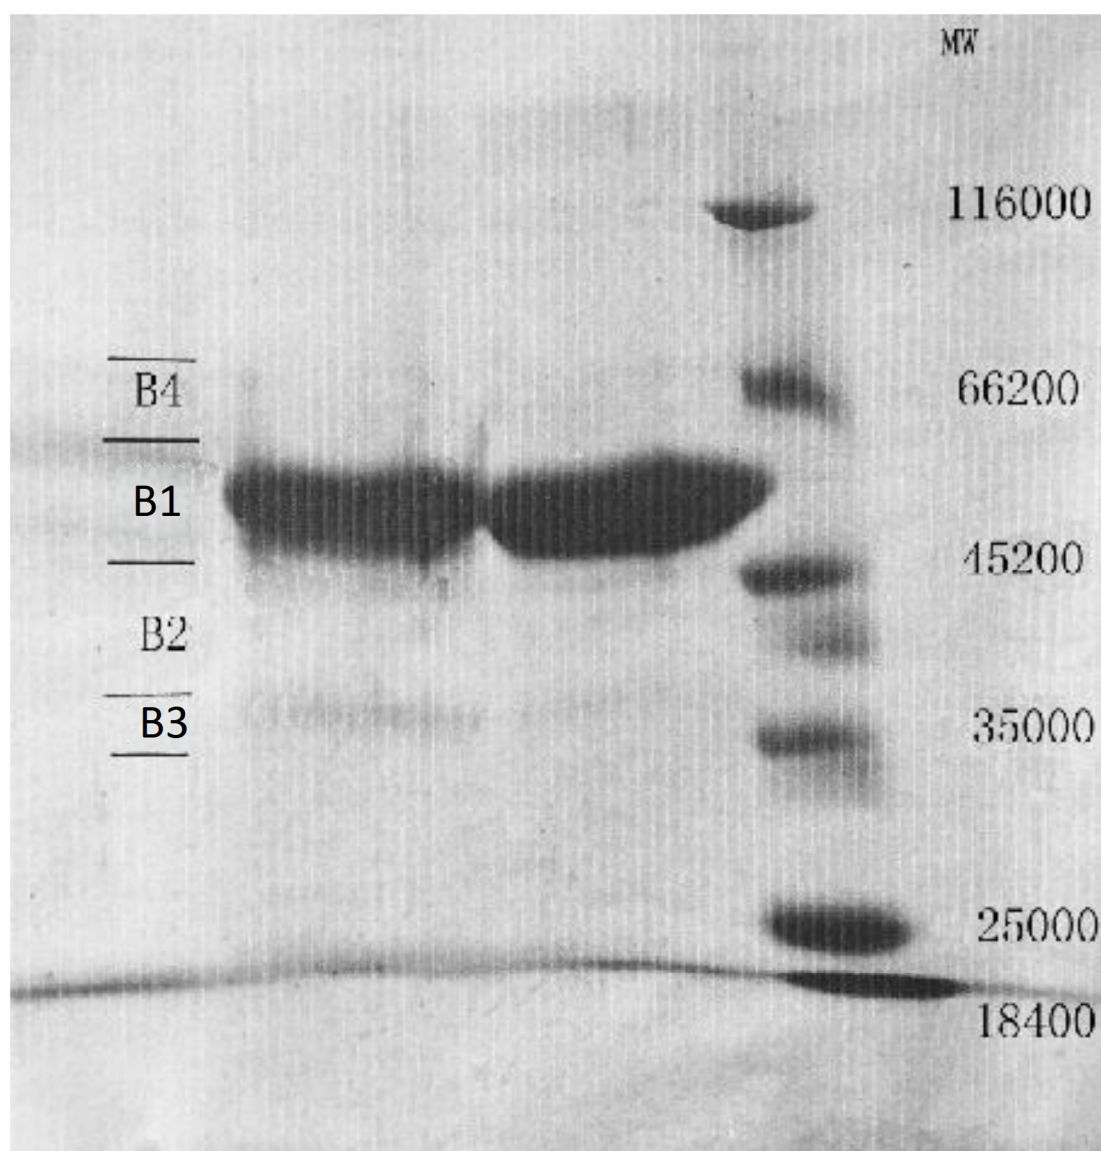


Fig 3 Preparative SDS-PAGE of vial 8(collected from HPLC C₁₈ reversed-phase column as showed in Fig 2.)