

1/28

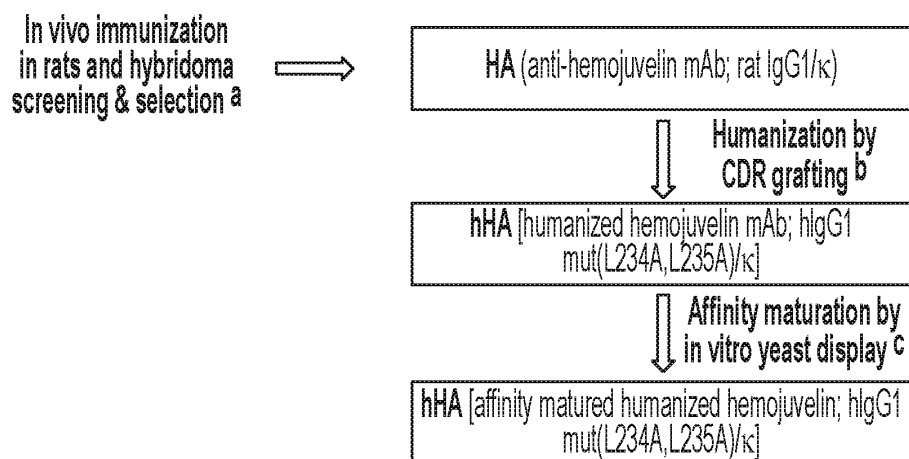


FIG. 1A

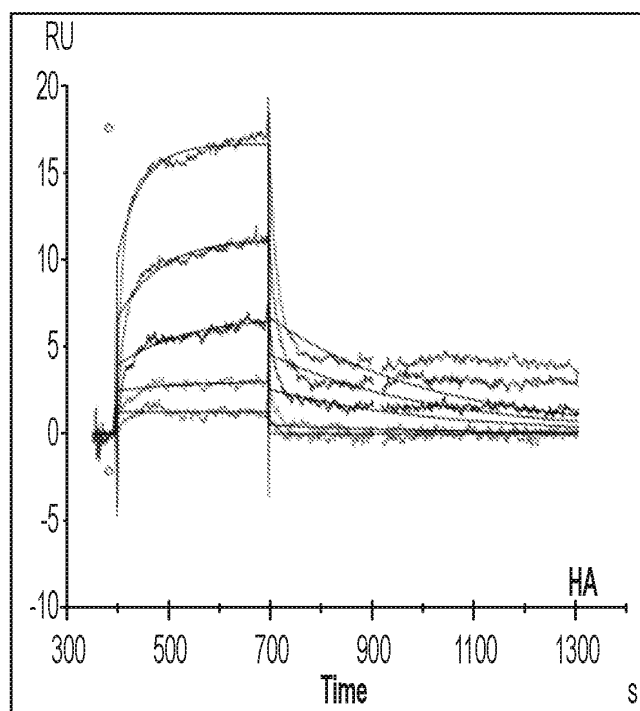


FIG. 1B

2/28

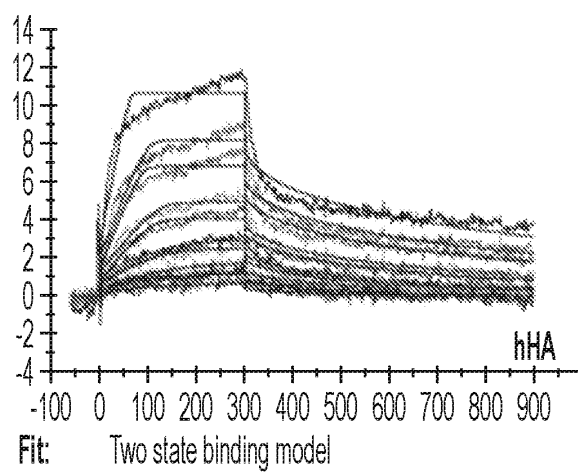


FIG. 1C

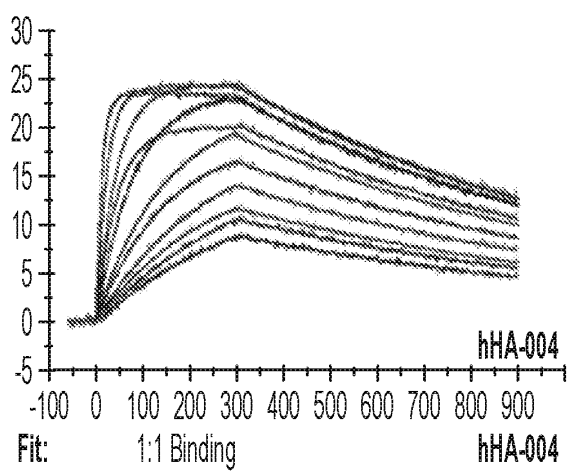


FIG. 1D

3/28

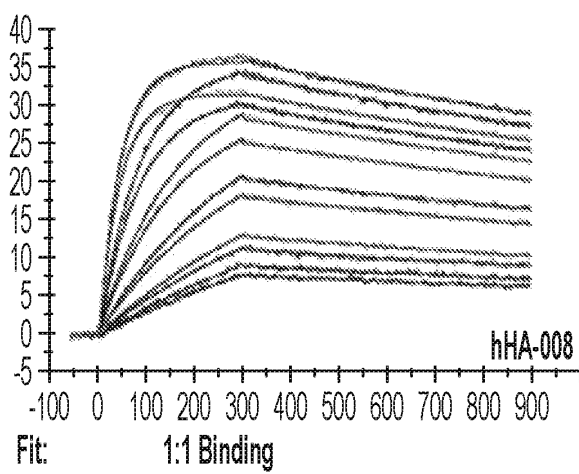


FIG. 1E

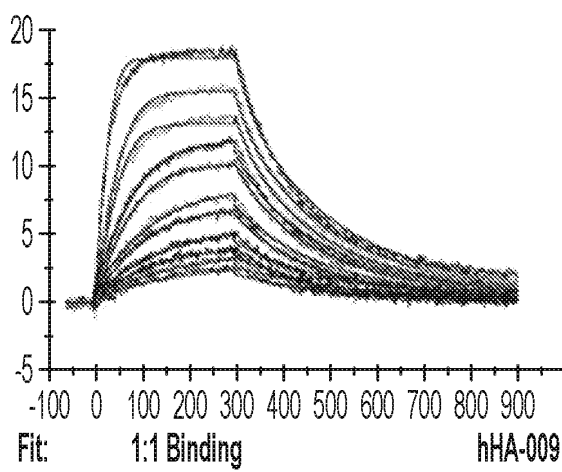


FIG. 1F

4/28

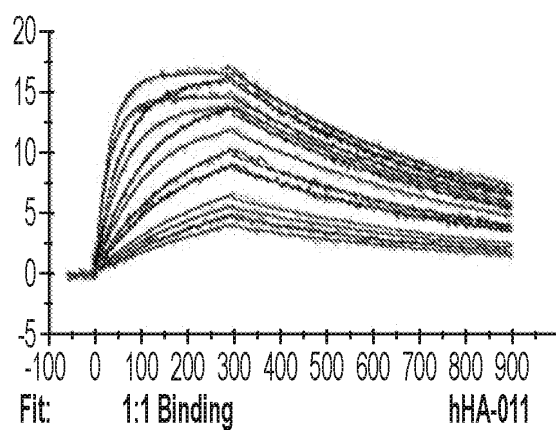


FIG. 1G

Principle of HJV BMP Reporter Assay

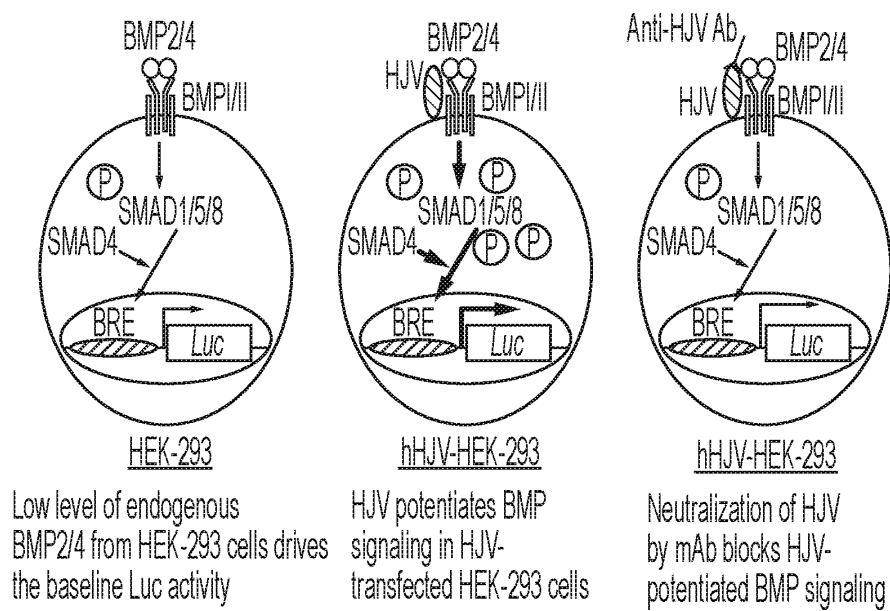


FIG. 2A

5/28

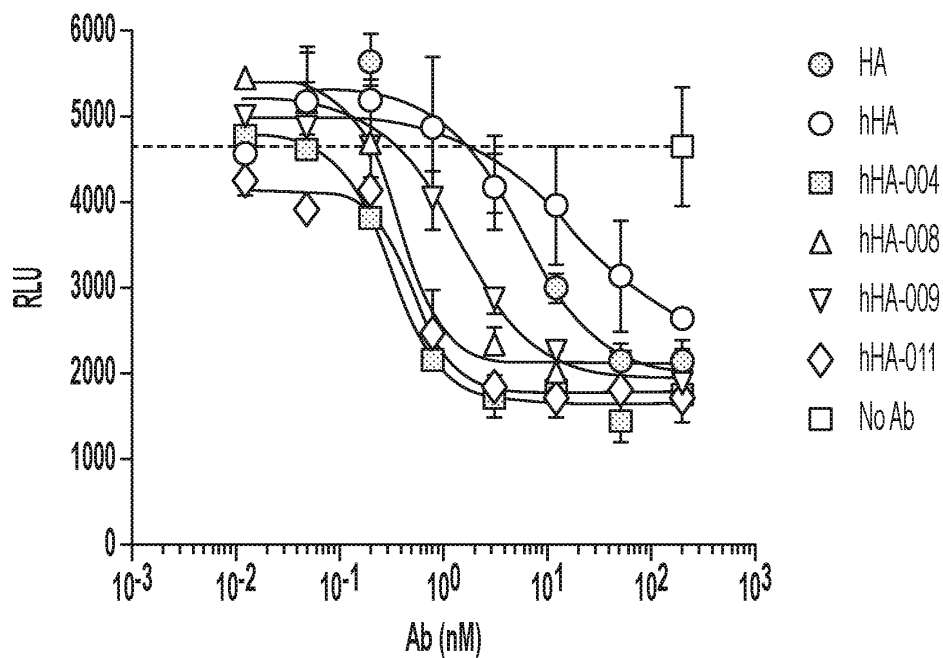


FIG. 2B

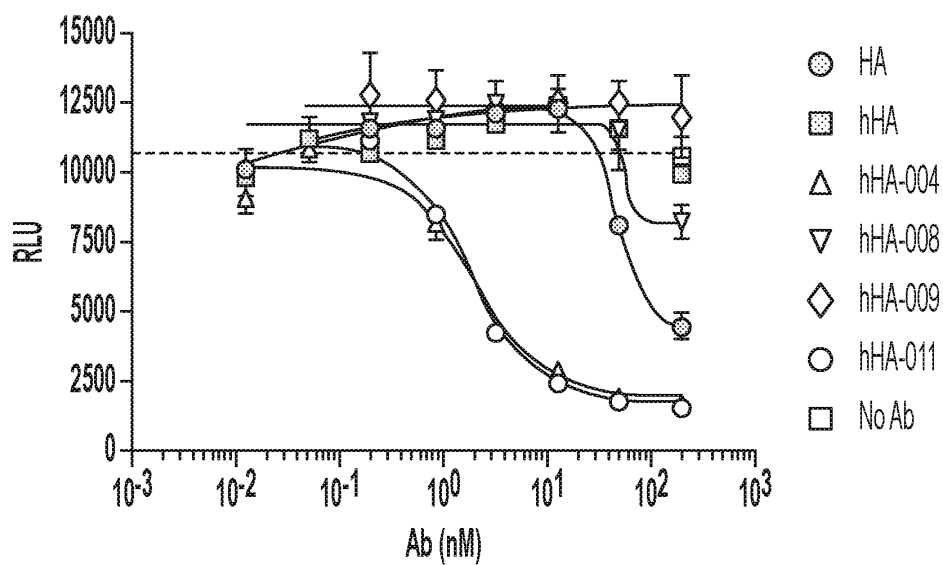


FIG. 2C

6/28

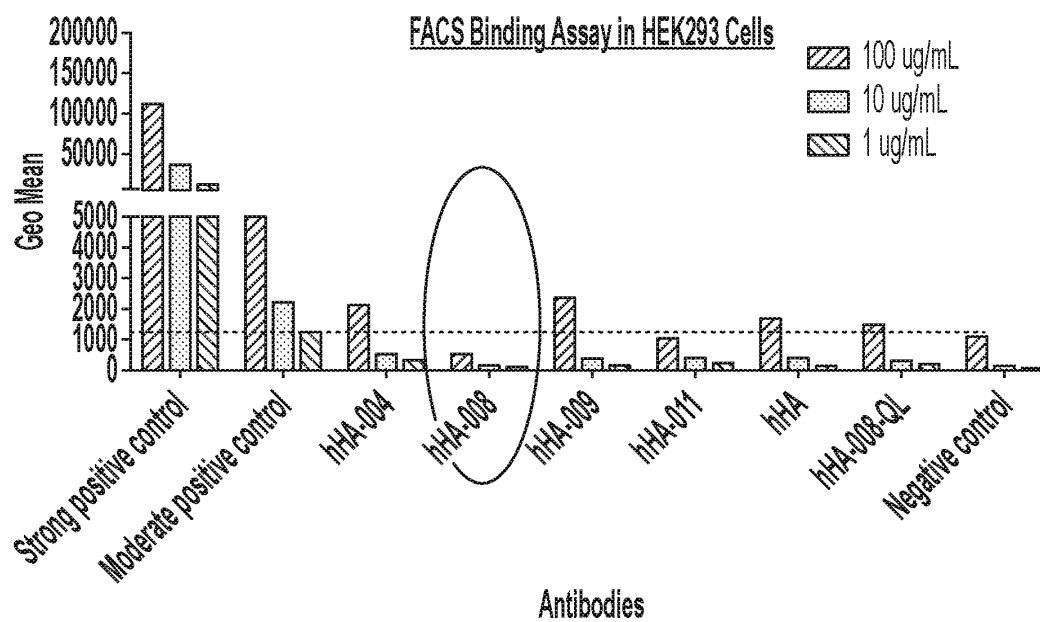


FIG. 3

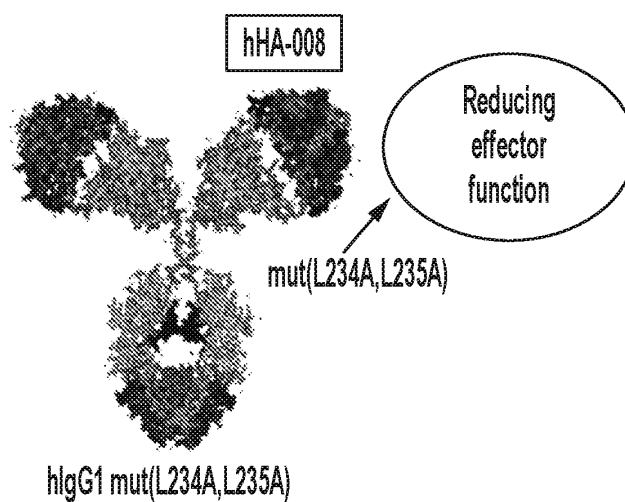


FIG. 4A

7/28

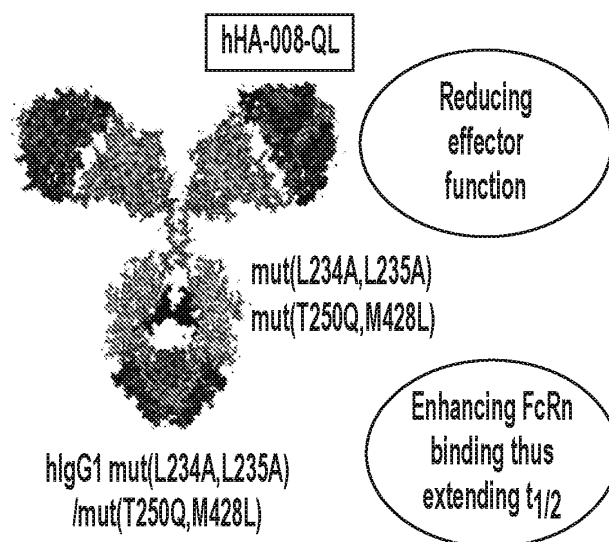


FIG. 4B

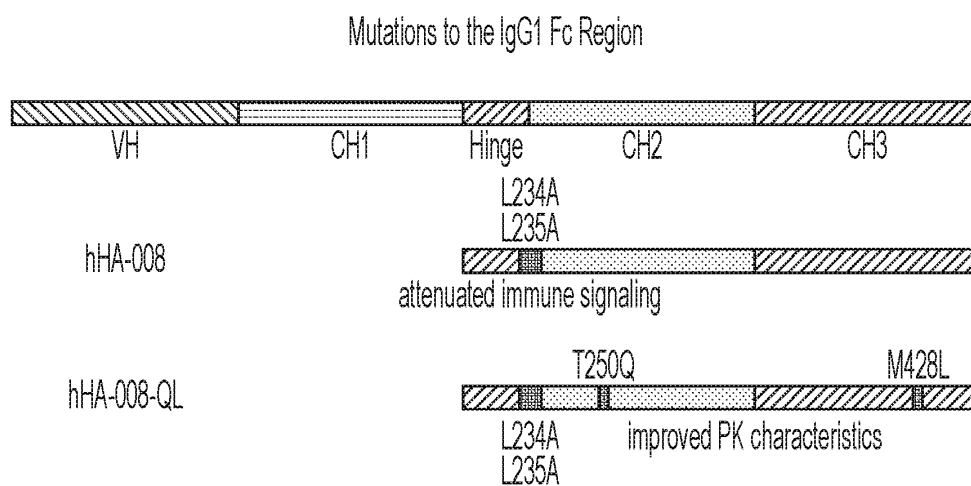


FIG. 4C

8/28

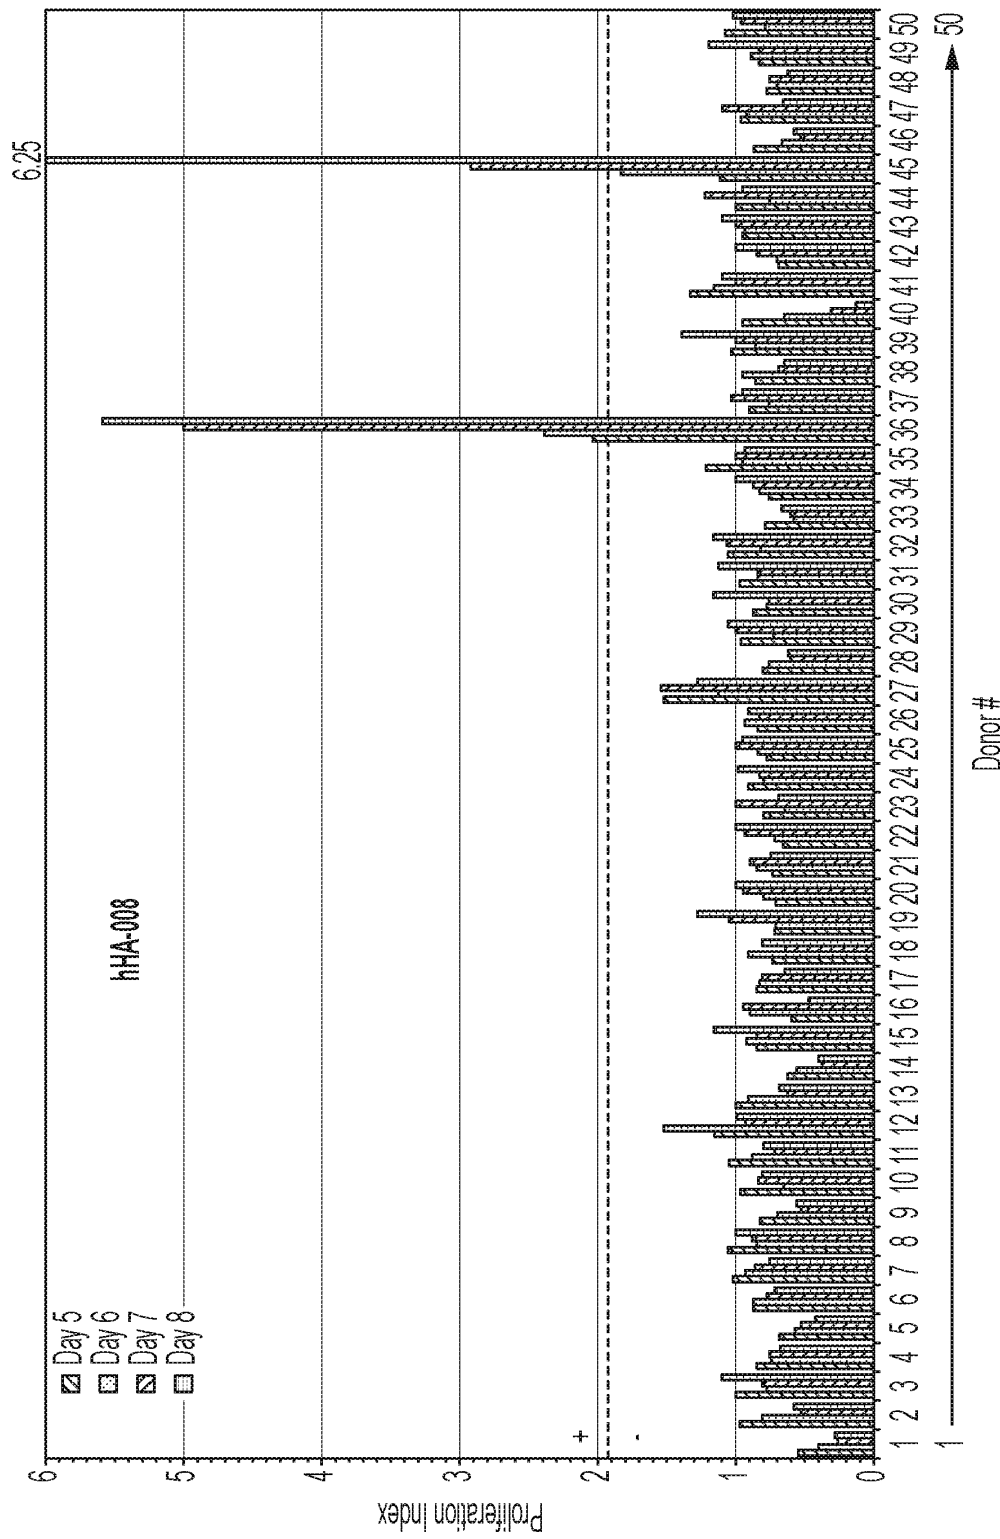


FIG. 5

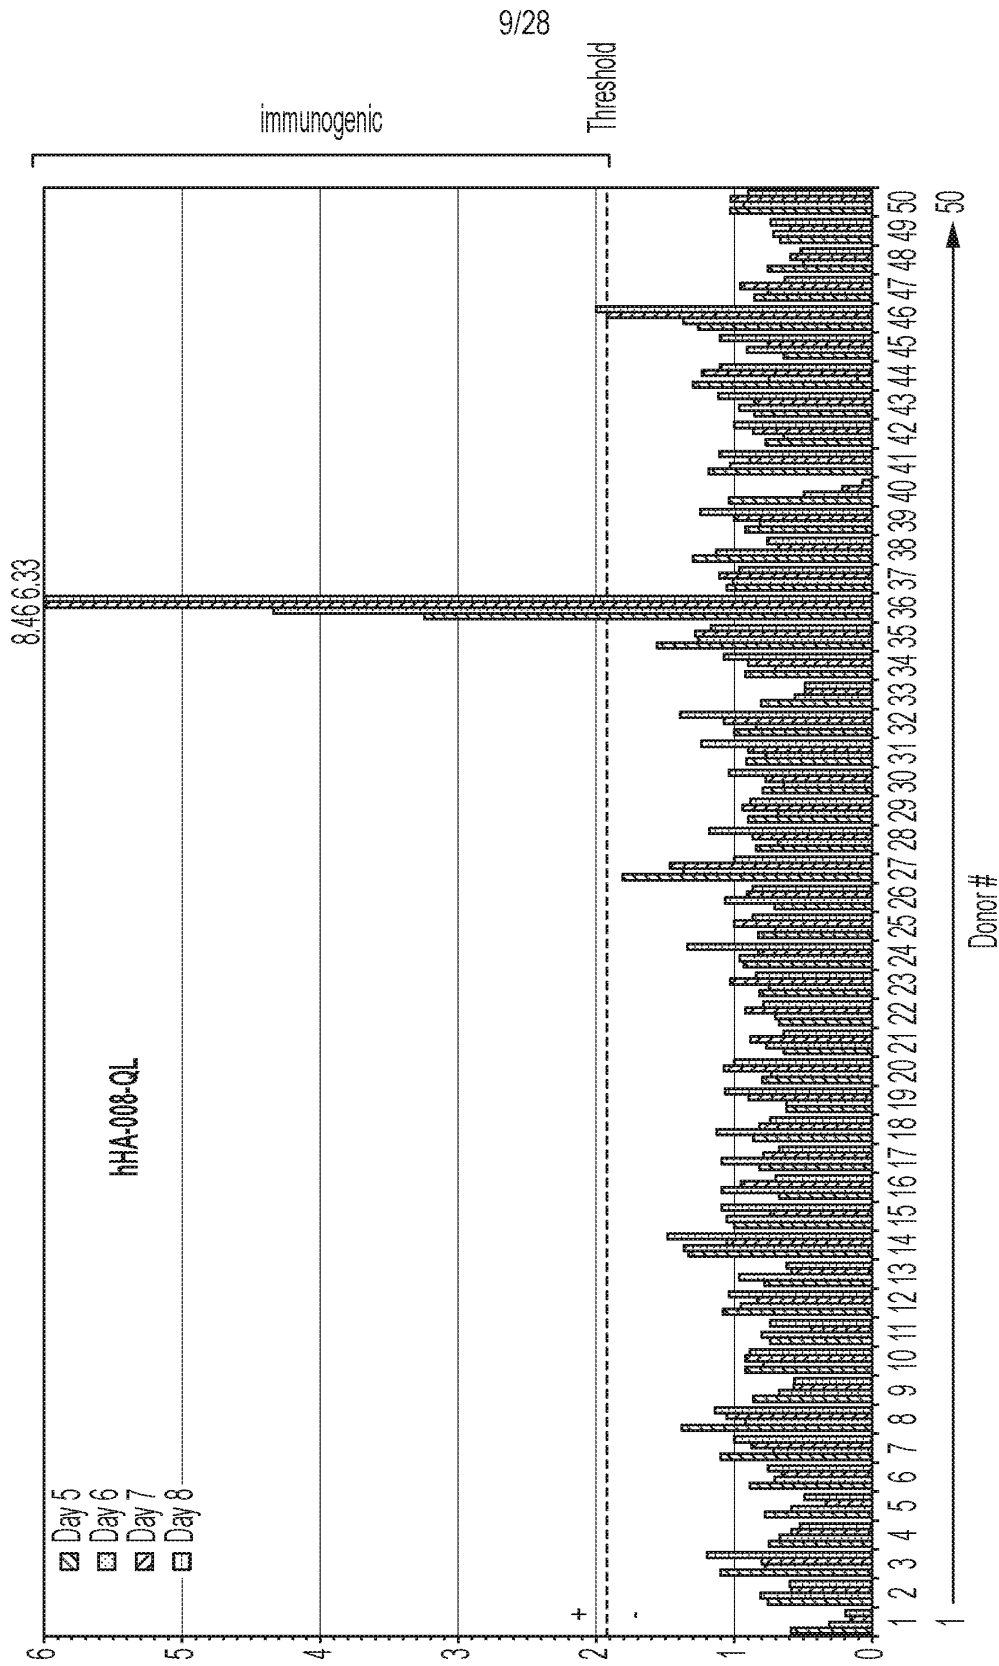


FIG. 5
CONTINUED

10/28

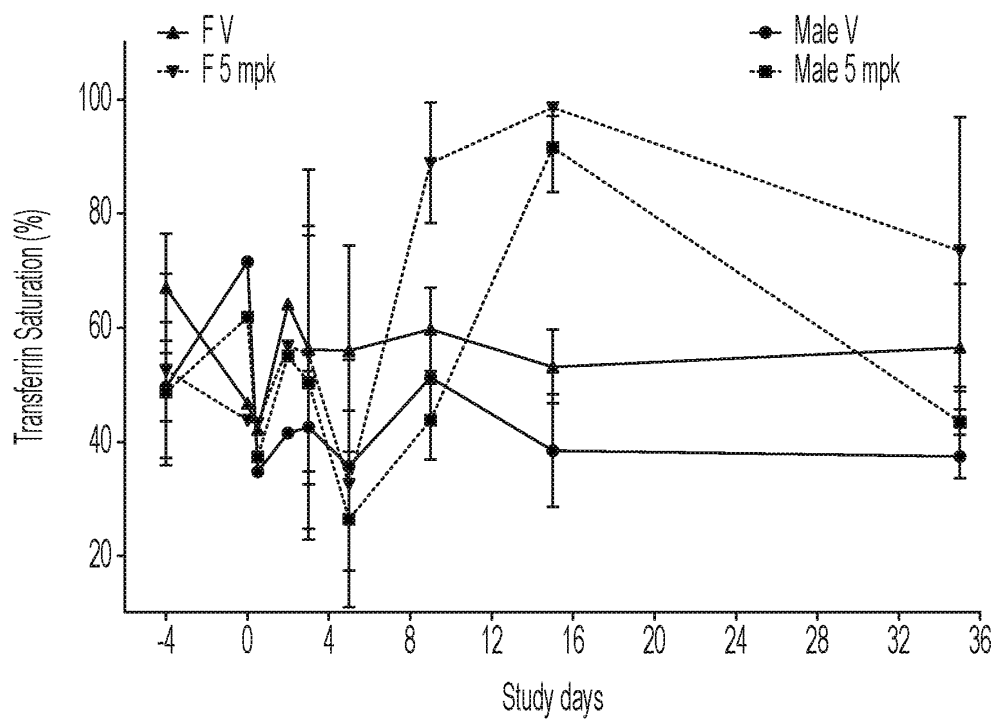


FIG. 6A

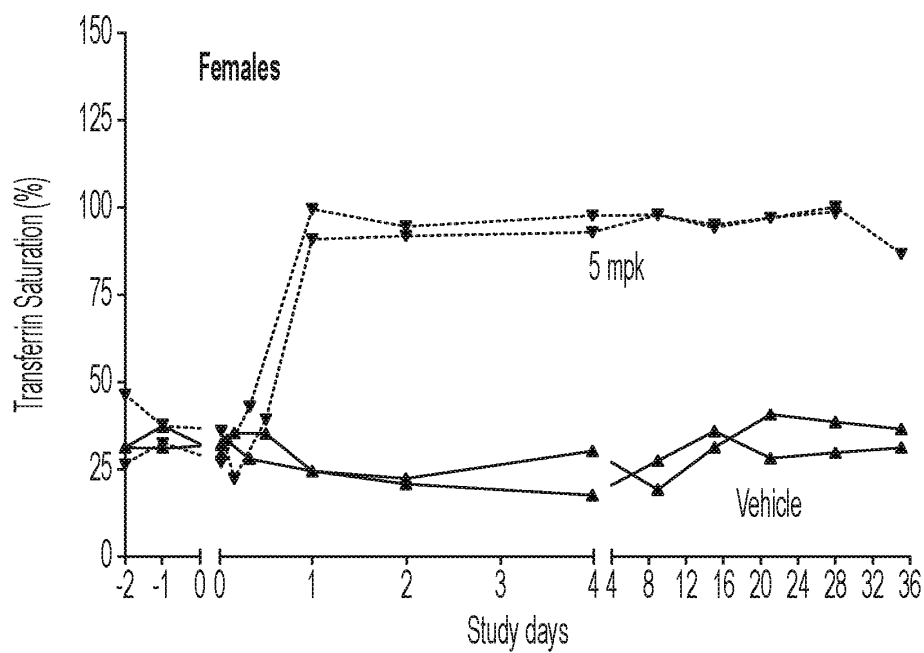


FIG. 6B

11/28

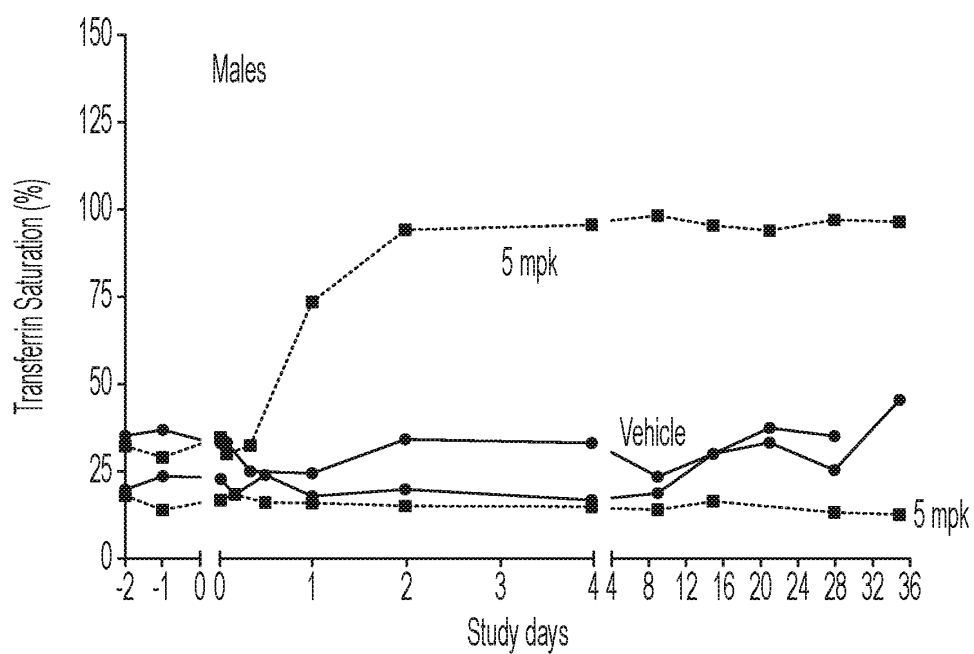


FIG. 6C

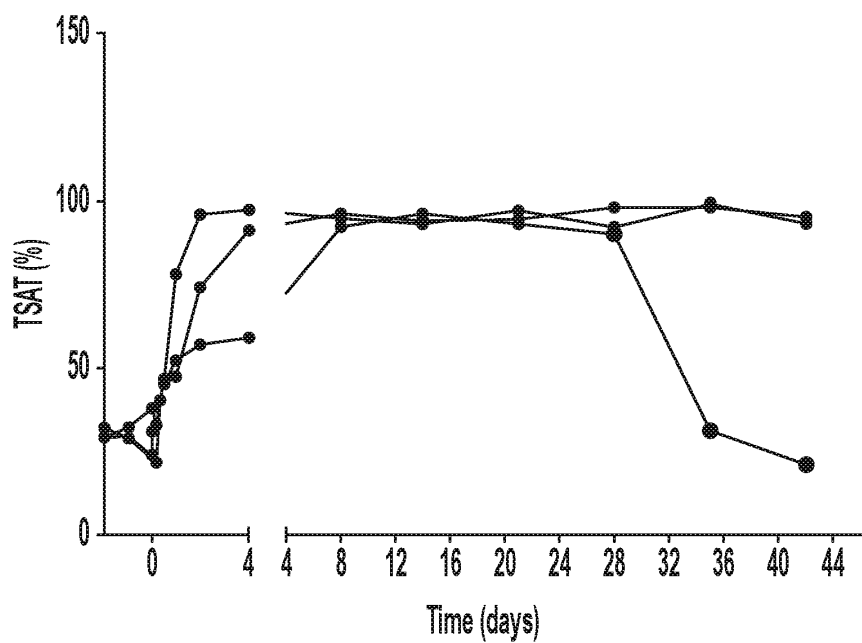


FIG. 7A

12/28

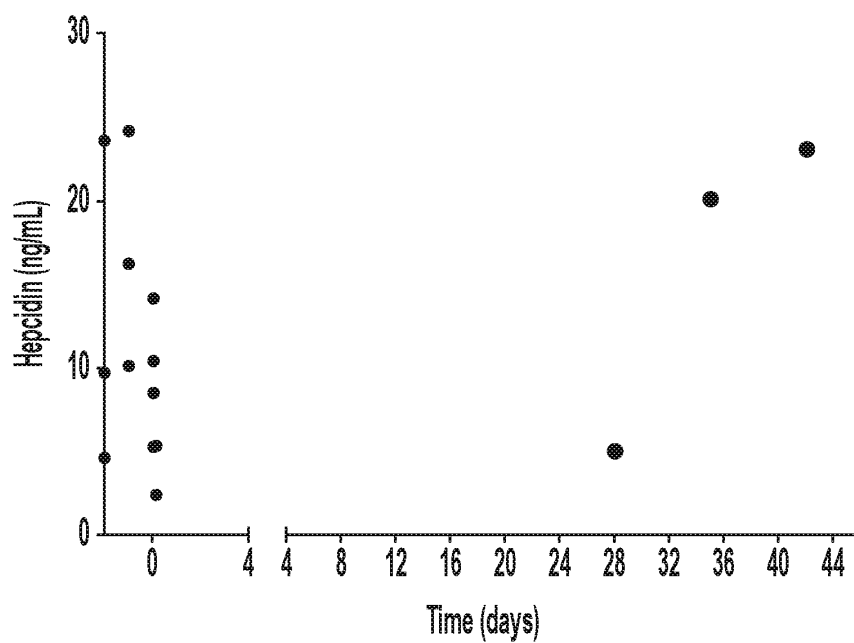


FIG. 7B

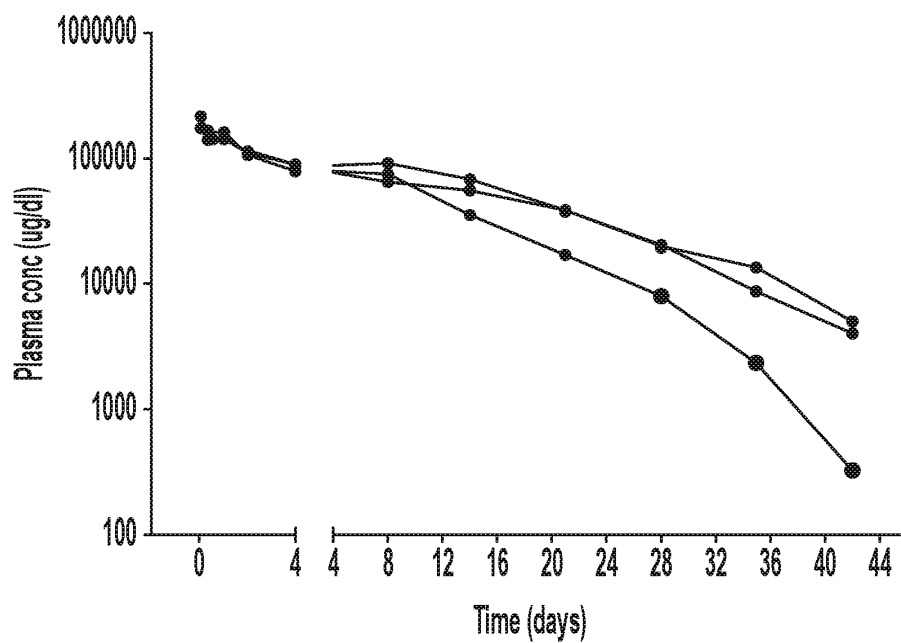


FIG. 7C

13/28

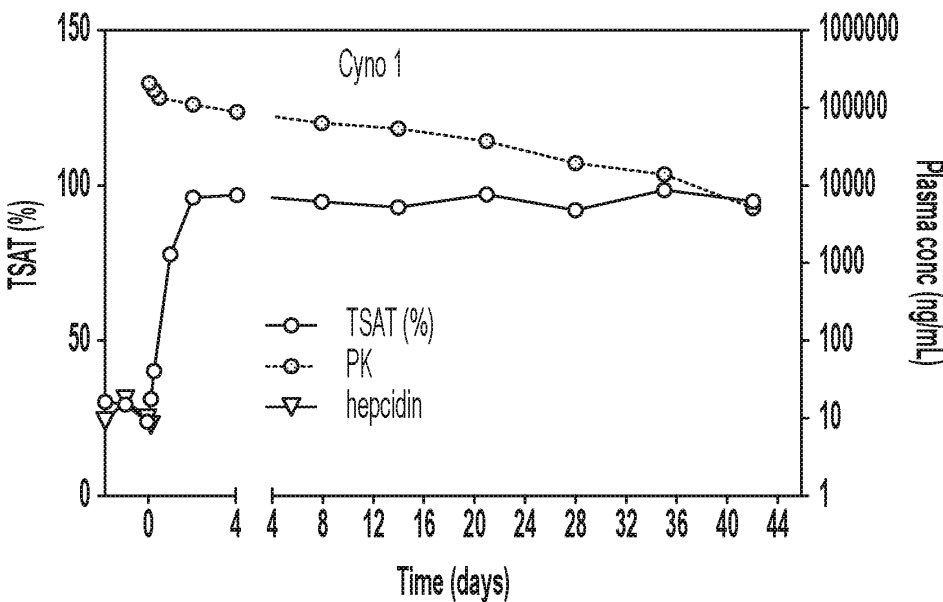


FIG. 7D

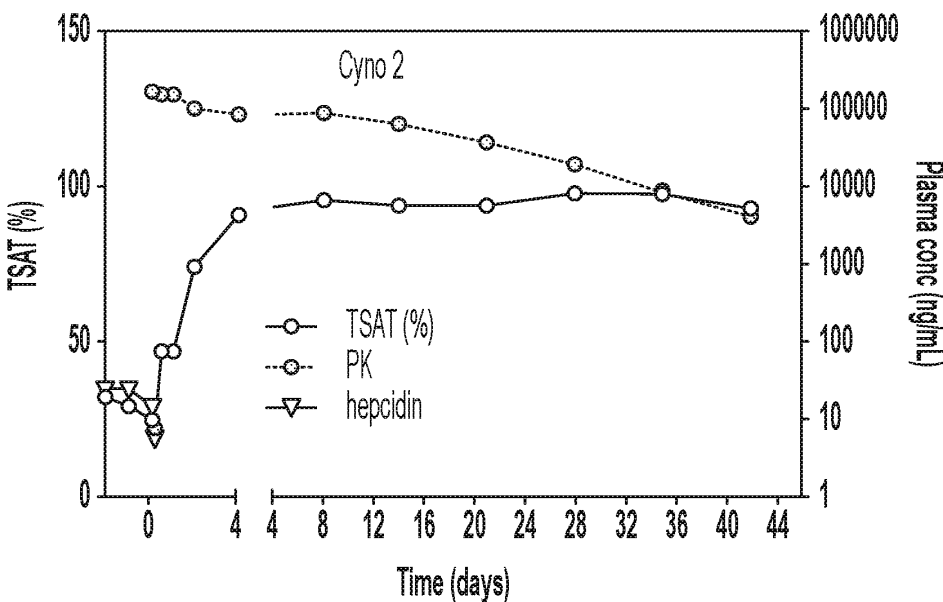


FIG. 7E

14/28

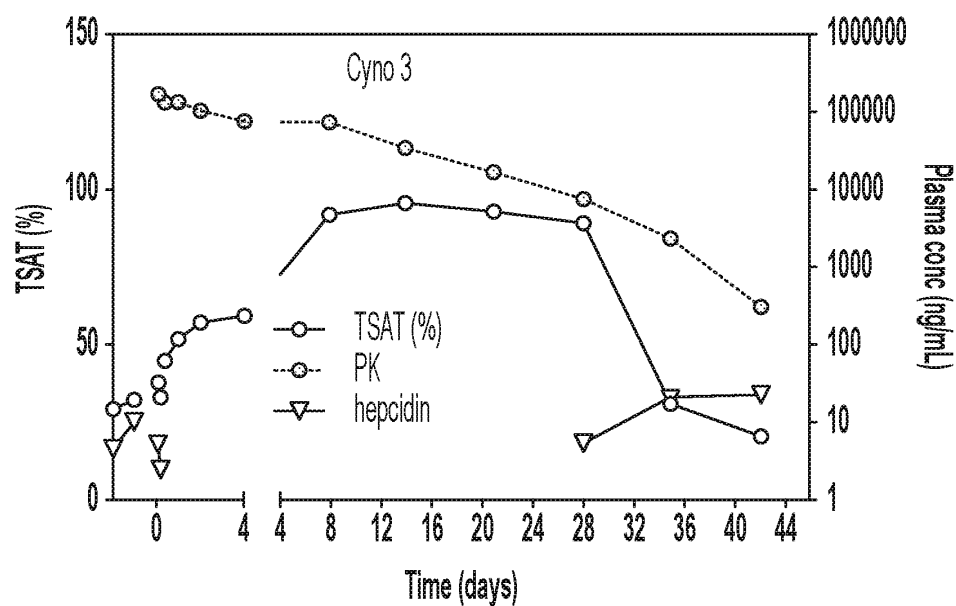


FIG. 7F

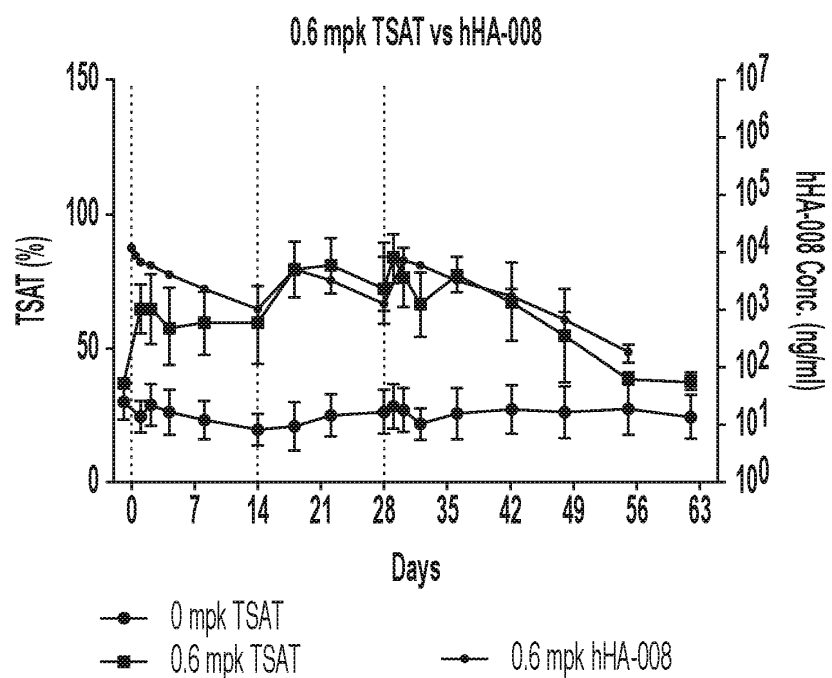


FIG. 8A

15/28

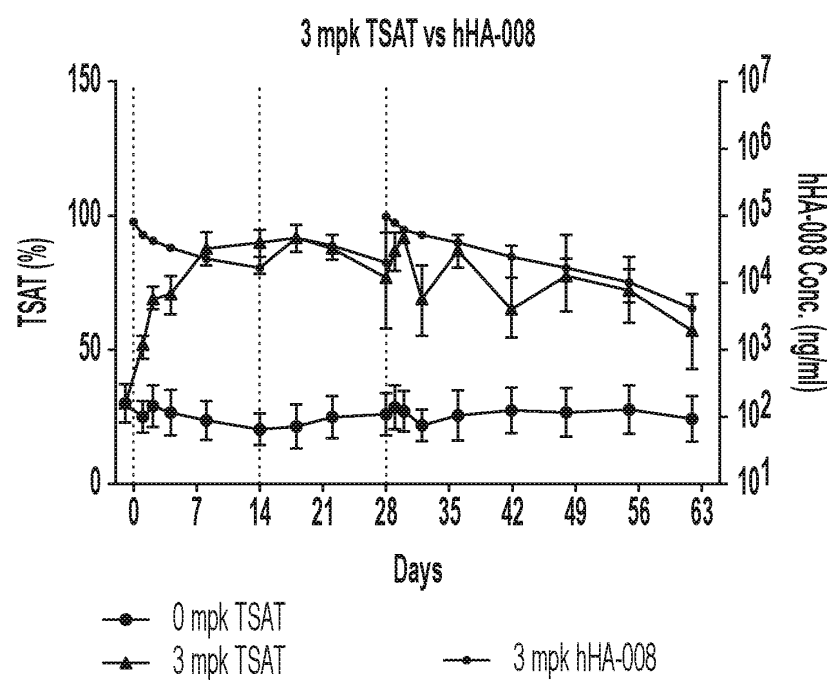


FIG. 8B

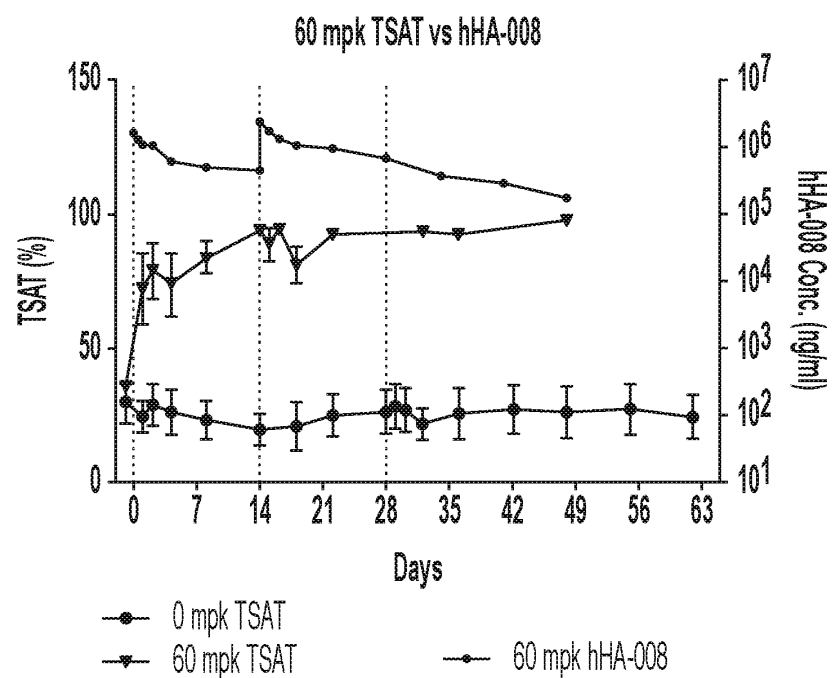


FIG. 8C

16/28

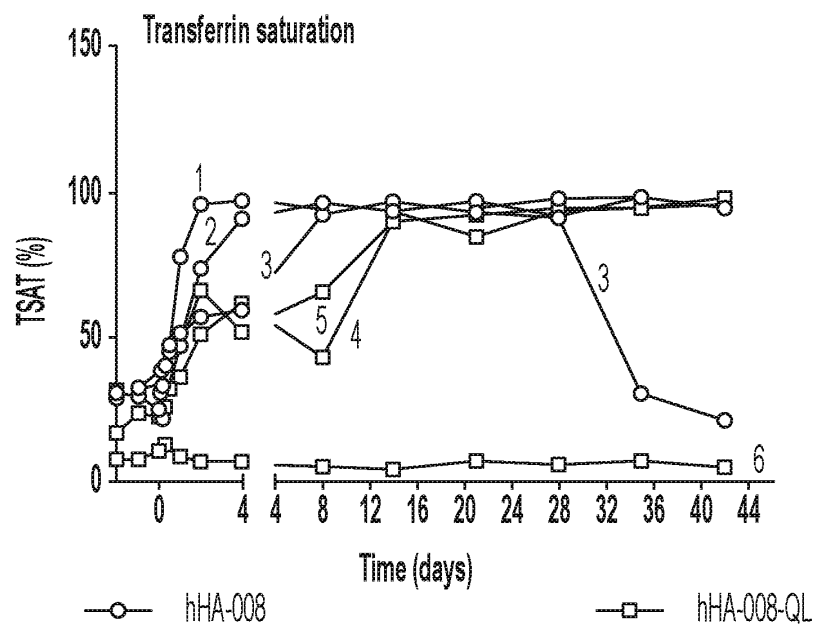


FIG. 9A

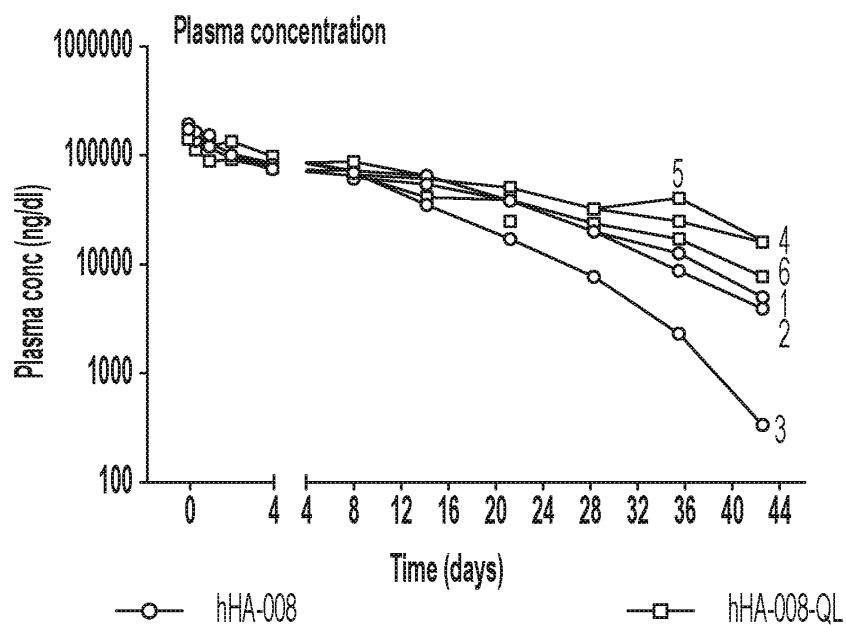


FIG. 9B

17/28

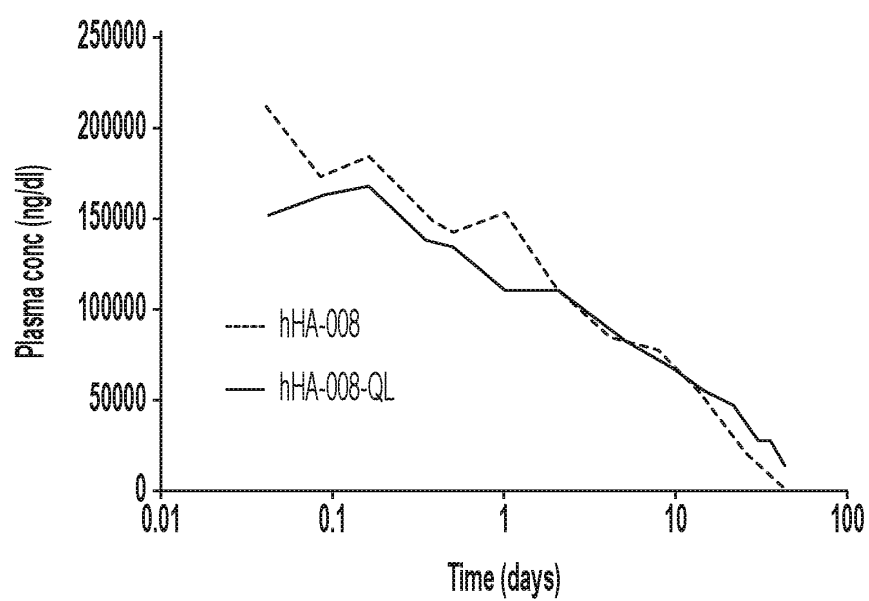


FIG. 9C

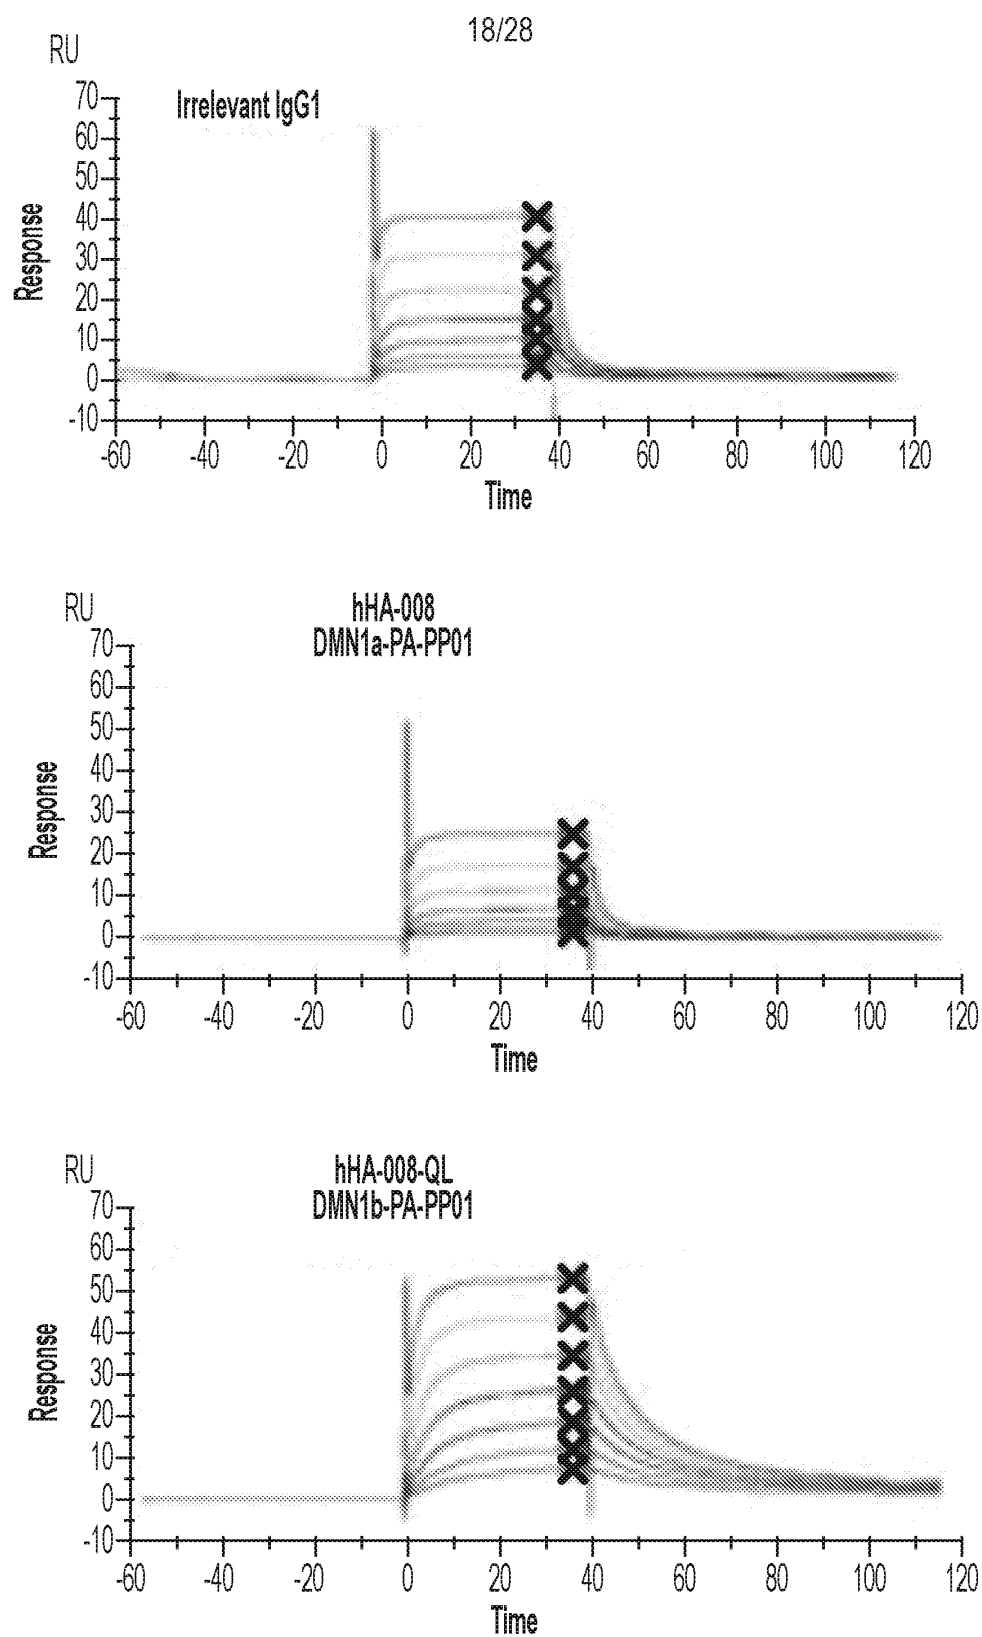
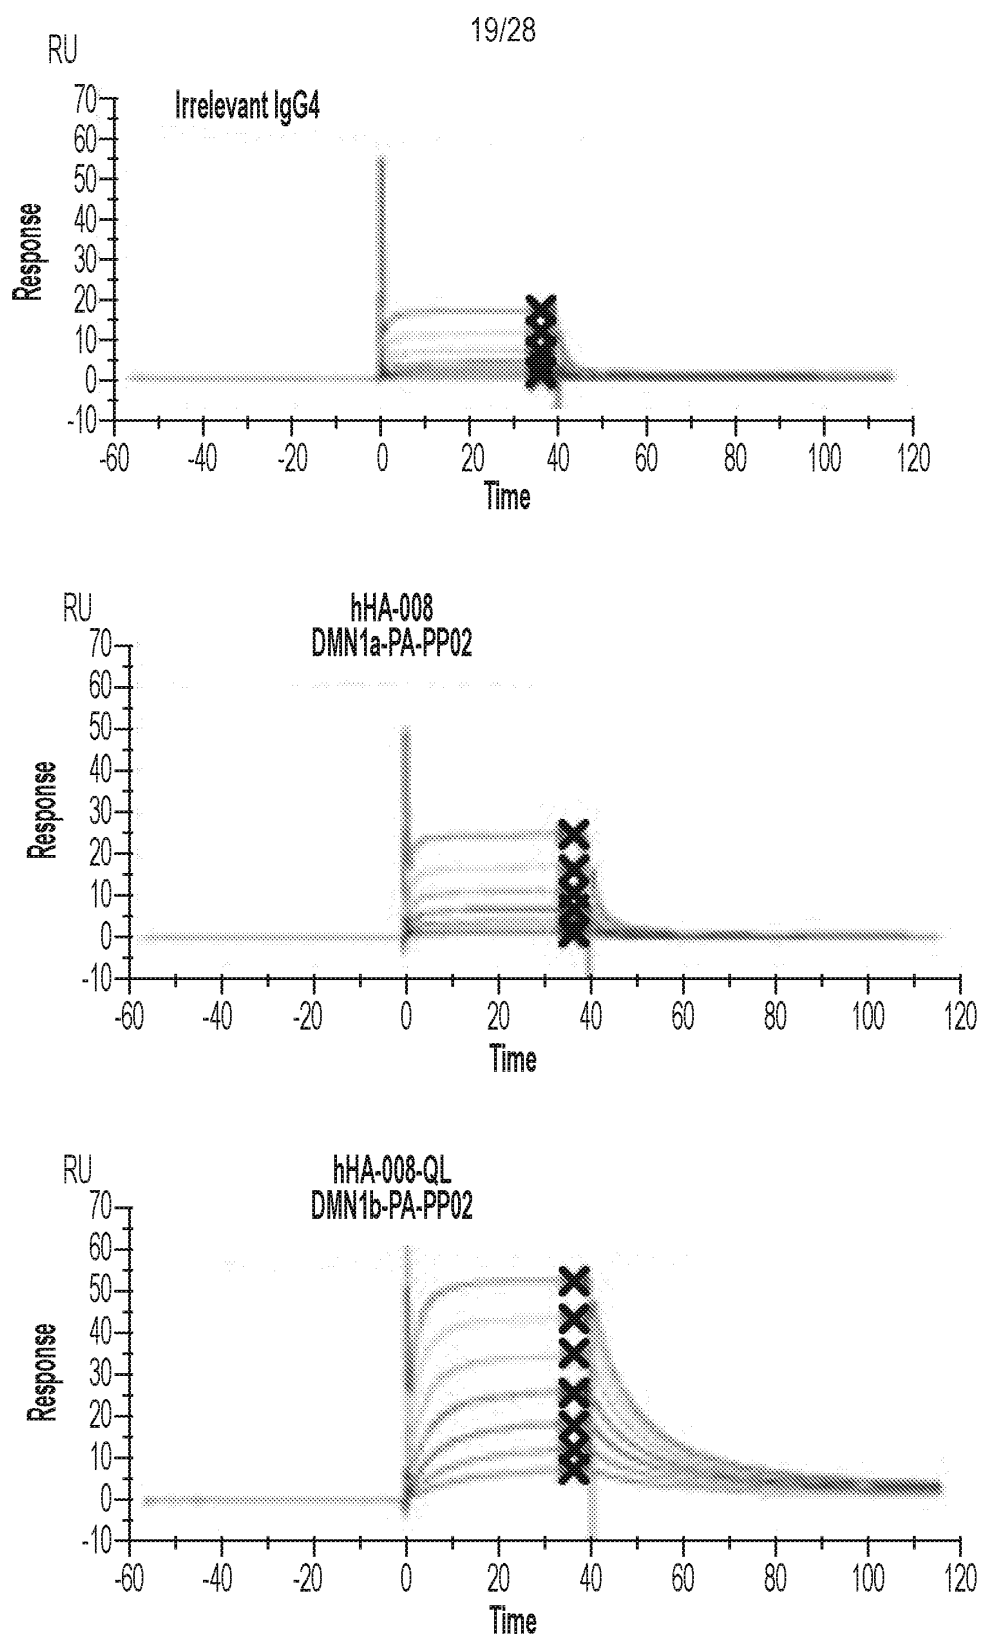


FIG. 10A



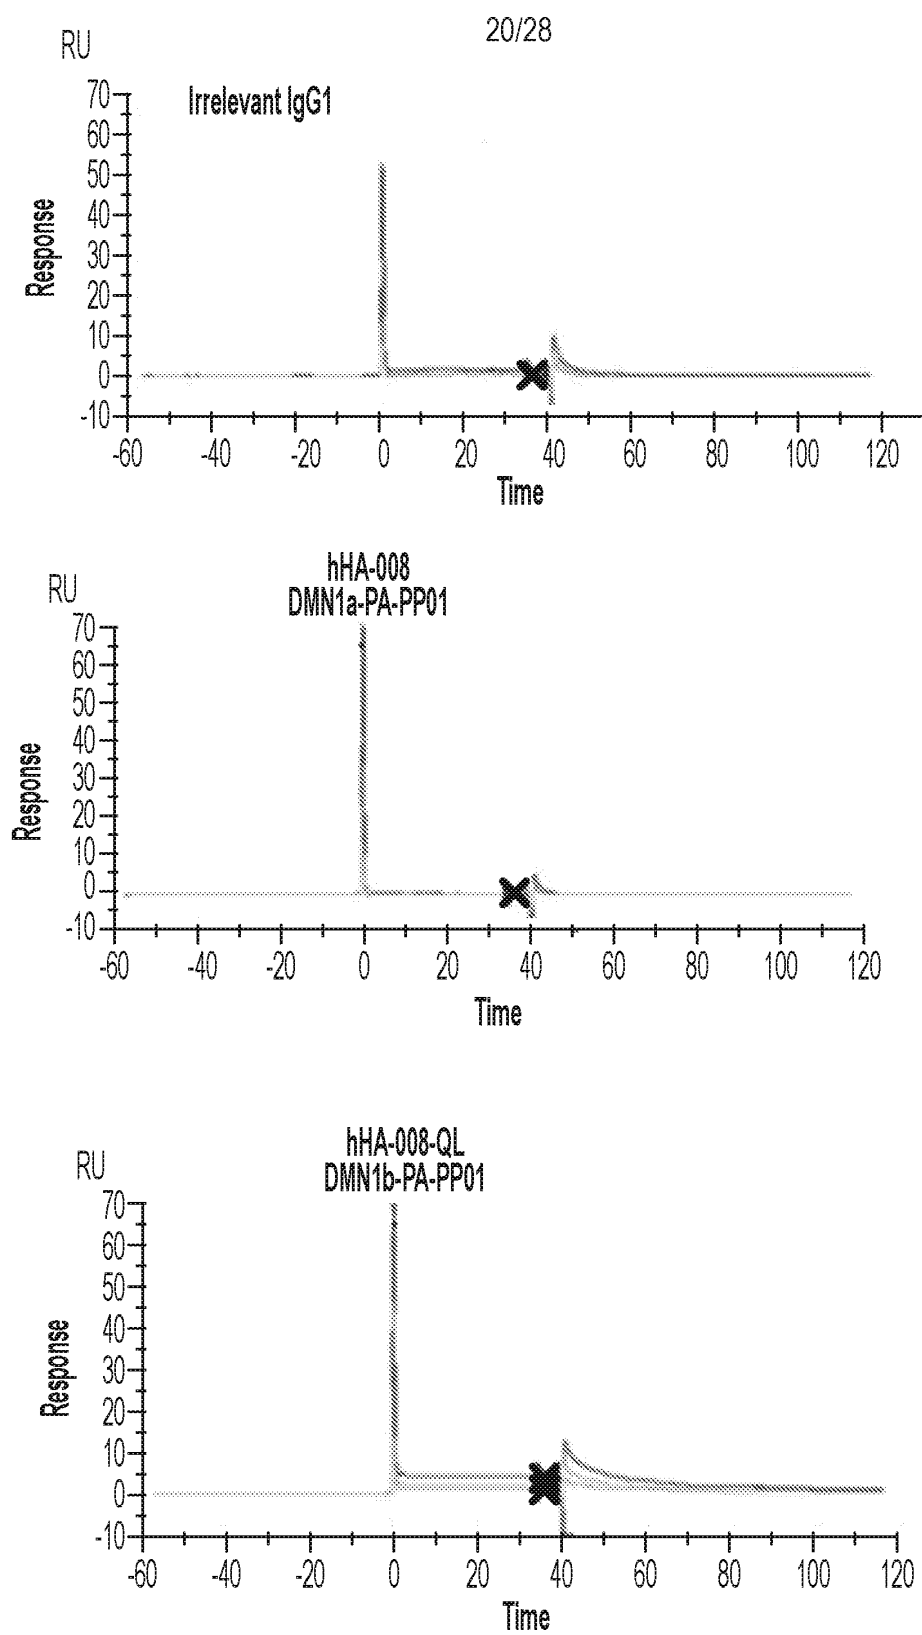


FIG. 10B

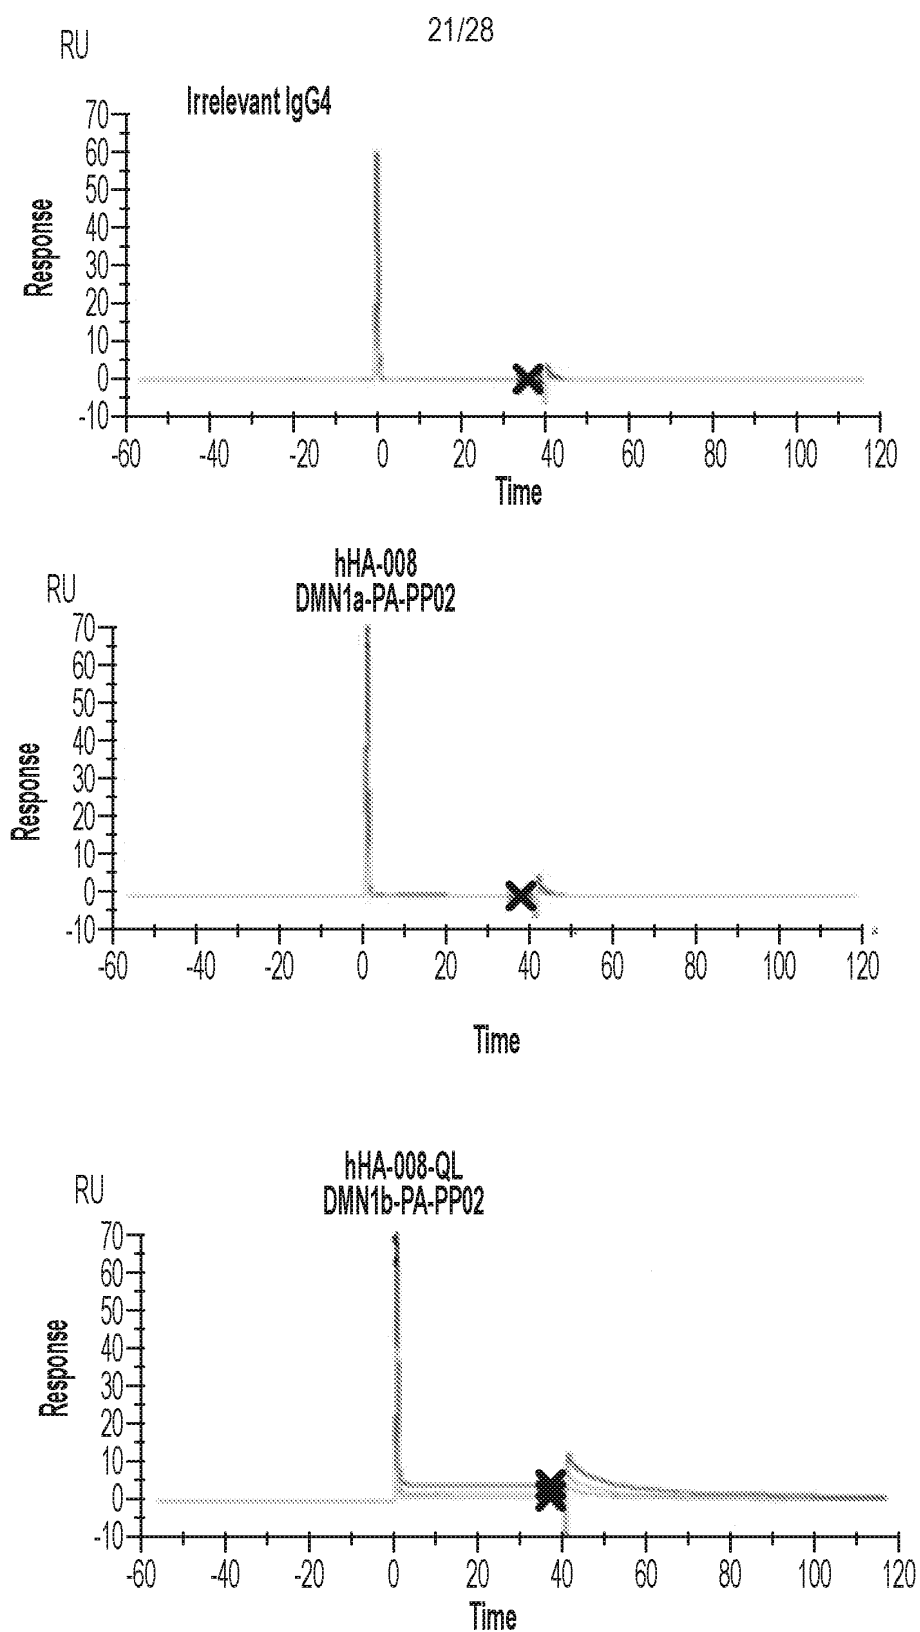


FIG. 10B
CONTINUED

22/28

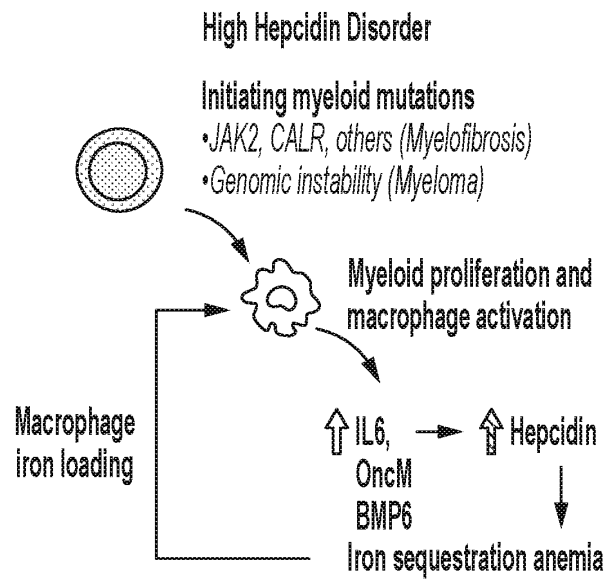


FIG. 11

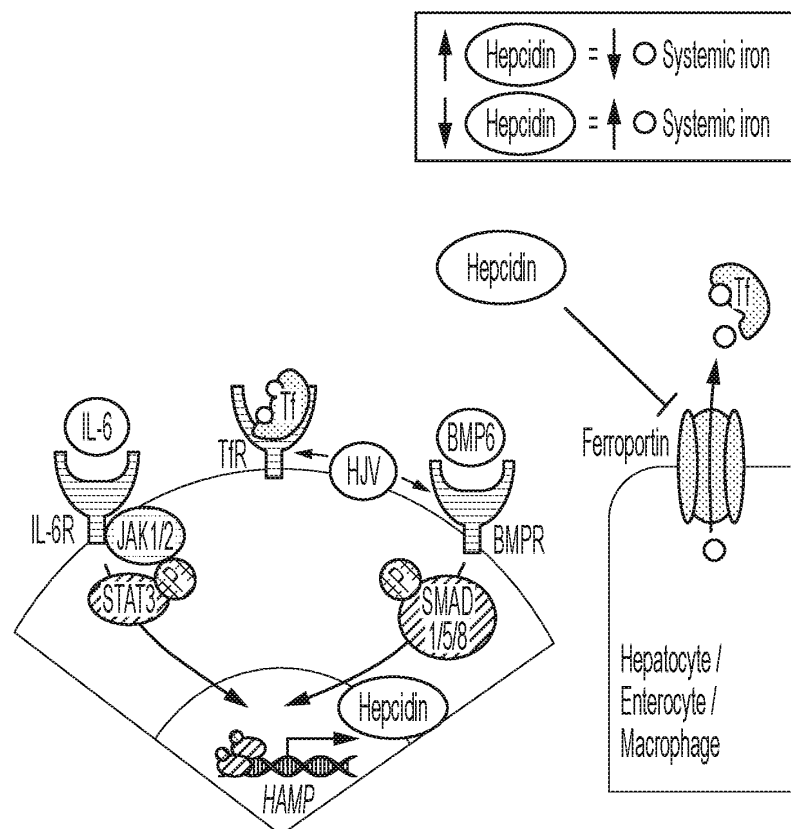


FIG. 12

23/28

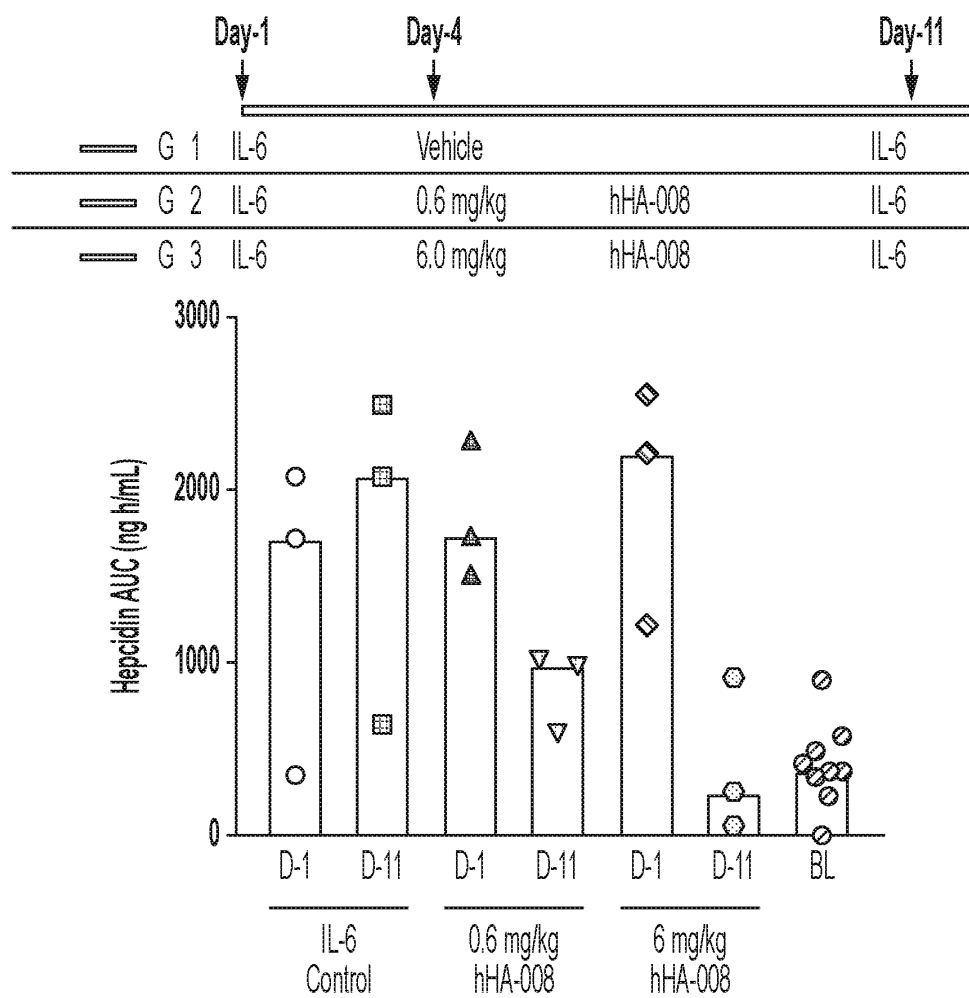


FIG. 13

24/28

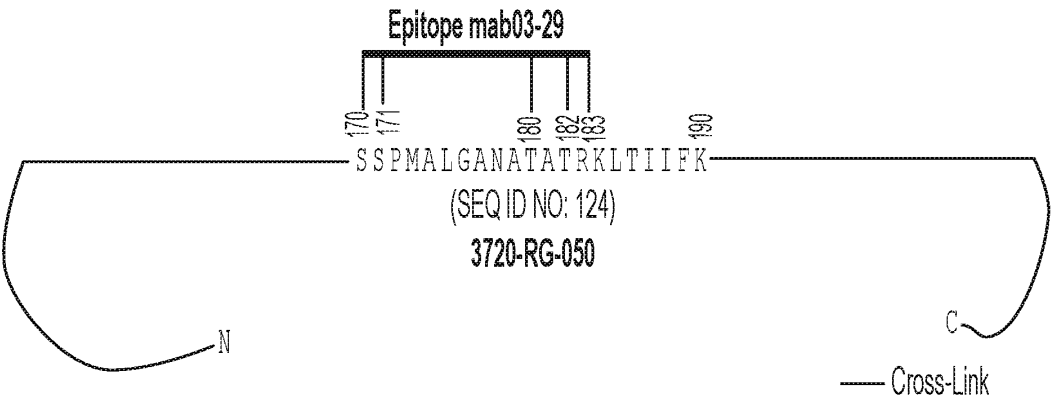


FIG. 14



FIG. 15A




FIG. 15B



FIG. 15C



FIG. 15D



FIG. 15E




FIG. 15F




FIG. 15G



FIG. 15H



FIG. 15I



FIG. 15J

25/28

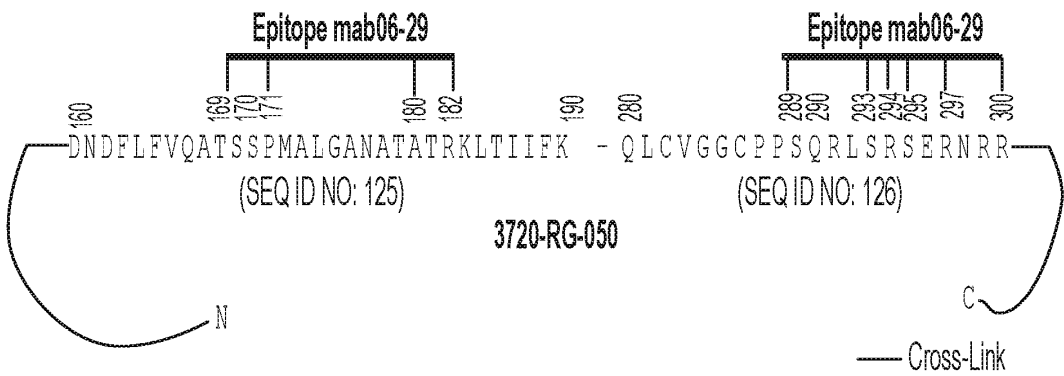


FIG. 16



FIG. 17A




FIG. 17B



FIG. 17C



FIG. 17D



FIG. 17E



FIG. 17F




FIG. 17G



FIG. 17H



FIG. 17I



FIG. 17J

26/28

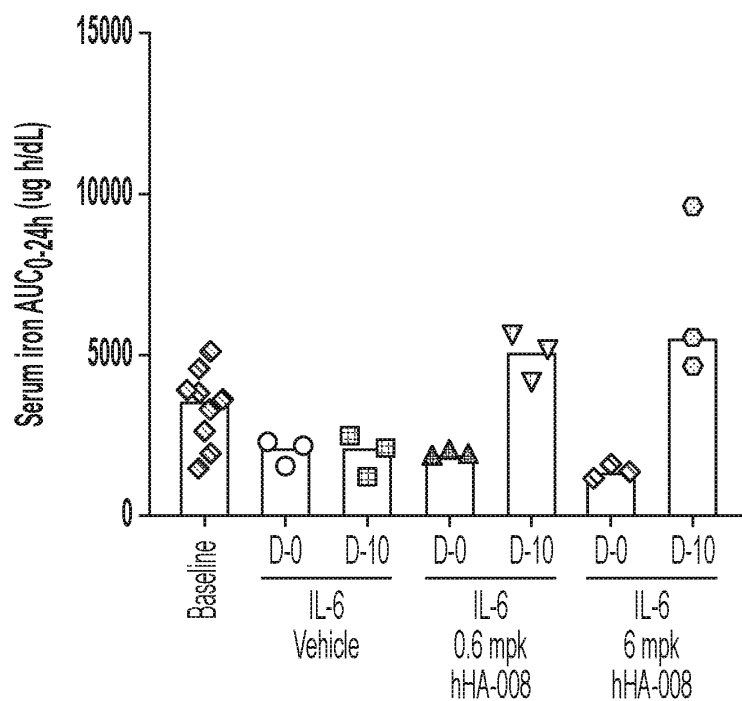


FIG. 18

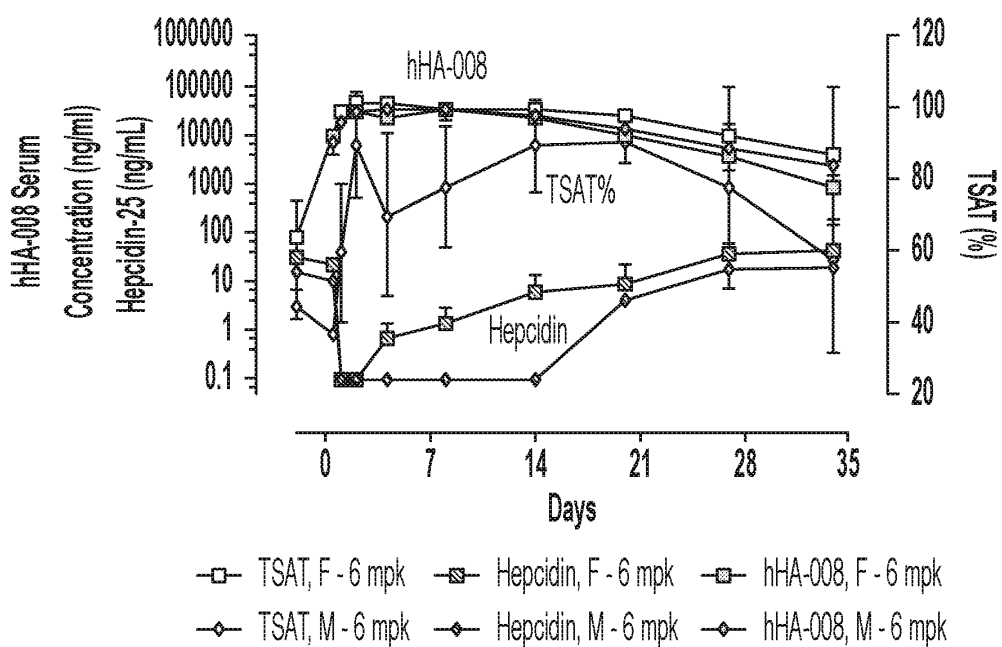


FIG. 19

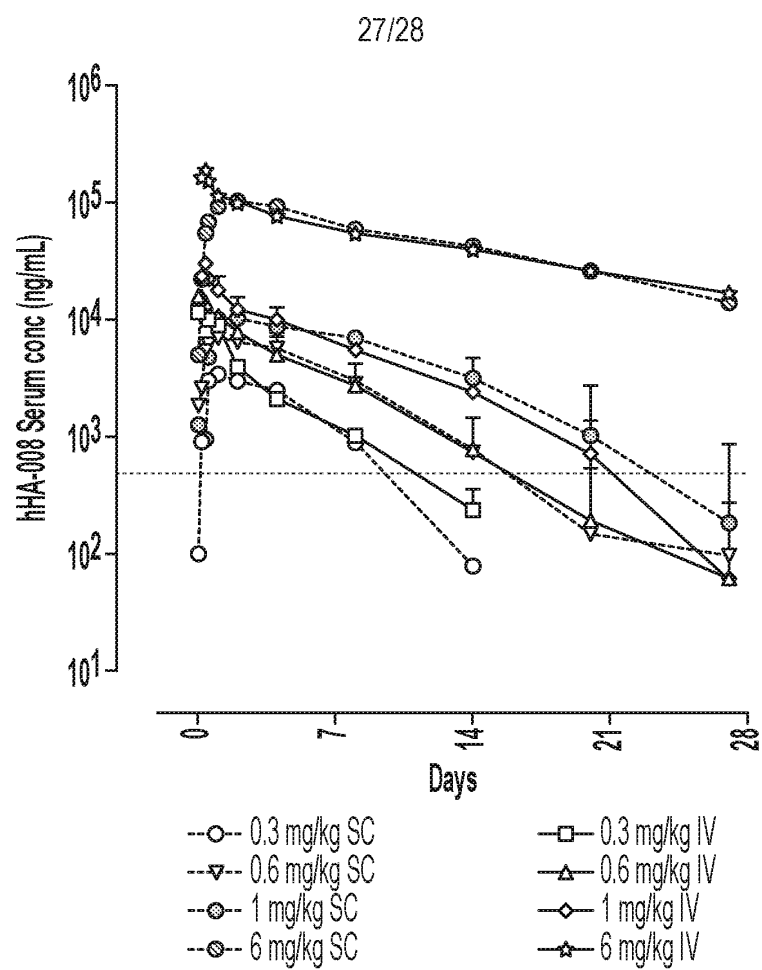


FIG. 20A

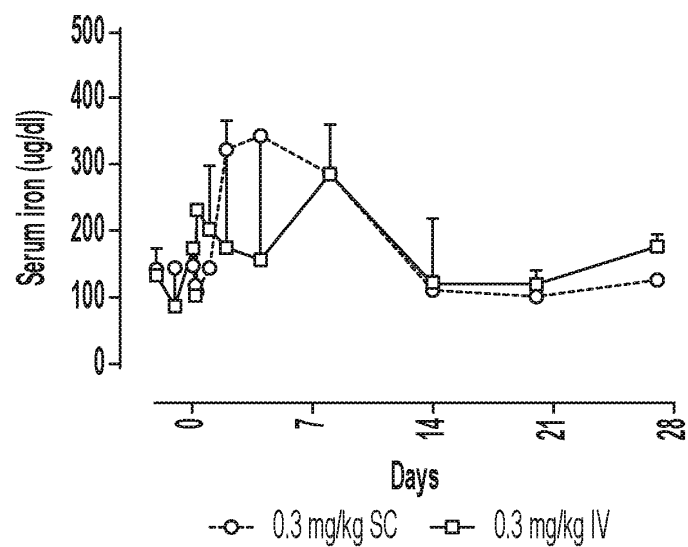


FIG. 20B

28/28

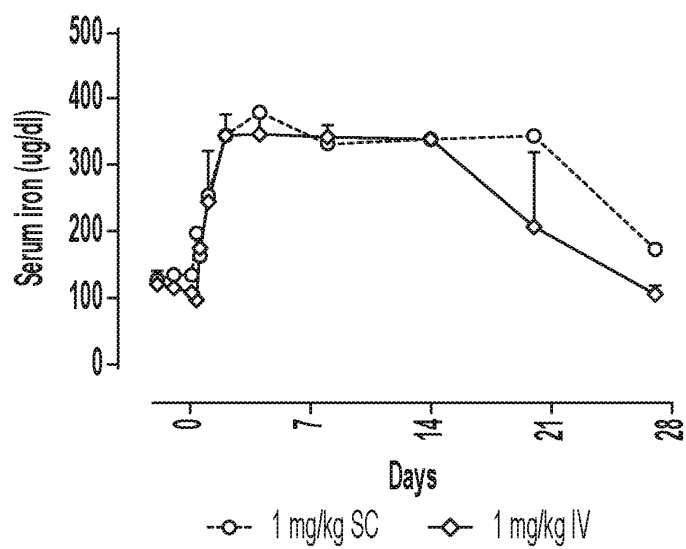


FIG. 20C

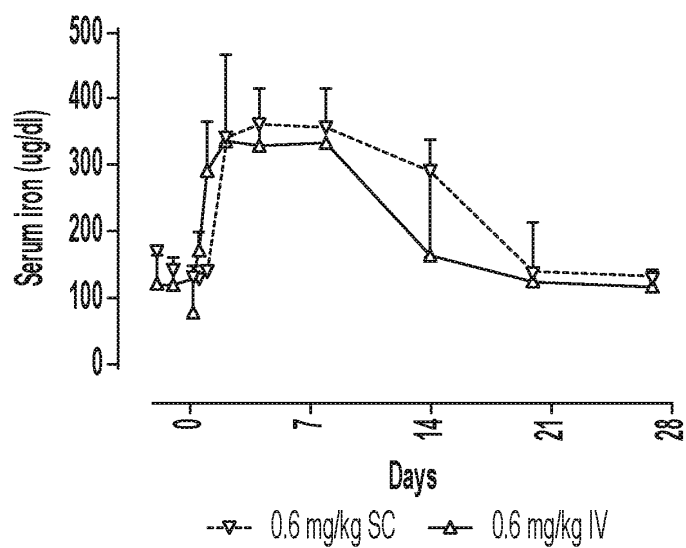


FIG. 20D