Fig. 1

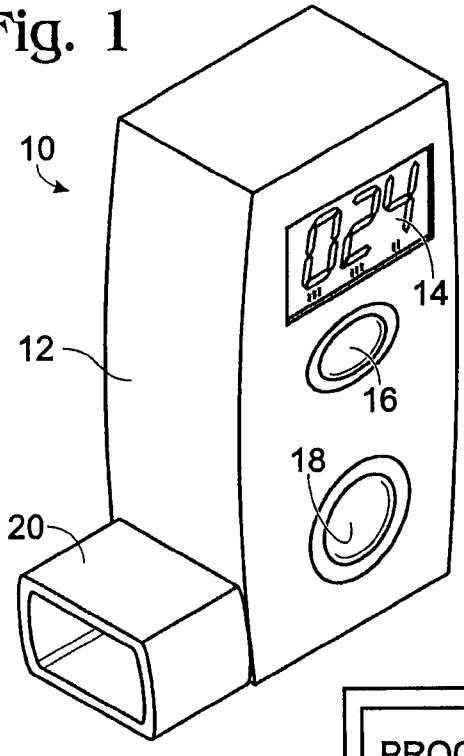


Fig. 2

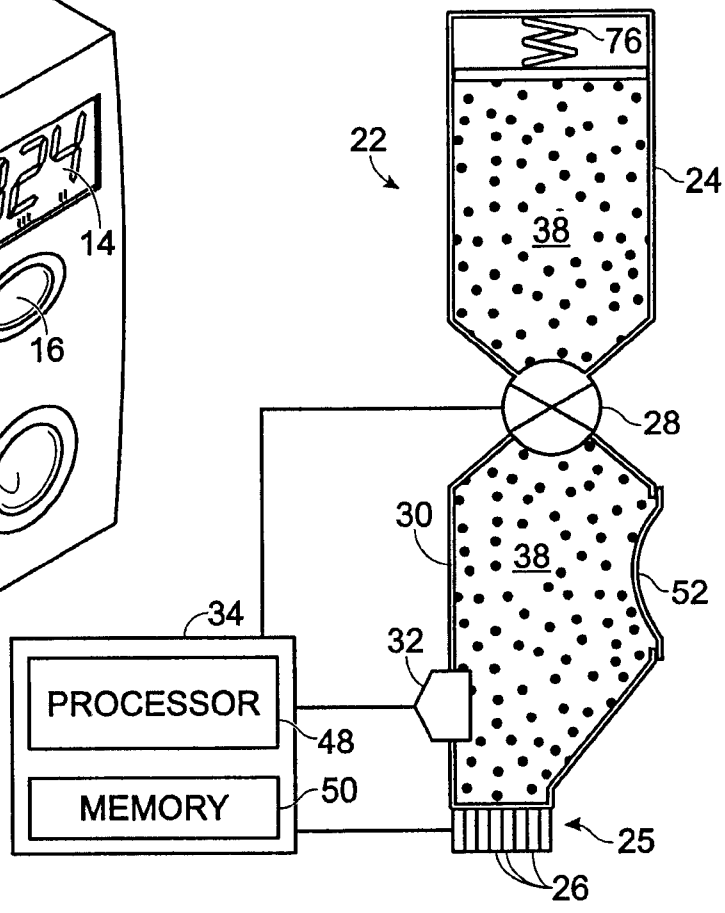


Fig. 3

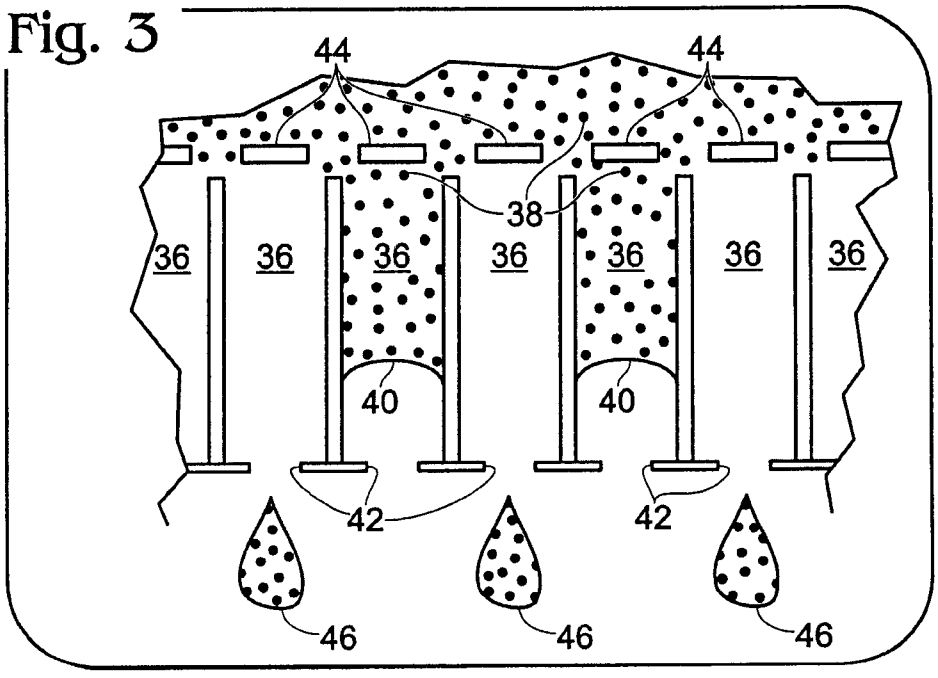


Fig. 4A

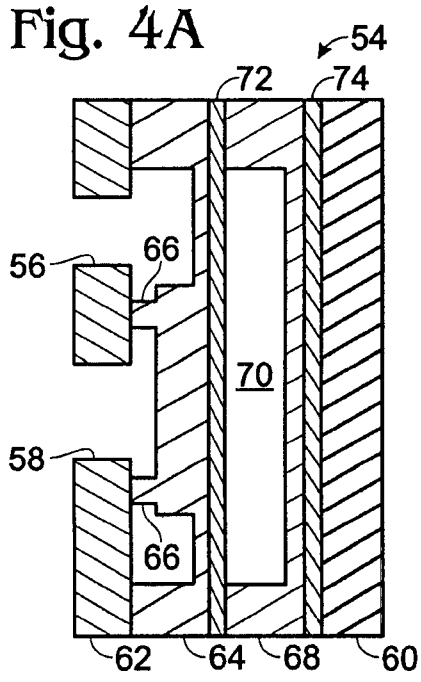


Fig. 4B

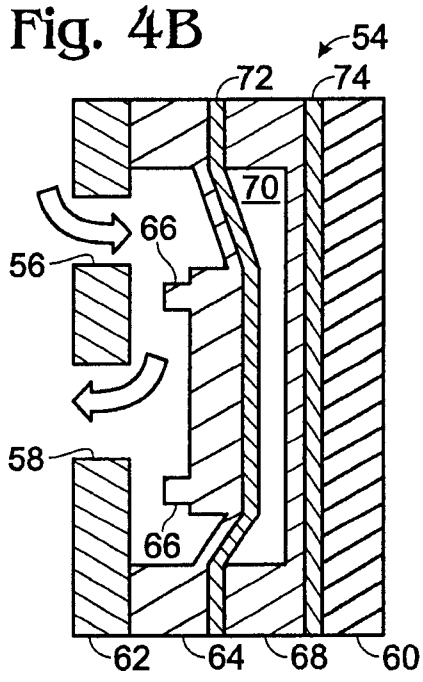


Fig. 5

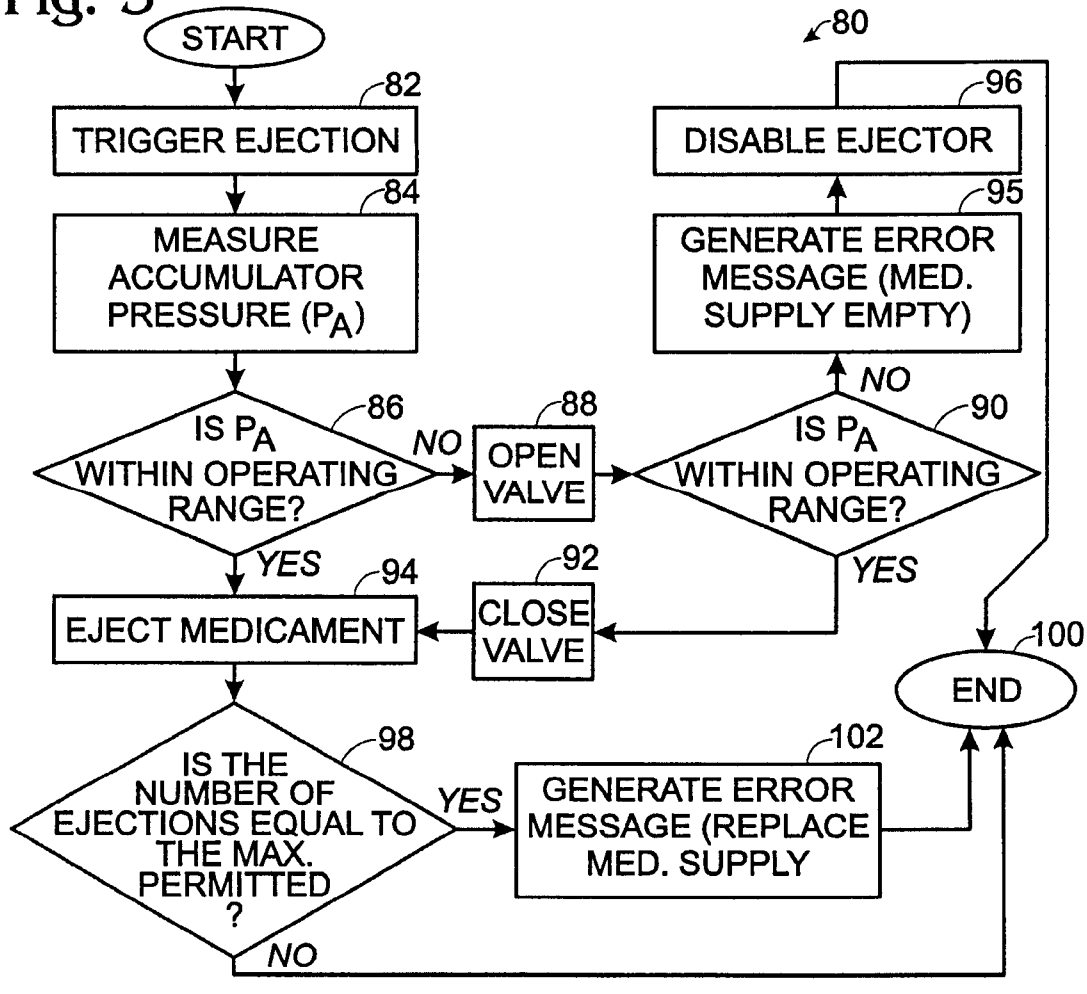
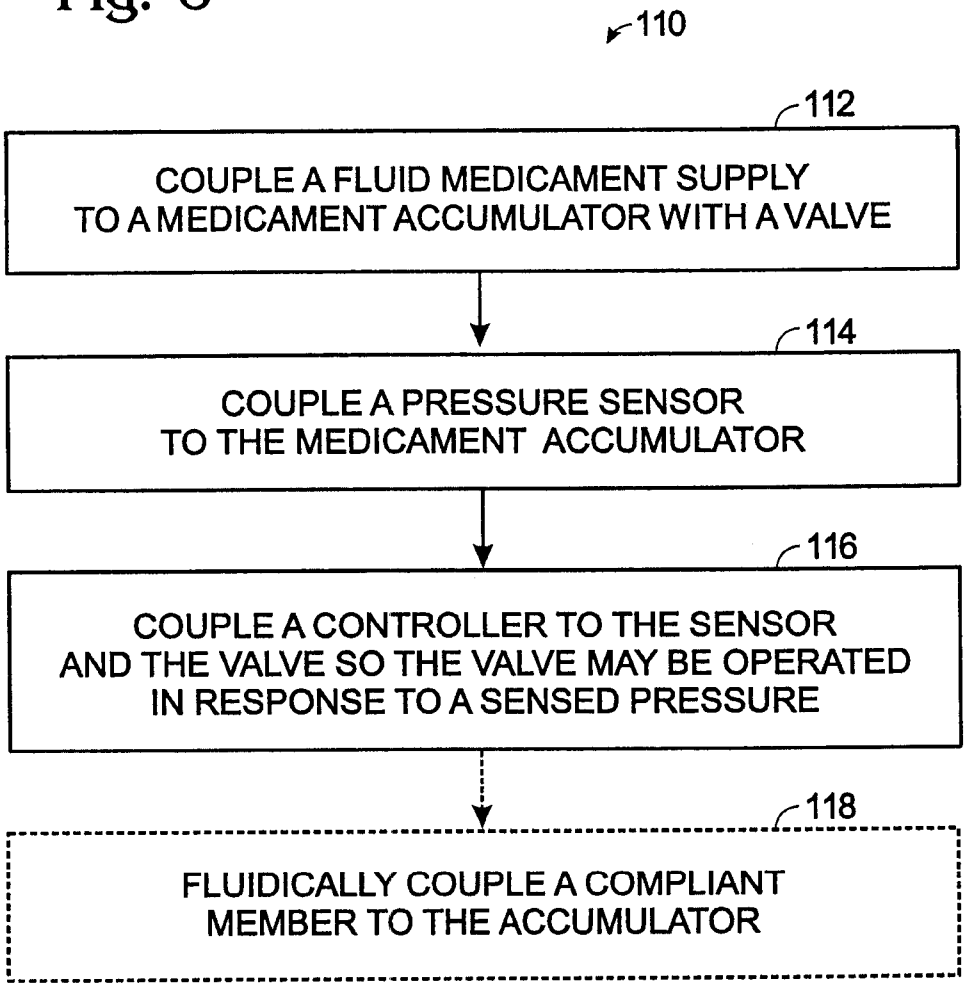


Fig. 6


110
112
COUPLE A FLUID MEDICAMENT SUPPLY TO A MEDICAMENT ACCUMULATOR WITH A VALVE
114
COUPLE A PRESSURE SENSOR TO THE MEDICAMENT ACCUMULATOR
116
COUPLE A CONTROLLER TO THE SENSOR AND THE VALVE SO THE VALVE MAY BE OPERATED IN RESPONSE TO A SENSED PRESSURE
118
FLUIDICALLY COUPLE A COMPLIANT MEMBER TO THE ACCUMULATOR