

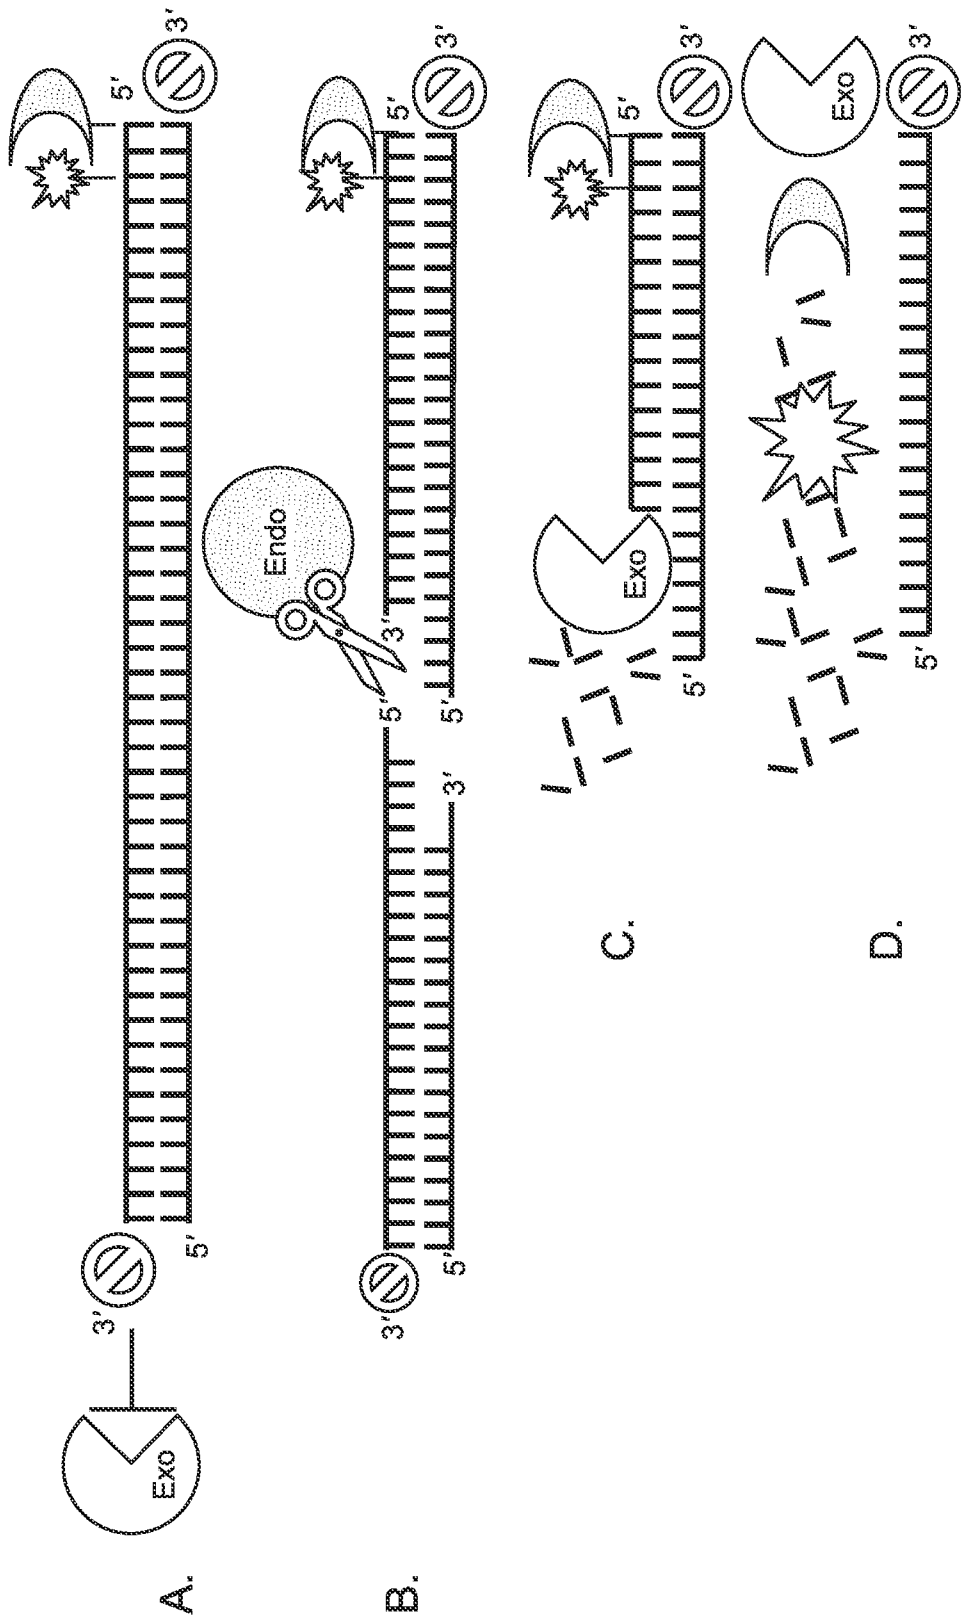


FIG. 1

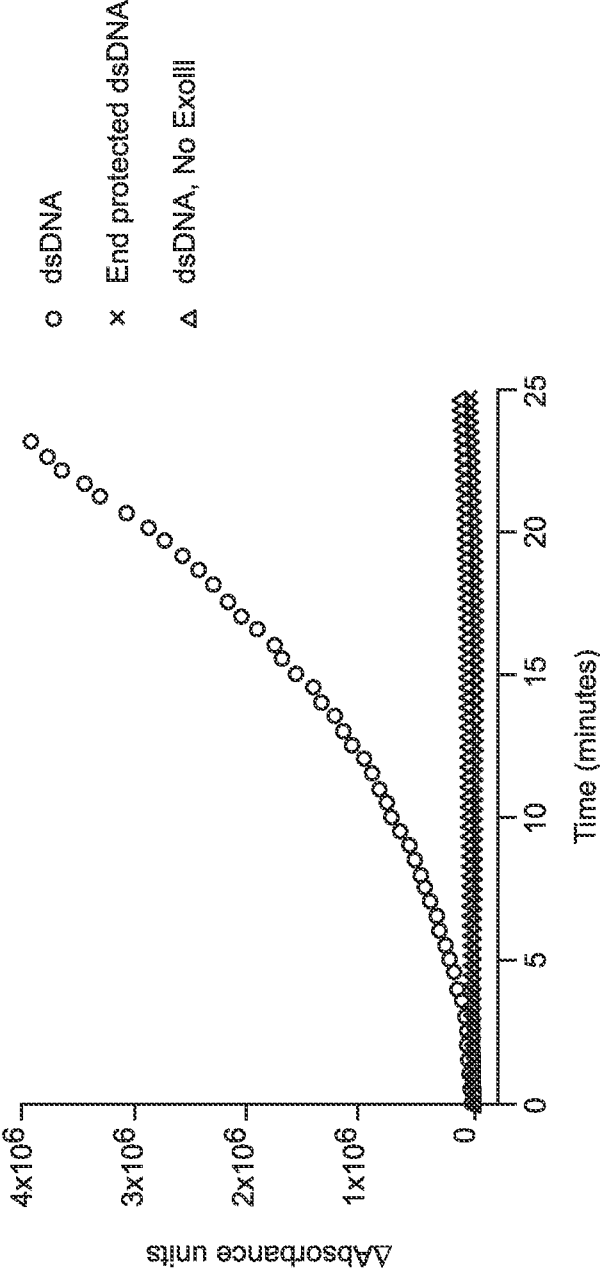


FIG. 2



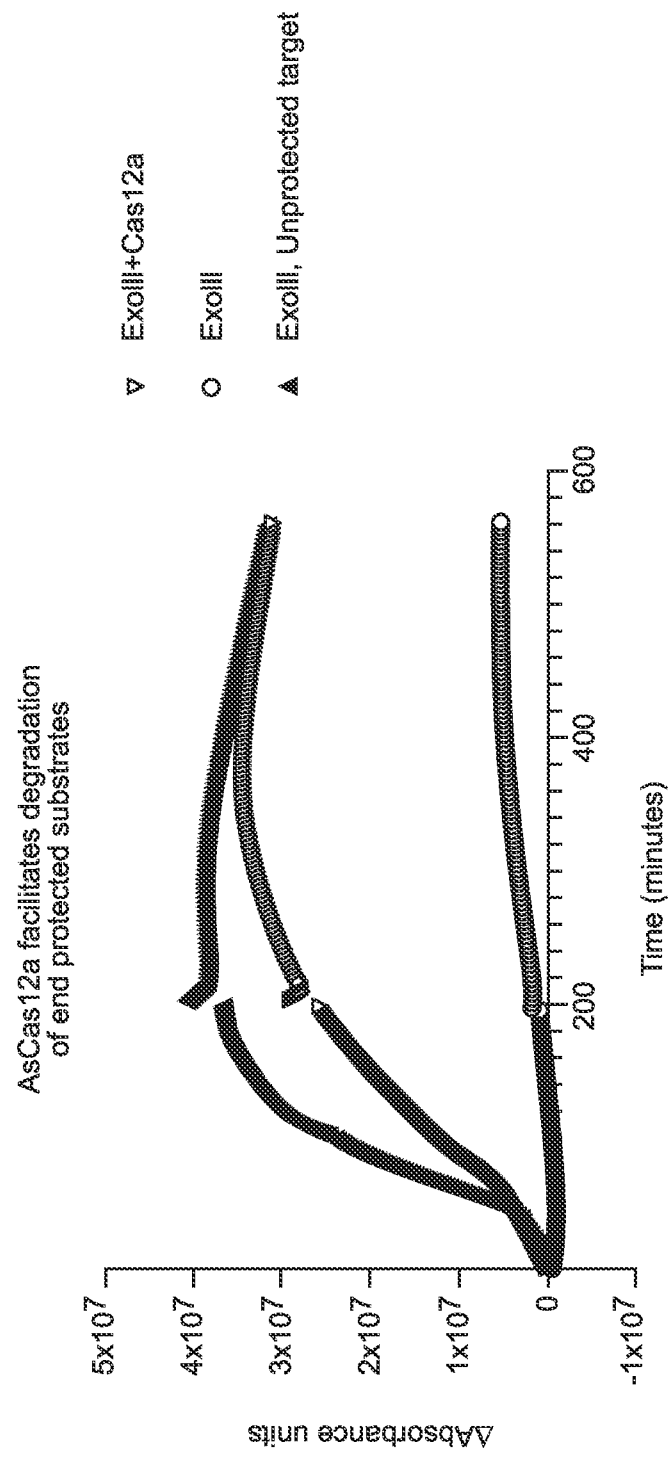


FIG. 3

4/16

**FIG. 4**

5/16

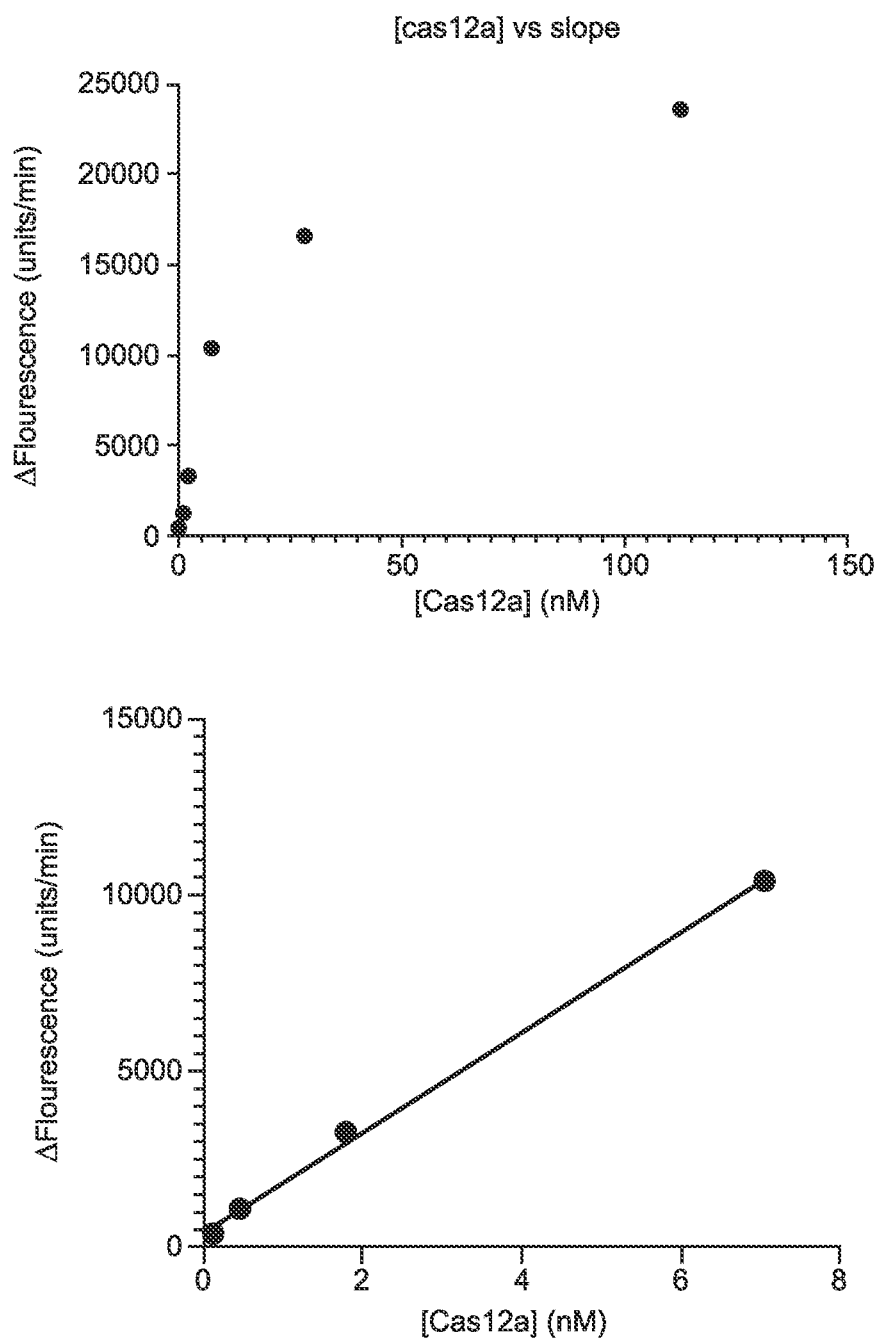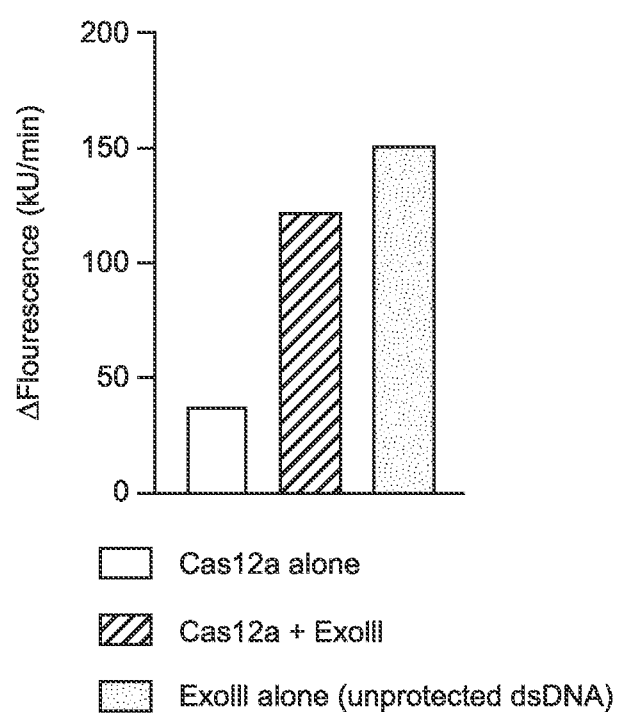

Assays performed in NEB buffer 1 pH 7.0

FIG. 5

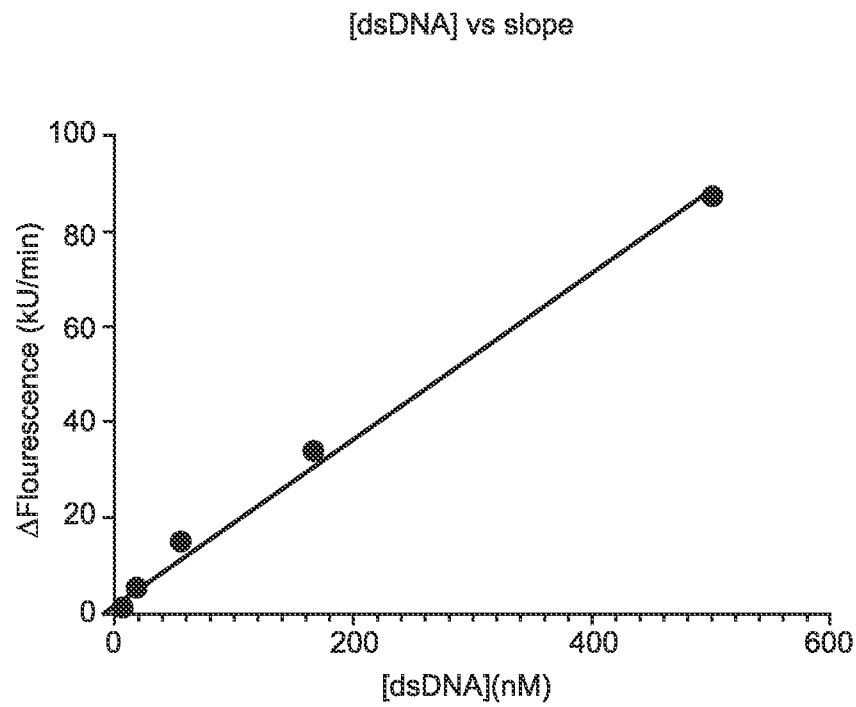


FIG. 6

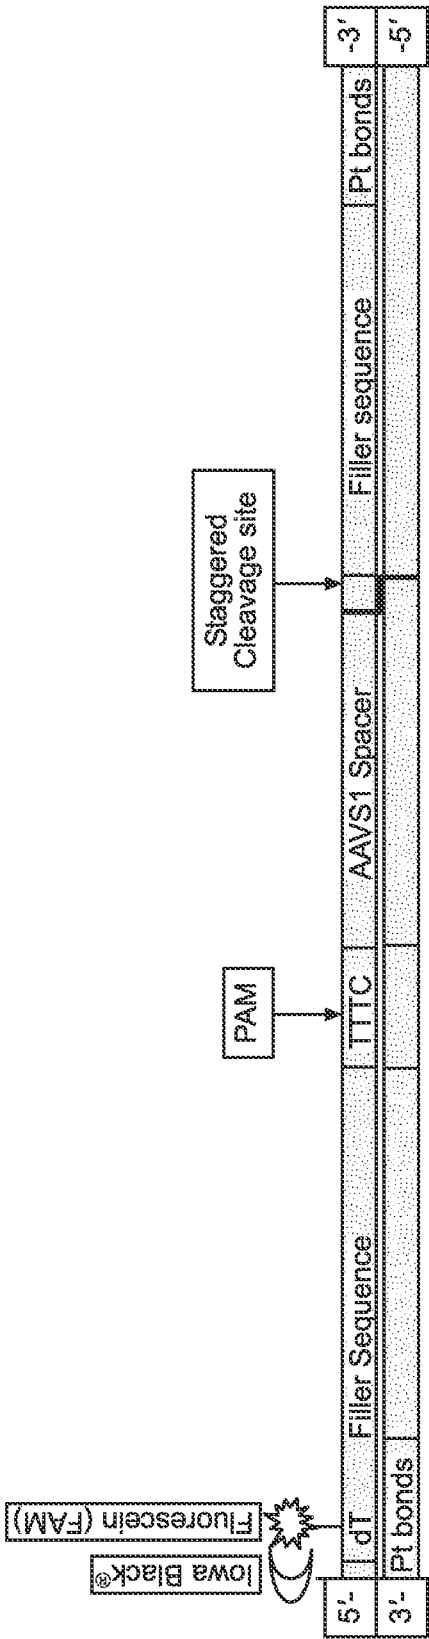


FIG. 7

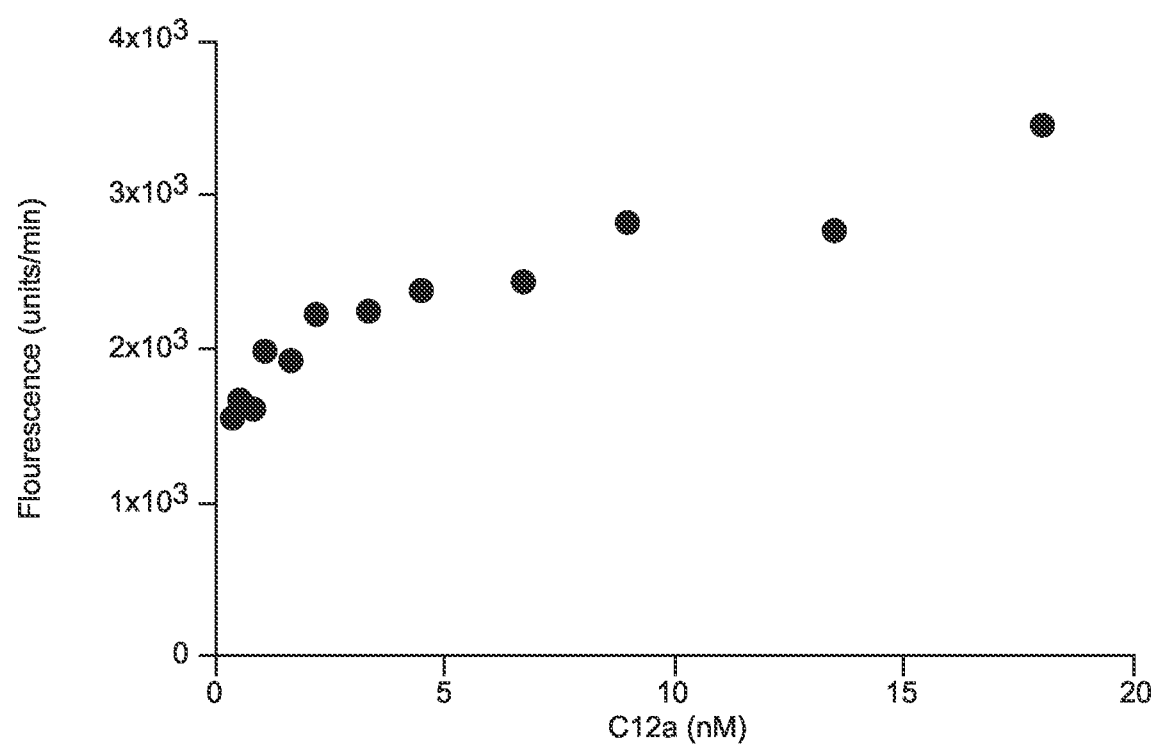
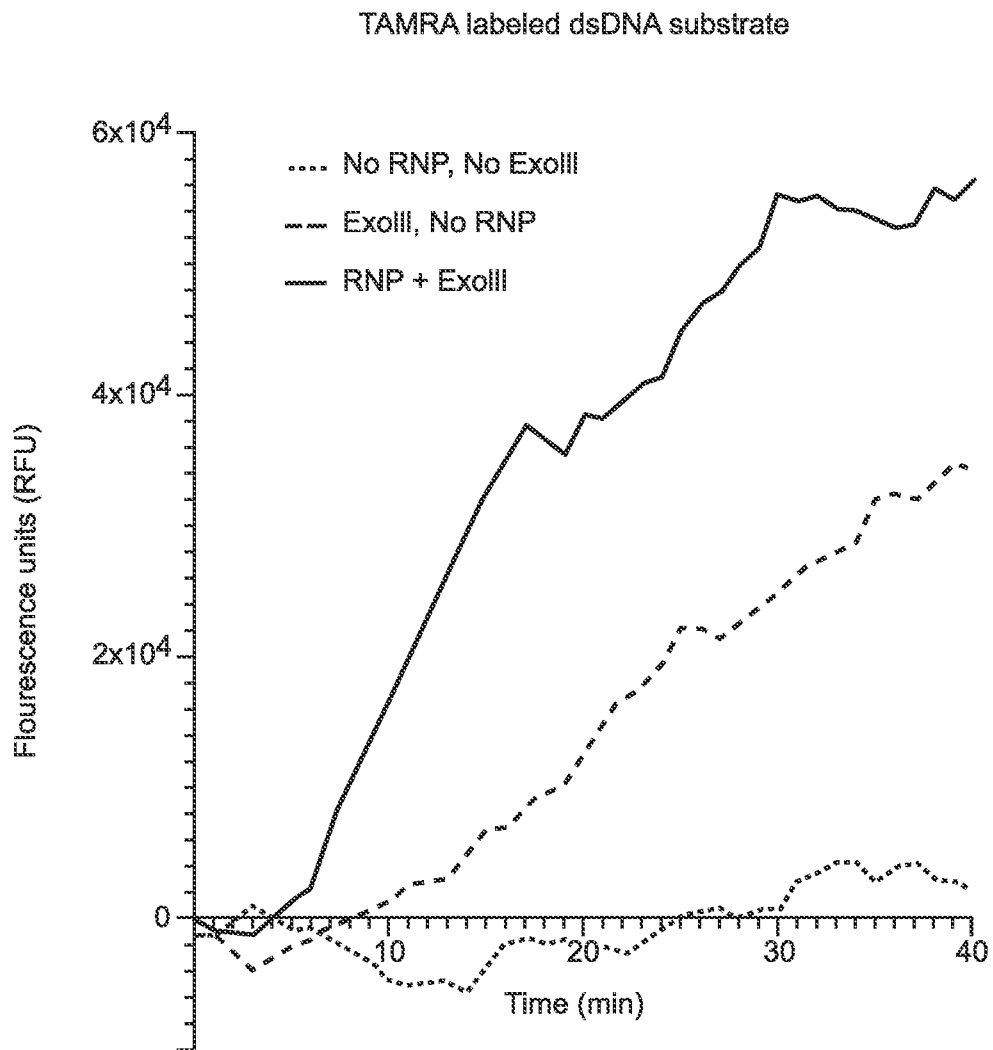


FIG. 8

9/16

**FIG. 9**

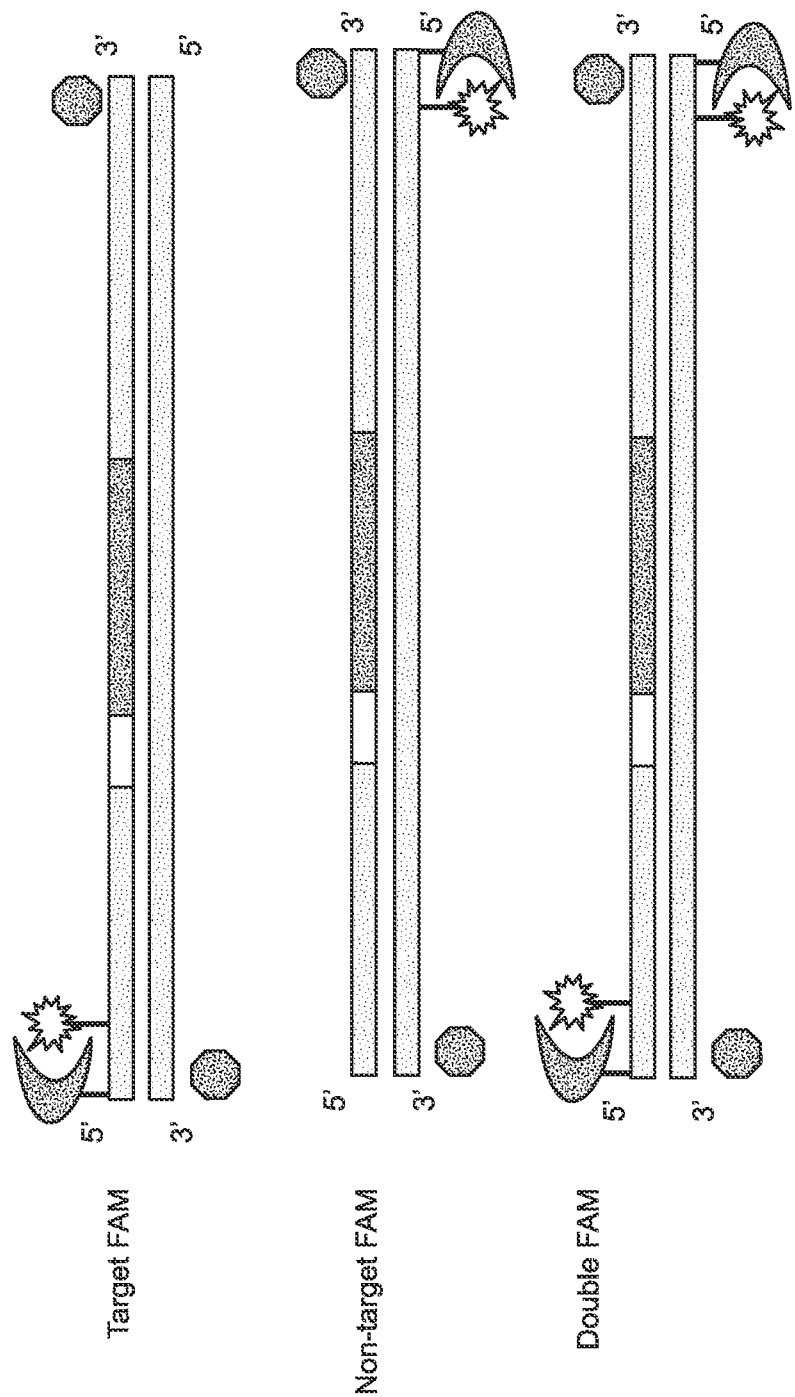


FIG. 10

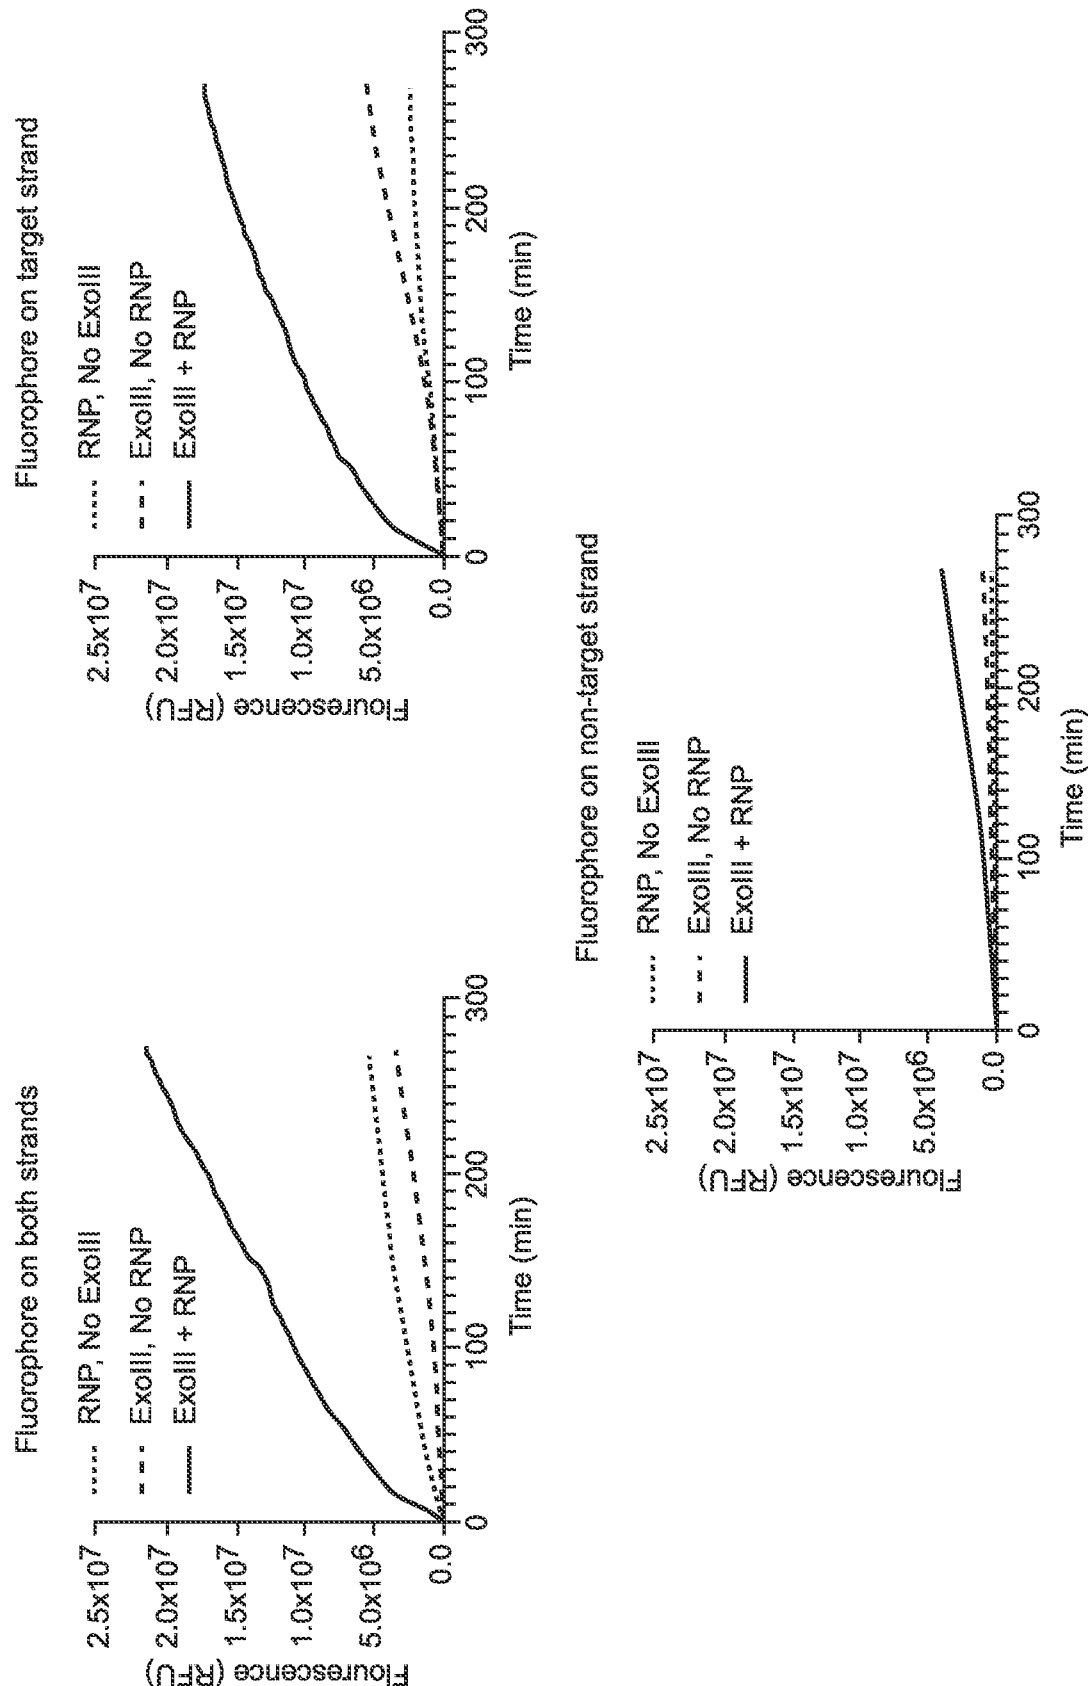


FIG. 11

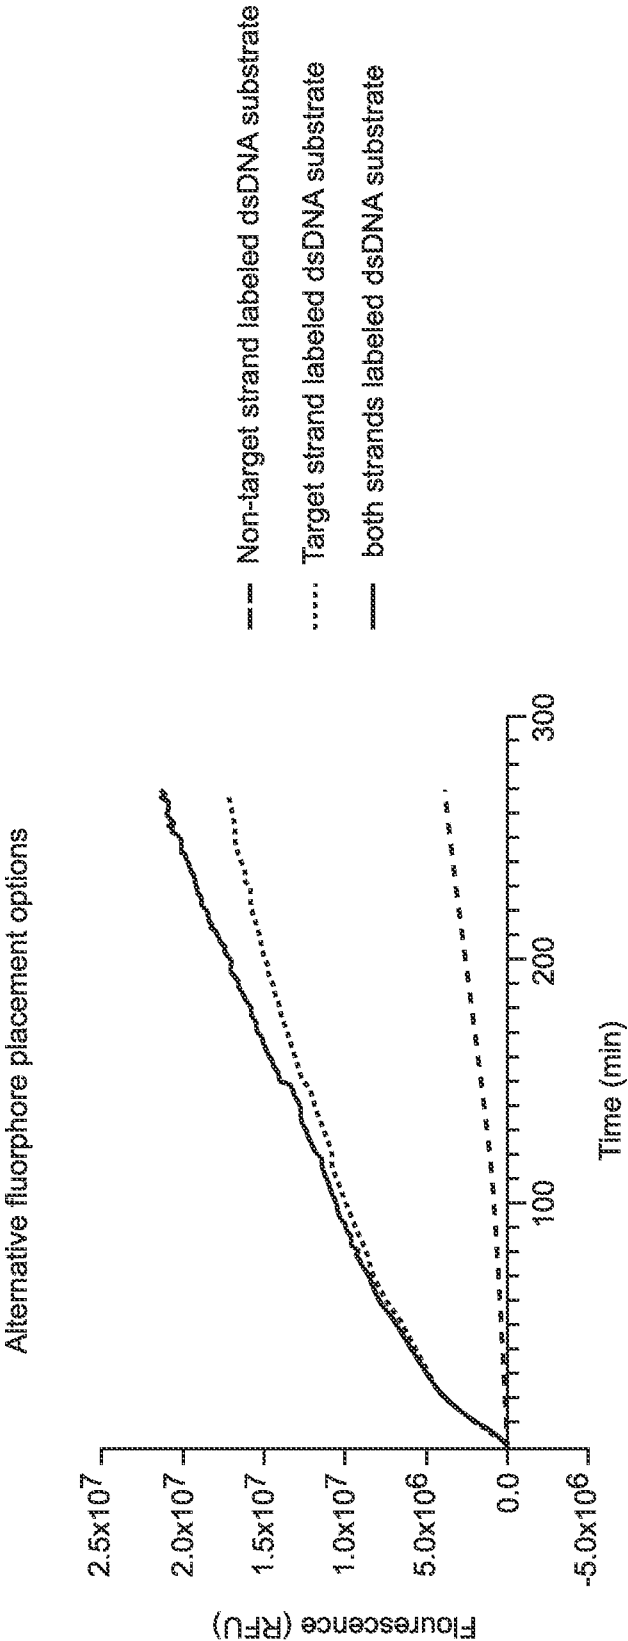


FIG. 12

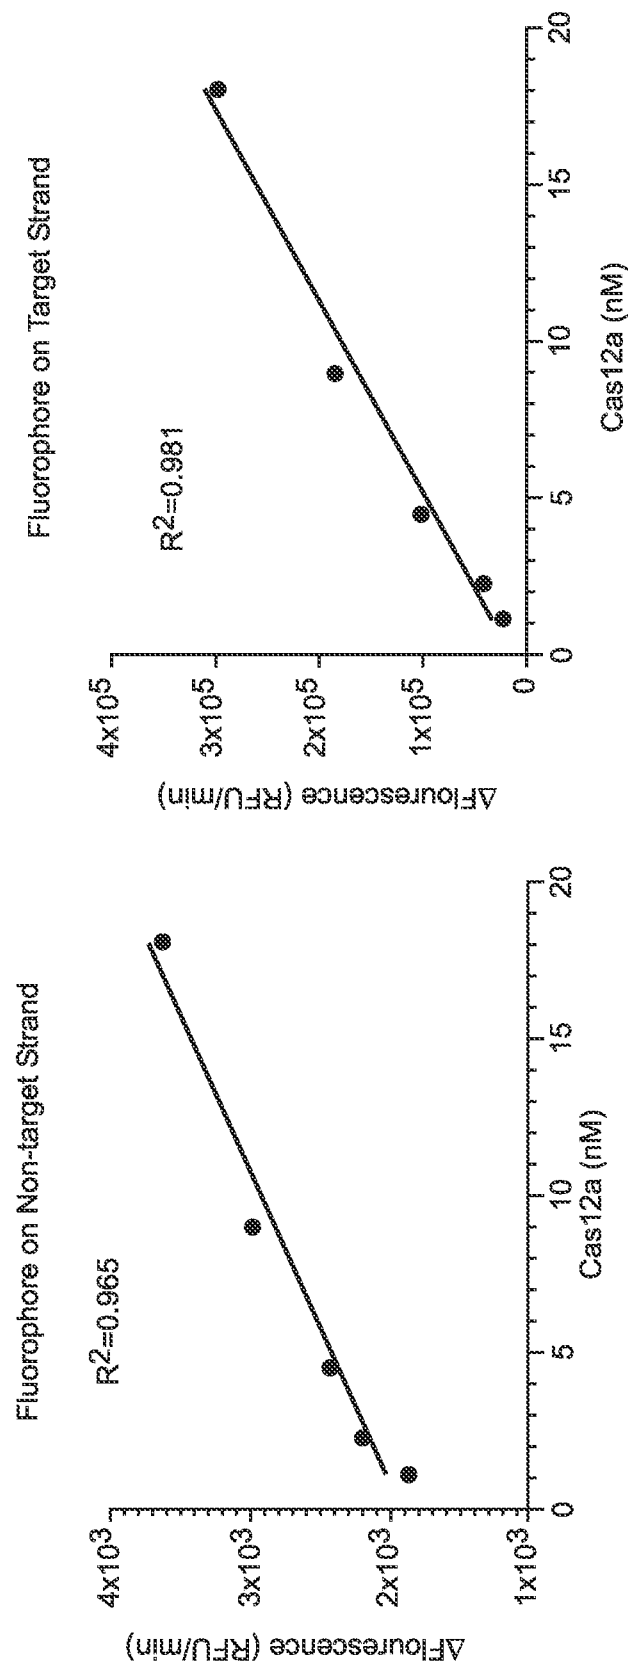


FIG. 13

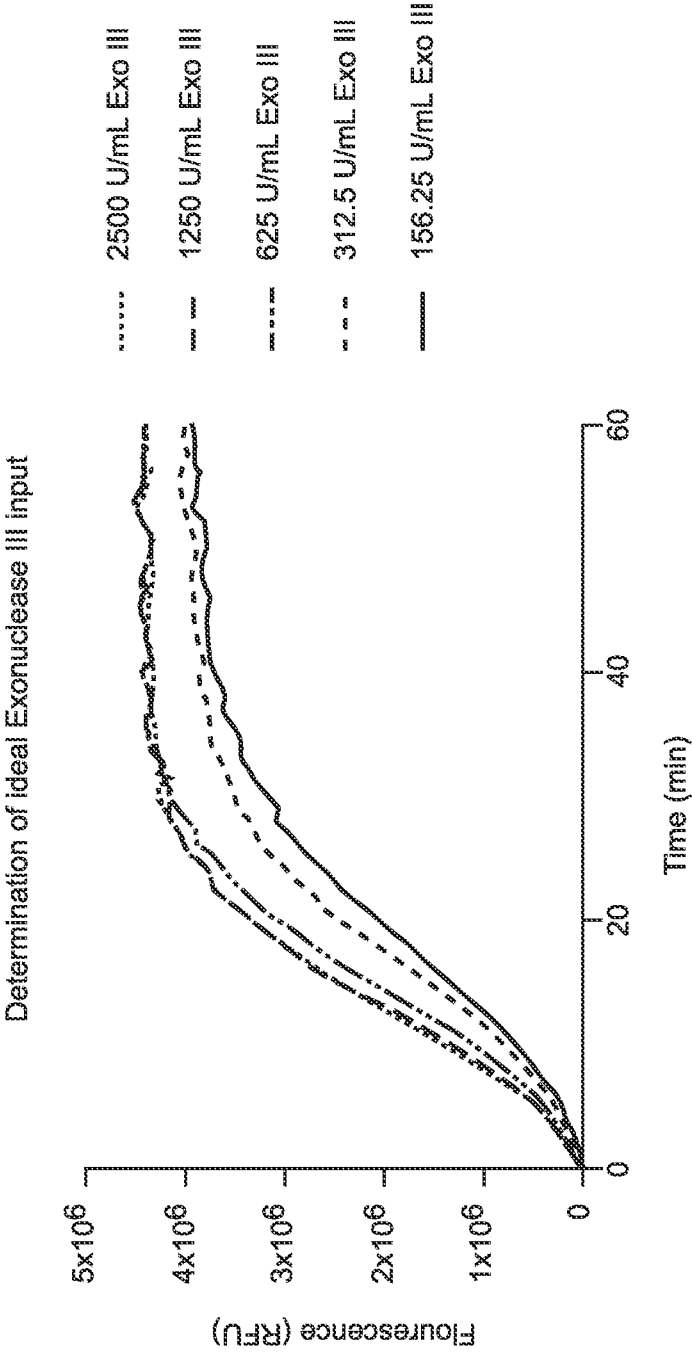


FIG. 14

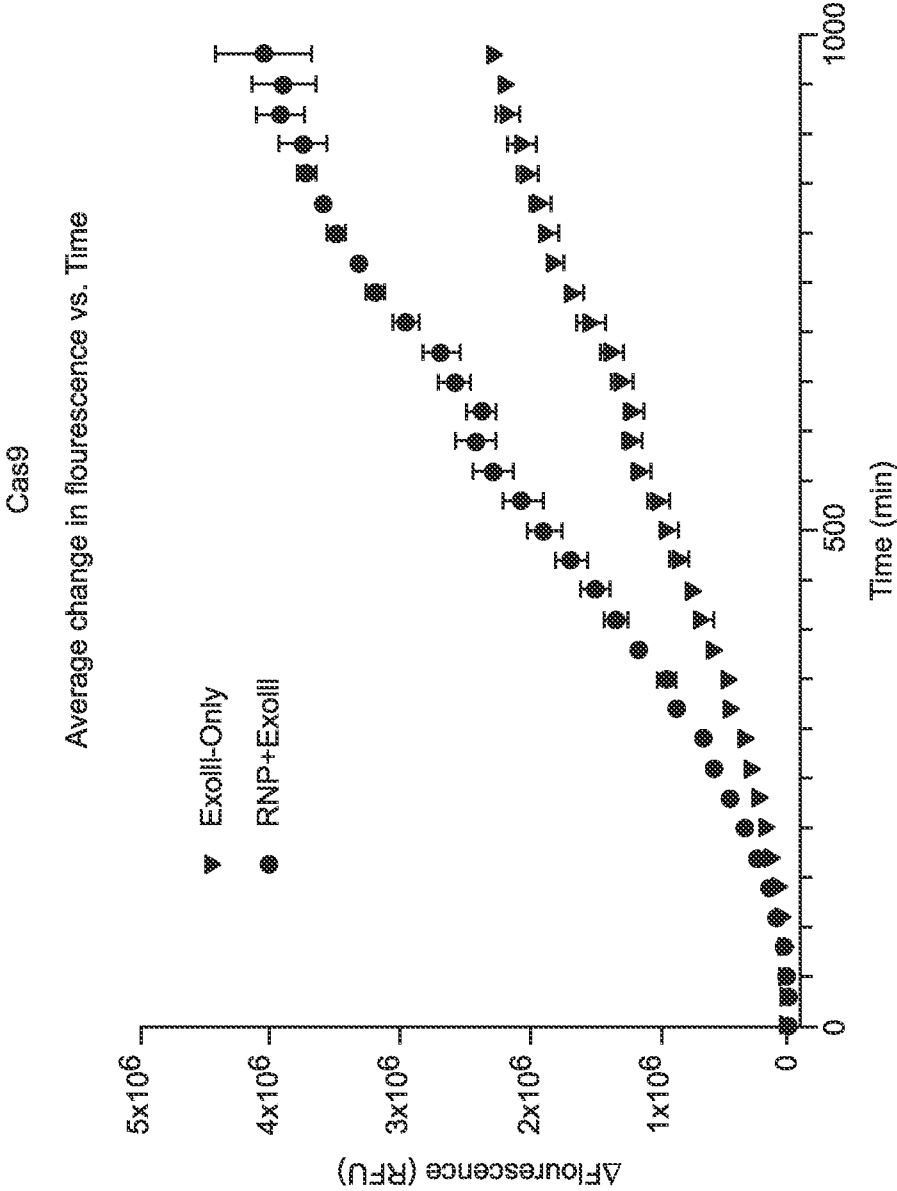


FIG. 15

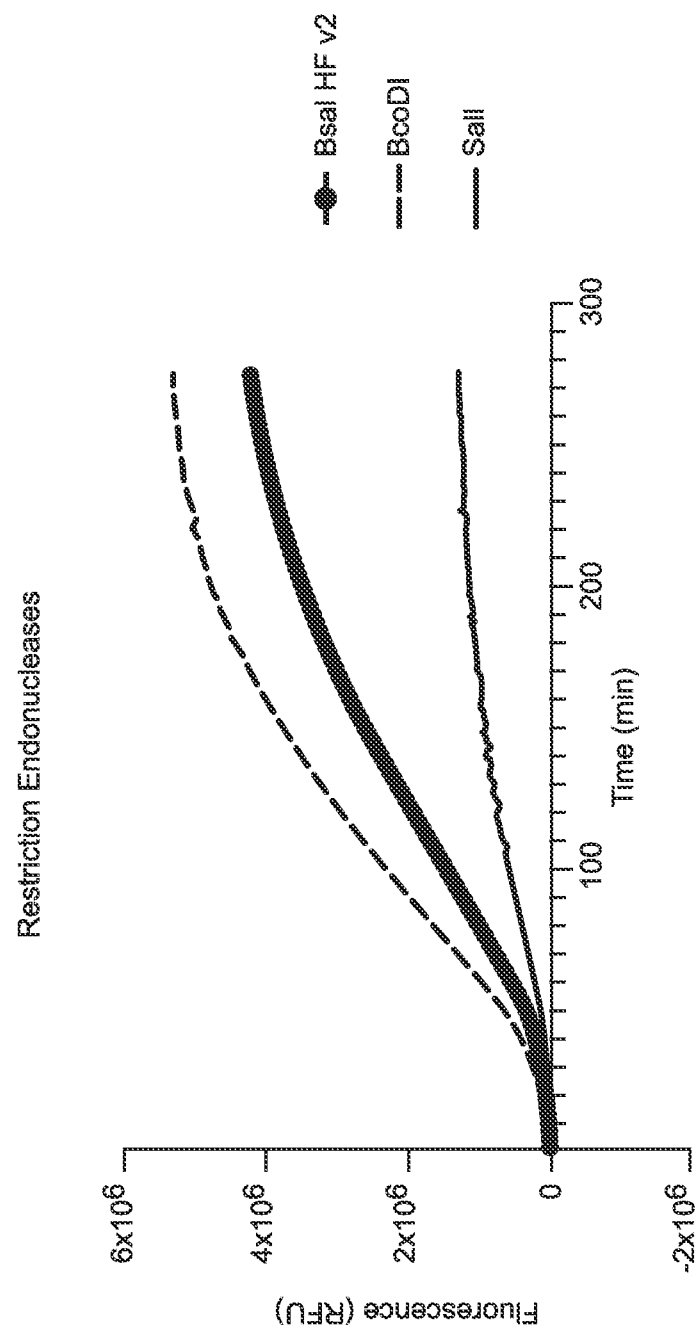


FIG. 16