

1/25

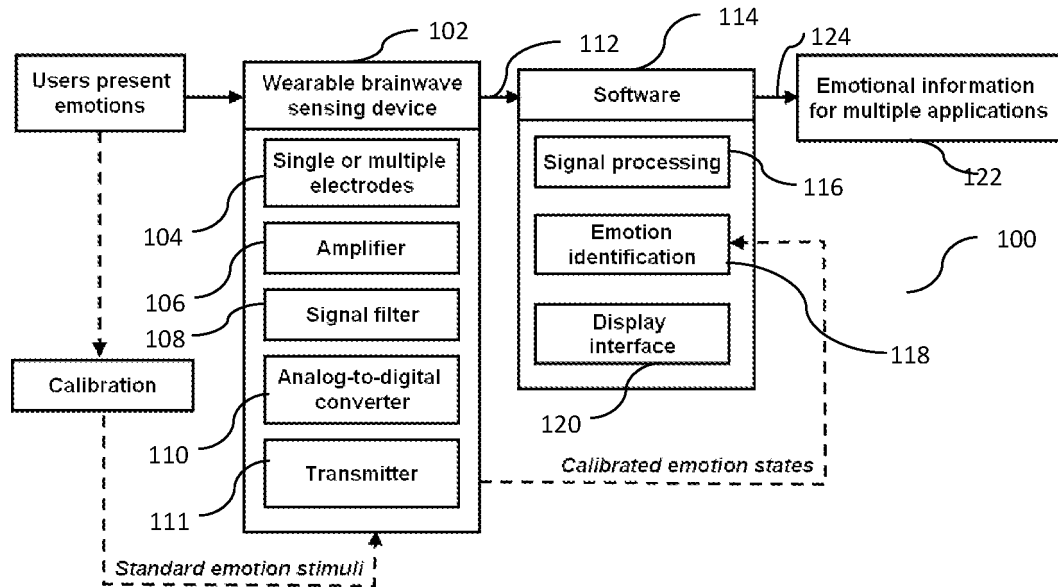


Fig. 1A)

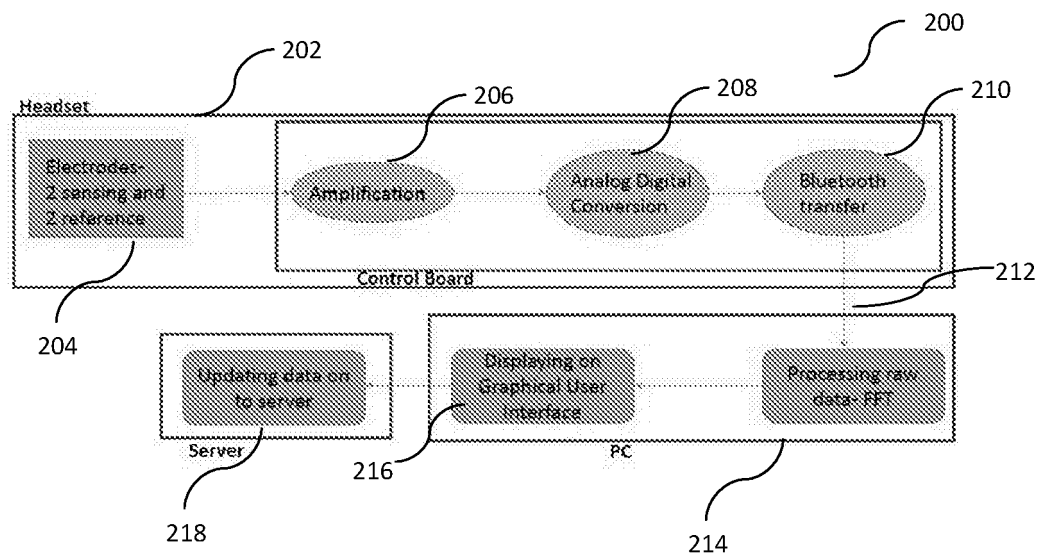


Fig. 1B)

2/25

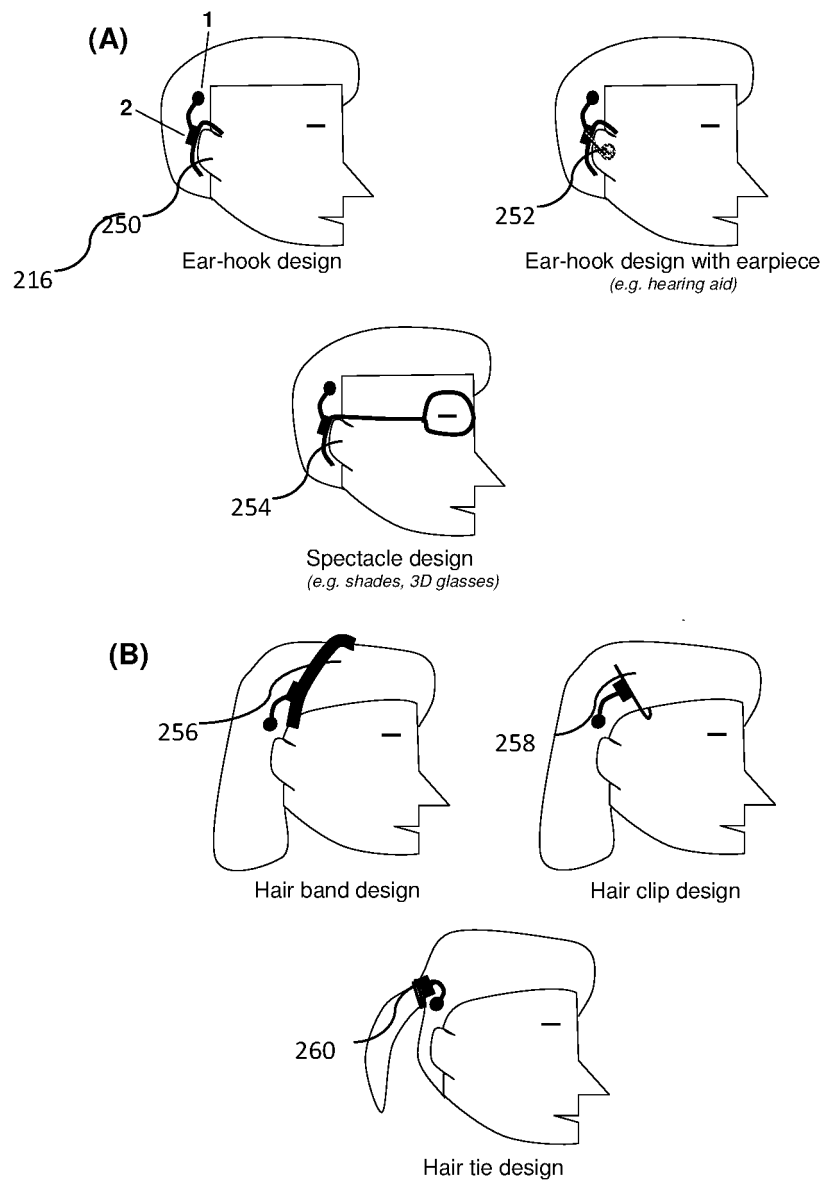


Fig. 2

3/25

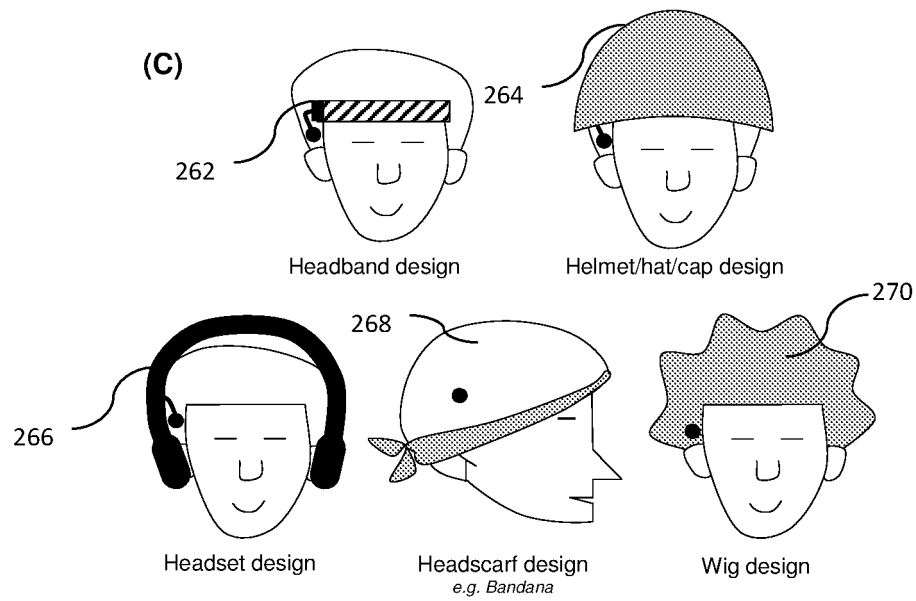


Fig. 2

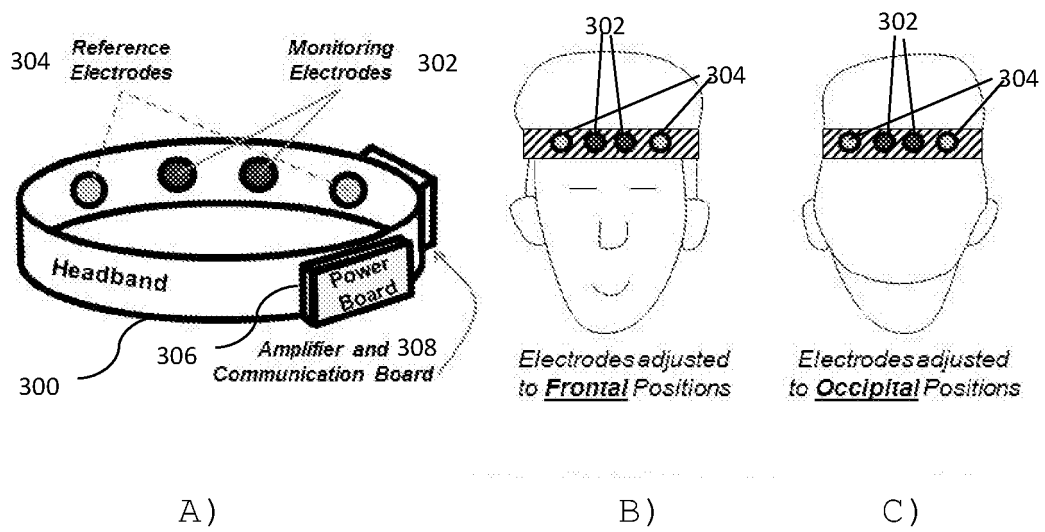


Fig. 3

4/25

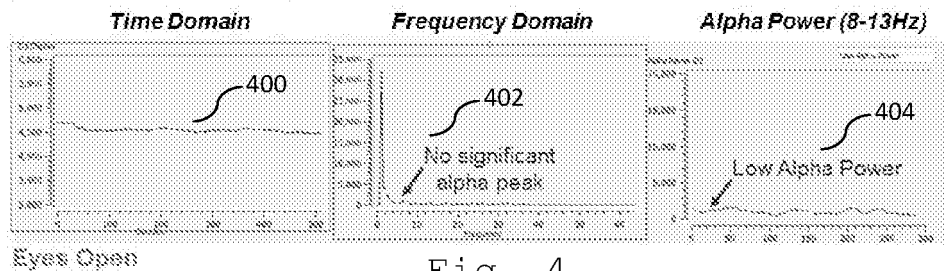
REAL TIME DATA DISPLAY

Fig. 4

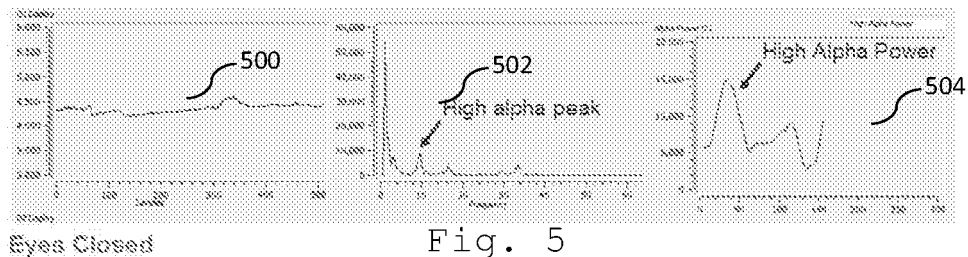


Fig. 5


**Headband EEG
- Real-time Online
Database Update and
Data Retrieval**

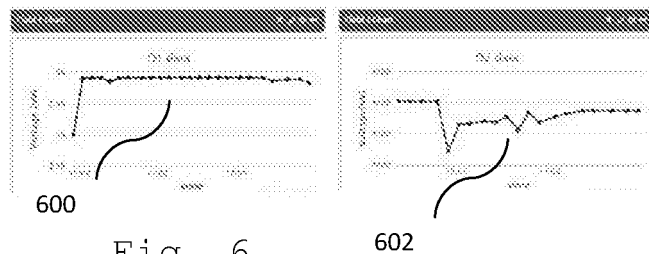Fig. 6

5/25

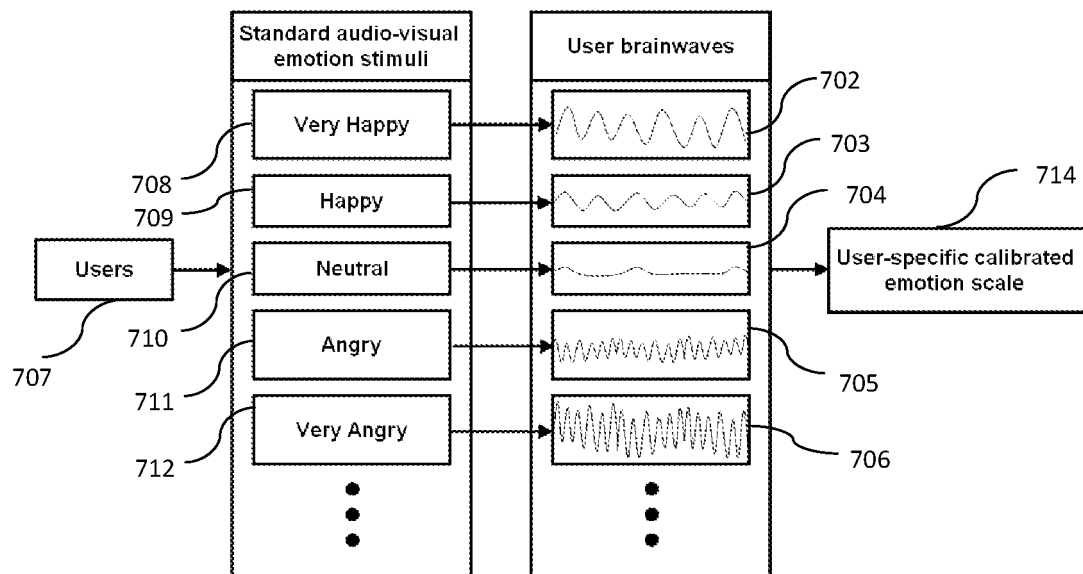


Fig. 7

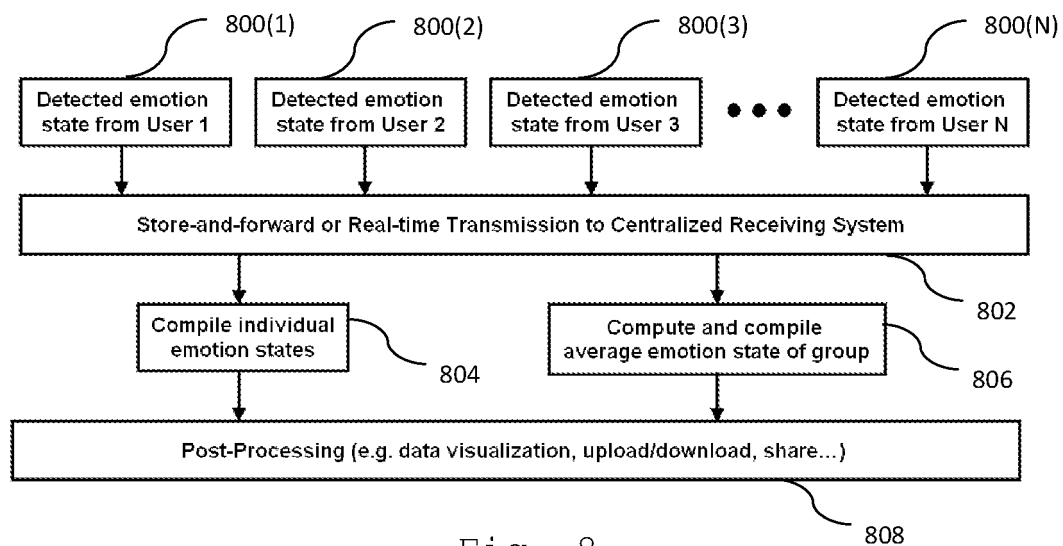


Fig. 8

6/25

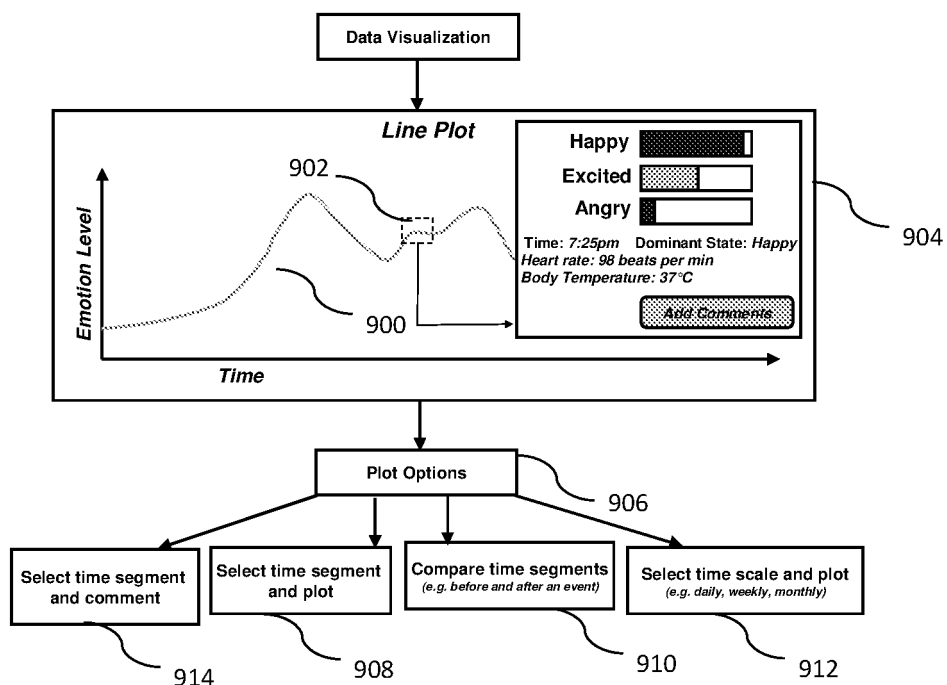


Fig. 9A)



Fig. 9B)

7/25

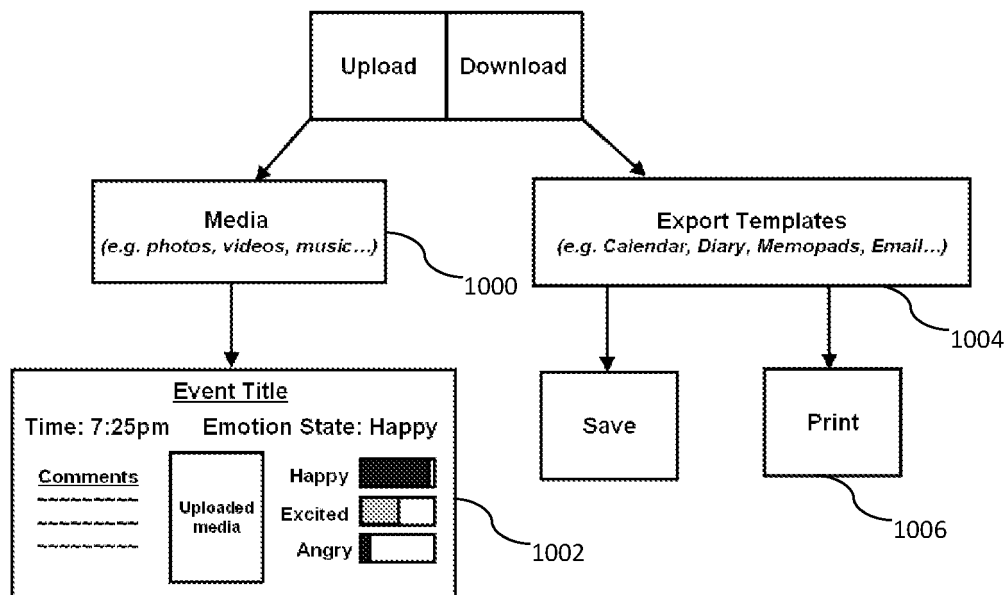


Fig. 10

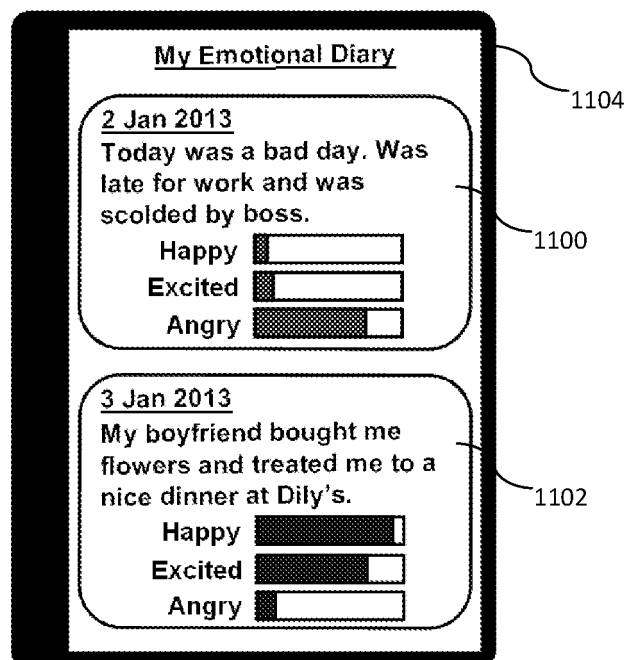


Fig. 11

8/25

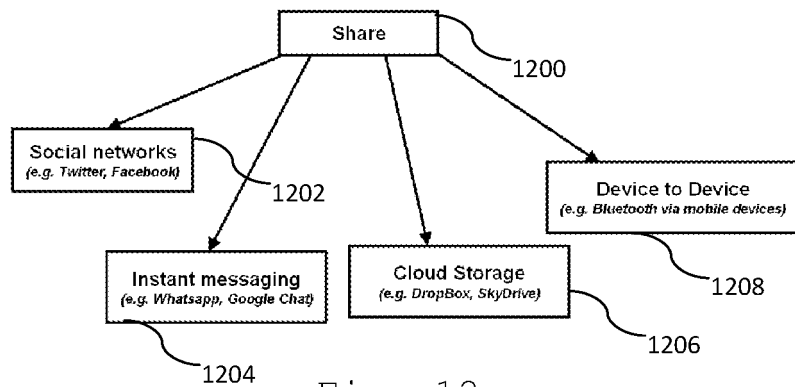


Fig. 12

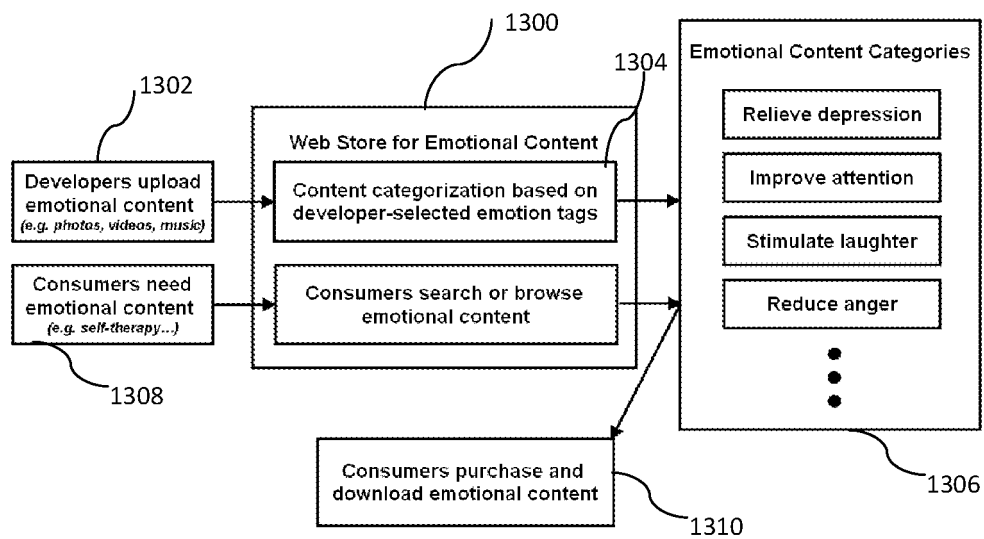


Fig. 13

9/25

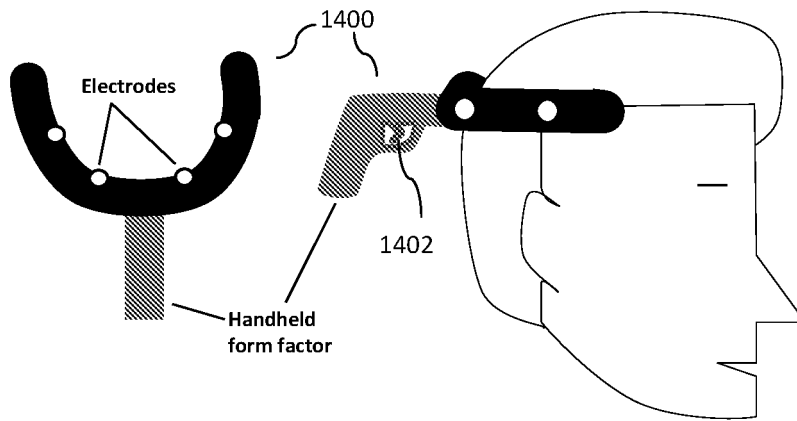


Fig. 14A)

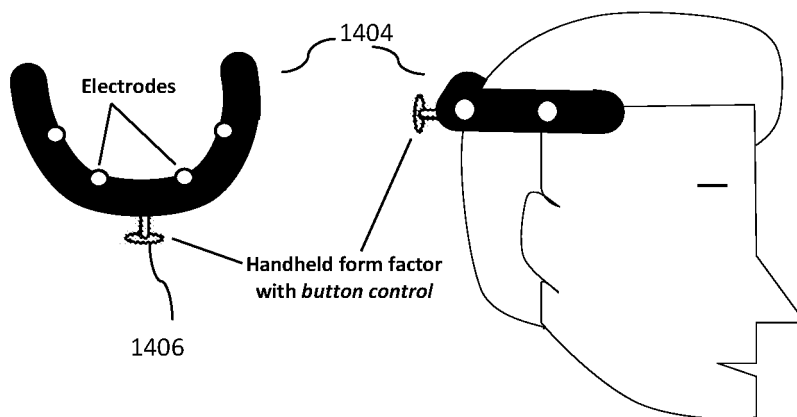


Fig. 14B)

10/25

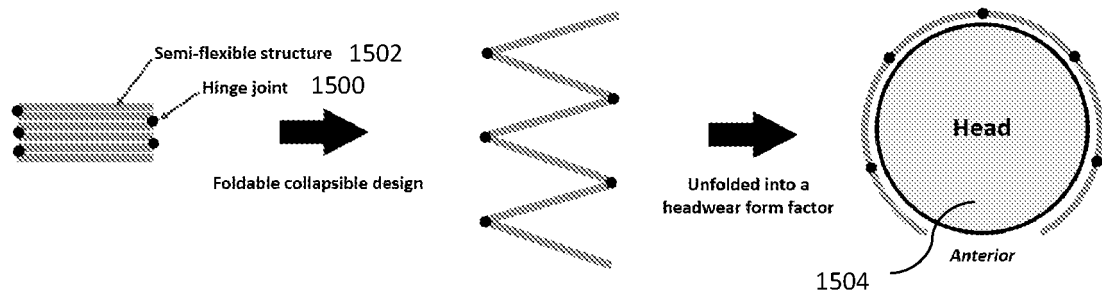


Fig. 15

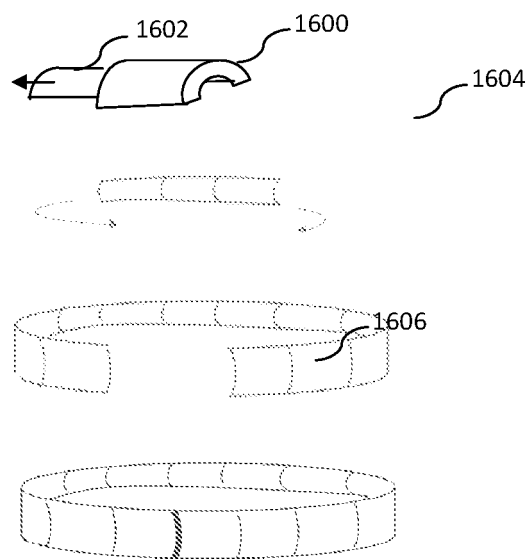


Fig. 16

11/25

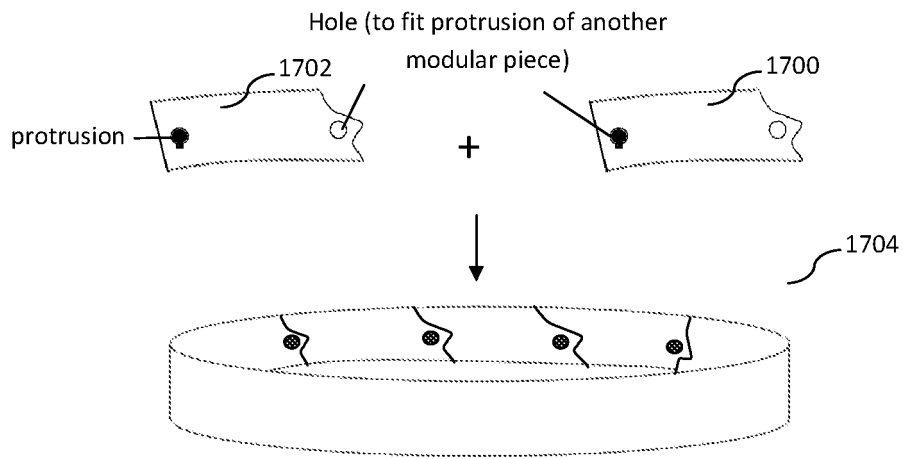


Fig. 17


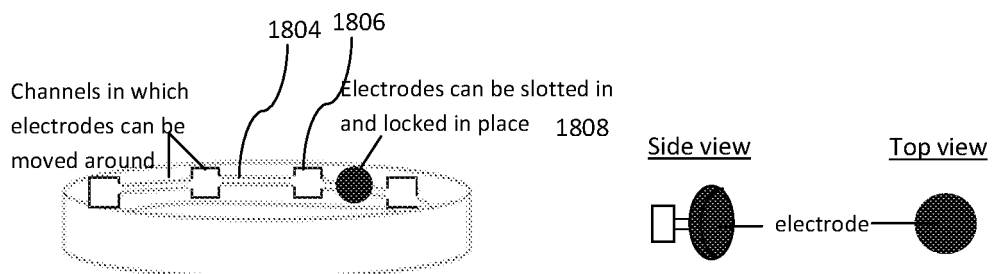



Fig. 18C)

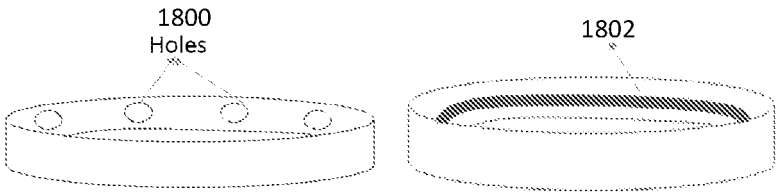

11a : Holes or Groove to allow electrodes to fit in


Fig. 18A)

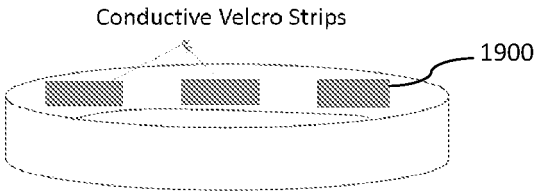Fig. 18B)



11b : Conductive Velcro strips attached to attach electrodes

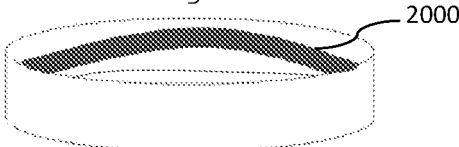Magnetized Strip
Fig. 19



11c : Magnetized Strip to attach electrodes

Fig. 20

13/25

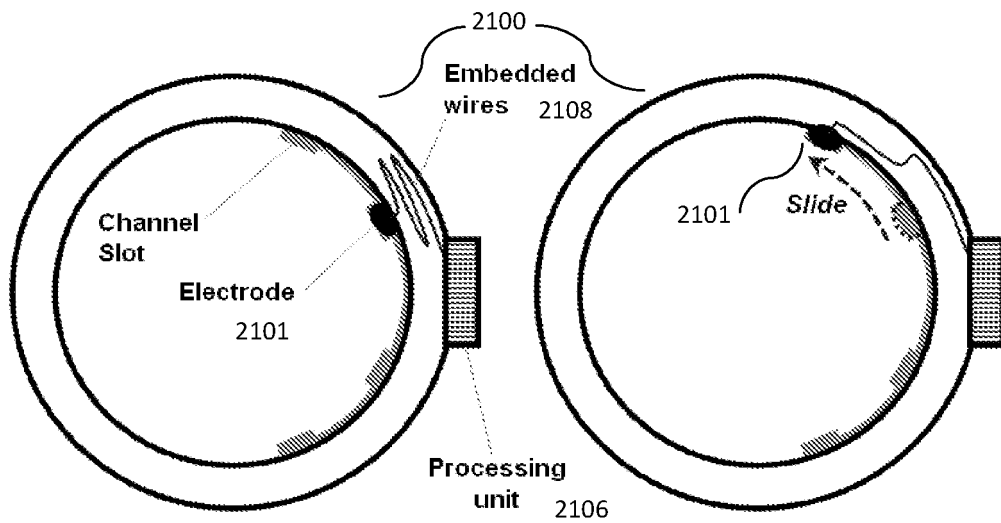


Fig. 21A)

Fig. 21B)

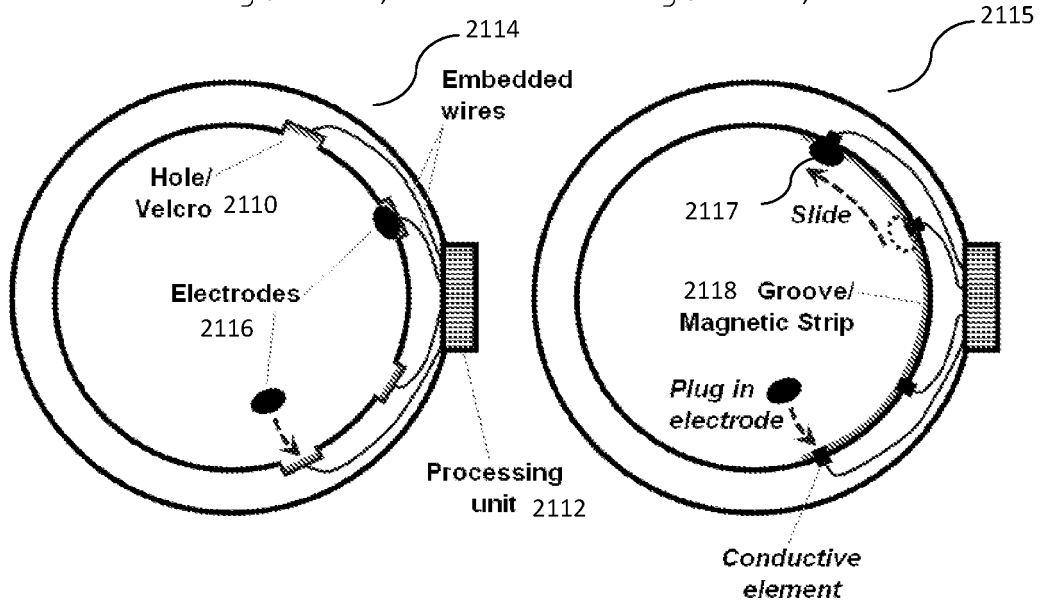


Fig. 21C)

Fig. 21D)

14/25

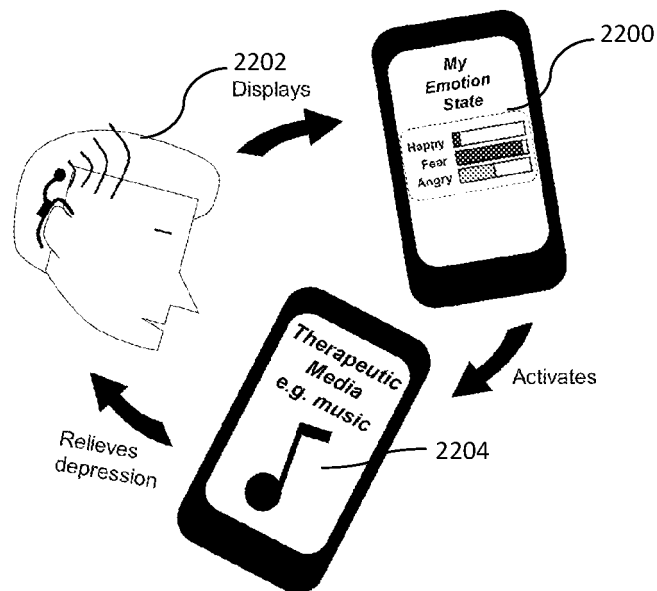


Fig. 22

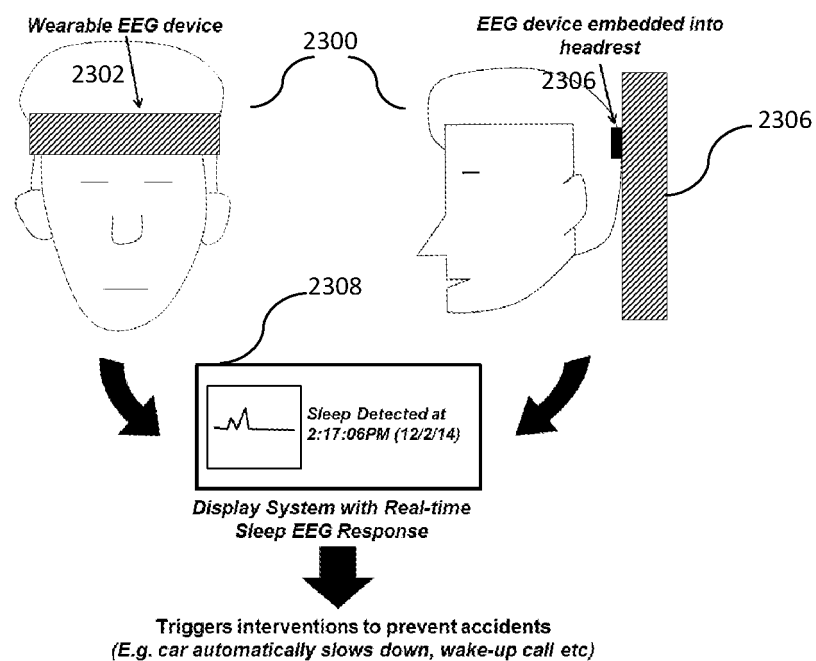


Fig. 23

15/25

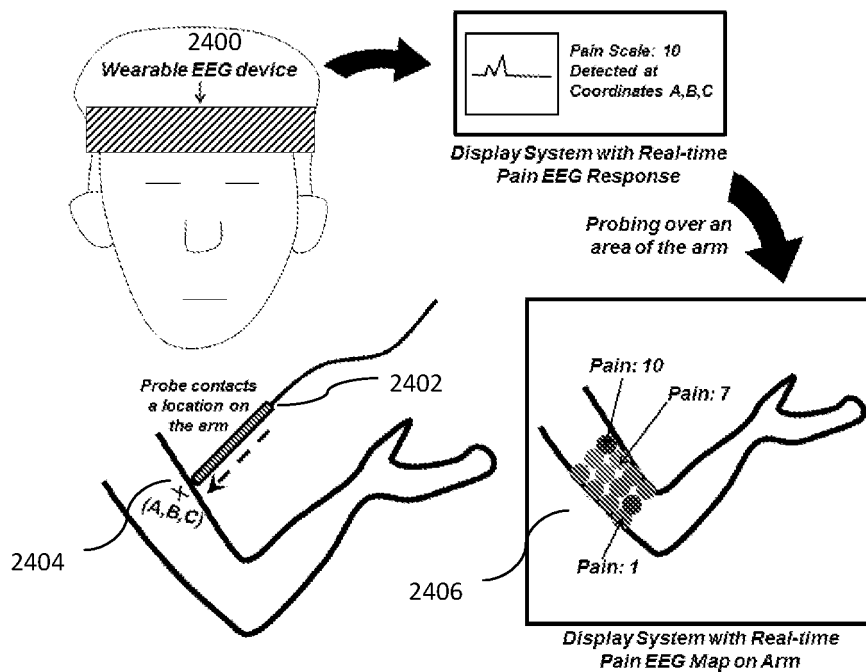


Fig. 24

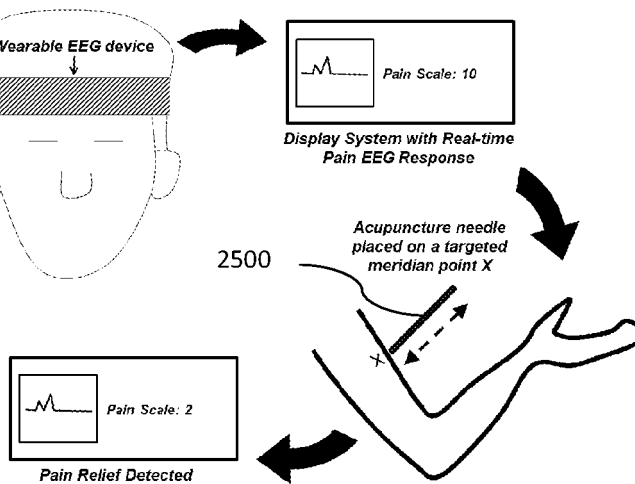


Fig. 25

16/25

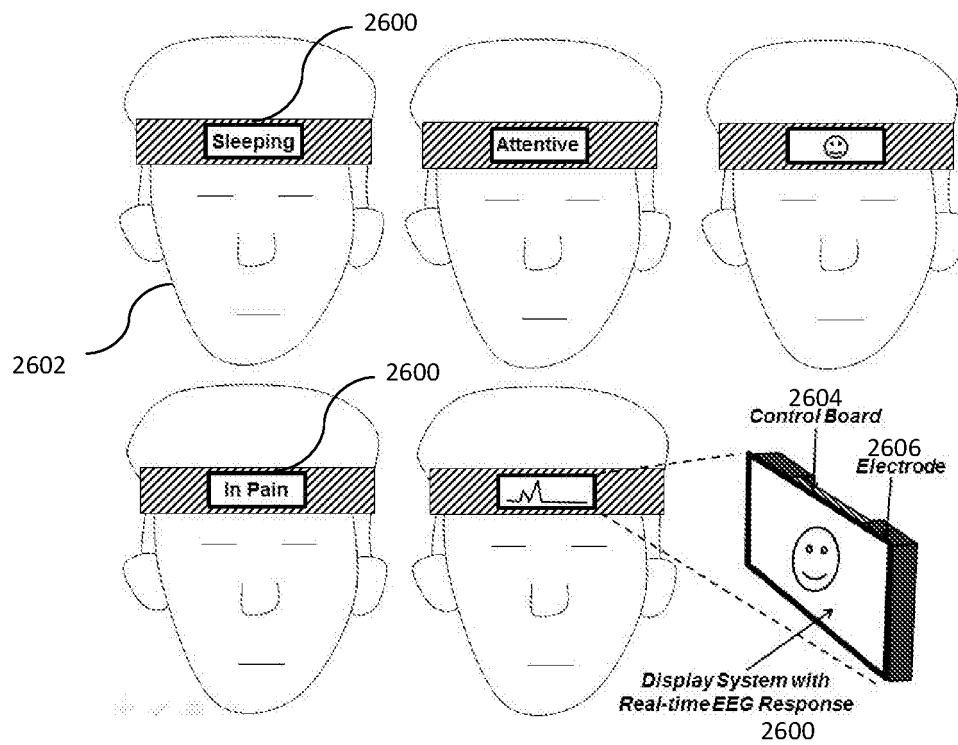


Fig. 26

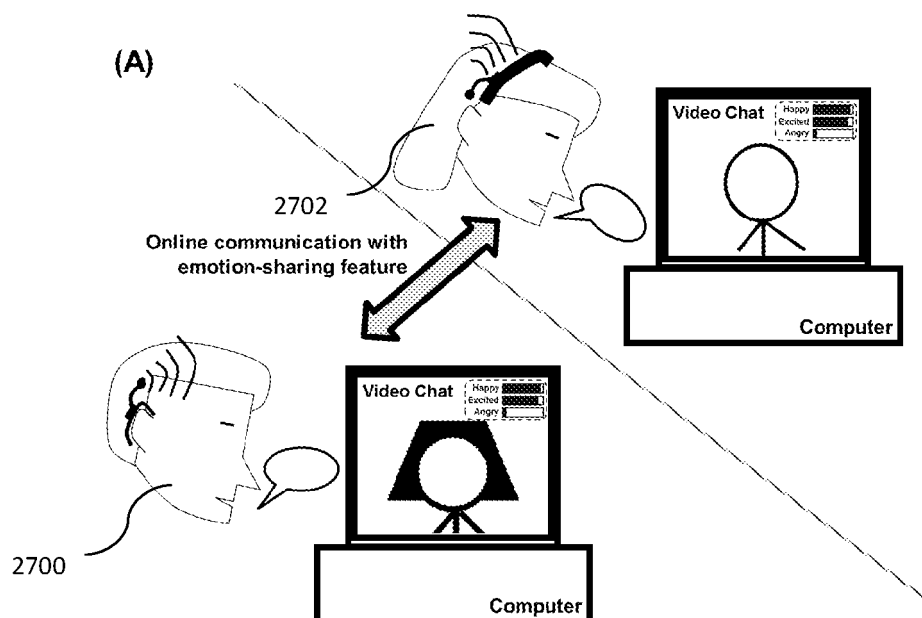


Fig. 27

17/25

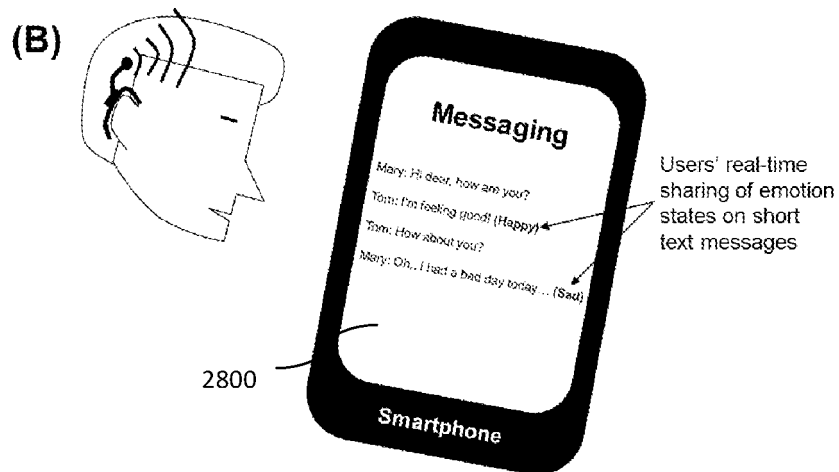


Fig. 28

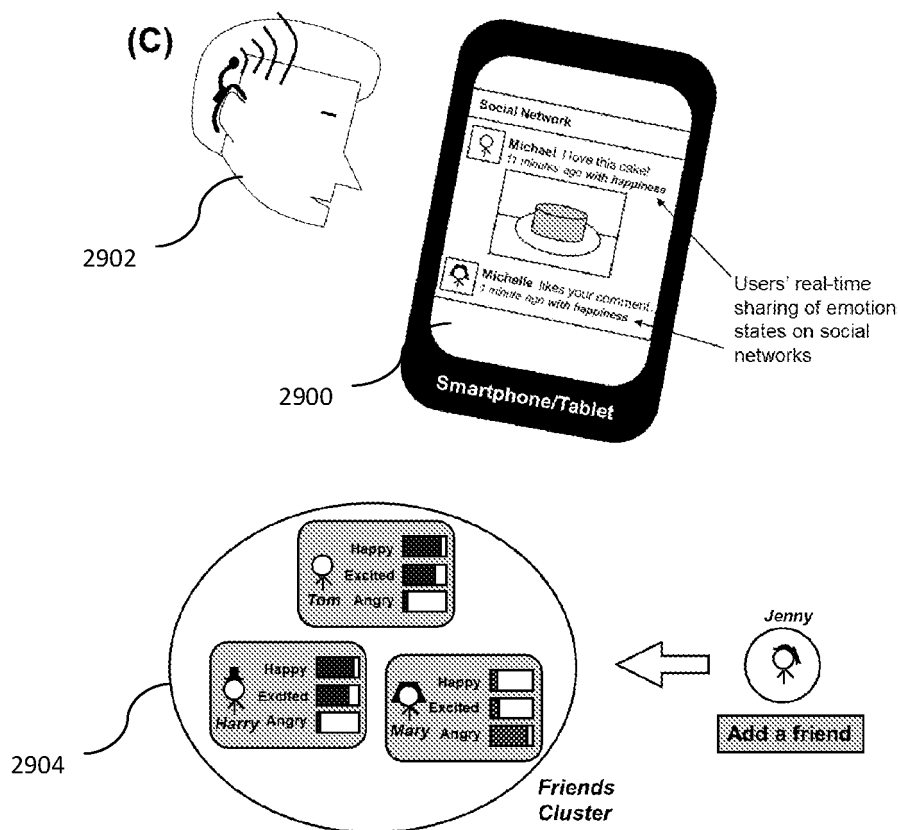


Fig. 29

18/25

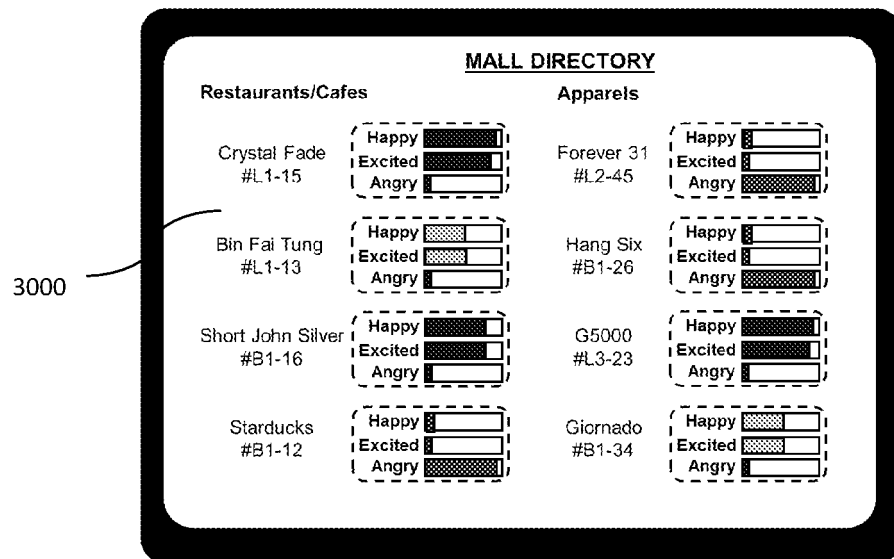


Fig. 30

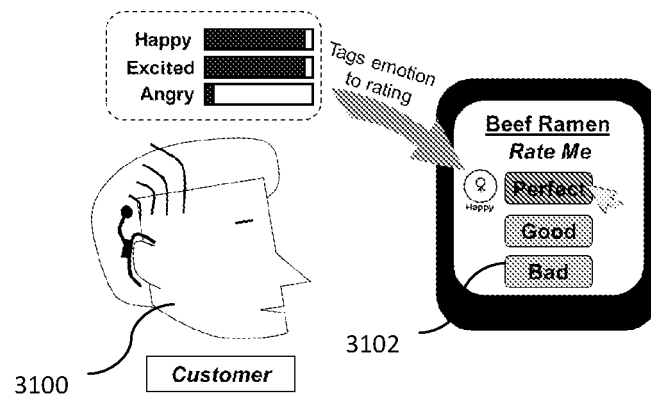


Fig. 31

19/25

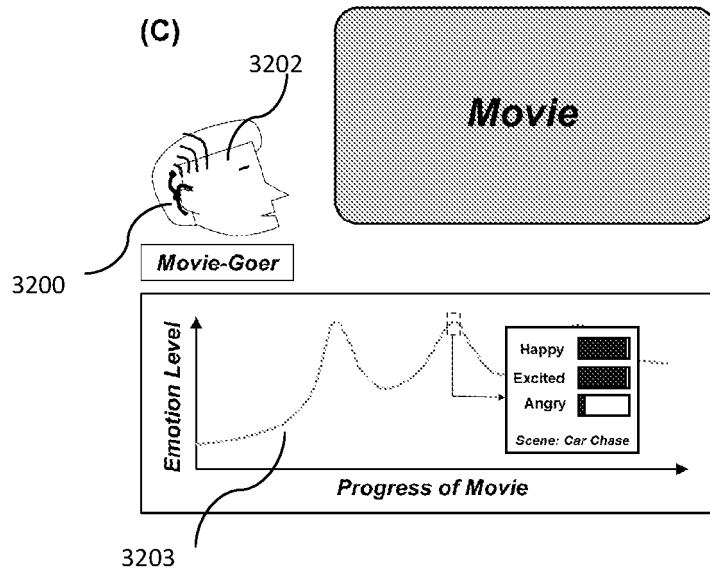


Fig. 32

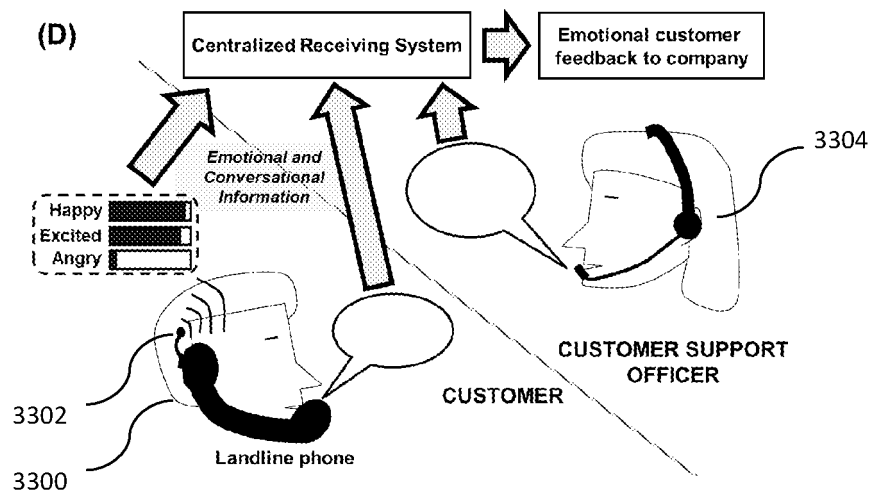


Fig. 33

20/25

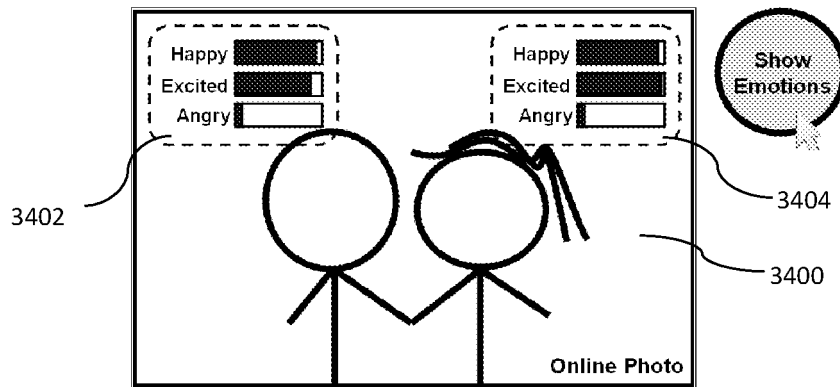


Fig. 34

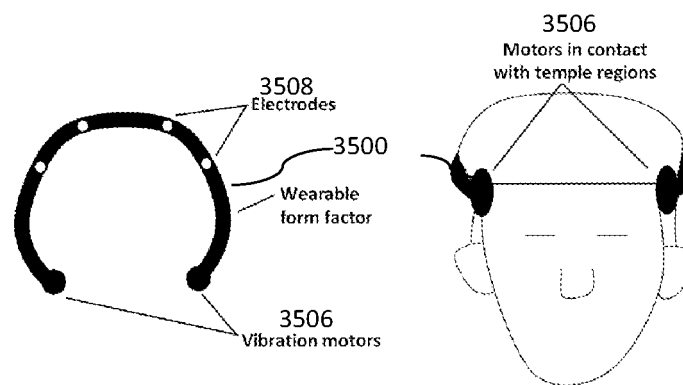


Fig. 35A)

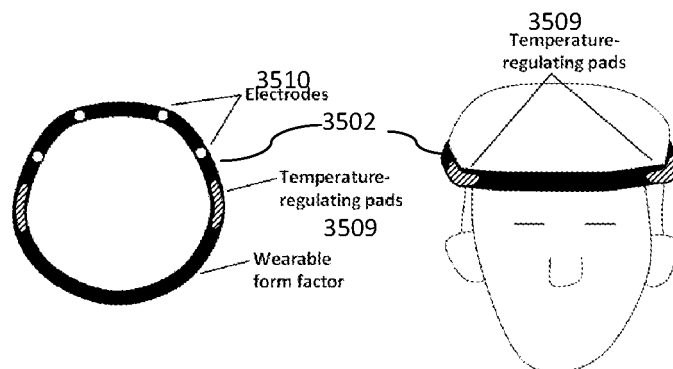


Fig. 35B)

21/25

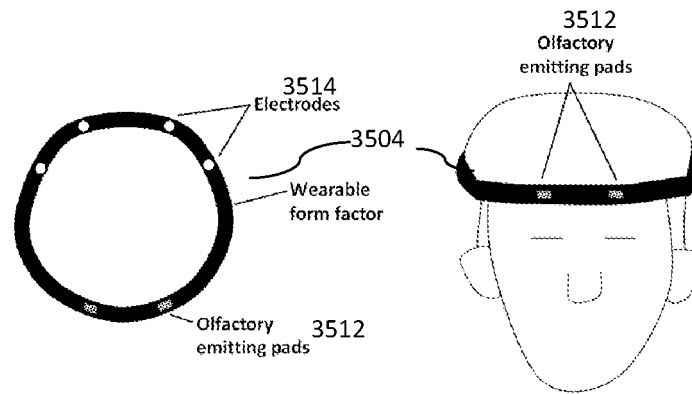


Fig. 35C)

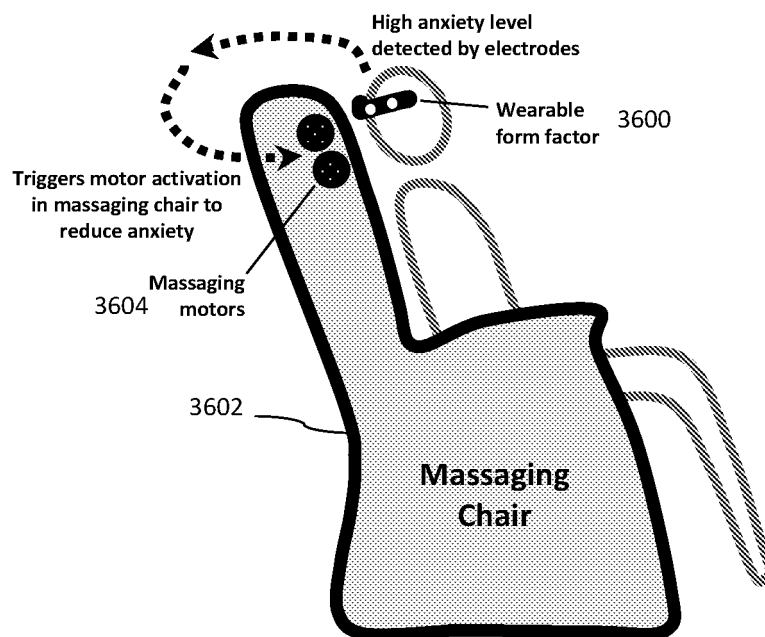


Fig. 36

22/25

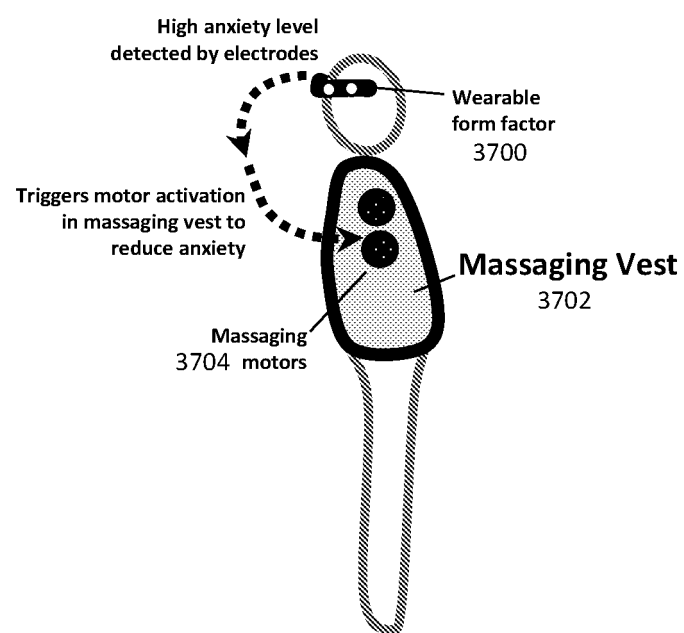


Fig. 37

23/25



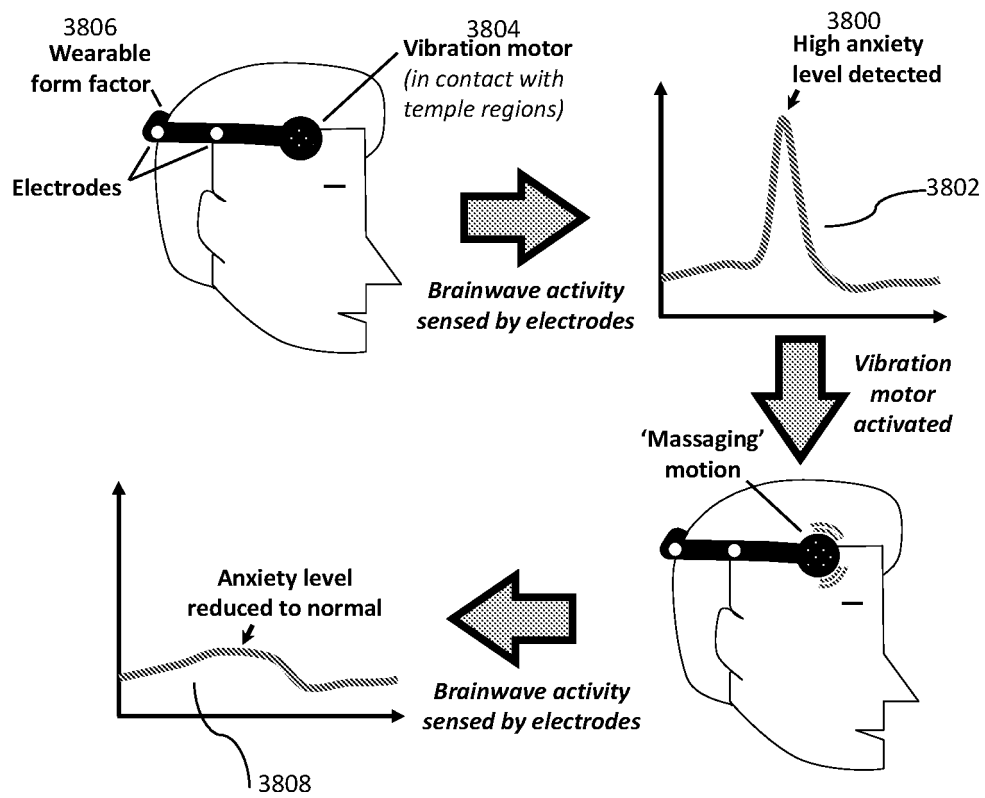


Fig. 38

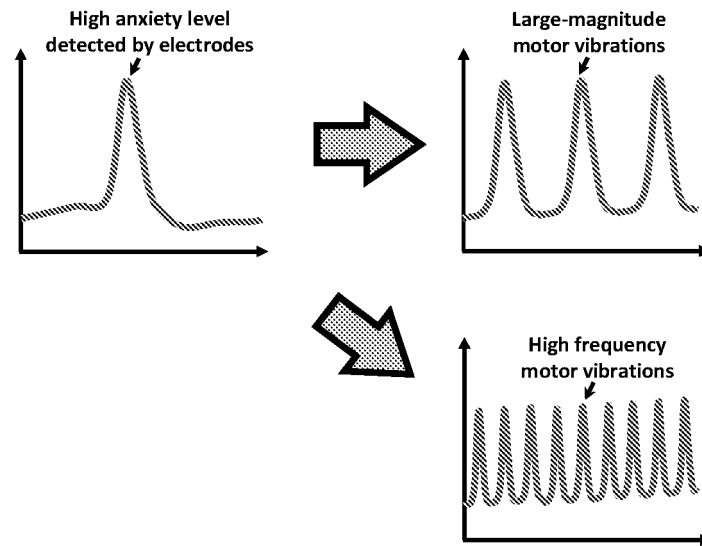24/25



A)

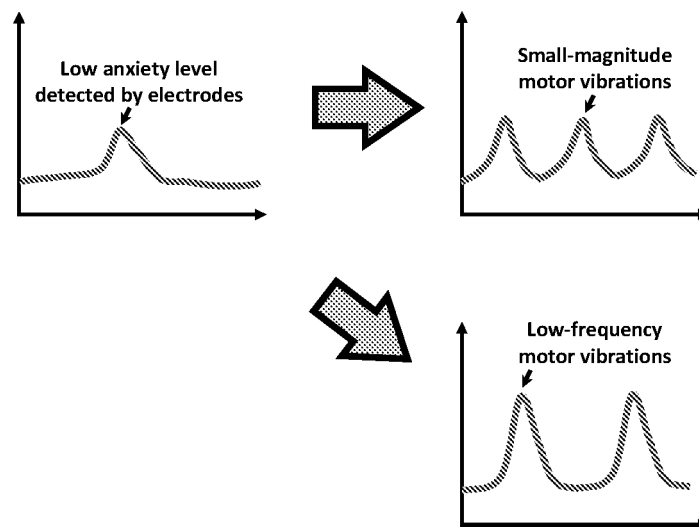

B)

Fig. 39

25/25

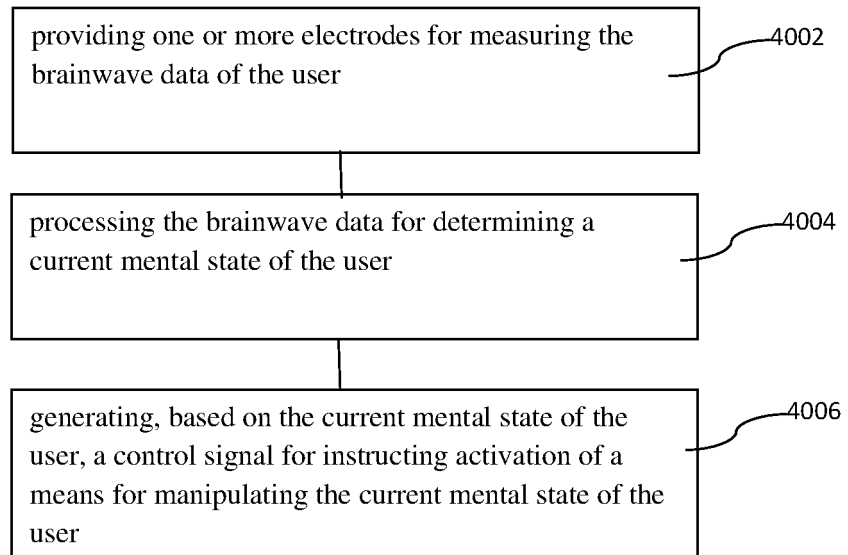


Fig. 40

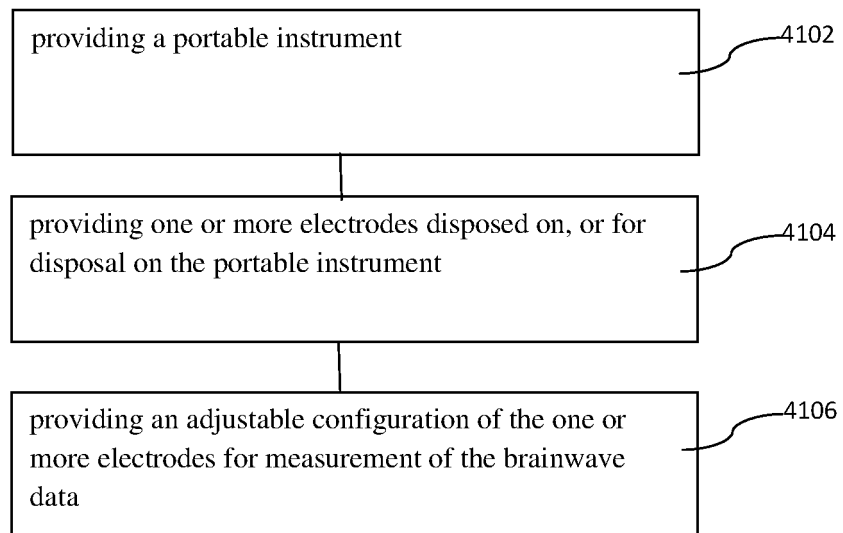


Fig. 41