

FIG. 1

FIG. 2

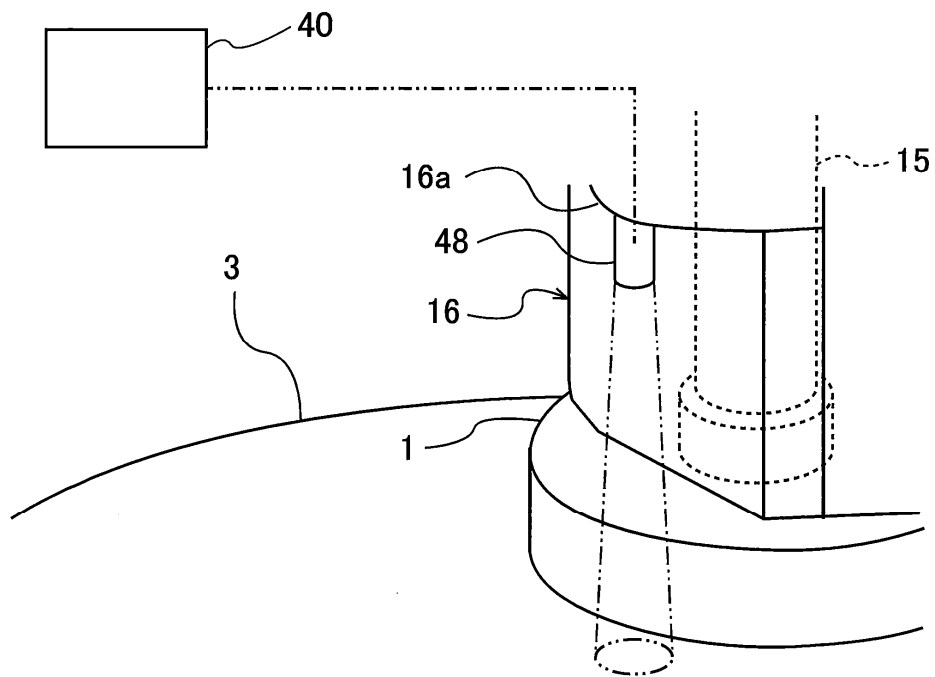


FIG. 3

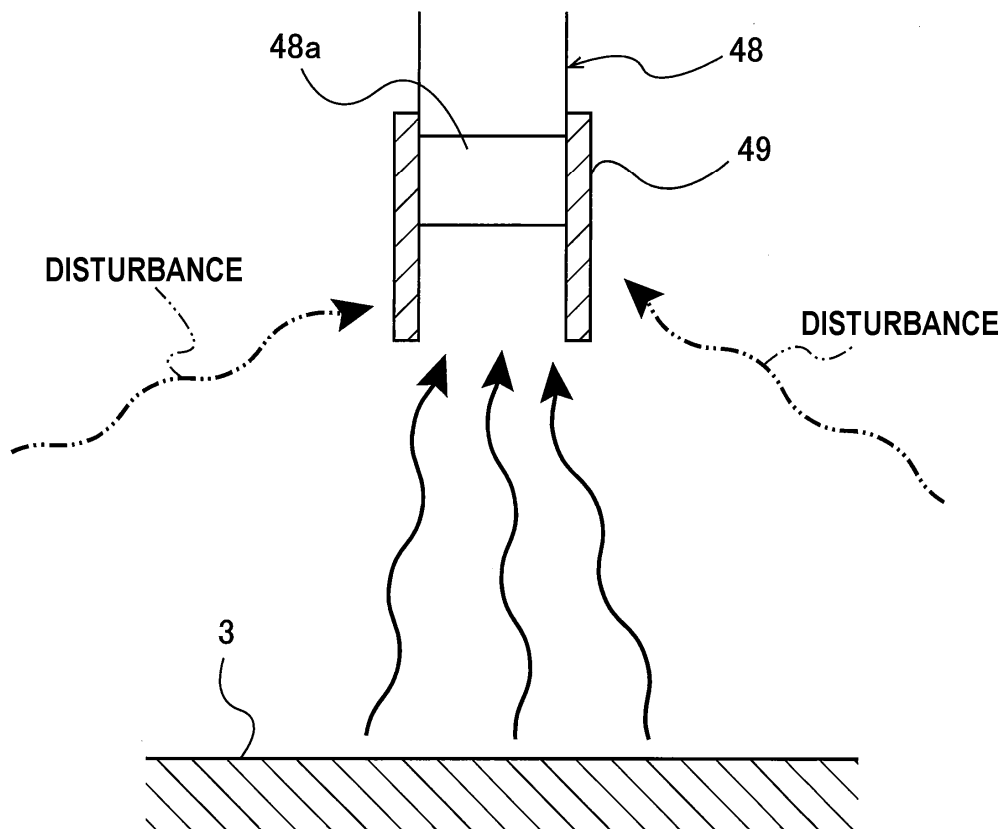


FIG. 4

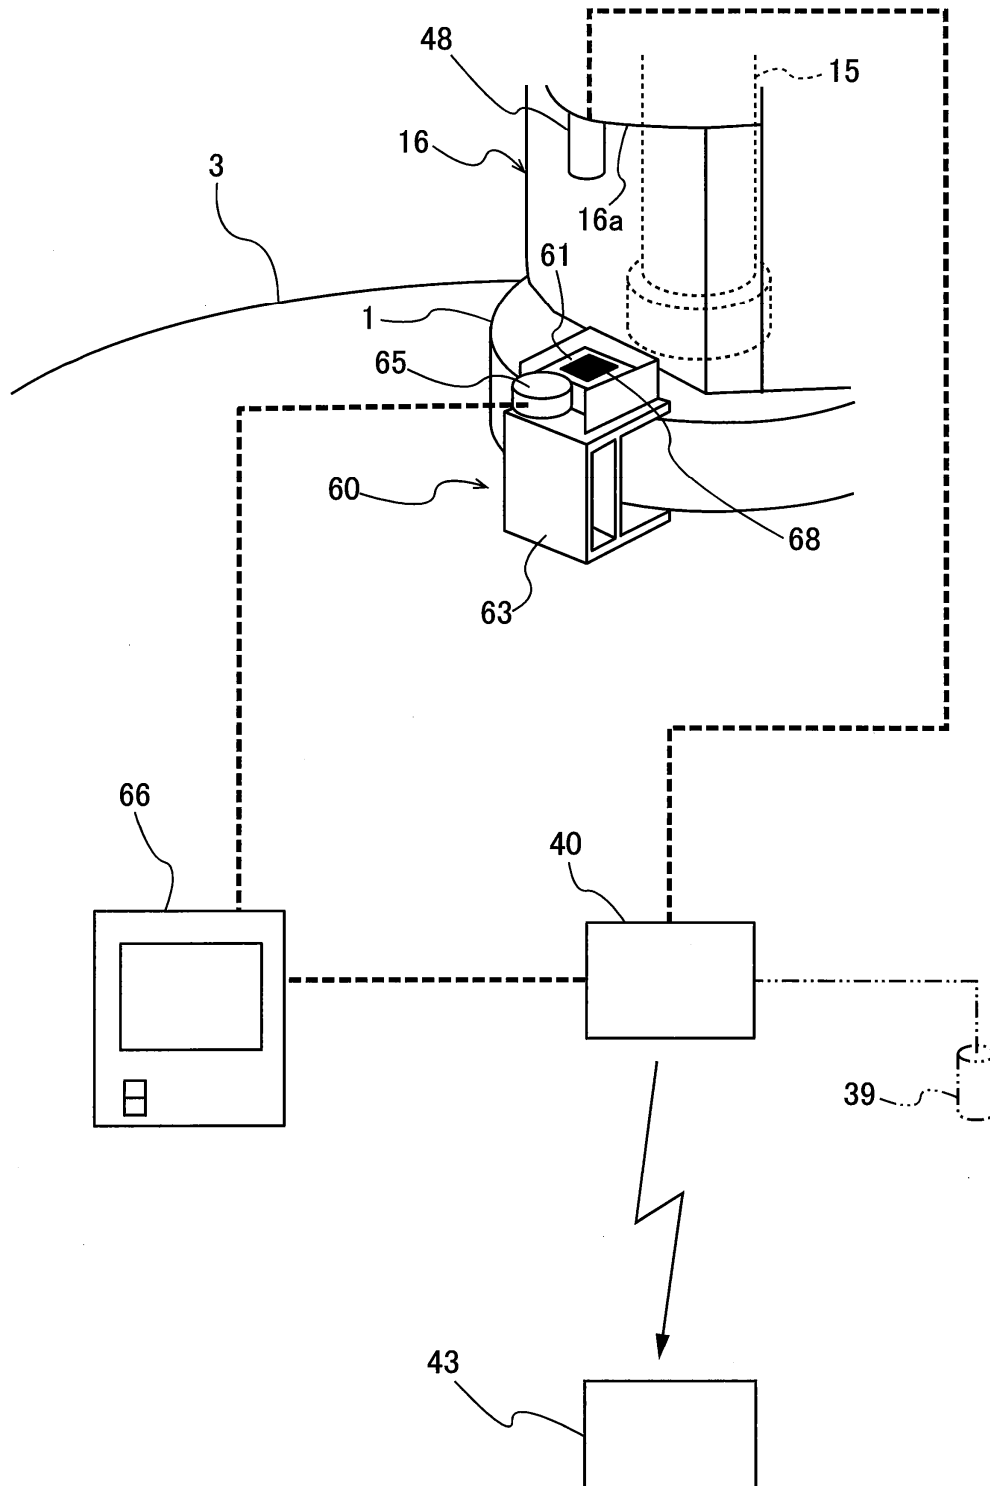


FIG. 5A

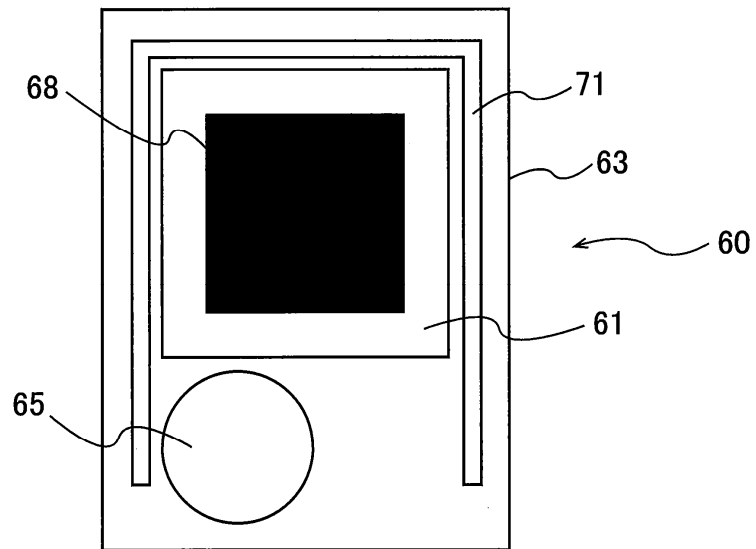


FIG. 5B

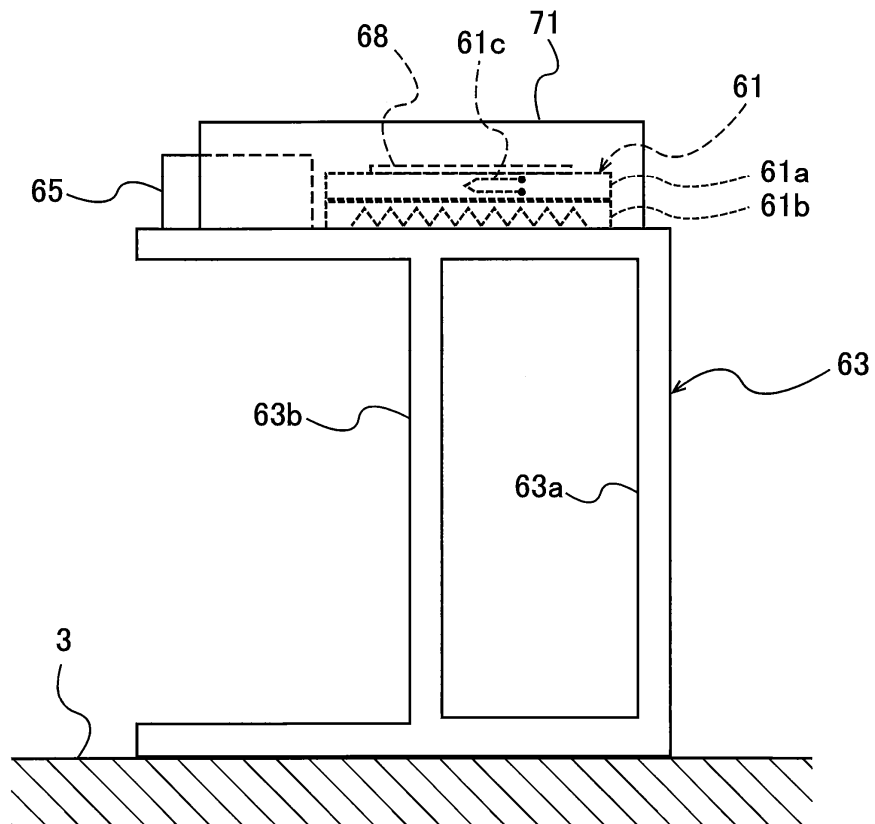


FIG. 6

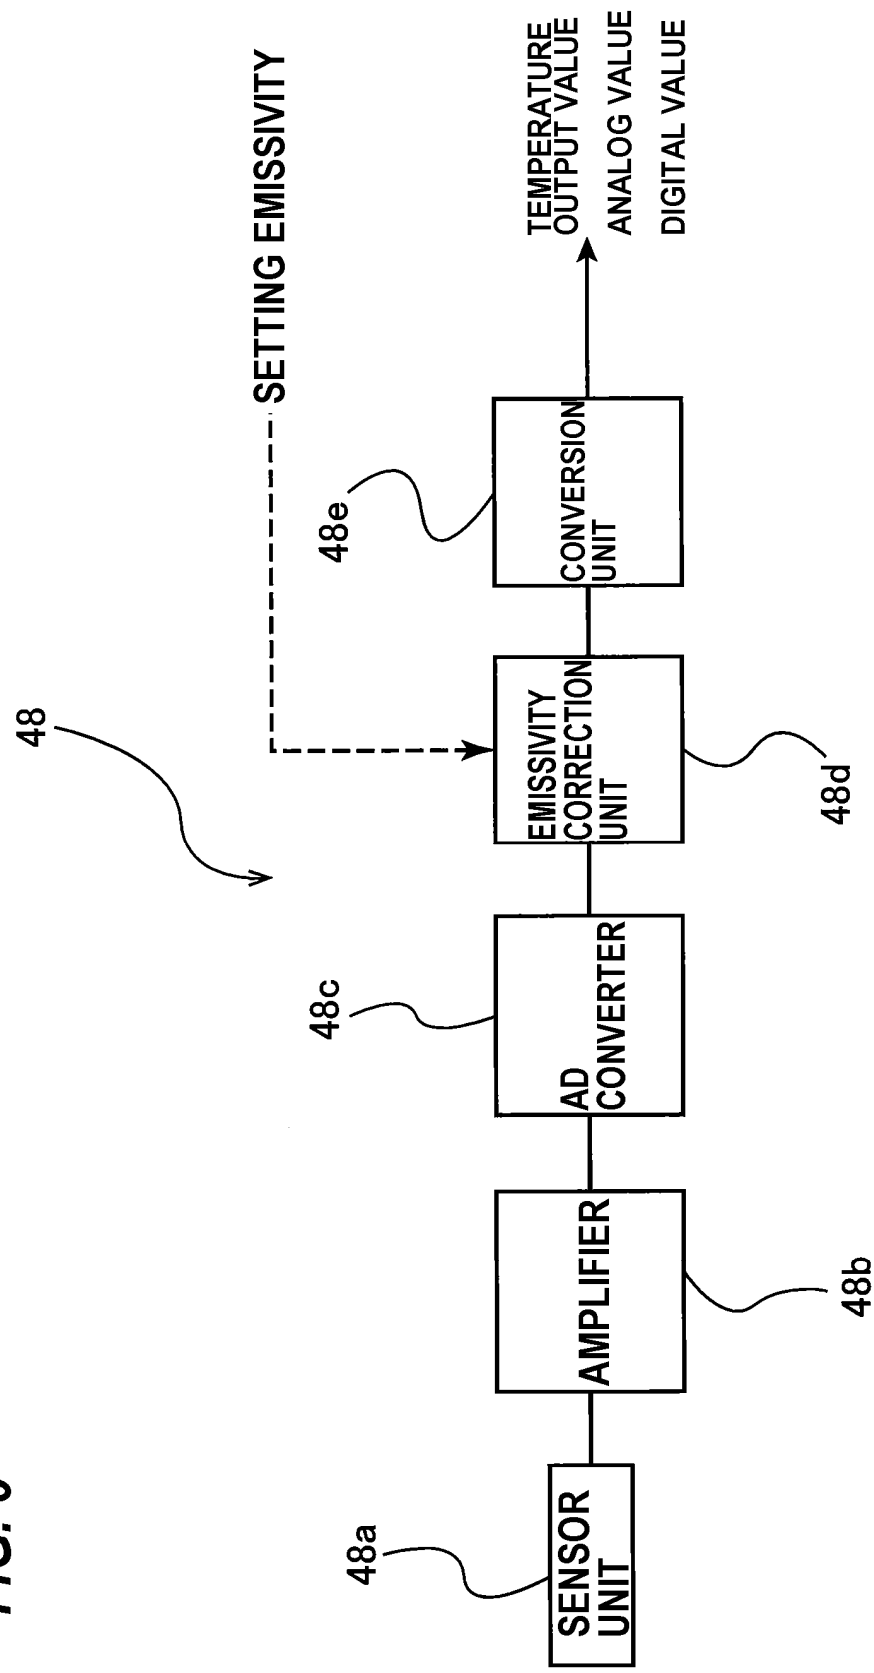


FIG. 7

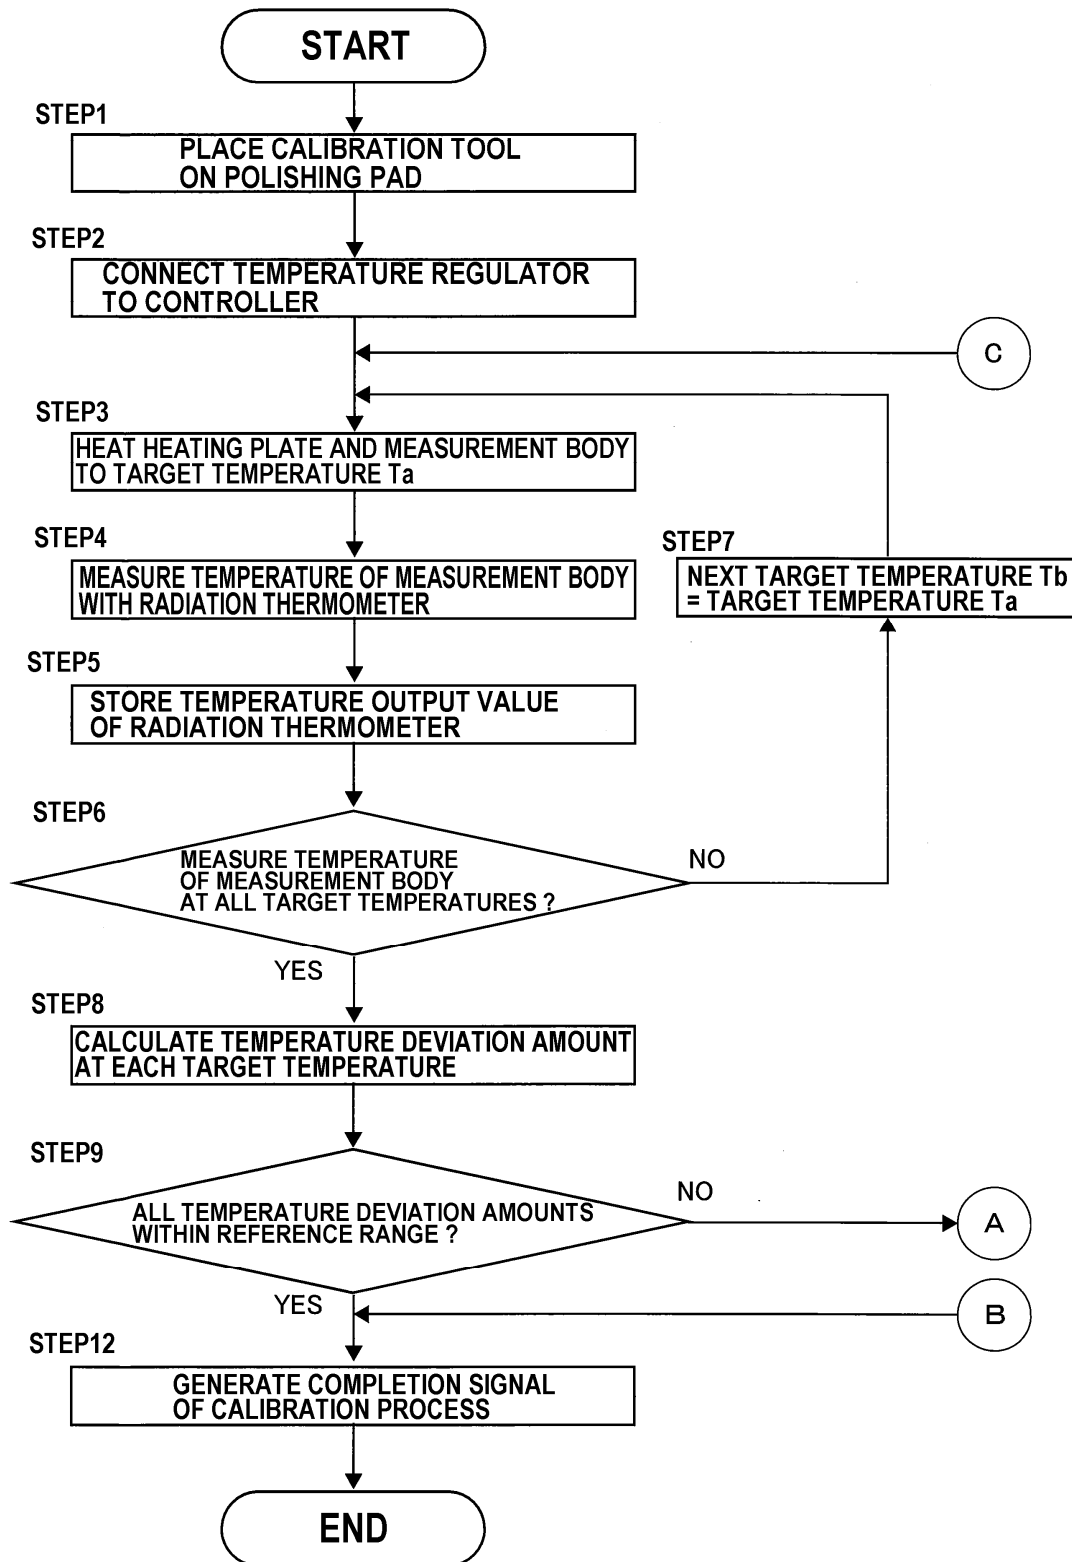


FIG. 8

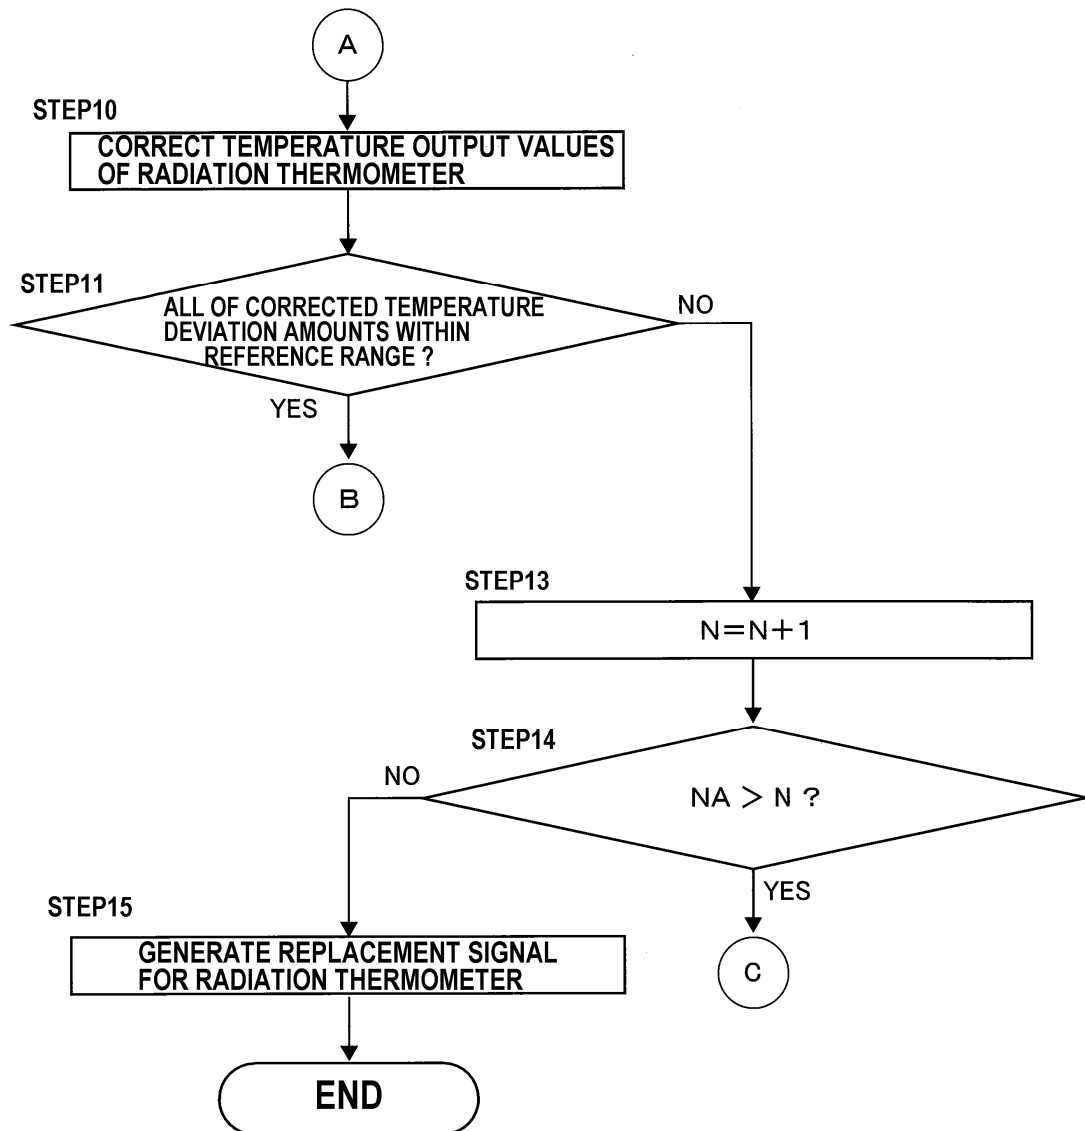
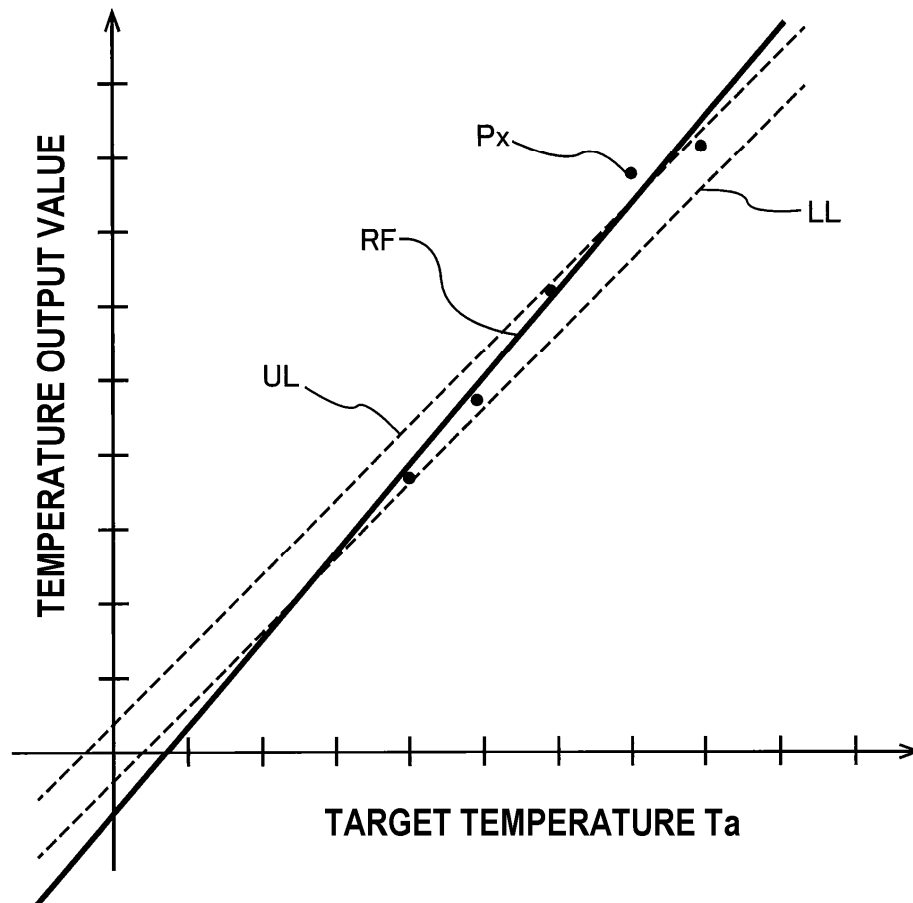


FIG. 9

9/20

FIG. 10


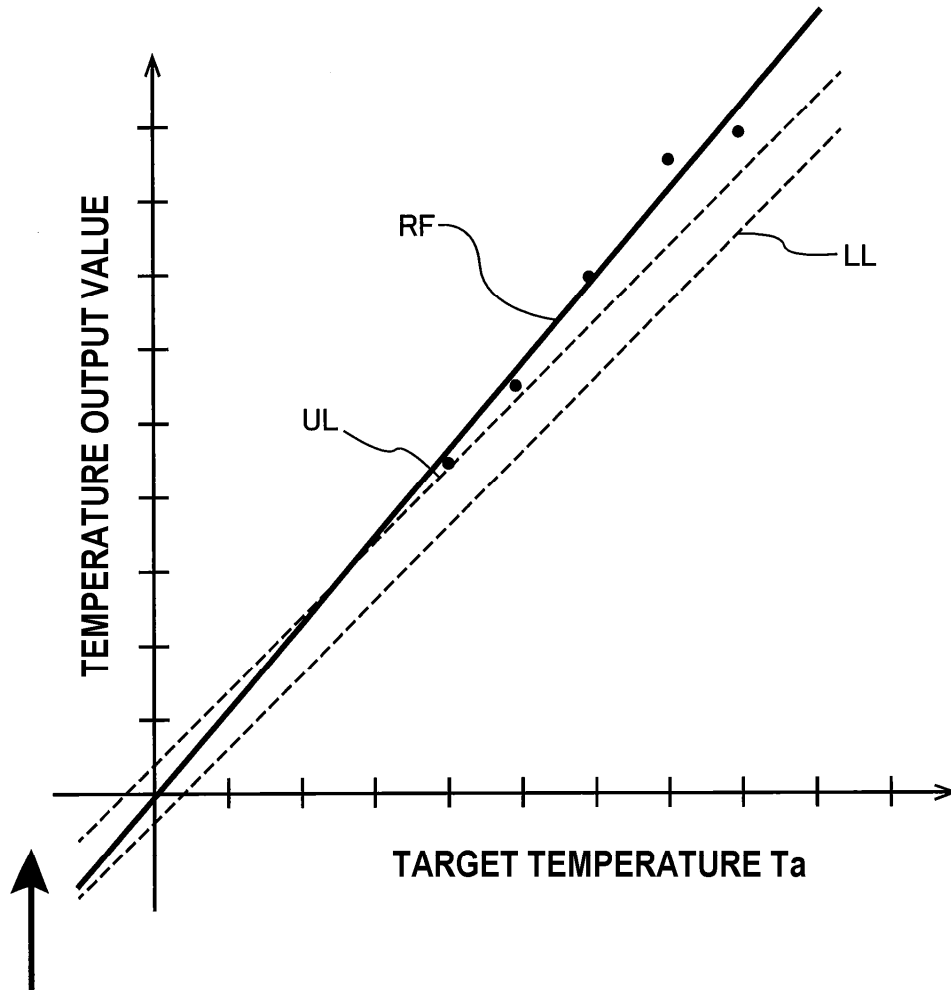


FIG. 11

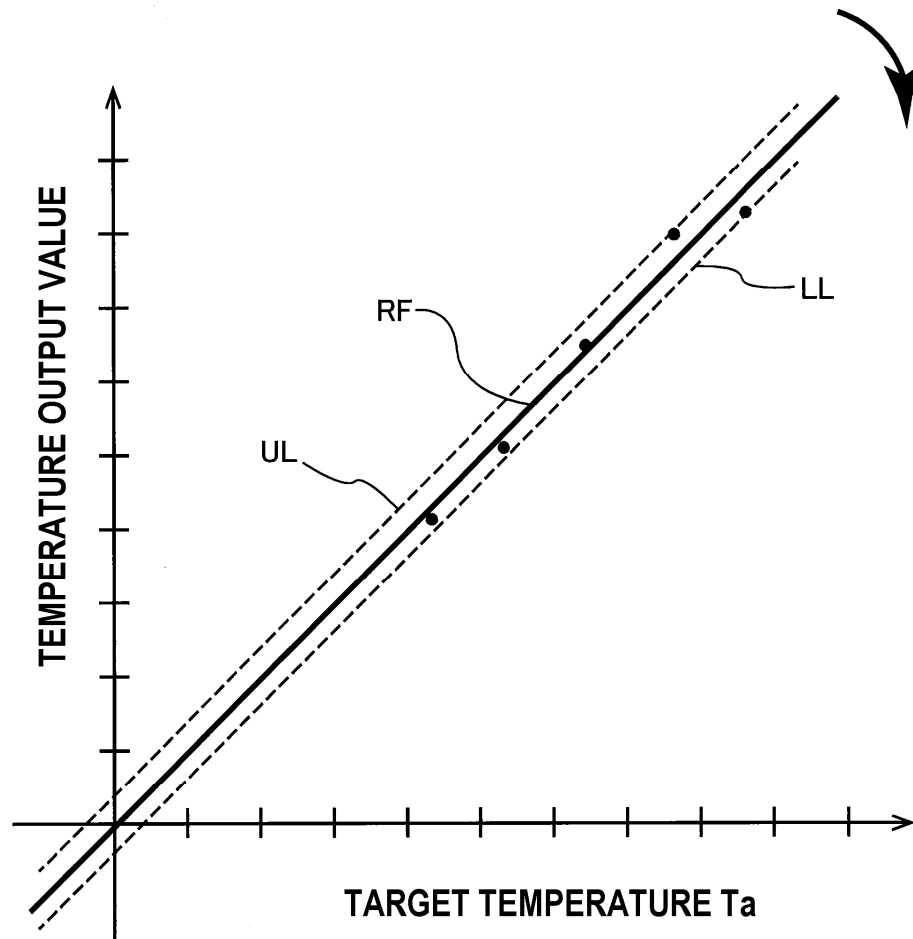

11/20

FIG. 12

DATE OF CALIBRATION: yy.mm.dd

RADIATION-THERMOMETER CALIBRATION SHEET

	BEFORE CORRECTION	AFTER CORRECTION
SLOPE (GAIN)	0.075000	0.075070
y-INTERCEPT (OFFSET)	0.194	0.000

THERMOMETER NAME	SECOND RADIATION THERMOMETER
---------------------	---------------------------------

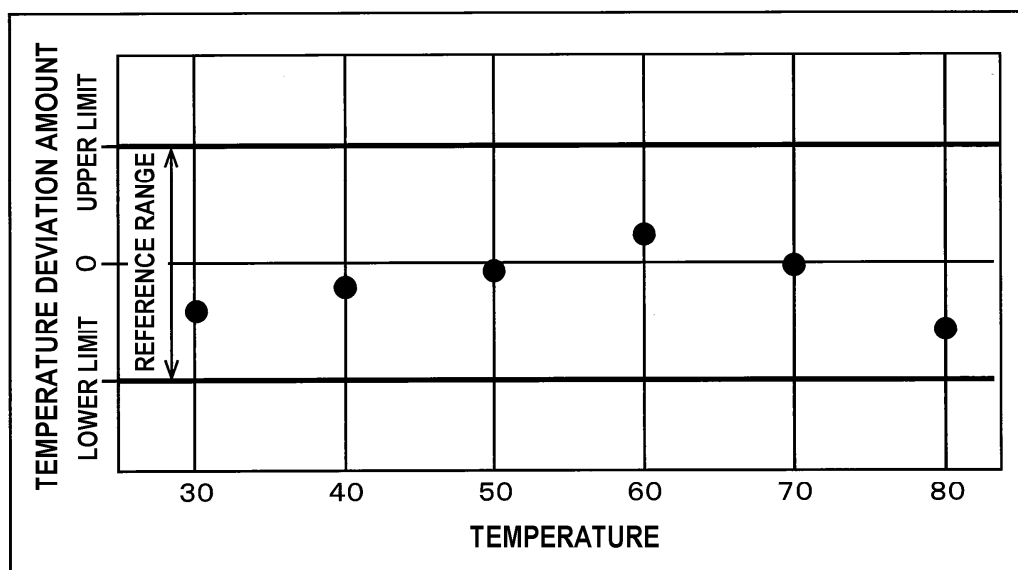


FIG. 13

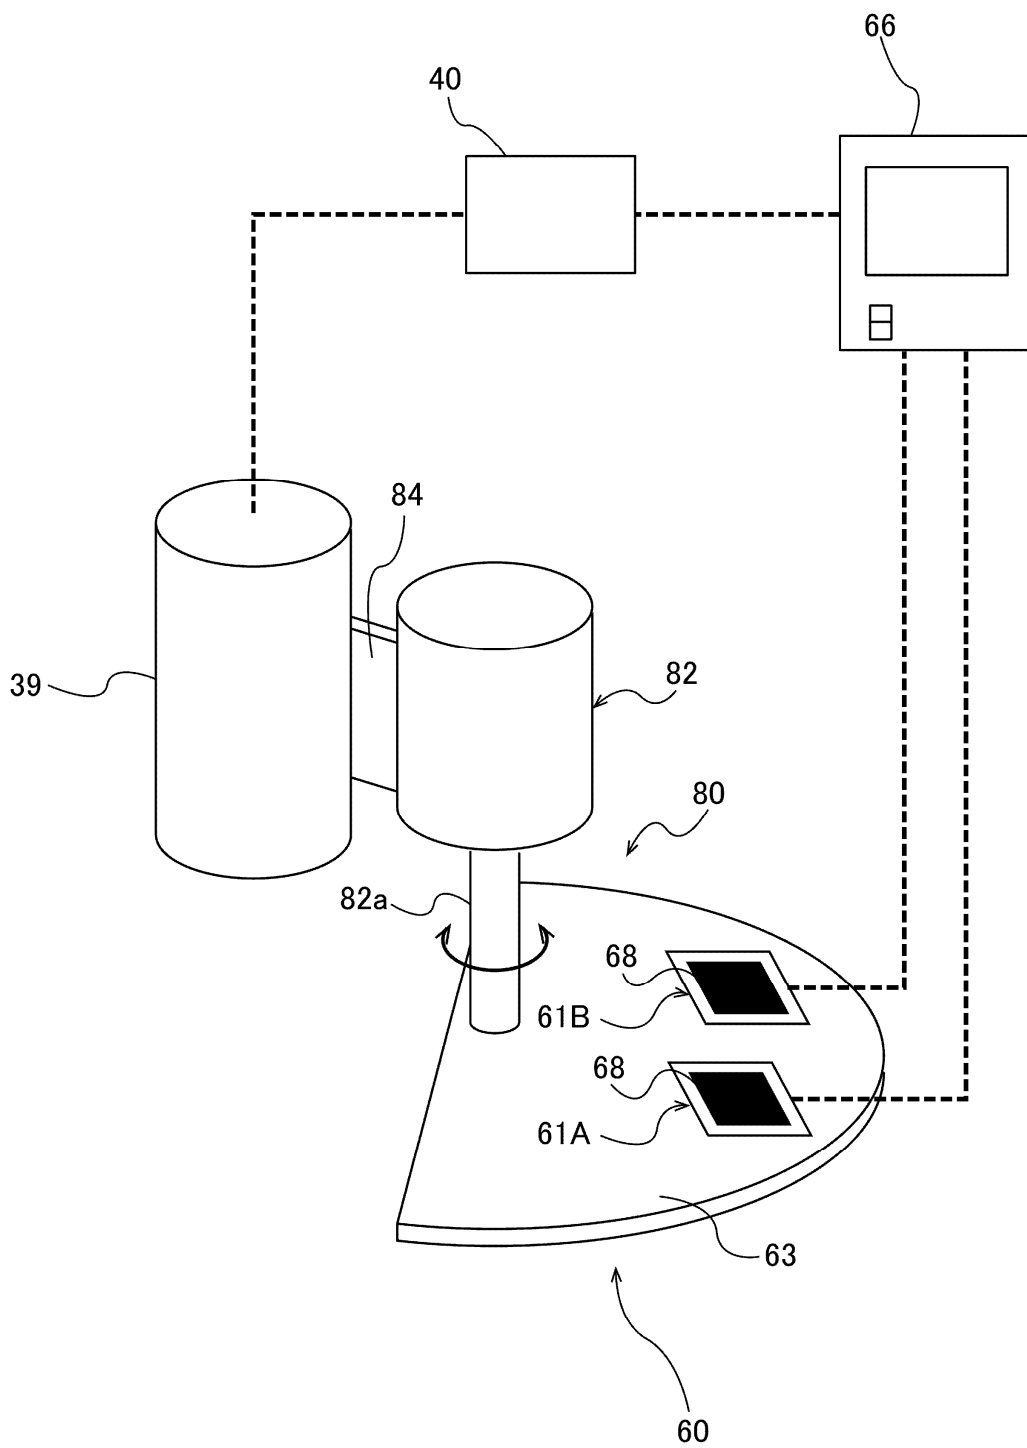


FIG. 14

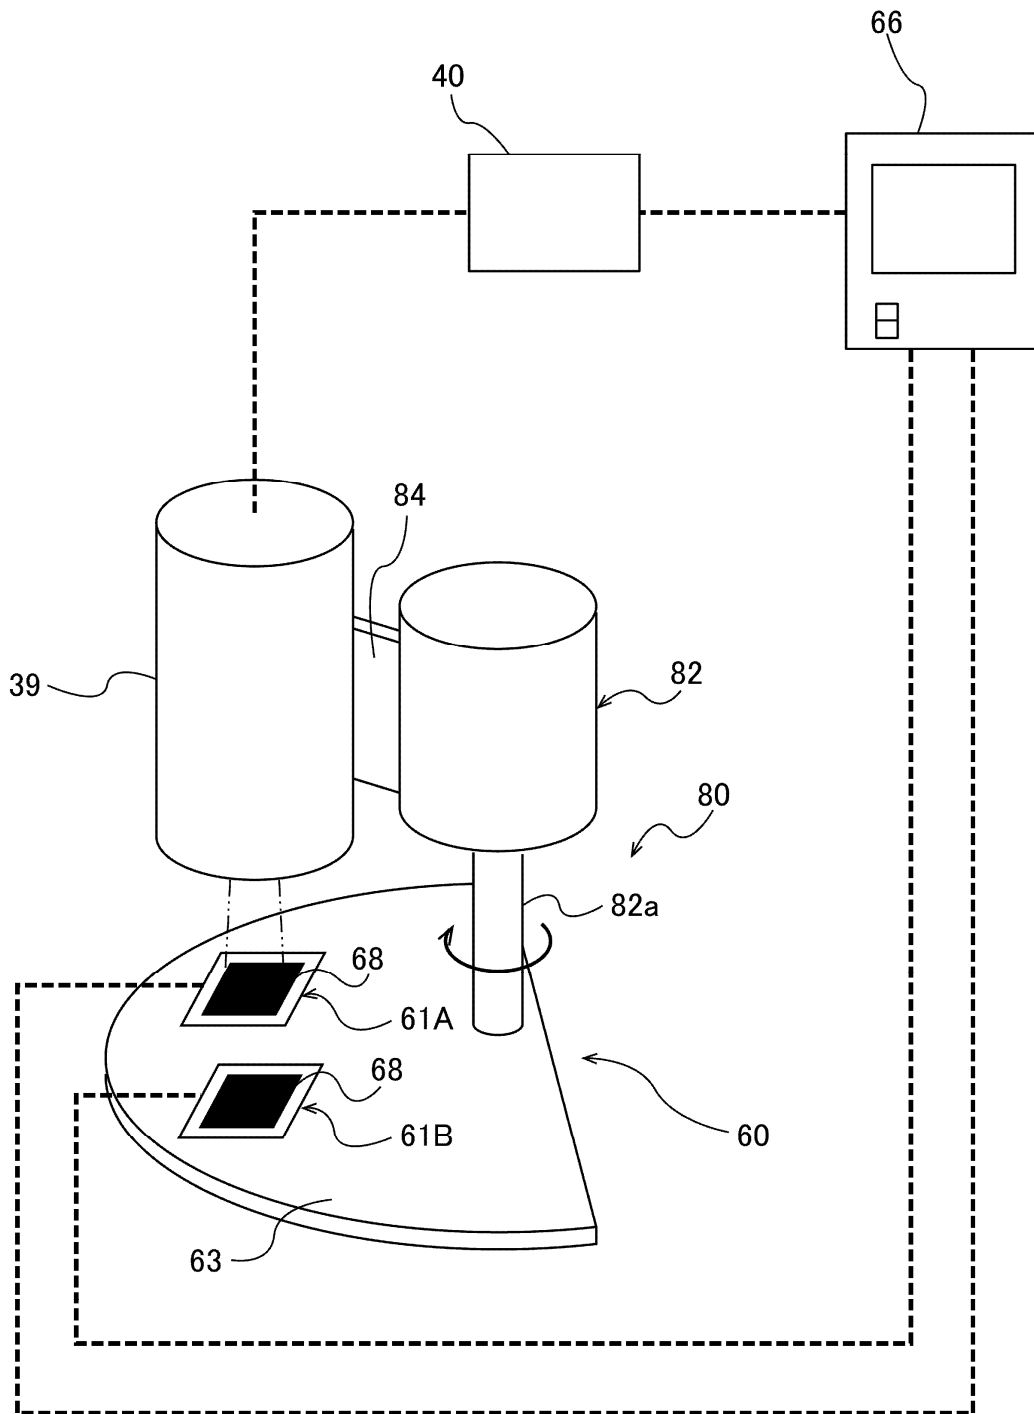


FIG. 15

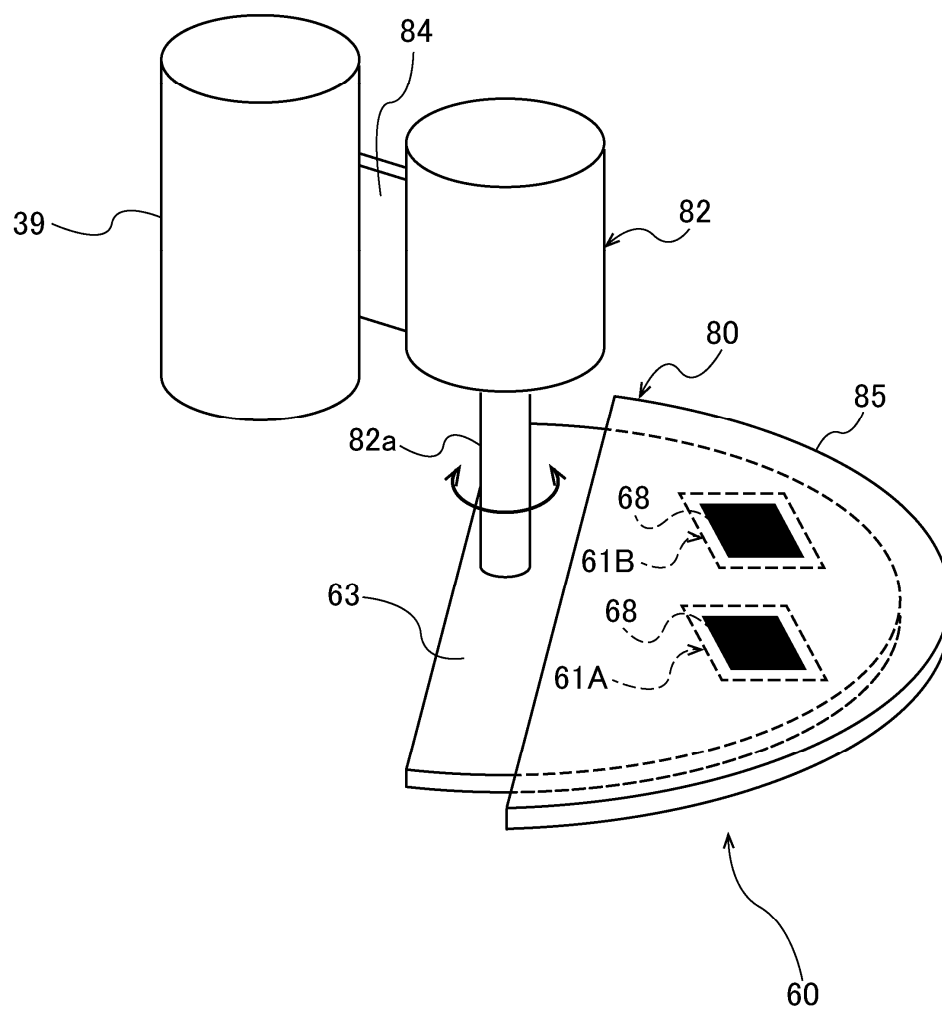


FIG. 16

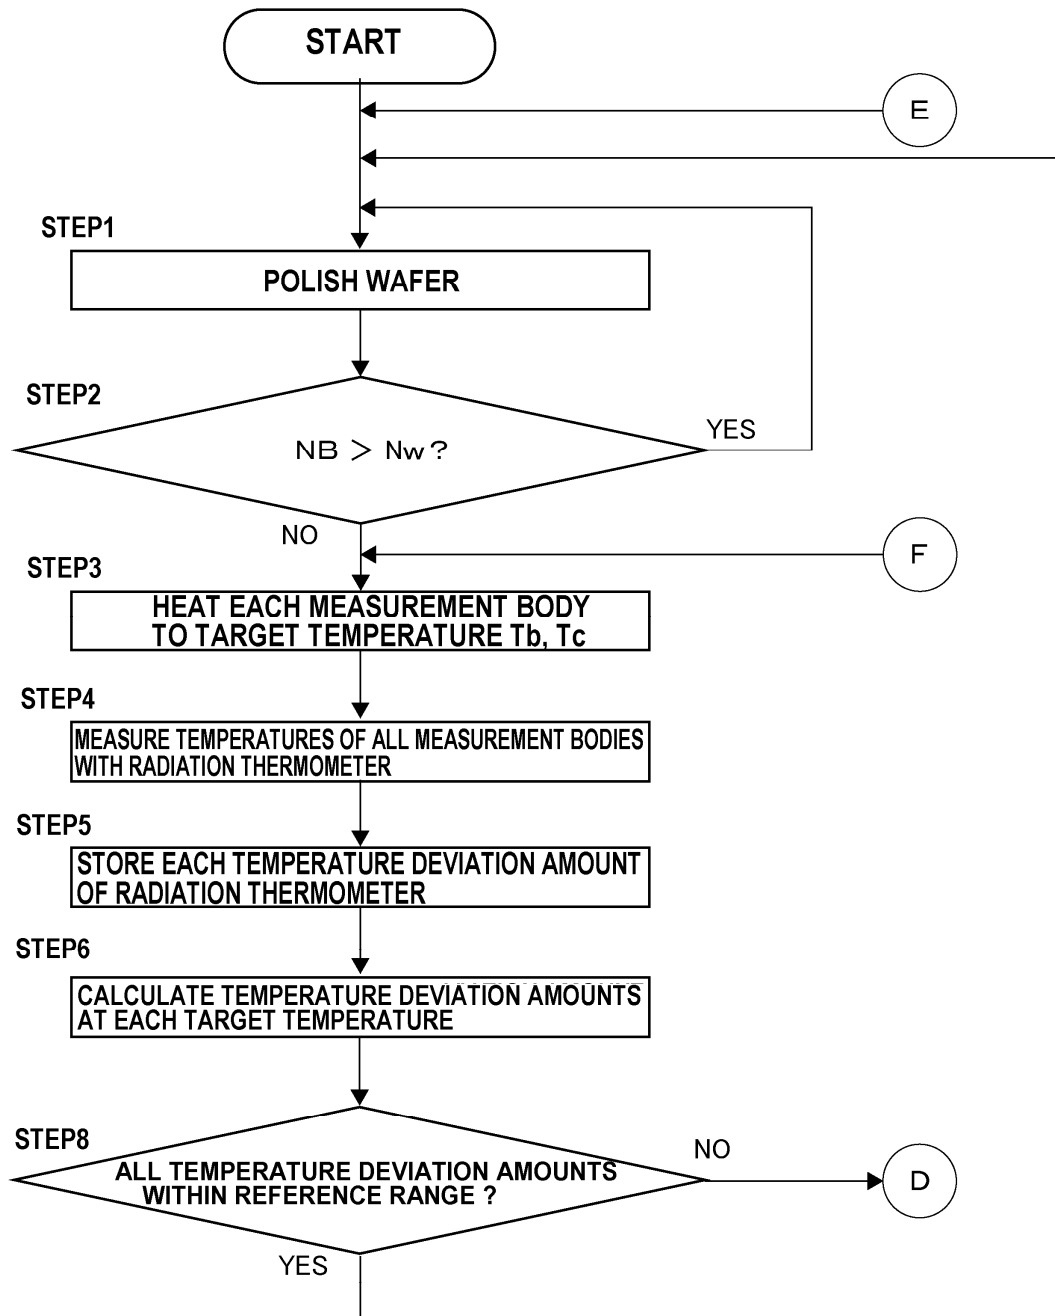


FIG. 17

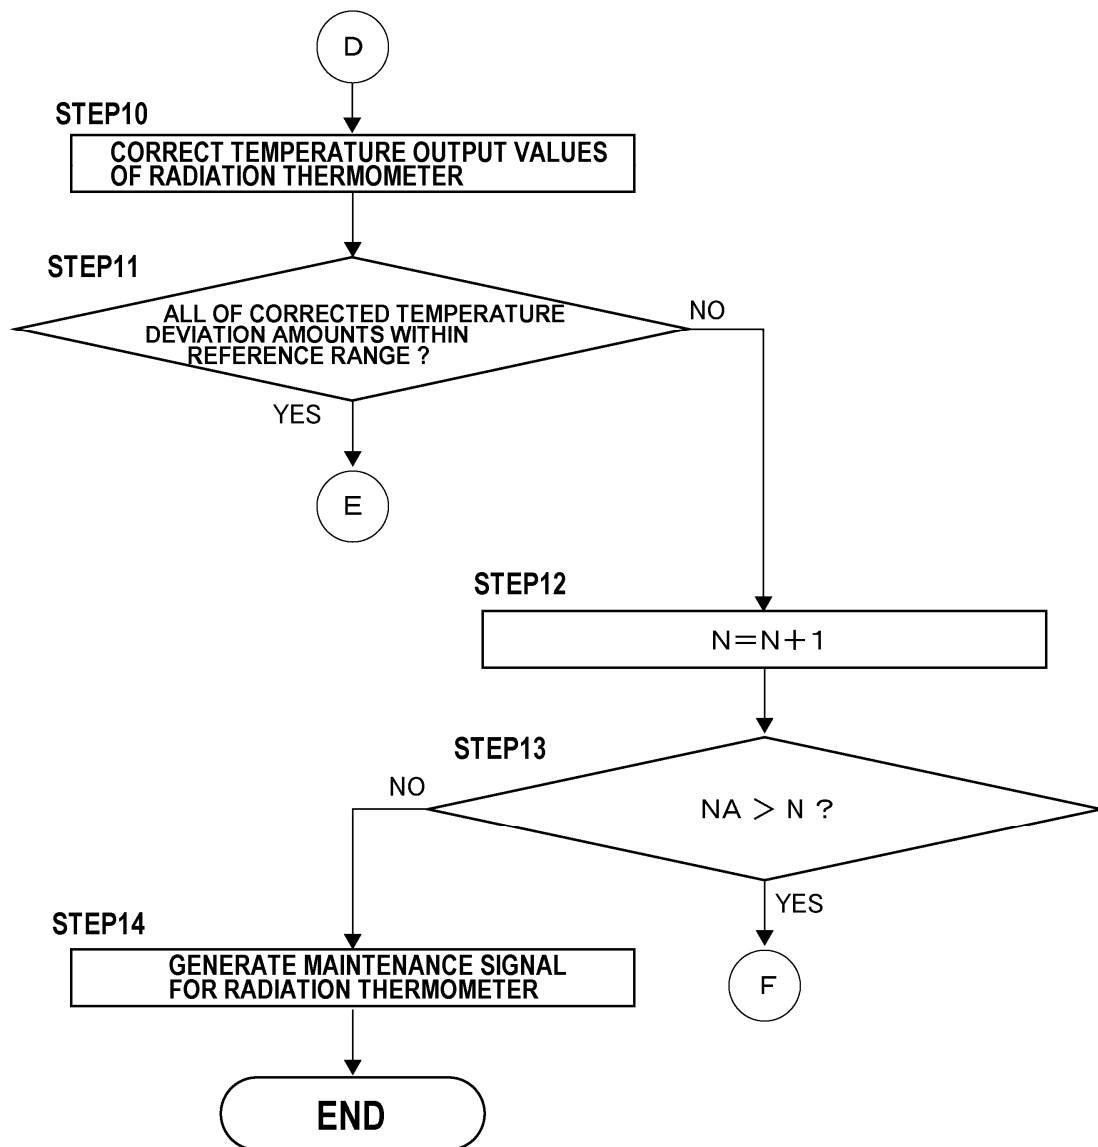


FIG. 18A

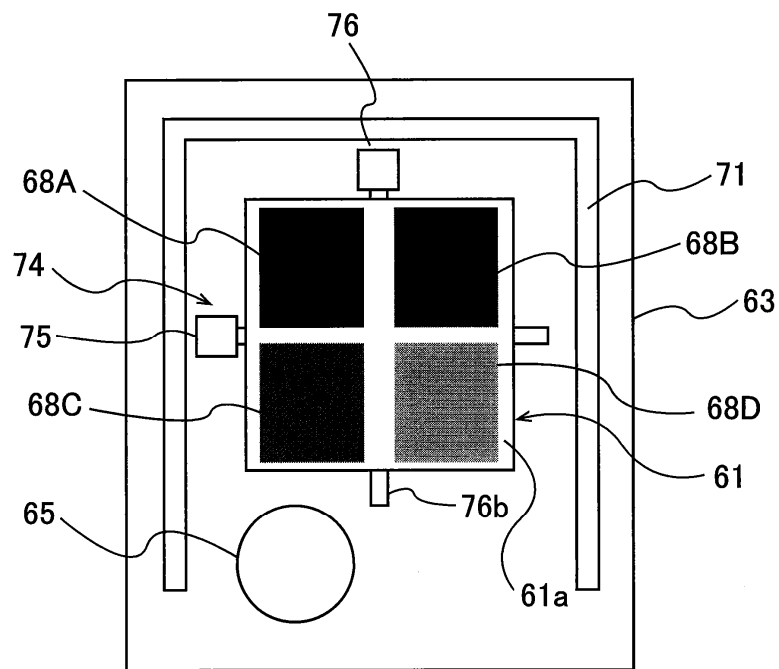


FIG. 18B

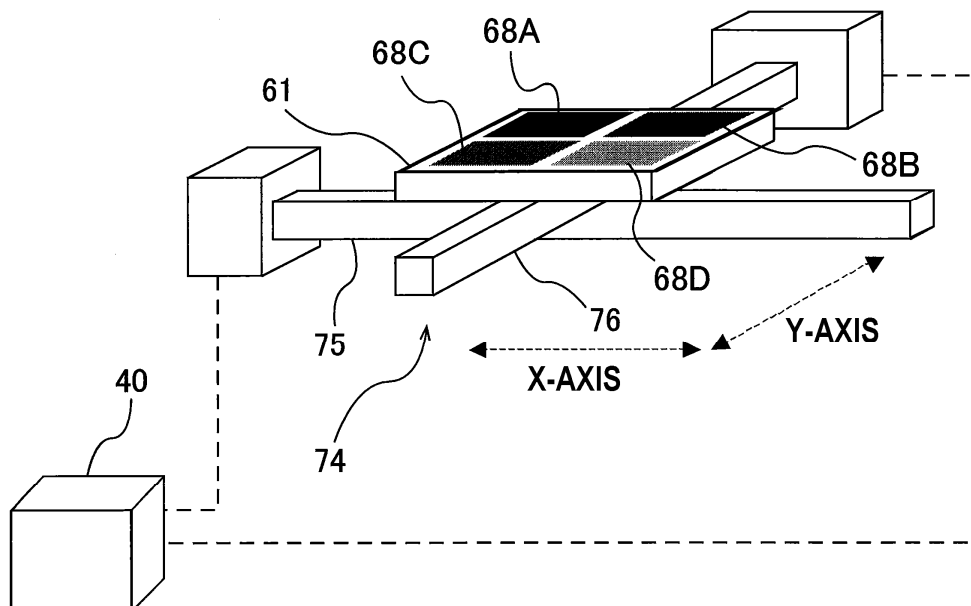


FIG. 19A

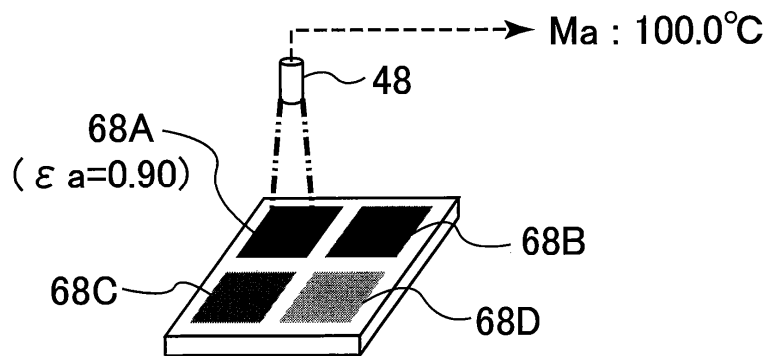


FIG. 19B

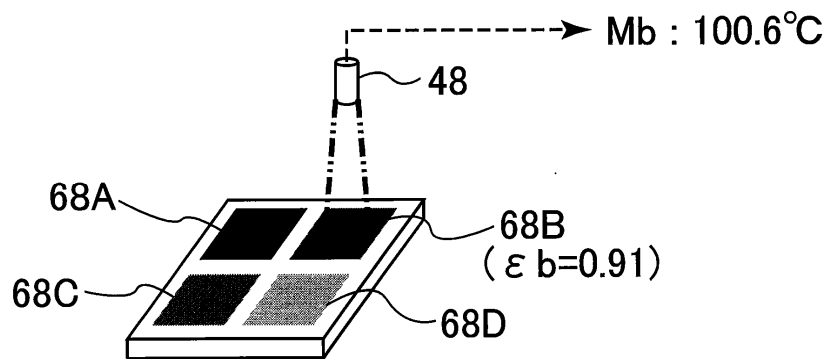


FIG. 19C

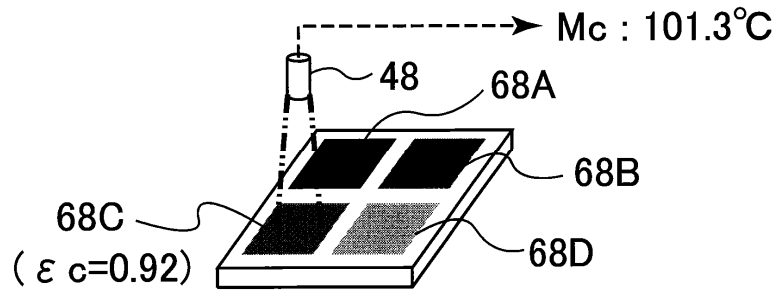


FIG. 19D

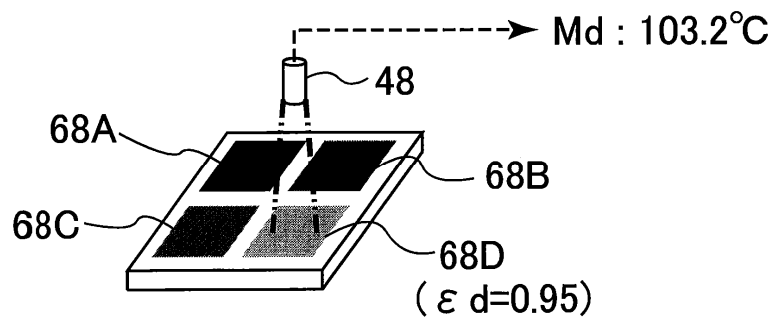


FIG. 20

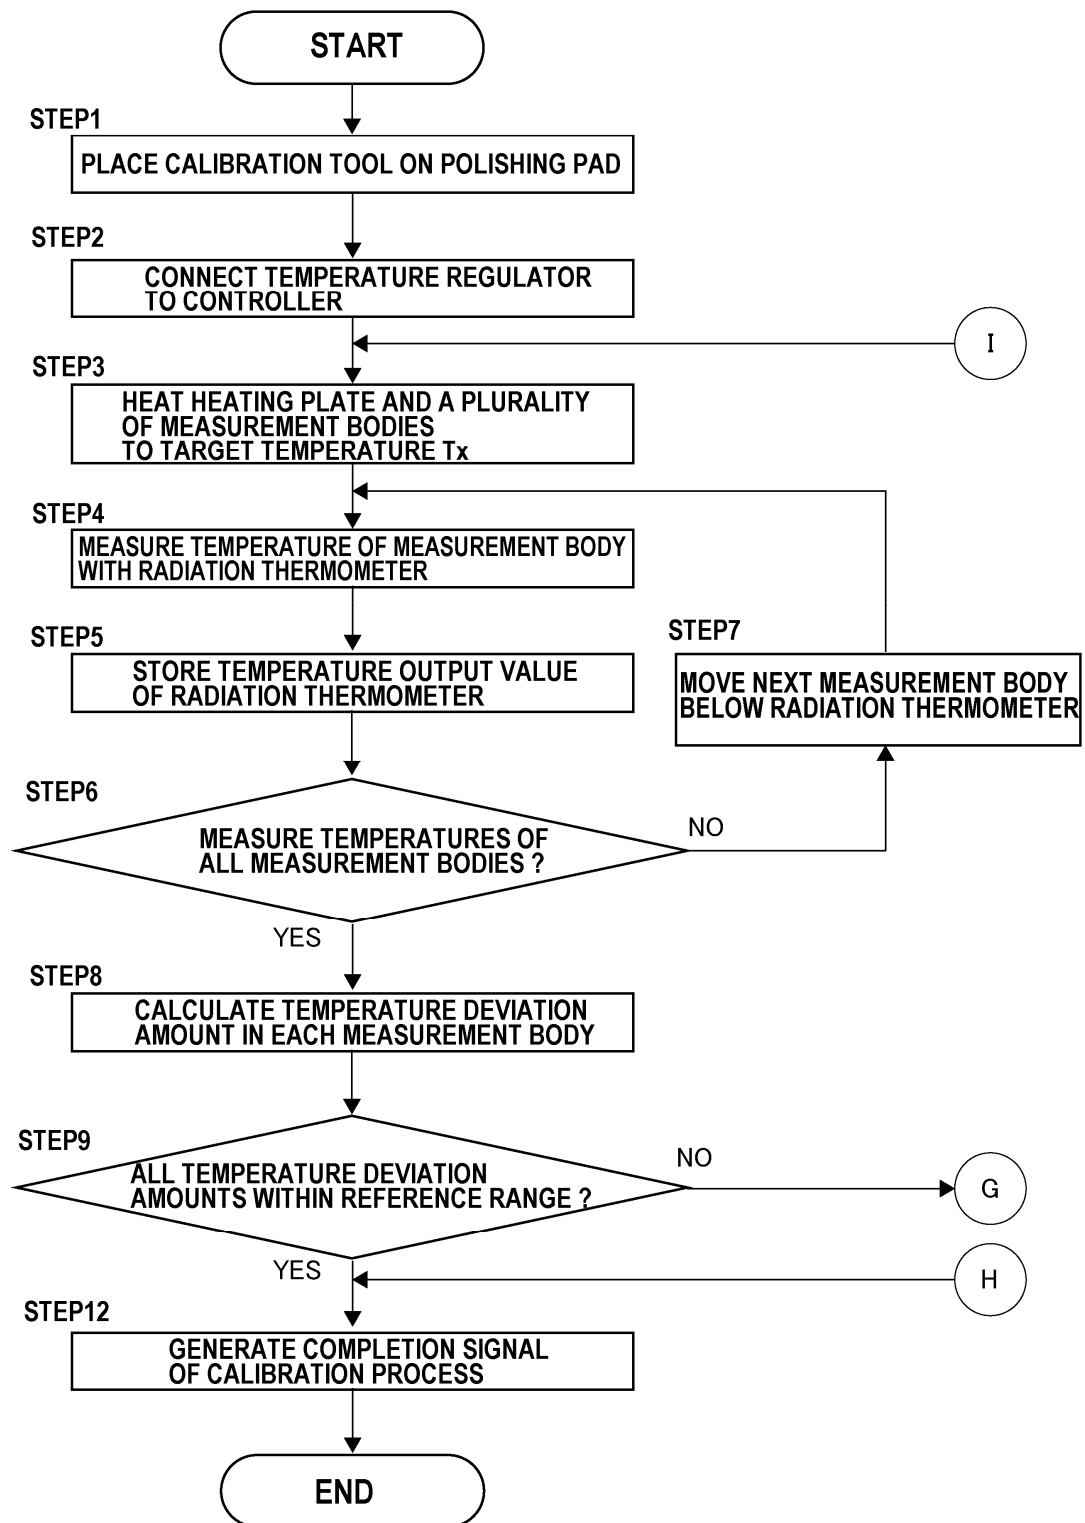


FIG. 21

