

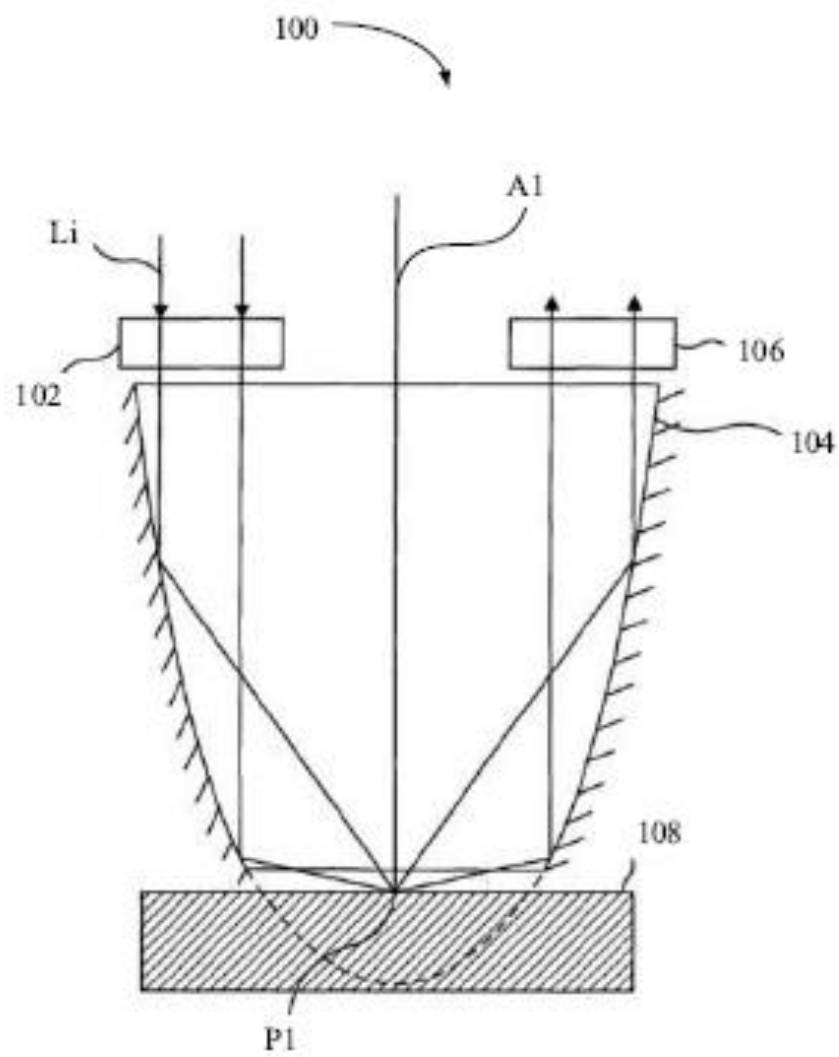


FIG. 1

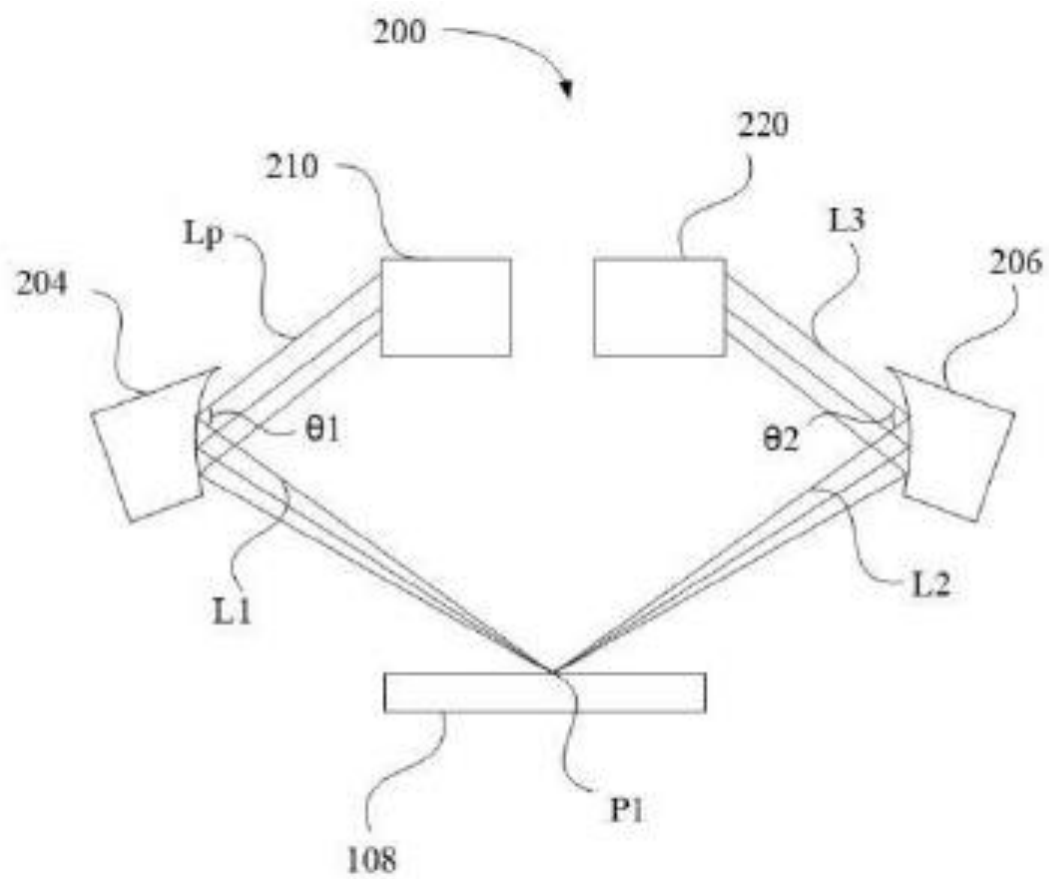


FIG. 2

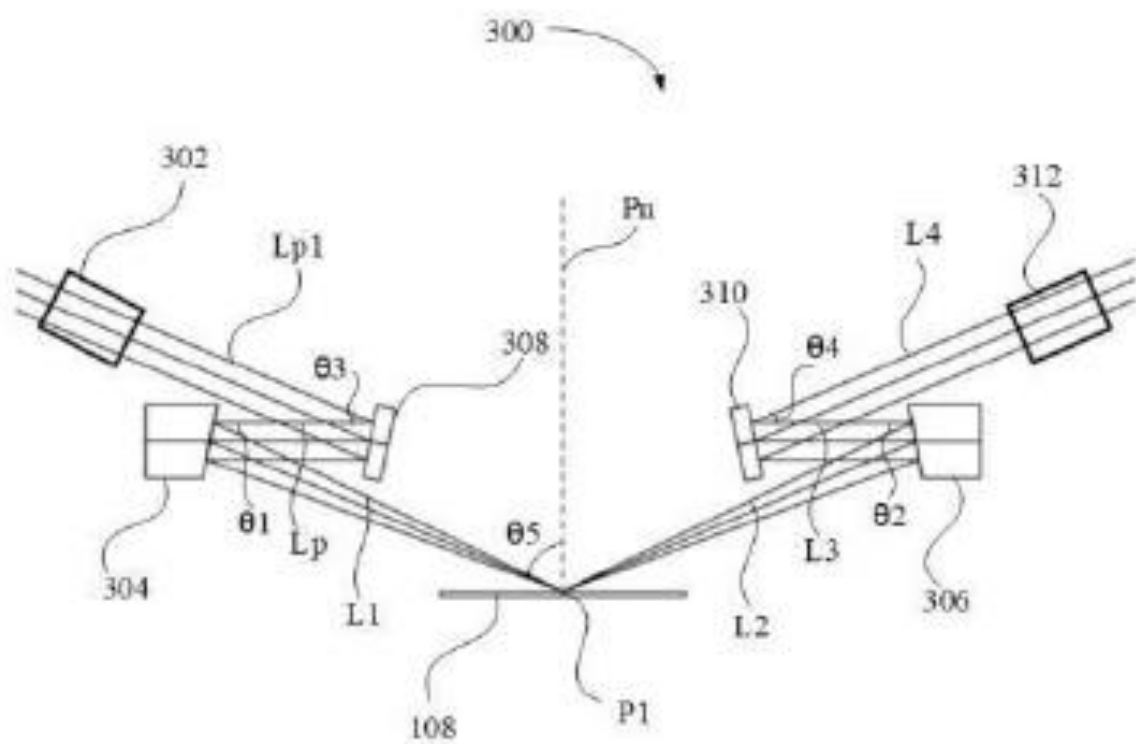


FIG. 3

Solution 1	190nm	234nm	368nm	607nm	854nm	1285nm	1900nm
Average value	1.94	1.06	7.54	6.37	5	4.22	3.64
Maximum value	2.17	1.19	8.51	7.18	5.64	4.76	4.1
Minimum value	1.74	0.95	6.68	5.65	4.43	3.74	3.23
Difference between the maximum value and the minimum value	0.42	0.24	1.83	1.53	1.2	1.02	0.88
Solution 2	190nm	234nm	368nm	607nm	854nm	1285nm	1900nm
Average value	1.94	1.06	8.81	7.39	5.8	4.89	4.22
Maximum value	2.17	1.19	15.84	13.19	10.35	8.73	7.54
Minimum value	1.74	0.95	3.93	3.32	2.61	2.2	1.9
Difference between the maximum value and the minimum value	0.42	0.24	11.91	9.87	7.74	6.53	5.64

FIG. 4



FIG. 5

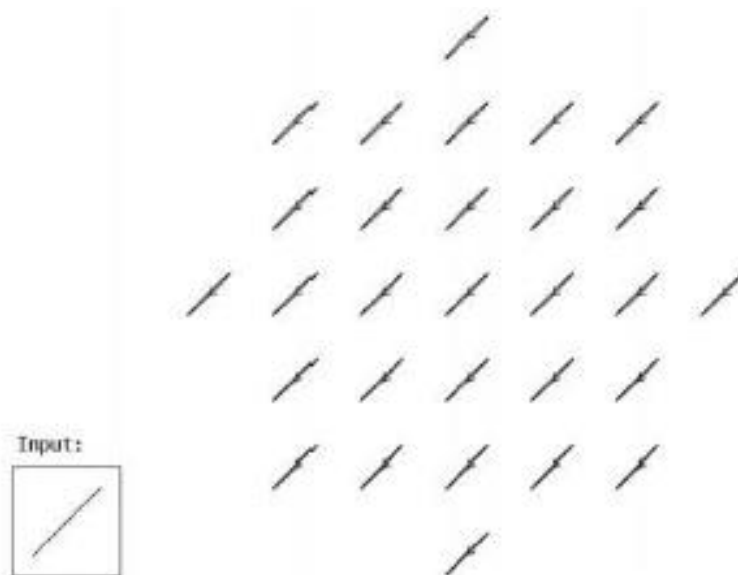


FIG. 6

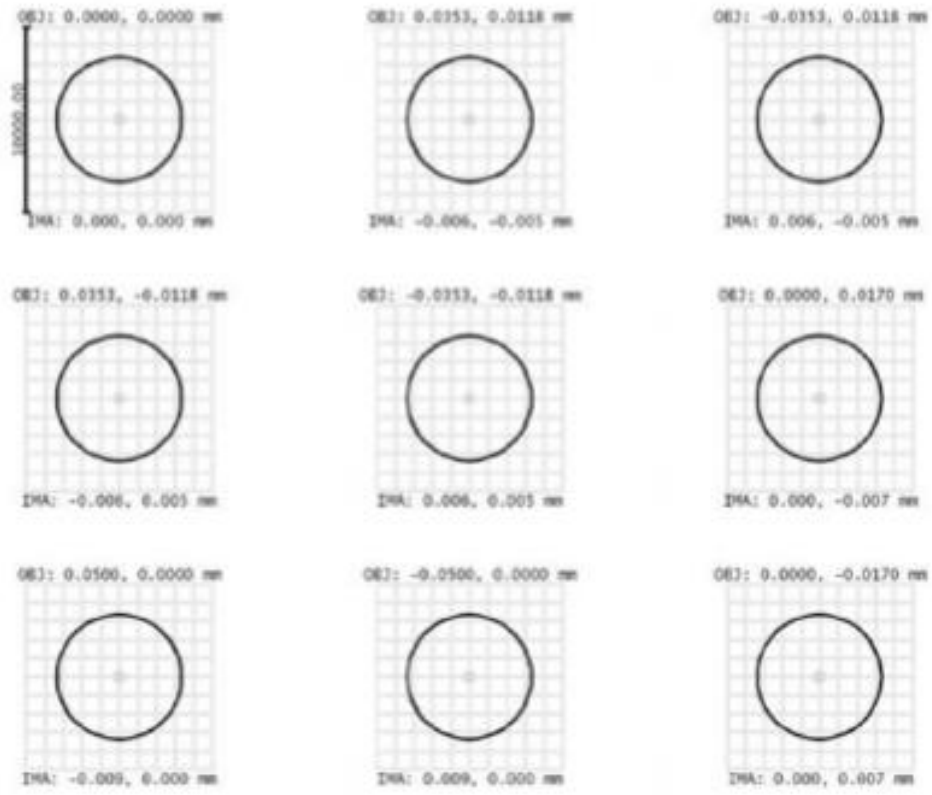


FIG. 7

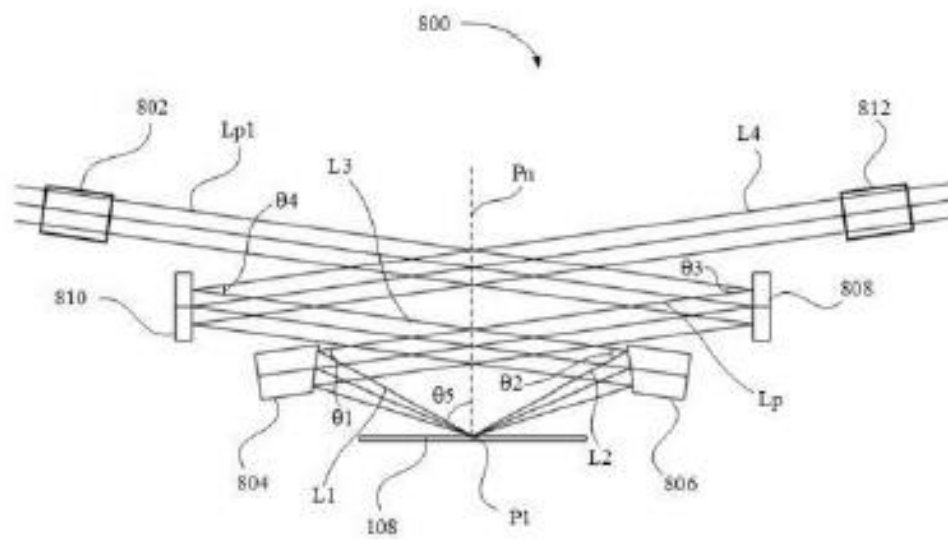


FIG. 8

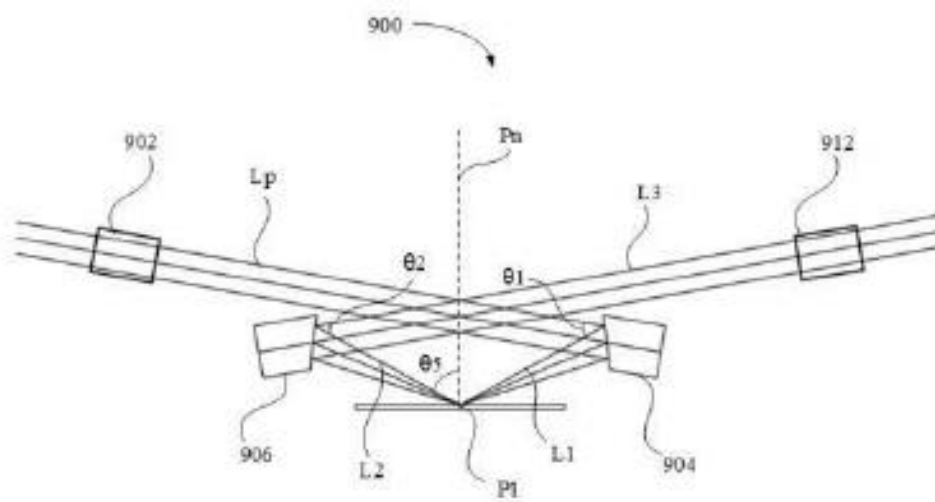


FIG. 9

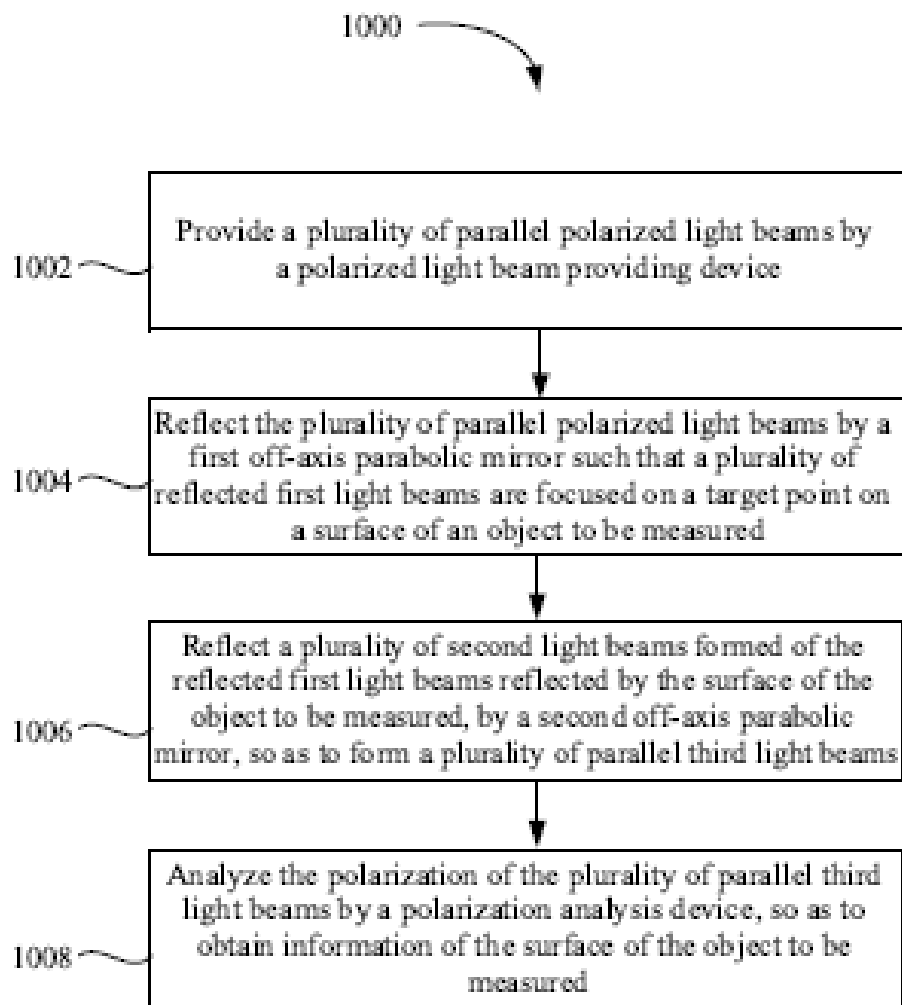


FIG. 10