URETERAL STENT WITH SMALL BLADDER TAIL(S)

Field of the Invention

This application relates to ureteral stents.

Background of the Invention

Ureteral stents are used to assist urinary drainage from the kidney to the bladder in patients with ureteral obstruction or injury, or to protect the integrity of the ureter in a variety of surgical manipulations. More specifically, stents may be used to treat or avoid ureter obstructions (such as ureteral stones or ureteral tumors) which disrupt the flow of urine from the kidneys to the bladder. Serious obstructions may cause urine to back up into the kidneys, threatening renal function. Ureteral stents may also be used after endoscopic inspection of the ureter.

Ureteral stents typically are tubular in shape, terminating in two opposing ends: a kidney (upper) end and a bladder (lower) end. The ends may be coiled in a pigtail or J-shape to prevent the upward or downward migration of the stent, e.g., with physiological movements. The kidney coil is designed to retain the stent within the renal pelvis of the kidney and to prevent stent migration down the ureter. The bladder coil sits in the bladder and is designed to prevent stent migration upwards toward the kidney. The bladder coil is also used to aid in retrieval and removal of the stent.

Ureteral stents, particularly the portion positioned in the ureter near the bladder and inside the bladder, may produce adverse effects including blood in the urine, a continual urge to urinate, strangury, and flank pain accompanying reflux of urine up the stent (e.g., when voiding) as pressure within the bladder is transmitted to the kidney. In short, stents may cause or

contribute to significant patient discomfort and serious medical problems. Figure 10 is a schematic drawing of the human urinary tract without a stent, showing the renal pelvis, the kidney, the ureter, and the ureteral orifices opening into the bladder. Figure 11 depicts a typical double-J stent 10 which comprises a small tube 12 which sits inside the urinary system and assists the flow of urine from the kidney (renal pelvis) to the bladder. Figure 12 depicts prior art indwelling ureteral stent 10 in position. Such stents are typically made of biocompatible plastic, coated plastic, or silicone material. Tube 12 typically varies in size from 4-8 fr. (mm in circumference), and it has multiple small holes throughout its length. A coiled shape pre-formed at each end 14 and 16 is designed to confine its movement within the urinary system, so that it will be maintained in the desired position. The upper (kidney) end 14 of the stent may be closed or tapered, depending on the method of insertion (e.g., the use of a guidewire). The tubular stent extends through the ureteral orifice 18a and into the bladder, fixing orifice 18a open, and thereby enhancing the opportunity for reflux. For clarity, the ureter entering bladder 20 through orifice 18b is not shown. A monofilament thread 22 may be attached to the bladder end of the stent for removal, usually without cystoendoscopy.

U.S. Patent No. 4,531,933 ("the '933 patent") discloses a ureteral stent having helical coils at each end which are provided for preventing migration and expulsion.

Summary of the Invention

We have discovered a ureteral stent design that avoids patient discomfort and urine reflux upward toward the kidney. Rather than rely on a tubular structure to contain and facilitate all (or, in some embodiments, any)

urine flow along the ureter, the invention features a thin flexible elongated tail member having an elongated external urine-transport surface. Urine flows along the outside surface of the structure, between that surface and the inside wall of the ureter. Without limiting ourselves to a specific mechanism, it appears that urine may remain attached to, and flow along, the external urine transport surface. The use of a foreign body that is as small as possible in the lower (bladder) end of the ureter and in the bladder itself decreases patient discomfort. Typically, the external urine transport surface is sized and configured to extend along at least part of the ureter near the bladder, across the ureter/bladder junction, and from there through the ureteral opening into the bladder.

While most or all of the length of the stent may rely on such an external surface to assist flow, more typically the stent will also include an upper elongated tubular segment to transport urine along a significant portion of the upper ureter. The upper tubular segment is connected at its lower end to an elongated tail which has the above described external urine-transport surface. The upper tubular segment comprises: a) an upper region having at least a first opening; b) a lower region having at least a second opening to be positioned in the ureter outside the bladder, and c) a central lumen connecting the first opening to the second opening. The elongated tail is a thin flexible tail member or filament(s) extending from the lower region of the tubular segment at a point outside the bladder so as to receive urine from the second opening of the tubular segment and to transport urine along the ureter from the lower region of the tubular segment across the ureter/bladder junction and into the bladder. Typically, but not exclusively,

the upper region of the tubular segment is configured and sized for placement in the renal cavity.

Typically the elongated tail member comprises at least one (and more preferably at least two) thread filament(s). Two or more of the filaments may be configured in at least one filament loop, and, advantageously, the tail comprises no unlooped filaments, so that the tail is free from loose ends. The loop(s) can be made by joining the ends of a single filament, in which case the filament loop comprises a junction of individual filament ends, which junction typically is positioned at the point where tail joins to the elongated tubular segment. Preferably, the tail is long enough to effectively prevent migration of the entire tail into the ureter, and the tail has a smaller outer diameter than the outer diameter of the tubular segment.

The tubular stent segment is stiff enough to avoid crimping during insertion through the ureter, so that it can be inserted by typical procedures. The tail, on the other hand, is extremely flexible (soft) in comparison to the tubular segment, and it has a much smaller diameter than the tubular segment to avoid discomfort. Even quite thin structures will provide urine transport, and the thinner and more flexible the tail is, the less likely it is to cause patient discomfort. On the other hand, the tail (and its connection to the rest of the stent) should have sufficient strength so the stent can be retrieved by locating the tail in the bladder and pulling on the tail to retrieve the stent from the kidney and ureter. Details of the tail size are discussed below. The use of reinforcing materials (e.g., sutures as described below) permits the use of thinner tails while still providing the ability to locate the tail in the bladder and to retrieve the stent. The tail may be a suture, and the suture may be coated to avoid encrusting.

The external urine-transport surface of the tail can be convex (circular or oval in section), concave or flat. The tail filament may be fluted. The tail may, but need not, include an accurately shaped anchor segment to control migration up the ureter. The tail may be either solid or hollow; even when hollow, it is not designed to transport a significant amount of urine internally. The tail may also be tapered.

The upper region of the tubular segment may have a portion designed for placement in the renal cavity, which portion has enlarged diameter and/or straight sides and corners. The stent may include an extractor thread attached to the lower end of the elongated tail member.

To make the stent, the tail may be molded in one piece with the tubular segment, or it may be made separately and attached to the bladder end region of the tubular segment at a point toward the kidney from the bladder end of the lower region of the tubular segment. In one specific embodiment, the tail is attached near or at the bladder end of the bladder end region of the tubular segment. The stent may include a suture securing the tail to the tubular segment, and the suture may be incorporated into the tail to impart strength to the tail so the tail may be used to retrieve the stent. If the tail includes a hollow lumen, the suture may be positioned inside that lumen. The suture may be attached to the tubular segment at a point in the bladder end region of the tubular segment, and the suture may extend from the point of attachment through an opening in the bladder end region to the central lumen of the tubular segment and from there to the hollow tail. Alternatively, at least the bladder end region of the tubular segment may include two lumens, a main urine-transporting lumen and a bladder lumen to encase the suture, so that the suture does not become encrusted.

The outer diameter of the tubular segment can be tapered so that it decreases approaching its lower region. The lower region of the tubular segment may include multiple openings positioned, e.g., axially along include its length or radially around its circumference, or in other patterns. In addition, the outer diameter of the stent's tubular segment may decrease approaching the upper region. In other words, the maximum diameter may be at the site of the injury to encourage a sufficiently large inner diameter in the repaired structure, and the tubular segment's outer diameter may decrease moving away from that point of maximum diameter to sections of the normal ureter that are not in need of a broad support structure. Typically, the outer diameter of the upper end of the tubular segment will be greater than the outer diameter of the bladder end. The upper region may include multiple openings (inlets).

In an alternative embodiment, the elongated external urine-transport surface is a continuous surface extending from the kidney to the bladder, e.g., it is the outer surface of a solid member extending from the kidney to the bladder.

Another aspect of the invention features a method of introducing a ureteral stent (described above) into a patient, by (a) positioning the kidney end region of the tubular segment within the renal pelvis; and (b) positioning the elongated flexible member(s) in the bladder.

Yet another aspect of the invention features a method of manufacturing a ureteral stent as described above. The method comprises: (a) providing a polymer pre-form having a tubular shape; (b) forming an elongated tubular stent segment from the polymer pre-form, and (c) providing tail member(s) at an end region of the tubular

segment designed to be positioned toward the patient's bladder.

As described in greater detail below, the stent may be manufactured from a polymer form having a tubular shape by forcing the form onto a mandrel to produce the desired three dimensional shape (coils, etc.). The elongated tubular member(s) is attached to one end of the tubular member(s) using sutures as described above. Heat treatments to fuse the structures and/or standard adhesives may be used. Alternatively, the tubular member(s) and the elongated member constitute a one-piece stent.

The use of relatively thin, flexible elongated member(s) to assist urine flow across the ureterovesical junction and into the bladder may reduce reflux and irritation and thereby reduce patient discomfort and medical problems associated with ureteral stents.

Other features and advantages of the invention will appear from the following description of the preferred embodiment, and from the claims.

Brief Description of the Drawings

Figure 1 is a side view of a ureteral stent with a central portion of the tubular segment omitted.

Figure 2 is a cross-sectional view along line 2-2 in Figure 1.

Figure 3 is an enlarged side-view of a portion of the ureteral stent in Figure 1.

Figure 4A is a view of an alternate embodiment of the stent in Figure 1, and Figure 4B is a section taken along 4B-4B of Figure 4A.

Figures 5A and 5B are schematic representations of another stent according to the invention, depicted in place.

Figures 6A-6D depict alternative cross-sections of the tail of a stent according to Figure 5.

Figure 7 is a schematic representation of yet another stent according to the invention, having an extraction thread.

Figure 7A is an enlargement of a portion of Figure 7.

Figure 8-8 is a schematic representation of the stent of Figure 7 shown in position.

Figure 8A is a detail of the connection between the tail and the extraction thread.

Figure 8B is a cross-section of threads of differing softness, showing the effect of compression on interstitial space.

Figure 9 shows an alternative embodiment of the stent.

Figure 10 is a schematic drawing of the human urinary tract without a stent, showing the renal pelvis, the kidney, the ureter, and the ureteral orifices opening into the bladder.

Figure 11 depicts a prior art double-J stent outside the body.

Figure 12 depicts a prior art J indwelling ureteral stent in position.

Description of the Preferred Embodiments

In Figure 1, ureteral stent 100 includes an elongated tubular body 130 connecting coil end 140 to straight end region 120. Tubular body 130 is designed to extend from the renal pelvis through the ureter to a terminus upstream of the bladder. Tail 110 is attached to straight end region 120, and tail 110 extends along the ureter, across the ureter/bladder junction and into the bladder.

The two opposing end regions 120 and 140 of elongated tubular body 130 are illustrated in Figure 1. Coiled end region 140 is designed to be placed in the renal pelvis of the kidney. For illustrative purposes,

coiled end region 140 is shown with a pigtail helical coil although any shape that will retain the stent in place within the kidney will do. Coiled end region 140 includes several openings 125 placed along the wall of the tubular body; the openings may be arranged in various geometries (e.g., axial, circumferential, spiral). The entire tubular segment, including the region between the kidney and the bladder end regions, may include additional openings.

The bladder end region 120 of the tubular stent segment is designed to terminate in the ureter, upstream of the bladder. For purposes of further description, the end region of stent 100 received in the kidney will be designated the kidney end and the opposite end of stent 100 toward the bladder will be termed the bladder end.

Figure 2 is a cross-sectional view of stent 100 of Fig. 1. In Fig. 2, elongated tubular body 130 has annular walls 250 having an inner and outer diameter. The outer diameter of tubular body 130 may be substantially uniform throughout much of the length of the tube, or it may taper from a relatively short region of larger diameter (the site of the repair, where there is a risk that the healing process will substantially restrict flow in the lumen) to a region of generally small diameter. The precise configuration may depend on the ureteral defect being corrected. Just one of the many classes of procedures that can benefit from the stent are endopyelotomies -- procedures for treating ureteropelvic junction (UPJ) obstruction by an incision which perforates the ureter at the stricture. In these and other procedures, the stent keeps the ureter lumen open during the healing process, so that the inner diameter of the resulting healed structure is adequate. The section of the tubular segment at the defect is large enough to support growth of repair tissue having an

adequate inner diameter. At other sections of the ureter (e.g., sections not being surgically repaired), the outer diameter of the tubular segment may be far smaller, but with an inner diameter adequate for passage over a guidewire. For example, the outer diameter of the bladder end region of the tubular segment typically is 2Fr.-12Fr. Preferably the outer diameter of tubular body 130 is greatest at the ureteropelvic junction obstruction but begins to taper approaching each end. Alternatively, for a patient with an upper ureteral obstruction, the upper (kidney) portion of the tubular member 130 may be uniform in diameter, tapering just in the lower (bladder) portion.

Tubular member 130 defines a central lumen or passageway 260, extending from kidney end region 140 to bladder end region 120. The inner diameter of lumen 260 is sufficient to permit passage over a guidewire. Tubular body 130 may also have openings 125 extending through its walls 250 to facilitate the flow of urine from the kidney into central lumen 260 and openings 127 to facilitate flow out of central lumen 260.

In Fig. 3, the outer diameter of elongated tubular body 130 tapers near bladder end region 120. The outer diameter of bladder end region 120 may be made as small as possible while maintaining the ability to pass over a guidewire. Elongated tubular body 130 may (but need not be) substantially straight in bladder end region 120, i.e. it does not coil or curve in the absence of external force. When tail 110 is a single filament, it typically is thinner than even the smallest portion of bladder end region 120 of the tubular stent segment. Alternatively, it may be desirable to design the tail from multiple filaments, each of which, by itself, is much thinner than the bladder end region of the tubular stent segment. Together, such a multi-filament tail has a larger

effective diameter, providing additional bulk while maintaining comfort. Tail 110 may be attached at or near the end of region 120, and it extends from that attachment into the bladder. Tail 110 is either solid or hollow. It can be generally cylindrical in shape; alternatively, it can be fluted, concave (quarter-moon)-shaped or it may assume other shapes.

The tail can have an outer diameter that is significantly less than the inner diameter of the ureter (typically 2-5mm) and no greater than the outer diameter of the tubular segment from which it extends. For example the tail diameter is less than 10Fr. and as low as a suture (about 0.5Fr). Preferably the tail diameter is between 2Fr. and 4Fr. The length of tail 110 is preferably between 1 and 100cm. In one embodiment, the tail is long enough so that at least a portion of it will remain in the bladder, and effectively the entire tail cannot migrate up into the ureter. Preferably the length is between 1 and 40cm. Tail 110 is flexible and, upon application of force, can be curved, but also has memory such that when the force is removed, it is generally straight.

Stent 100, including tail 110 and tube 130, may be a single unit. Thus, tail 110 can be a unified piece, extending from bladder end region 120 with no additional attachment means. Alternatively tail 110 can be secured to elongated tube 130 or bladder end region 120 by physical or mechanical methods.

For example, in Fig. 4A, a suture 415 is inserted through an opening 418 in the tubular member and then threaded through the lumen 417 of tubular member 430. In Fig. 4B, tail 410 is a hollow member having suture 415 threaded through its inner lumen 412.

Fig. 5 is a schematic of another stent 510. The kidney end A of the stent has a pre-formed memory bend,

to coil 512 as shown. Kidney end A is larger and more rectangular to help prevent upward as well as downward stent migration. End A may be closed or tapered to accommodate various insertion techniques. For the upper portion (A--B) of the stent, diameter, lumen size, perforations and materials are conventional. The lower end 514 of the tubular stent segment ends at B. The distance A--B could vary depending on the patient's anatomy. At B, the stent is tapered (or at least smooth and constant in diameter).

Two or more monofilament or coated (plastic or silicone) threads 516 exit from the lumen or from the stent wall. These threads only partially fill the ureter and are as flexible (soft) as possible. Typically, they are cut to a length which forces confinement within the bladder.

The portion of the upper segment 512 lying within the renal pelvis (e.g, from the kidney end of the stent to point A) is expanded so that it is larger in section, and it may even be oval or rectangular in cross-section, to help prevent upward as well as downward stent migration. The kidney end of the stent may be closed and/or tapered to accommodate the desired insertion technique. The upper portion 512 is made of a relatively stiff material (among the materials currently used in ureteral stents), and it should be designed to effectively restrict the motion of the stent to prevent proximal as well as distal migration of the catheter during normal physiological activity (required because the lower pre-formed portion is deleted). The length of the straight portion of the upper segment (Fig. 5A point A to B) will vary with patient size and anatomy. In the preferred configuration, the upper segment extends more than halfway down the ureter when in proper position. The lowest end of the upper segment (Fig. 5A point B)

should be tapered or beveled to facilitate withdrawal. Otherwise, the upper segment is a typical stent in diameter, materials and shape.

The lower segment (Fig. 5A point B to point C) consists of two or more (e.g four) monofilament, plastic coated or silicone coated threads (shown in section in Fig. 5B) which extend from the lumen or sidewall of the lower end of the upper segment (Fig. 5A point B) along ureter 513 into the bladder. These threads are extremely flexible, and their diameter is selected to maintain a passage for urine flow and yet drastically reduce bladder and ureteral irritation. By avoiding distortion of the ureter wall, the threads may inhibit urinary reflux as well. The threads should be long enough to reach well into the bladder (Fig. 5A point C), but not so long as to wash into the urethra with voiding. One thread 518 (or two or more threads in a loop) may be long enough to exit through the urethra (Fig. 5A point B to point D) to permit ready removal by pulling (avoiding cystoendoscopy).

These extended threads may also be used for stent exchange, in which a second catheter is exchanged for the catheter already in place. According to that procedure, these extended threads are captured with a snare that has been inserted through the central lumen of a second catheter. The snare is used to pull the threads through the lumen as the second catheter is advanced into the ureter. A guidewire is then inserted through the central lumen of the second catheter to the kidney (outside the first catheter's tubular body). The first stent is then removed by pulling on the threads, leaving the guidewire in position for placement of a new stent using standard techniques.

Figs. 6A-6D are alternative cross sectional sketches (taken at the same location as Fig. 5B) of some

possible arrays of threads passing within the lower ureter 517. Multiple threads 516 (2 and 4, respectively) are shown in Figs. 6A and 6B. A substantially similar conduit could be achieved by fluted type cross sections in a single filament Figs. 6C and 6D). The shapes of Figs. 6C and 6D could also be effective in reducing stiffness and hence irritability at the bladder end (i.e., lower segment), e.g., in a single filament design. Multiple threads may have the advantage of better surgical manipulability and superior comfort to the patient.

Further refinements are described below and in Figs. 7 and 7A which deal with: a) proximal or upward stent migration of either the entire stent or individual threads in the lower segment independent of upper segment movement; b) bunching of one or more threads within the ureter so as to obstruct flow or cause ureteral injury or knotting at the time of removal; and c) in multi-thread embodiments, discomfort and/or reduced drainage through the ureter resulting from the use of threads of different lengths. In Fig. 7, 6 F (F = French size = circumference in mm) stent is a generally a good size for adult urinary systems. It is large enough to provide good drainage and small enough to minimize local irritation and inflammation of the ureter. In this embodiment, the upper segment need be only a single loop of conventional size because a change in the design of the lower segment (see later discussion and Fig. 8) should prevent proximal migration. The upper segment (Fig. 7 point A to point C) is constructed of a relatively firm material because, during insertion, the pusher tubing should be removed after the guidewire is removed. This means that there will be some drag on the threads during removal of the pusher tubing which could dislodge the stent if the coil (Fig. 7 point A to point B, about 2.5 cm) does not

provide adequate resistance. The coil may be tapered or closed depending on the insertion technique desired (i.e., over a previously placed guidewire.

Fig. 7 point B to point C should have an approximate length of 12 cm. This is long enough to prevent dislocation of the upper segment in a large renal pelvis and short enough to end well above the point where the ureter crosses the common iliac vessels. At the iliac vessels, the ureter takes a fairly sharp turn and the threads will more easily follow the natural curves at this point. This design should reduce the inflammation that is normally seen in this region when a conventional double-J stent is left indwelling on a chronic basis.

The junction of the upper and lower segments at Fig. 7 point C is important. See Fig. 7A, which enlarges this junction. At point C (Fig. 7) the threads are attached to the upper segment in a manner that achieves the following goals: 1) the threads are securely attached to the upper segment and to each other (at least for a short distance of about 0.8 mm) so that their orientation to themselves is maintained (to the maintenance of lower end asymmetry); 2) the threads do not obstruct the lumen of the upper segment and they allow for the easy passage of a standard guidewire (e.g., 0.035 guidewire); 3) the transition diameters in this region closely preserve the 6F standard so that this point can pass in both directions smoothly throughout the instruments used for insertion and through the ureter; 4) there is no cause for a localized ureteral obstruction; and 5) there is an effective abutment for the pusher tubing. For an average size ureter a good starting string diameter for a four string lower segment (Fig. 7 point C to point E) would be 0.020 inches. A simple monofilament nylon thread is an easy potential solution but may be too stiff. A more supple monofilament or woven thread with silicone or

other coating may be required to achieve minimal irritability. However, the threads should be sufficiently resistant to compression so that tissue generated pressures cannot collapse the interspaces of the threads. See Fig. 8B, showing cross-sections of threads (left) which retain interstitial space under some modest compression and of threads (right) which are so soft that they compress into a plug with reduced interstitial space. These threads may have centimeter markings beginning at a point no more than 20 centimeters from point B (Fig. 7) so that functional ureteral and total stent length may be noted.

The portion of the lower segment which lies within the bladder when the stent is in proper anatomic position (Fig. 7 point D to point E) is important to both comfort and function. Proximal migration can be controlled by using asymmetrical lengths of the thread pairs, with one pair being 2 cm longer that the other pair, so that the fused junction of these threads tends to intersect with the ureteral orifice at and angle (e.g., ~90°) with the stiffened length of 6 mm (see detail Fig. 8B). In the ideally fitted stent of this embodiment, the thread pairs will extend beyond the ureteral orifice (Fig. 7 point D) by 1 cm at the short limb and 3 cm at the long limb. However, this lower segment configuration allows for considerable tolerance in sizing (unlike unsecured independent threads which must be selected to have a length so as to avoid upward migration of the thread through the ureter orifice) and a chosen length which is 1 cm shorter or 2-3 cm longer than the ideal length should be satisfactory. Using this configuration the threads should form a continuous loop of 3.5 cm length to prevent free ends from poking the bladder wall or prolapsing through the urethra. Buoyant threads may add to patient comfort, because they will float away from the

trigone region of the bladder, where most of the sensory nerve fibers are located. A typical small gauge filament extraction thread may be attached to the longer limb of the thread pairs, which is a suitable pulling point for removal.

From this embodiment, a small diameter pusher tubing of 4--4.5 F should be used to aid insertion. Soft percuflex is near optimal for the lower segment, and firm or regular percuflex is used for the upper segment.

The bladder end should be easily inserted using instruments, and it should prevent proximal migration of the stent. The design of Fig. 7 will avoid tangling and migration of the stent. Alternatively, soft percuflex, for example, has good resistance to extreme flexion at small radii (e.g., even 0.020" diameter) so that a simple continuous loop extending from the junction of the upper and lower segments (see Fig. 9) may be adequate to prevent upward migration. The design of Fig. 9 also has the advantage of relative ease of manufacture and relative ease of insertion, as well as ease and comfort of removal.

Other dimensions that can be used (without limitation) are 12 cm straight portion of the upper hollow shaft, and 12 cm, 14 cm, or 16 cm length of added loops of soft percuflex. For the 0.020" diameter material, either 2 or 3 loops may be used providing 4 or 6 strings, total. For 0.040" inch material, either 1 or 2 loops is recommended.

Fig. 9 shows such an alternative embodiment having a simple coil at the kidney end. The lower end is constructed of looped stringlike elements with ends fused at the junction between the lower and the upper end. Therefore, there are an even number of string elements, with no free ends. Circle E in Fig. 9 represents an idealized depiction of the ureteral opening into the

bladder. While not shown in Fig. 9, the loops may be fused over a very short distance at the bladder end in order to prevent tangling of loops and to improve stent handling. Any conventional means of fusion may be used. Optionally, organization of the loops can be maintained by pre-placing them inside the pusher tubing using a long monofilament nylon loop tail, similar to those used for the non-invasive removal stents (i.e. without sensor endoscopy).

Methods for insertion and removal of ureteral stents are known in the art. Generally, stent placement is achieved by advancing the tubular stent segment over a guidewire in the ureter. A pushing catheter passes the tubular segment into the kidney, while maintaining the tail in the bladder. Other methods such as a stiff sheath can be used to position the stent. Once in position, the sheath can be removed.

The tubular portion of the stent may be manufactured by extruding a tube according to known techniques. The elongated tail may be separately manufactured by conventional techniques and attached to the tubular portion, e.g., using biocompatible adhesive materials or heat. Alternatively, the stent may be made by injection molding the tube and the tail as a single piece, using a pin to create hollow segments. The stent may be manufactured from any of a number of biocompatible polymers commonly used inside the body, including polyurethane and polyethylene. In still other embodiments, the entire stent may be solid, so that urine is conveyed entirely on an external stent surface.

What is claimed is:

1. A ureteral stent for assisting flow of urine within a patient's ureter and into the patient's bladder, the stent comprising a thin flexible elongated member having an elongated external urine-transport surface sized and configured to transport urine along the surface within the ureter.

2. The stent of claim 1 in which the external urine transporting surface is sized and configured to extend along at least part of the ureter, across the ureter/bladder junction, and from there through the ureteral opening into the bladder.

3. The stent of claim 2 further comprising an elongated tubular segment attached to said elongated member, the tubular segment comprising:

a) an upper region having at least a first opening,

b) a lower region having at least a second opening to be positioned in the ureter outside the bladder, and

c) a central lumen connecting the first opening to the second opening;

the elongated member being at least one thin flexible tail extending from the lower region of the tubular segment at a point outside the bladder so as to receive urine from the second opening of the tubular segment and to transport urine from the second region across the ureter/bladder junction and into the bladder.

4. The stent of claim 3 in which the upper region is configured and sized for placement in the renal cavity.

THIS SHEET HAS BEEN REPLACED

This Sheet Has Been Replaced

5. The stent of claim 1 or claim 3 in which the elongated member is a tail comprising at least one thread filament.

6. The stent of claim 5 in which the tail comprises multiple thread filaments.

7. The stent of claim 5 in which the tail comprises at least one filament loop.

8. The stent of claim 7 in which the tail comprises no unlooped filaments, so that the tail is free from loose ends.

9. The stent of claim 7 in which the filament loop comprises a junction of individual filament ends.

10. The stent of claim 9 in which the junction of filament ends is positioned at the point where tail joins to the elongated tubular segment.

11. The stent of claim 6, comprising at least two filaments loops.

12. The stent of claim 3 in which the elongated member is softer than the elongated tubular segment.

13. The stent of claim 4 in which the upper region comprises a portion of enlarged diameter, designed for placement in the renal cavity.

14. The stent of claim 13 in which the upper region has an external section having straight sides and corners.

This Sheet Has Been Replaced

THIS SHEET HAS BEEN REPLACED

15. The stent of claim 5 in which the tail is a fluted filament.

16. The stent of claim 1 further comprising an extractor thread attached to the lower end of the elongated member.

17. The stent of claim 3 in which the external urine-transport surface is concave.

18. The stent of claim 3 in which the external urine-transport surface is convex.

19. The stent of claim 3 in which the tubular segment is stiff enough to avoid crimping during insertion through the ureter.

20. The stent of claim 3 in which the tail and its attachment to the tubular segment are strong enough to permit retrieval of the stent from the kidney and ureter by locating the tail in the bladder and pulling on it.

21. The stent of claim 3 in which the tail includes an accurately shaped anchor segment to control migration up the ureter.

22. The stent of claim 3 in which the tail is long enough to effectively prevent migration of the entire tail into the ureter.

23. The stent of claim 3 in which the tail has a smaller outer diameter than the outer diameter of the tubular segment.

This Sheet Has Been Replaced

THIS SHEET HAS BEEN REPLACED

24. The stent of claim 3 in which tail is solid.

25. The stent of claim 3 in which at least part of the tail is hollow.

26. The stent of claim 3 in which the outer diameter of the tubular segment decreases approaching the bladder end region.

27. The stent of claim 3 or claim 26 in which the tubular member includes multiple openings along its length.

28. The stent of claim 3 in which the outer diameter of the tubular segment decreases approaching the kidney end region.

29. The stent of claim 3 in which the kidney end region includes multiple openings.

30. The stent of claim 3 in which the tail is attached to the bladder end region at a point toward the kidney with respect to the bladder end terminus of the bladder end region.

31. The stent of claim 26 further comprising a suture securing the tail to the tubular segment.

32. The stent of claim 31 in which the suture is incorporated in the tail to impart strength to the tail.

33. The stent of claim 32 in which the tail comprises a hollow lumen and the suture is positioned inside the hollow tail lumen.

This Sheet Has Been Replaced

THIS SHEET HAS BEEN REPLACED

34. The stent of claim 33 in which the tail is hollow, and the suture is attached to the tubular segment at a point toward the kidney with respect to the bladder end terminus of the bladder end region of the tubular segment, and the suture extends toward the bladder from the point of attachment through an opening in the bladder end region to the central lumen of the tubular segment and from there along the inside of the tail.

35. The stent of claim 3 in which at least the bladder end region of the tubular segment comprises multiple lumens, one of the lumens enclosing the suture from the point of attachment to the tubular segment to the terminus of the bladder end region.

36. The stent of claim 1 wherein the elongated external urine-transport surface is a continuous surface extending from the kidney to the bladder.

37. The stent of claim 36 wherein the elongated external surface is the outer surface of a solid member extending from the kidney to the bladder.

38. The stent of claim 3 wherein the tubular member and the elongated member comprise a one-piece stent.

39. A method of introducing a ureteral stent into a patient, the stent comprising a) a thin flexible elongated member having an elongated external urine-transport surface sized and configured to transport urine along the surface within the ureter; and b) an elongated tubular segment attached to said elongated member, the tubular segment comprising: i) an upper region having at least a first opening, ii) a lower

This Sheet Has Been Replaced

THIS SHEET HAS BEEN REPLACED

region having at least a second opening to be positioned in the ureter outside the bladder, and iii) a central lumen connecting the first opening to the second opening; the elongated member being a thin flexible tail extending from the lower region of the tubular segment at a point outside the bladder so as to receive urine from the second opening of the tubular segment and to transport urine from the second region across the ureter/bladder junction and into the bladder, the method comprising:

(a) positioning the kidney end region of the tubular segment within the renal pelvis; and

(b) positioning the elongated flexible member in the bladder.

40. A method of manufacturing a ureteral stent, the stent comprising a thin flexible elongated tail member having an elongated external urine-transport surface sized and configured to transport urine along the surface within the ureter, the method comprising:

providing a polymer pre-form having a tubular shape, forming an elongated tubular stent segment from the polymer pre-form, and

providing a tail member at an end region of the tubular segment designed to be positioned toward the patient's bladder.

THIS SHEET HAS BEEN REPLACED

This Sheet Has Been Replaced

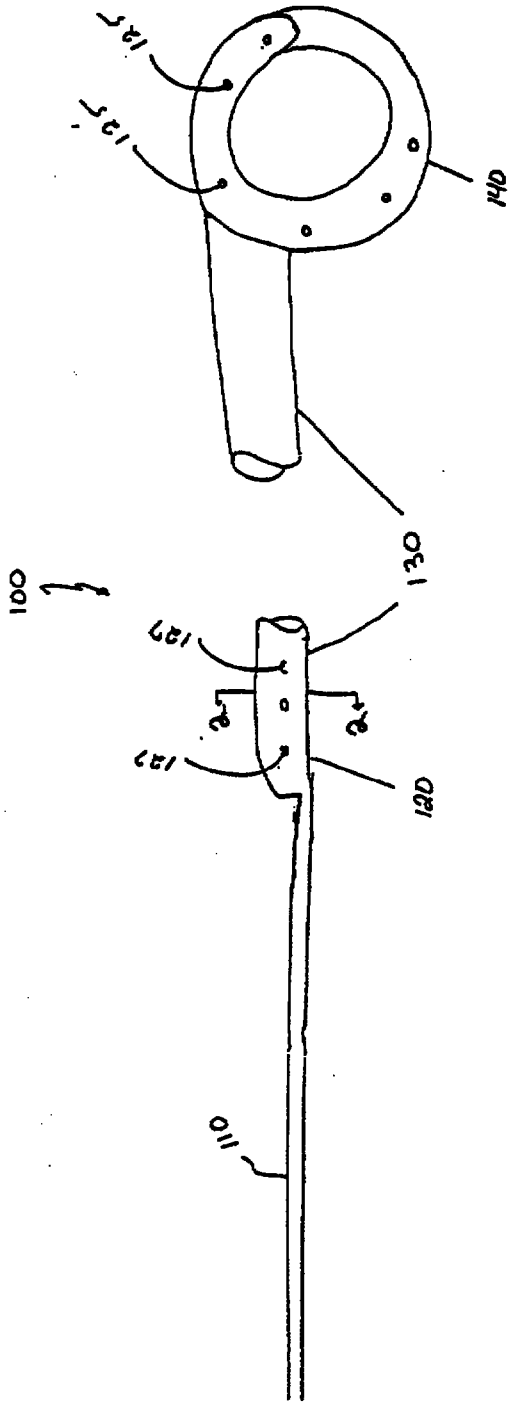


Figure 1

This Sheet Has Been Replaced

THIS SHEET HAS BEEN REPLACED

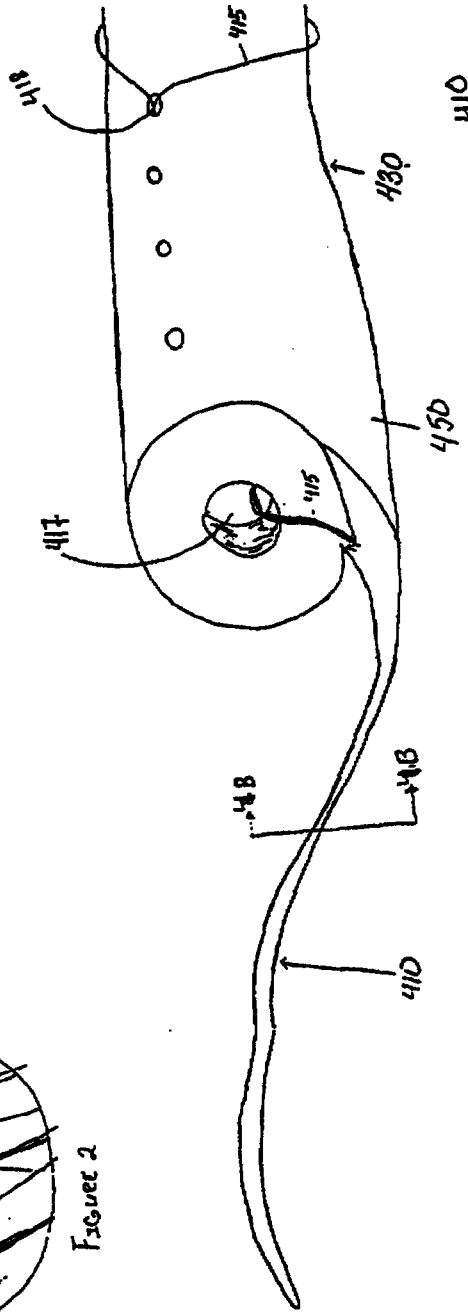


FIGURE 4A

FIGURE 4B

FIGURE 2

THIS SHEET HAS BEEN REPLACED

This Sheet Has Been Replaced

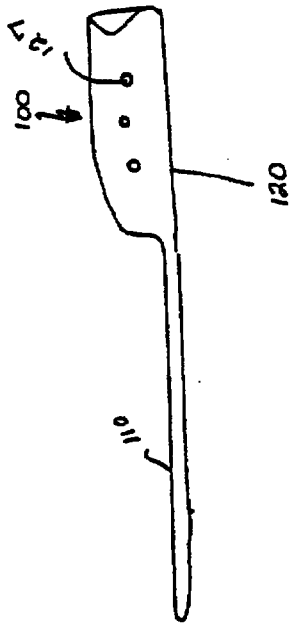


Figure 3

THIS SHEET HAS BEEN REPLACED

This Sheet Has Been Replaced

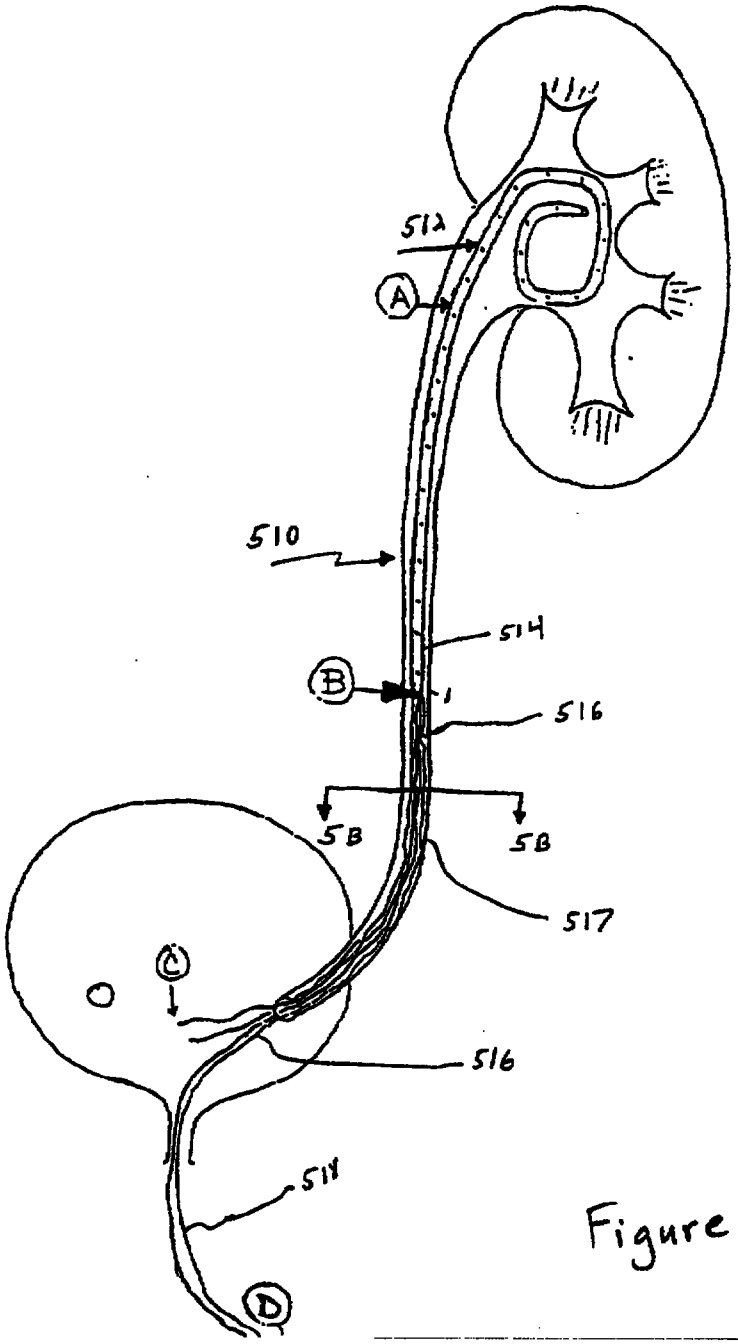


Figure 5A




Figure 5B

This Sheet Has Been Replaced

THIS SHEET HAS BEEN REPLACED




Figure 6A

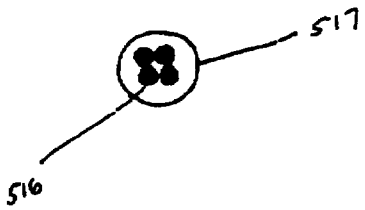


Figure 6B

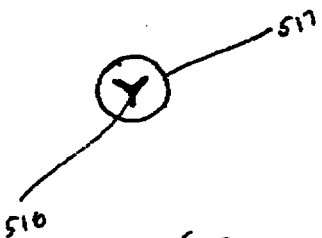


Figure 6C

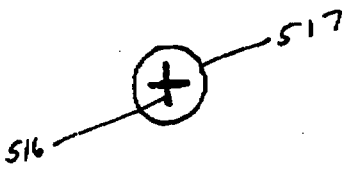


Figure 6D

THIS SHEET HAS BEEN REPLACED

This Sheet Has Been Replaced

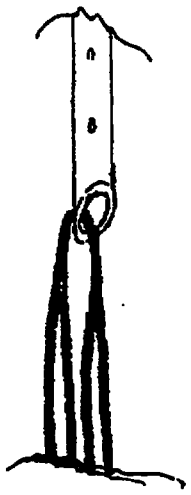


Figure 7A

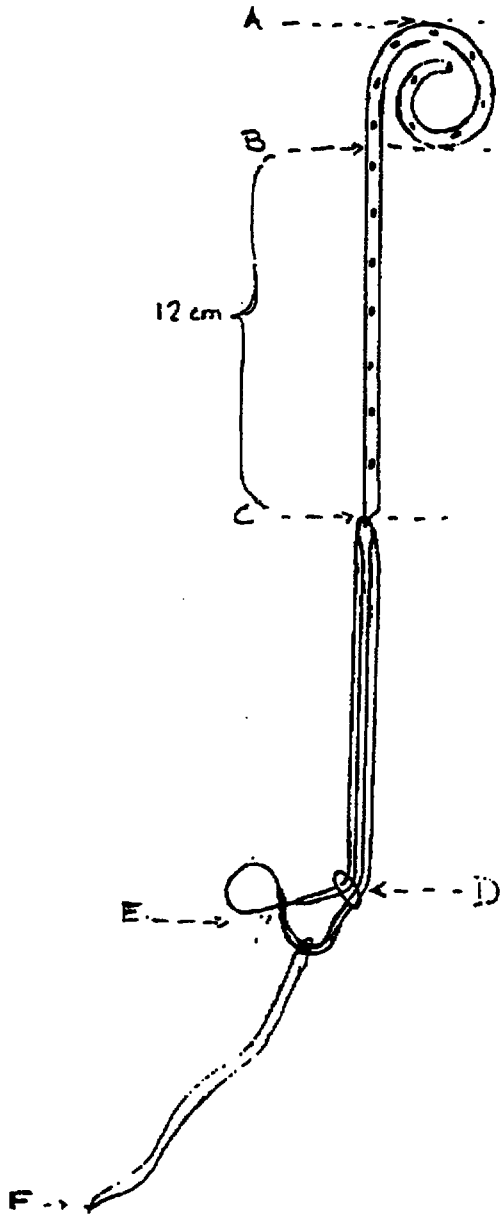


Figure 7

This Sheet Has Been Replaced

THIS SHEET HAS BEEN REPLACED

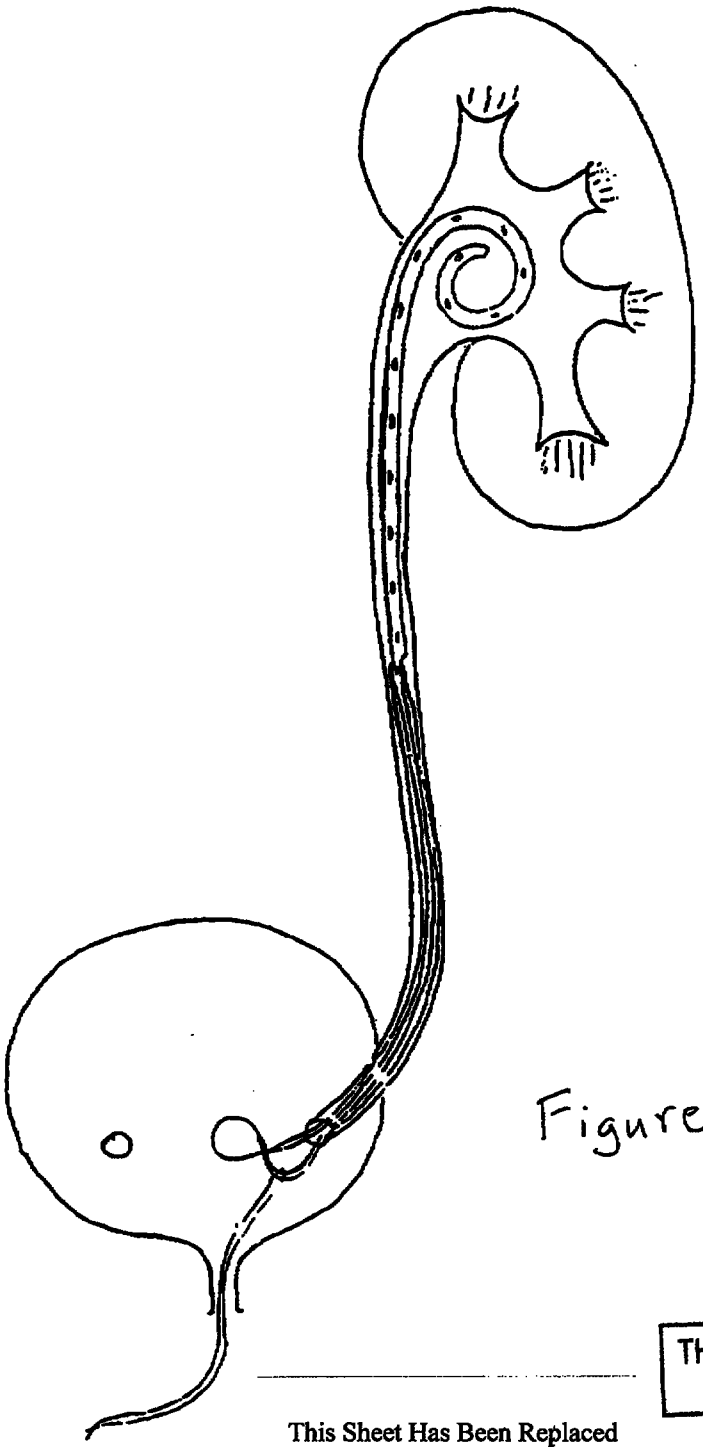


Figure 8

THIS SHEET HAS BEEN REPLACED

This Sheet Has Been Replaced

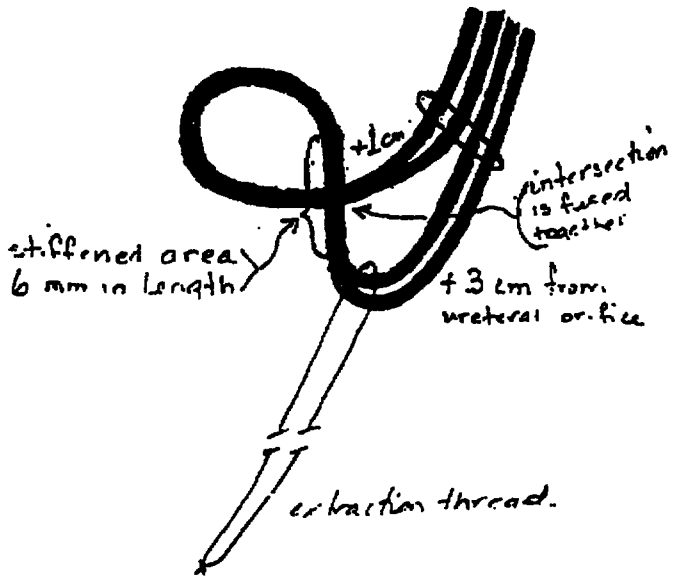


Figure 8A

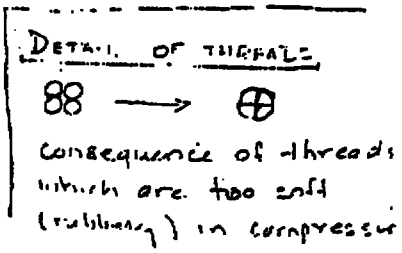


Figure 8B

This Sheet Has Been Replaced

THIS SHEET HAS BEEN REPLACED

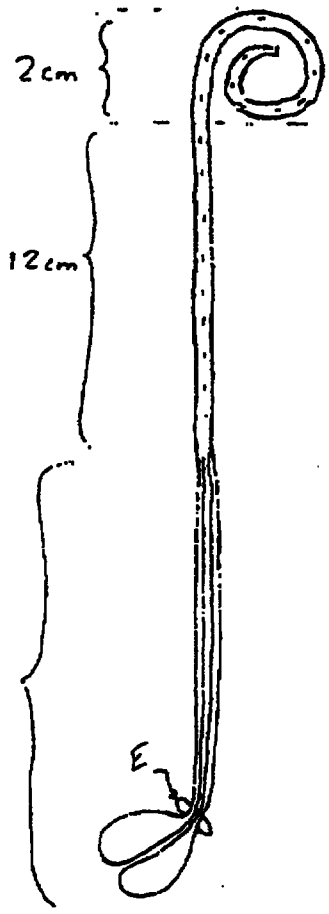


Figure 9

THIS SHEET HAS BEEN REPLACED

This Sheet Has Been Replaced

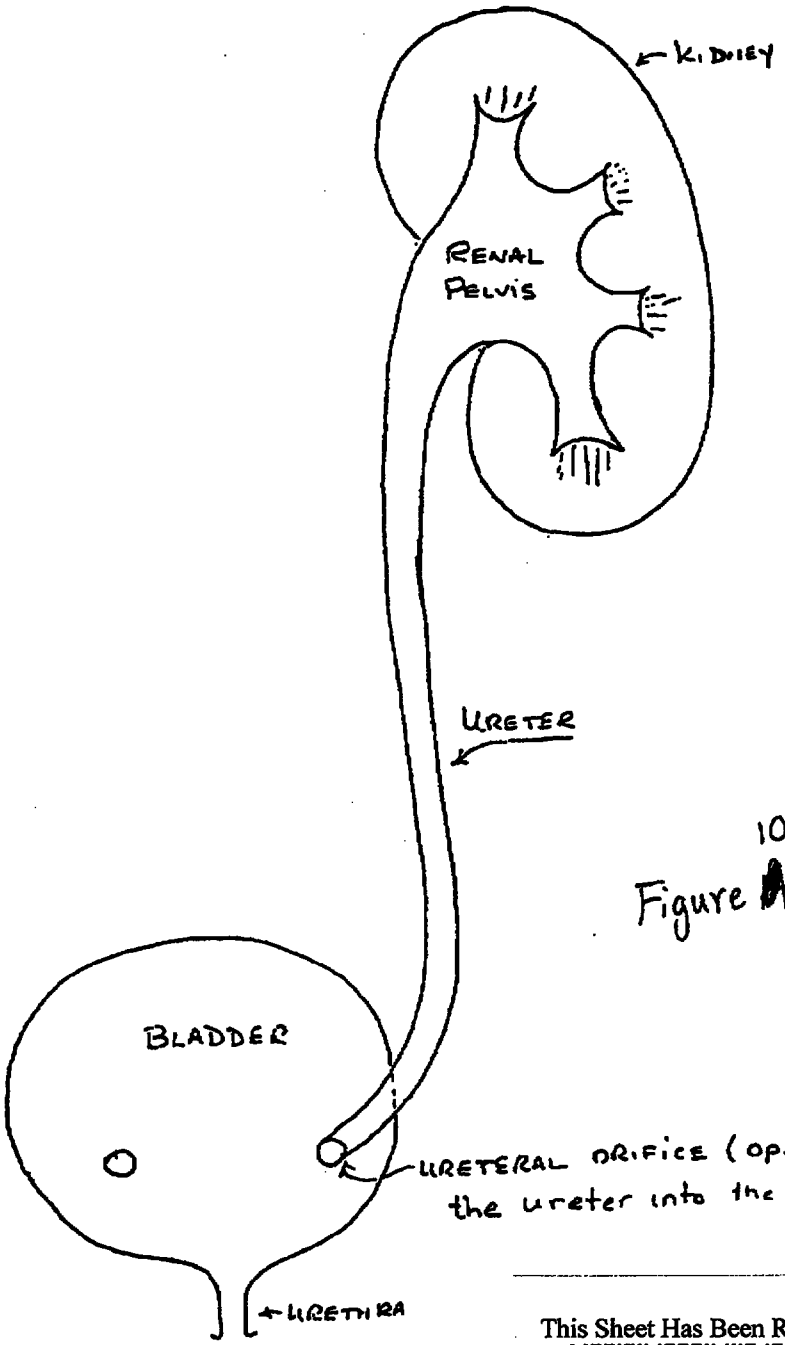


Figure 10

This Sheet Has Been Replaced

THIS SHEET HAS BEEN REPLACED


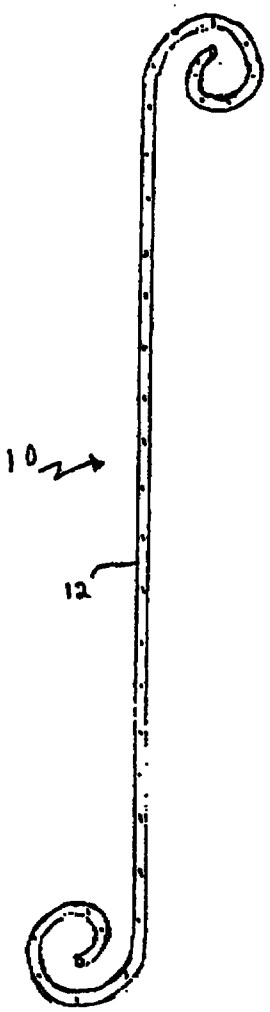


Figure 11

PRIOR ART

THIS SHEET HAS BEEN REPLACED

This Sheet Has Been Replaced

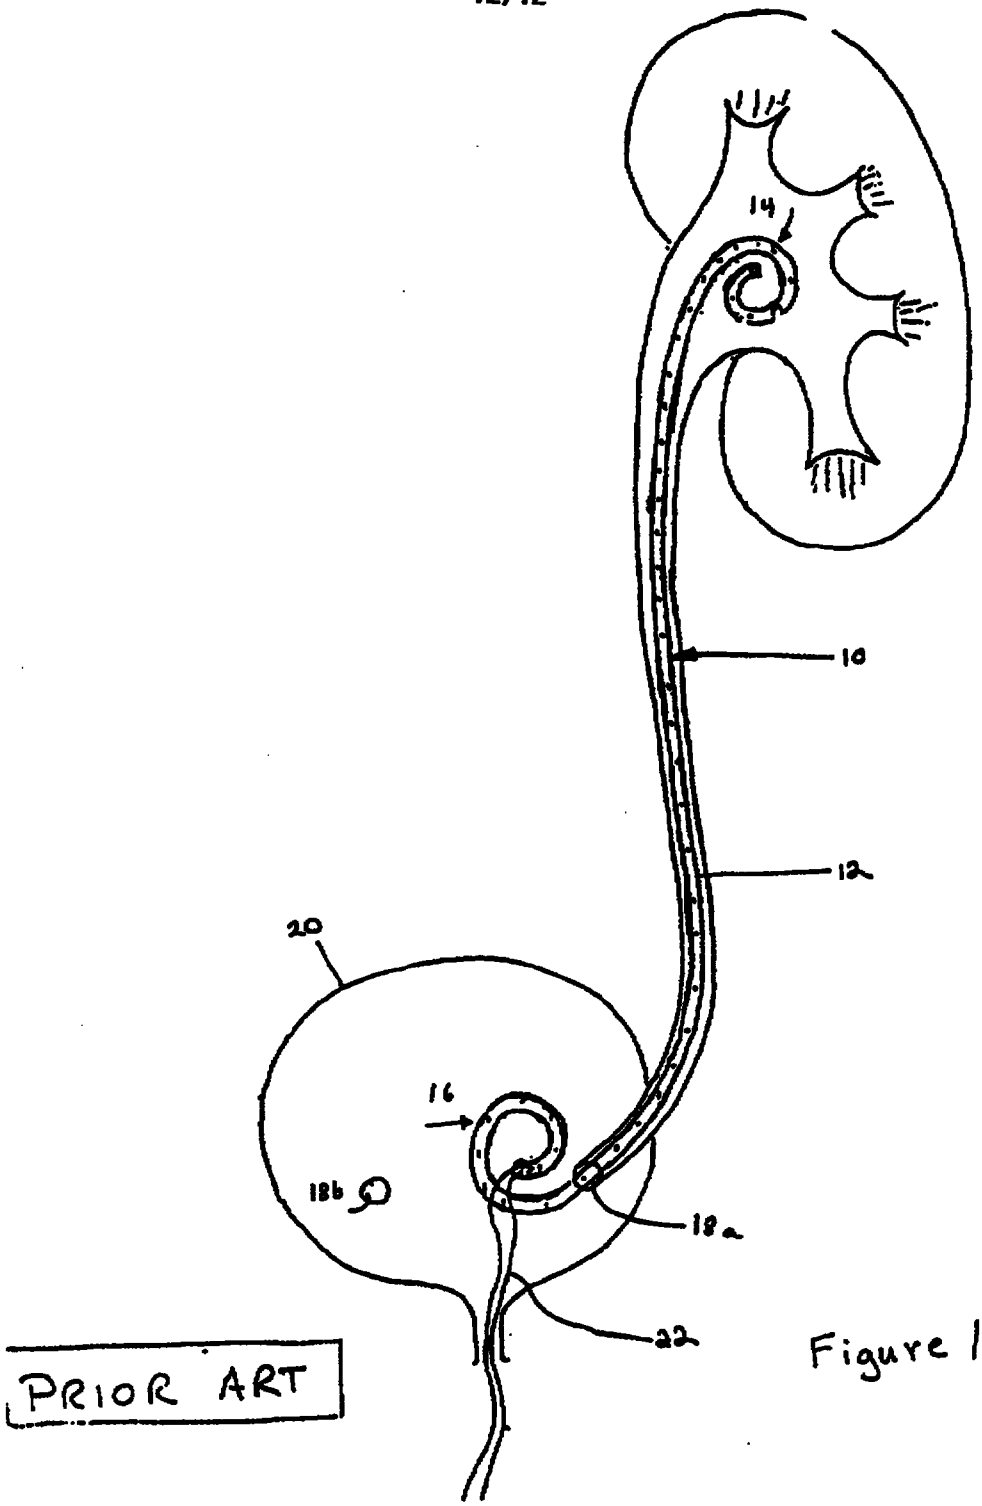

PRIOR ART

Figure 12

THIS SHEET HAS BEEN REPLACED

This Sheet Has Been Replaced

PCT/US 96/17795
IPEA/US 06 JUN 1997

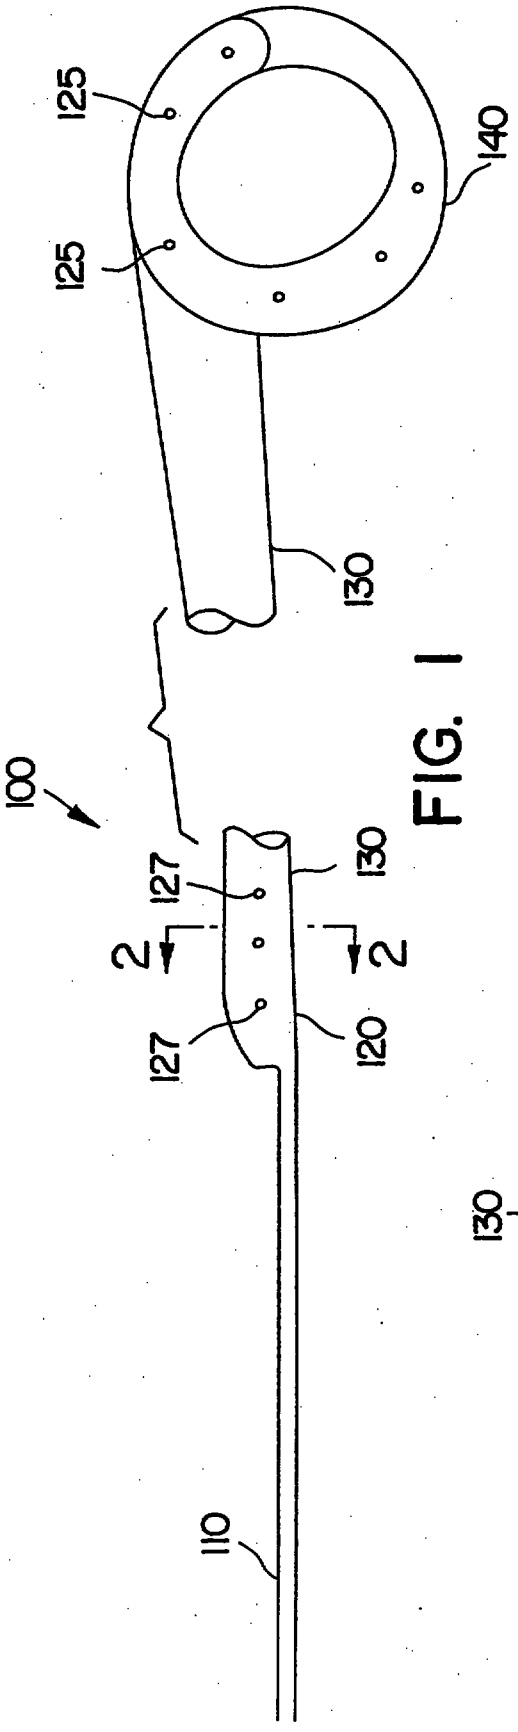


FIG. 1

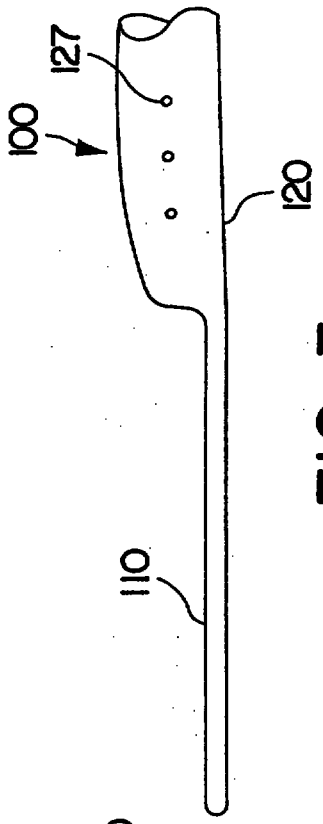


FIG. 3

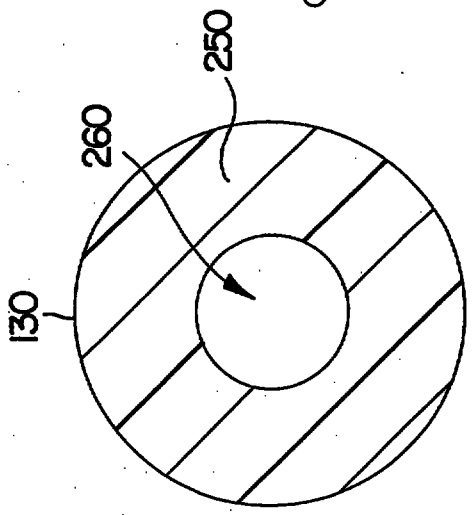


FIG. 2

PCT/US 95/
IPEA/US 05 JUN 1997

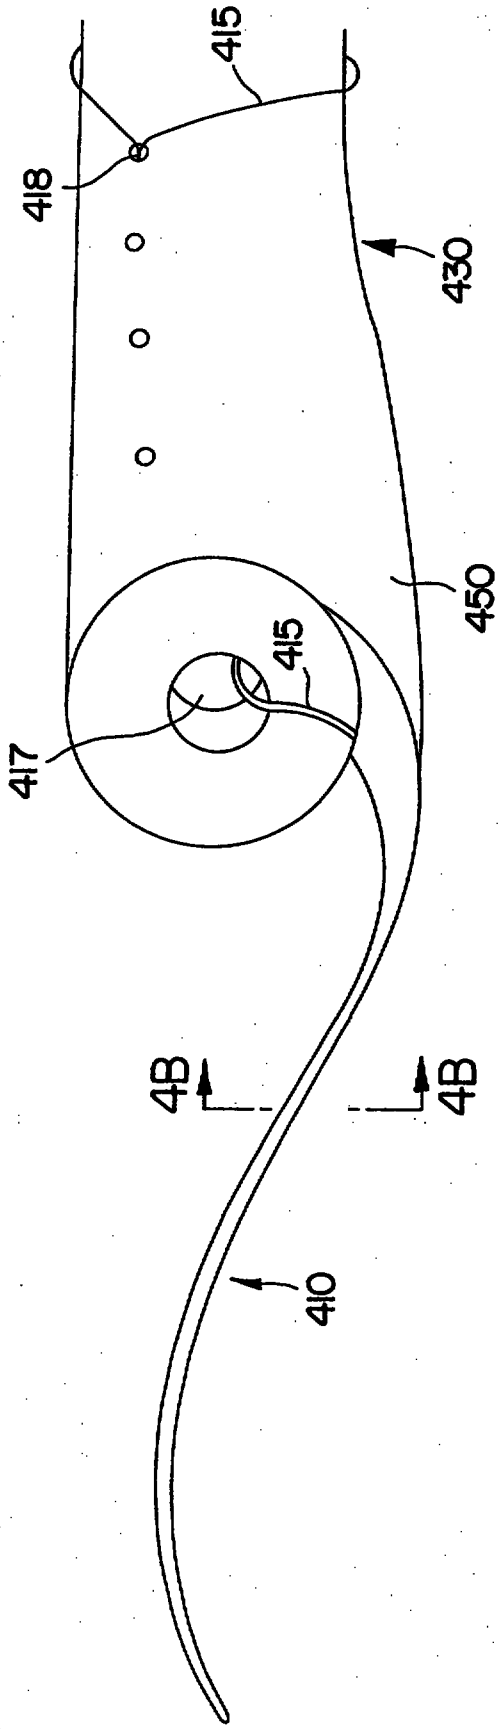


FIG. 4A

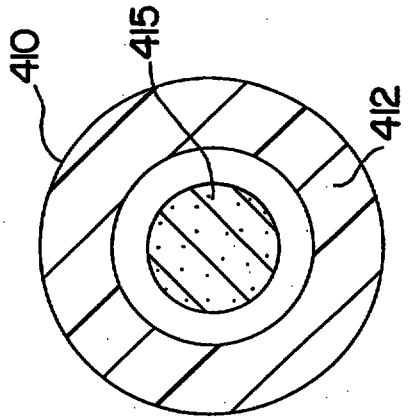


FIG. 4B

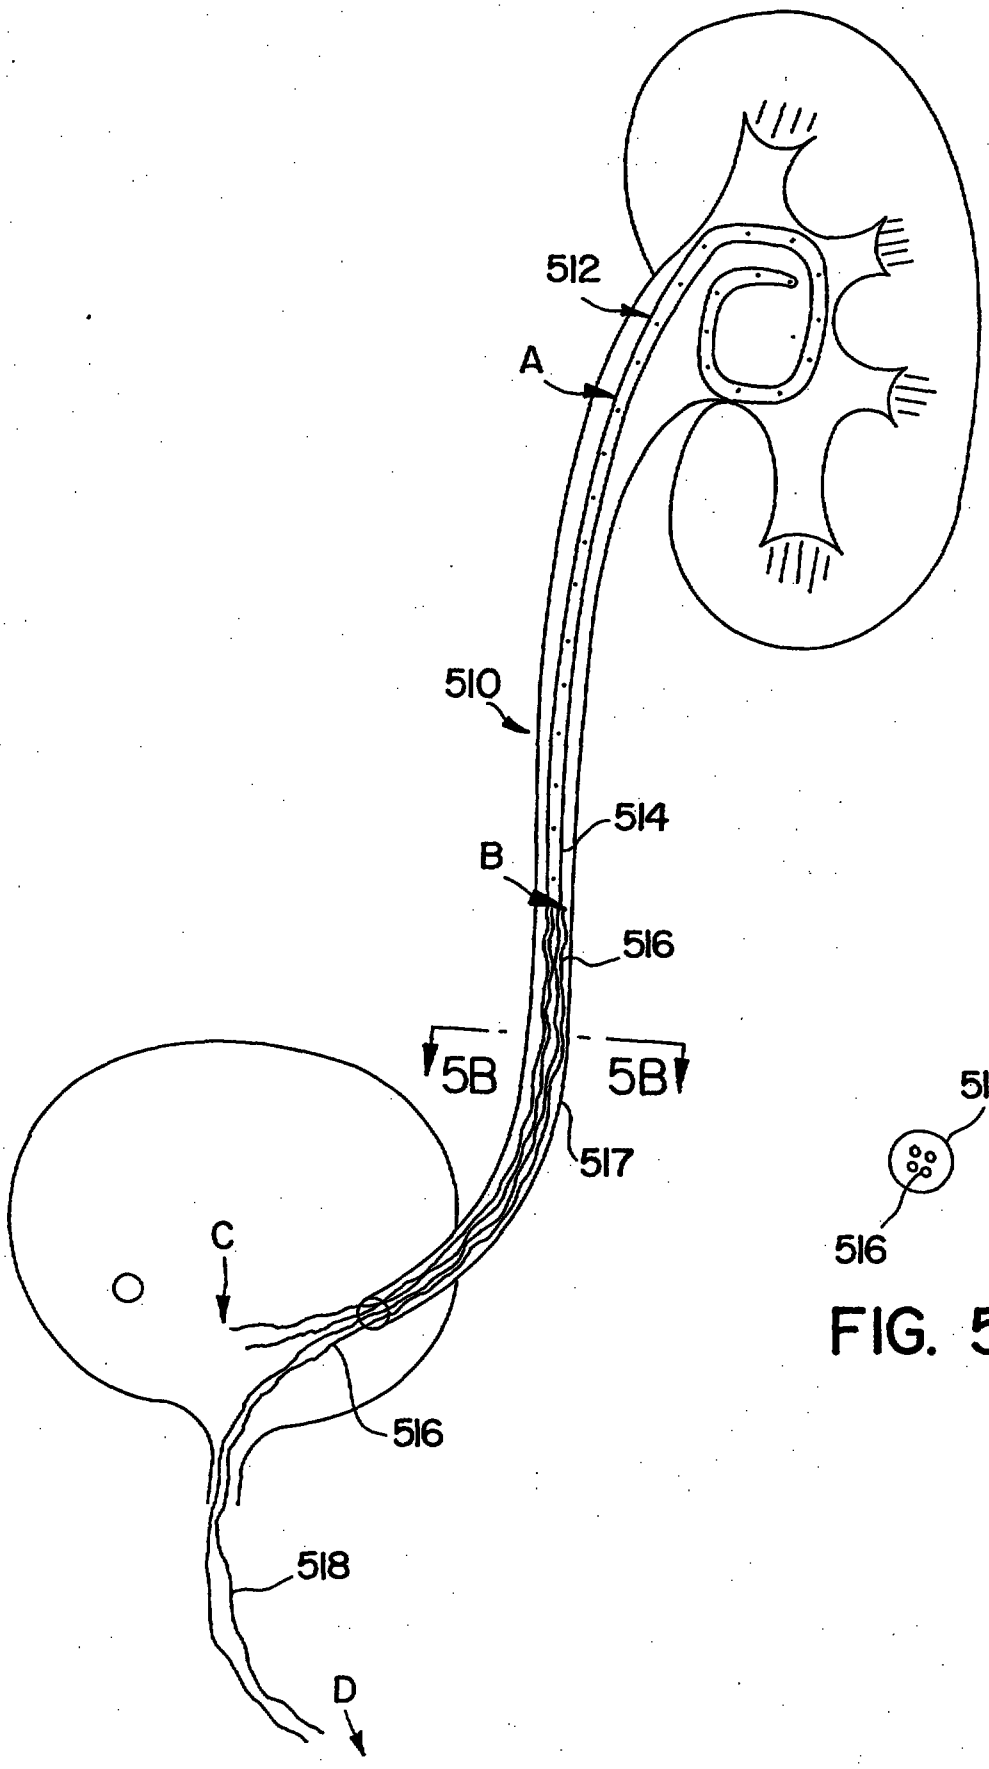


FIG. 5A

FIG. 5B

PCT/US 96/17795
IPEA/US 05 JUN 1997




FIG. 6A




FIG. 6B




FIG. 6C




FIG. 6D

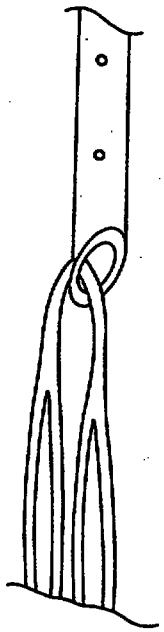


FIG. 7A

FIG. 7

PCT/US 96/17795
IPEA/US 05 JUN 1997

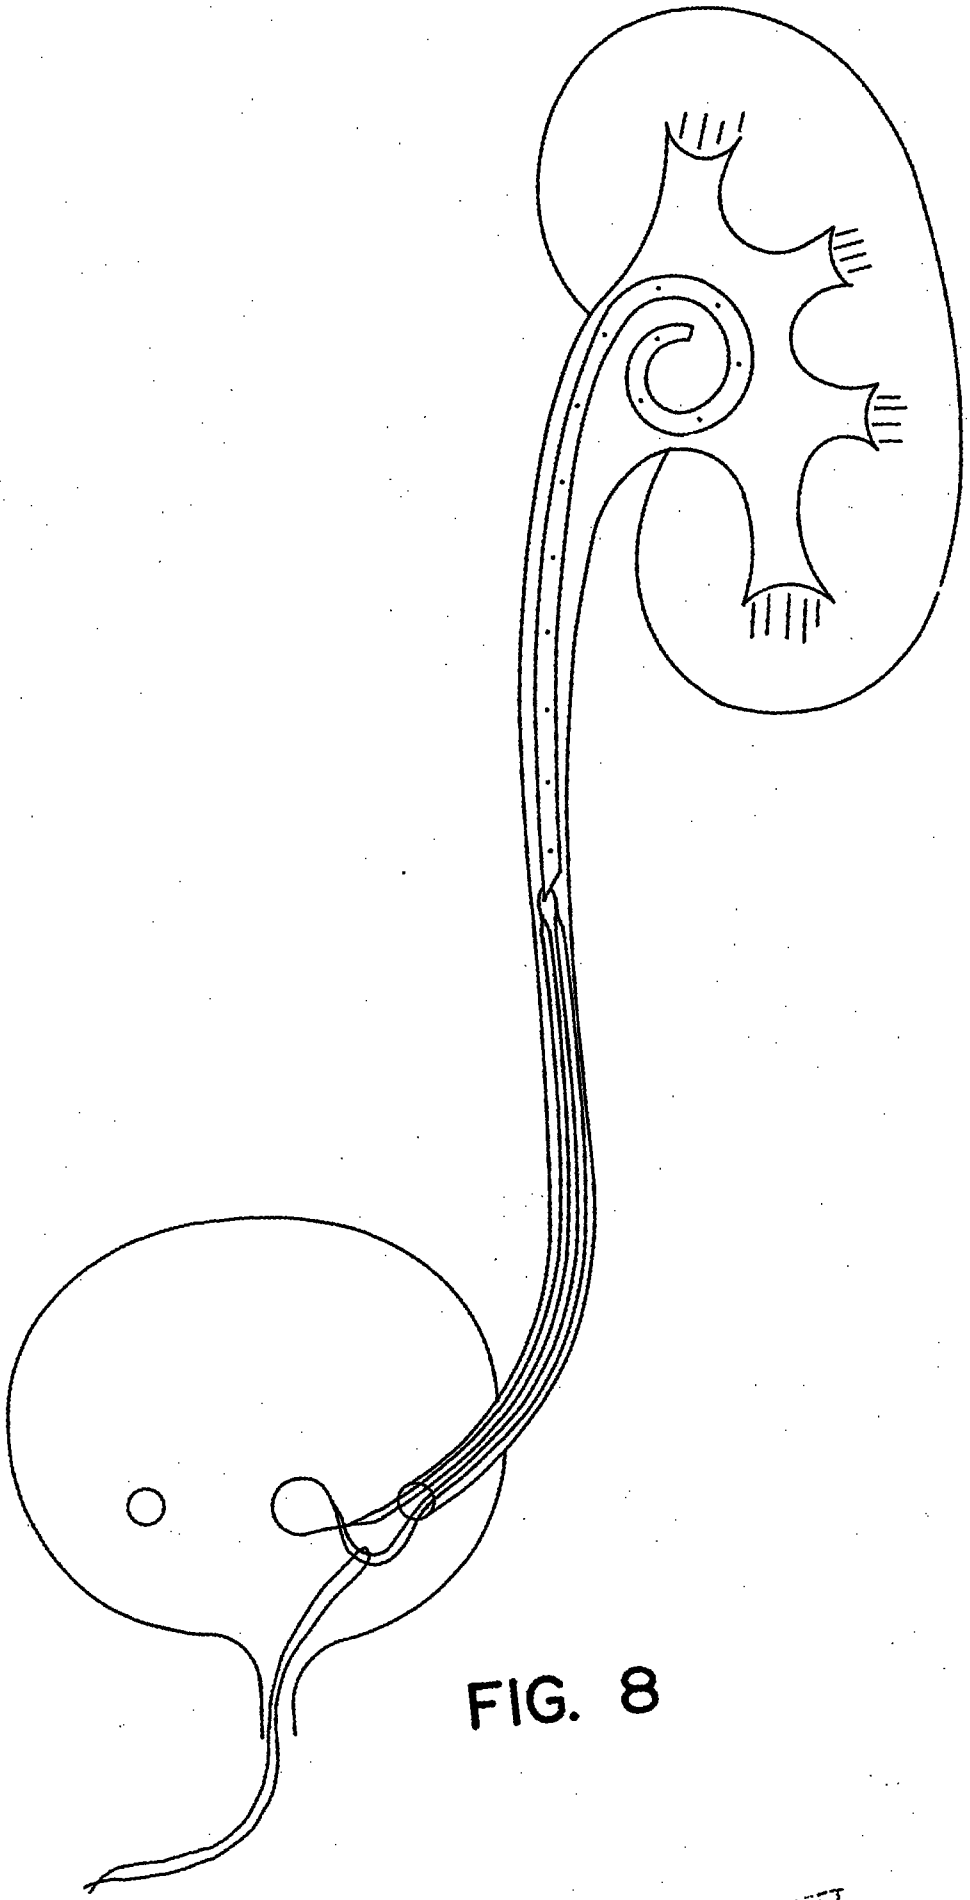


FIG. 8

PCT/US 96/17795
IPEA/US 0 JUN 1997

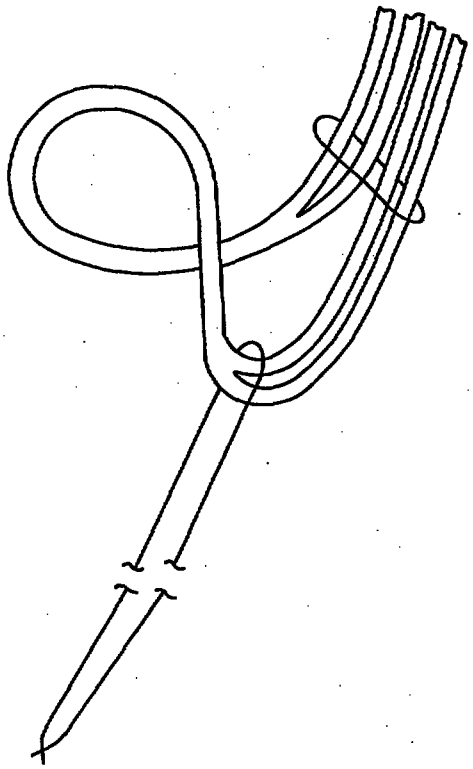


FIG. 8A

DETAIL OF THREADS

88 ⟶ ⊕

CONSEQUENCE OF THREADS
WHICH ARE TOO SOFT
(RUBBERY) IN COMPRESSION

FIG. 8B

PCT/US 96/17795
IPEA/US 05 JUN 1997

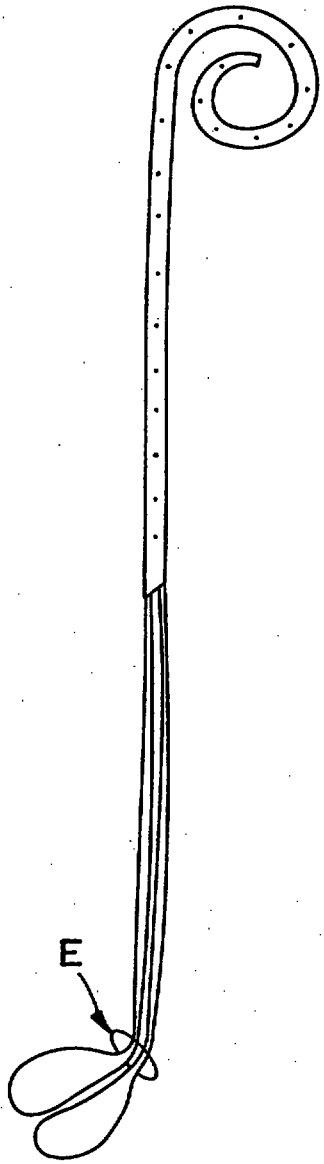


FIG. 9

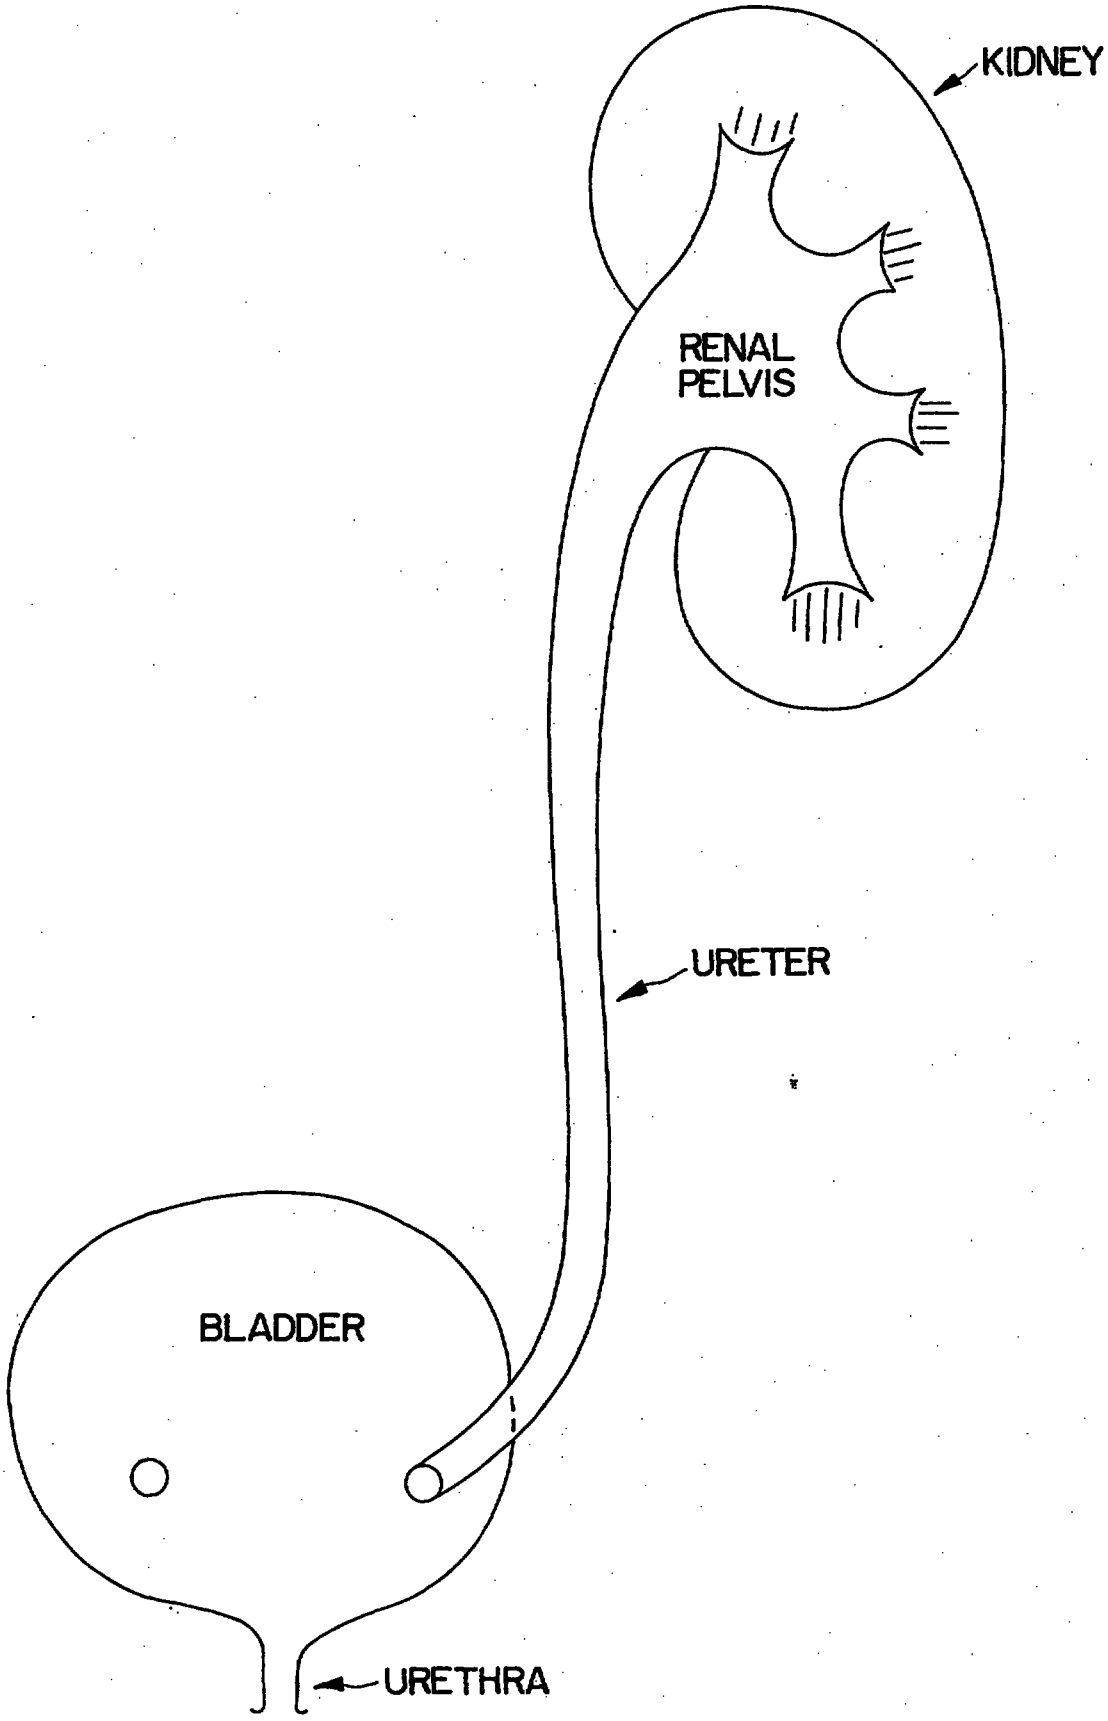


FIG. 10

PCT/US 96/17795
IPEA/US 06 JUN 1997

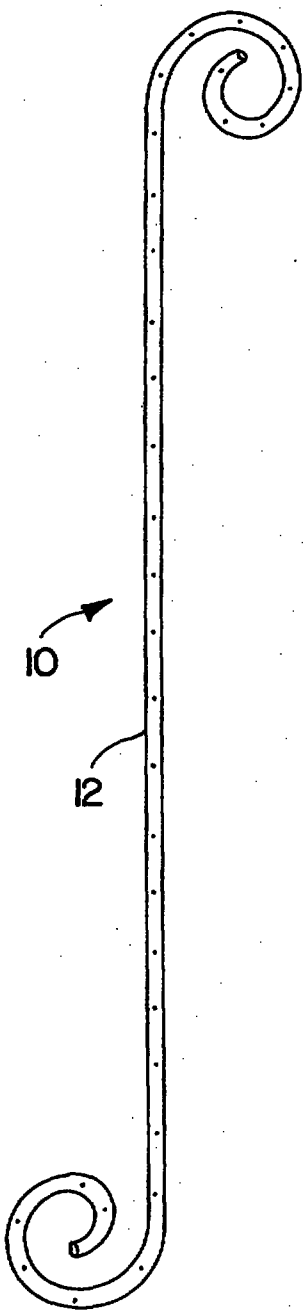


FIG. 11
PRIOR ART

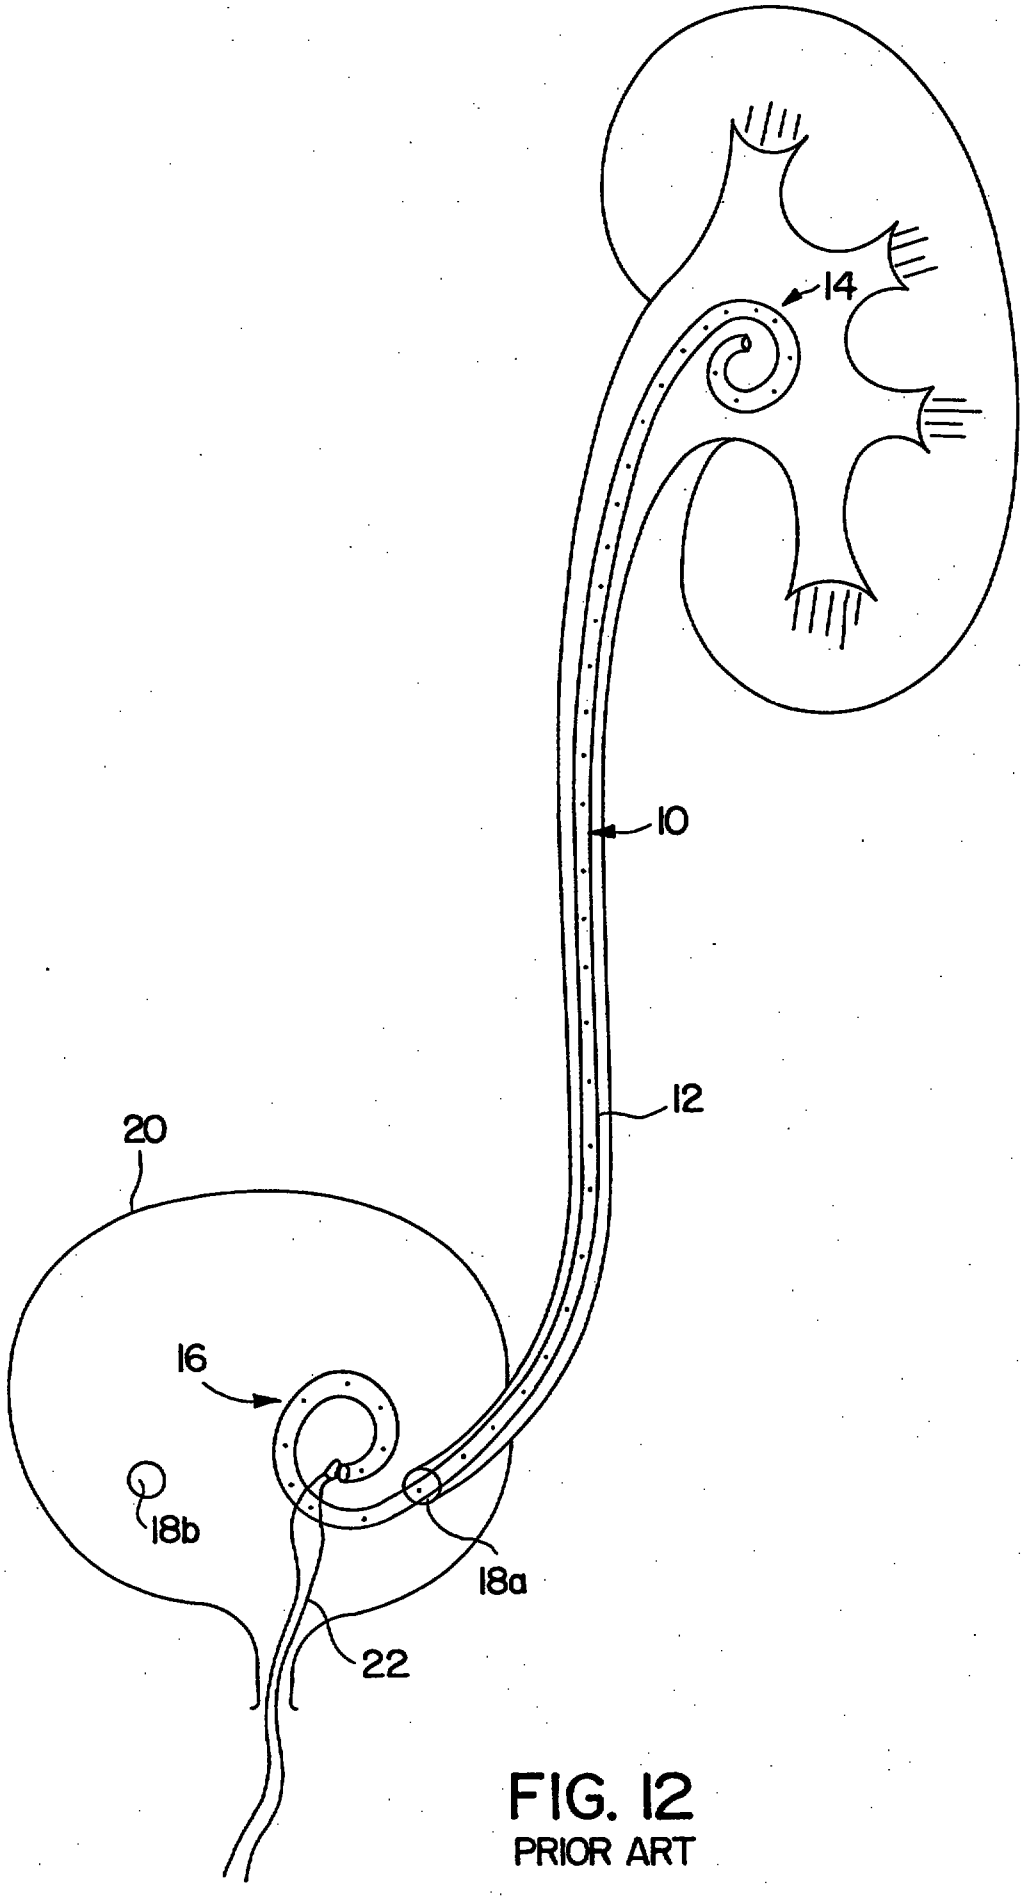


FIG. 12
PRIOR ART

IPOS copy 9802785-7

* C L M S *

Claims

1. A ureteral stent for assisting flow of urine, the stent comprising:

a tubular segment comprising (a) an upper region including at least a first opening, (b) a lower region having an external surface and including at least a second opening, the lower region to be positioned outside the bladder when the ureteral stent is in use, and (c) a lumen connecting the first opening to the second opening; and

a thin flexible elongated tail having an external urine-transport surface, the thin flexible tail being substantially straight and transitioning from the lower region of the tubular segment so as to receive urine from the lower region of the tubular segment and to transport the urine along the urine-transport surface, the transition from the external surface of the lower region of the tubular segment to the urine-transport surface of the thin flexible tail being continuous.

2. The stent of claim 1 in which the external urine-transport surface when the ureteral stent is in use extends along at least part of the ureter, across the ureter/bladder junction, and from there through the ureteral opening into the bladder.

3. The stent of claim 1 in which the thin flexible tail is solid.

4. The stent of claim 1 in which at least part of the tail is hollow.

5. The stent of claim 1 in which the tubular segment includes multiple openings along its length.

6. The stent of claim 1 wherein the external urine-transport surface of the tail is continuous and uninterrupted.

REPLACEMENT SHEETS SG
☐ Description : paged ..... to paged .....
☒ Claim(s) : paged 19 to paged 25
☐ Drawing(s) : paged ..... to paged .....
☐ Abstract : paged ..... to paged .....
DATE OF RECEIPT 7.5.99

7. A method of introducing a ureteral stent into a patient, the stent comprising a) a thin flexible elongated member having an elongated external urine-transport surface sized and configured to transport urine along the surface within the ureter; and b) an elongated tubular segment attached to said elongated member, the tubular segment comprising: i) an upper region having at least a first opening, ii) a lower region having at least a second opening to be positioned in the ureter outside the bladder, and iii) a central lumen connecting the first opening to the second opening; the elongated member being a thin flexible tail extending from the lower region of the tubular segment at a point outside the bladder so as to receive urine from the second opening of the tubular segment and to transport urine from the second region across the ureter/bladder junction and into the bladder, the method comprising:

(a) positioning the kidney end region of the tubular segment within the renal pelvis; and

(b) positioning the elongated flexible member in the bladder.

8. A method of manufacturing a ureteral stent, the stent comprising a thin flexible elongated tail member having an elongated external urine-transport surface sized and configured to transport urine along the surface within the ureter, the method comprising:

providing a polymer pre-form having a tubular shape,

forming an elongated tubular stent segment from the polymer pre-form, and

providing a tail member at an end region of the tubular segment designed to be positioned toward the patient's bladder.

9. The stent of claim 1 in which the tail tapers to a smaller outer diameter as it transitions from the lower region.

10. A ureteral stent for assisting flow of urine, the stent comprising:

a tubular segment comprising (a) an upper region including at least a first opening, (b) a lower region having an outer diameter and including at least a second opening, the lower region

to be positioned upstream from the bladder when the ureteral stent is in use, and (c) a lumen connecting the first opening to the second opening; and

a thin flexible elongated tail transitioning from the lower region of the tubular segment, the thin flexible tail having a generally circular cross-section and an outer diameter that tapers from the outer diameter of the lower region to a smaller diameter, the thin flexible tail having a urine-transport surface so as to receive urine from the lower region of the tubular segment and to transport the urine along the urine-transport surface.

11. The stent of claim 10 in which the urine-transport surface is continuous and uninterrupted.

12. The stent of claim 10 in which the thin flexible tail is solid.

13. The stent of claim 10 in which the first opening is an end opening, the second opening is an end opening, the tubular segment further comprises an outer surface with a plurality of third openings arranged on the outer surface of the tubular segment from the upper region to the lower region, and the lumen communicates with the third openings.

14. The stent of claim 10 in which at least a portion of the thin flexible tail is hollow.

15. The stent of claim 10 in which the thin flexible tail is substantially straight.

16. A device for assisting flow of urine, the device comprising:

a tubular segment with an outer surface, comprising (a) an upper region, (b) a lower region positioned upstream from the bladder when the device is in use, (c) a plurality of openings arranged on the outer surface of the tubular segment from the upper region to the lower region, and (d) a lumen extending through the length of the tubular segment, and communicating with the openings arranged on the outer surface of the tubular segment; and

a thin flexible elongated member comprising at least one thin flexible tail having a urine-transport surface, the thin flexible tail being substantially straight and transitioning from the lower region of the tubular segment so as to receive urine from the lower region of the tubular segment and to transport the urine along the urine-transport surface.

17. The device of claim 16 in which the urine-transport surface is continuous and uninterrupted.

18. The device of claim 16 in which the thin flexible tail is solid.

19. The device of claim 16 in which at least a portion of the thin flexible tail is hollow.

20. The device of claim 16 in which the tubular segment has a substantially circular cross-section.

21. The device of claim 16 wherein the tubular segment and the elongated member comprise a one-piece stent.

22. A device for assisting flow of urine, the device comprising:

a first segment having an outer surface and opposed first and second ends, the first segment comprising (a) an upper region including the first end and having an outer diameter, the upper region being configured to be positioned in the kidney when the device is in use, (b) a lower region including the second end, the lower region being configured to be positioned upstream from the bladder when the device is in use, (c) a plurality of openings arranged on the outer surface of the first segment from the upper region to the lower region, and (d) a lumen extending through the length of the first segment, and communicating with the openings arranged on the outer surface of the first segment; and

* C L M S *

a second segment transitioning from the first segment at the second end of the lower region, the second segment comprising one or more elongated, flexible tail members, each tail member having a urine-transport surface and an outer tail diameter, the outer tail diameter of each tail member being smaller than the outer diameter of the upper region of the first segment.

23. The device of claim 22 in which the first segment has a substantially circular cross-section.

24. The device of claim 22 in which the second segment transitions substantially straight from the first segment at the second end of the lower region.

25. The device of claim 22 in which the urine-transport surface of each tail member is continuous and uninterrupted.

26. The device of claim 22 in which the one or more flexible tail members are solid.

27. A medical device, the device comprising:

a first segment having opposed first and second terminal ends, the first segment comprising (a) an upper region including the first terminal end, (b) a substantially straight lower region including the second terminal end, and (c) an intermediate region connecting the upper region and the lower region; and

a second segment extending from the first segment at the second terminal end, the second segment comprising a plurality of elongated, flexible tail members.

28. The medical device of claim 27 in which the device is for assisting flow of urine, and each tail member comprises a urine-transport surface so as to receive urine at the second terminal end of the lower region and to transport the urine along the urine-transport surface when the device is in use.

* C L M S *

29. The medical device of claim 27 in which the tail members are solid.

30. The medical device of claim 28 in which the urine-transport surface of the tail members is continuous and uninterrupted.

31. The medical device of claim 27 in which the upper region of the first segment has an outer diameter and each tail member has an outer diameter, the outer diameter of each tail member being smaller than the outer diameter of the upper region of the first segment.

32. The device of claim 27 in which the tail members comprise at least one thread filament.

33. The device of claim 32 in which the tail members comprise a plurality of thread filaments.

34. The device of claim 32 in which the tail members comprise at least one filament loop.

35. The device of claim 34 in which the tail members comprise no unlooped filaments, so that the tail members are free from loose ends.

36. The device of claim 33, in which the tail members comprise at least two filament loops.

37. The device of claim 32 in which the tail members comprise a fluted filament.

38. The device of claim 28 in which the tail members when the device is in use extend into the bladder and include an accurately shaped anchor segment to control migration of the device up the ureter.

39. A medical device, the device comprising:

a first segment having opposed first and second terminal ends, the first segment comprising (a) an upper region including the first terminal end, (b) a substantially straight lower region including the second terminal end, and (c) an intermediate region connecting the upper region and the lower region;

a second segment independent of the first segment and attached to the first segment at the second terminal end, the second segment comprising one or more elongated, flexible tail members.

40. The medical device of claim 39 in which the device is for assisting flow of urine, and each tail member comprises a urine-transport surface so as to receive urine at the second terminal end of the lower region and to transport the urine along the urine-transport surface when the device is in use.

41. The medical device of claim 39 in which the tail members are solid.

42. The medical device of claim 40 in which the urine-transport surface of the tail members is continuous and uninterrupted.

43. The medical device of claim 39 in which the upper region of the first segment has an outer diameter and each tail member has an outer diameter, the outer diameter of each tail member being smaller than the outer diameter of the upper region of the first segment.

44. The medical device of claim 39 in which the first segment is tubular and includes a lumen connecting the first and second terminal ends.

45. The medical device of claim 44 in which multiple openings are positioned along the length of the first segment communicating with the lumen of the first segment.

46. The medical device of claim 40 in which the one or more tail members comprise thread filaments.

47. The medical device of claim 40 in which the one or more tail members comprise at least one filament loop.

*NO COVER LETTER

IPOS COPY 9802785-7.

PCT WORLD INTELLECTUAL PROPERTY ORGANIZATION
International Bureau

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 6 : A61M 5/00 — A1

(11) International Publication Number: WO 97/17094

(43) International Publication Date: 15 May 1997 (15.05.97)

(21) International Application Number: PCT/US96/17795

(22) International Filing Date: 6 November 1996 (06.11.96)

(30) Priority Data:
60/006,259 — 7 November 1995 (07.11.95) — US
60/025,284 — 19 September 1996 (19.09.96) — US

(60) Parent Applications or Grants
(63) Related by Continuation
US — 60/025,284 (CON)
Filed on — 19 September 1996 (19.09.96)
US — 60/006,259 (CON)
Filed on — 7 November 1995 (07.11.95)

(71) Applicant *(for all designated States except US)*: BOSTON SCIENTIFIC CORPORATION [US/US]; One Boston Scientific Place, Natick, MA 01760-1537 (US).

(72) Inventors; and
(75) Inventors/Applicants *(for US only)*: CLAYMAN, Ralph, V. [US/US]; Boston Scientific Corporation, One Boston Scientific Place, Natick, MA 01760-1537 (US). DASSA, Alyssa, J. [US/US]; Boston Scientific Corporation, One Boston Scientific Place, Natick, MA 01760-1537 (US). FISHBEIN, Christopher [US/US]; Boston Scientific Corporation, One Boston Scientific Place, Natick, MA 01760-1537 (US). GODSHALL, Douglas, E. [US/US]; Boston Scientific Corporation, One Boston Scientific Place, Natick, MA 01760-1537 (US). WHITMORE, Willet, F. III [US/US]; Boston Scientific Corporation, One Boston Scientific Place, Natick, MA 01760-1537 (US).

(74) Agent: FREEMAN, John, W.; Fish & Richardson P.C., 225 Franklin Street, Boston, MA 02110-2804 (US).


(81) Designated States: AL, AM, AT, AU, AZ, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, HU, IL, IS, JP, KE, KG, KP, KR, KZ, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, TJ, TM, TR, TT, UA, UG, US, UZ, VN, ARIPO patent (KE, LS, MW, SD, SZ, UG), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG).

Published
With international search report.

(54) Title: URETERAL STENT WITH SMALL BLADDER TAIL(S)

(57) Abstract

This invention is a ureteral stent (100) for assisting movement of urine along a patient's ureter and into the patient's bladder. The stent (100) includes an elongated tubular segment (130) extending toward the bladder from a kidney end region for placement in the renal cavity to a bladder end region. A central lumen (260) connects at least one opening (127) at the first end region to at least one opening in the bladder end region. At least one flexible tail (110) is attached to the bladder end region of the tubular segment (130) at a point outside the bladder so as to receive urine from the opening in the bladder end region of the tubular segment (130) and to transport urine from there across the ureter/bladder junction and into the bladder. The tail (110) includes an elongated external urine transport surface sized and configured to transport urine along the ureter. The urine transporting surface is sized and configured to extend along at least part of the ureter, across the ureter/bladder junction, and from there into the bladder.

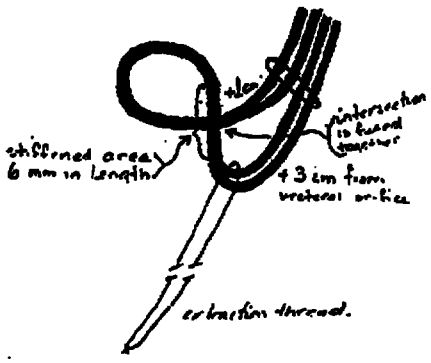

Detail of thread
88 → ⊕
Consequence of threads which are too soft (rubbery) in compression