

FIG. 1

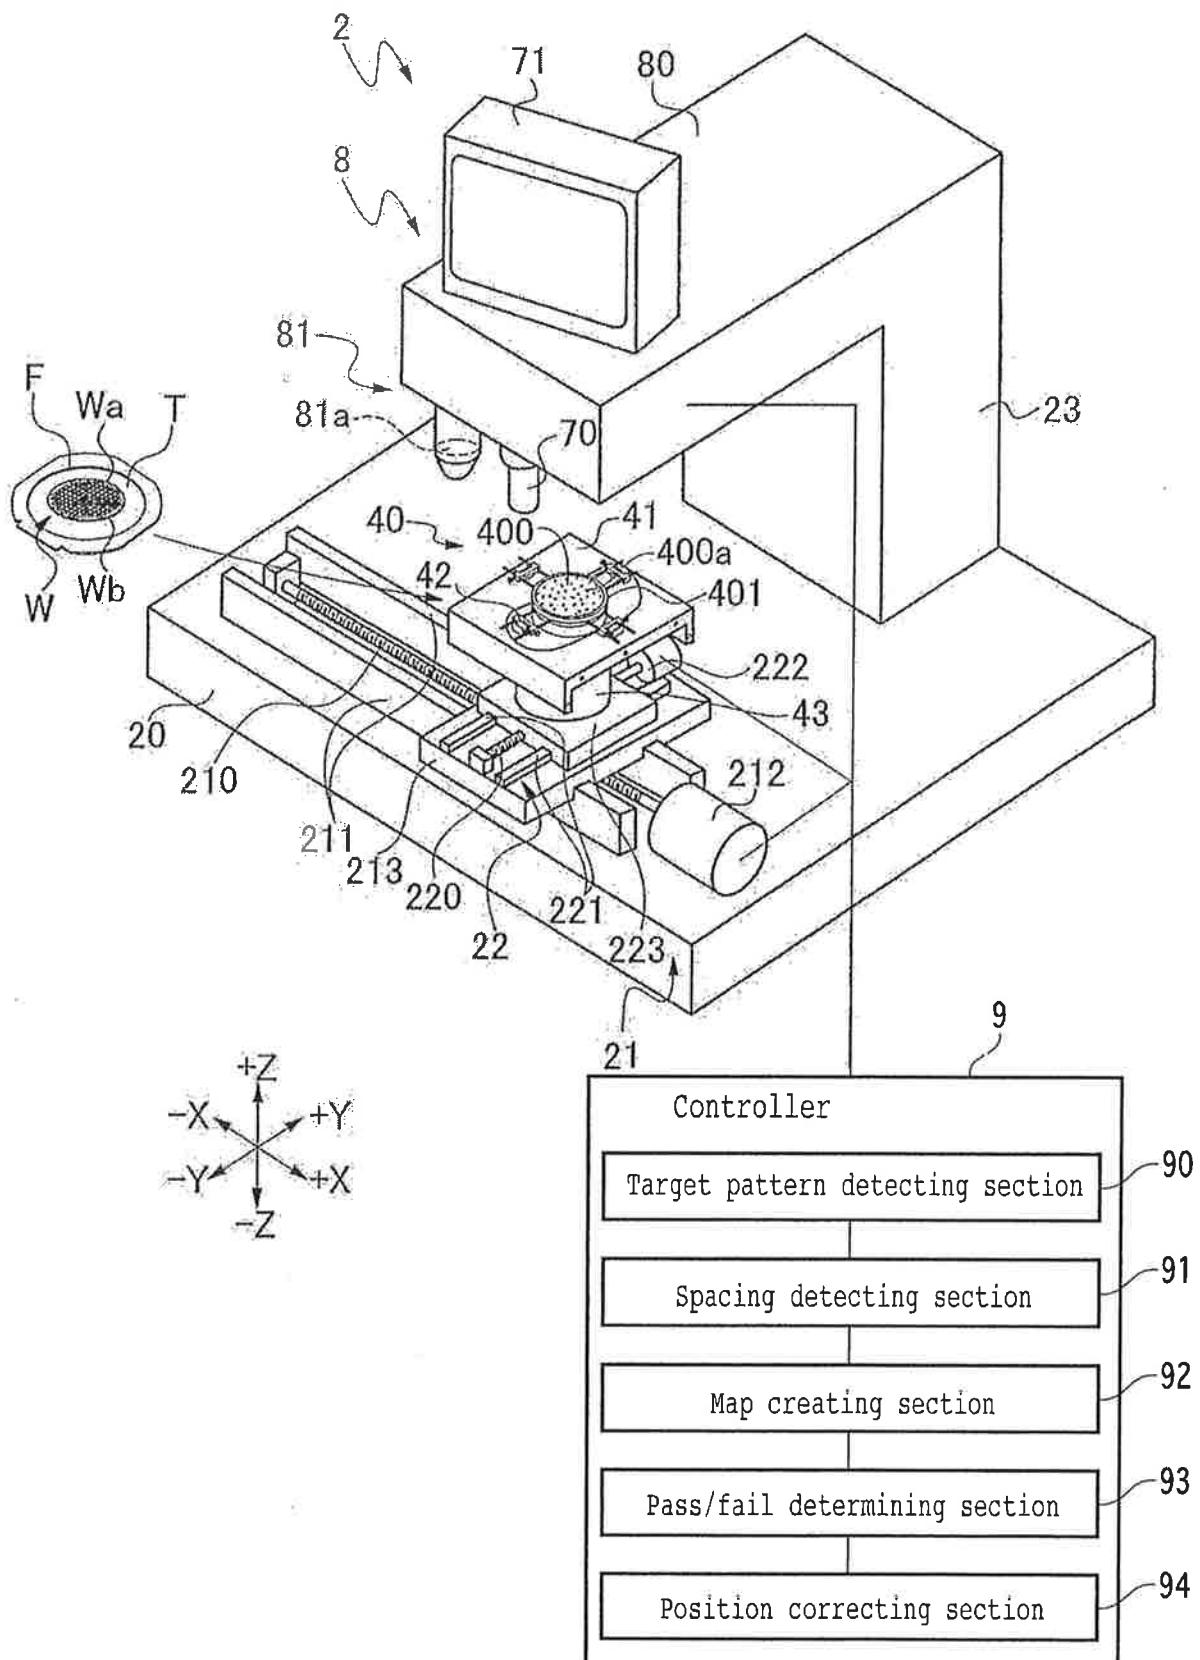


FIG.2

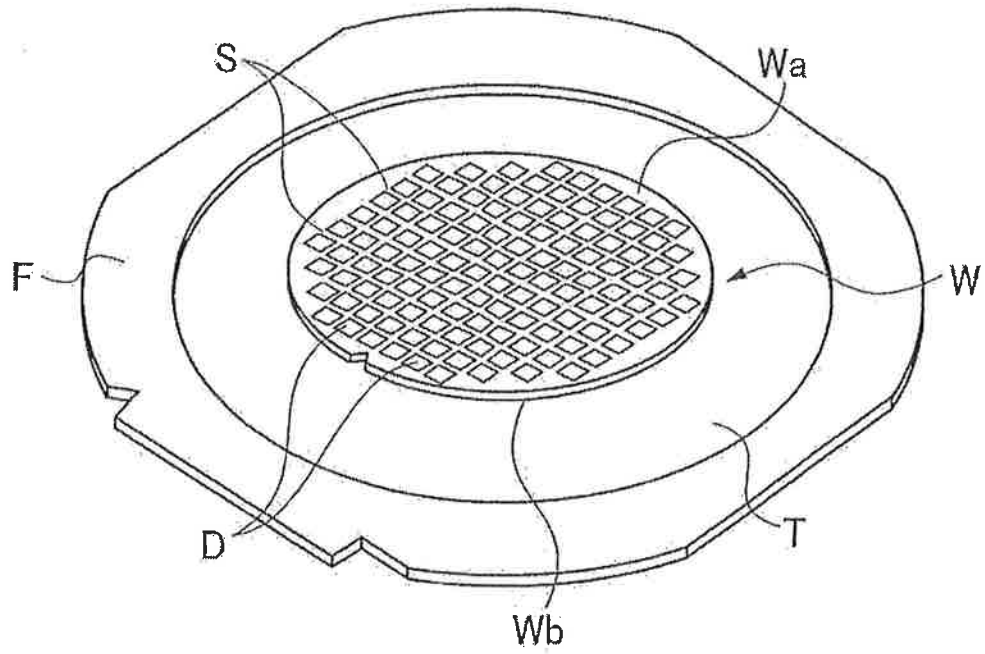


FIG.3

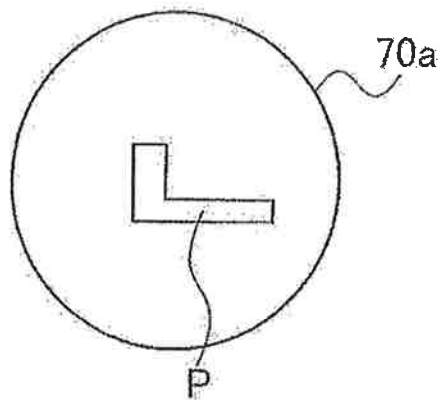


FIG. 4

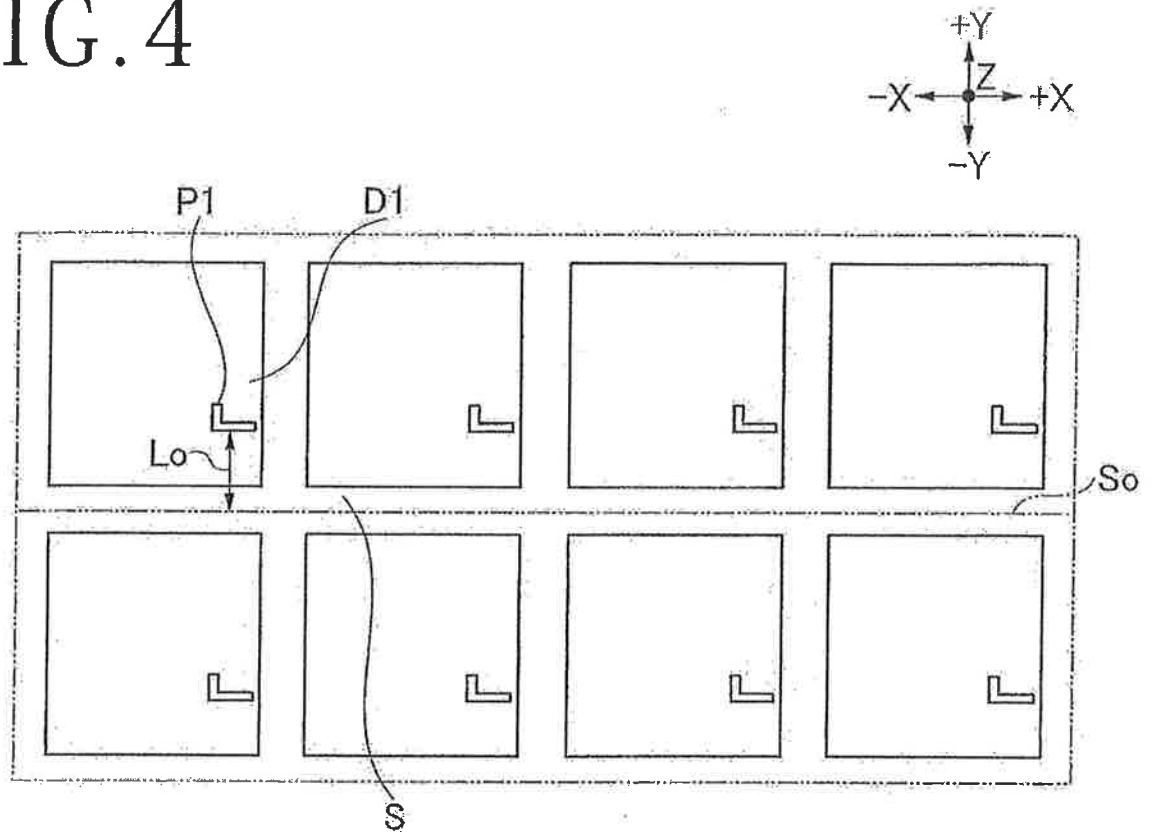


FIG. 5

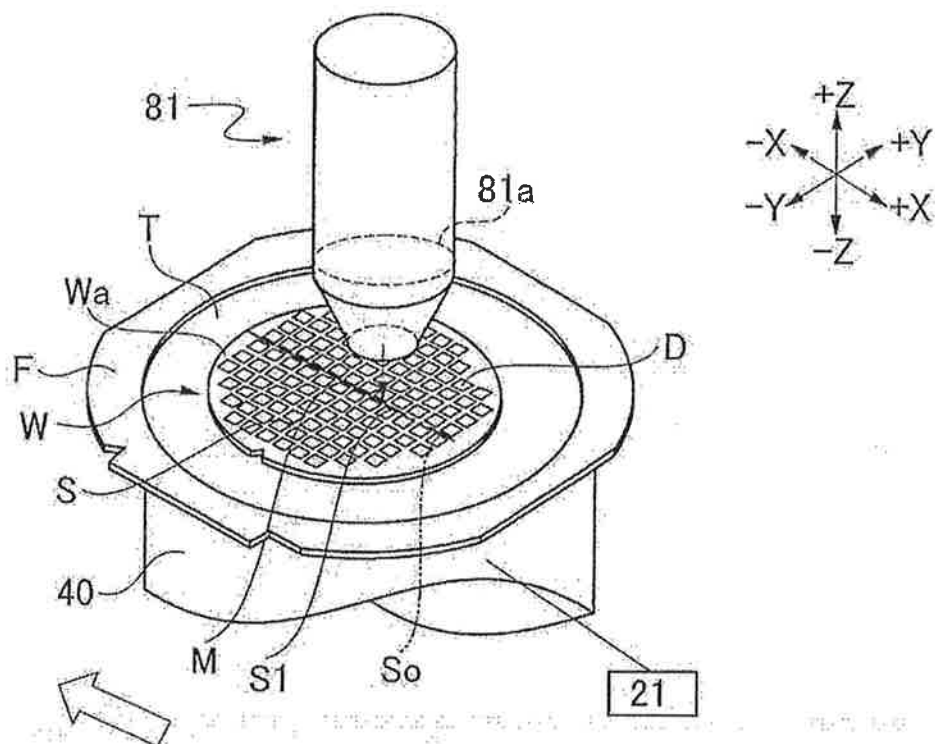


FIG. 6

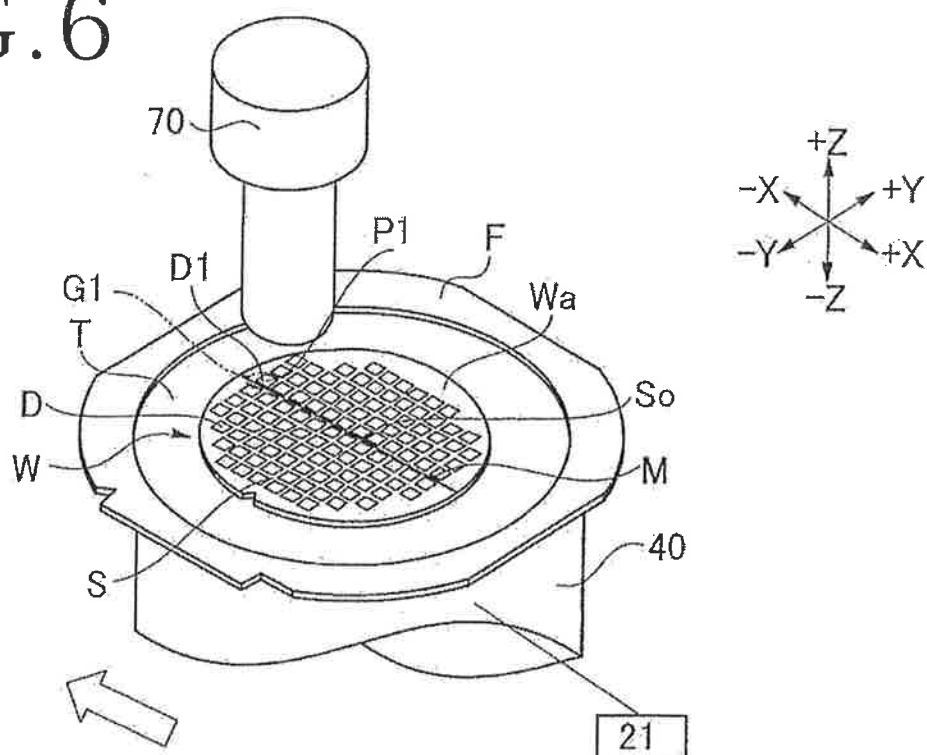


FIG. 7

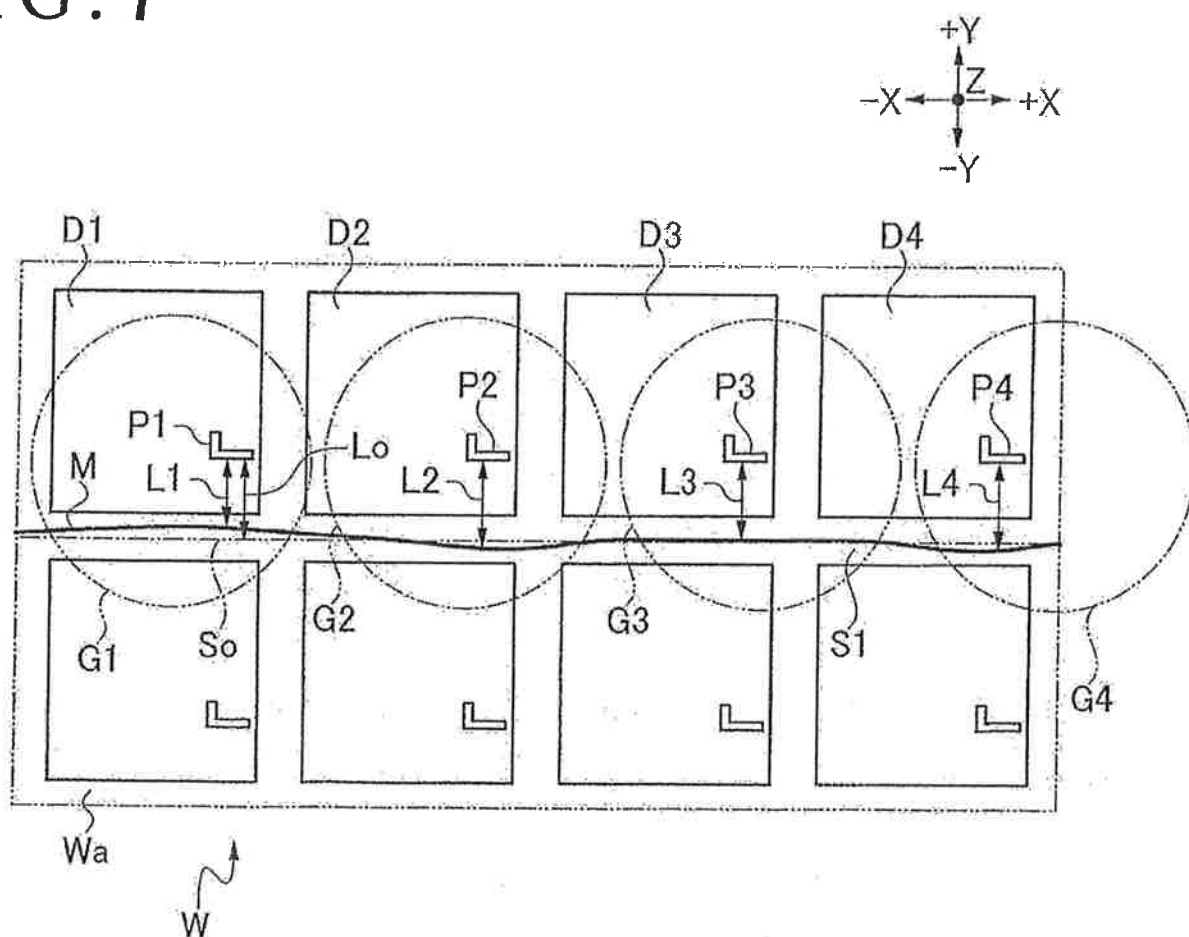


FIG. 8

C	Device	Target pattern	Spacing (μm) in Y direction between target pattern and ablation groove M
	D1	P1	203
	D2	P2	241
	D3	P3	220
	D4	P4	232

D(m-3)	P(m-3)	220
D(m-2)	P(m-2)	226
D(m-1)	P(m-1)	210
Dm	Pm	215