


[図1]

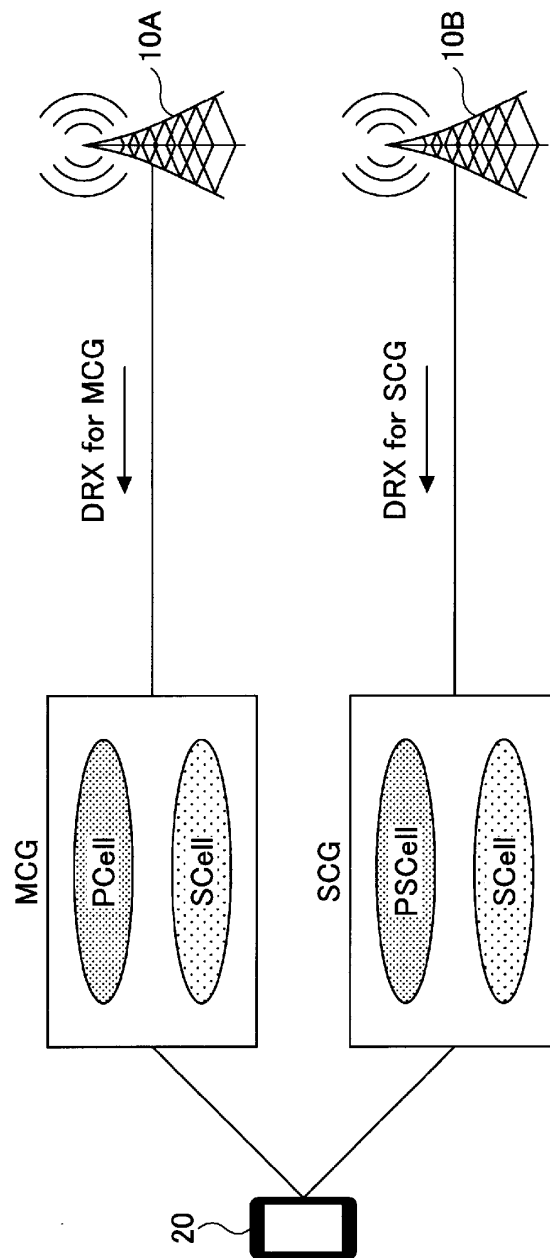


[図2]


Table 9.2.5.2-1: Measurement period for intrafrequency measurements without gaps(Frequency FR1)

DRX cycle	$T_{SSB_measurement_period}$
No DRX	$\max[200\text{ ms}, \text{ceil}(5 \times K_p) \times \text{SMTC period}]^{\text{Note 1}}$
DRX cycles $\leq 320\text{ ms}$	$\max[200\text{ ms}, \text{ceil}(1.5 \times 5 \times K_p) \times \max(\text{SMTC period}, \text{DRX cycle})]$
DRX cycle $> 320\text{ ms}$	$\text{ceil}(5 \times K_p) \times \text{DRX cycle}$
NOTE 1: If different SMTC periodicities are configured for different cells, the SMTC period in the requirement is the one used by the cell being identified	


[図3]

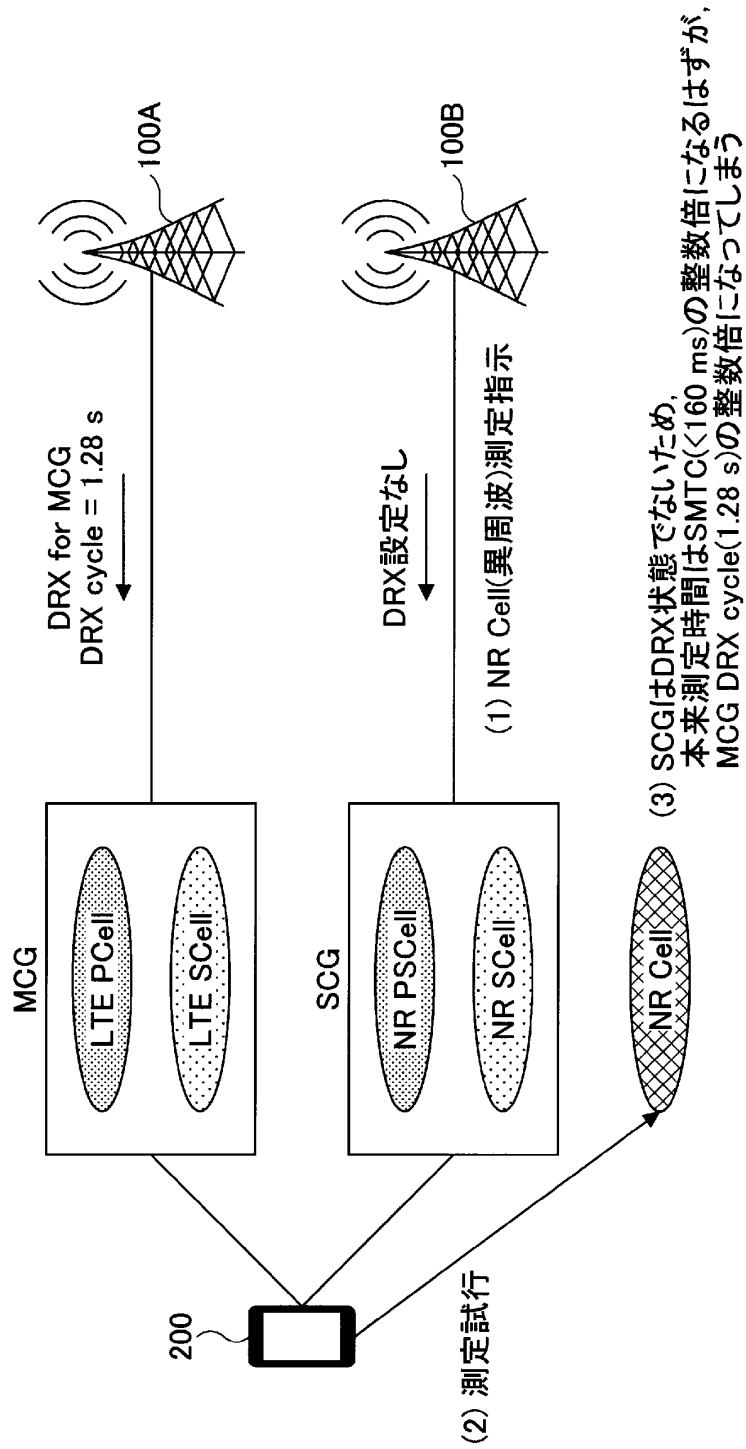


[図4]

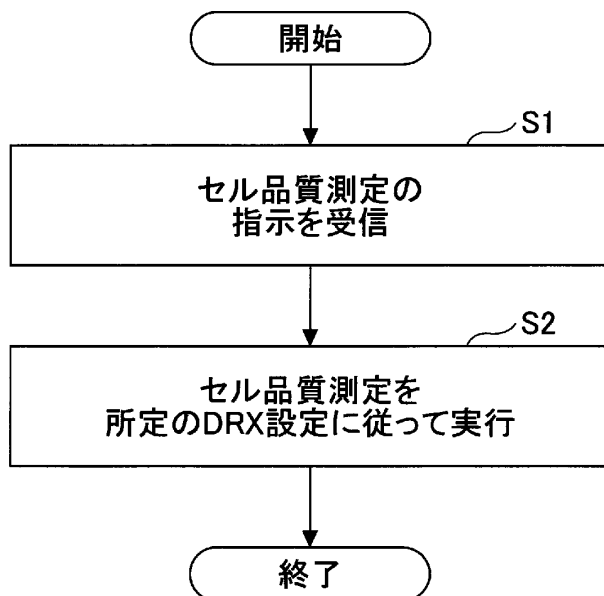

[図5]

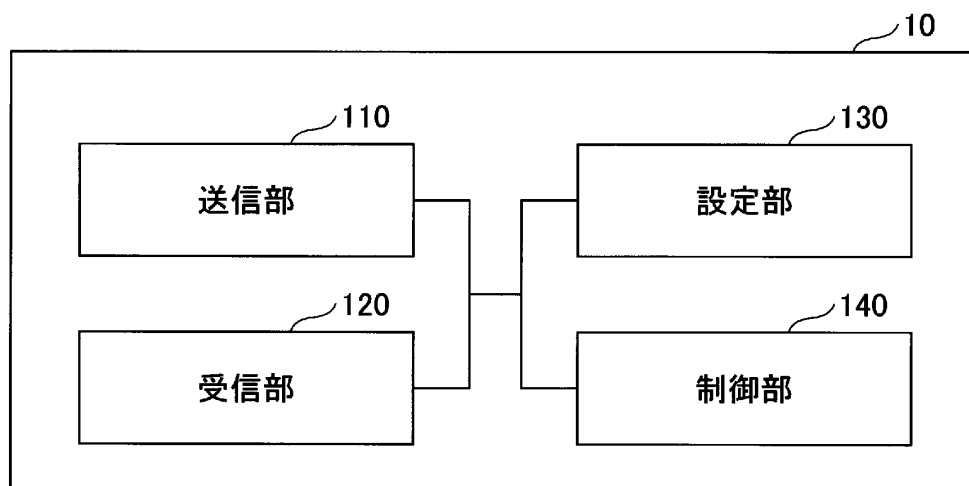

[図6]

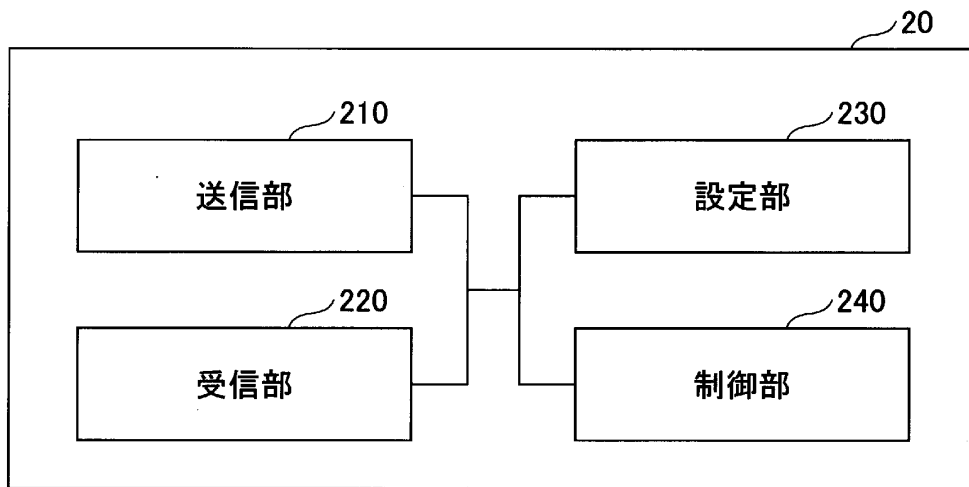

[図7]

