

(43) International Publication Date
2 October 2014 (02.10.2014)(51) International Patent Classification:
G09B 23/28 (2006.01)(21) International Application Number:
PCT/EP2014/056137(22) International Filing Date:
27 March 2014 (27.03.2014)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
13161552.8 28 March 2013 (28.03.2013) EP(71) Applicant: **F. HOFFMANN-LA ROCHE AG** [CH/CH];
Grenzacherstrasse 124, CH-4070 Basel (CH).(72) Inventors: **GAILLOT, Maxime**; 3, rue de l'église, F-68130 Zaessingue (FR). **CHIPPERFIELD, Mark Anthony**; Ettingerstrasse 3, CH-4147 Aesch (CH). **TEUCHER, Mark**; 17 Somerset Lane, Lansdown Bath BA1 5SW (GB). **HAYTON, Paul**; 35 Waverley Road, Redland Bristol BS66ES (GB).(74) Agent: **BOHEST AG**; Holbeinstrasse 36-38, CH-4051 Basel (CH).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: TRAINING DEVICE FOR MEDICINE INJECTION DEVICES AND RESET DEVICE FOR RESETTING SUCH A TRAINING DEVICE

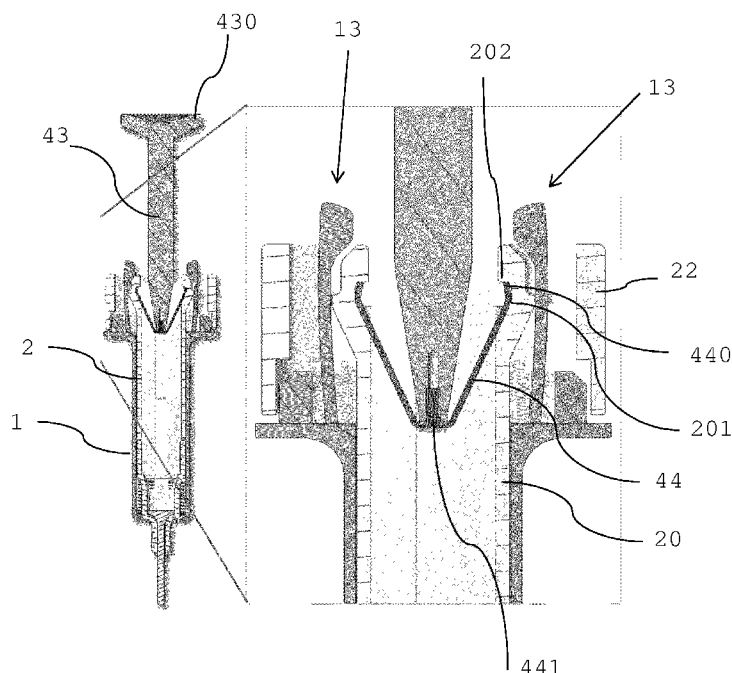


Fig. 3

(57) Abstract: The training device for medicine injection devices comprises a plunger (43) slidably arranged in the cavity of a body (2). The plunger comprises a compressible element (44) arranged at a distal end of the plunger (43) and adapted to provide a resistance between compressible element (44) and inner wall of the cavity of the body (2) when the plunger (43) is moved in the cavity towards the distal end of the body. The resistance corresponds to an injection resistance of a medicine injected into a patient. The invention also comprises a reset device for resetting the training device from a used status to a condition for reuse.