

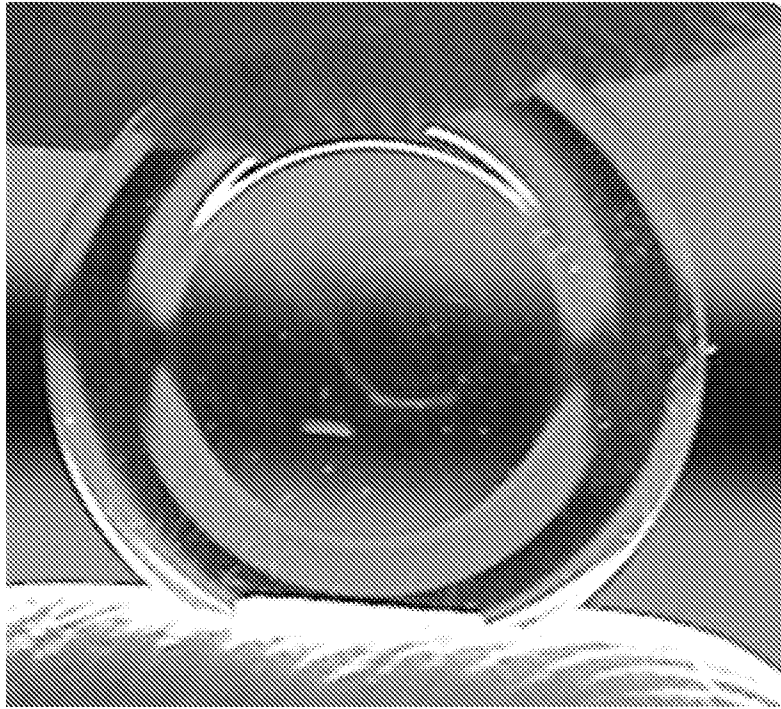


Fig. 1A

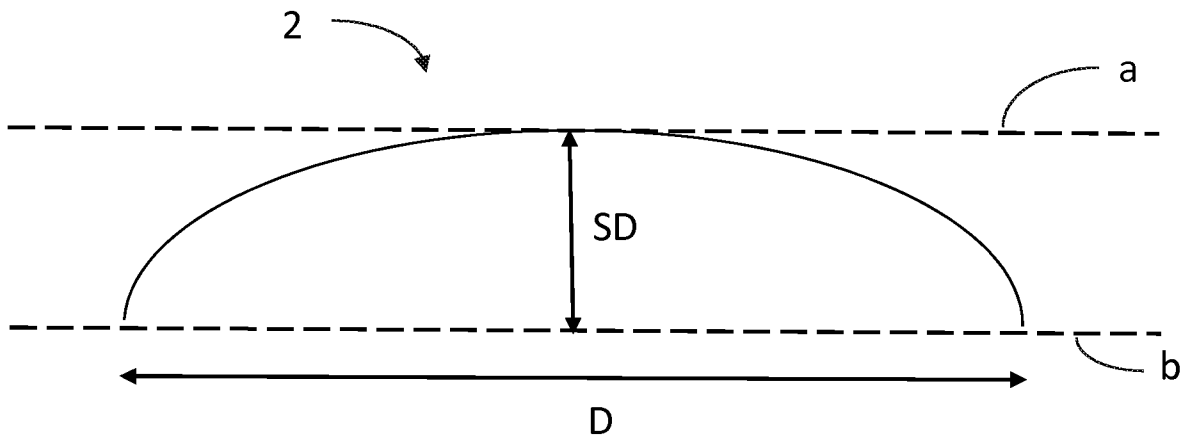
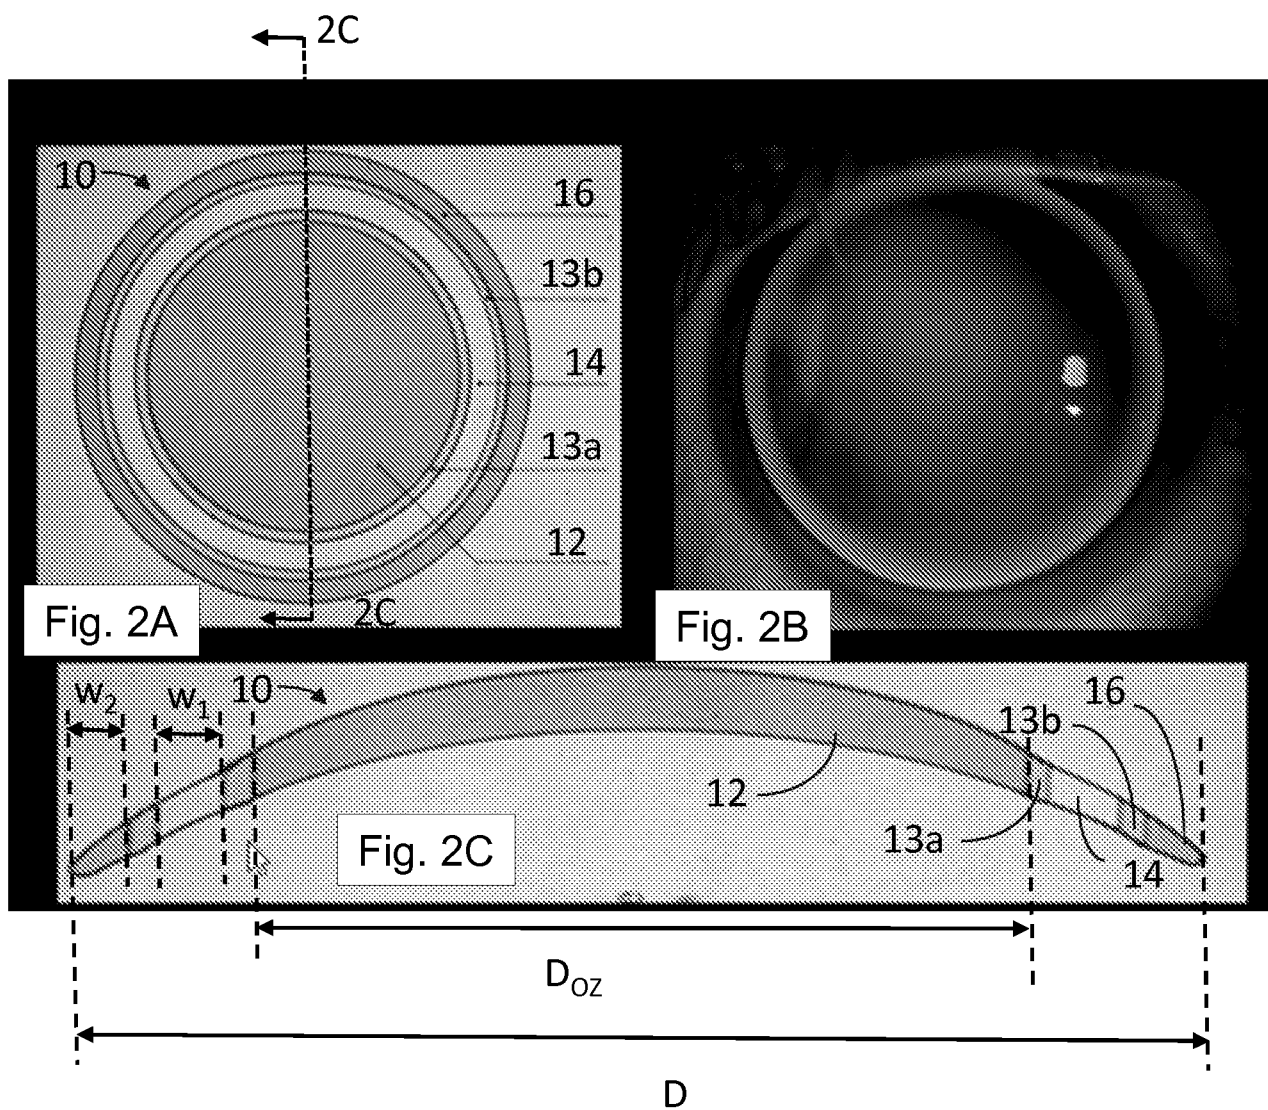


Fig. 1B



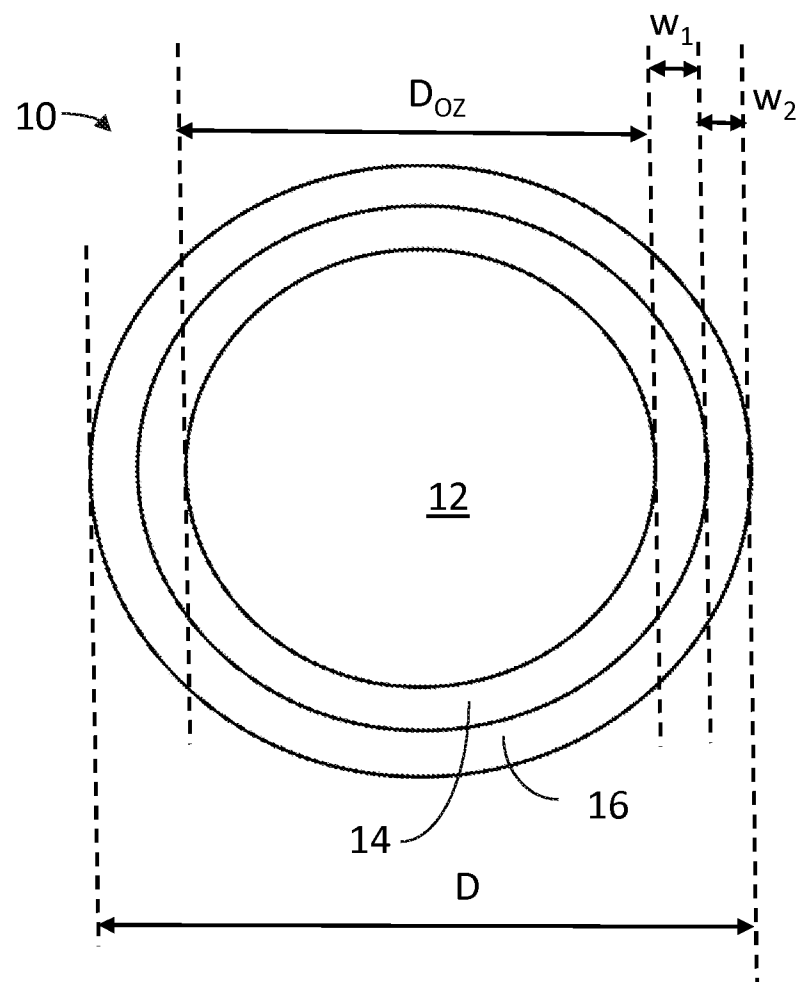


Fig. 2D

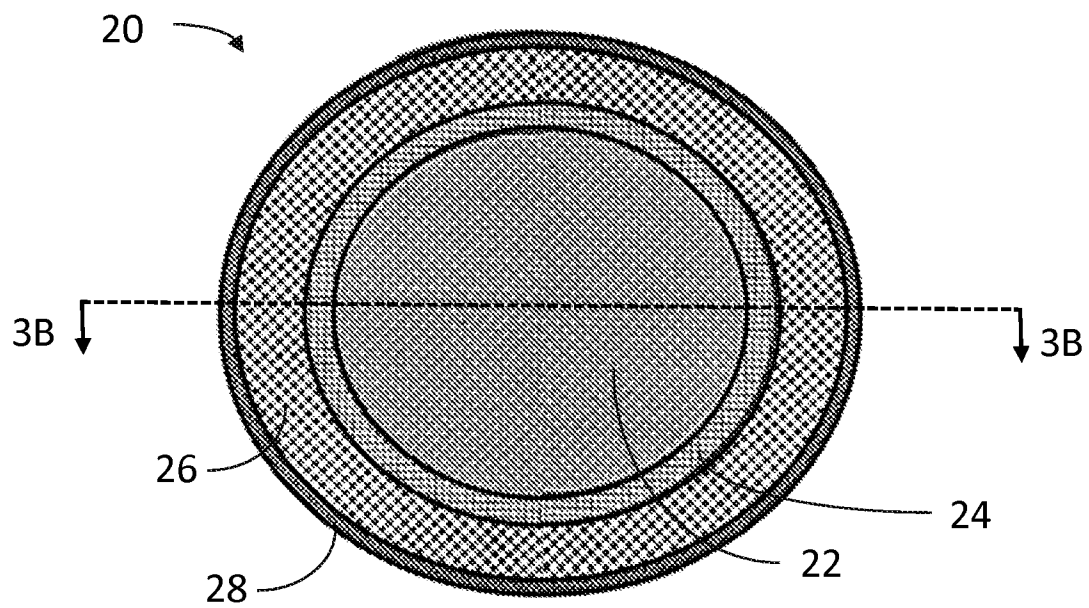


Fig. 3A

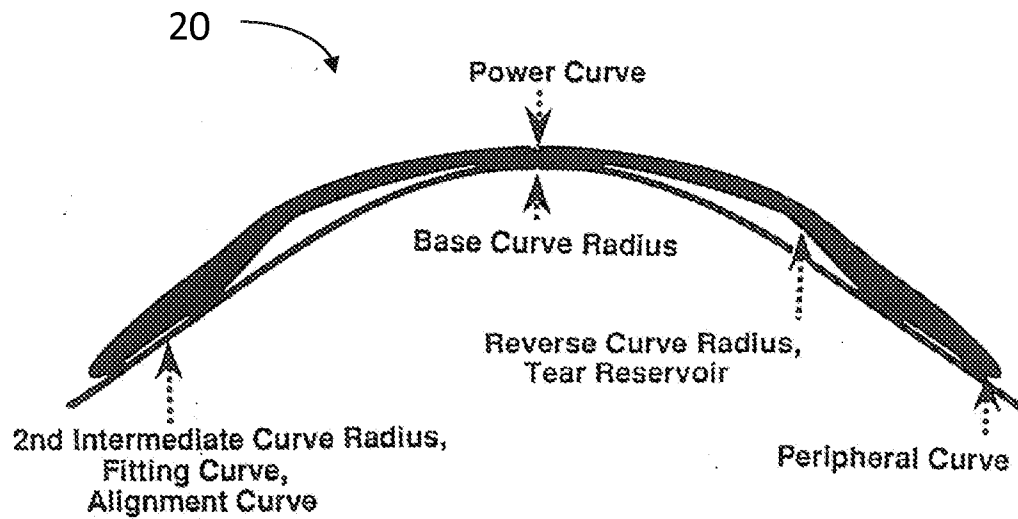


Fig. 3B

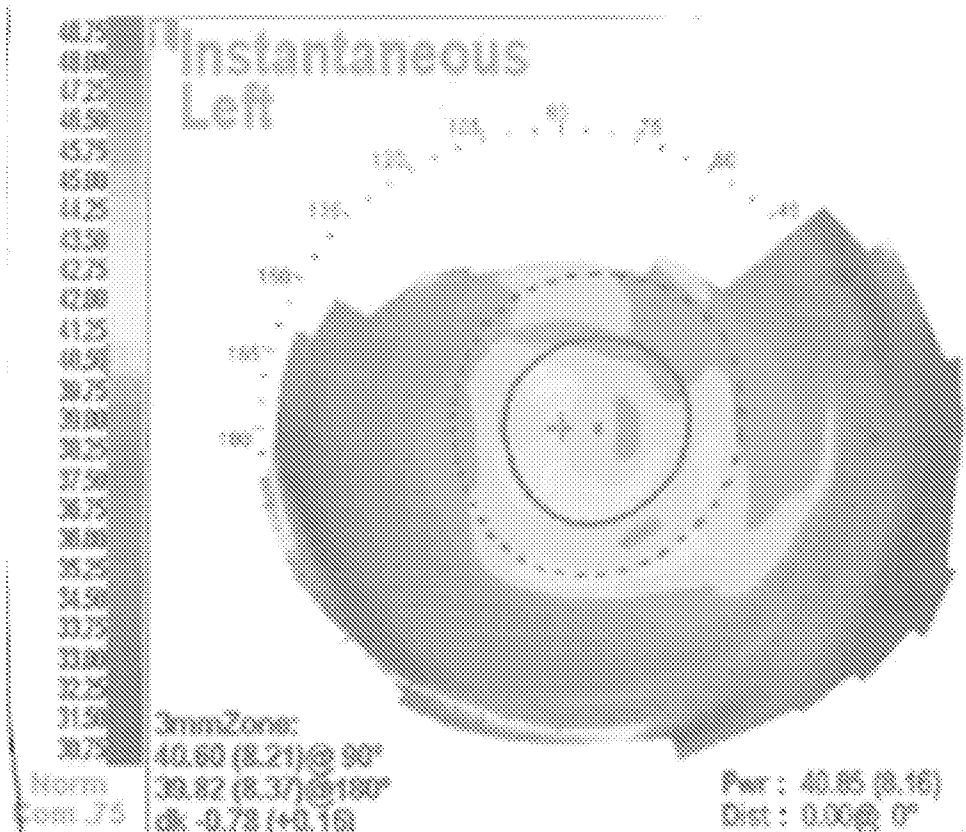


Fig. 4A

Keratometry

SimK1: 40.90 @ 89

SimK2: 40.40 @ 179

CYL : -0.50

Asphericity 8.0mm

e : 0.22 (-0.26, 0.71)

Q: -0.22 (0.07, -0.50)

Pupilometry mm

Photopic: 2.44

Mesopic: 4.00

MPdist: 0.08 @ 90

Pdist : 0.50 @ 355

Mdist : 0.50 @ 5

Fig. 4B

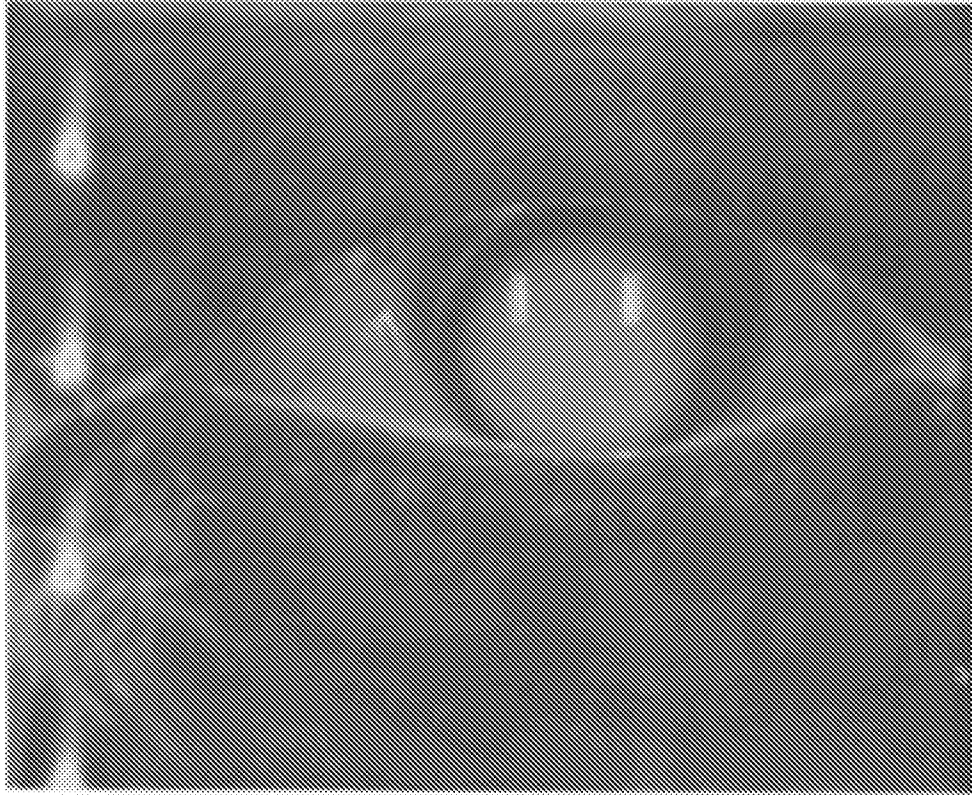


Fig. 4C

Table 1. Near Vision and Far Vision Measurements										
Patient	Far Vision before treatment	Near Vision before treatment	Far Vision 7 days Post	Near Vision 7 days Post	Far Vision 4 months Post	Near Vision 4 months Post	Far Vision 6 months Post	Near Vision 6 months Post	Far Vision 8 months Post	Near Vision 8 months Post
1	20/20	J8	20/20	J 3	20/15	J 2	20/15-1	J 1	20/15-1	J1
2	20/20	J6	20/15	J 3	20/15-1	J 3	20/15	J 2	20/15	J2
3	20/20	J10	20/15-3	J 10	20/15-1	J 6	20/15	J 5	20/15	J5
4	20/20	J10	20/20	J 3	20/15	J 4	20/15	J 5	20/15	J5
5	20/25	J8	20/15	J 3	20/15-1	J 3	20/20-1	J 2	20/20-1	J2
6	20/15	J10	20/15	J 3	20/20+2	J 5	20/20+2	J 5	-	-
7	20/20	J10	20/15	J 1	20/15	J 2	20/15	J 2	20/15	J1
8	20/25	J6	20/20	J 2	20/20+3	J 3	20/15-1	J 2	20/15-1	J2
9	20/20	J10	20/15	J 6	20/15-1	J 4	20/15-2	J 5	20/15-2	J5
10	20/25	J10	20/20	J 10	20/20	J 10	-	-	-	-
11	20/20	J5	20/15	J 2	20/15-1	J 3	20/15-1	J 3	-	-
12	20/25	J8	20/15-1	J 3	20/15-2	J 3	20/15-2	J 3	-	-

Fig. 5A

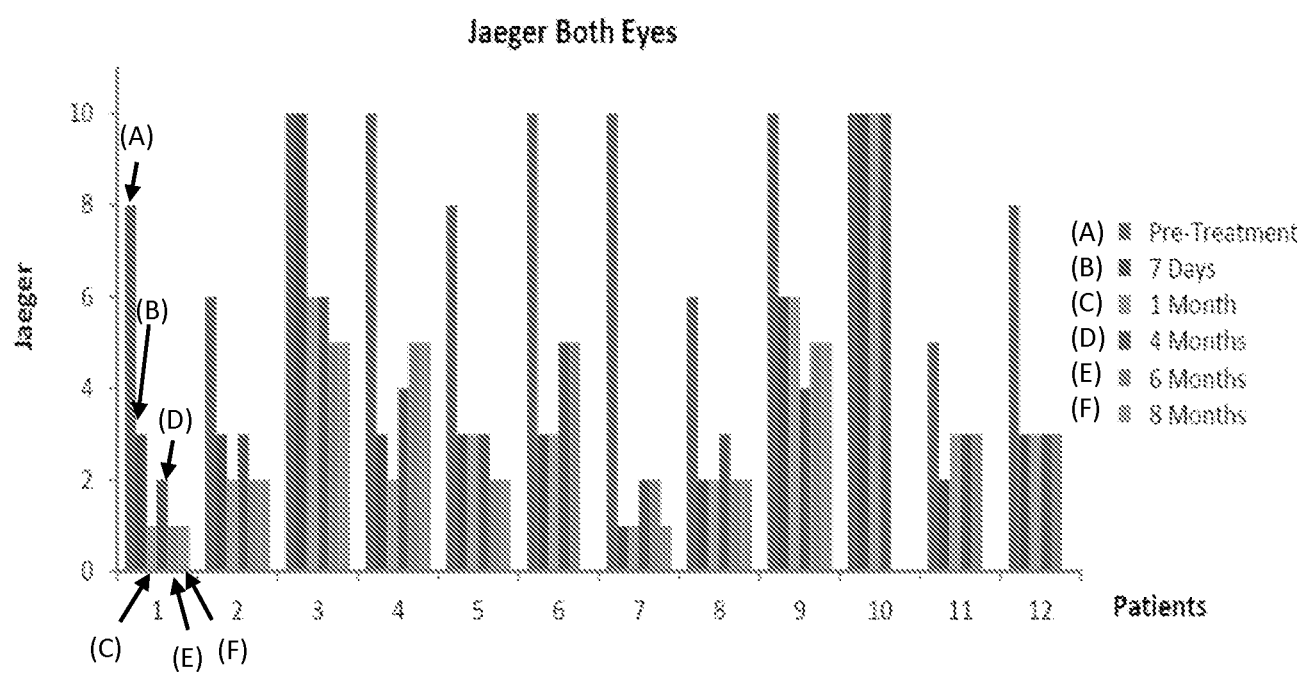


Fig. 5B